

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022120\
 Data File : P0066756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2020 2:39
 Operator : DD\AJ
 Sample : L1625-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-050-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 04:10:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 14:58:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.124	3.405	1059718	1272642	25.219	23.562
2)	SA Decachlor...	9.594	8.286	865929	1050349	21.100	18.901

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022120\
Data File : P0066756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2020 2:39
Operator : DD\AJ
Sample : L1625-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-050-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 04:10:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 14:58:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

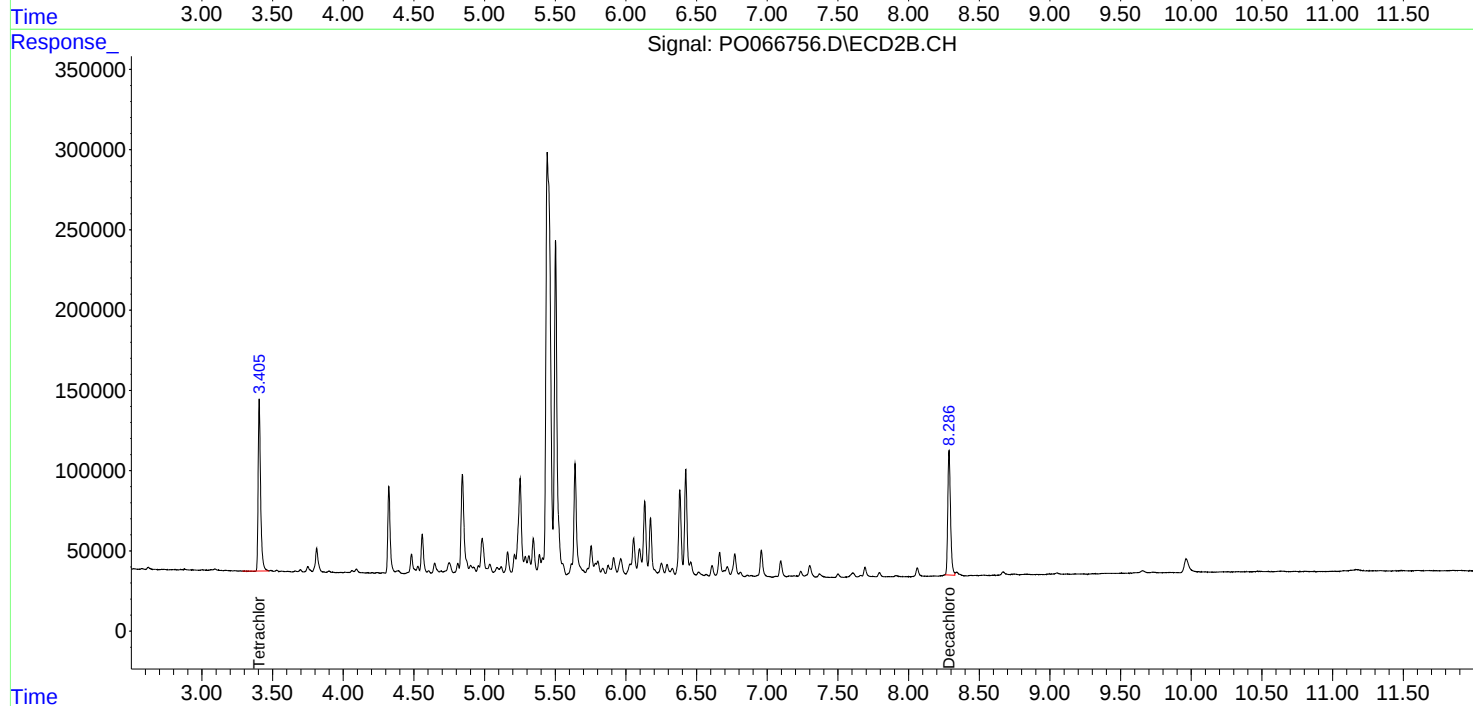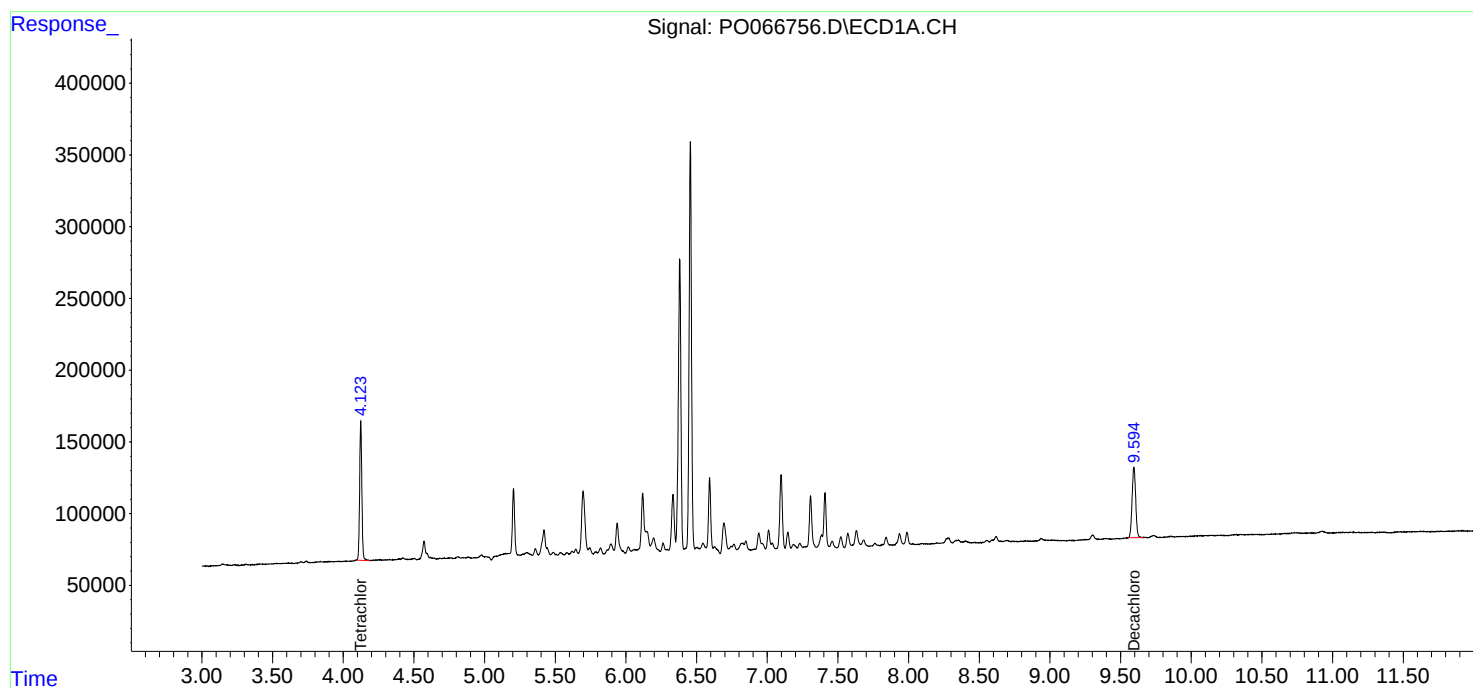


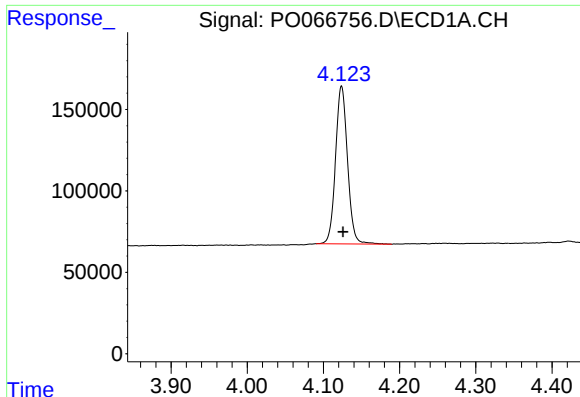

#1 Tetrachloro-m-xylene


R.T.: 4.124 min
Delta R.T.: -0.002 min
Response: 1059718
Conc: 25.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-050-B

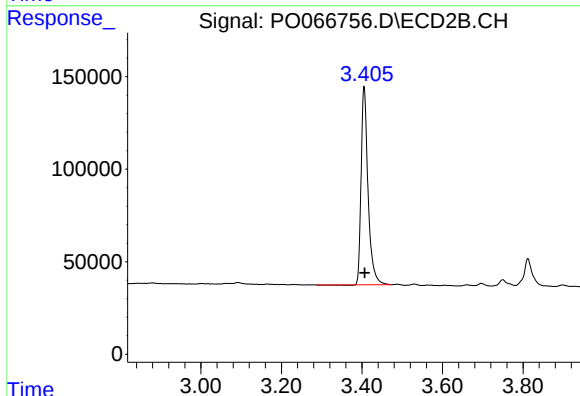


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: -0.001 min
Response: 1272642
Conc: 23.56 ng/ml

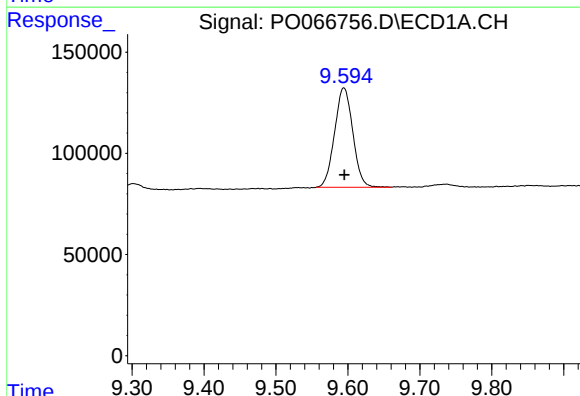

#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: 0.000 min
Response: 865929
Conc: 21.10 ng/ml

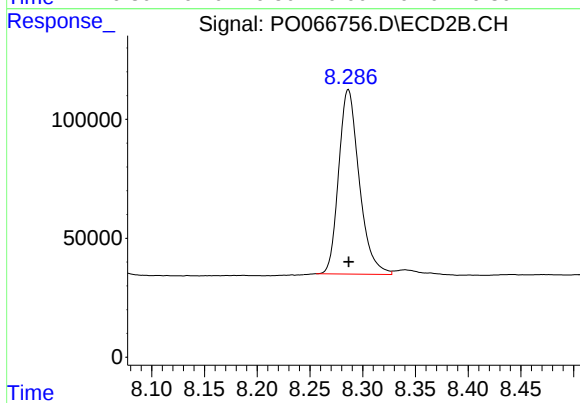

#2 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 1050349
Conc: 18.90 ng/ml