

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022122\
Data File : P0084761.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2022 13:41
Operator : YP\AJ
Sample : PB142830BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB142830BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:46:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.596	4237864	933769	21.553	20.705
2) SA Decachlor...	10.427	8.622	3157786	766491	25.448	21.026

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022122\
Data File : P0084761.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2022 13:41
Operator : YP\AJ
Sample : PB142830BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB142830BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:46:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

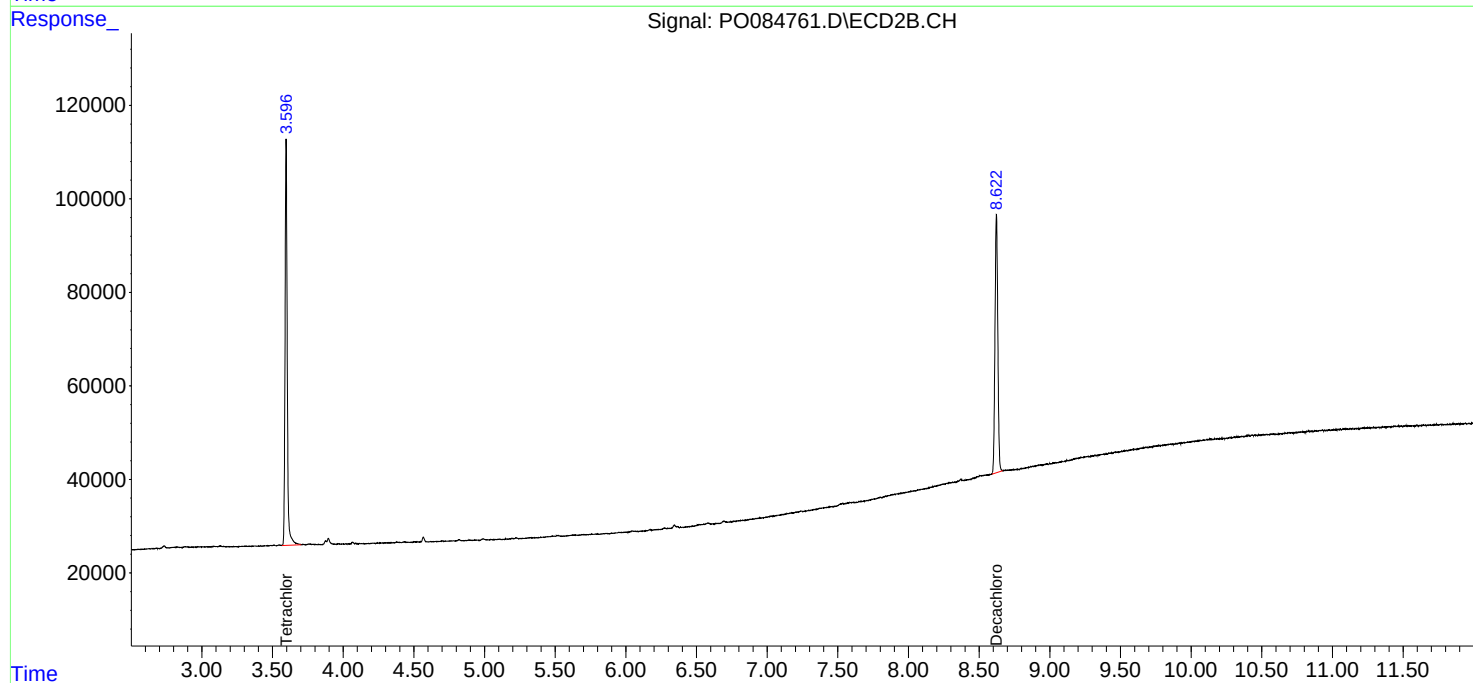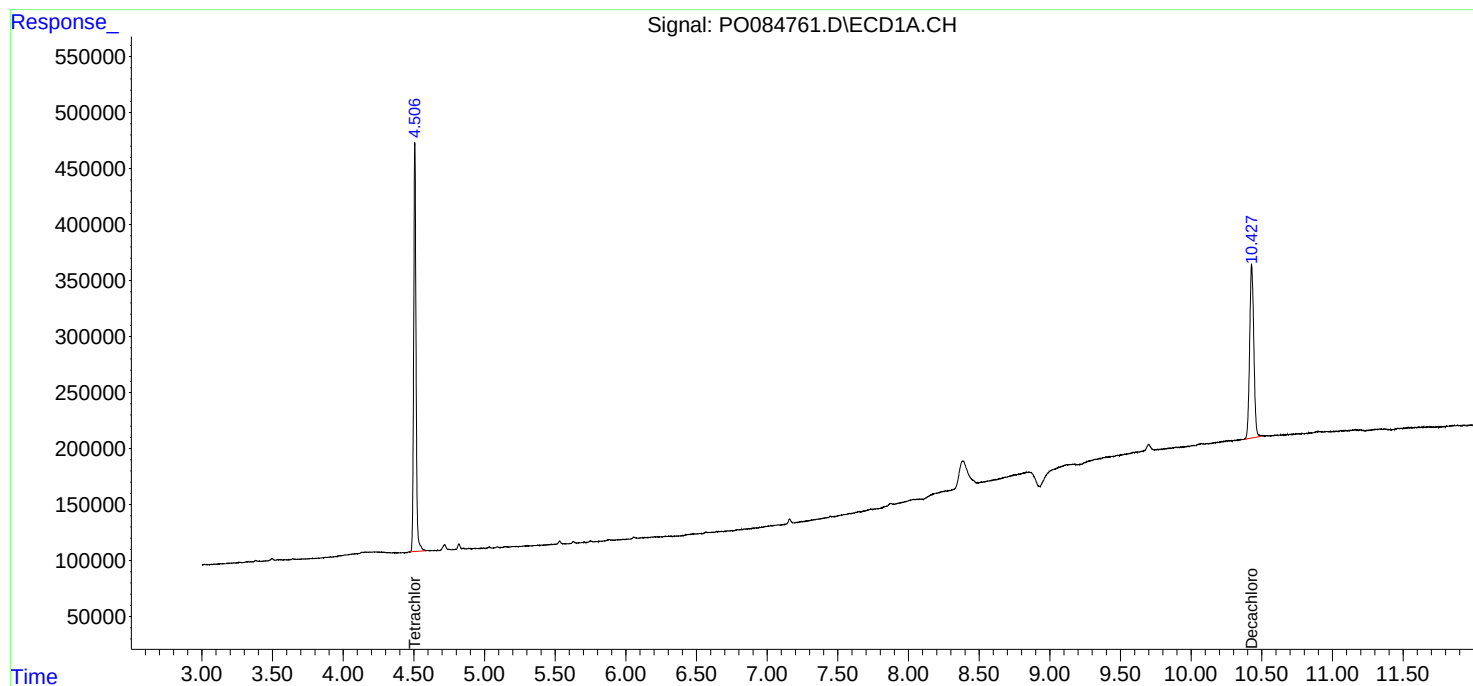


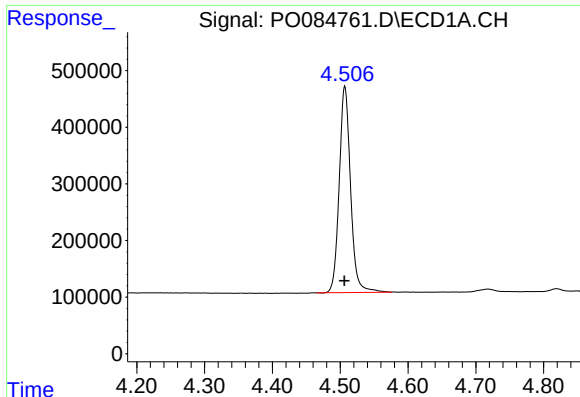

#1 Tetrachloro-m-xylene


R.T.: 4.507 min
Delta R.T.: 0.000 min
Response: 4237864
Conc: 21.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB142830BL

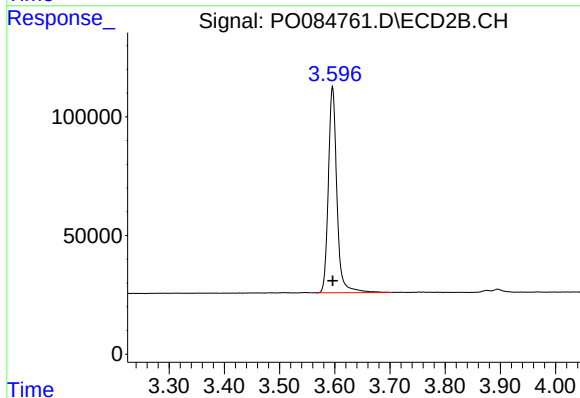


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 933769
Conc: 20.71 ng/ml

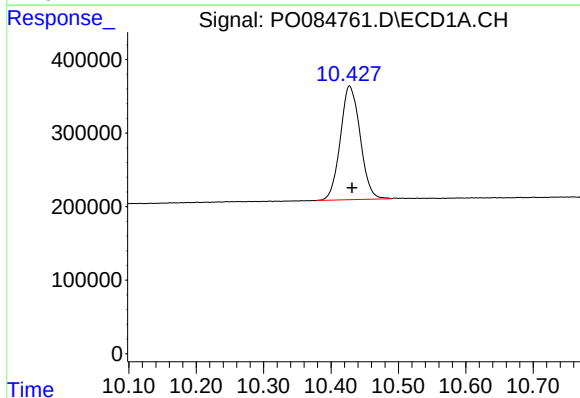

#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: -0.004 min
Response: 3157786
Conc: 25.45 ng/ml

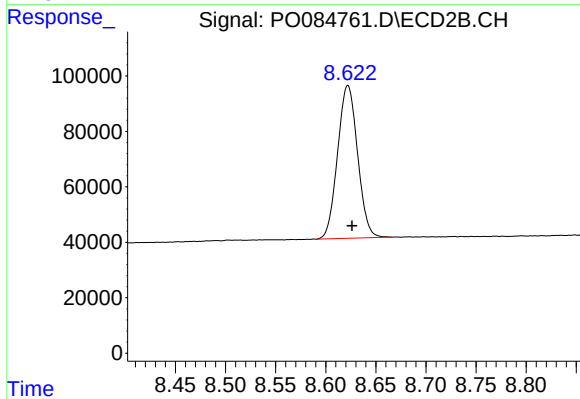

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.004 min
Response: 766491
Conc: 21.03 ng/ml