

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022124\
 Data File : P0101938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 10:59
 Operator : YP/AJ
 Sample : P1516-01RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/22/2024
 Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 11:48:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.272	3.394	12790198	3078050	4.148m	1.158 #
2) SA Decachlor...	9.837	8.273	8158223	4202135	3.891	2.212 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022124\
Data File : PO101938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 10:59
Operator : YP/AJ
Sample : P1516-01RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 11:48:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

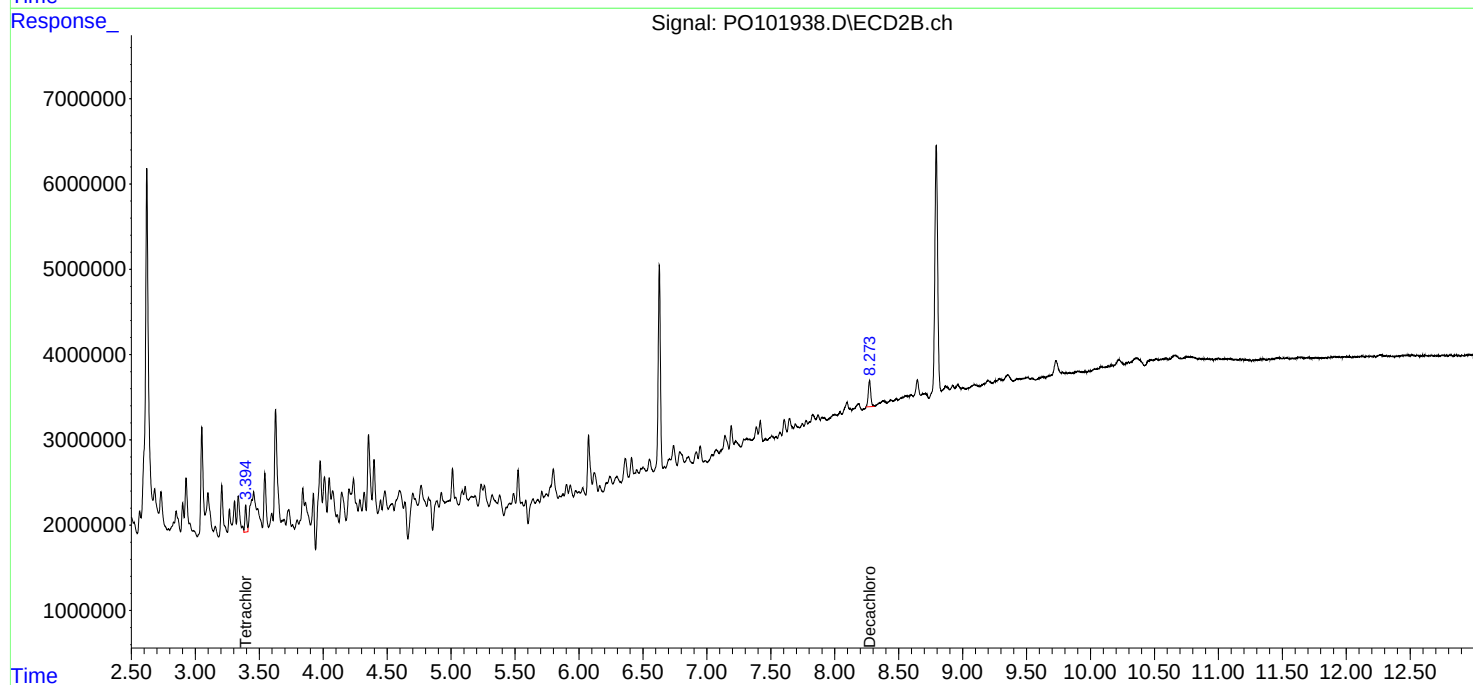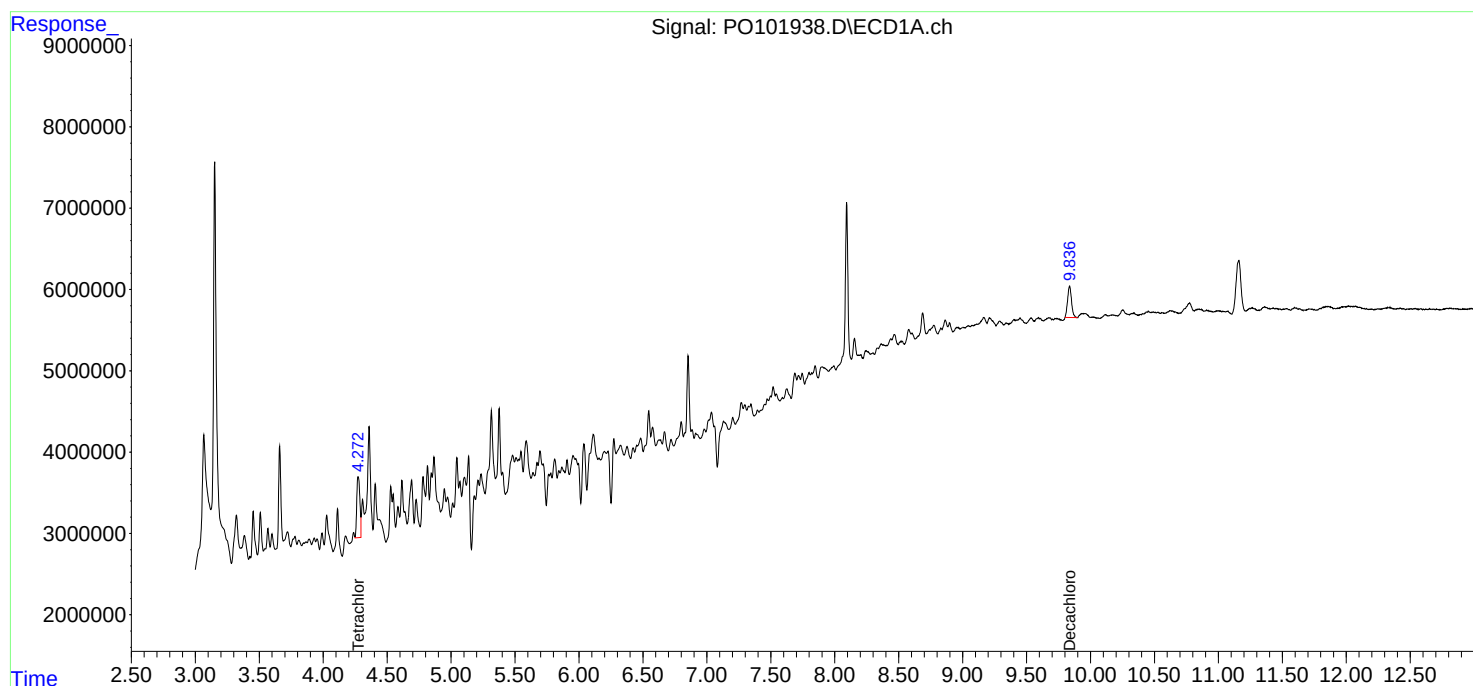

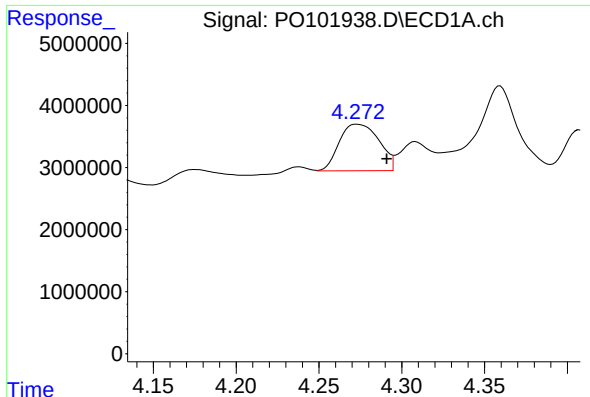


#1 Tetrachloro-m-xylene

R.T.: 4.272 min
Delta R.T.: -0.019 min
Response: 12790198
Conc: 4.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

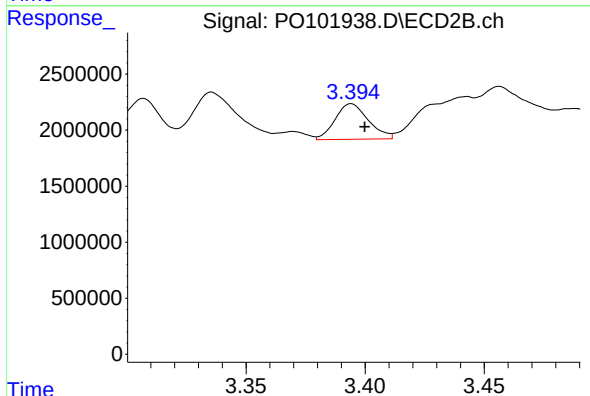


#1 Tetrachloro-m-xylene

R.T.: 3.394 min
Delta R.T.: -0.006 min
Response: 3078050
Conc: 1.16 ng/ml

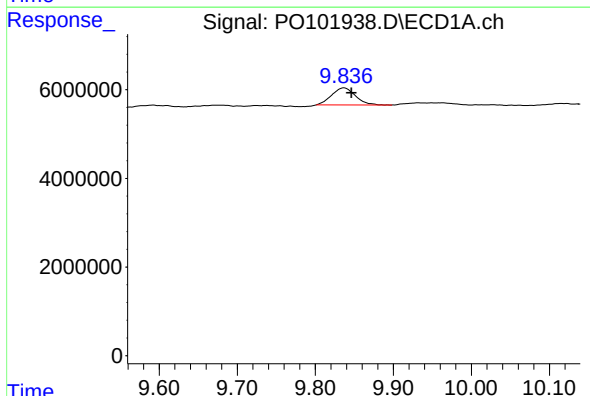

#2 Decachlorobiphenyl

R.T.: 9.837 min
Delta R.T.: -0.010 min
Response: 8158223
Conc: 3.89 ng/ml

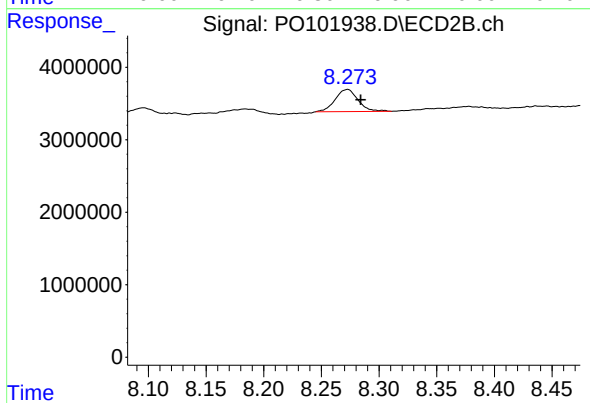

#2 Decachlorobiphenyl

R.T.: 8.273 min
Delta R.T.: -0.011 min
Response: 4202135
Conc: 2.21 ng/ml