

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022124\
 Data File : P0101946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 13:17
 Operator : YP/AJ
 Sample : P1491-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20241095-35N-N-FIELD-BLANK-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/22/2024
 Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 14:20:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.283	3.394	84028000	64600169	27.251	24.303
2) SA Decachlor...	9.832	8.268	44490553	34537916	21.217m	18.179m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022124\
Data File : PO101946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 13:17
Operator : YP/AJ
Sample : P1491-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20241095-35N-N-FIELD-BLANK-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 14:20:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

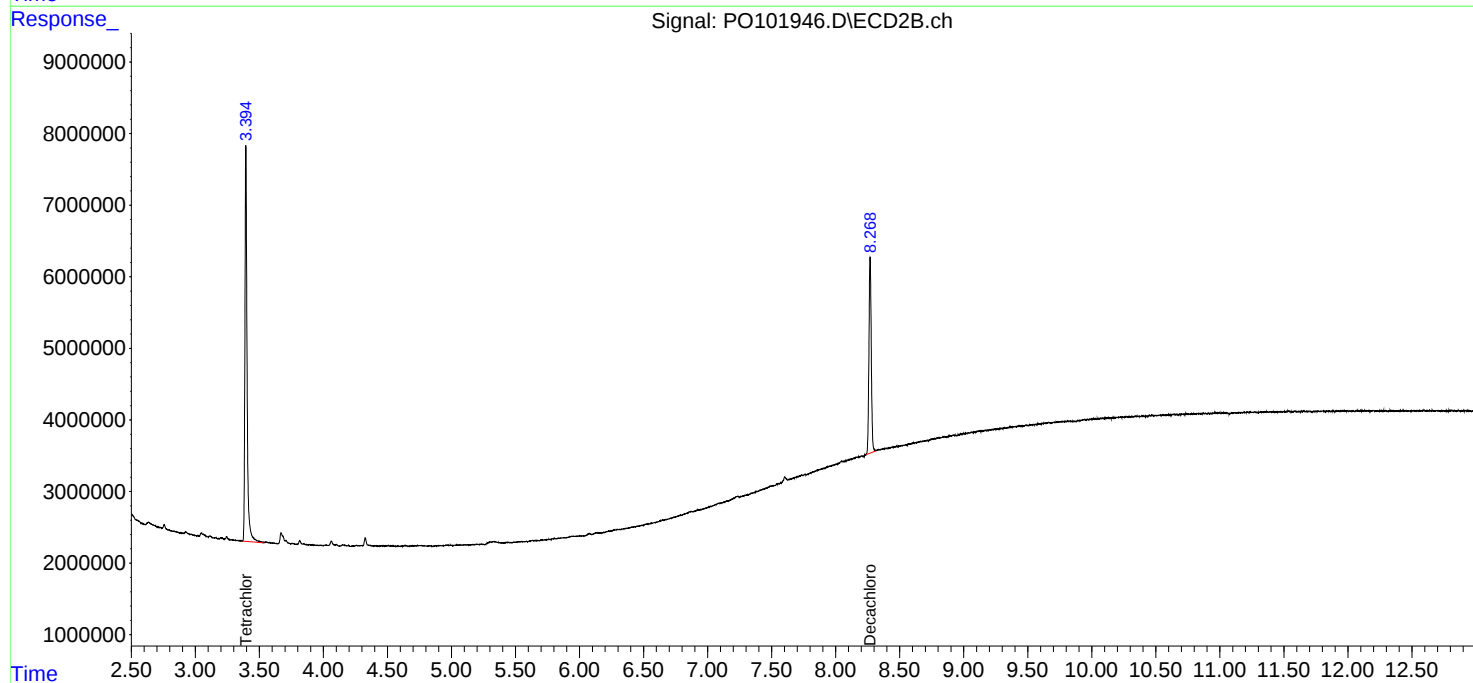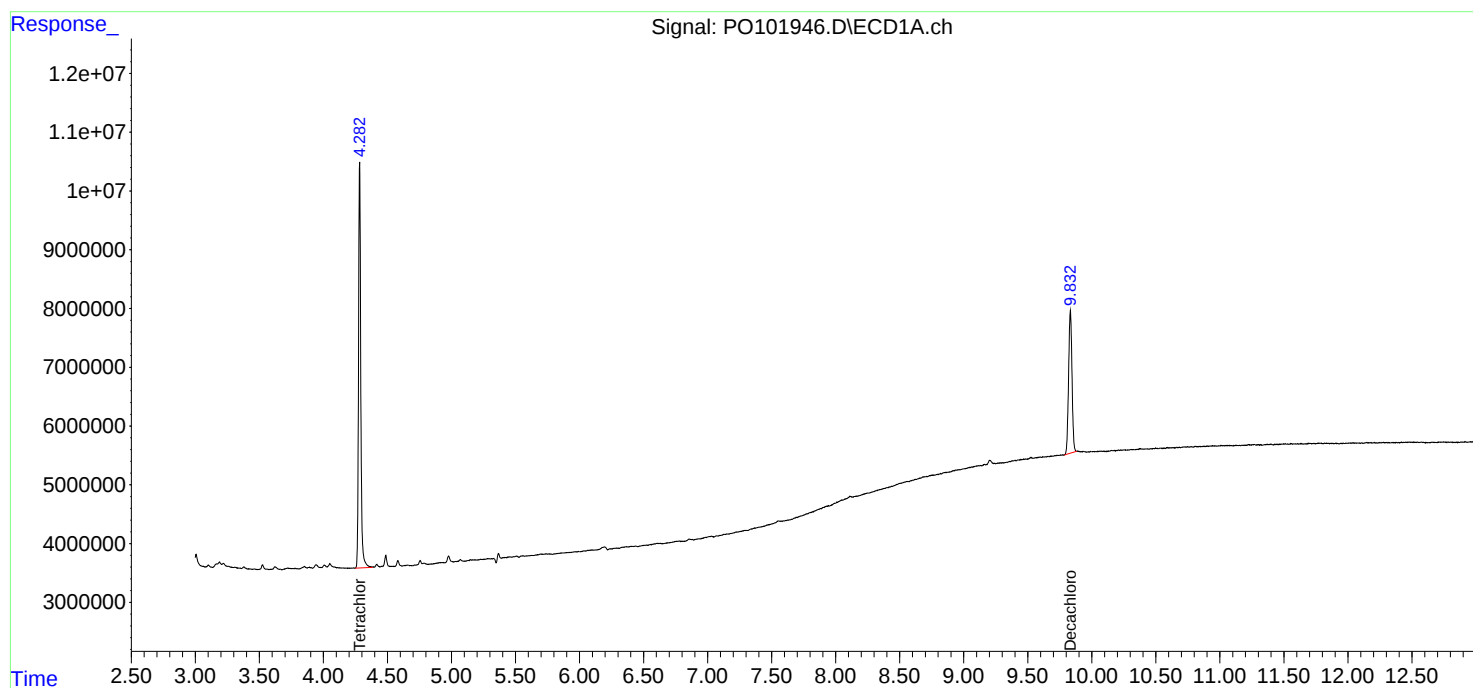

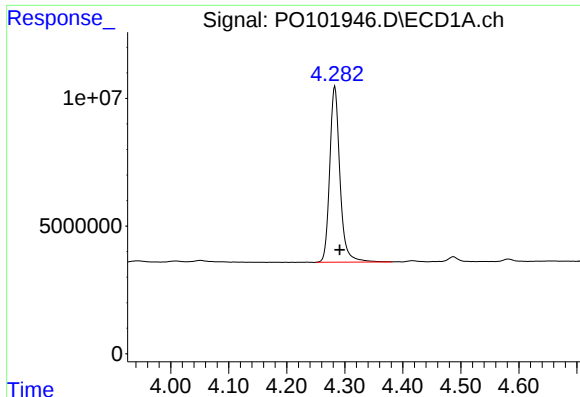


#1 Tetrachloro-m-xylene

R.T.: 4.283 min
Delta R.T.: -0.008 min
Response: 84028000
Conc: 27.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
20241095-35N-N-FIELD-BLANK-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

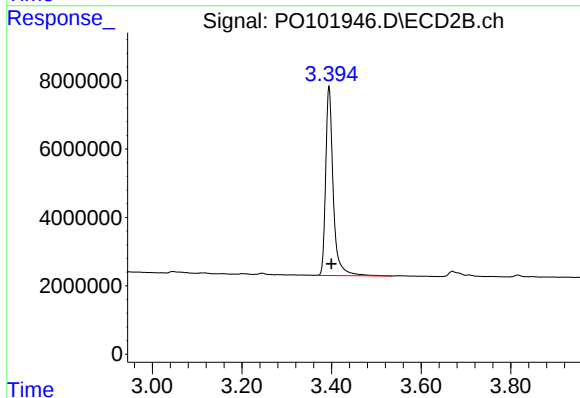


#1 Tetrachloro-m-xylene

R.T.: 3.394 min
Delta R.T.: -0.005 min
Response: 64600169
Conc: 24.30 ng/ml

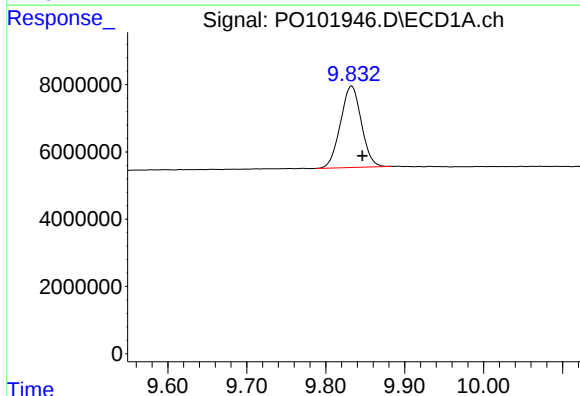

#2 Decachlorobiphenyl

R.T.: 9.832 min
Delta R.T.: -0.014 min
Response: 44490553
Conc: 21.22 ng/ml m

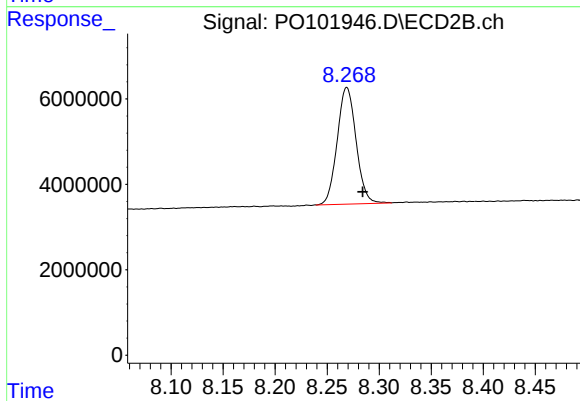

#2 Decachlorobiphenyl

R.T.: 8.268 min
Delta R.T.: -0.016 min
Response: 34537916
Conc: 18.18 ng/ml m