

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022124\
 Data File : P0101959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 17:17
 Operator : YP/AJ
 Sample : P1521-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CG-MW-23

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/22/2024
 Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:17:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.283	3.394	67521945	51514206	21.898	19.380m
2) SA Decachlor...	9.832	8.269	40217583	28728024	19.179m	15.121

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022124\
Data File : PO101959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 17:17
Operator : YP/AJ
Sample : P1521-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CG-MW-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:17:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

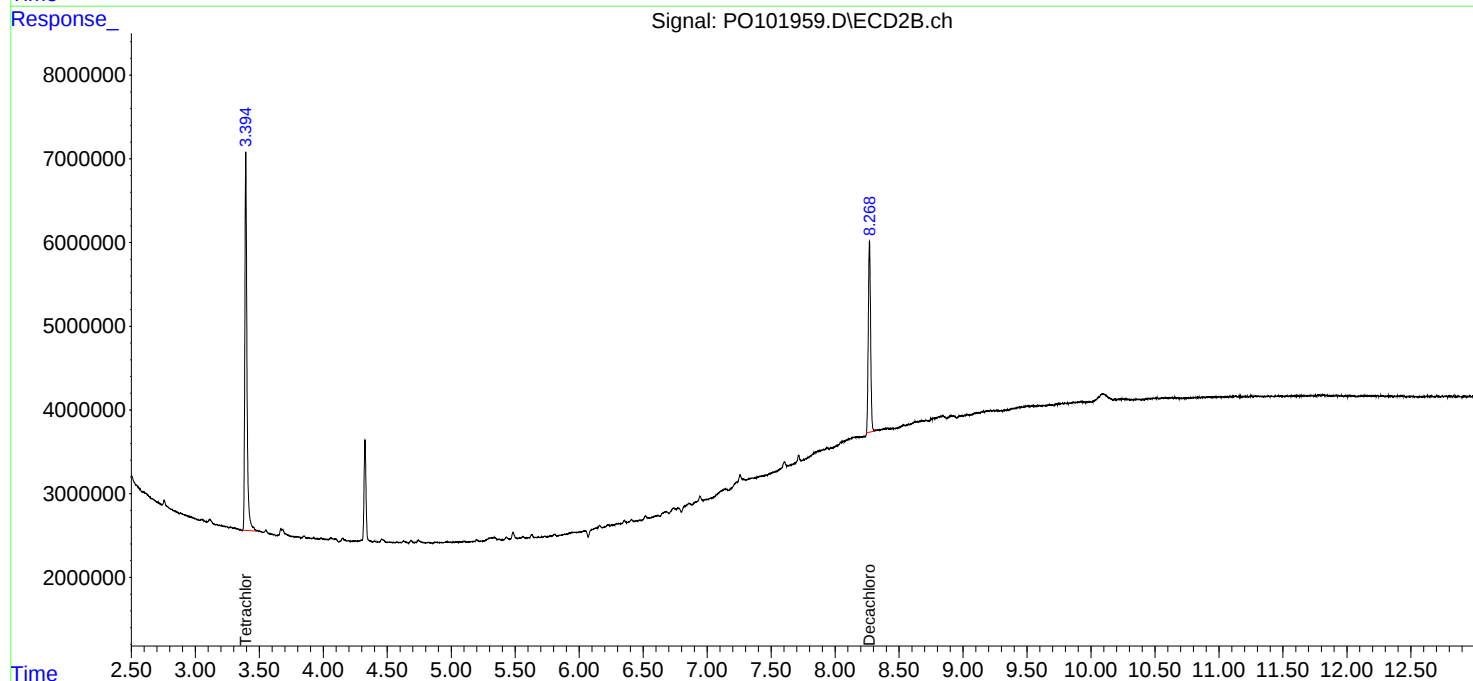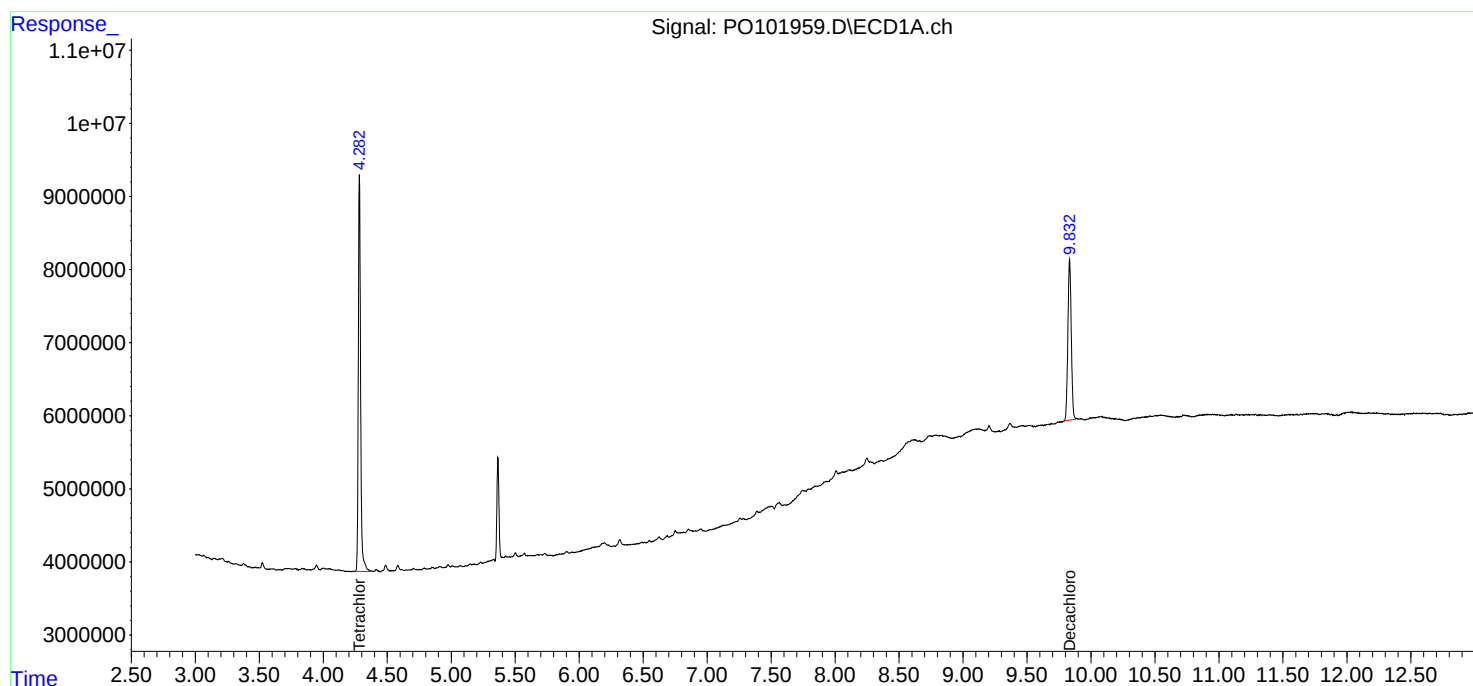

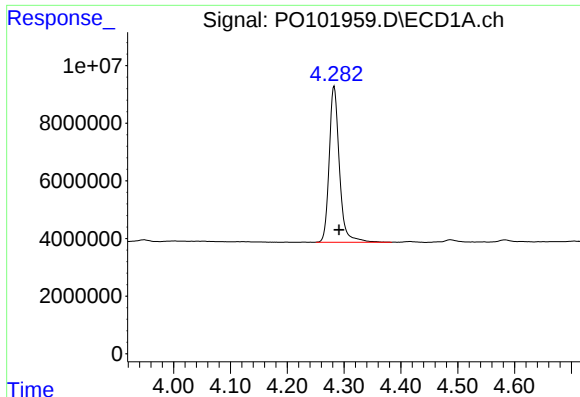

#1 Tetrachloro-m-xylene

R.T.: 4.283 min
Delta R.T.: -0.008 min
Response: 67521945
Conc: 21.90 ng/ml

Instrument :


ECD_O

ClientSampleId :

CG-MW-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

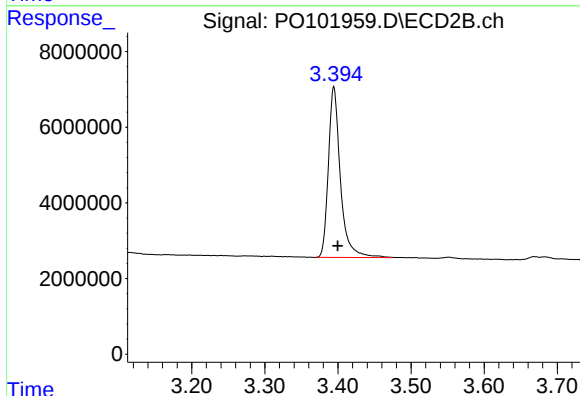


#1 Tetrachloro-m-xylene

R.T.: 3.394 min
Delta R.T.: -0.006 min
Response: 51514206
Conc: 19.38 ng/ml m

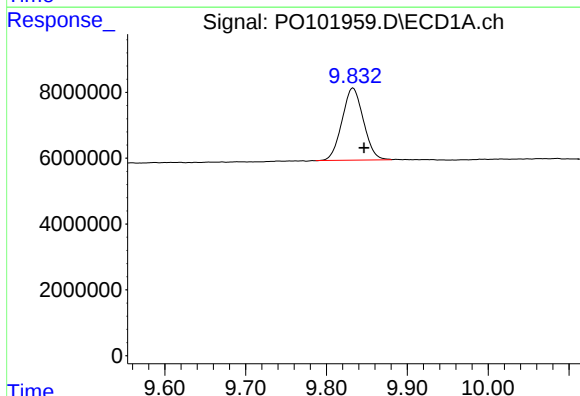

#2 Decachlorobiphenyl

R.T.: 9.832 min
Delta R.T.: -0.014 min
Response: 40217583
Conc: 19.18 ng/ml m

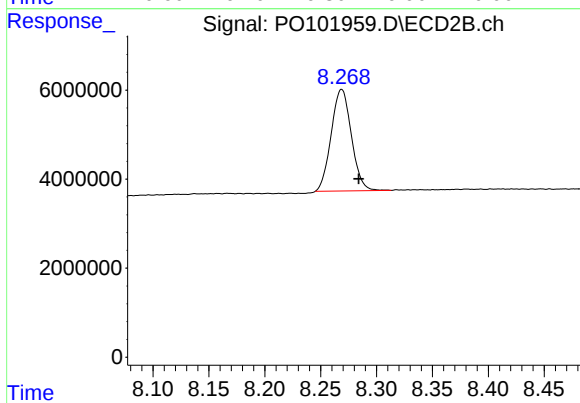

#2 Decachlorobiphenyl

R.T.: 8.269 min
Delta R.T.: -0.015 min
Response: 28728024
Conc: 15.12 ng/ml