

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022219\
 Data File : P0054021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2019 23:57
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:19:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.059	3.138	46722406	5803310	15.579	21.748 #
2) SA Decachlor...	9.401	7.718	24177888	5159454	19.254	17.218
Target Compounds						
20) L4 AR-1242-5	6.154	0.000	1677406	0	45.983	N.D. #
24) L5 AR-1248-4	6.026	0.000	715379	0	11.438	N.D. #
25) L5 AR-1248-5	6.154	0.000	1677406	0	27.723	N.D. #
26) L6 AR-1254-1	6.026	0.000	715379	0	4.529	N.D. #
30) L6 AR-1254-5	7.259	5.992	2665752	1620610	14.884	33.445 #
36) L8 AR-1262-1	0.000	5.992	0	1620610	N.D.	68.073 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022219\
Data File : P0054021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 23:57
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:19:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

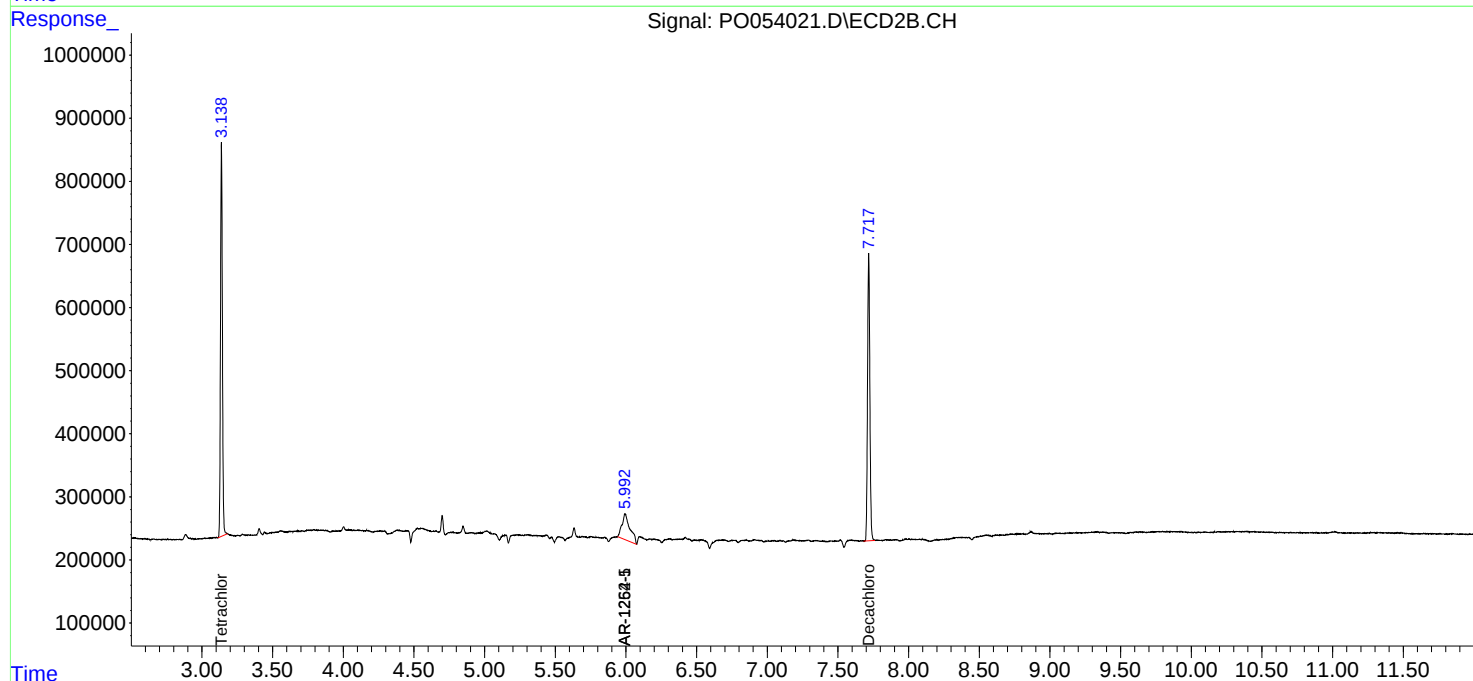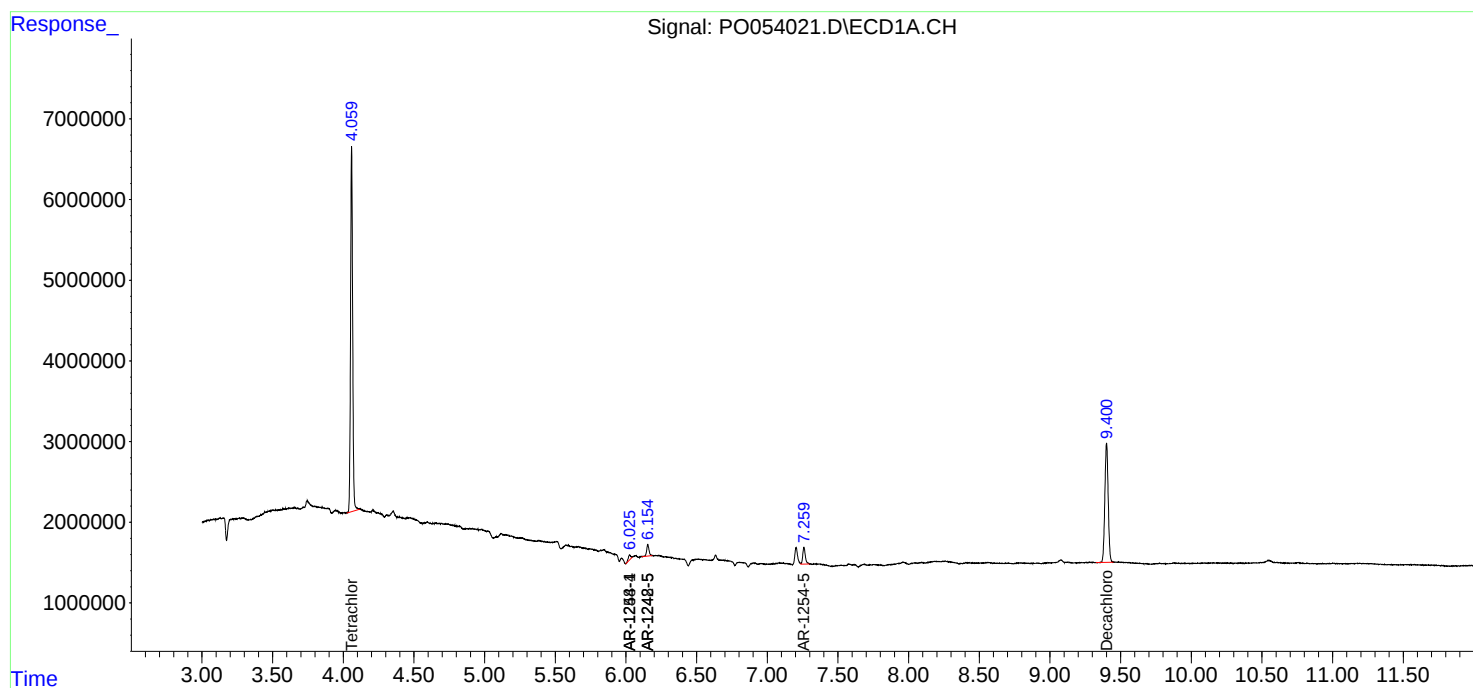


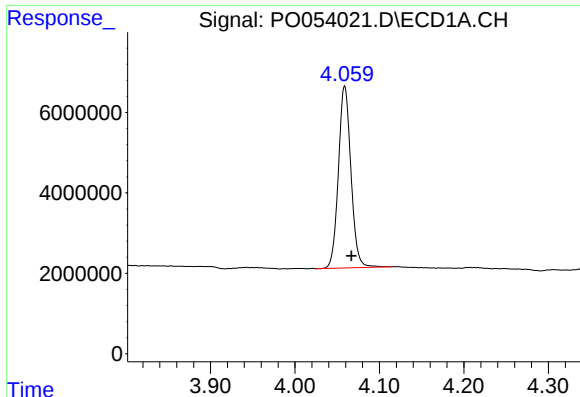

#1 Tetrachloro-m-xylene


R.T.: 4.059 min
Delta R.T.: -0.008 min
Response: 46722406
Conc: 15.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

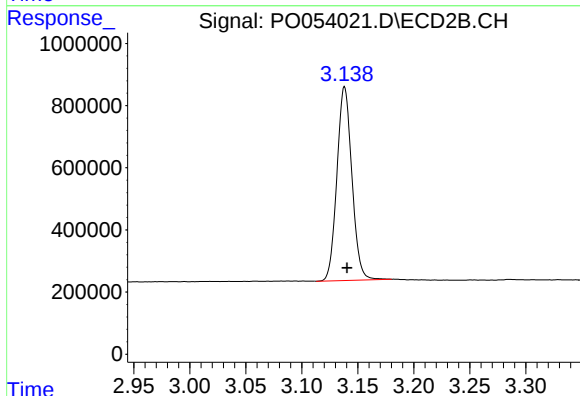


#1 Tetrachloro-m-xylene

R.T.: 3.138 min
Delta R.T.: -0.002 min
Response: 5803310
Conc: 21.75 ng/ml

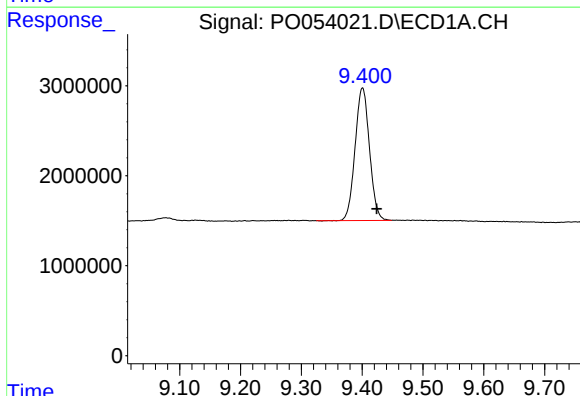


#2 Decachlorobiphenyl

R.T.: 9.401 min
Delta R.T.: -0.023 min
Response: 24177888
Conc: 19.25 ng/ml

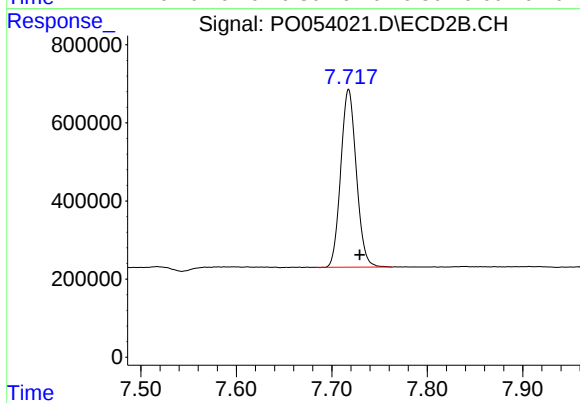

#2 Decachlorobiphenyl


R.T.: 7.718 min
Delta R.T.: -0.012 min
Response: 5159454
Conc: 17.22 ng/ml

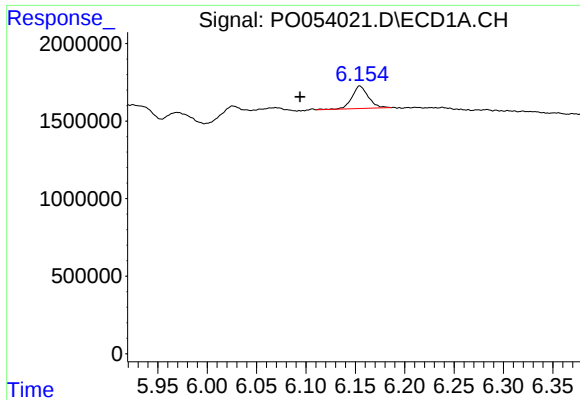

#20 AR-1242-5


R.T.: 6.154 min
Delta R.T.: 0.060 min
Response: 1677406
Conc: 45.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

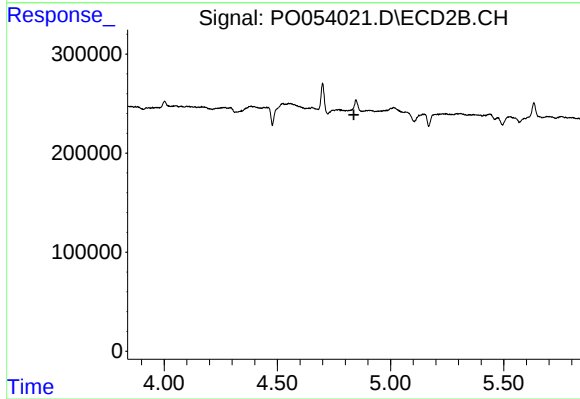


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 4.838 min
Response: 0
Conc: N.D.

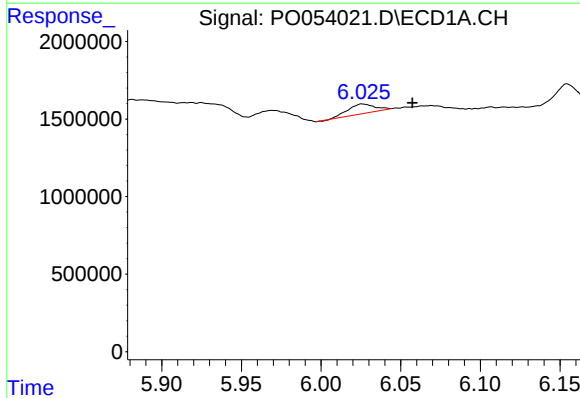


#24 AR-1248-4

R.T.: 6.026 min
Delta R.T.: -0.032 min
Response: 715379
Conc: 11.44 ng/ml

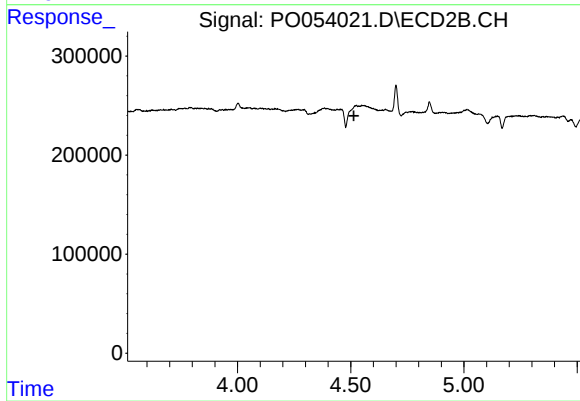

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.514 min
Response: 0
Conc: N.D.

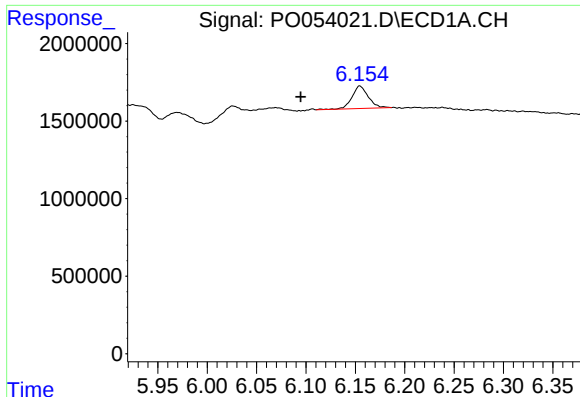

#25 AR-1248-5


R.T.: 6.154 min
Delta R.T.: 0.060 min
Response: 1677406
Conc: 27.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

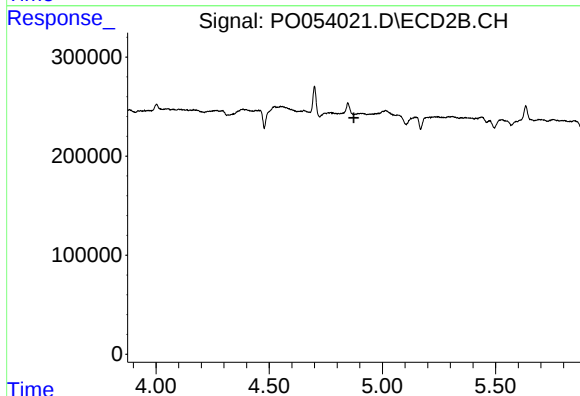


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 4.874 min
Response: 0
Conc: N.D.

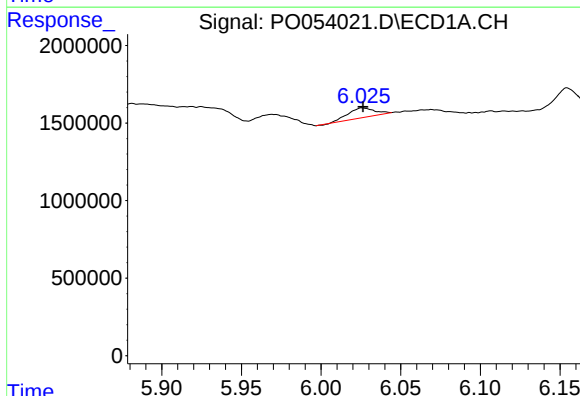


#26 AR-1254-1

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 715379
Conc: 4.53 ng/ml

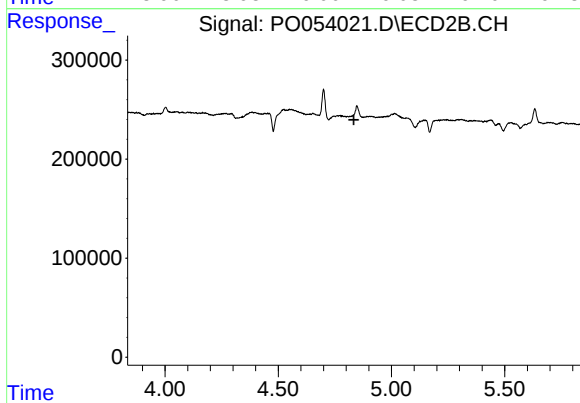

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 4.834 min
Response: 0
Conc: N.D.

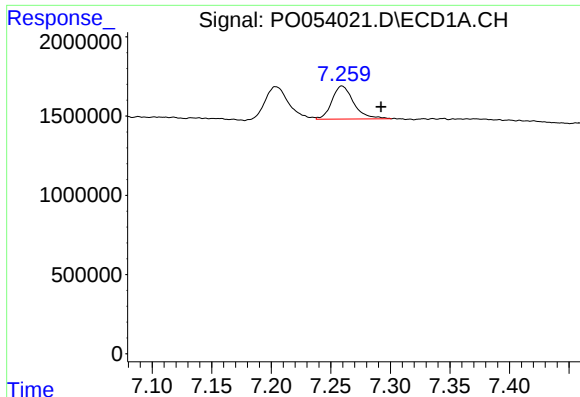

#30 AR-1254-5


R.T.: 7.259 min
Delta R.T.: -0.033 min
Response: 2665752
Conc: 14.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

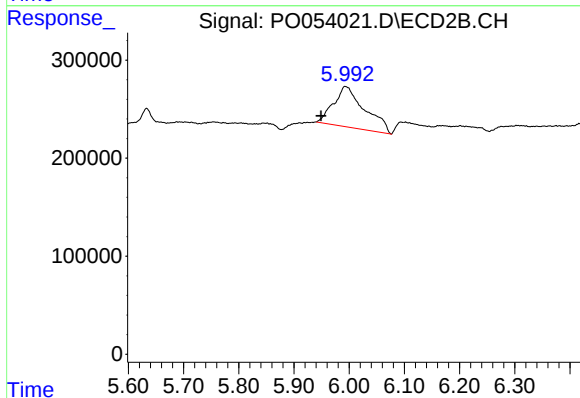


#30 AR-1254-5

R.T.: 5.992 min
Delta R.T.: 0.043 min
Response: 1620610
Conc: 33.44 ng/ml

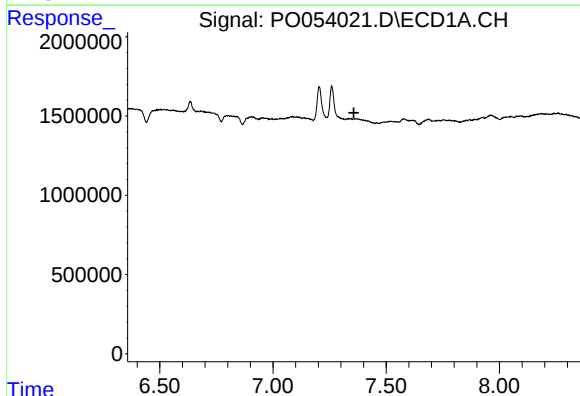

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

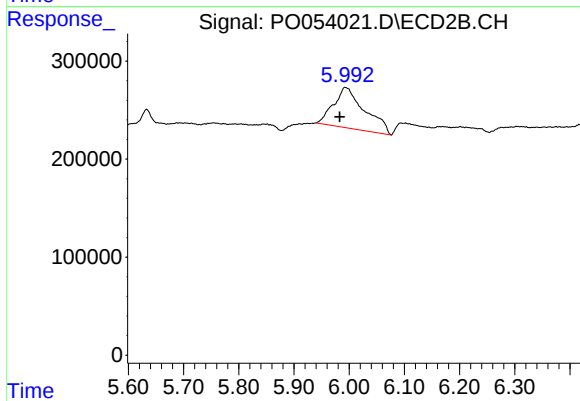

#36 AR-1262-1

R.T.: 5.992 min
Delta R.T.: 0.009 min
Response: 1620610
Conc: 68.07 ng/ml