

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022219\
Data File : P0054000.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 18:02
Operator : SM/SJ
Sample : K1567-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 21:51:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.059	3.139	68360026	6456549	22.794m	24.197
2) SA Decachlor...	9.409	7.726	28639235	9418866	22.807m	31.432 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022219\
Data File : P0054000.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 18:02
Operator : SM/SJ
Sample : K1567-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 21:51:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

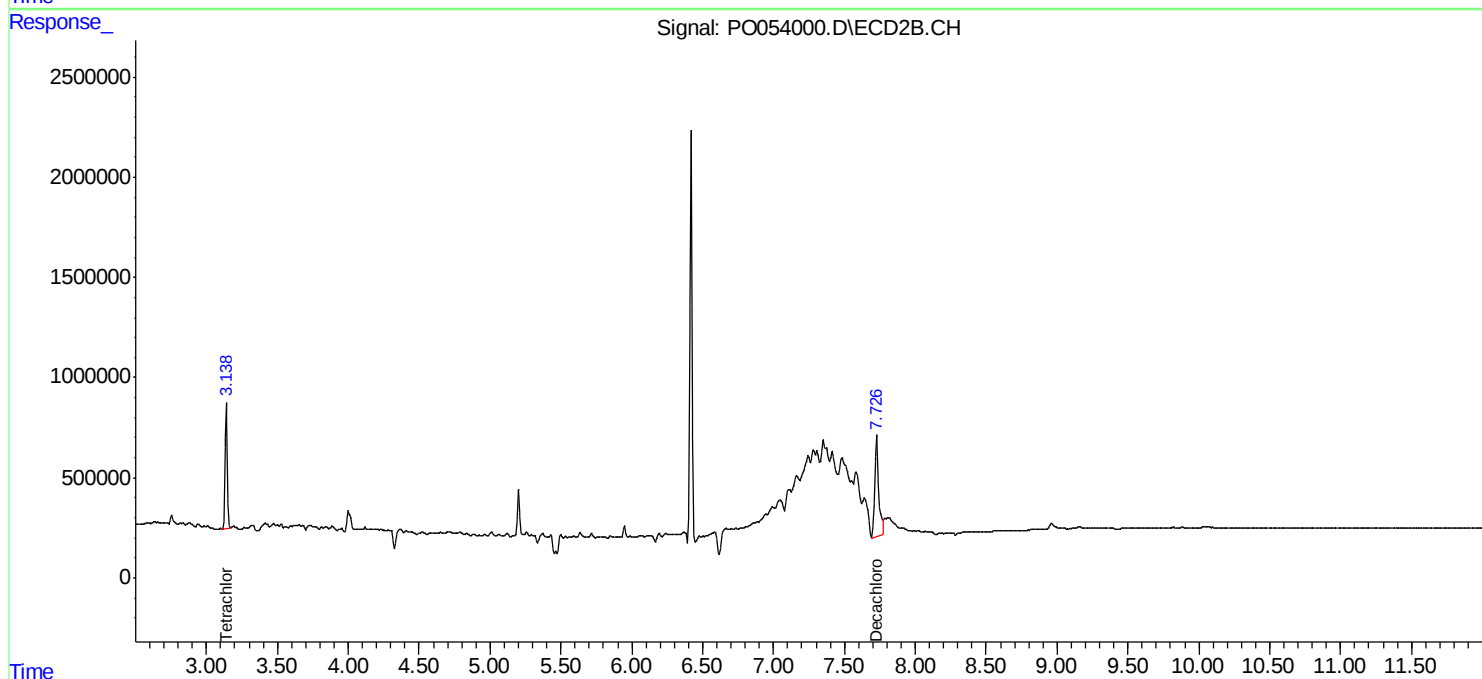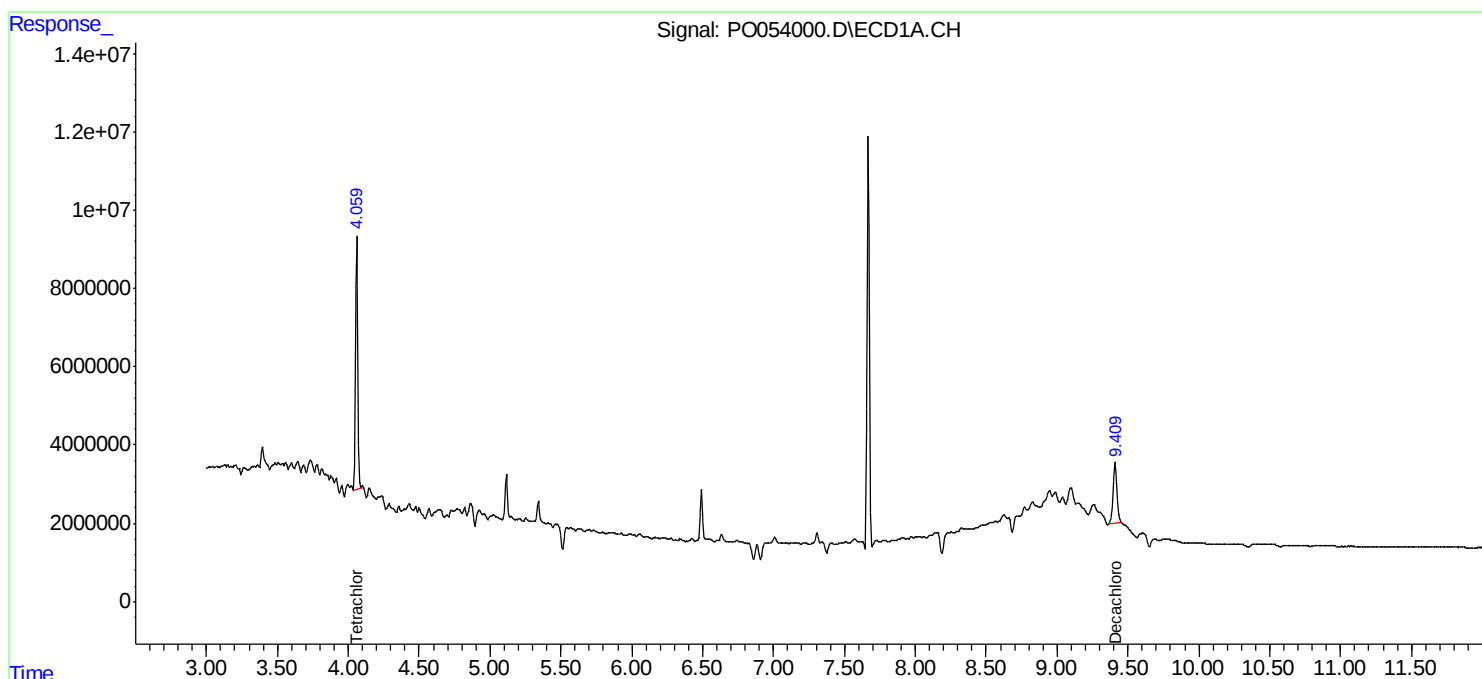


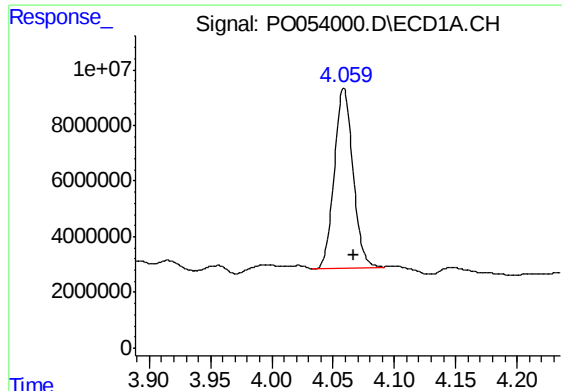

#1 Tetrachloro-m-xylene


R.T.: 4.059 min
Delta R.T.: -0.008 min
Response: 68360026
Conc: 22.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1

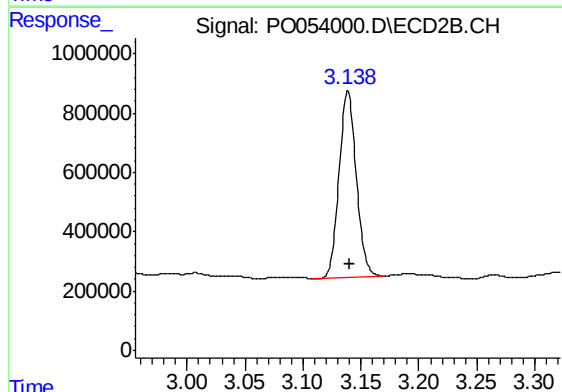


#1 Tetrachloro-m-xylene

R.T.: 3.139 min
Delta R.T.: -0.002 min
Response: 6456549
Conc: 24.20 ng/ml

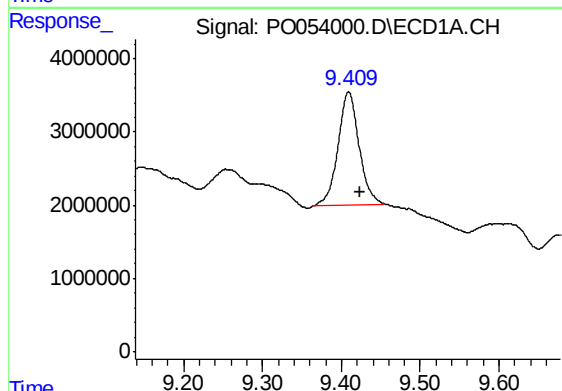

#2 Decachlorobiphenyl

R.T.: 9.409 min
Delta R.T.: -0.015 min
Response: 28639235
Conc: 22.81 ng/ml m

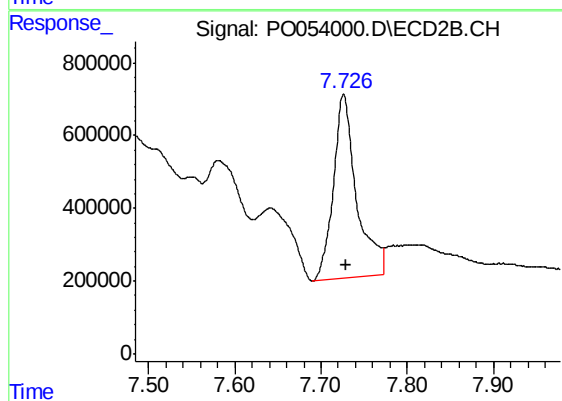

#2 Decachlorobiphenyl

R.T.: 7.726 min
Delta R.T.: -0.003 min
Response: 9418866
Conc: 31.43 ng/ml