

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022219\
Data File : P0054002.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 18:36
Operator : SM/SJ
Sample : K1572-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 21:52:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.059	3.138	10537805	965599	3.514	3.619
2) SA Decachlor...	9.402	7.718	3418025	925809	2.722	3.090

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022219\
Data File : P0054002.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2019 18:36
Operator : SM/SJ
Sample : K1572-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 21:52:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

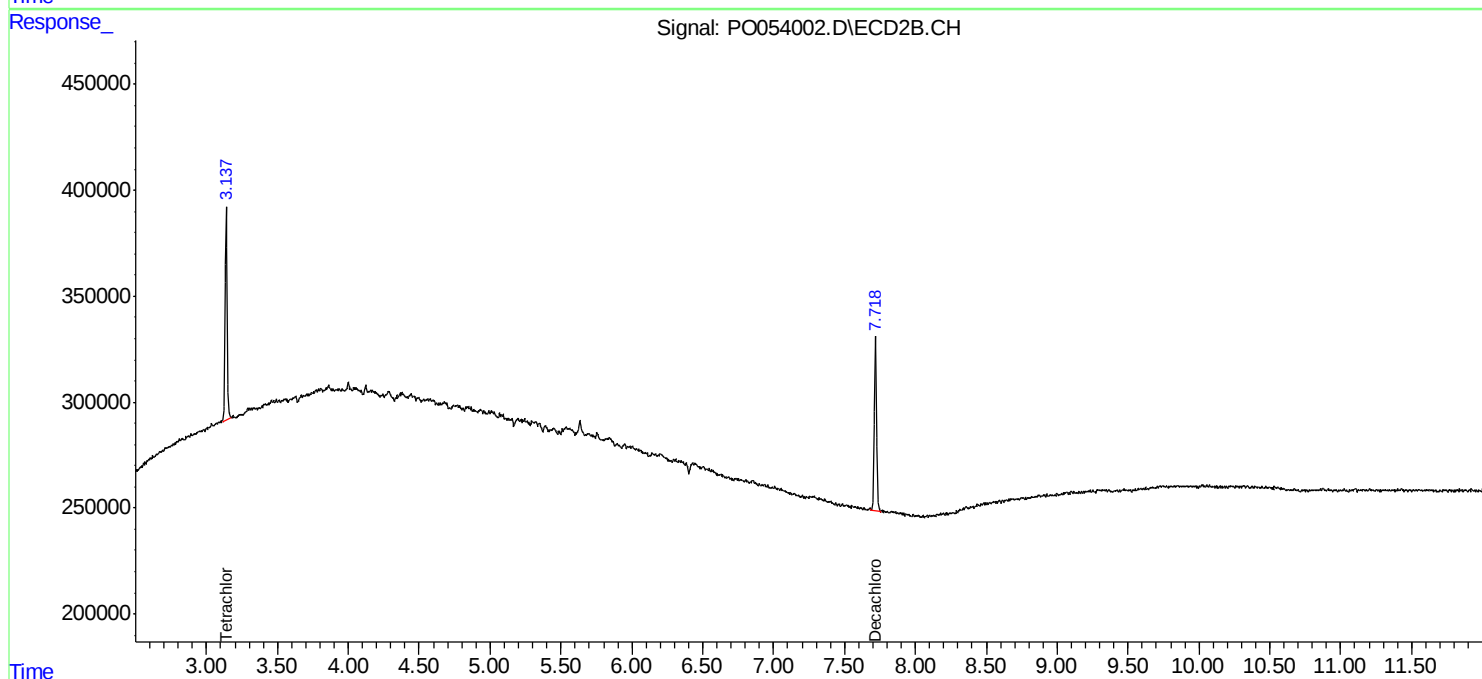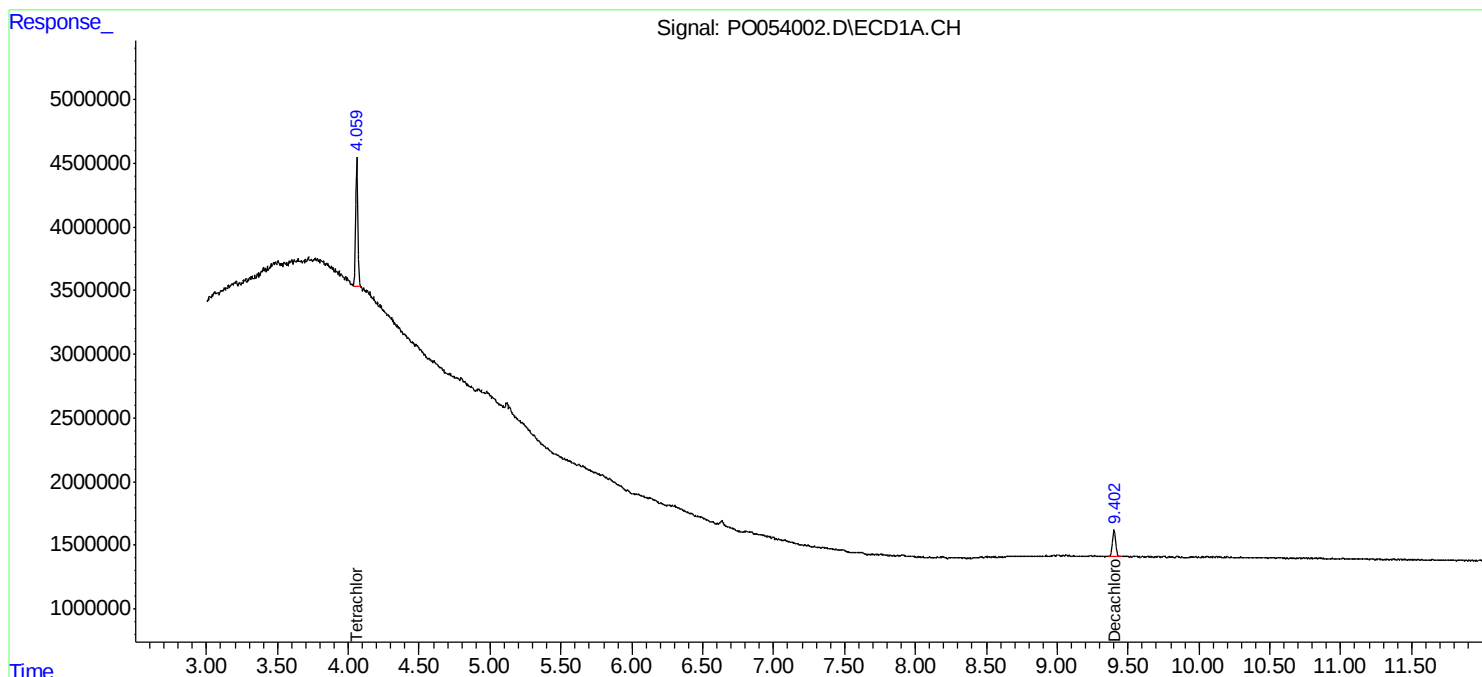


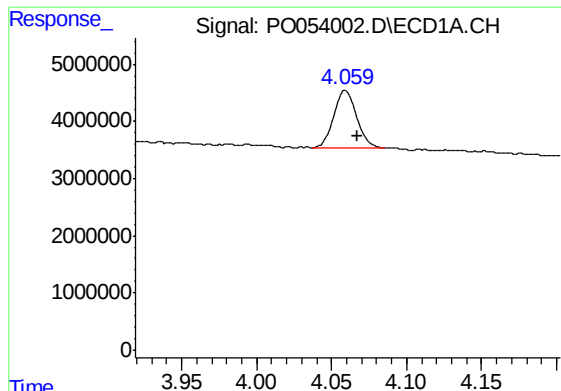

#1 Tetrachloro-m-xylene


R.T.: 4.059 min
Delta R.T.: -0.008 min
Response: 10537805
Conc: 3.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2

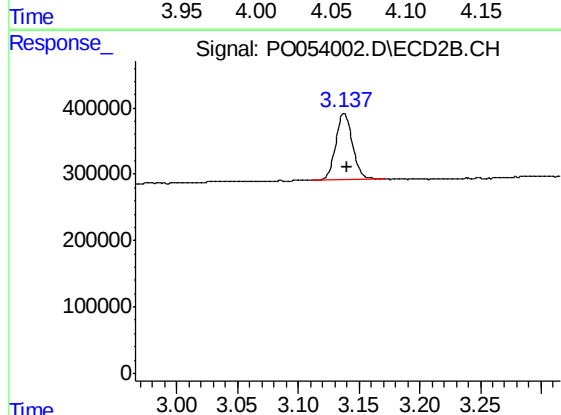


#1 Tetrachloro-m-xylene

R.T.: 3.138 min
Delta R.T.: -0.003 min
Response: 965599
Conc: 3.62 ng/ml

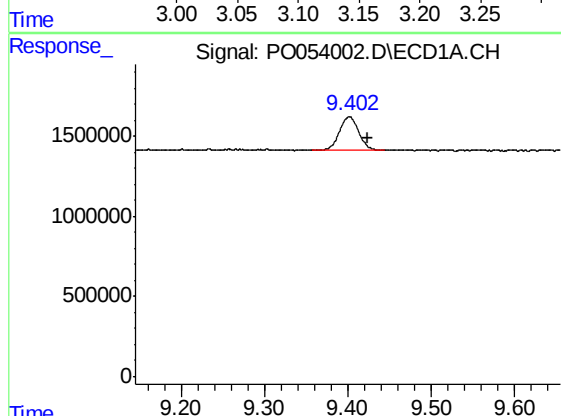

#2 Decachlorobiphenyl

R.T.: 9.402 min
Delta R.T.: -0.022 min
Response: 3418025
Conc: 2.72 ng/ml

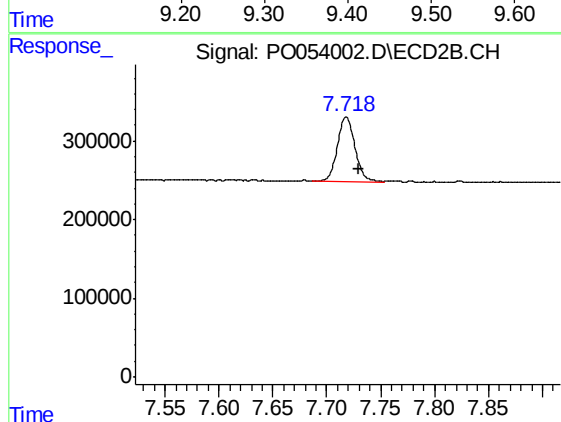

#2 Decachlorobiphenyl

R.T.: 7.718 min
Delta R.T.: -0.011 min
Response: 925809
Conc: 3.09 ng/ml