

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022221\
 Data File : P0075656.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Feb 2021 2:51
 Operator : AJ/MA
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022221

Manual Integrations
 APPROVED

Ankita
 2/23/2021 10:22:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 07:12:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 23 07:07:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.944	3.963	3317675	2236512	50.367	54.006
2) SA Decachlor...	10.992	9.257	2943324	2518973	50.079	51.799
Target Compounds						
26) L6 AR-1254-1	7.174	6.088	1263528	1342958	481.464	493.506
27) L6 AR-1254-2	7.404	6.248	1943539	1172439	475.521	490.532
28) L6 AR-1254-3	7.787	6.667	2062100	1919591	465.457	491.122
29) L6 AR-1254-4	8.085	6.906	1553331	1284542	477.165	494.208
30) L6 AR-1254-5	8.515	7.335	1659229	1768621	474.006m	497.925

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022221\
Data File : PO075656.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Feb 2021 2:51
Operator : AJ/MA
Sample : AR1254ICV500
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
ICVPO022221


Manual Integrations
APPROVED

Ankita
2/23/2021 10:22:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 07:12:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 23 07:07:50 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

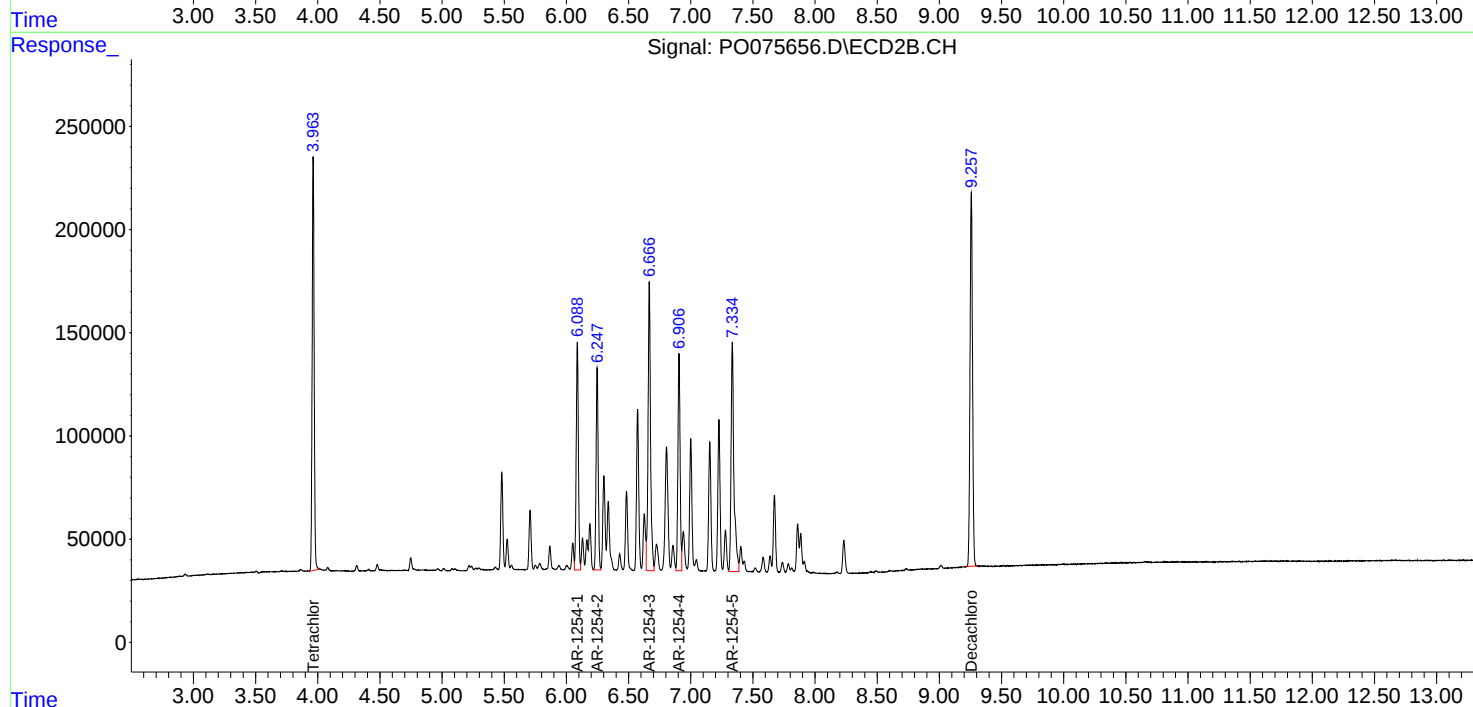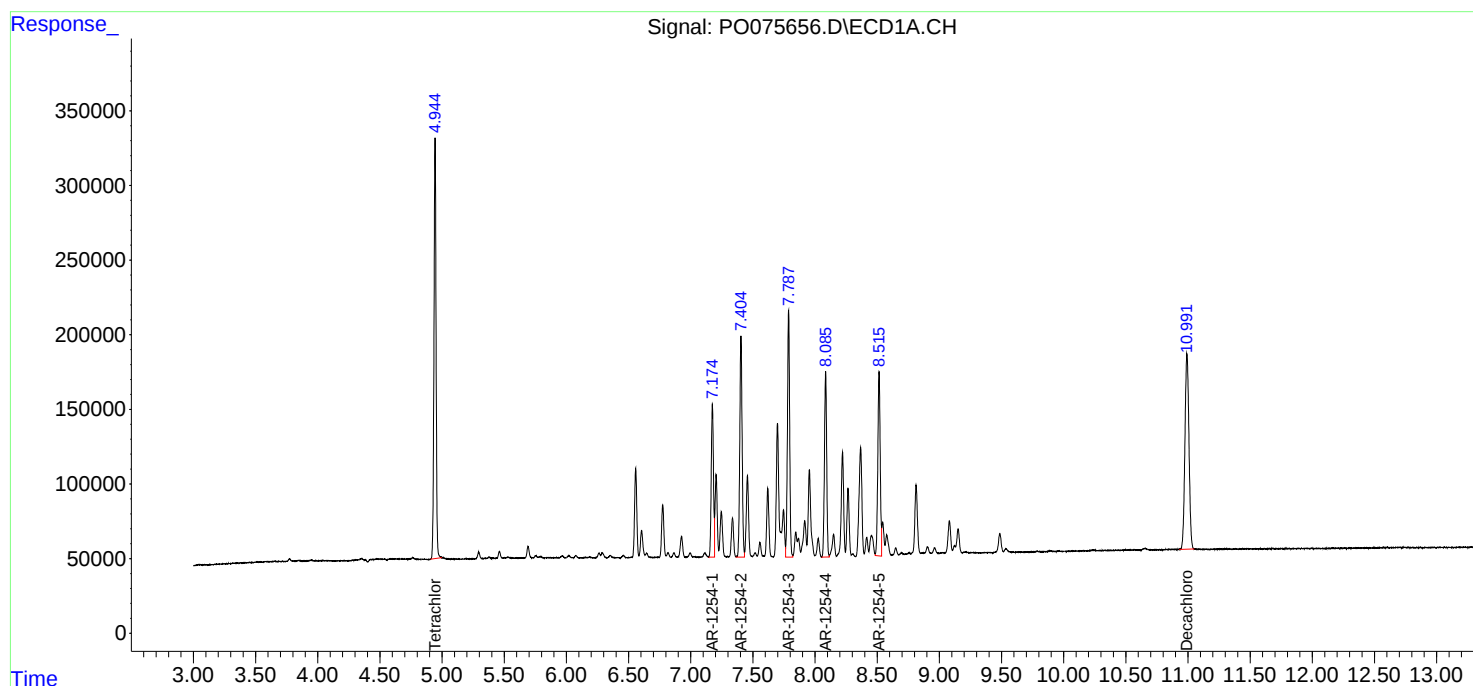

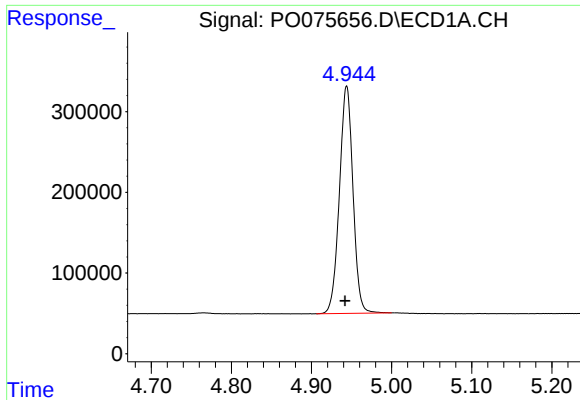


#1 Tetrachloro-m-xylene

R.T.: 4.944 min
Delta R.T.: 0.002 min
Response: 3317675
Conc: 50.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO022221


Manual Integrations
APPROVED

Ankita
2/23/2021 10:22:40 AM

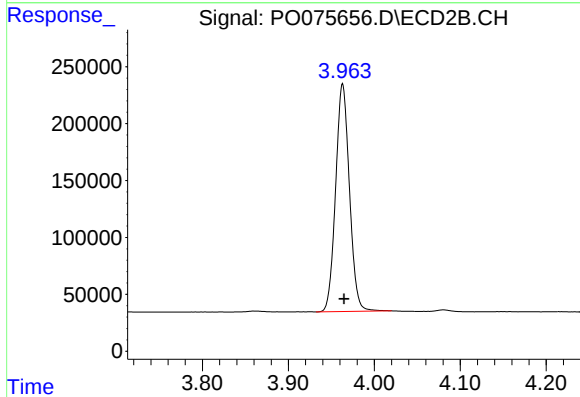


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.002 min
Response: 2236512
Conc: 54.01 ng/ml

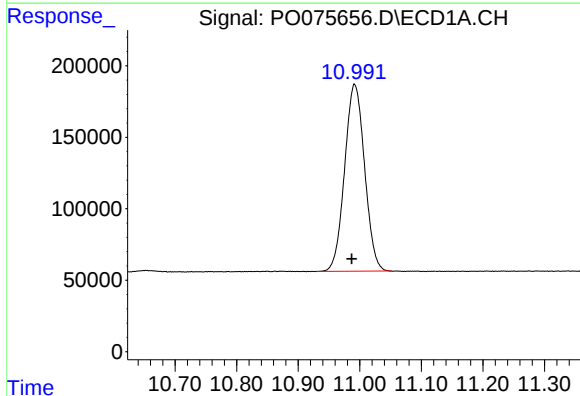


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: 0.005 min
Response: 2943324
Conc: 50.08 ng/ml

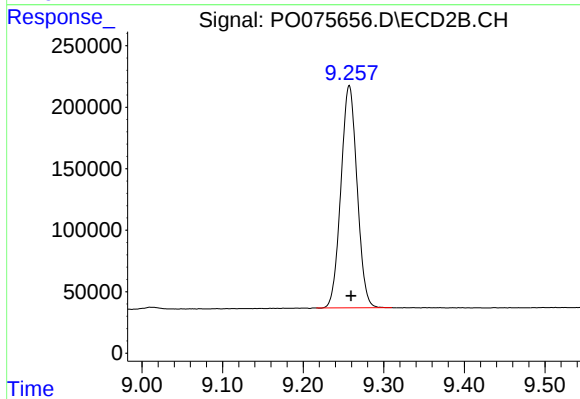

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.002 min
Response: 2518973
Conc: 51.80 ng/ml

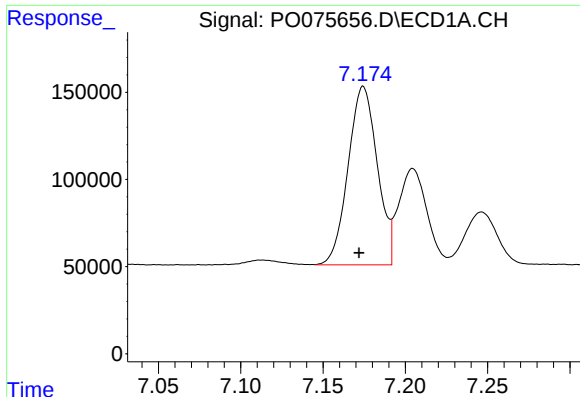


#26 AR-1254-1

R.T.: 7.174 min
Delta R.T.: 0.003 min
Response: 1263528
Conc: 481.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO022221


Manual Integrations
APPROVED

Ankita
2/23/2021 10:22:40 AM

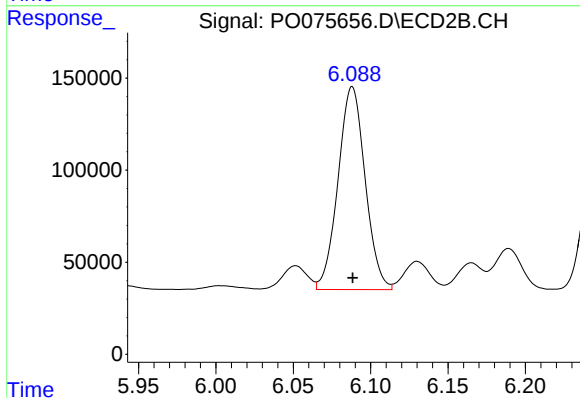


#26 AR-1254-1

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 1342958
Conc: 493.51 ng/ml

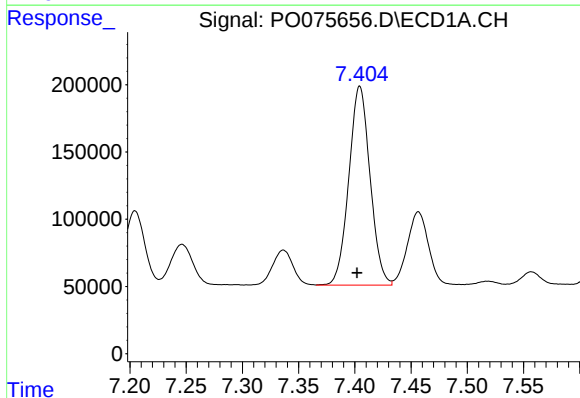


#27 AR-1254-2

R.T.: 7.404 min
Delta R.T.: 0.002 min
Response: 1943539
Conc: 475.52 ng/ml

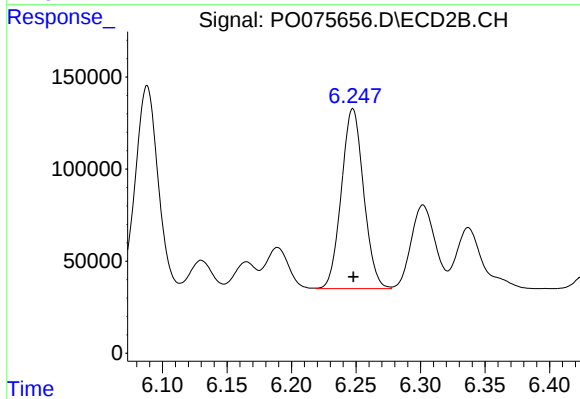

#27 AR-1254-2

R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 1172439
Conc: 490.53 ng/ml

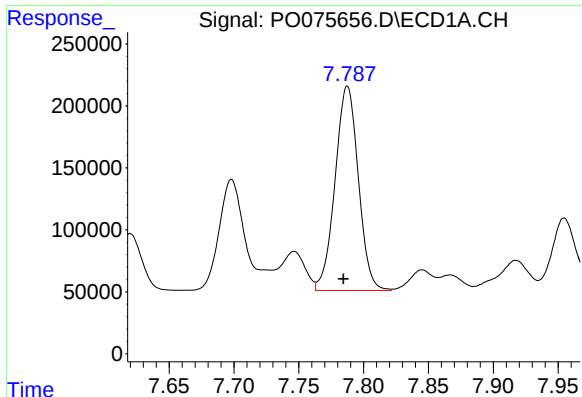


#28 AR-1254-3

R.T.: 7.787 min
Delta R.T.: 0.003 min
Response: 2062100
Conc: 465.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO022221


Manual Integrations
APPROVED

Ankita
2/23/2021 10:22:40 AM

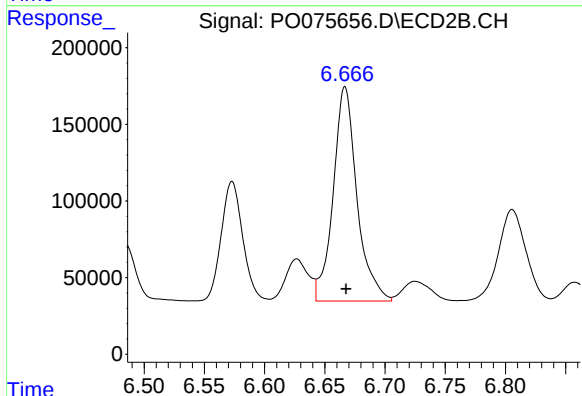


#28 AR-1254-3

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 1919591
Conc: 491.12 ng/ml

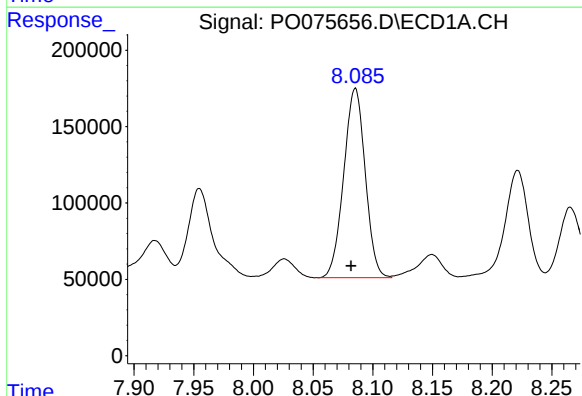


#29 AR-1254-4

R.T.: 8.085 min
Delta R.T.: 0.003 min
Response: 1553331
Conc: 477.17 ng/ml

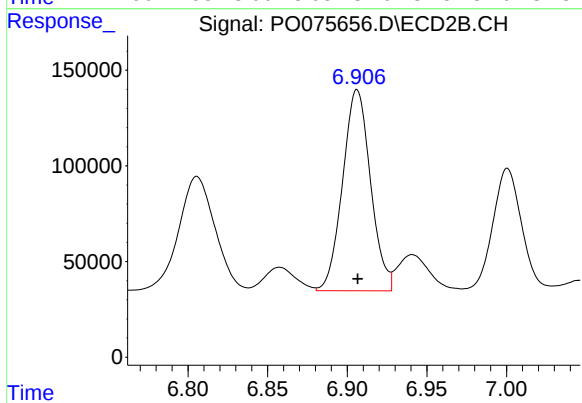

#29 AR-1254-4

R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 1284542
Conc: 494.21 ng/ml

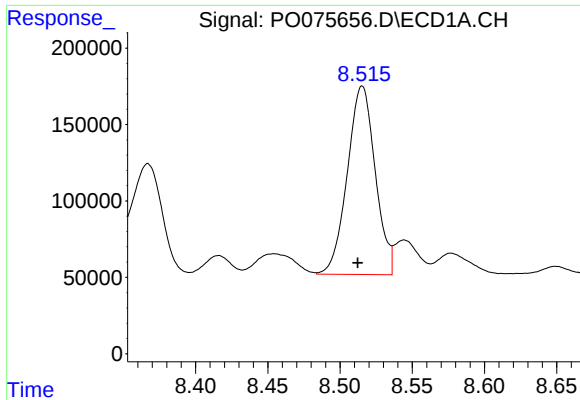


#30 AR-1254-5

R.T.: 8.515 min
Delta R.T.: 0.003 min
Response: 1659229
Conc: 474.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ICVPO022221

Manual Integrations
APPROVED

Ankita
2/23/2021 10:22:40 AM

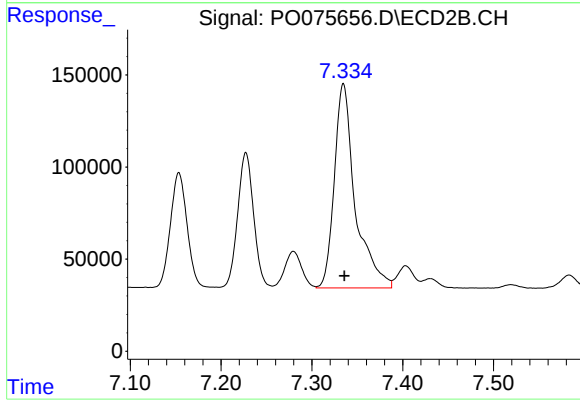

#30 AR-1254-5

R.T.: 7.335 min
Delta R.T.: -0.001 min
Response: 1768621
Conc: 497.92 ng/ml