

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022222\
 Data File : P0084815.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2022 10:17
 Operator : YP\AJ
 Sample : N1611-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WATER-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 16:18:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.598	4750499	911322	24.161	20.207
2) SA Decachlor...	10.428	8.621	2608795	629407	21.024	17.266

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022222\
Data File : PO084815.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2022 10:17
Operator : YP\AJ
Sample : N1611-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 16:18:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

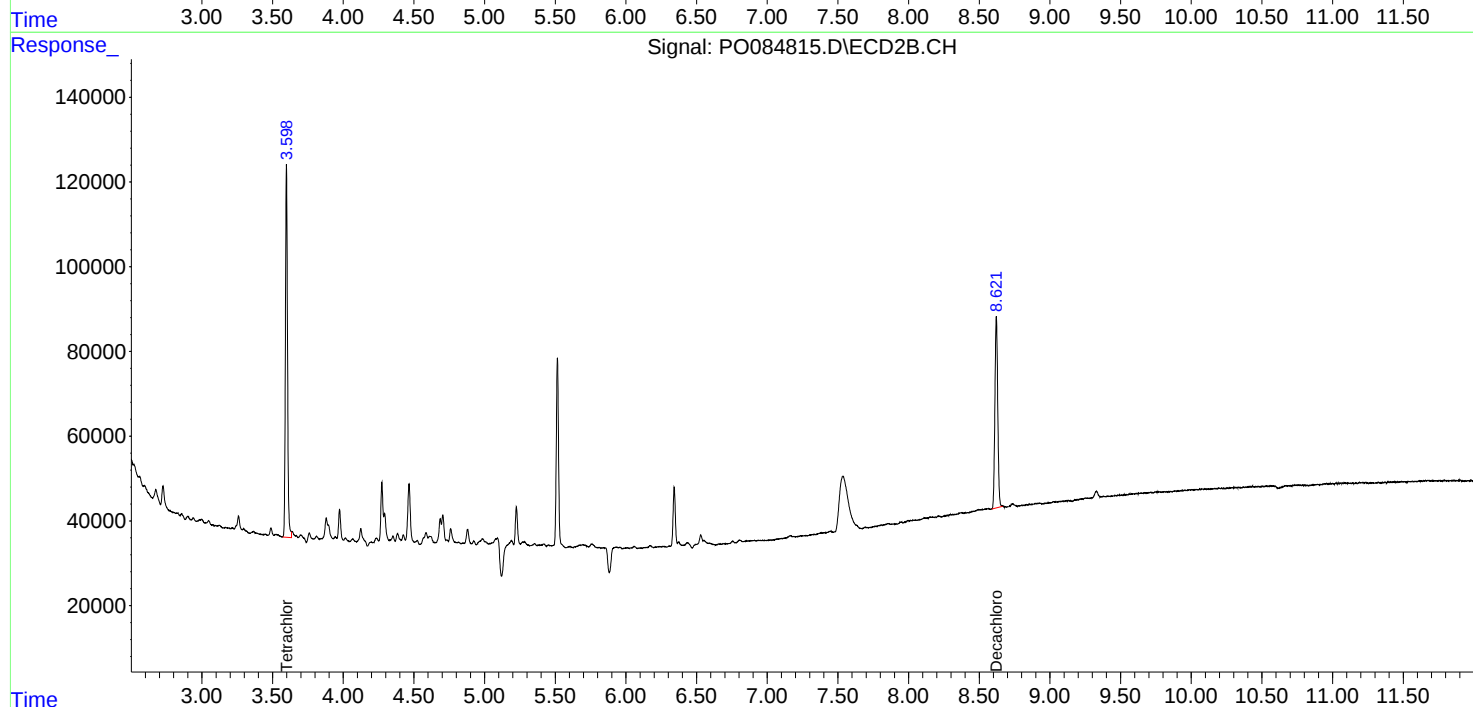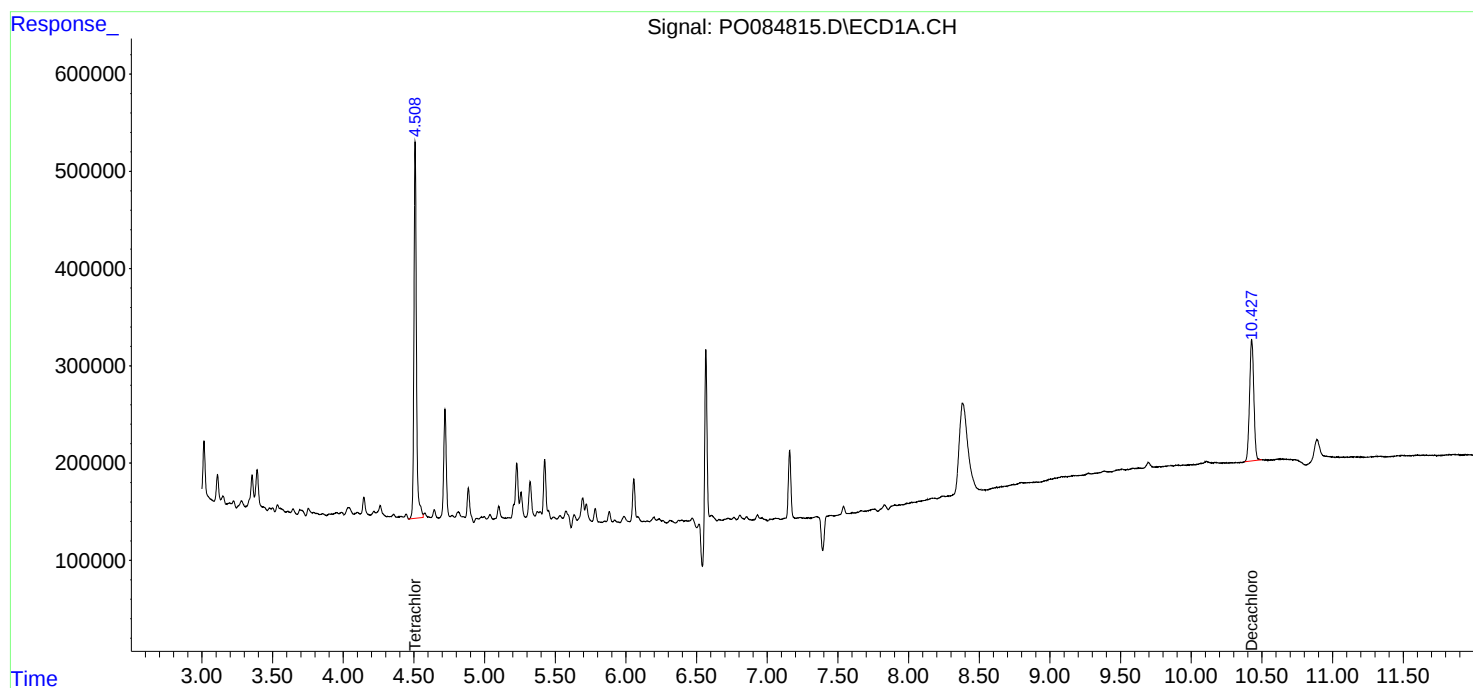


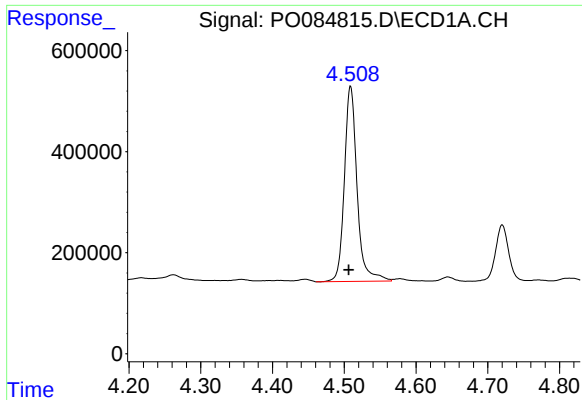

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 4750499
Conc: 24.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-COMP

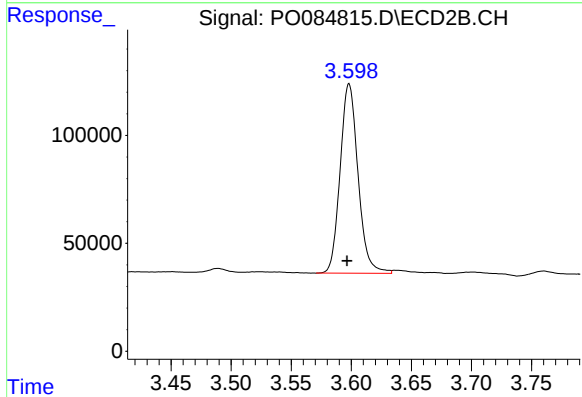


#1 Tetrachloro-m-xylene

R.T.: 3.598 min
Delta R.T.: 0.002 min
Response: 911322
Conc: 20.21 ng/ml

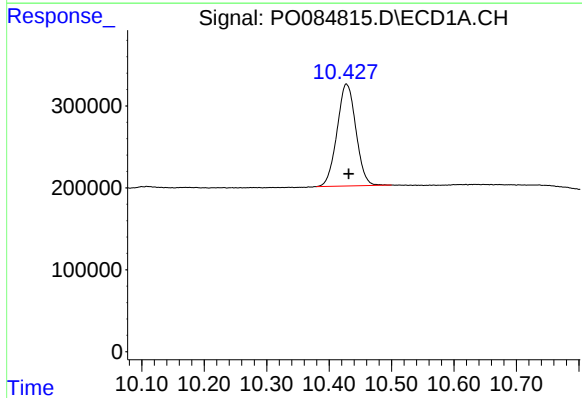

#2 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: -0.004 min
Response: 2608795
Conc: 21.02 ng/ml

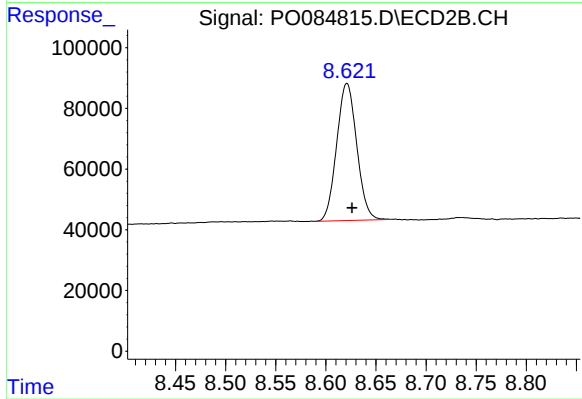

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: -0.005 min
Response: 629407
Conc: 17.27 ng/ml