

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022222\
 Data File : P0084829.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2022 14:25
 Operator : YP\AJ
 Sample : N1626-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CC-A8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 04:45:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.509	3.597	3307242	862557	16.820	19.126
2)	SA Decachlor...	10.429	8.622	2476165	589610	19.955	16.174

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022222\
Data File : PO084829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2022 14:25
Operator : YP\AJ
Sample : N1626-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CC-A8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 04:45:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

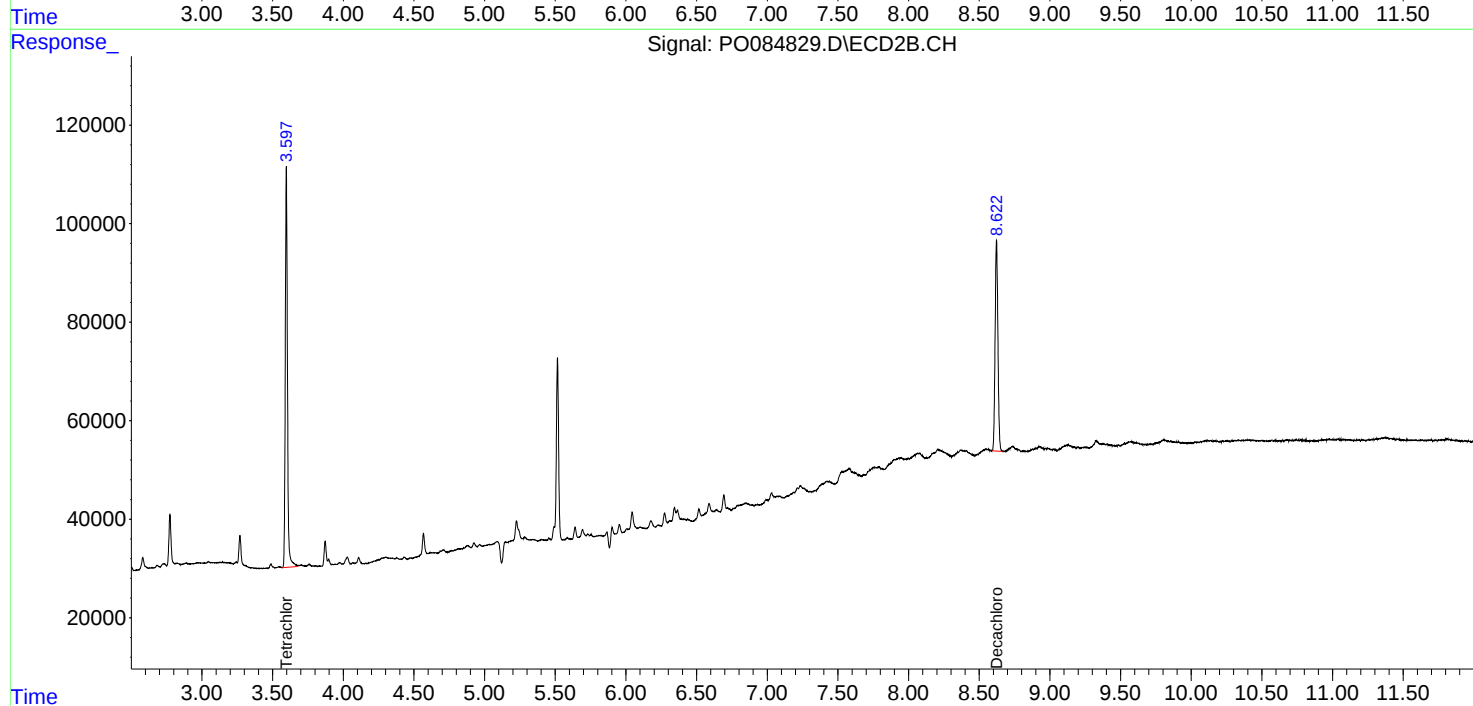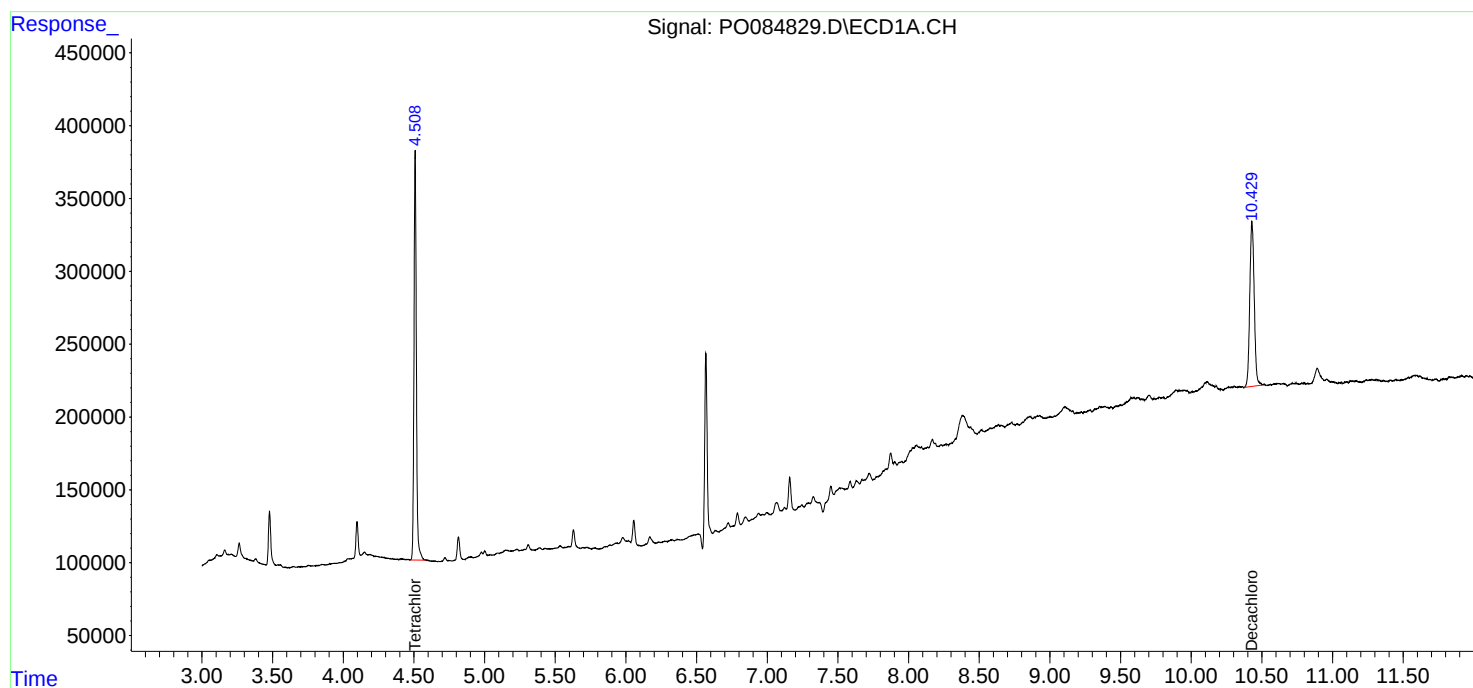


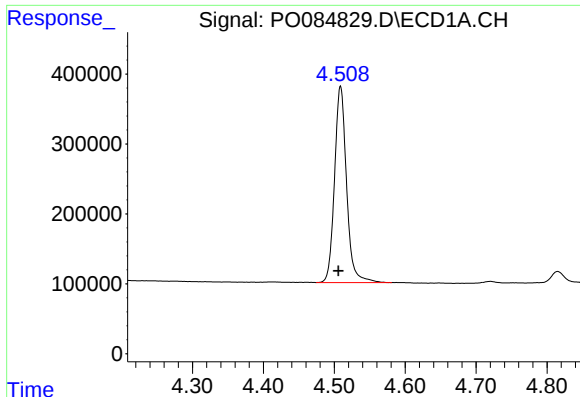

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 3307242
Conc: 16.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC-A8

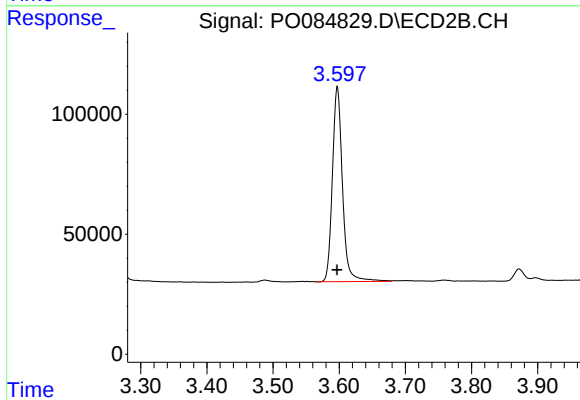


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.000 min
Response: 862557
Conc: 19.13 ng/ml

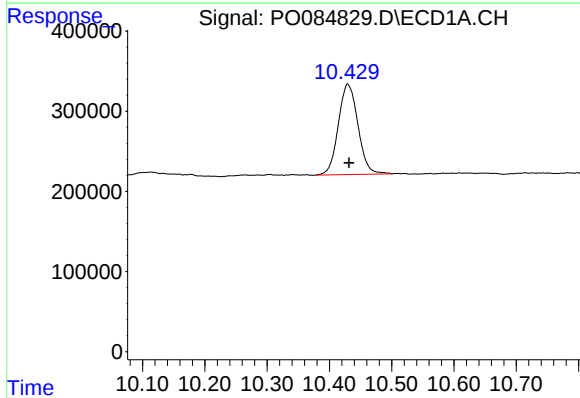

#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: -0.002 min
Response: 2476165
Conc: 19.95 ng/ml

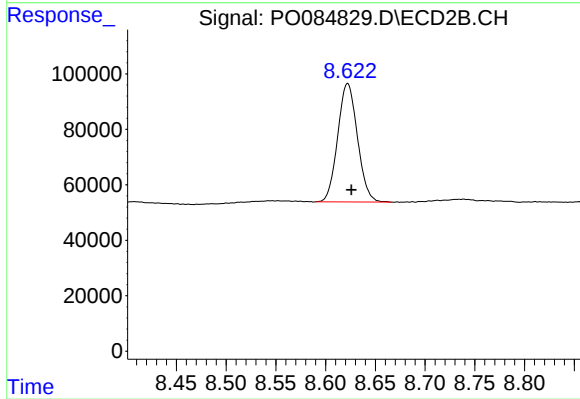

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.004 min
Response: 589610
Conc: 16.17 ng/ml