

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022222\
 Data File : P0084853.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2022 21:59
 Operator : YP\AJ
 Sample : N1630-03 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/23/2022
 Supervised By :Ankita Jodhani 02/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:57:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.597	492901	101955	2.507	2.261
2) SA Decachlor...	10.434	8.623	238455	86218	1.922m	2.365m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022222\
Data File : P0084853.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2022 21:59
Operator : YP\AJ
Sample : N1630-03 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:57:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

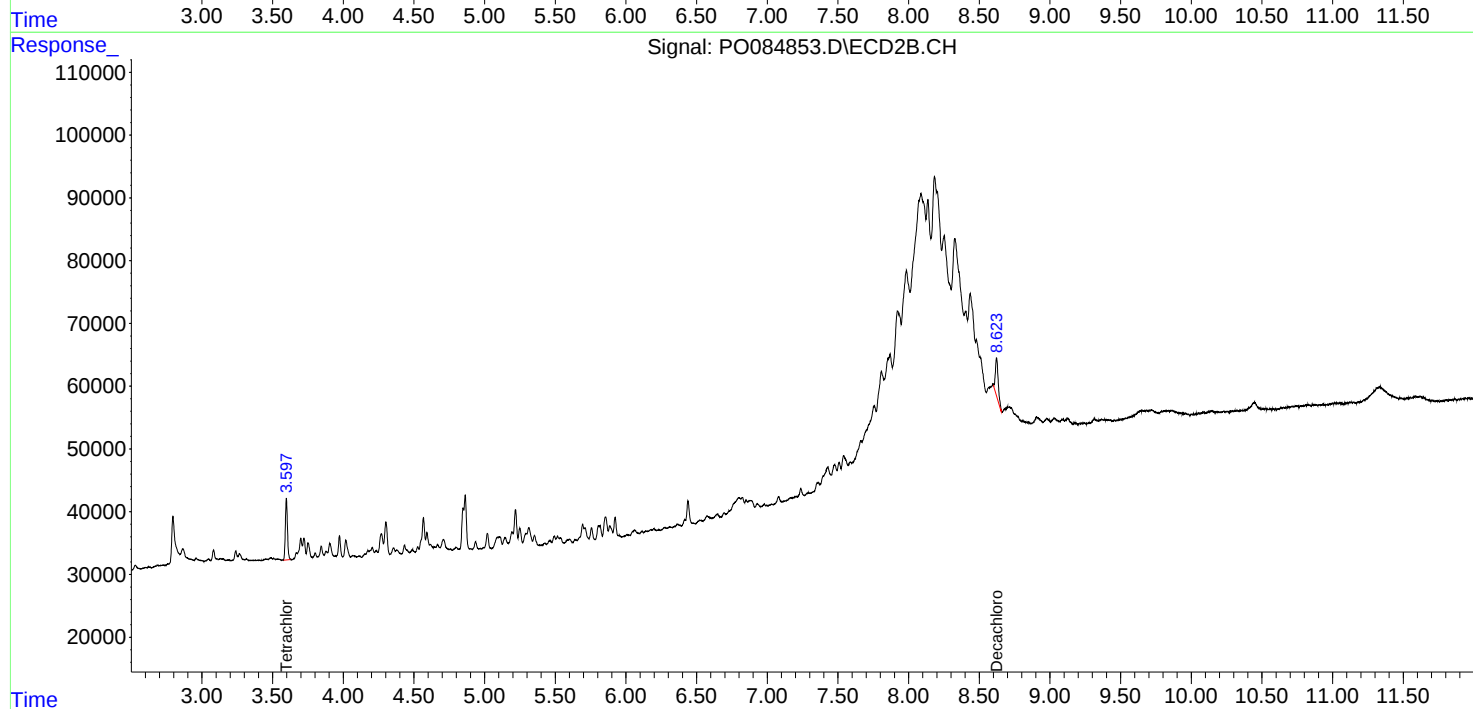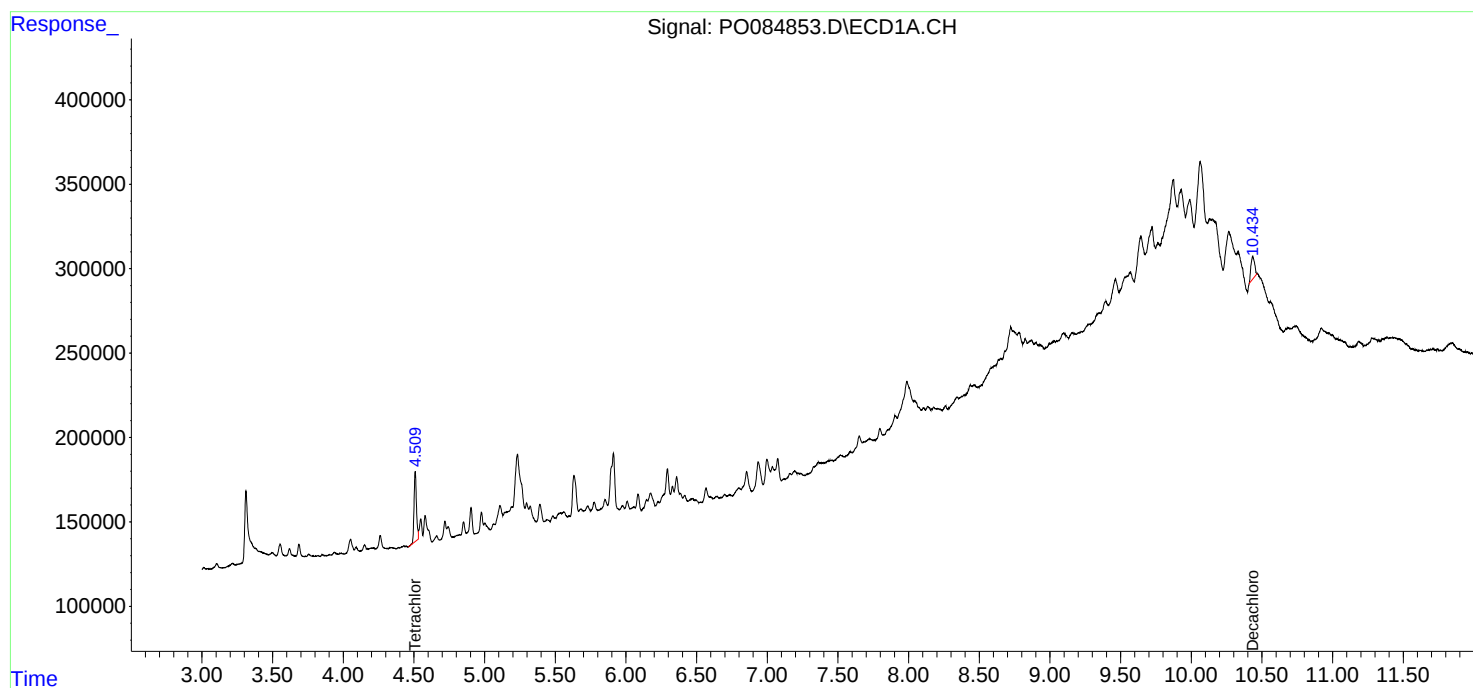

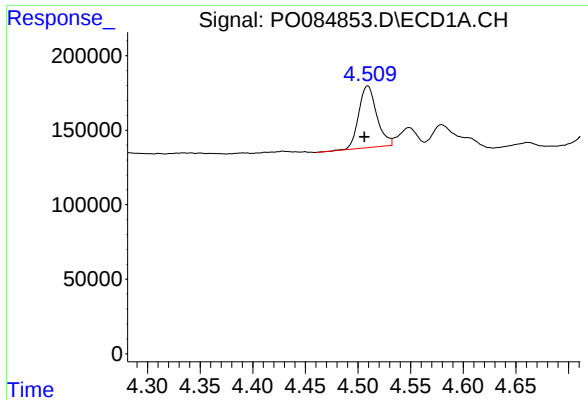


#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 492901
Conc: 2.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

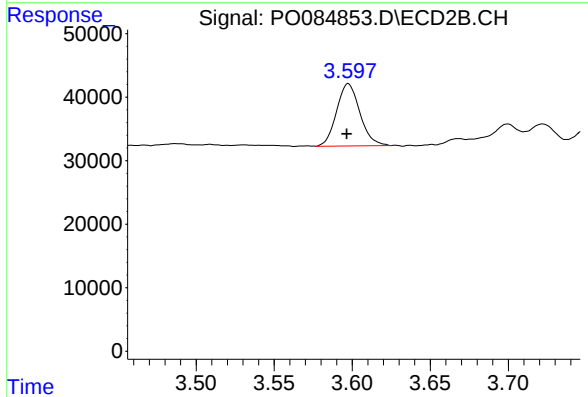


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.000 min
Response: 101955
Conc: 2.26 ng/ml

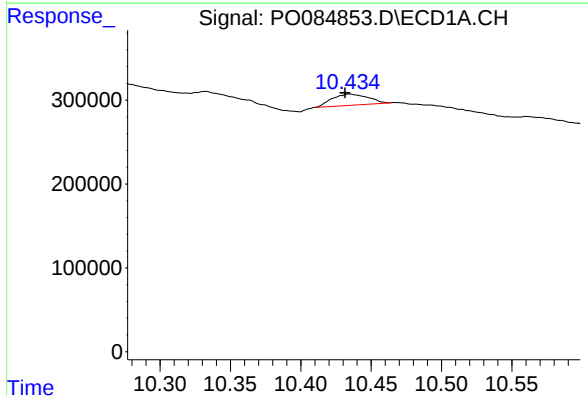

#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.002 min
Response: 238455
Conc: 1.92 ng/ml m

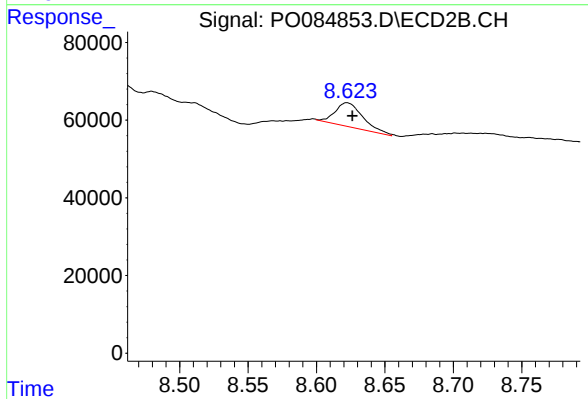

#2 Decachlorobiphenyl

R.T.: 8.623 min
Delta R.T.: -0.003 min
Response: 86218
Conc: 2.37 ng/ml m