

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
 Data File : P0075692.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Feb 2021 23:45
 Operator : AJ/MA
 Sample : M1467-02 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 01:16:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 23 07:07:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.943	3.963	176113	103806	2.674	2.507
2)	SA Decachlor...	10.992	9.253	139258	124438	2.369	2.559
Target Compounds							
28)	L6 AR-1254-3	7.802f	0.000	126729	0	28.605	N.D. #
30)	L6 AR-1254-5	8.516	0.000	23159	0	6.616	N.D. #
33)	L7 AR-1260-3	0.000	7.151	0	32436	N.D.	11.505 #
34)	L7 AR-1260-4	8.813	0.000	11373	0	3.487	N.D. #
35)	L7 AR-1260-5	0.000	7.874	0	46477	N.D.	7.883 #
37)	L8 AR-1262-2	0.000	7.874	0	46477	N.D.	6.934 #
39)	L8 AR-1262-4	0.000	8.209f	0	45996	N.D.	9.106 #
42)	L9 AR-1268-2	0.000	8.209f	0	45996	N.D.	6.557 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022321\
Data File : PO075692.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Feb 2021 23:45
Operator : AJ/MA
Sample : M1467-02 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 01:16:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 23 07:07:50 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

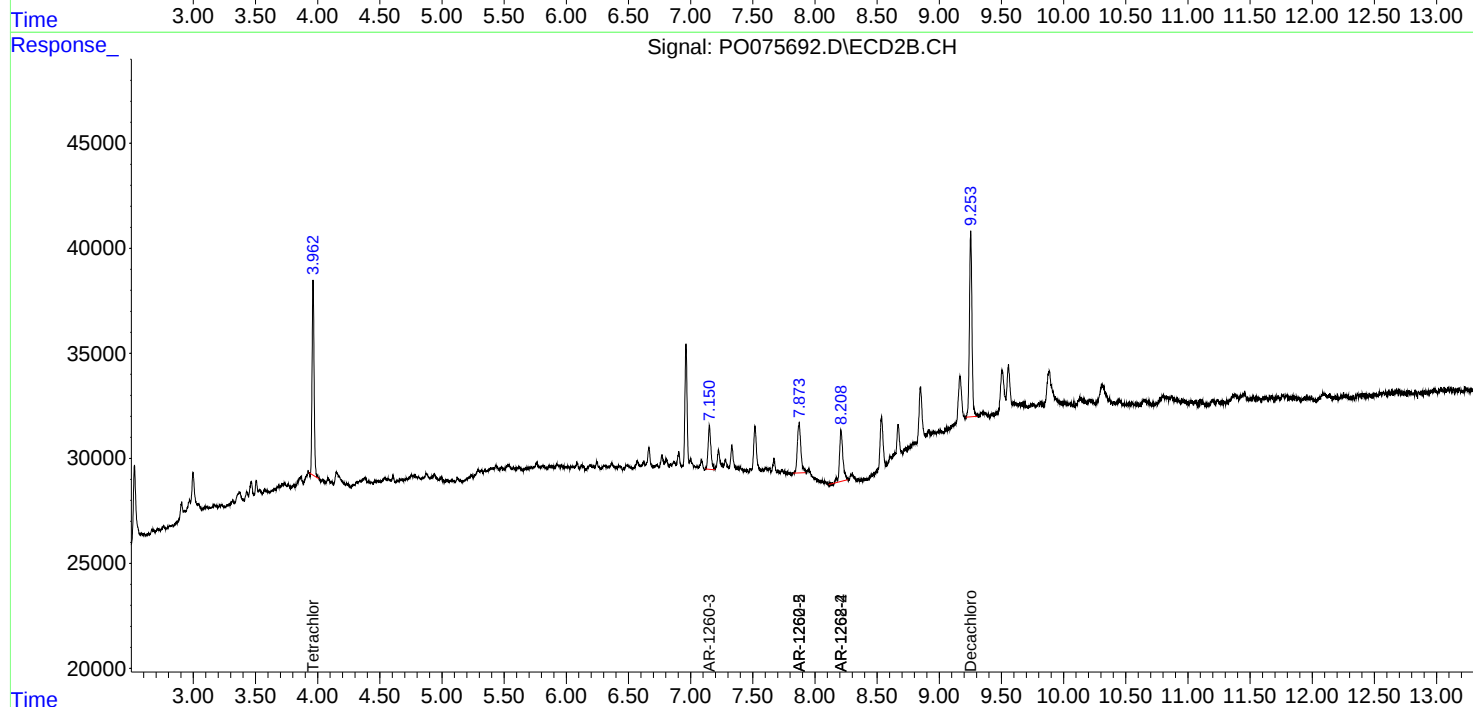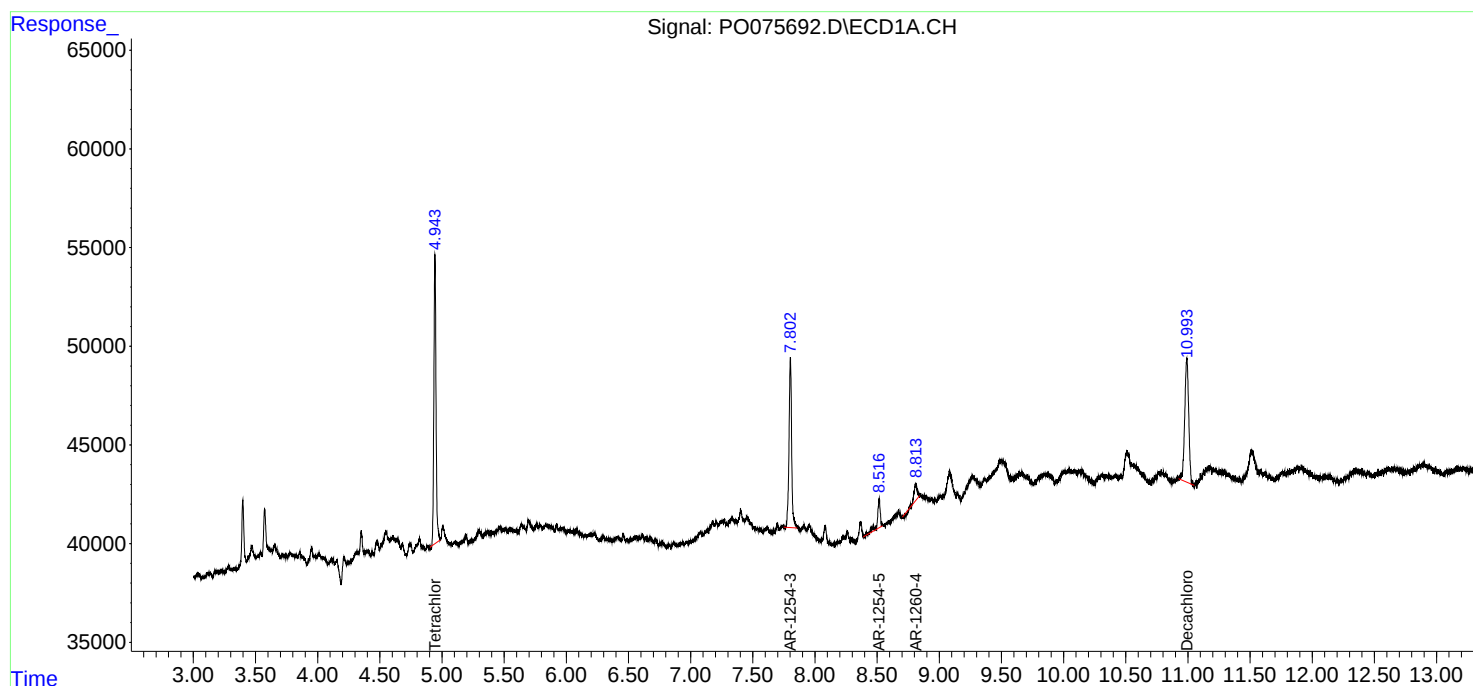


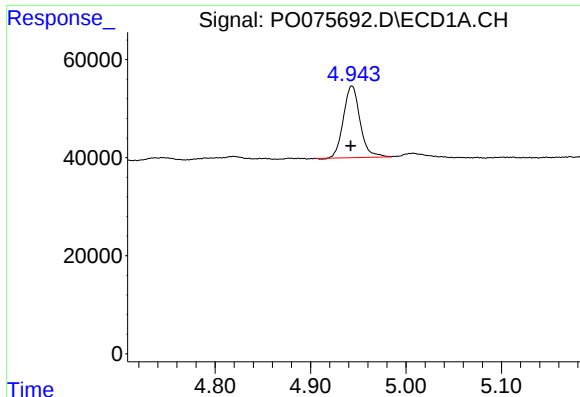

#1 Tetrachloro-m-xylene


R.T.: 4.943 min
Delta R.T.: 0.001 min
Response: 176113
Conc: 2.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

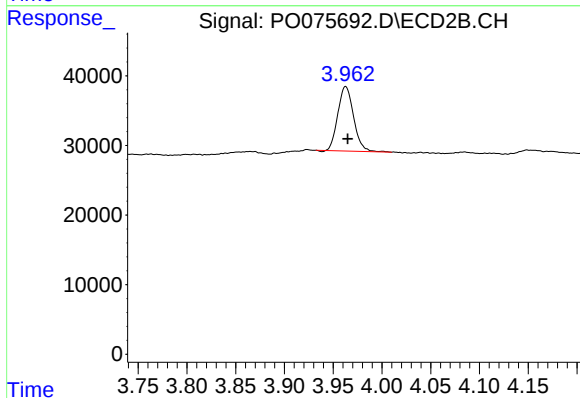


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.002 min
Response: 103806
Conc: 2.51 ng/ml

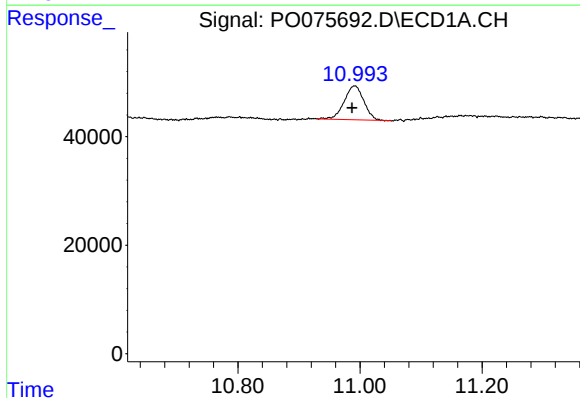


#2 Decachlorobiphenyl

R.T.: 10.992 min
Delta R.T.: 0.005 min
Response: 139258
Conc: 2.37 ng/ml

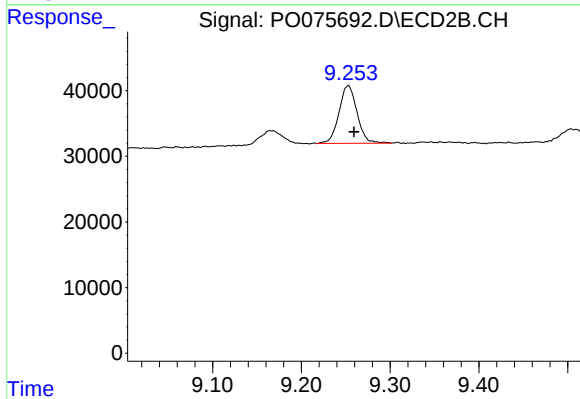

#2 Decachlorobiphenyl


R.T.: 9.253 min
Delta R.T.: -0.007 min
Response: 124438
Conc: 2.56 ng/ml

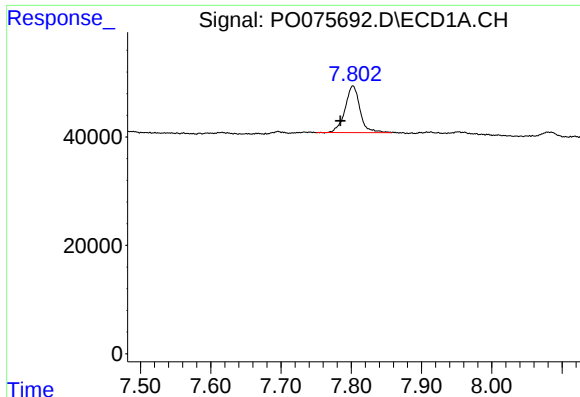

#28 AR-1254-3


R.T.: 7.802 min
Delta R.T.: 0.018 min
Response: 126729
Conc: 28.61 ng/ml

Instrument :
ECD_O
ClientSampleId :

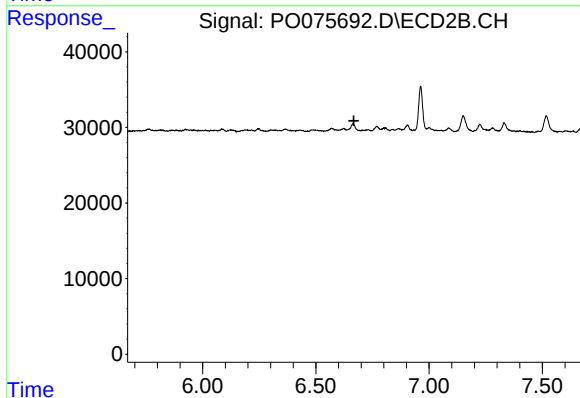


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.668 min
Response: 0
Conc: N.D.

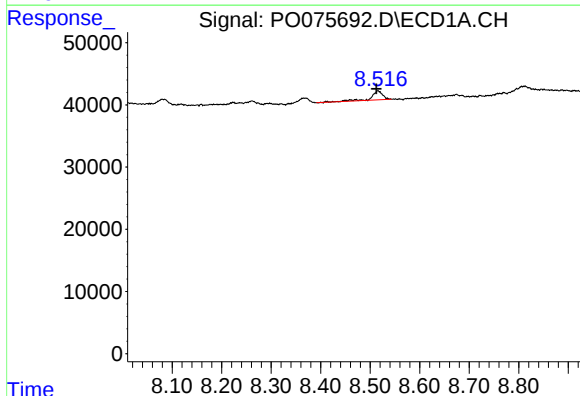


#30 AR-1254-5

R.T.: 8.516 min
Delta R.T.: 0.003 min
Response: 23159
Conc: 6.62 ng/ml

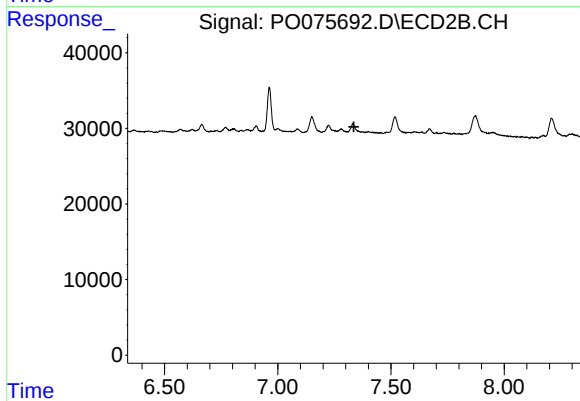

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.336 min
Response: 0
Conc: N.D.

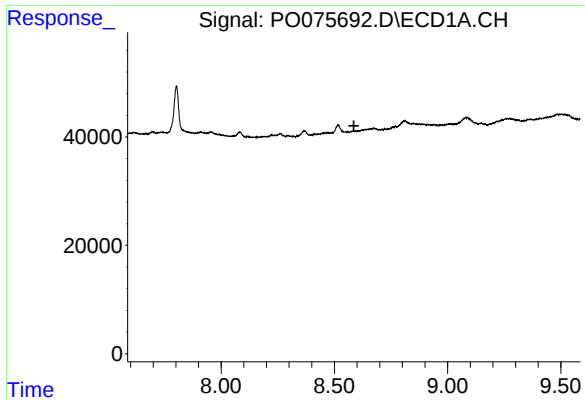

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

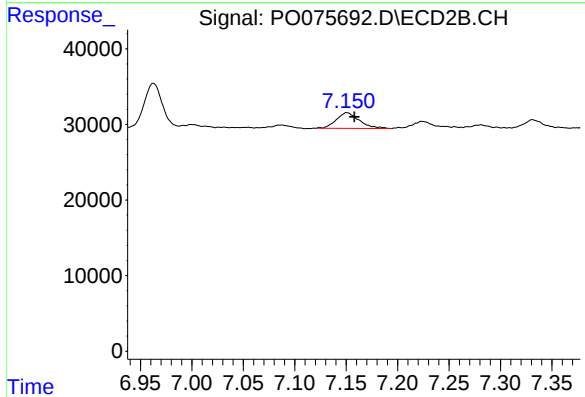


#33 AR-1260-3

R.T.: 7.151 min
Delta R.T.: -0.007 min
Response: 32436
Conc: 11.51 ng/ml

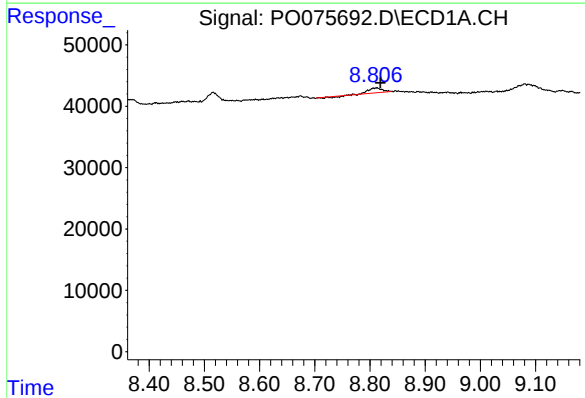


#34 AR-1260-4

R.T.: 8.813 min
Delta R.T.: -0.006 min
Response: 11373
Conc: 3.49 ng/ml

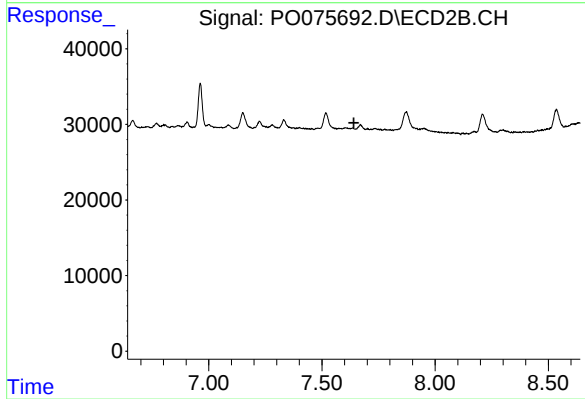

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.641 min
Response: 0
Conc: N.D.

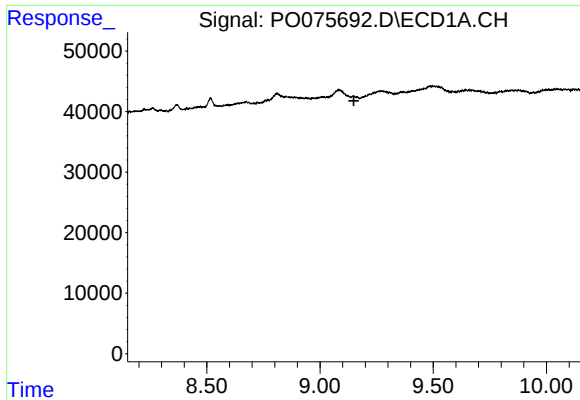

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

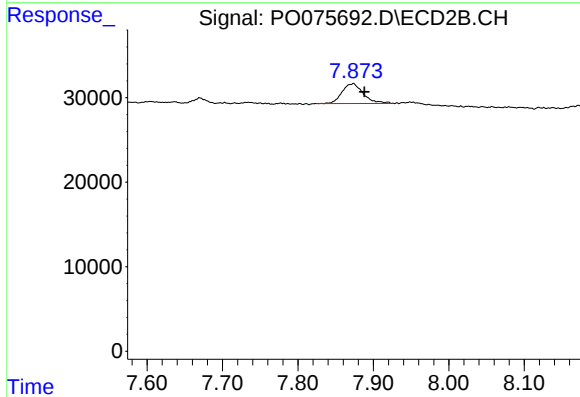


#35 AR-1260-5

R.T.: 7.874 min
Delta R.T.: -0.014 min
Response: 46477
Conc: 7.88 ng/ml

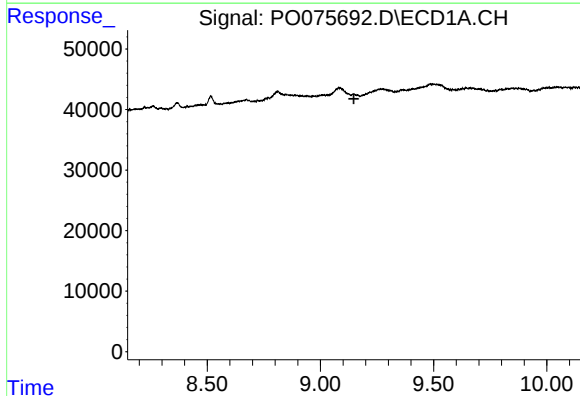


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

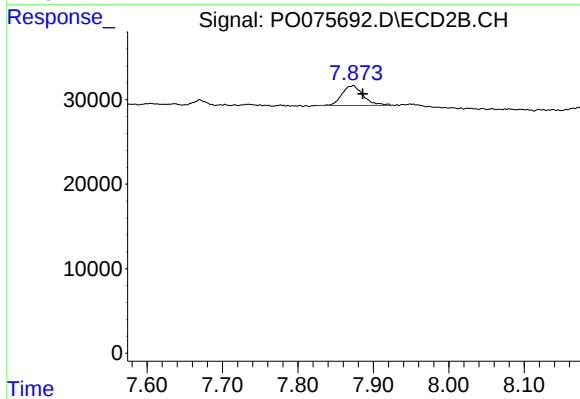

#37 AR-1262-2


R.T.: 7.874 min
Delta R.T.: -0.013 min
Response: 46477
Conc: 6.93 ng/ml

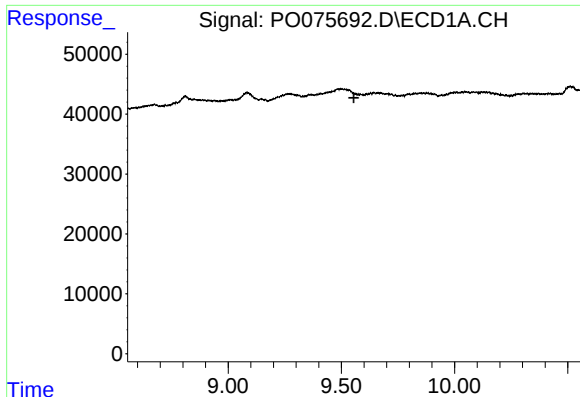

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

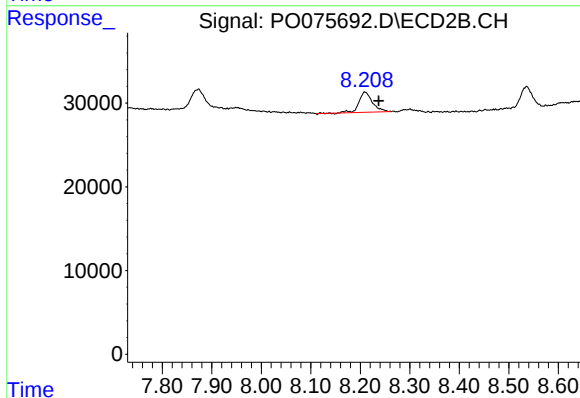


#39 AR-1262-4

R.T.: 8.209 min
Delta R.T.: -0.029 min
Response: 45996
Conc: 9.11 ng/ml

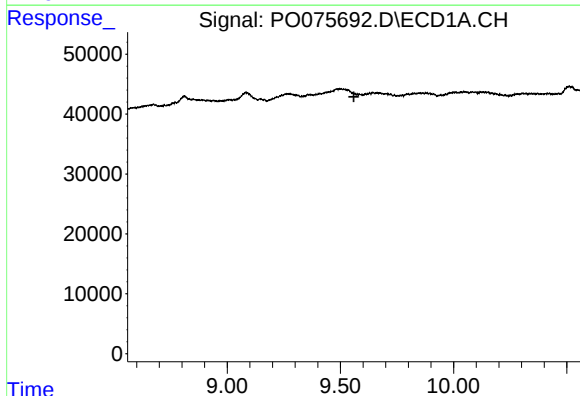

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.559 min
Response: 0
Conc: N.D.

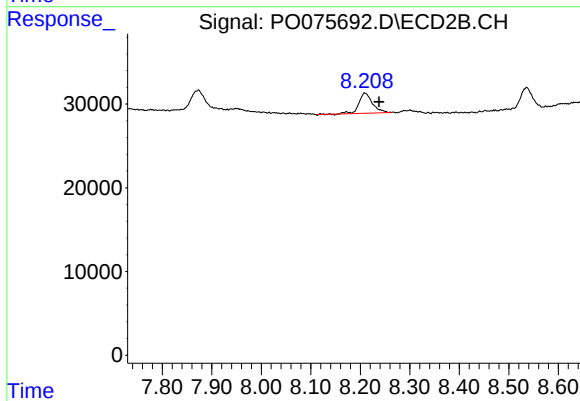

#42 AR-1268-2

R.T.: 8.209 min
Delta R.T.: -0.029 min
Response: 45996
Conc: 6.56 ng/ml