

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
 Data File : P0075666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Feb 2021 15:11
 Operator : AJ/MA
 Sample : M1460-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-01-022221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 01:00:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 23 07:07:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	3.961	184237	106304	2.797	2.567
2) SA Decachlor...	10.993	9.255	132539	122153	2.255	2.512

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
Data File : P0075666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Feb 2021 15:11
Operator : AJ/MA
Sample : M1460-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HD-01-022221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 01:00:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 23 07:07:50 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

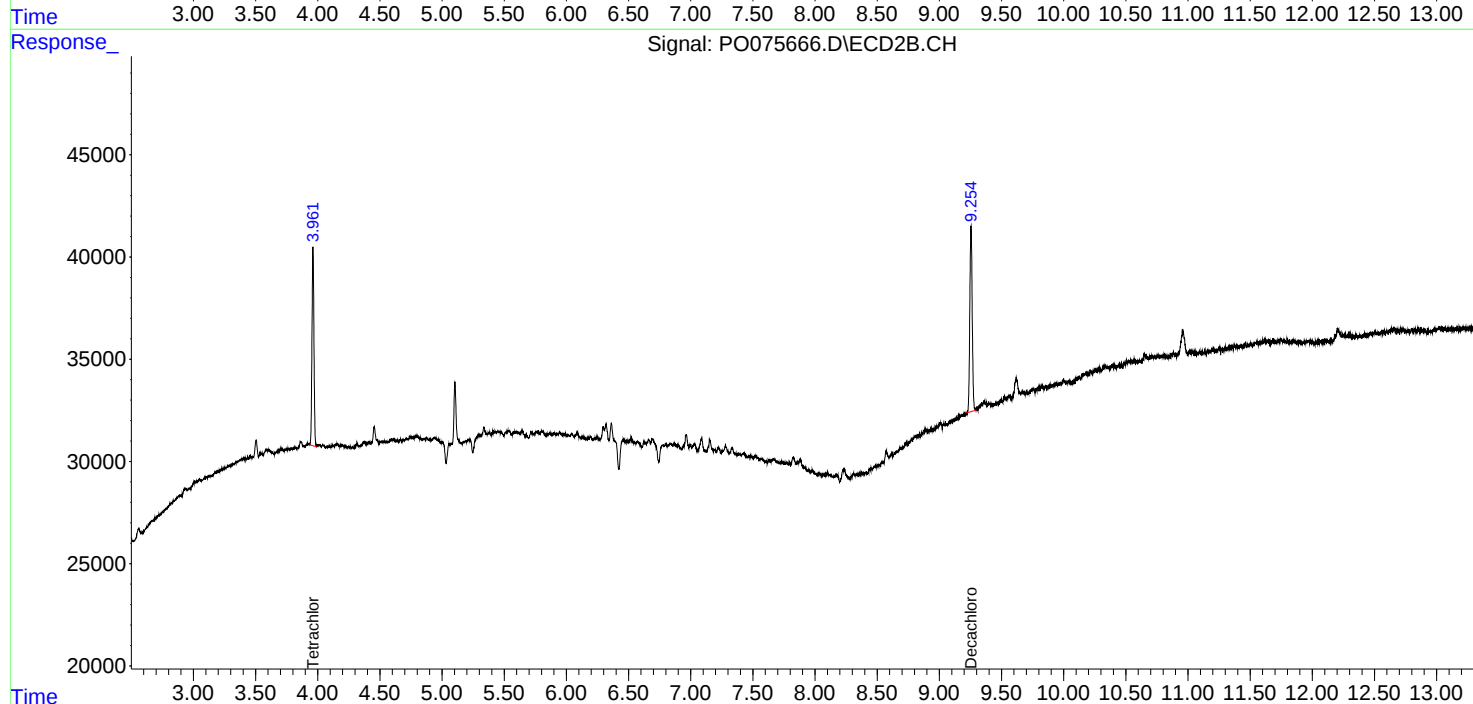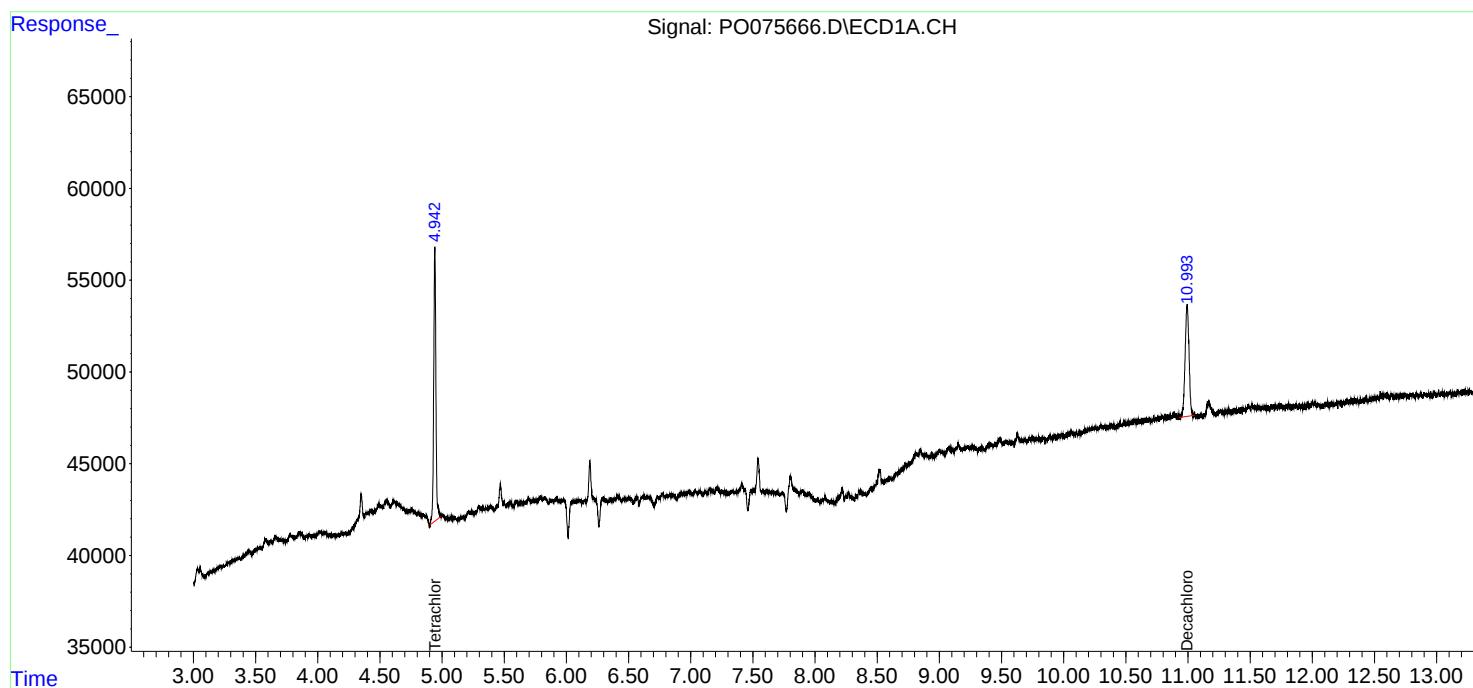


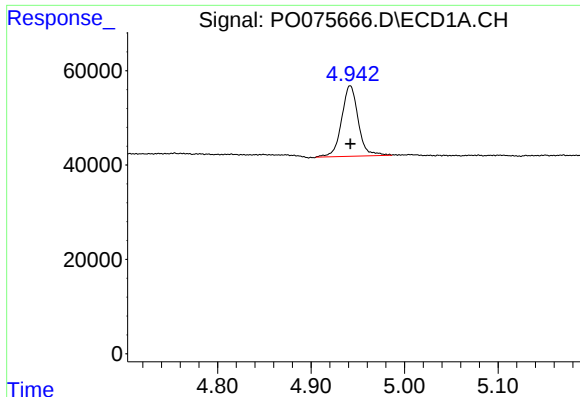

#1 Tetrachloro-m-xylene


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 184237
Conc: 2.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-01-022221

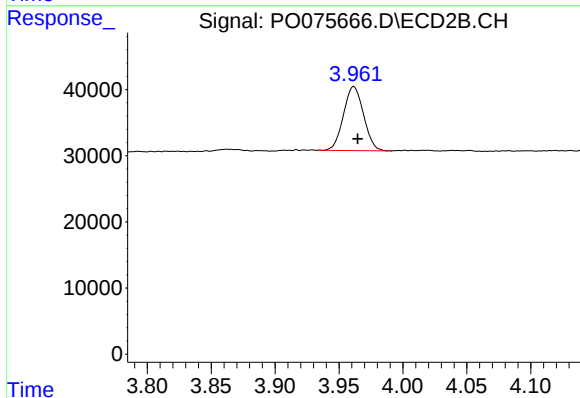


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.003 min
Response: 106304
Conc: 2.57 ng/ml

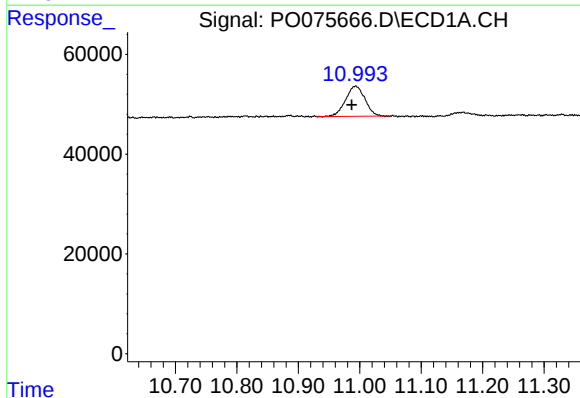

#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: 0.006 min
Response: 132539
Conc: 2.26 ng/ml

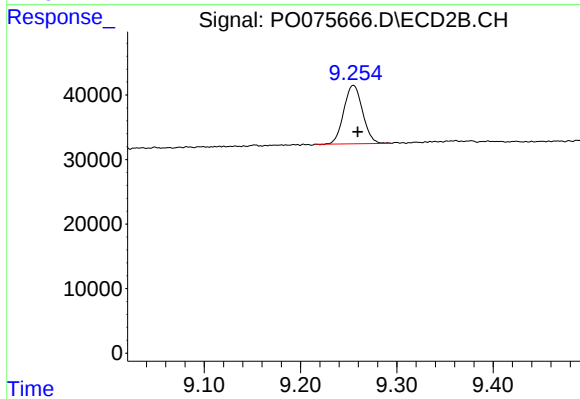

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.005 min
Response: 122153
Conc: 2.51 ng/ml