

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
 Data File : P0075671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Feb 2021 16:37
 Operator : AJ/MA
 Sample : M1464-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2-22A

Manual Integrations
 APPROVED

Ankita
 2/24/2021 1:45:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 01:03:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 23 07:07:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.943	3.962	160511	101129	2.437	2.442
2) SA Decachlor...	10.993	9.250	113913	197752	1.938	4.066m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
Data File : P0075671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Feb 2021 16:37
Operator : AJ/MA
Sample : M1464-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2-22A


Manual Integrations
APPROVED

Ankita
2/24/2021 1:45:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 01:03:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 23 07:07:50 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

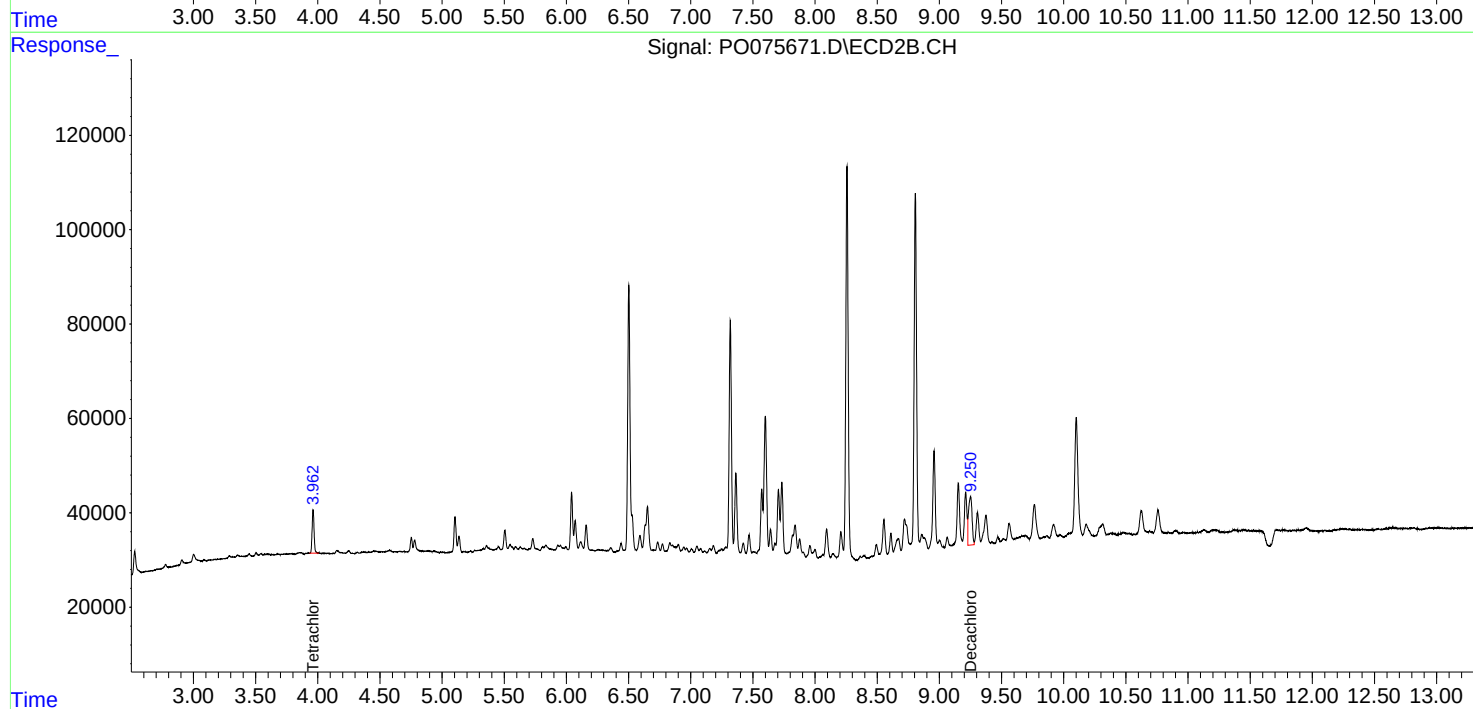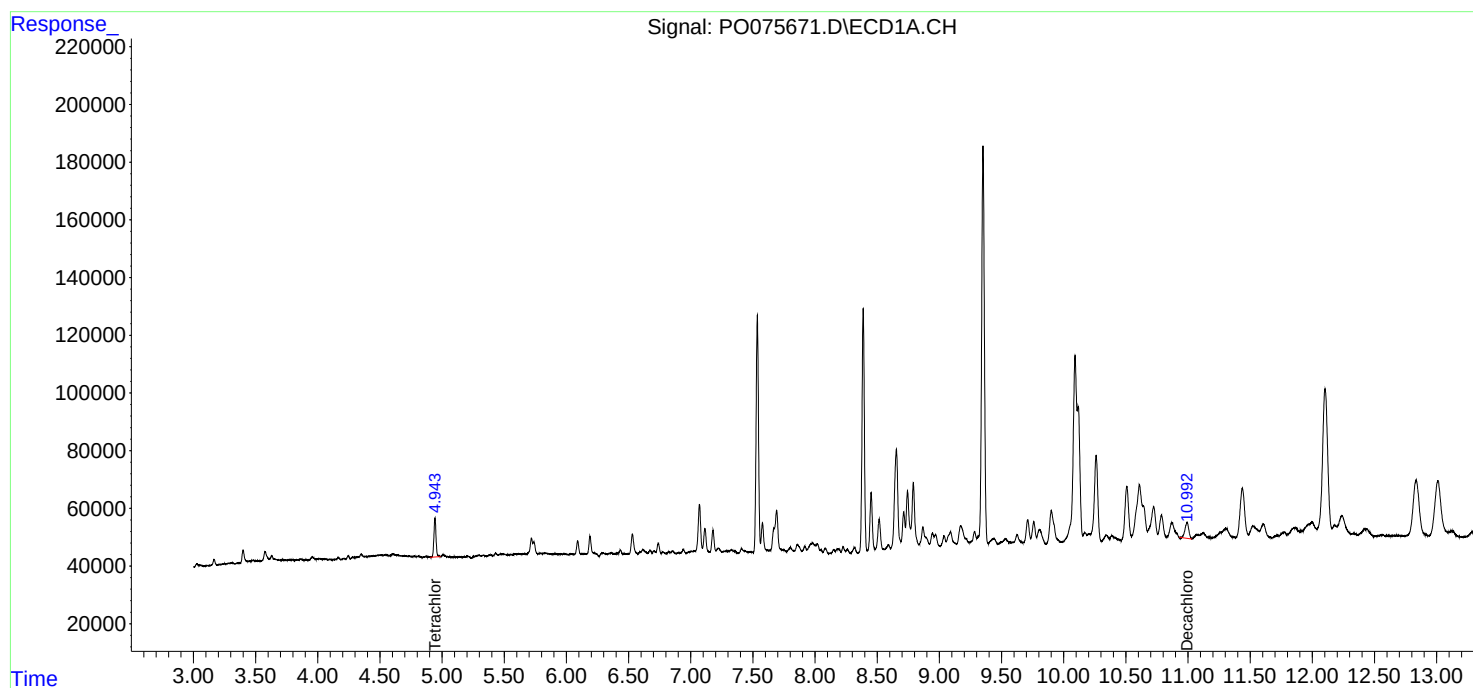

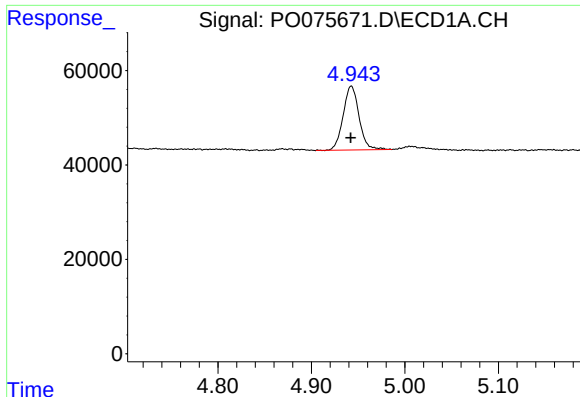


#1 Tetrachloro-m-xylene

R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 160511
Conc: 2.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
2-22A


Manual Integrations
APPROVED

Ankita
2/24/2021 1:45:53 PM

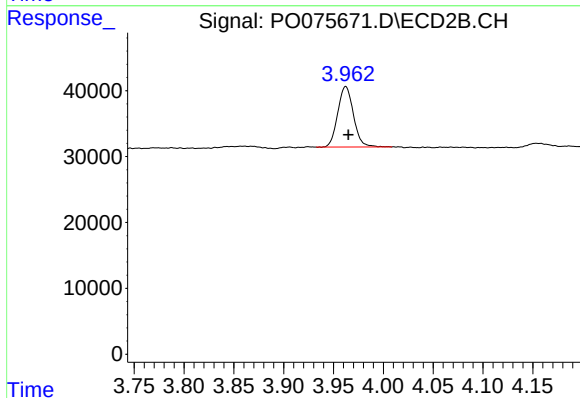


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.002 min
Response: 101129
Conc: 2.44 ng/ml

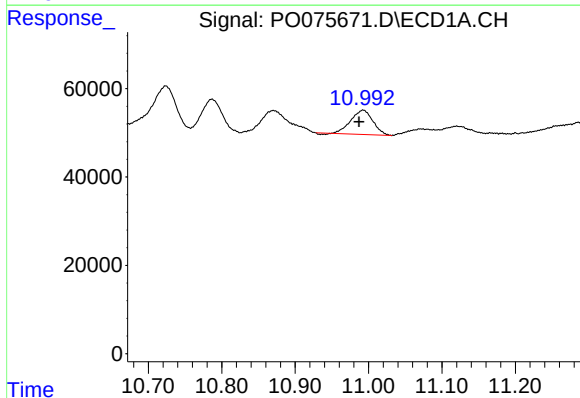

#2 Decachlorobiphenyl

R.T.: 10.993 min
Delta R.T.: 0.006 min
Response: 113913
Conc: 1.94 ng/ml

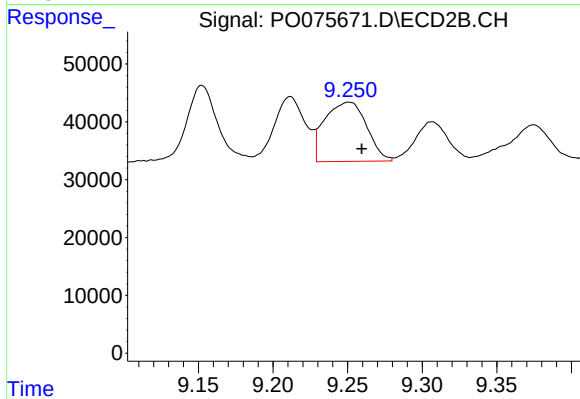

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.009 min
Response: 197752
Conc: 4.07 ng/ml m