

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
 Data File : P0075678.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Feb 2021 19:11
 Operator : AJ/MA
 Sample : M1464-04 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2-22D

Manual Integrations
 APPROVED

Ankita
 2/24/2021 9:32:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 01:07:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 23 07:07:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	3.962	168201	106305	2.554	2.567
2) SA Decachlor...	10.991	9.253	125652	140258	2.138	2.884m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022321\
Data File : P0075678.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Feb 2021 19:11
Operator : AJ/MA
Sample : M1464-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2-22D


Manual Integrations
APPROVED

Ankita
2/24/2021 9:32:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 01:07:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 23 07:07:50 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

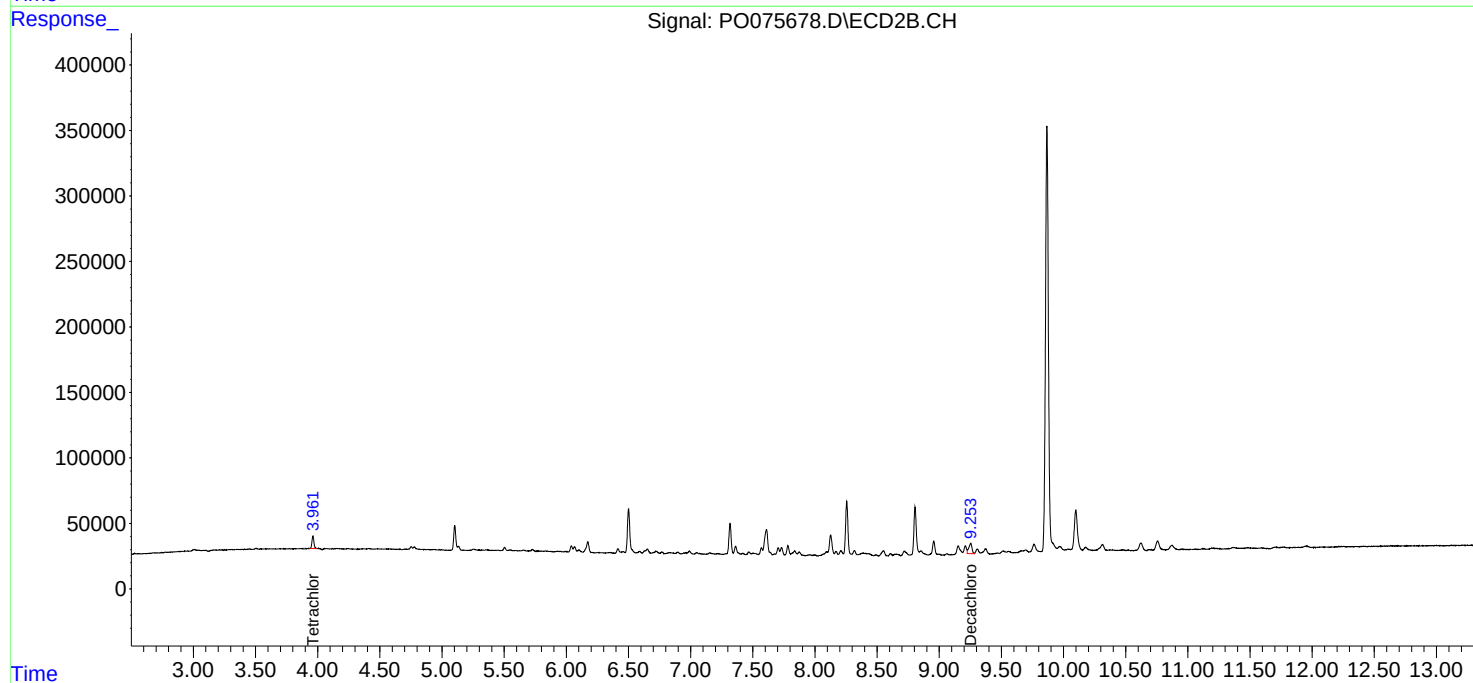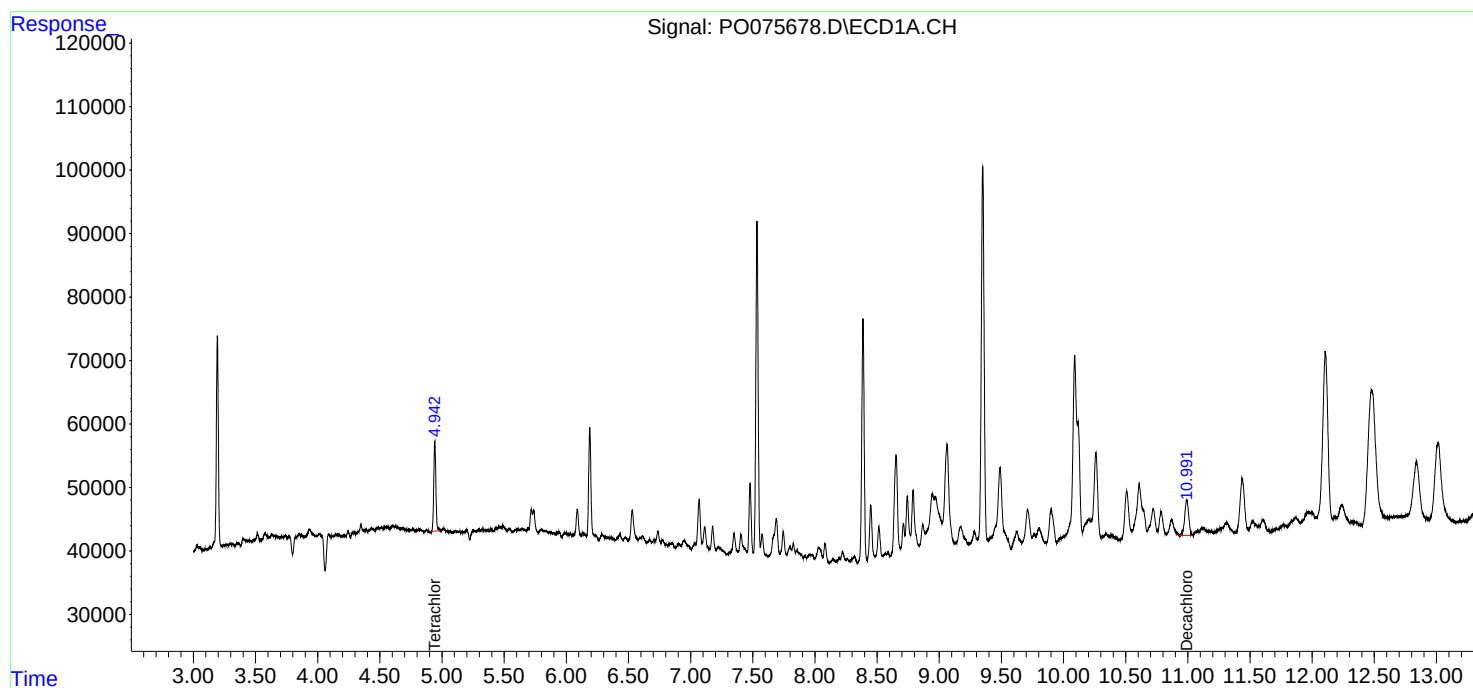

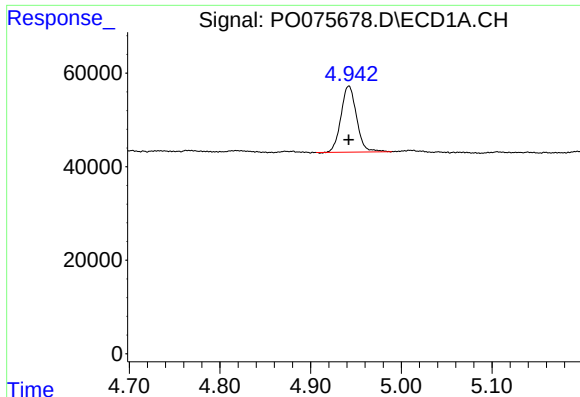


#1 Tetrachloro-m-xylene

R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 168201
Conc: 2.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
2-22D


Manual Integrations
APPROVED

Ankita
2/24/2021 9:32:48 AM

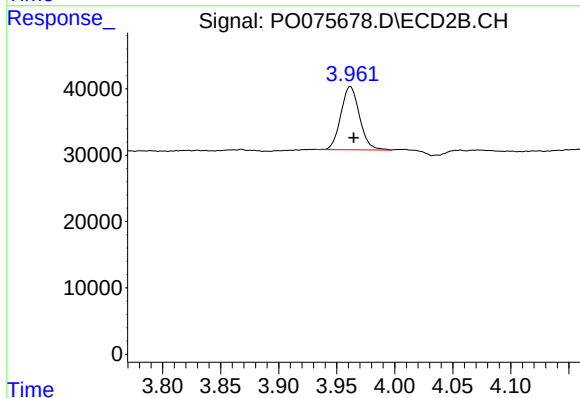


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.003 min
Response: 106305
Conc: 2.57 ng/ml

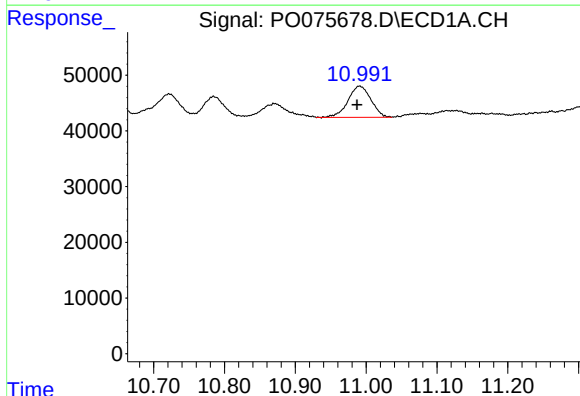

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: 0.004 min
Response: 125652
Conc: 2.14 ng/ml

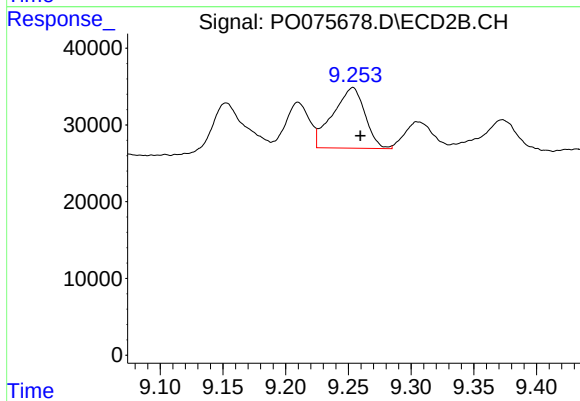

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.006 min
Response: 140258
Conc: 2.88 ng/ml m