

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022322\
 Data File : P0084872.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Feb 2022 20:02
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/24/2022
 Supervised By :Ankita Jodhani 02/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 00:56:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 24 00:55:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.594	7382474	1209651	25.166	25.528m
2) SA Decachlor...	10.429	8.622	4757252	1024059	25.691	26.544
Target Compounds						
16) L4 AR-1242-1	5.697	4.686	2017901	362781	262.364	271.908
17) L4 AR-1242-2	5.720	4.704	2850687	506852	256.969	265.660
18) L4 AR-1242-3	5.784	4.880	1746581	274339	260.322	263.108
19) L4 AR-1242-4	5.884	4.965	1466813	284019	262.077	270.708
20) L4 AR-1242-5	6.632	5.490	1475890	339503	261.656	268.677

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022322\
Data File : P0084872.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Feb 2022 20:02
Operator : YP\AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :Ankita Jodhani 02/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 00:56:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022322.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 24 00:55:51 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

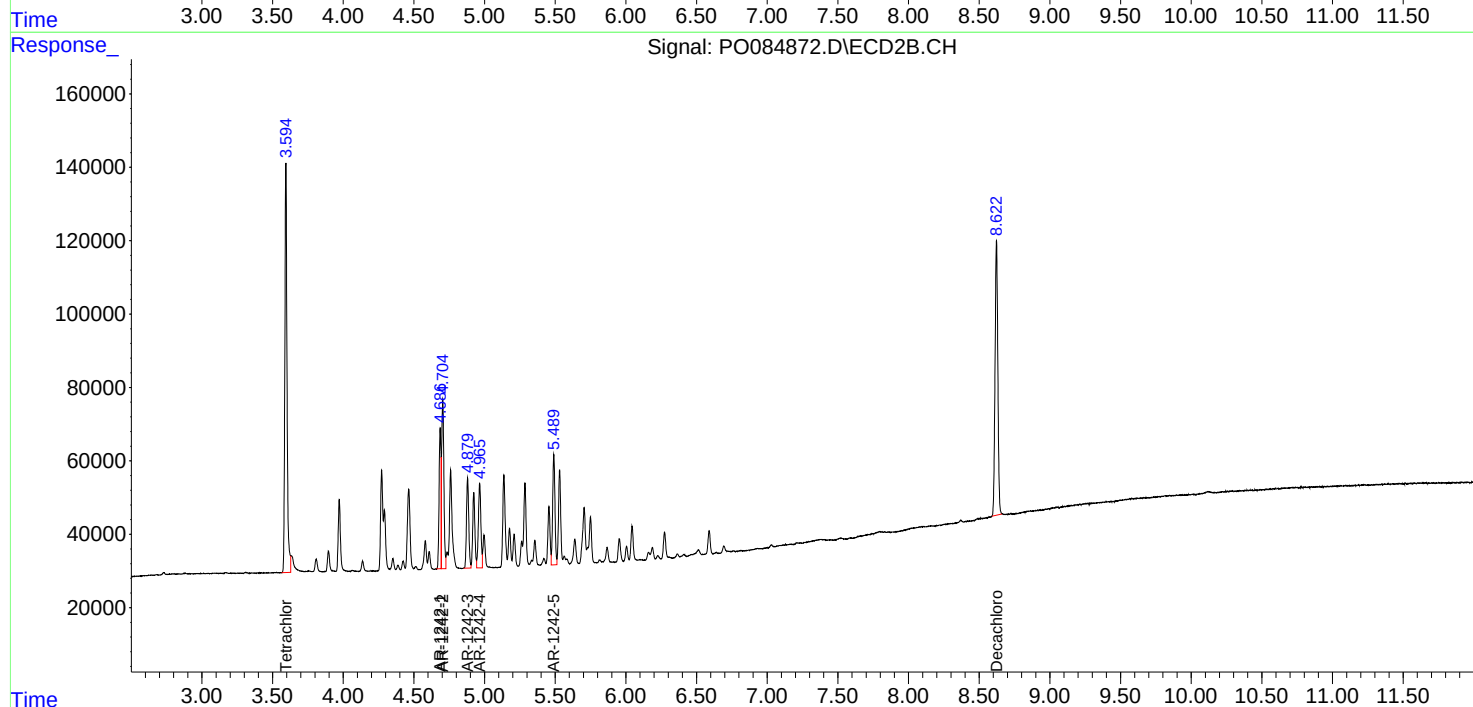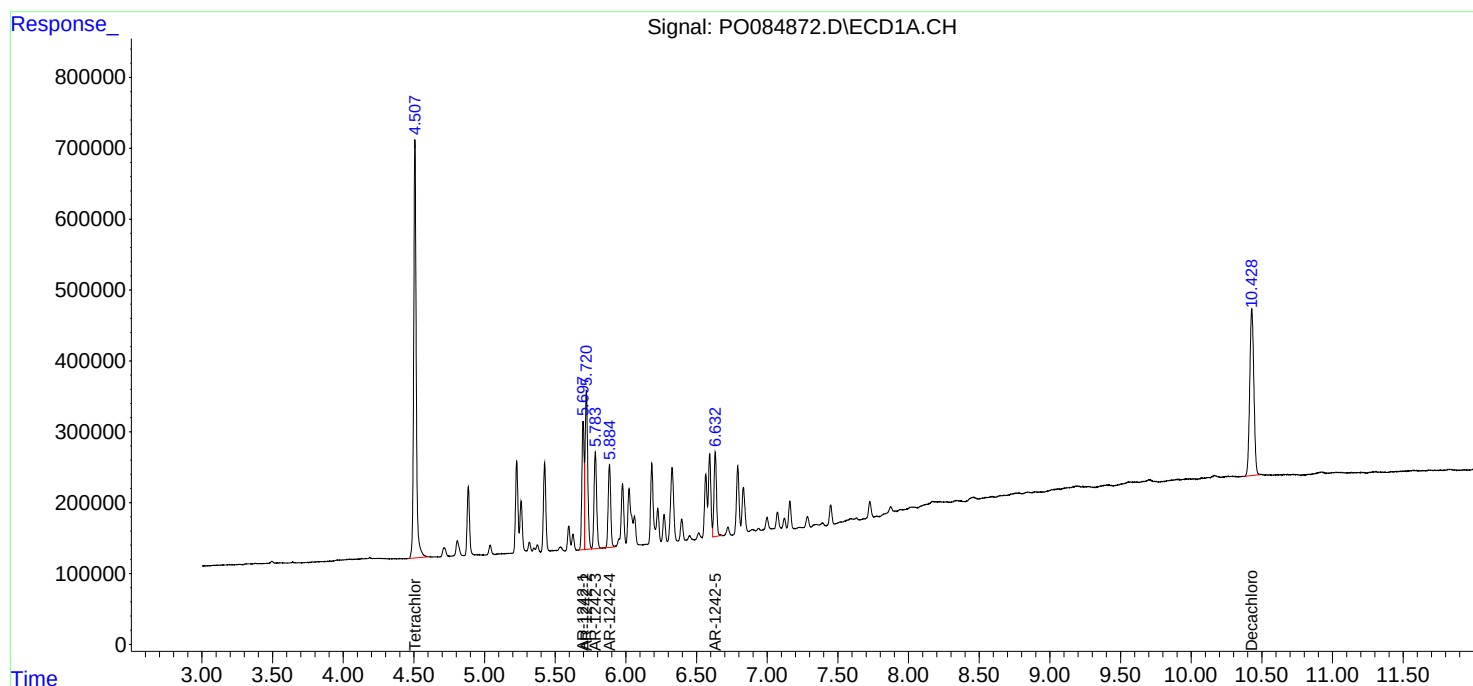

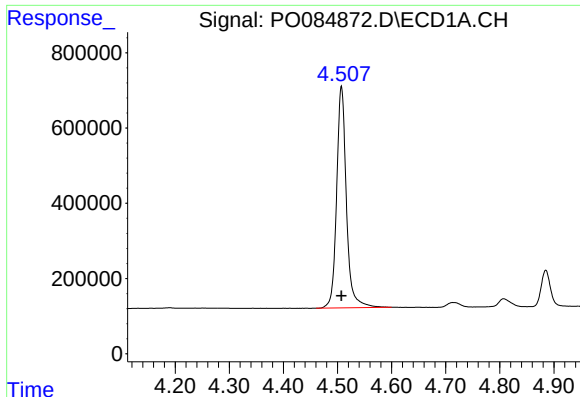


#1 Tetrachloro-m-xylene

R.T.: 4.507 min
Delta R.T.: 0.000 min
Response: 7382474
Conc: 25.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :Ankita Jodhani 02/24/2022

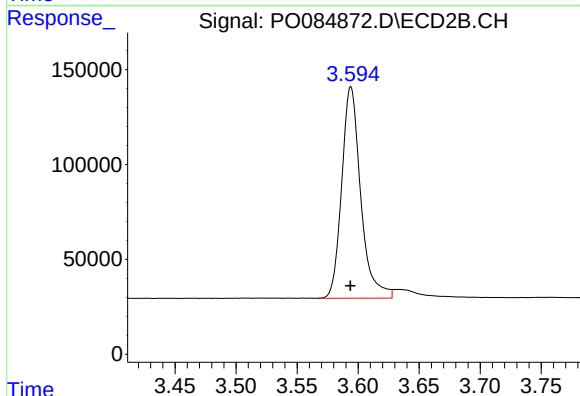


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 1209651
Conc: 25.53 ng/ml m

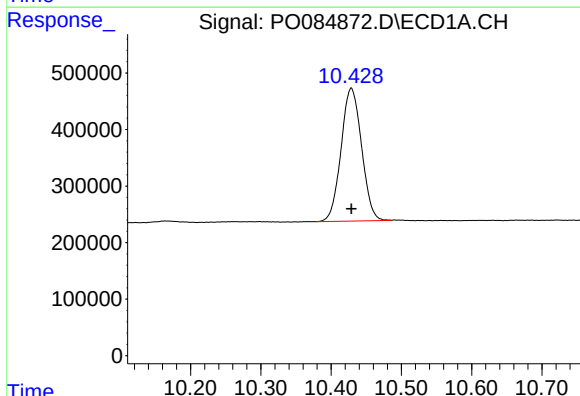


#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: 0.000 min
Response: 4757252
Conc: 25.69 ng/ml

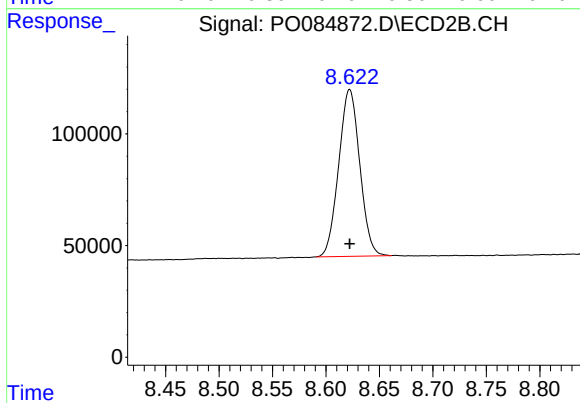

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: 0.000 min
Response: 1024059
Conc: 26.54 ng/ml

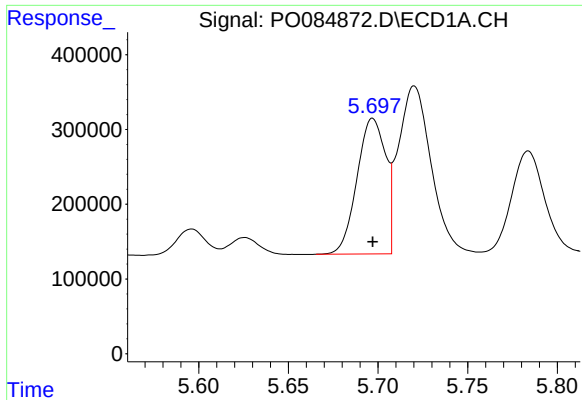


#16 AR-1242-1

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 2017901
Conc: 262.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :Ankita Jodhani 02/24/2022

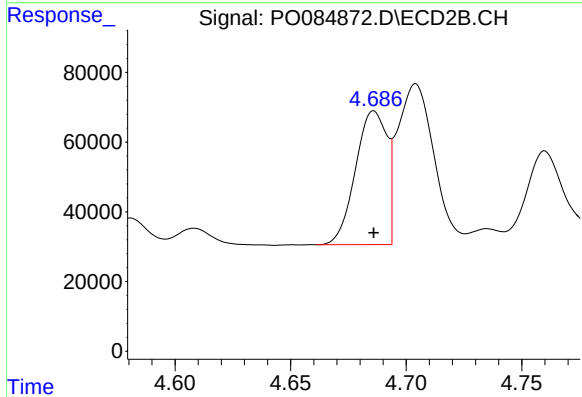


#16 AR-1242-1

R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 362781
Conc: 271.91 ng/ml

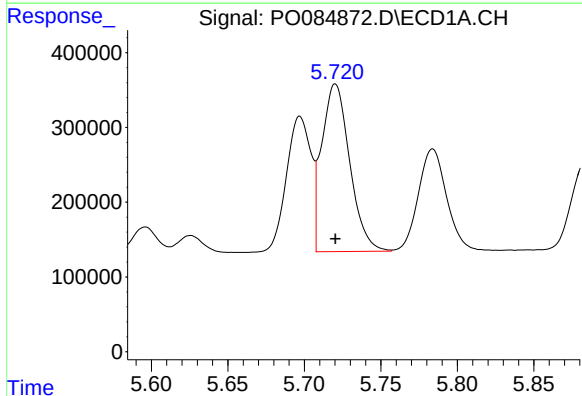


#17 AR-1242-2

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 2850687
Conc: 256.97 ng/ml

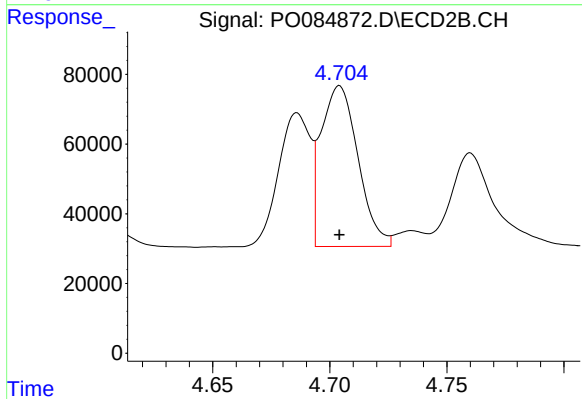

#17 AR-1242-2

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 506852
Conc: 265.66 ng/ml

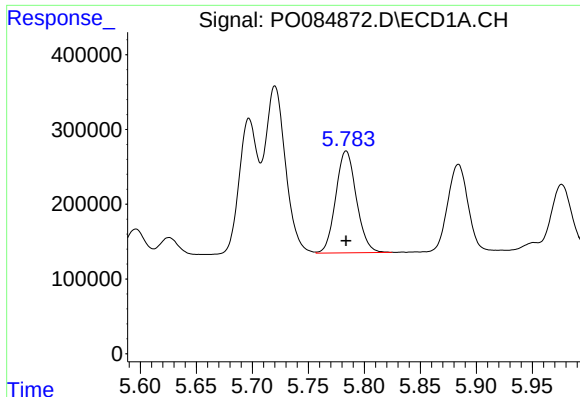


#18 AR-1242-3

R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 1746581
Conc: 260.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :Ankita Jodhani 02/24/2022

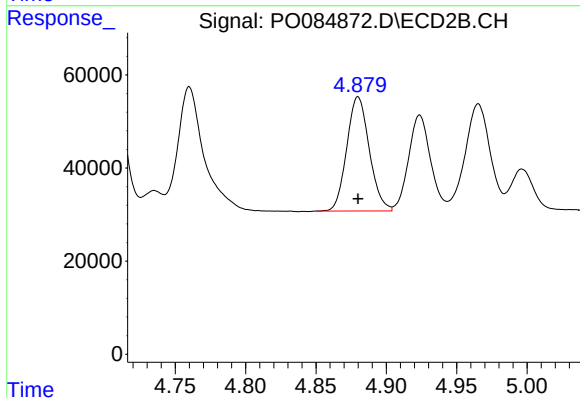


#18 AR-1242-3

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 274339
Conc: 263.11 ng/ml

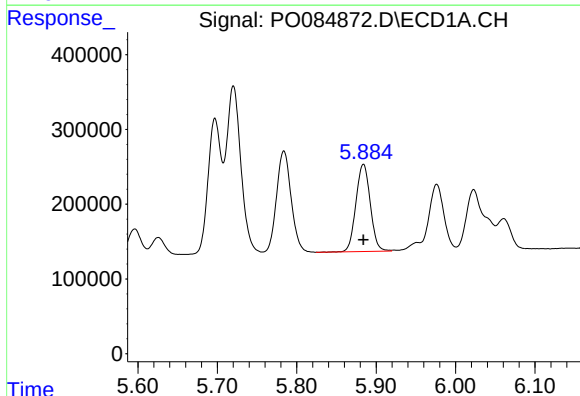


#19 AR-1242-4

R.T.: 5.884 min
Delta R.T.: 0.000 min
Response: 1466813
Conc: 262.08 ng/ml

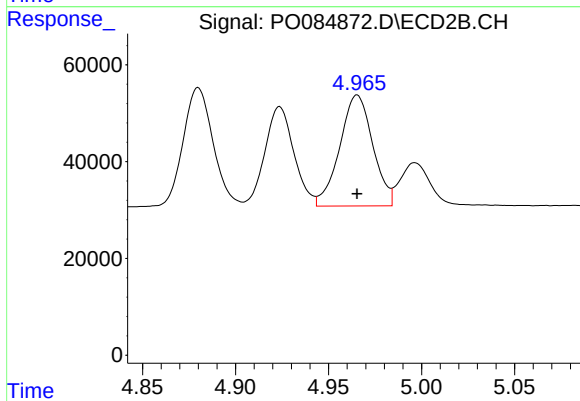

#19 AR-1242-4

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 284019
Conc: 270.71 ng/ml

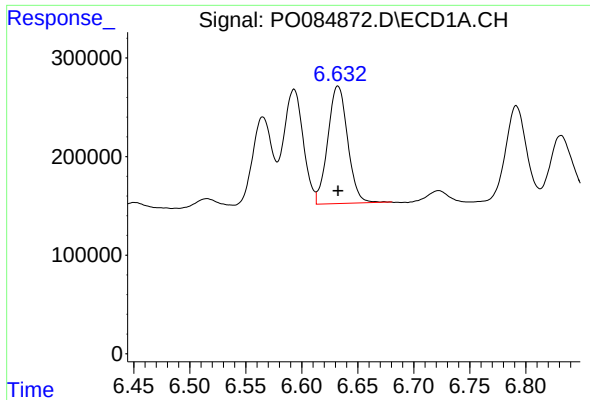


#20 AR-1242-5

R.T.: 6.632 min
Delta R.T.: 0.000 min
Response: 1475890
Conc: 261.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :Ankita Jodhani 02/24/2022

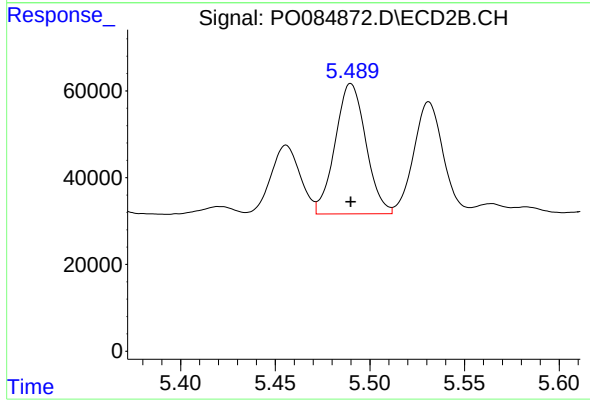

#20 AR-1242-5

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 339503
Conc: 268.68 ng/ml