

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022423\
 Data File : P0092749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2023 04:36
 Operator : YP/AJ
 Sample : 01627-03
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 08:30:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.431	3.636	68093529	26776320	22.677	21.006
2)	SA Decachlor...	10.261	8.670	48679998	25451100	25.308	21.839
Target Compounds							
3)	L1 AR-1016-1	5.541f	0.000	1349718	0	14.685	N.D. #
8)	L2 AR-1221-1	4.640	3.851	971568	381770	24.580	23.630
9)	L2 AR-1221-2	4.733	3.936	1561833	608246	54.281	50.239
10)	L2 AR-1221-3	4.803	4.012	2558090	973622	29.046	26.148
11)	L3 AR-1232-1	4.803	4.012	2558090	973622	36.403	31.099
16)	L4 AR-1242-1	5.541f	0.000	1349718	0	17.106	N.D. #
21)	L5 AR-1248-1	5.541f	0.000	1349718	0	22.018	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022423\
Data File : PO092749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2023 04:36
Operator : YP/AJ
Sample : 01627-03
Misc : AR1221 MDL 25 PPB
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 08:30:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

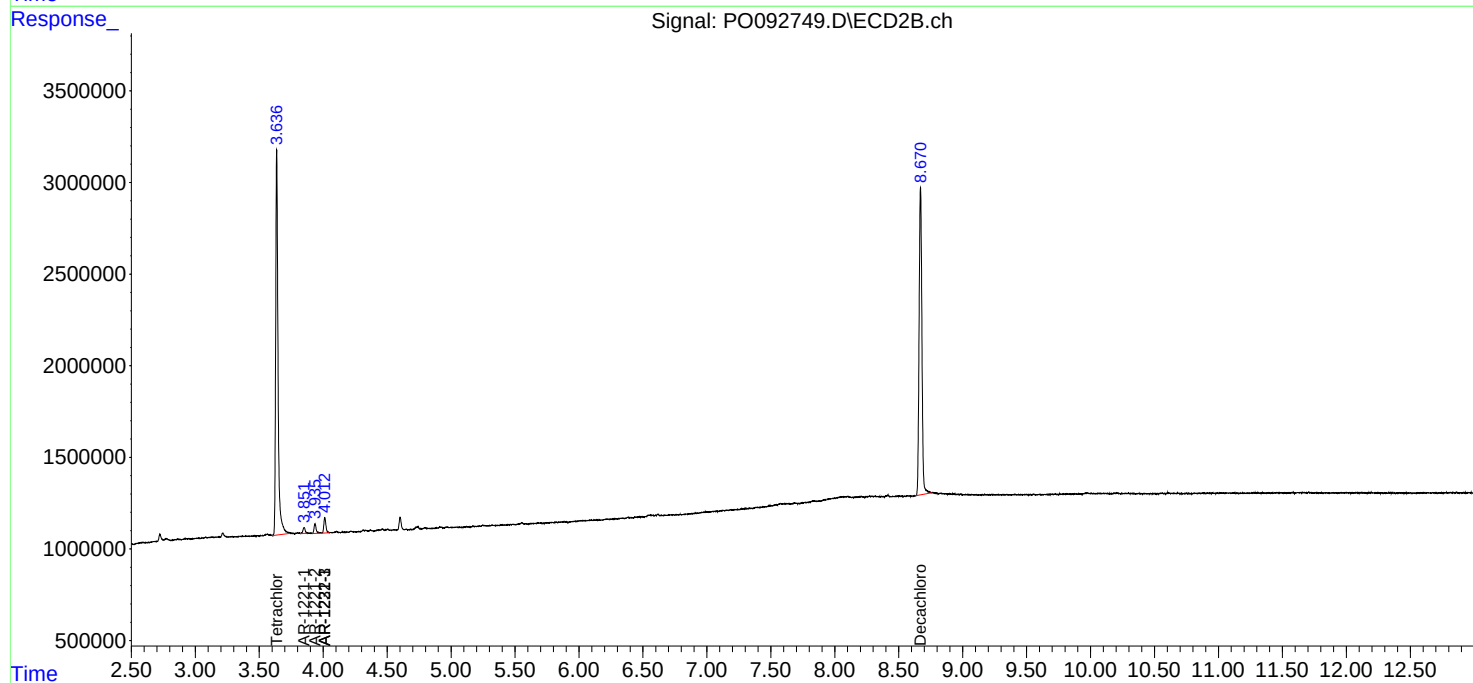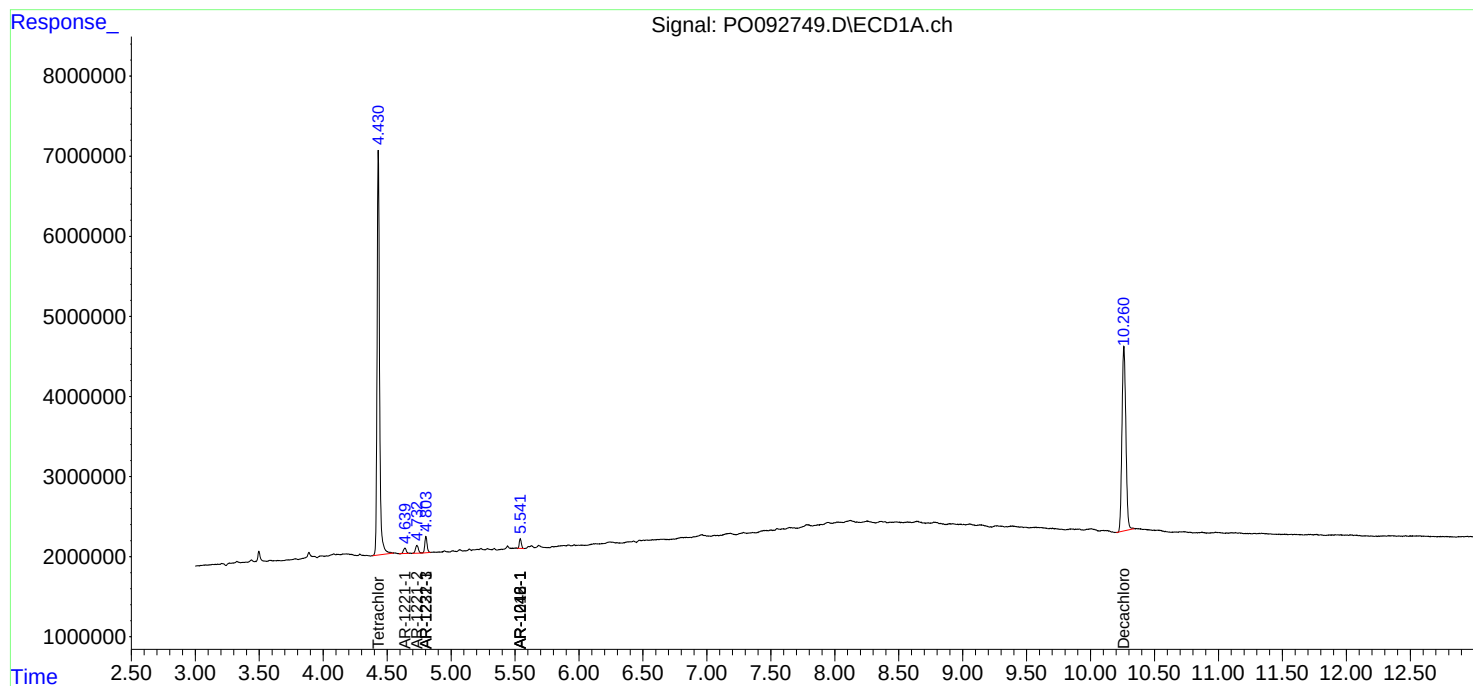


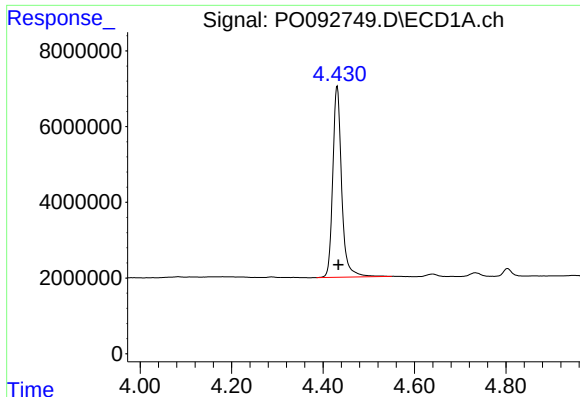

#1 Tetrachloro-m-xylene


R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 68093529
Conc: 22.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

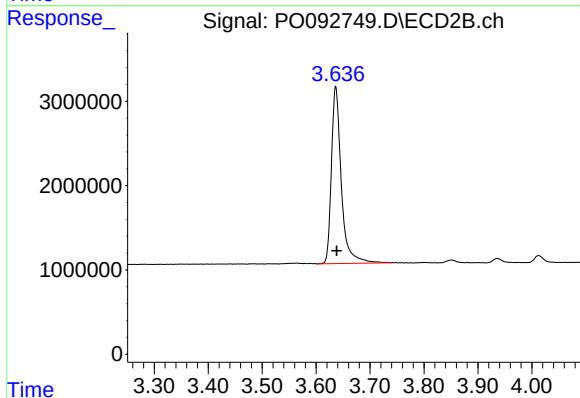


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 26776320
Conc: 21.01 ng/ml

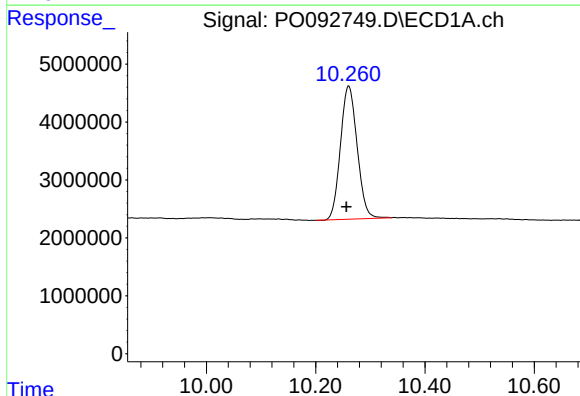


#2 Decachlorobiphenyl

R.T.: 10.261 min
Delta R.T.: 0.004 min
Response: 48679998
Conc: 25.31 ng/ml

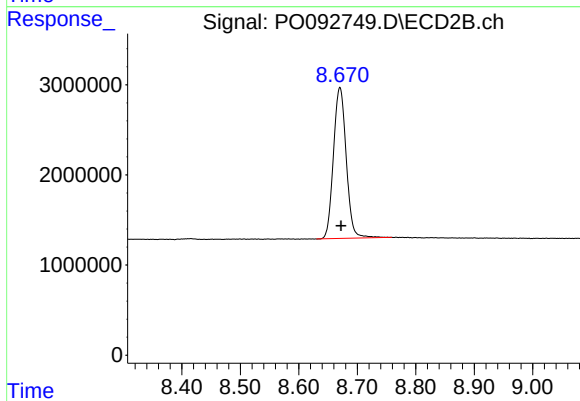

#2 Decachlorobiphenyl


R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 25451100
Conc: 21.84 ng/ml

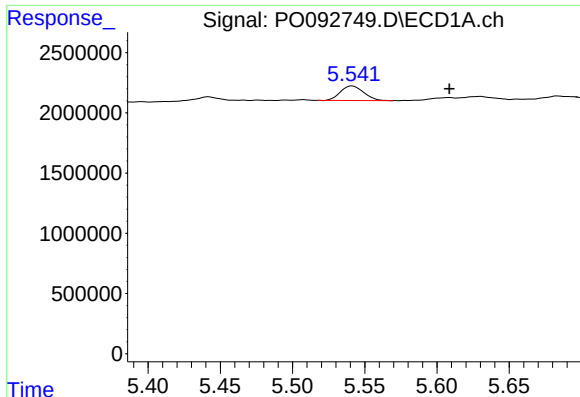

#3 AR-1016-1


R.T.: 5.541 min
Delta R.T.: -0.067 min
Response: 1349718
Conc: 14.69 ng/ml

Instrument :
ECD_O
ClientSampleId :

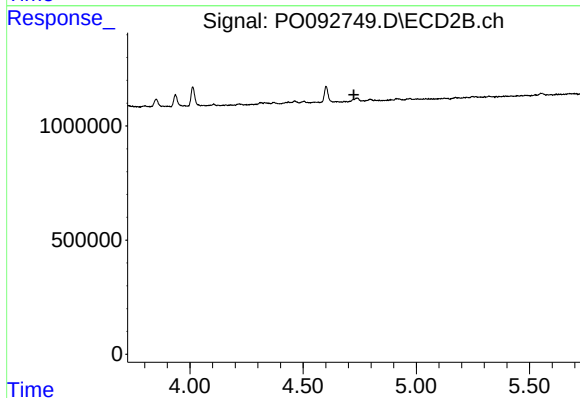


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

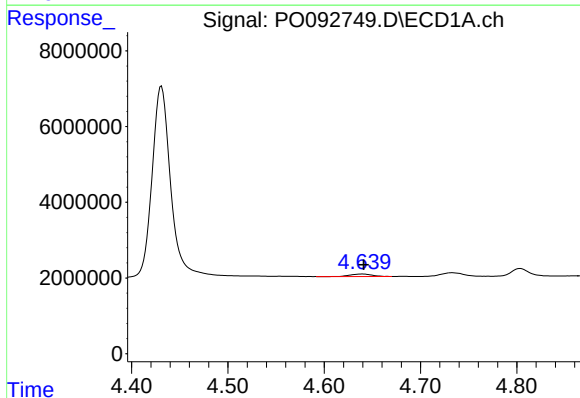


#8 AR-1221-1

R.T.: 4.640 min
Delta R.T.: -0.001 min
Response: 971568
Conc: 24.58 ng/ml

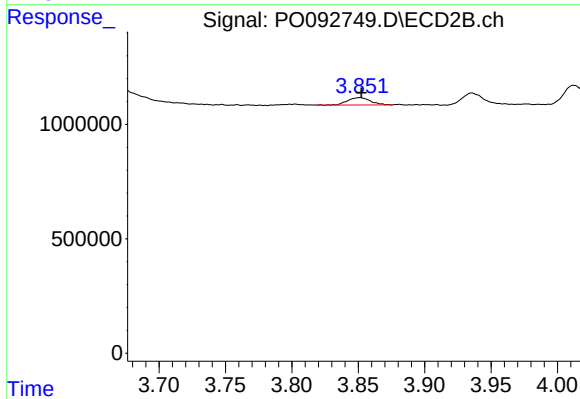

#8 AR-1221-1


R.T.: 3.851 min
Delta R.T.: -0.001 min
Response: 381770
Conc: 23.63 ng/ml

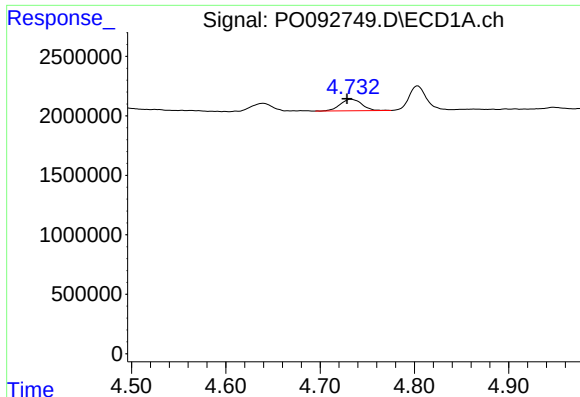

#9 AR-1221-2


R.T.: 4.733 min
Delta R.T.: 0.004 min
Response: 1561833
Conc: 54.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

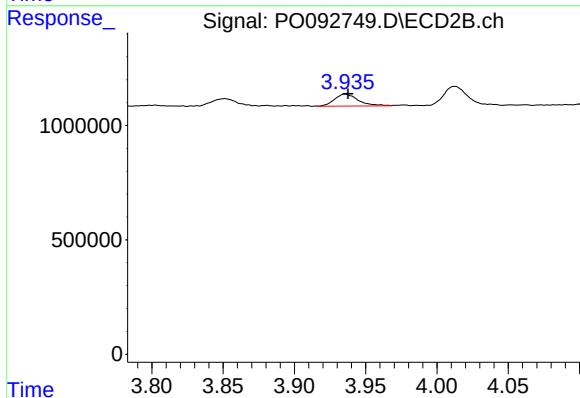


#9 AR-1221-2

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 608246
Conc: 50.24 ng/ml

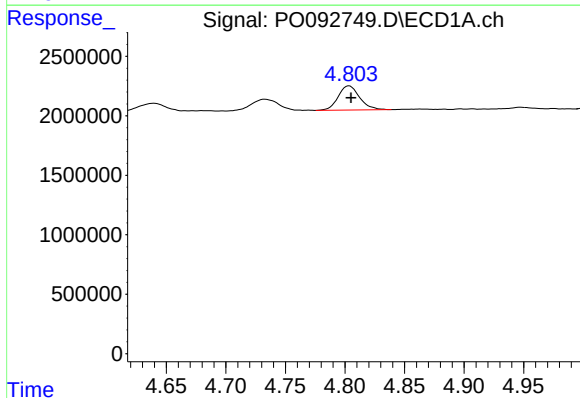


#10 AR-1221-3

R.T.: 4.803 min
Delta R.T.: -0.002 min
Response: 2558090
Conc: 29.05 ng/ml

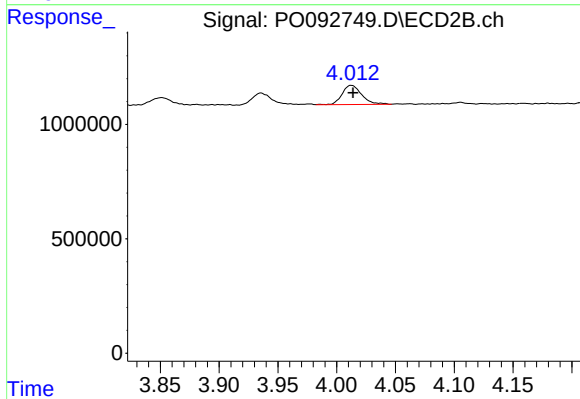

#10 AR-1221-3


R.T.: 4.012 min
Delta R.T.: -0.001 min
Response: 973622
Conc: 26.15 ng/ml

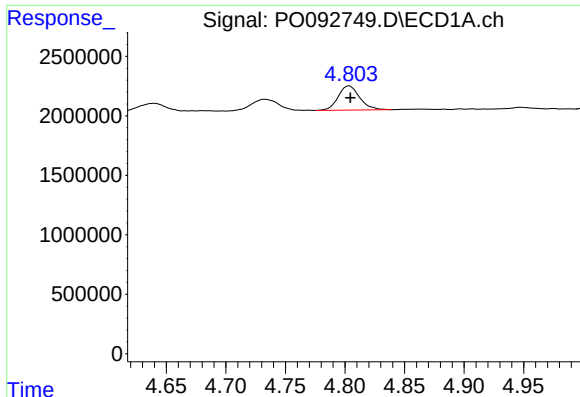

#11 AR-1232-1


R.T.: 4.803 min
Delta R.T.: -0.001 min
Response: 2558090
Conc: 36.40 ng/ml

Instrument :
ECD_O
ClientSampleId :

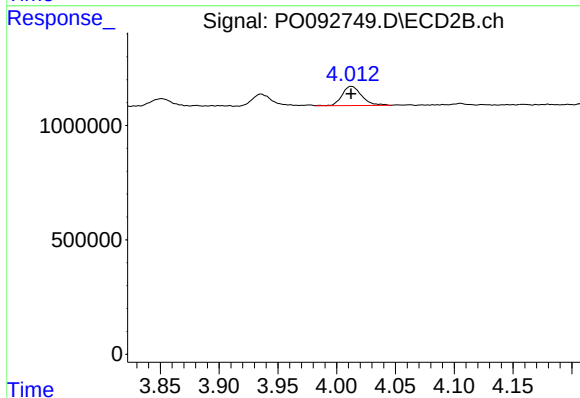


#11 AR-1232-1

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 973622
Conc: 31.10 ng/ml

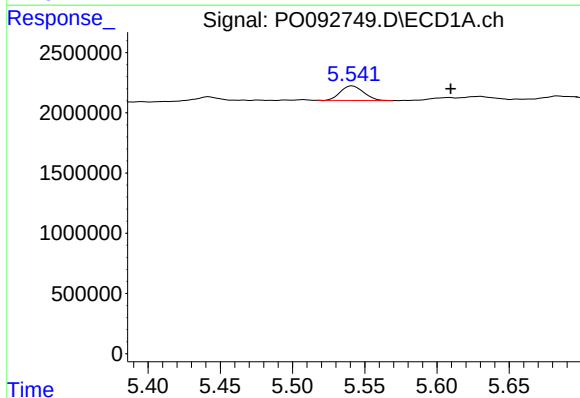


#16 AR-1242-1

R.T.: 5.541 min
Delta R.T.: -0.068 min
Response: 1349718
Conc: 17.11 ng/ml

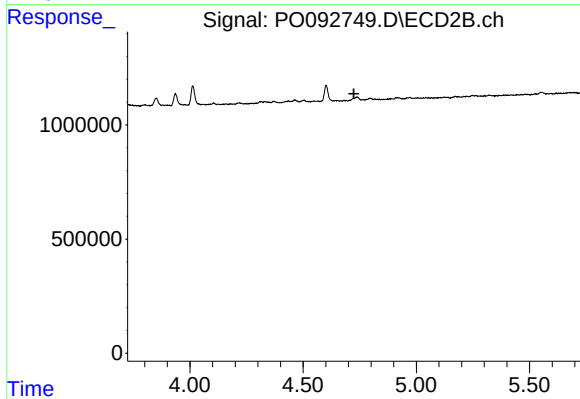

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.724 min
Response: 0
Conc: N.D.

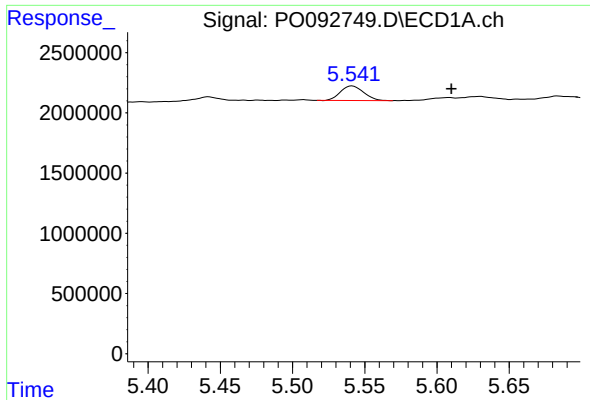

#21 AR-1248-1

R.T.: 5.541 min
Delta R.T.: -0.069 min
Response: 1349718
Conc: 22.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

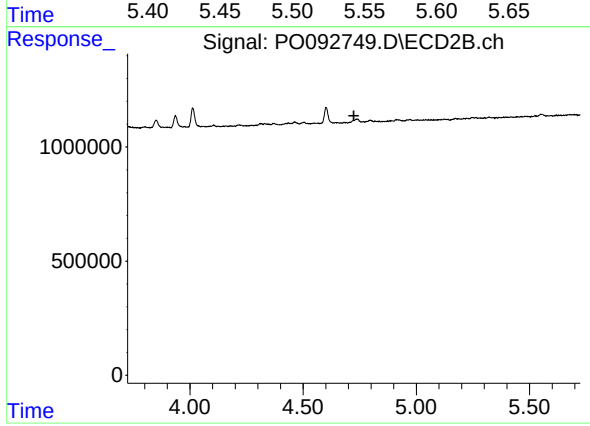

#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.724 min
Response: 0
Conc: N.D.