

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022423\
 Data File : P0092717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2023 19:30
 Operator : YP/AJ
 Sample : 01627-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:18:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.638	60643256	23549024	20.196	18.475
2) SA Decachlor...	10.265	8.672	43269879	22533265	22.496	19.335
Target Compounds						
8) L2 AR-1221-1	4.641	3.853	1511818	568108	38.249	35.163
9) L2 AR-1221-2	4.734	3.938	1632641	744892	56.742	61.526
10) L2 AR-1221-3	4.805	4.014	3553724	1388861	40.351	37.300



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022423\
Data File : PO092717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2023 19:30
Operator : YP/AJ
Sample : 01627-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:18:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

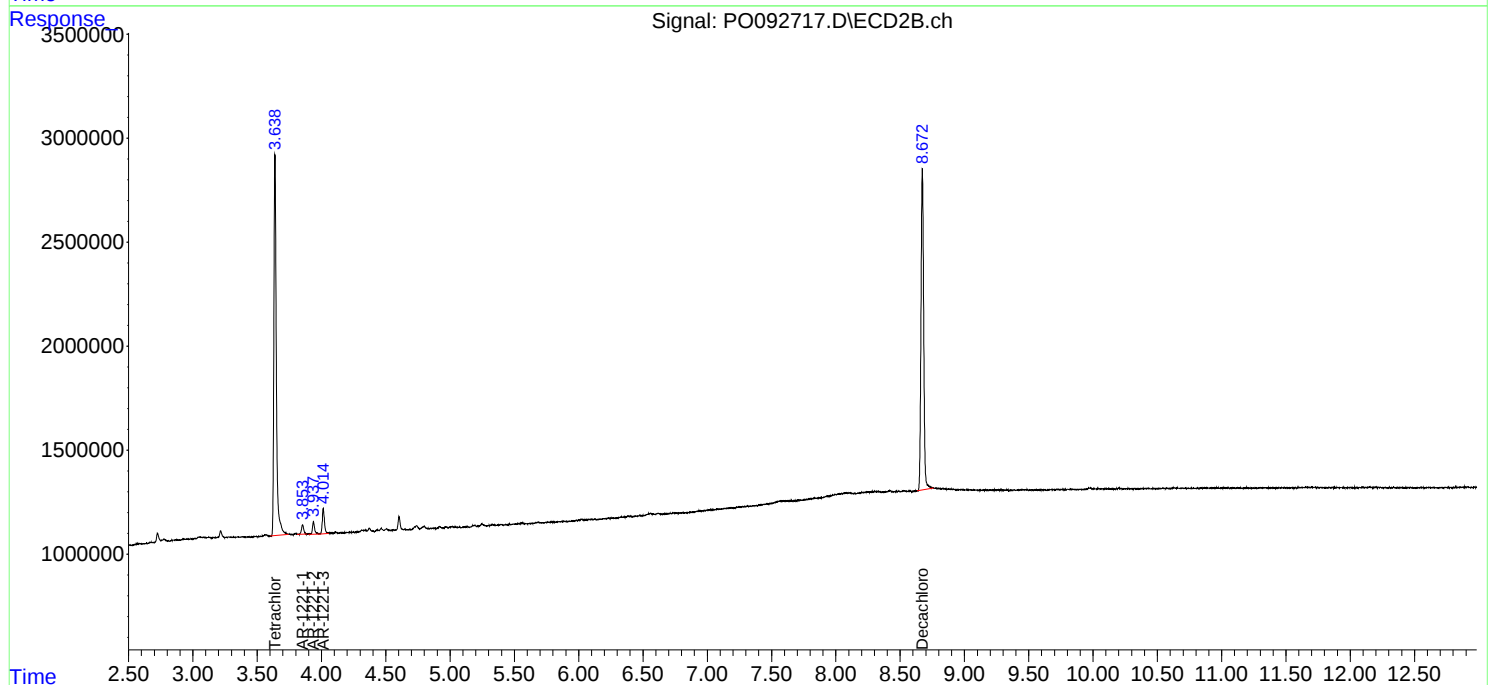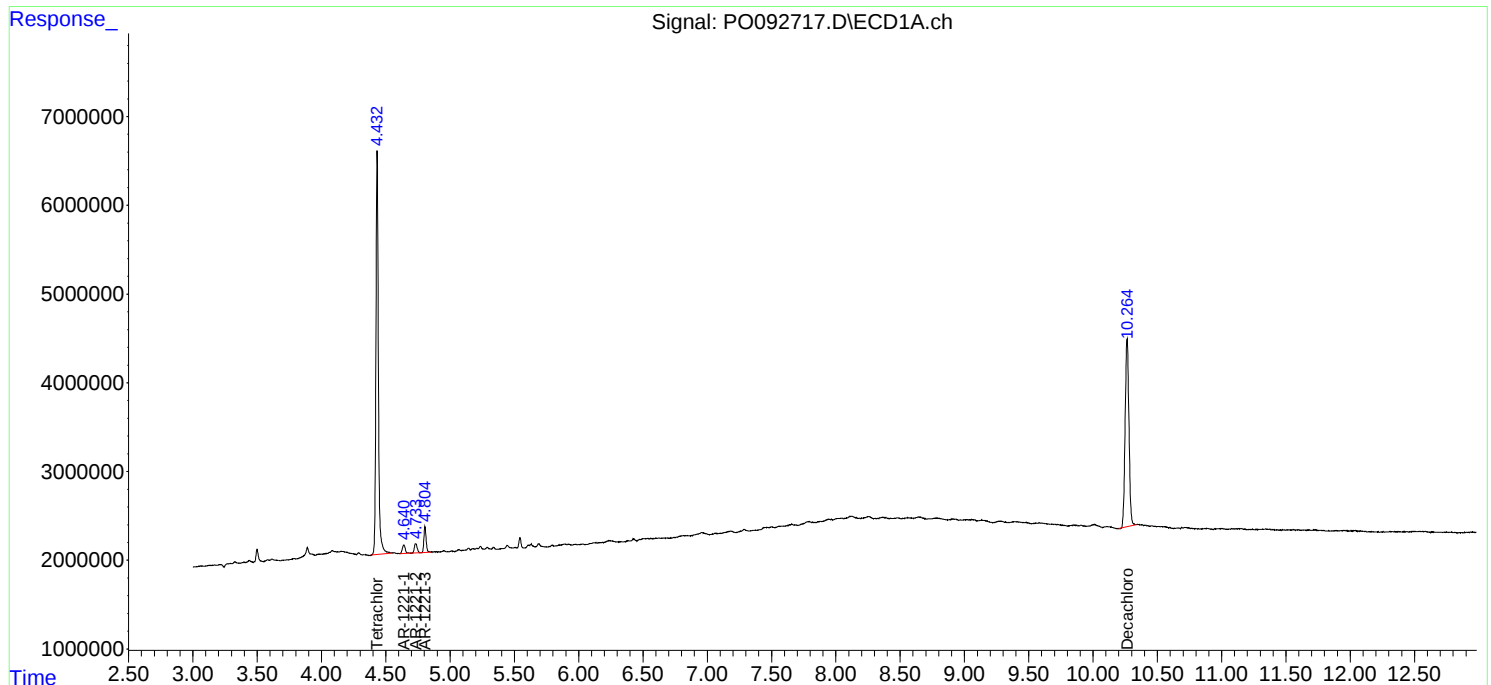


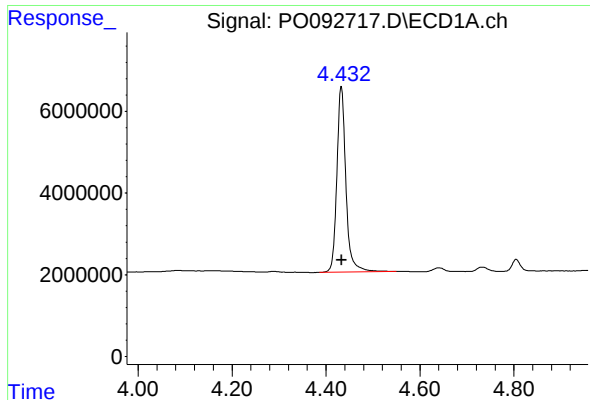

#1 Tetrachloro-m-xylene


R.T.: 4.433 min
Delta R.T.: -0.001 min
Response: 60643256
Conc: 20.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

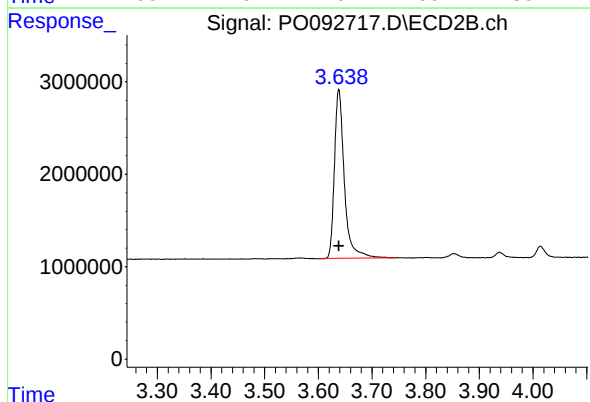


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 23549024
Conc: 18.47 ng/ml

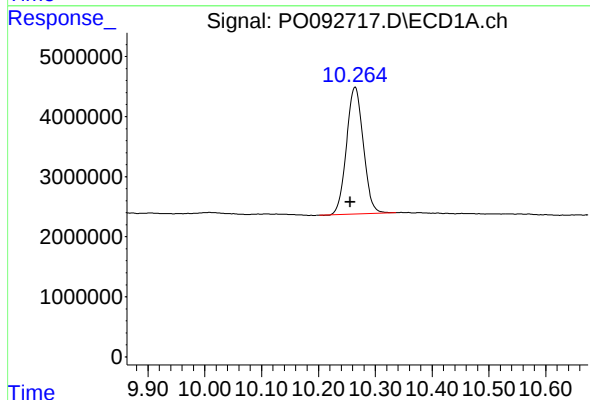


#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: 0.008 min
Response: 43269879
Conc: 22.50 ng/ml

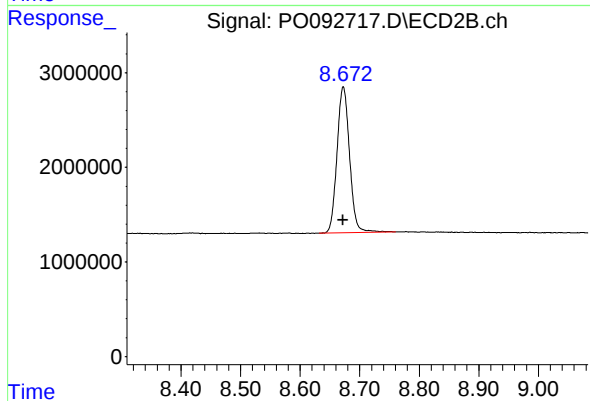

#2 Decachlorobiphenyl


R.T.: 8.672 min
Delta R.T.: 0.000 min
Response: 22533265
Conc: 19.34 ng/ml

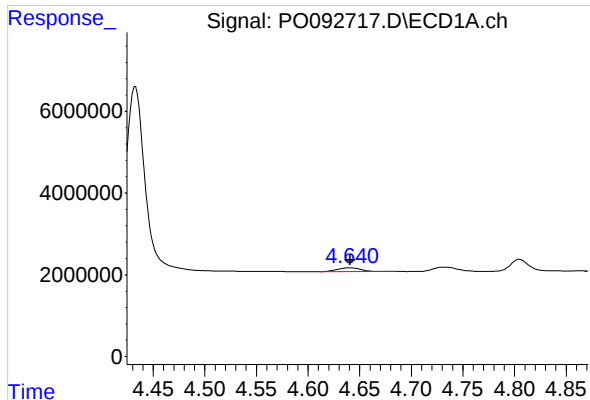

#8 AR-1221-1


R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 1511818
Conc: 38.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

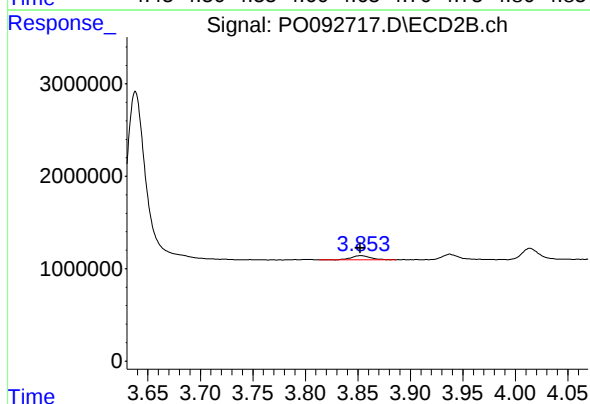


#8 AR-1221-1

R.T.: 3.853 min
Delta R.T.: 0.000 min
Response: 568108
Conc: 35.16 ng/ml

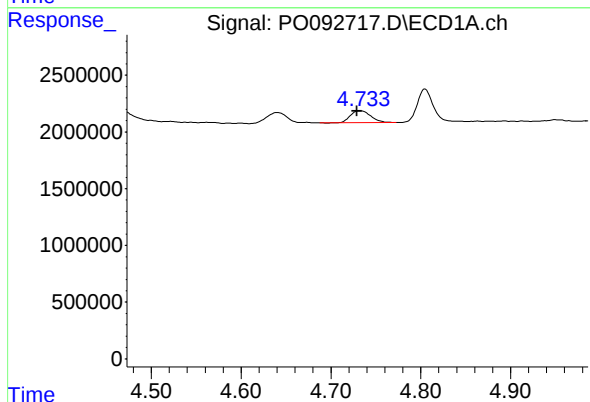


#9 AR-1221-2

R.T.: 4.734 min
Delta R.T.: 0.005 min
Response: 1632641
Conc: 56.74 ng/ml

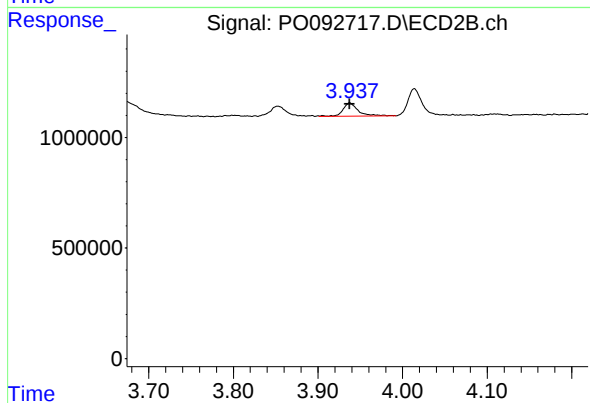

#9 AR-1221-2


R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 744892
Conc: 61.53 ng/ml

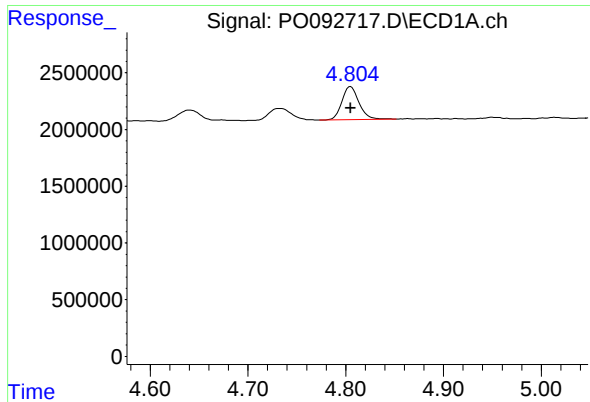

#10 AR-1221-3

R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 3553724
Conc: 40.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

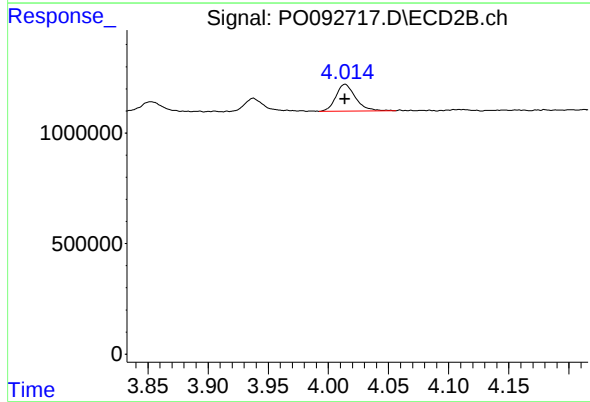

#10 AR-1221-3

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 1388861
Conc: 37.30 ng/ml