

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022423\
 Data File : P0092759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2023 07:26
 Operator : YP/AJ
 Sample : 01627-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 08:37:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 22 05:46:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.636	64172517	25268120	21.371	19.823
2) SA Decachlor...	10.263	8.670	45410972	24167853	23.609	20.738
Target Compounds						
8) L2 AR-1221-1	4.639	3.851	926887	422198	23.450	26.132
9) L2 AR-1221-2	4.734	3.935	1369052	563512	47.581	46.545
10) L2 AR-1221-3	4.803	4.012	2339054	931040	26.559	25.005



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022423\
Data File : PO092759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2023 07:26
Operator : YP/AJ
Sample : 01627-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 08:37:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022123.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 22 05:46:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

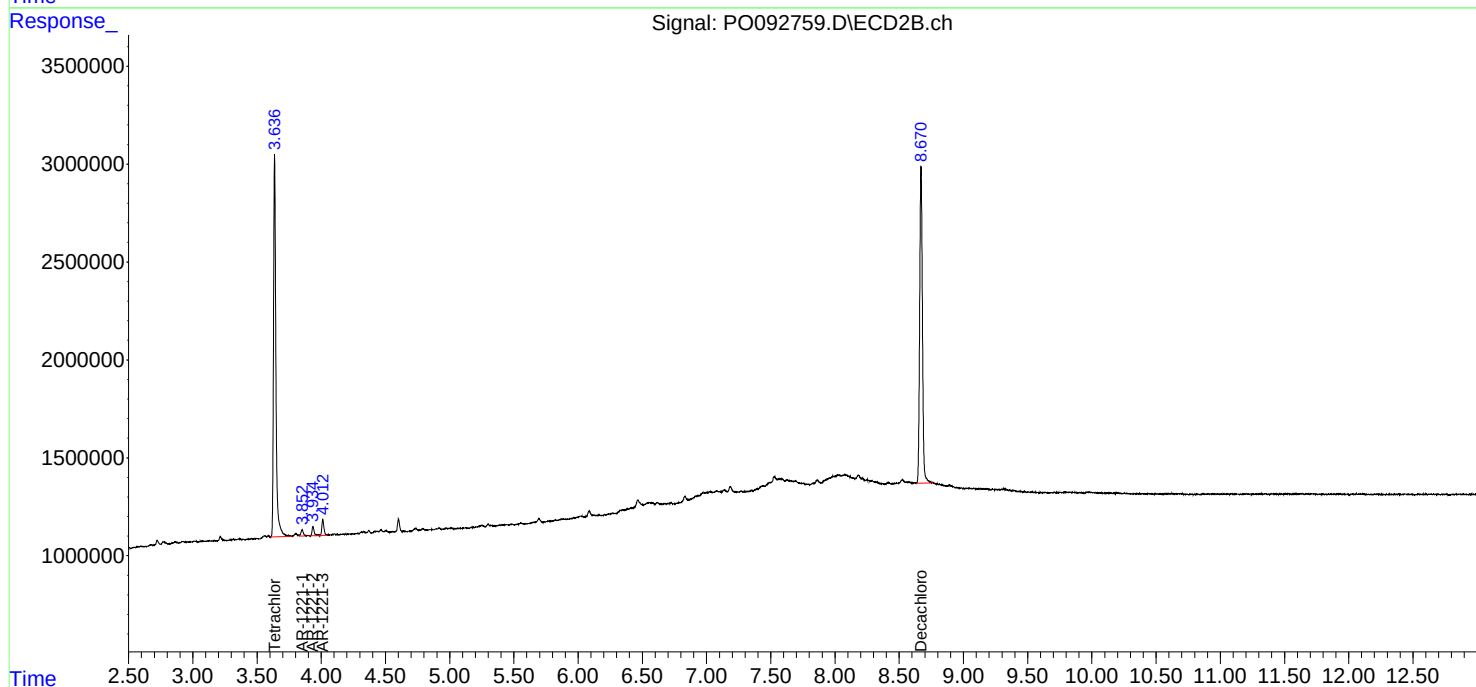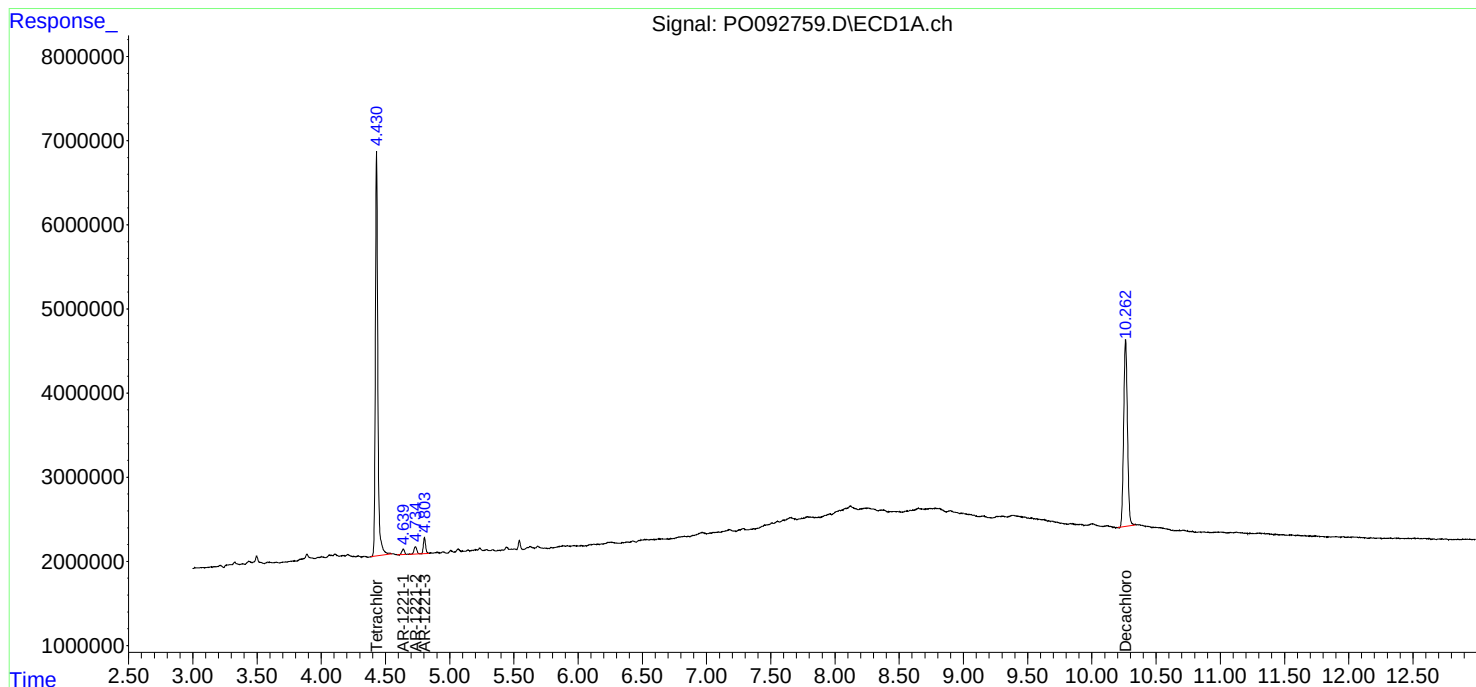


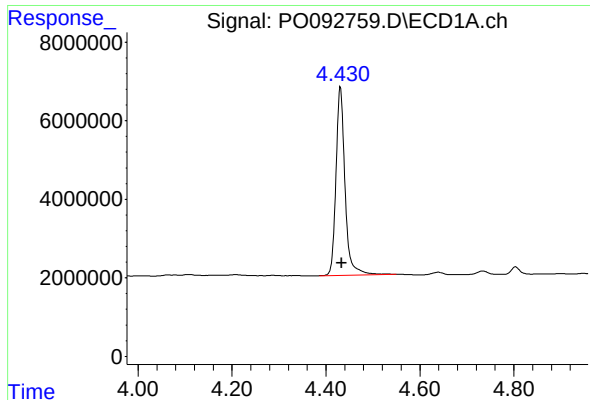

#1 Tetrachloro-m-xylene


R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 64172517
Conc: 21.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2023

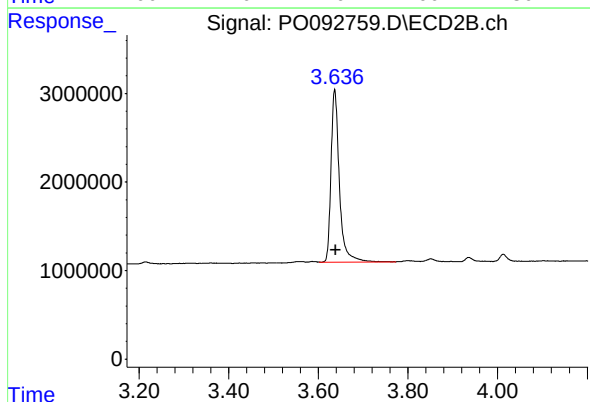


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 25268120
Conc: 19.82 ng/ml

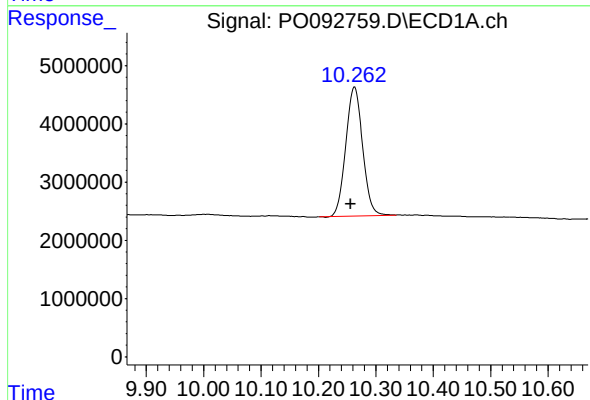


#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: 0.006 min
Response: 45410972
Conc: 23.61 ng/ml

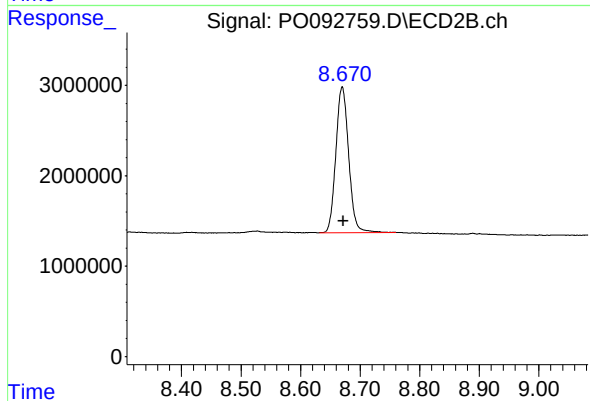

#2 Decachlorobiphenyl


R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 24167853
Conc: 20.74 ng/ml

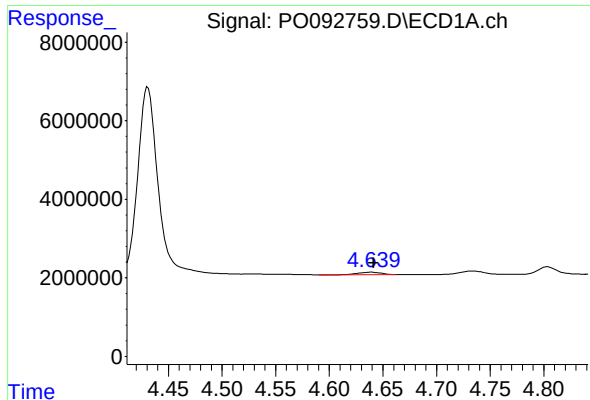

#8 AR-1221-1


R.T.: 4.639 min
Delta R.T.: -0.002 min
Response: 926887
Conc: 23.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2023

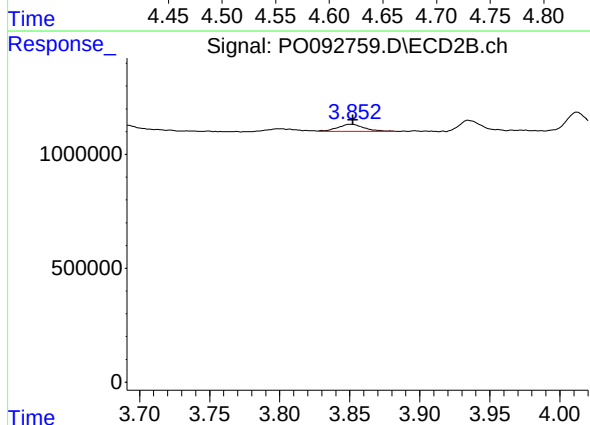


#8 AR-1221-1

R.T.: 3.851 min
Delta R.T.: -0.001 min
Response: 422198
Conc: 26.13 ng/ml

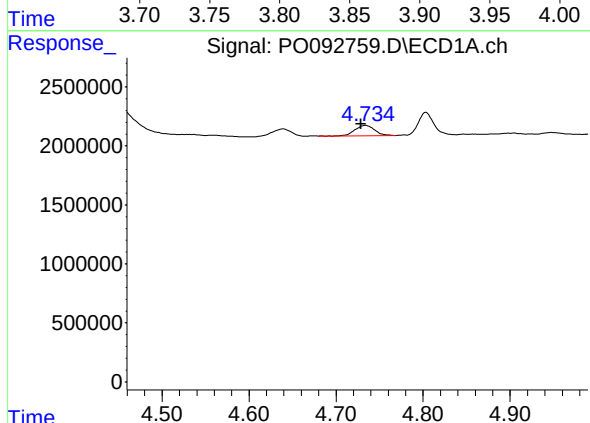


#9 AR-1221-2

R.T.: 4.734 min
Delta R.T.: 0.005 min
Response: 1369052
Conc: 47.58 ng/ml

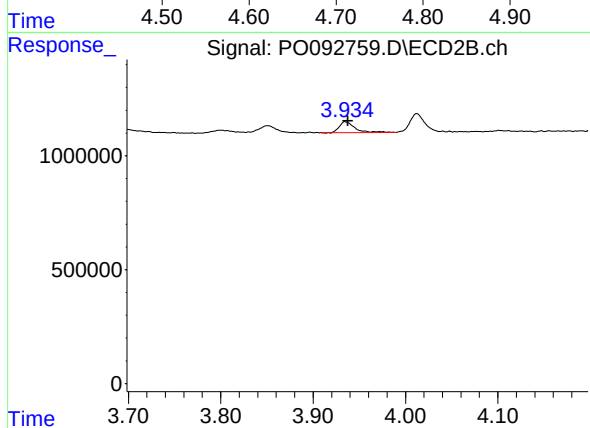

#9 AR-1221-2


R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 563512
Conc: 46.54 ng/ml

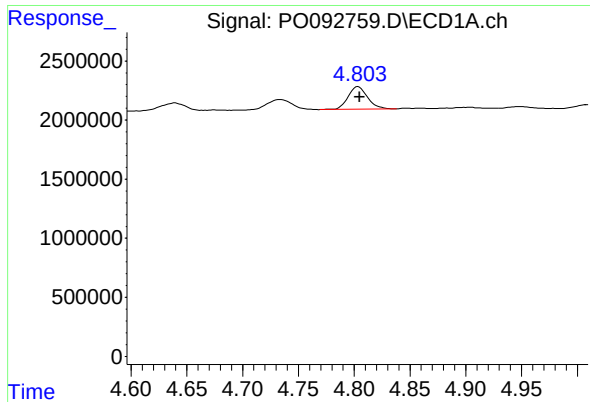

#10 AR-1221-3

R.T.: 4.803 min
Delta R.T.: -0.002 min
Response: 2339054
Conc: 26.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2023

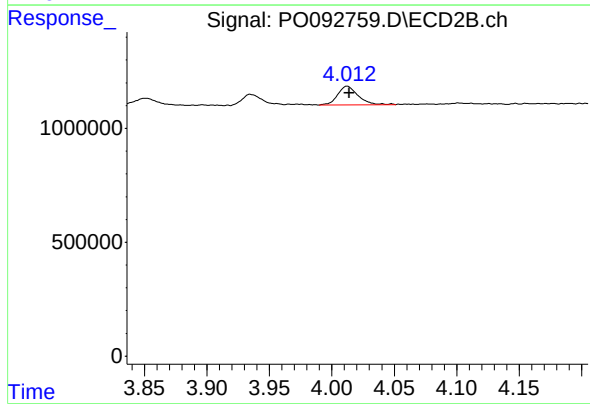

#10 AR-1221-3

R.T.: 4.012 min
Delta R.T.: -0.001 min
Response: 931040
Conc: 25.00 ng/ml