

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022624\
 Data File : P0102091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2024 20:01
 Operator : YP/AJ
 Sample : P1564-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LKWD-BACKFILL-14

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/27/2024
 Supervised By :Ankita Jodhani 02/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:13:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.391	95780352	65308360	20.653	20.098
2) SA Decachlor...	9.830	8.266	48781276	37950285	19.157m	18.344

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022624\
Data File : PO102091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2024 20:01
Operator : YP/AJ
Sample : P1564-11
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LKWD-BACKFILL-14


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2024
Supervised By :Ankita Jodhani 02/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:13:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

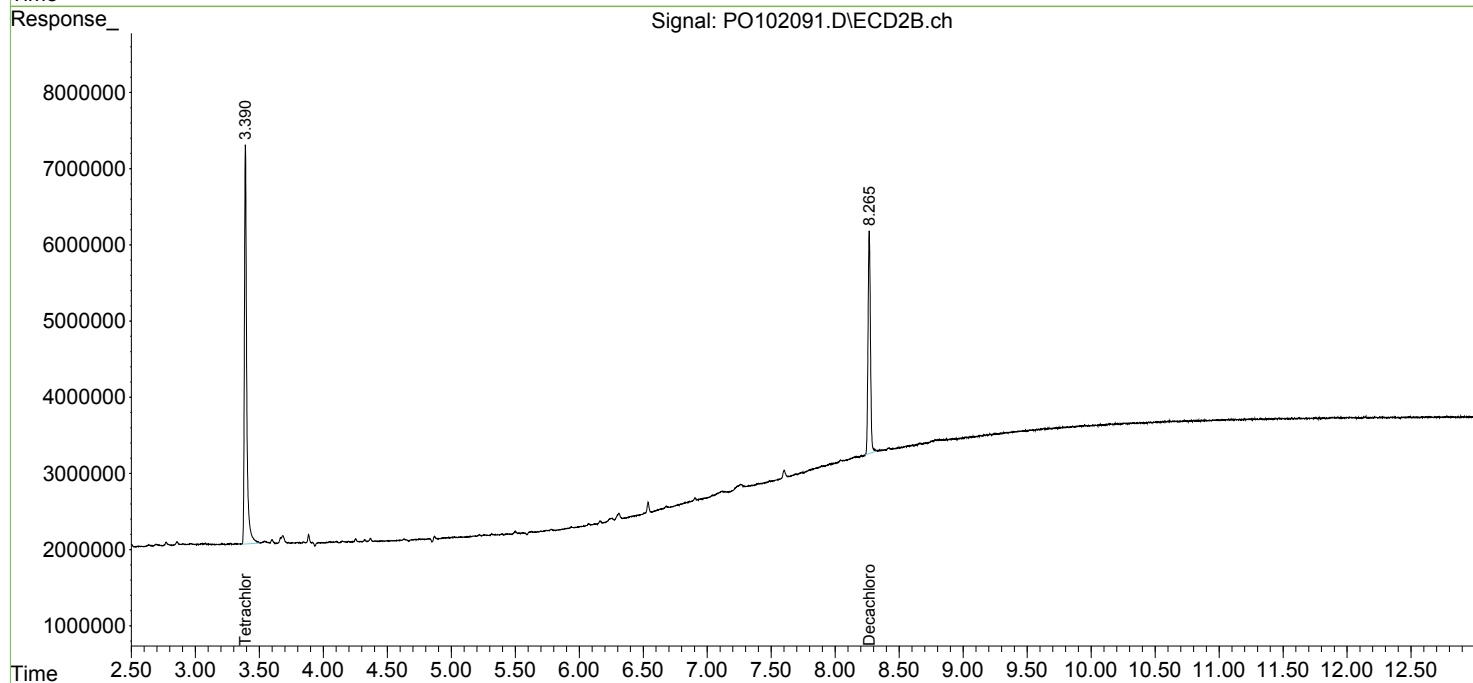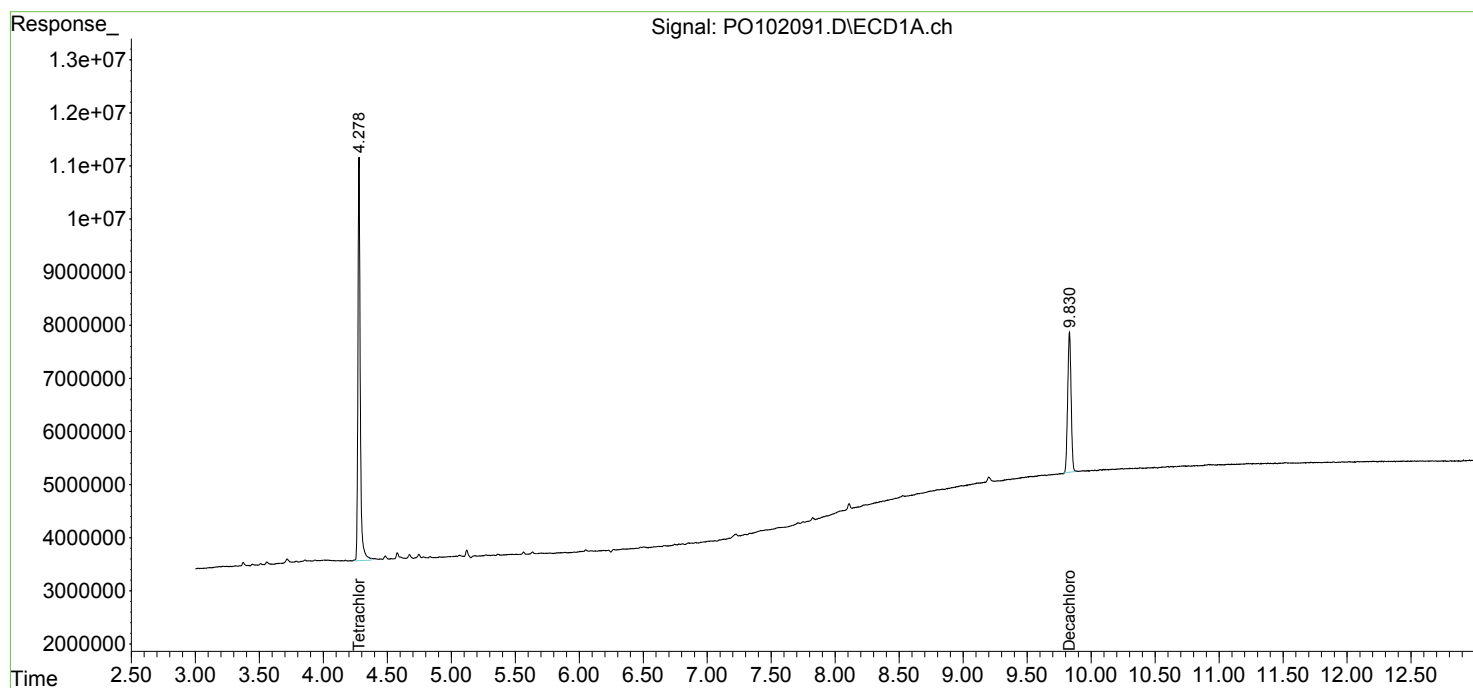

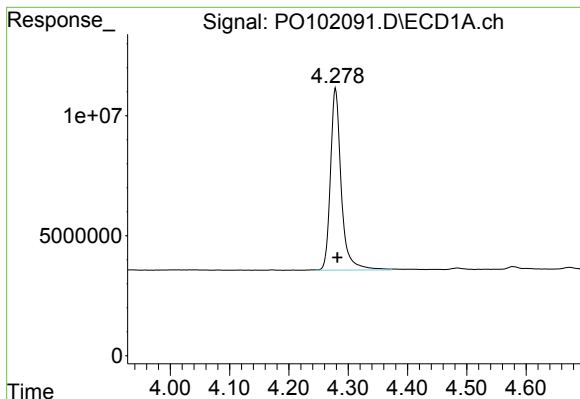

#1 Tetrachloro-m-xylene

R.T.: 4.279 min
Delta R.T.: -0.003 min
Response: 95780352
Conc: 20.65 ng/ml


Instrument :

ECD_O

ClientSampleId :
LKWD-BACKFILL-14


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2024
Supervised By :Ankita Jodhani 02/27/2024

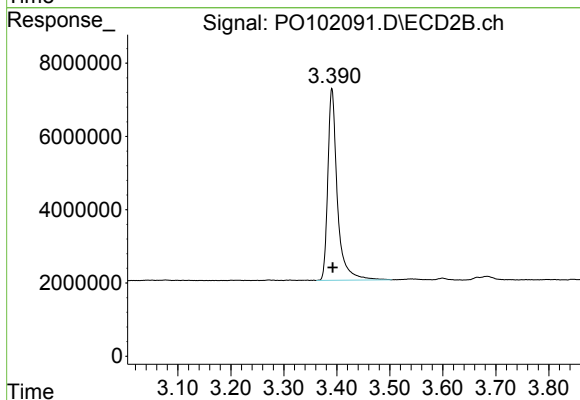


#1 Tetrachloro-m-xylene

R.T.: 3.391 min
Delta R.T.: -0.001 min
Response: 65308360
Conc: 20.10 ng/ml

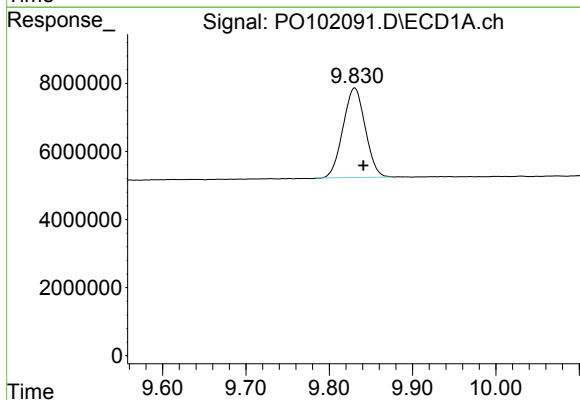

#2 Decachlorobiphenyl

R.T.: 9.830 min
Delta R.T.: -0.011 min
Response: 48781276
Conc: 19.16 ng/ml m

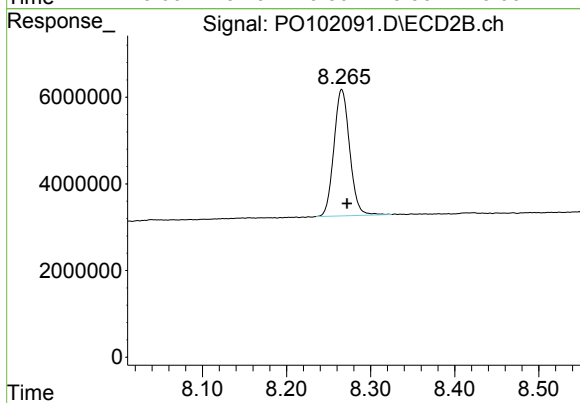

#2 Decachlorobiphenyl

R.T.: 8.266 min
Delta R.T.: -0.006 min
Response: 37950285
Conc: 18.34 ng/ml