

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
 Data File : P0054090.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Feb 2019 16:56
 Operator : SM/SJ
 Sample : K1350-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-022619-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:18:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.048	3.130	37539236	5061401	17.503	19.743
2) SA Decachlor...	9.383	7.707	16324280	3359057	14.959	12.643

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
Data File : P0054090.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2019 16:56
Operator : SM/SJ
Sample : K1350-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EO-01-022619-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:18:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

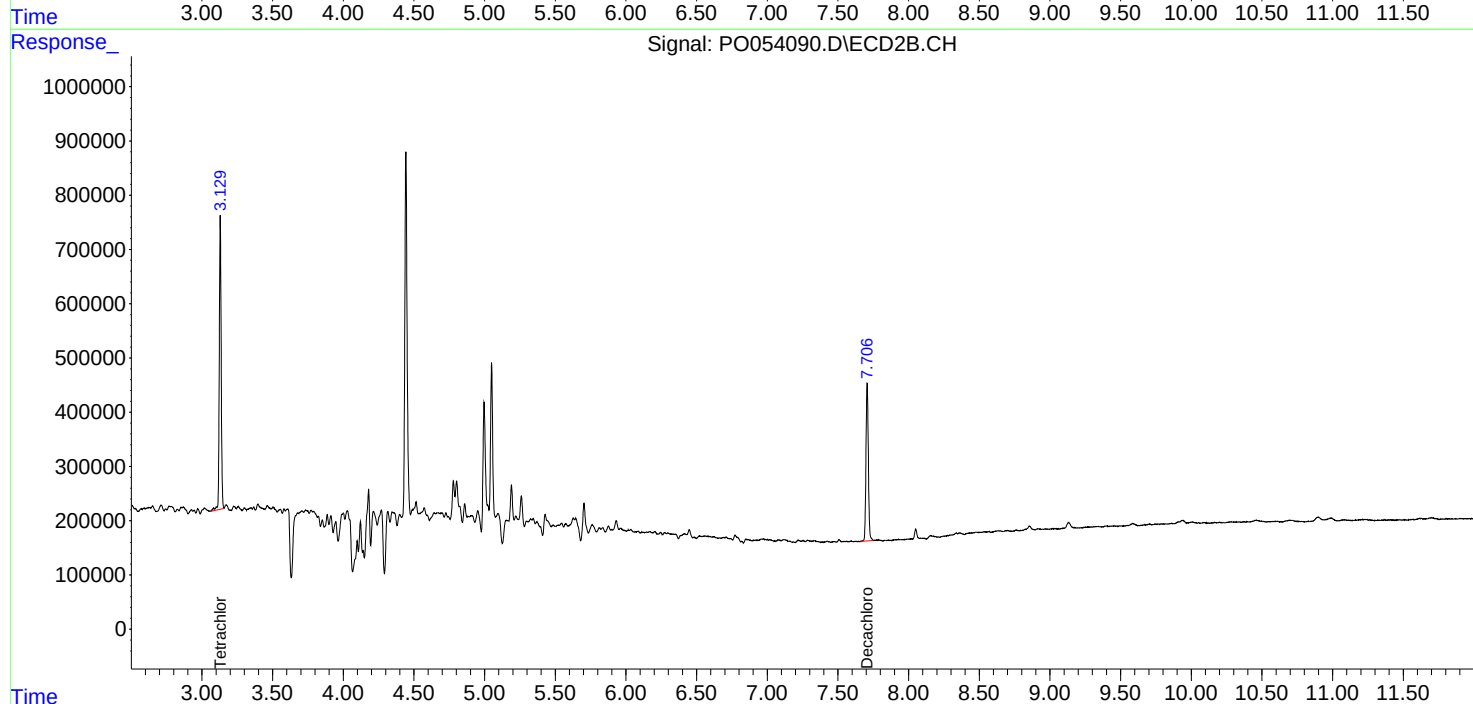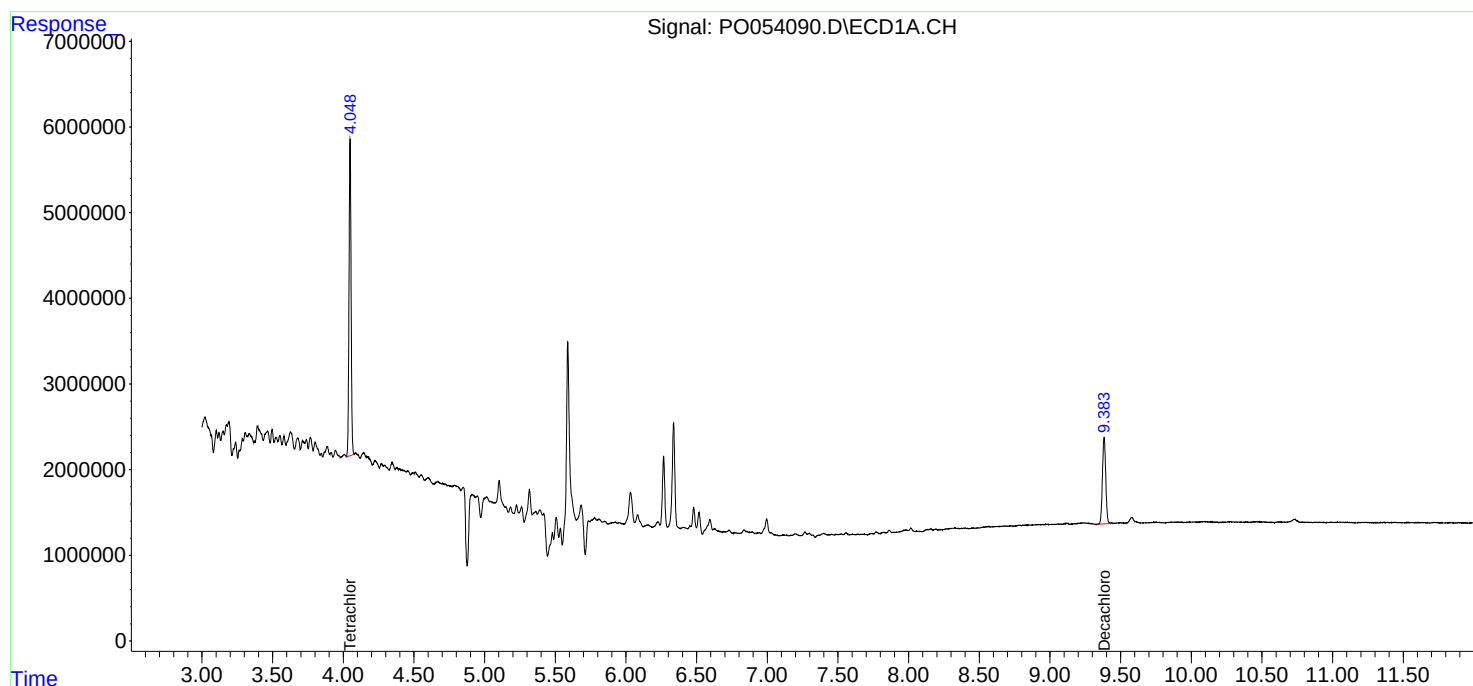


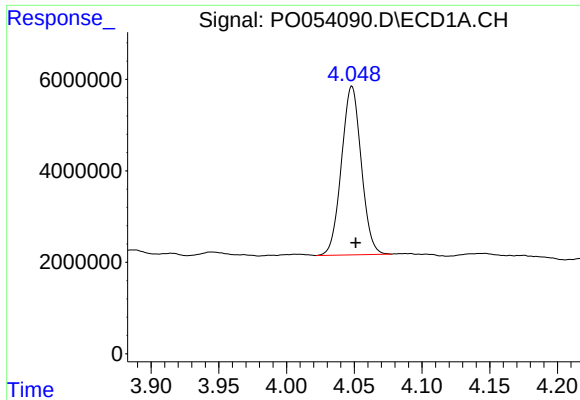

#1 Tetrachloro-m-xylene


R.T.: 4.048 min
Delta R.T.: -0.003 min
Response: 37539236
Conc: 17.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-01-022619-A

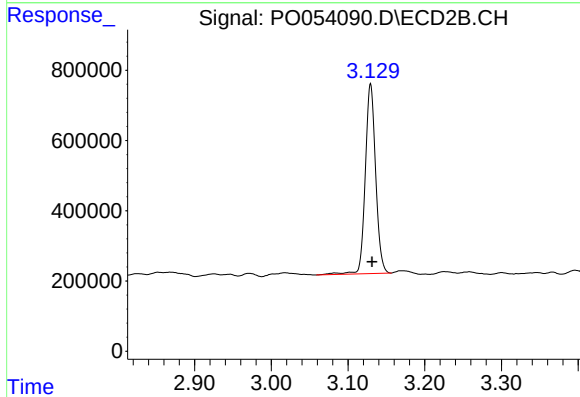


#1 Tetrachloro-m-xylene

R.T.: 3.130 min
Delta R.T.: -0.002 min
Response: 5061401
Conc: 19.74 ng/ml

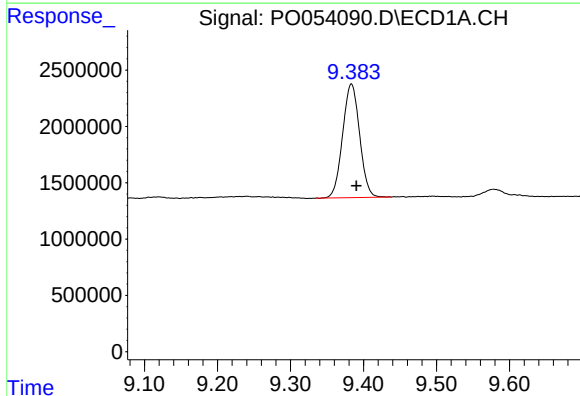

#2 Decachlorobiphenyl

R.T.: 9.383 min
Delta R.T.: -0.007 min
Response: 16324280
Conc: 14.96 ng/ml

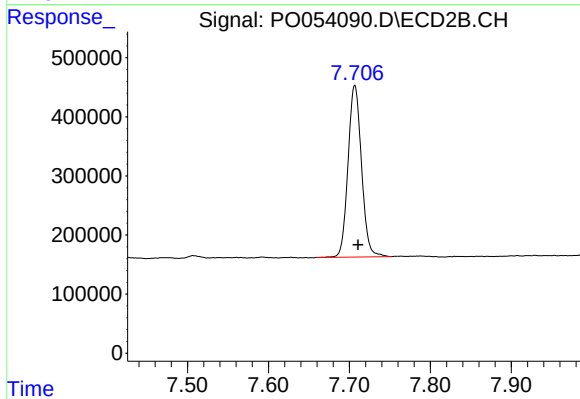

#2 Decachlorobiphenyl

R.T.: 7.707 min
Delta R.T.: -0.004 min
Response: 3359057
Conc: 12.64 ng/ml