

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
 Data File : P0054100.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Feb 2019 19:45
 Operator : SM/SJ
 Sample : K1627-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-01-(6-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:22:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.047	3.129	62441765	6401286	29.113	24.969
2) SA Decachlor...	9.380	7.706	17699205	4049406	16.219	15.242

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
Data File : P0054100.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2019 19:45
Operator : SM/SJ
Sample : K1627-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-01-(6-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:22:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

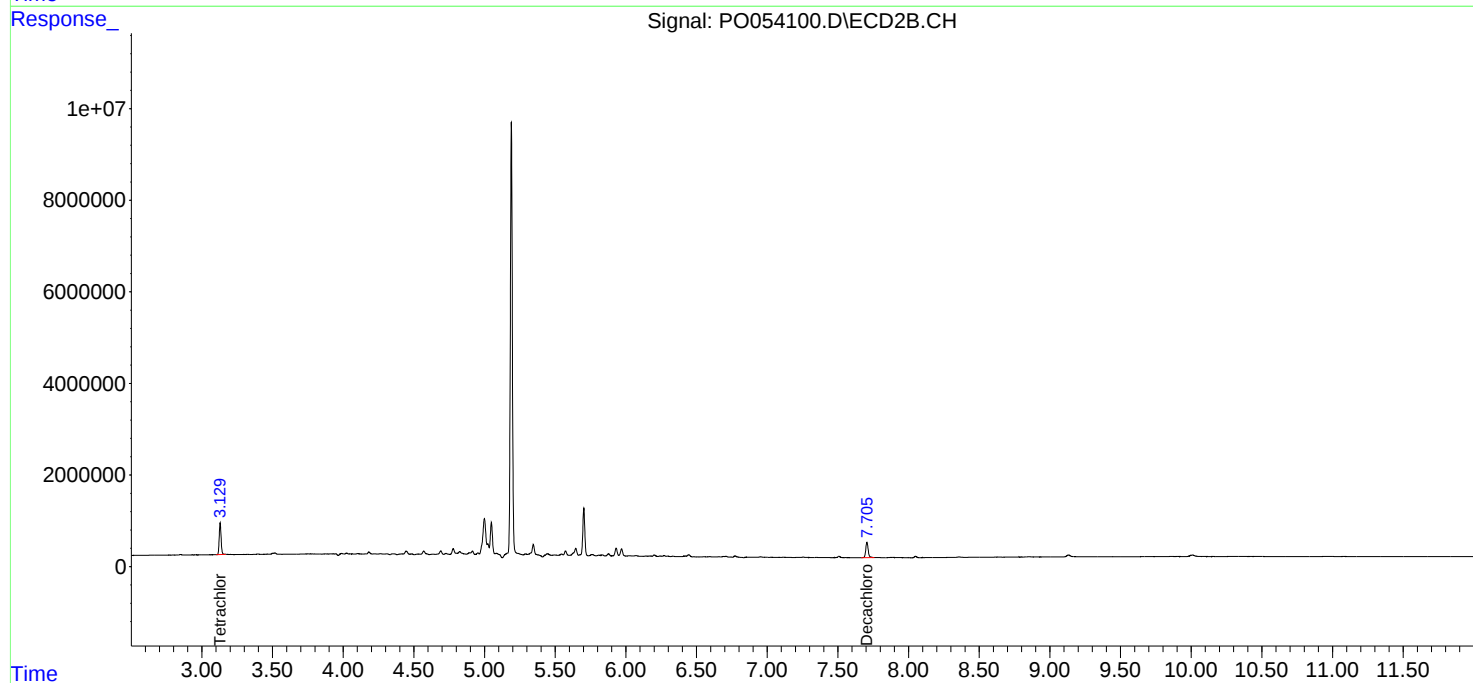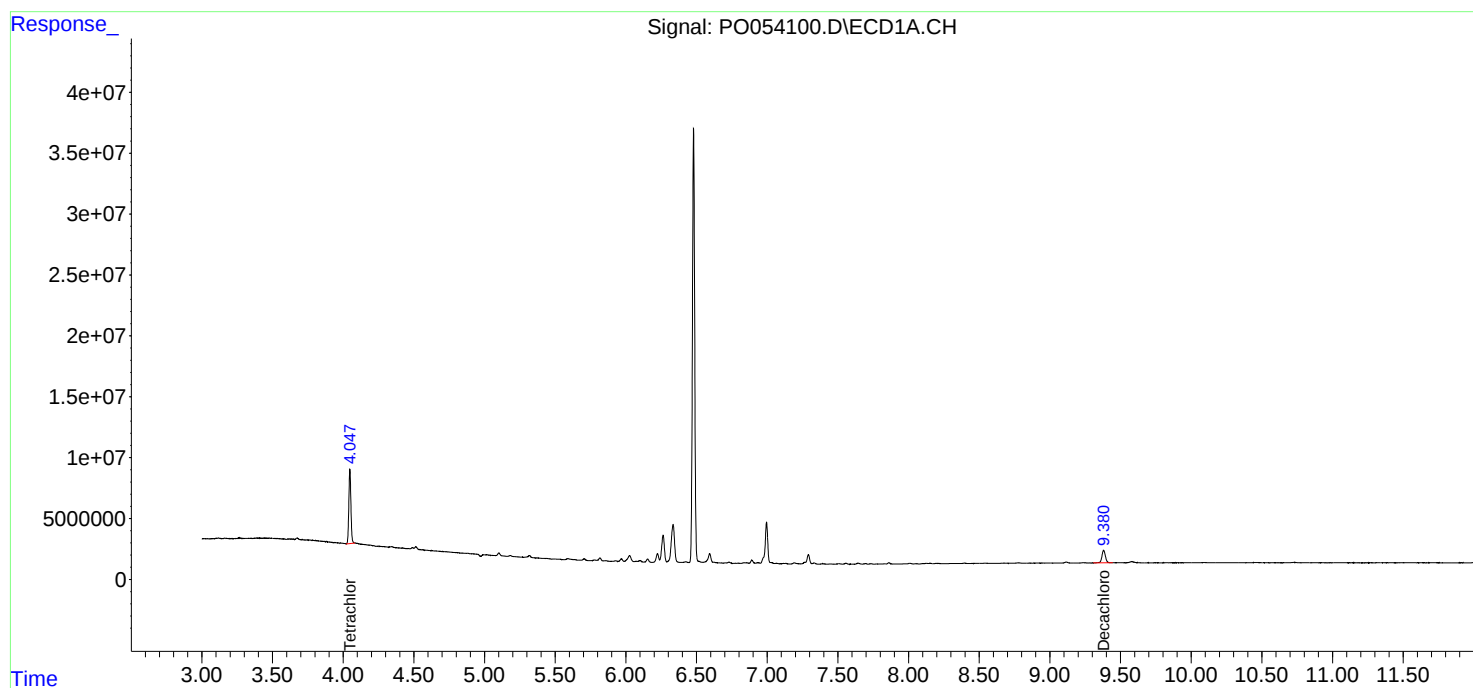


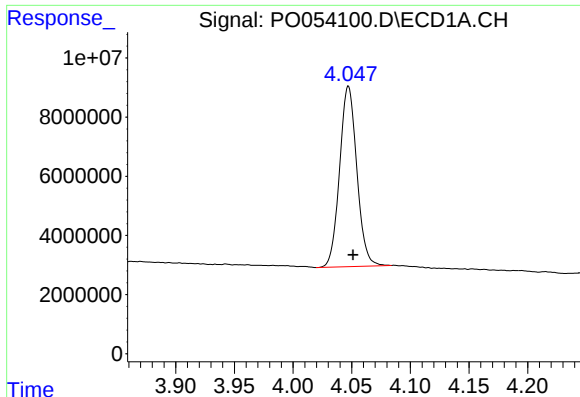

#1 Tetrachloro-m-xylene


R.T.: 4.047 min
Delta R.T.: -0.004 min
Response: 62441765
Conc: 29.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-(6-2)

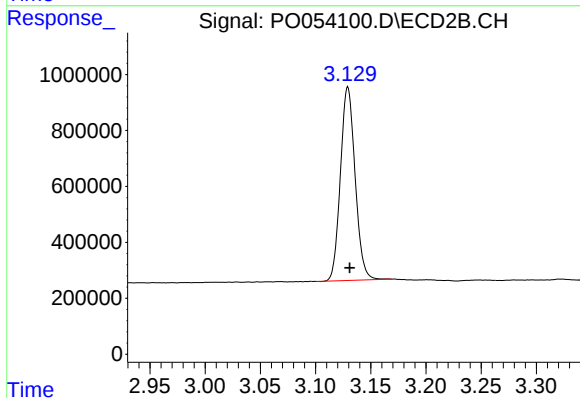


#1 Tetrachloro-m-xylene

R.T.: 3.129 min
Delta R.T.: -0.002 min
Response: 6401286
Conc: 24.97 ng/ml

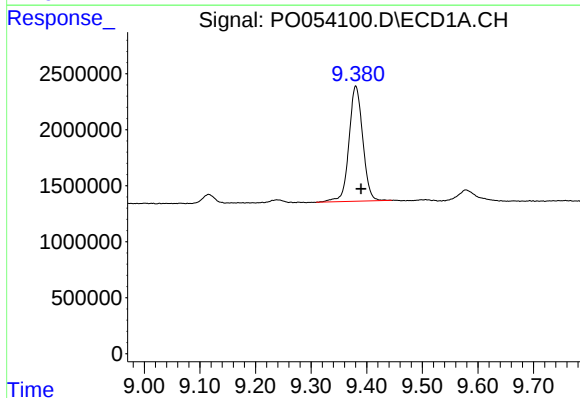

#2 Decachlorobiphenyl

R.T.: 9.380 min
Delta R.T.: -0.010 min
Response: 17699205
Conc: 16.22 ng/ml

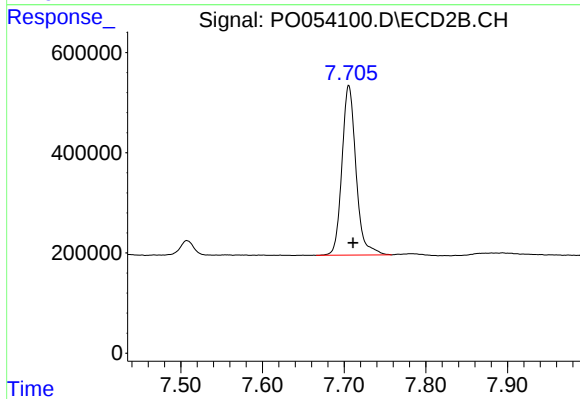

#2 Decachlorobiphenyl

R.T.: 7.706 min
Delta R.T.: -0.005 min
Response: 4049406
Conc: 15.24 ng/ml