

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
 Data File : P0054101.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Feb 2019 20:02
 Operator : SM/SJ
 Sample : K1627-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-02-(2-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:22:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.048	3.130	48224804	5104674	22.485	19.911
2) SA Decachlor...	9.383	7.706	15853236	3734937	14.527	14.058

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
Data File : P0054101.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2019 20:02
Operator : SM/SJ
Sample : K1627-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-02-(2-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:22:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

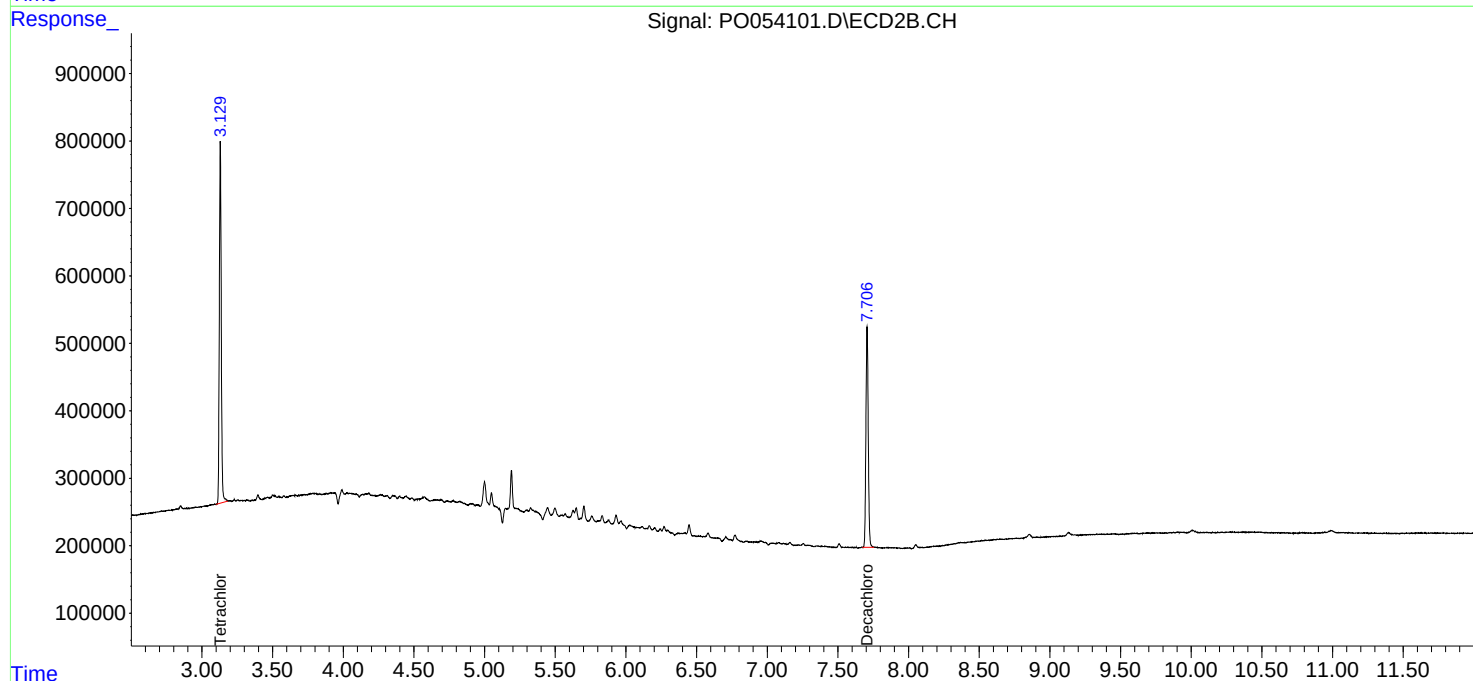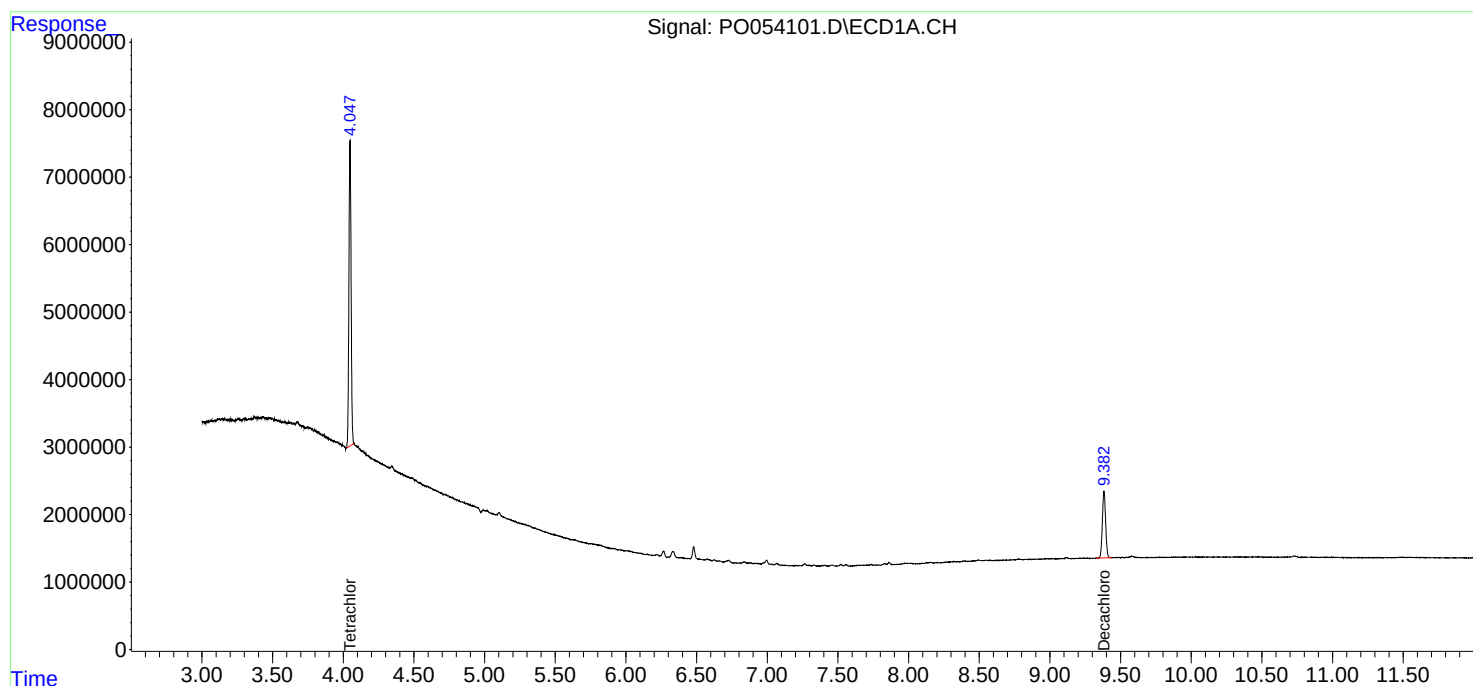


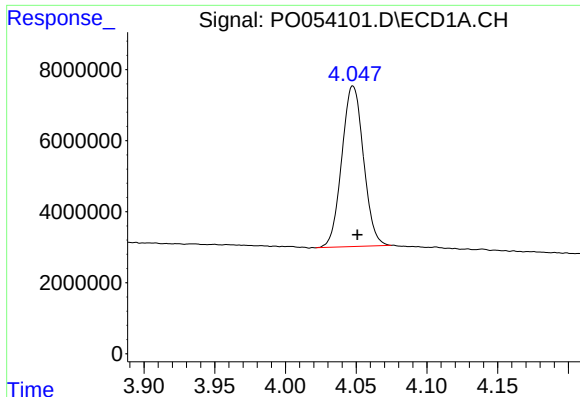

#1 Tetrachloro-m-xylene


R.T.: 4.048 min
Delta R.T.: -0.003 min
Response: 48224804
Conc: 22.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-(2-5)

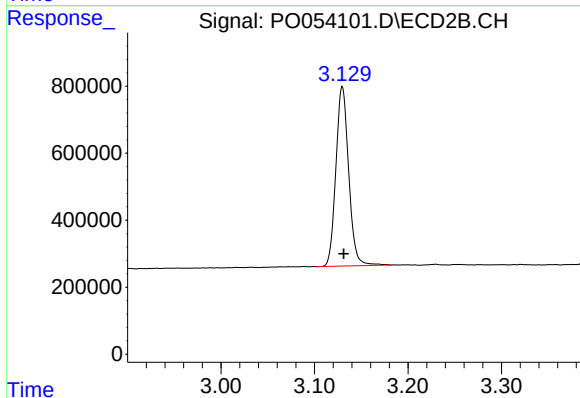


#1 Tetrachloro-m-xylene

R.T.: 3.130 min
Delta R.T.: -0.001 min
Response: 5104674
Conc: 19.91 ng/ml

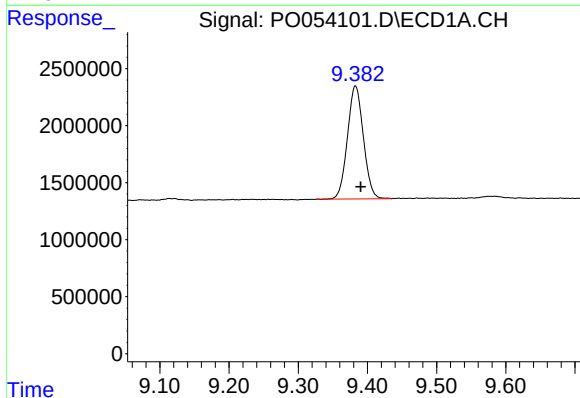

#2 Decachlorobiphenyl

R.T.: 9.383 min
Delta R.T.: -0.008 min
Response: 15853236
Conc: 14.53 ng/ml

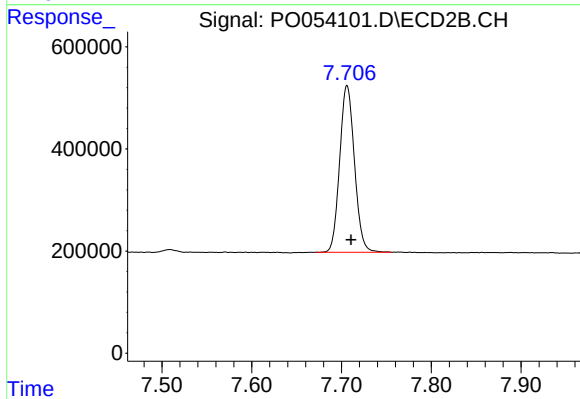

#2 Decachlorobiphenyl

R.T.: 7.706 min
Delta R.T.: -0.005 min
Response: 3734937
Conc: 14.06 ng/ml