

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022719\
 Data File : P0054110.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Feb 2019 22:34
 Operator : SM/SJ
 Sample : K1632-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 50153

Manual Integrations
 APPROVED

Sohil
 2/28/2019 11:52:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:24:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.047	3.130	38474125	4736336	17.938m	18.475m
2) SA Decachlor...	9.387	7.712	19733809	4028641	18.083	15.163

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022719\
Data File : PO054110.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2019 22:34
Operator : SM/SJ
Sample : K1632-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
50153


Manual Integrations
APPROVED

Sohil
2/28/2019 11:52:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:24:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

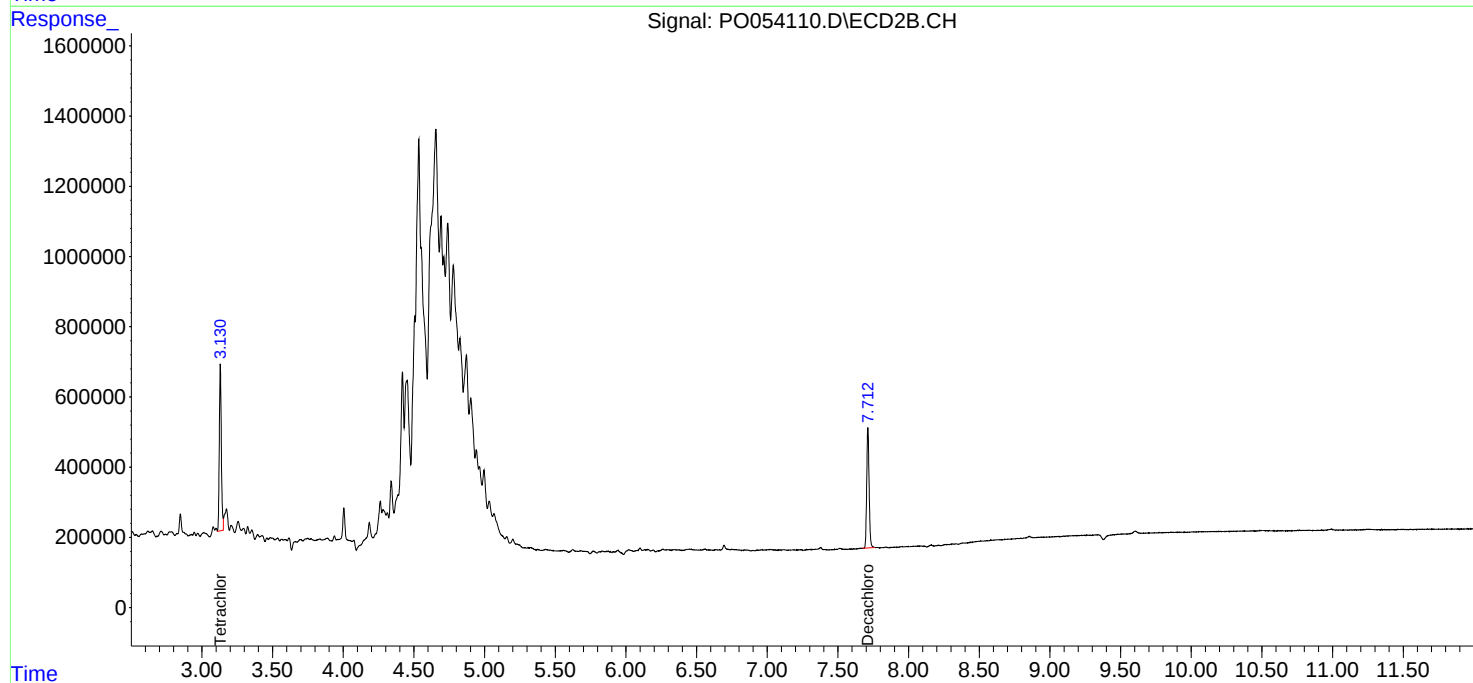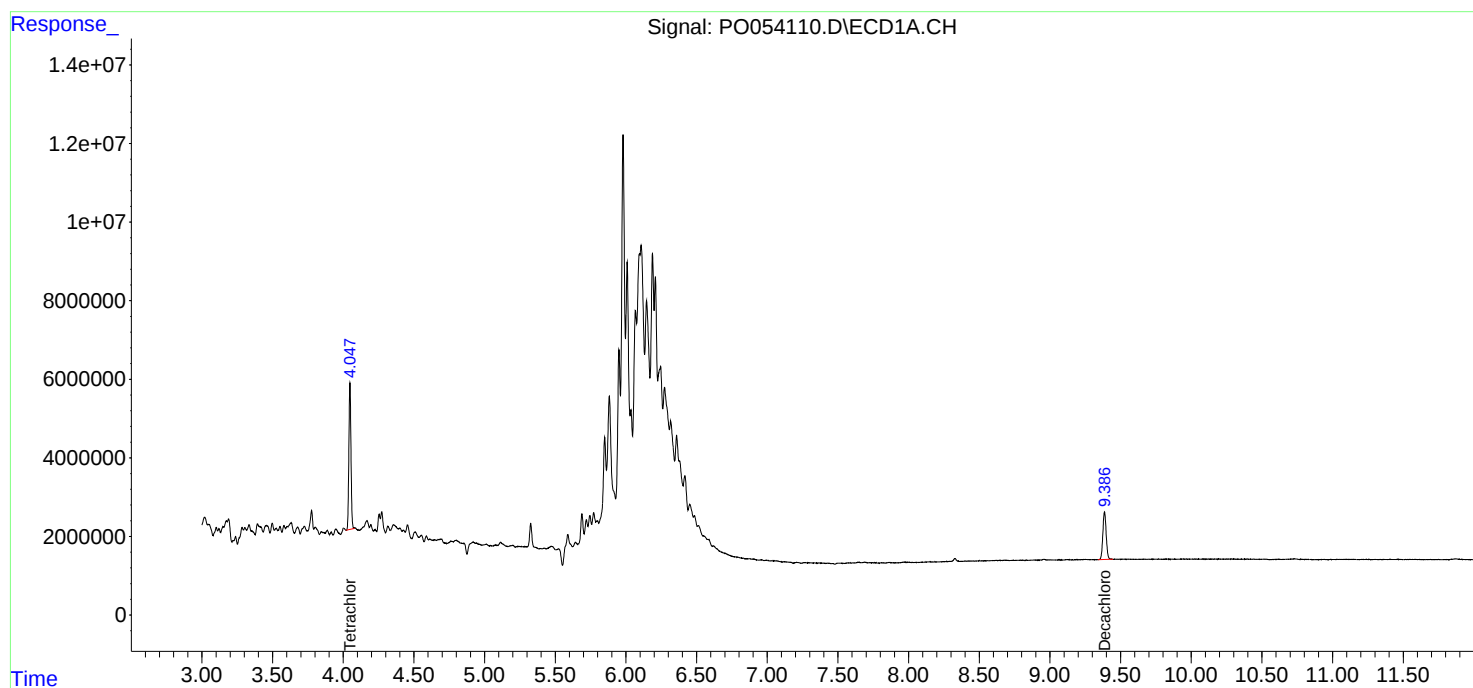

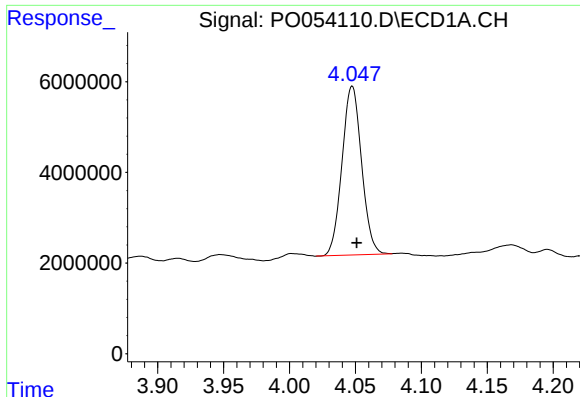


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: -0.004 min
Response: 38474125
Conc: 17.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
50153


Manual Integrations
APPROVED

Sohil
2/28/2019 11:52:46 AM

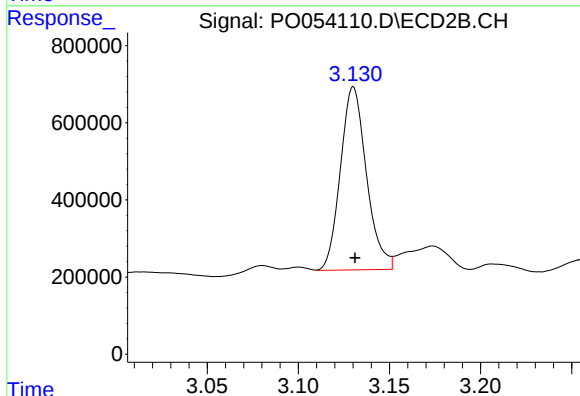


#1 Tetrachloro-m-xylene

R.T.: 3.130 min
Delta R.T.: -0.001 min
Response: 4736336
Conc: 18.47 ng/ml m

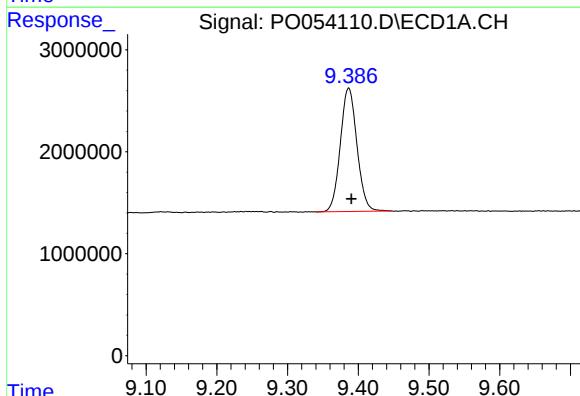

#2 Decachlorobiphenyl

R.T.: 9.387 min
Delta R.T.: -0.004 min
Response: 19733809
Conc: 18.08 ng/ml

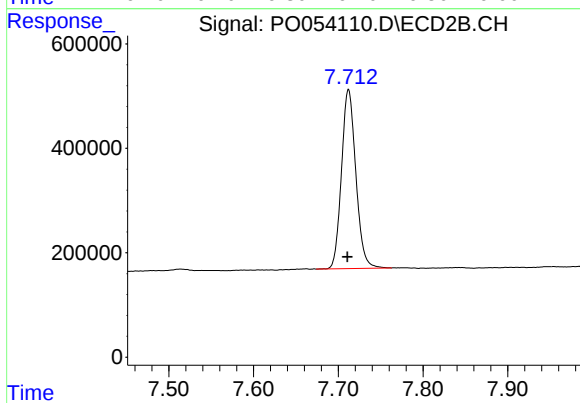

#2 Decachlorobiphenyl

R.T.: 7.712 min
Delta R.T.: 0.001 min
Response: 4028641
Conc: 15.16 ng/ml