

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022724\
 Data File : P0102125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 15:16
 Operator : YP/AJ
 Sample : P1600-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPEEDY-DRY-DRUM

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/28/2024
 Supervised By :Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:24:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.283	3.403	51488109	29234192	11.102m	8.997
2) SA Decachlor...	9.832	8.269	46513273	27037704	18.266	13.069 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO022724\
Data File : PO102125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 15:16
Operator : YP/AJ
Sample : P1600-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SPEEDY-DRY-DRUM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/28/2024
Supervised By :Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:24:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

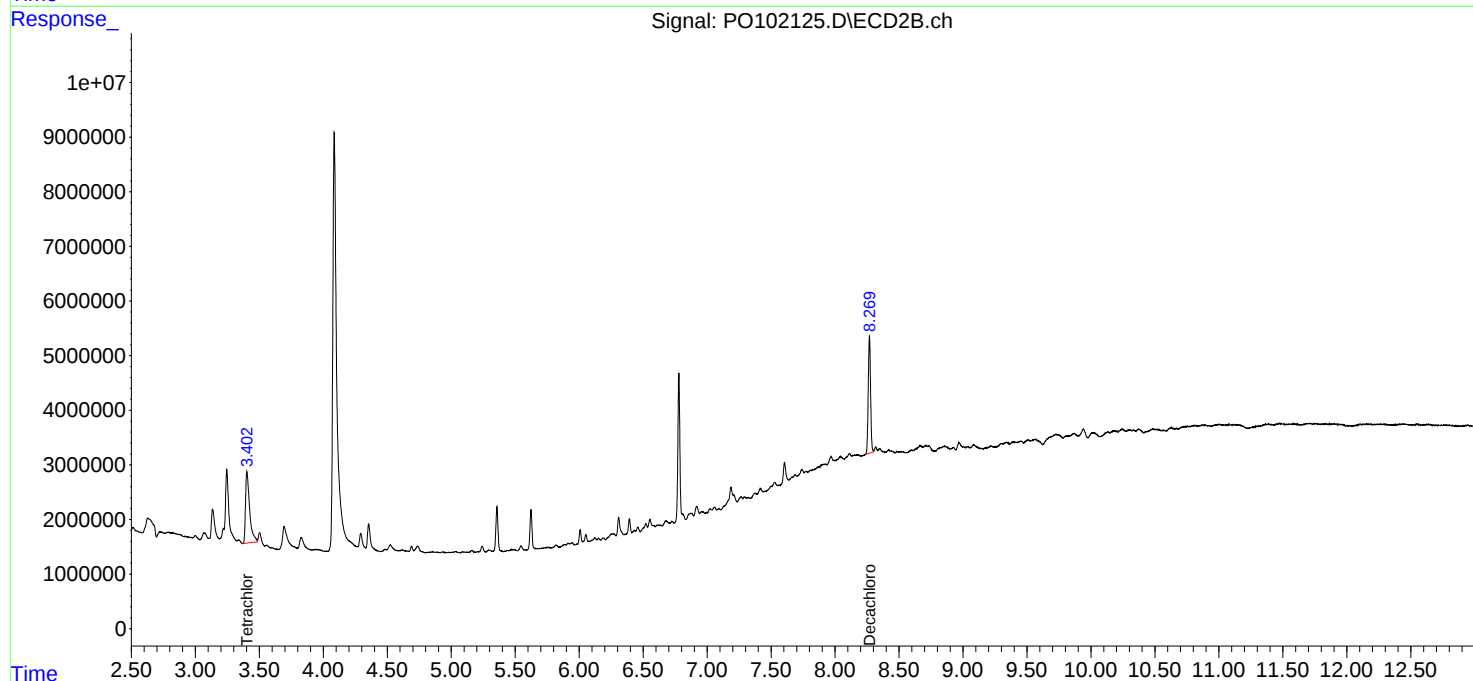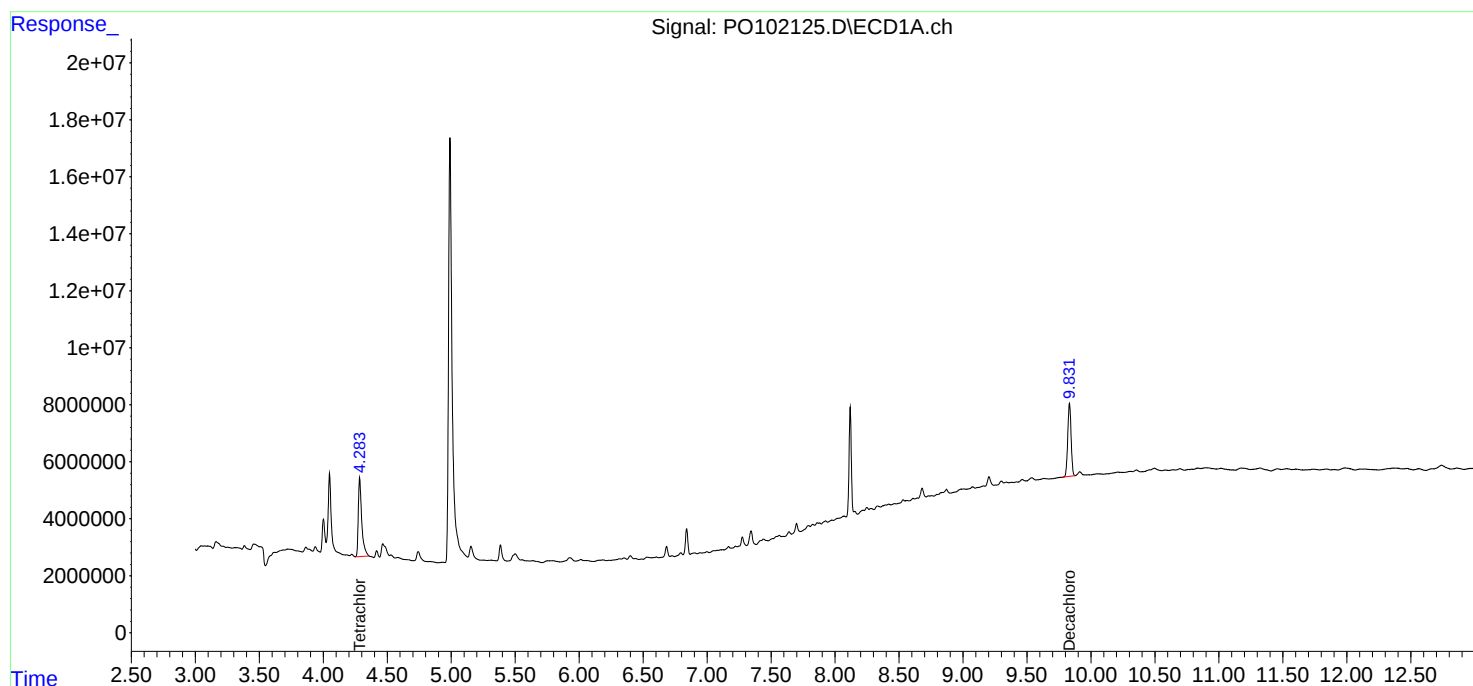

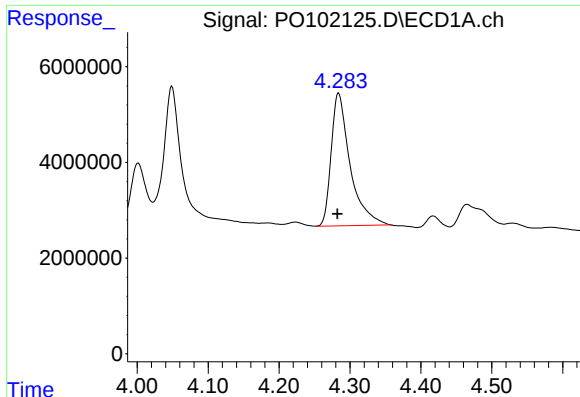

#1 Tetrachloro-m-xylene

R.T.: 4.283 min
Delta R.T.: 0.001 min
Response: 51488109
Conc: 11.10 ng/ml

Instrument :

ECD_O


ClientSampleId :

SPEEDY-DRY-DRUM

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 02/28/2024
Supervised By :Ankita Jodhani 02/28/2024

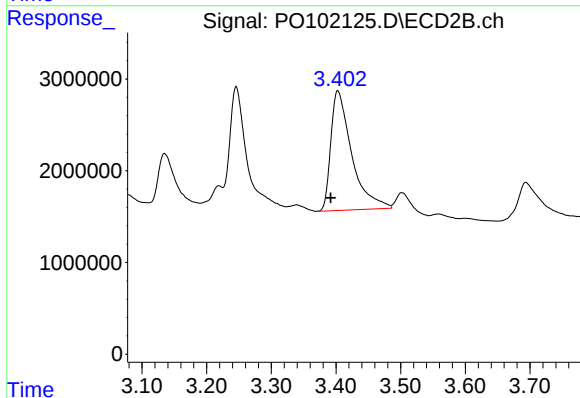


#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.011 min
Response: 29234192
Conc: 9.00 ng/ml

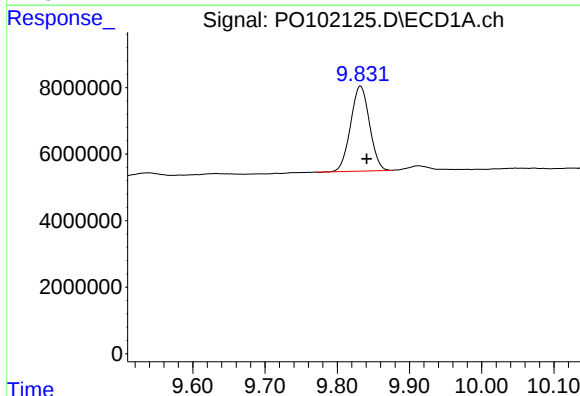

#2 Decachlorobiphenyl

R.T.: 9.832 min
Delta R.T.: -0.009 min
Response: 46513273
Conc: 18.27 ng/ml

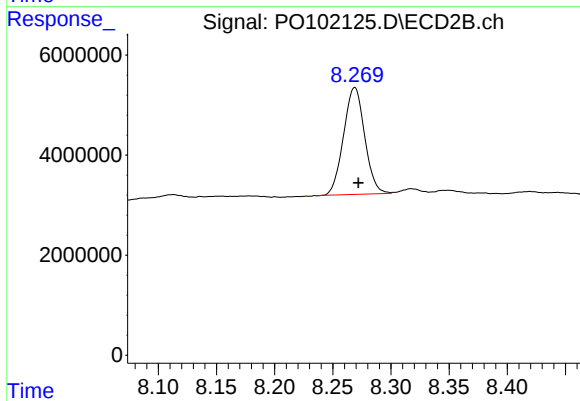

#2 Decachlorobiphenyl

R.T.: 8.269 min
Delta R.T.: -0.003 min
Response: 27037704
Conc: 13.07 ng/ml