

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022724\
 Data File : P0102153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2024 00:42
 Operator : YP/AJ
 Sample : P1583-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MANHOLE-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/28/2024
 Supervised By :Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 01:07:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.278	3.391	79880170	54476220	17.225m	16.765
2) SA Decachlor...	9.830	8.265	36085650	25357559	14.171	12.257

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO022724\
Data File : PO102153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2024 00:42
Operator : YP/AJ
Sample : P1583-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
MANHOLE-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/28/2024
Supervised By :Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 01:07:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

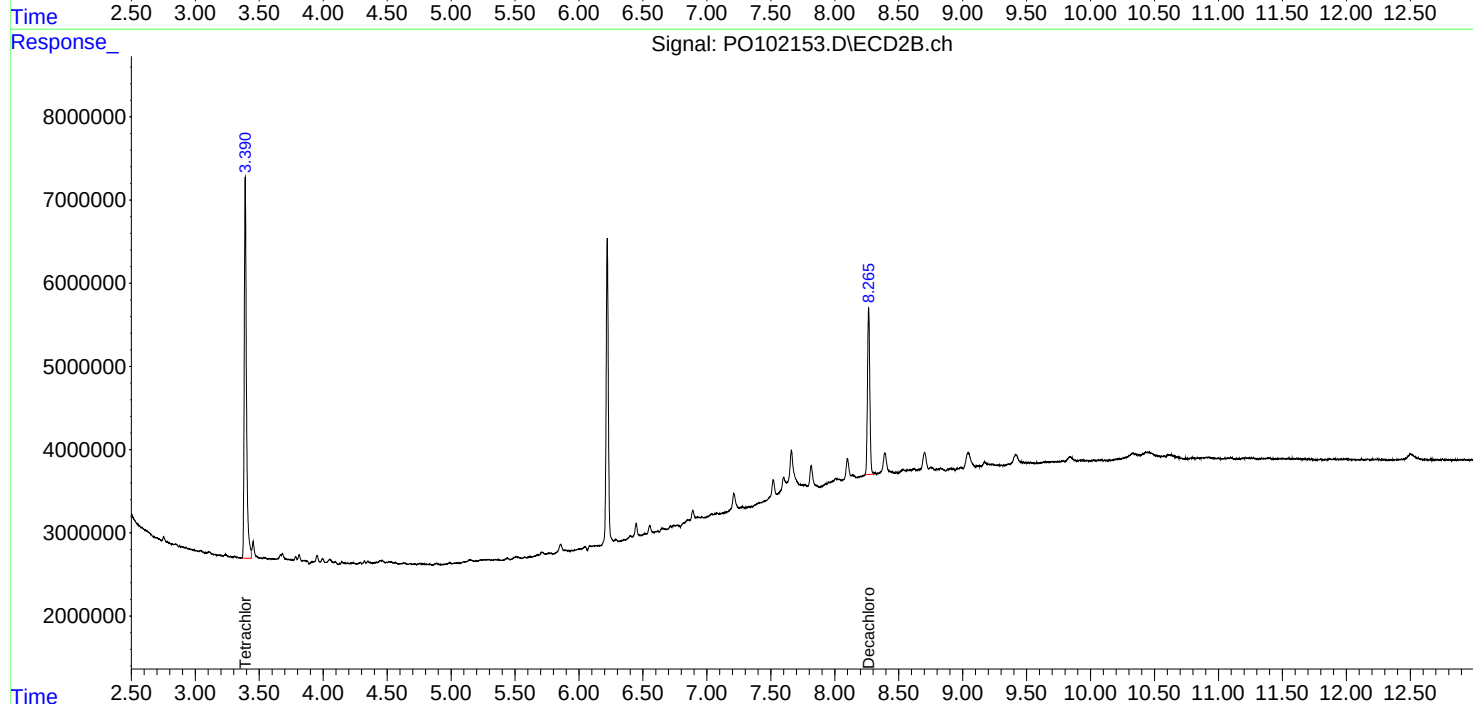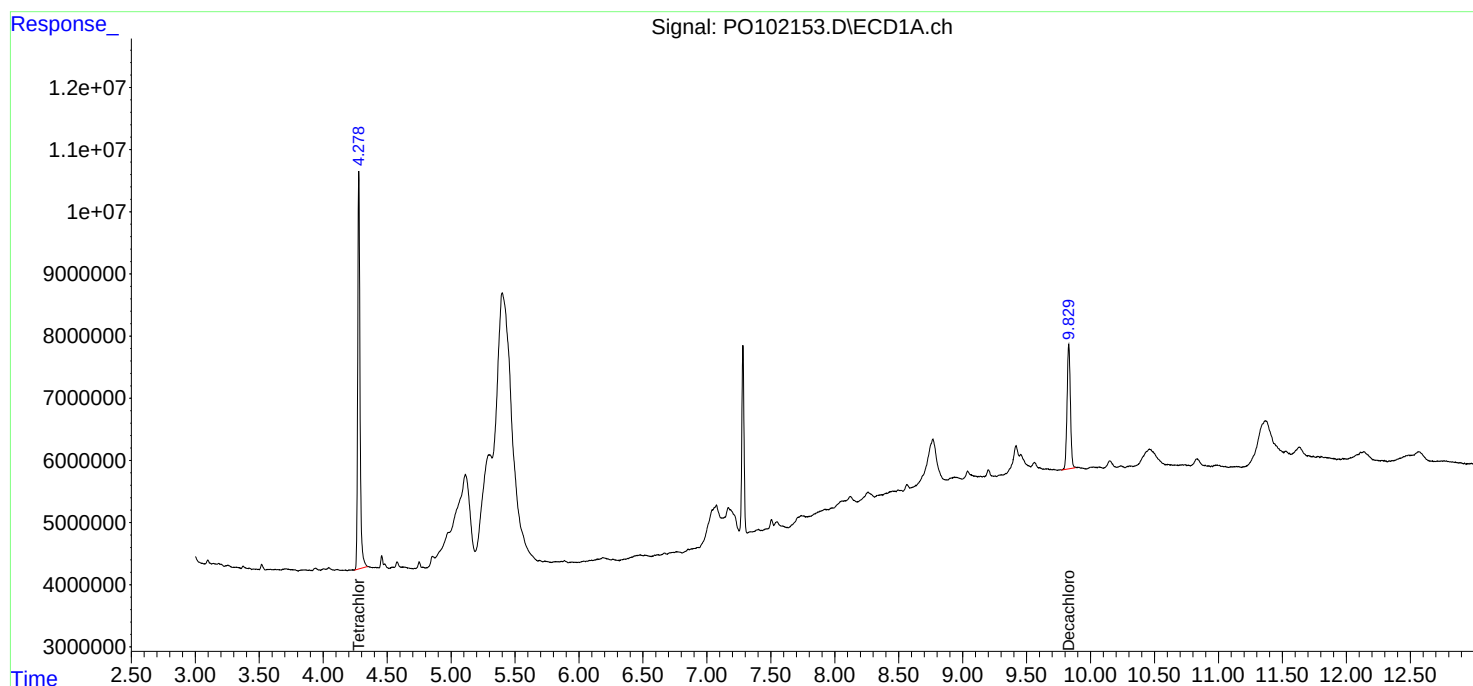

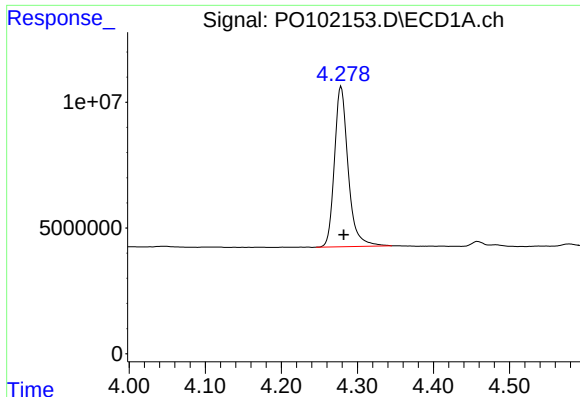


#1 Tetrachloro-m-xylene

R.T.: 4.278 min
Delta R.T.: -0.004 min
Response: 79880170
Conc: 17.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MANHOLE-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/28/2024
Supervised By :Ankita Jodhani 02/28/2024

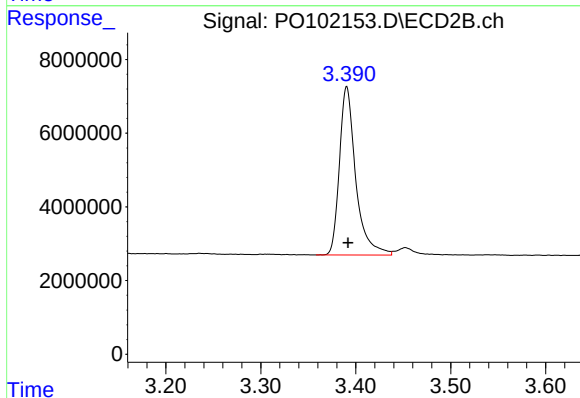


#1 Tetrachloro-m-xylene

R.T.: 3.391 min
Delta R.T.: -0.001 min
Response: 54476220
Conc: 16.76 ng/ml

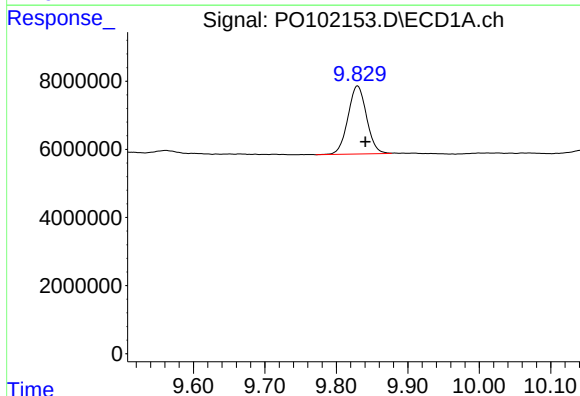

#2 Decachlorobiphenyl

R.T.: 9.830 min
Delta R.T.: -0.011 min
Response: 36085650
Conc: 14.17 ng/ml

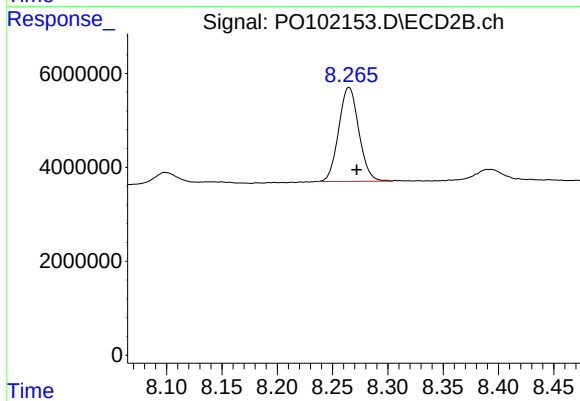

#2 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: -0.007 min
Response: 25357559
Conc: 12.26 ng/ml