

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022824\
 Data File : P0102175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2024 10:53
 Operator : YP/AJ
 Sample : P1587-10RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1653RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/29/2024
 Supervised By :Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 23:56:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.278	3.389	131.0E6	136.7E6	28.251	42.059m#
2) SA Decachlor...	9.822	8.266	94165292	33621855	36.980	16.252m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022824\
Data File : PO102175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2024 10:53
Operator : YP/AJ
Sample : P1587-10RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1653RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/29/2024
Supervised By :Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 23:56:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

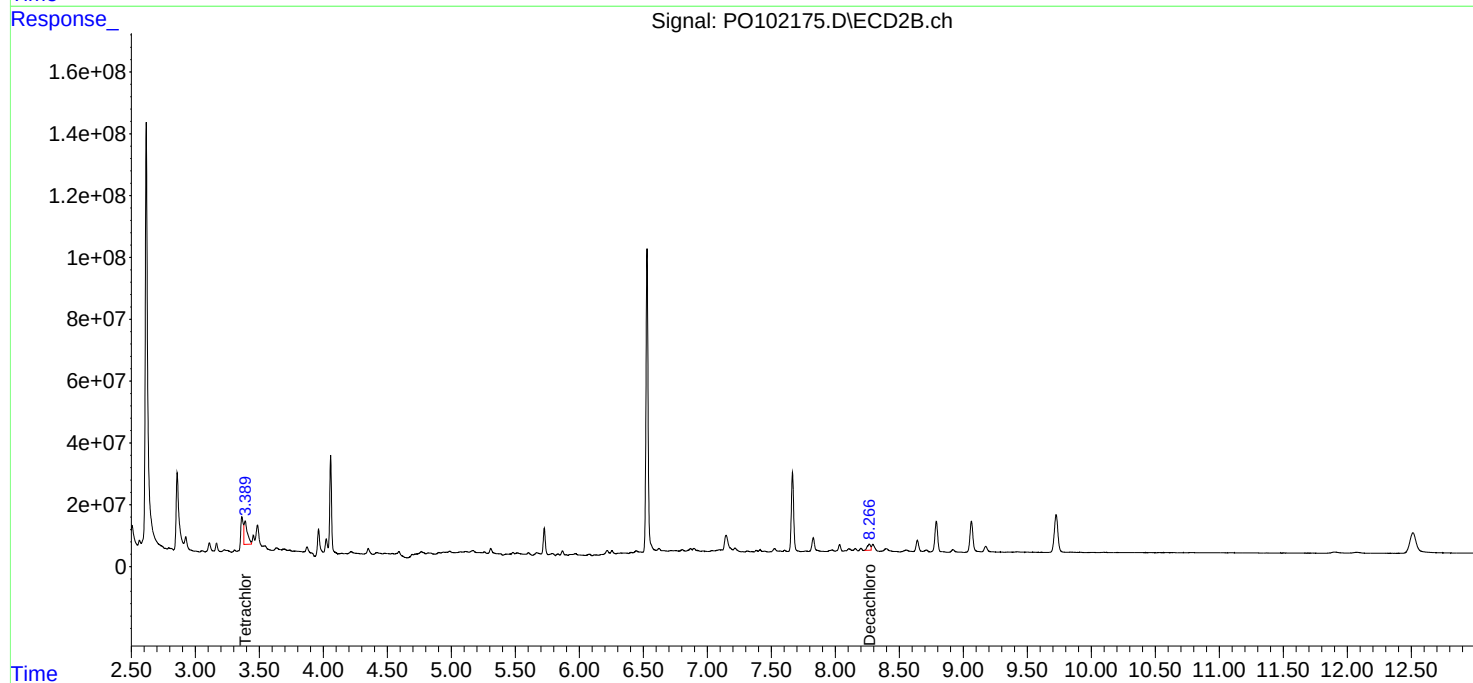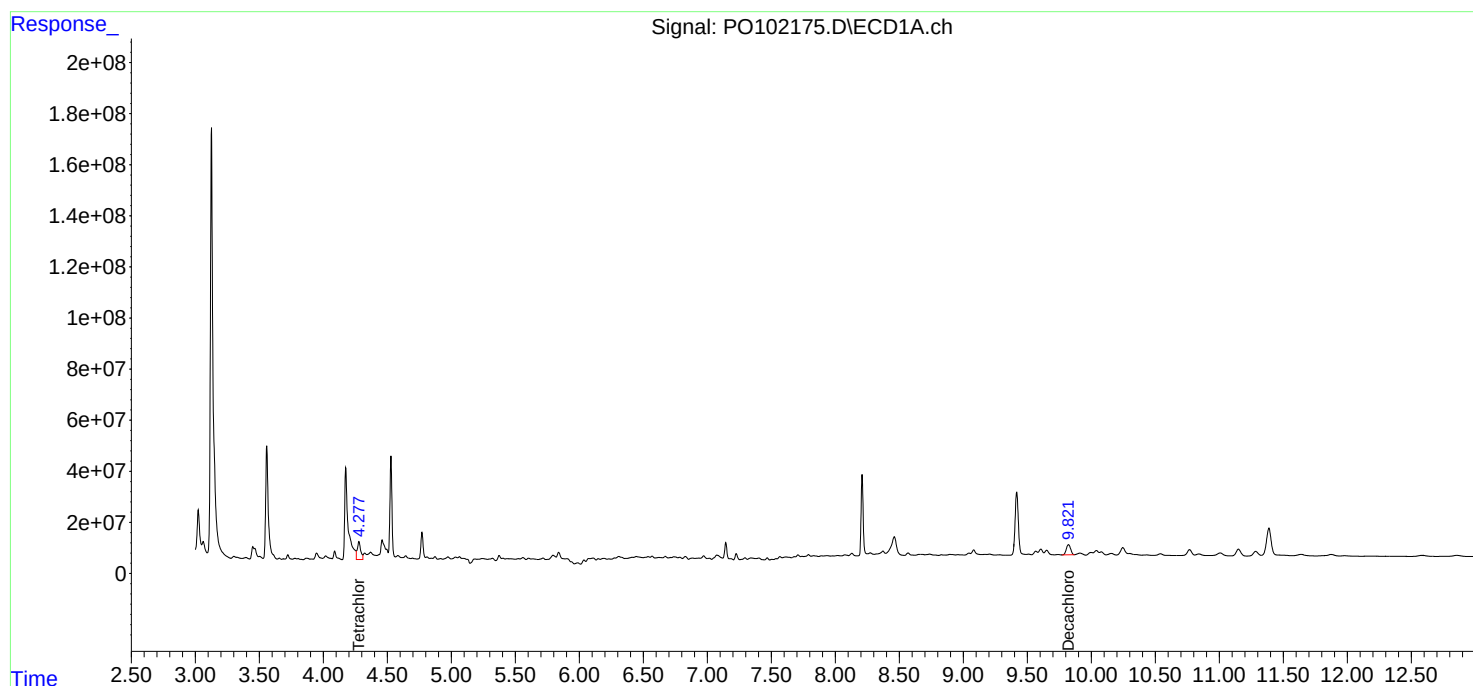

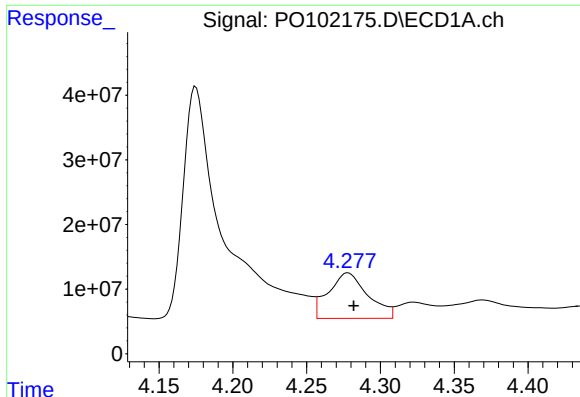


#1 Tetrachloro-m-xylene

R.T.: 4.278 min
Delta R.T.: -0.004 min
Response: 131017508
Conc: 28.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
1653RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/29/2024
Supervised By :Ankita Jodhani 02/29/2024

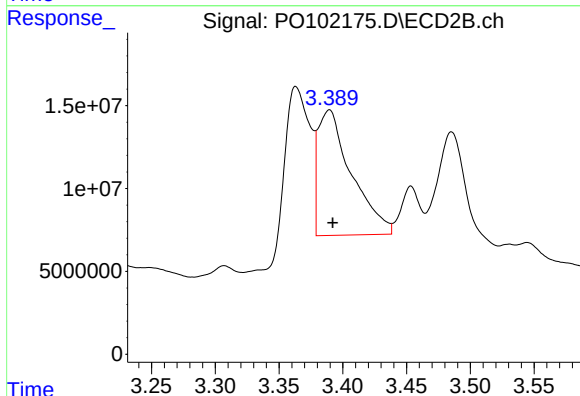


#1 Tetrachloro-m-xylene

R.T.: 3.389 min
Delta R.T.: -0.003 min
Response: 136669169
Conc: 42.06 ng/ml m

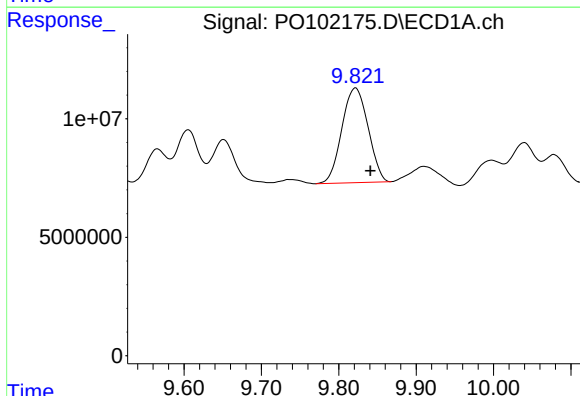

#2 Decachlorobiphenyl

R.T.: 9.822 min
Delta R.T.: -0.019 min
Response: 94165292
Conc: 36.98 ng/ml

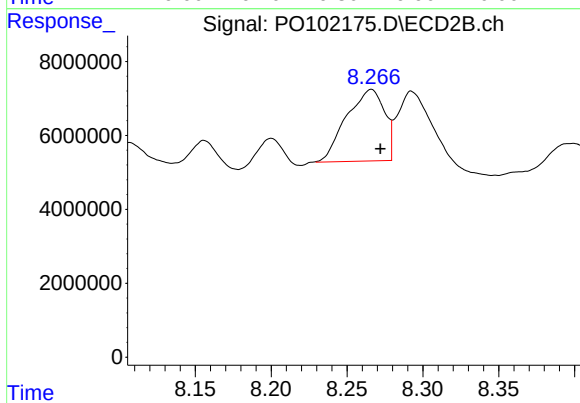

#2 Decachlorobiphenyl

R.T.: 8.266 min
Delta R.T.: -0.006 min
Response: 33621855
Conc: 16.25 ng/ml m