

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022824\
 Data File : P0102204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2024 20:14
 Operator : YP/AJ
 Sample : P1619-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPILL-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel
 02/29/2024

Supervised By :Ankita
 Jodhani
 02/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:08:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.278	3.391	68904988	42748843	14.858m	13.156m
2) SA Decachlor...	9.833	8.269	38493245	23384299	15.117	11.303 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022824\
Data File : PO102204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2024 20:14
Operator : YP/AJ
Sample : P1619-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPILL-1



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
02/29/2024

Supervised By :Ankita
Jodhani
02/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:08:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

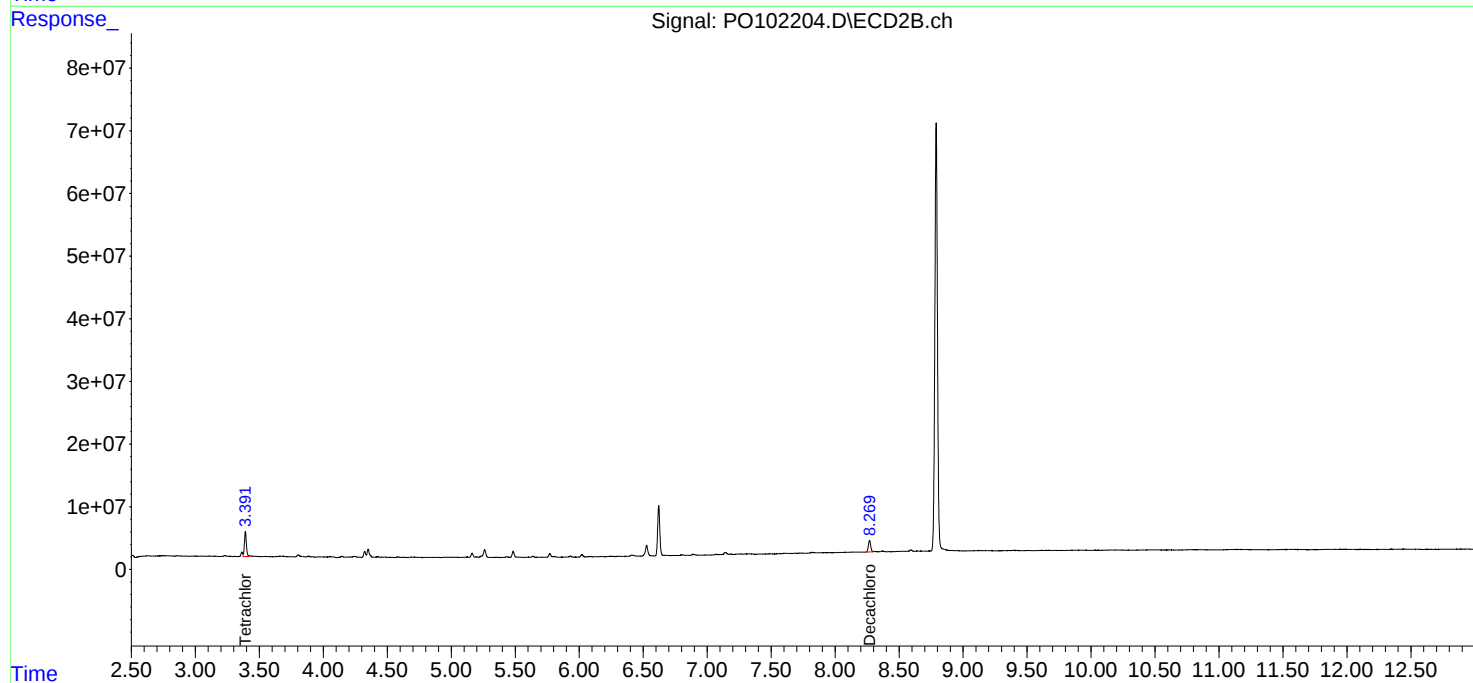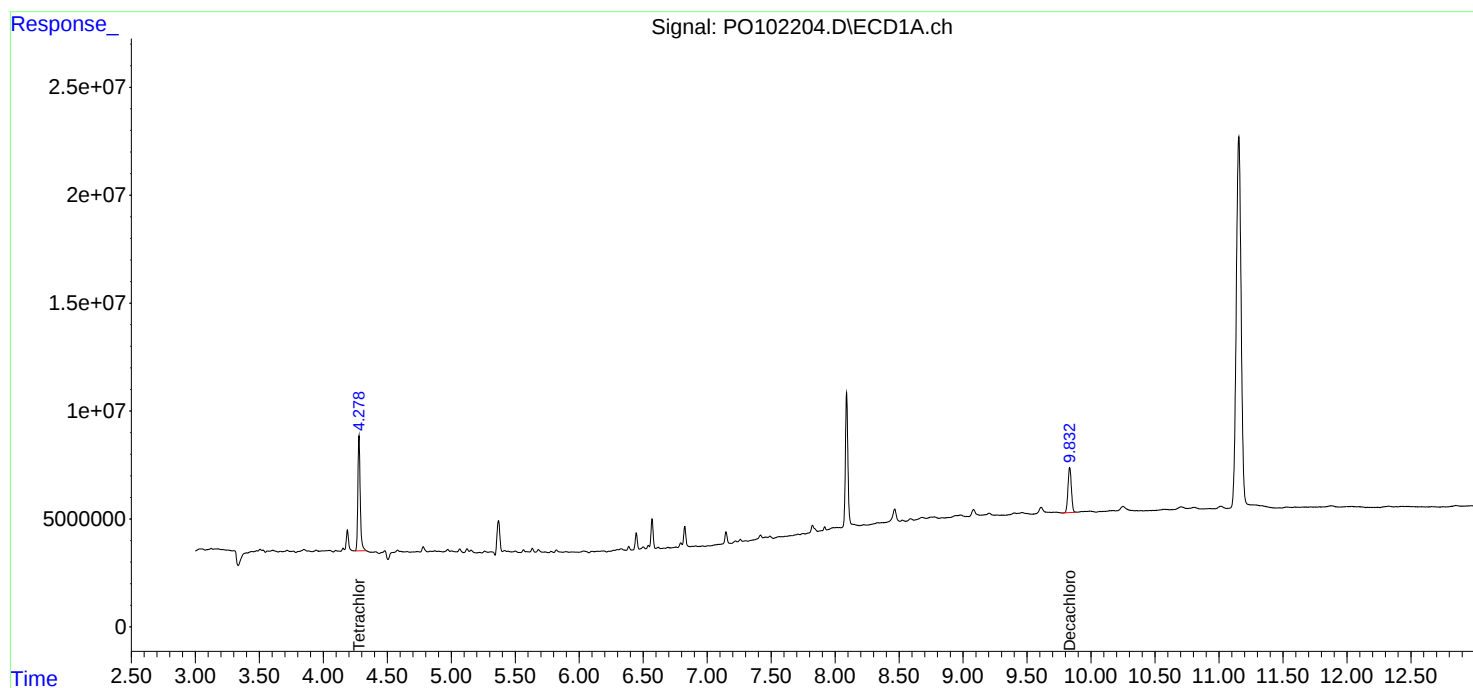

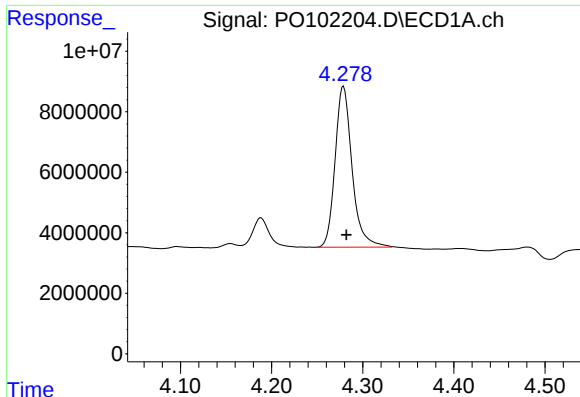

#1 Tetrachloro-m-xylene


R.T.: 4.278 min
Delta R.T.: -0.004 min
Response: 68904988
Conc: 14.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPILL-1

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
02/29/2024

Supervised By :Ankita
Jodhani
02/29/2024

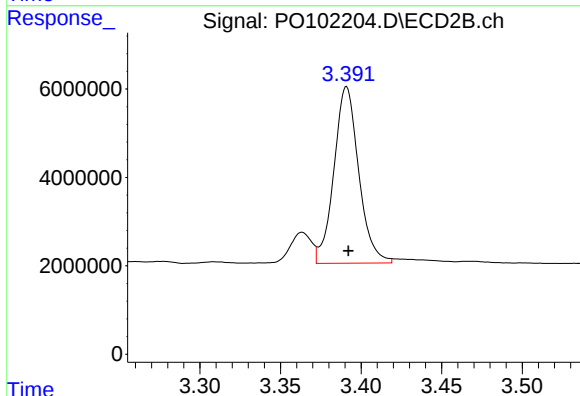


#1 Tetrachloro-m-xylene

R.T.: 3.391 min
Delta R.T.: -0.001 min
Response: 42748843
Conc: 13.16 ng/ml m

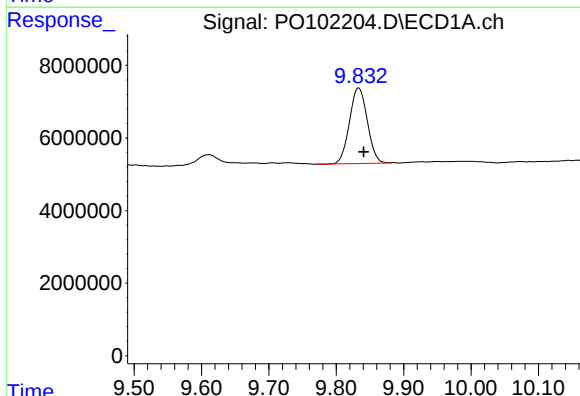

#2 Decachlorobiphenyl

R.T.: 9.833 min
Delta R.T.: -0.008 min
Response: 38493245
Conc: 15.12 ng/ml

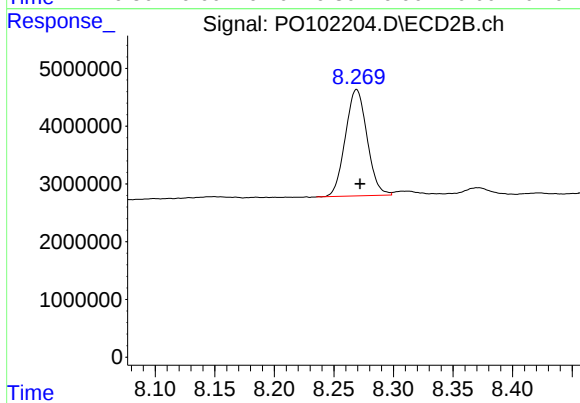

#2 Decachlorobiphenyl

R.T.: 8.269 min
Delta R.T.: -0.003 min
Response: 23384299
Conc: 11.30 ng/ml