

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030121\
 Data File : P0075767.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2021 14:07
 Operator : AJ/MA
 Sample : PB134862BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB134862BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 03:42:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.938	3.955	1238624	924816	20.263	20.934
2)	SA Decachlor...	10.957	9.229	978274	890956	21.499	20.531
Target Compounds							
8)	L2 AR-1221-1	5.192	0.000	520967	0	763.555	N.D. #
9)	L2 AR-1221-2	5.292	4.304	21838	6916	41.094	16.521 #
28)	L6 AR-1254-3	7.807f	0.000	46317	0	12.197	N.D. #
30)	L6 AR-1254-5	8.514	7.315	12039	13497	4.297	3.844
34)	L7 AR-1260-4	8.816	0.000	12420	0	4.776	N.D. #
36)	L8 AR-1262-1	0.000	7.315	0	13497	N.D.	6.444 #
45)	L9 AR-1268-5	0.000	8.985	0	15607	N.D.	0.927 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030121\
Data File : P0075767.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2021 14:07
Operator : AJ/MA
Sample : PB134862BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
PB134862BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 03:42:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

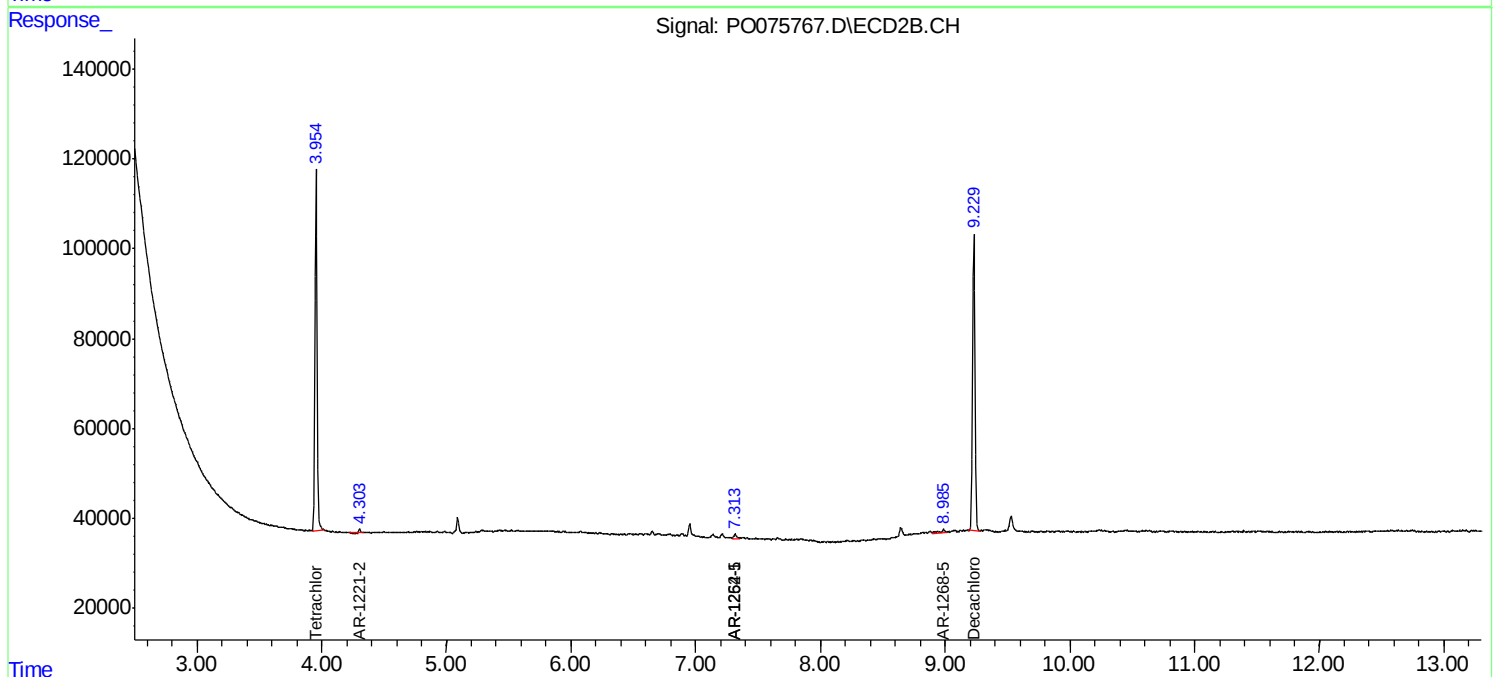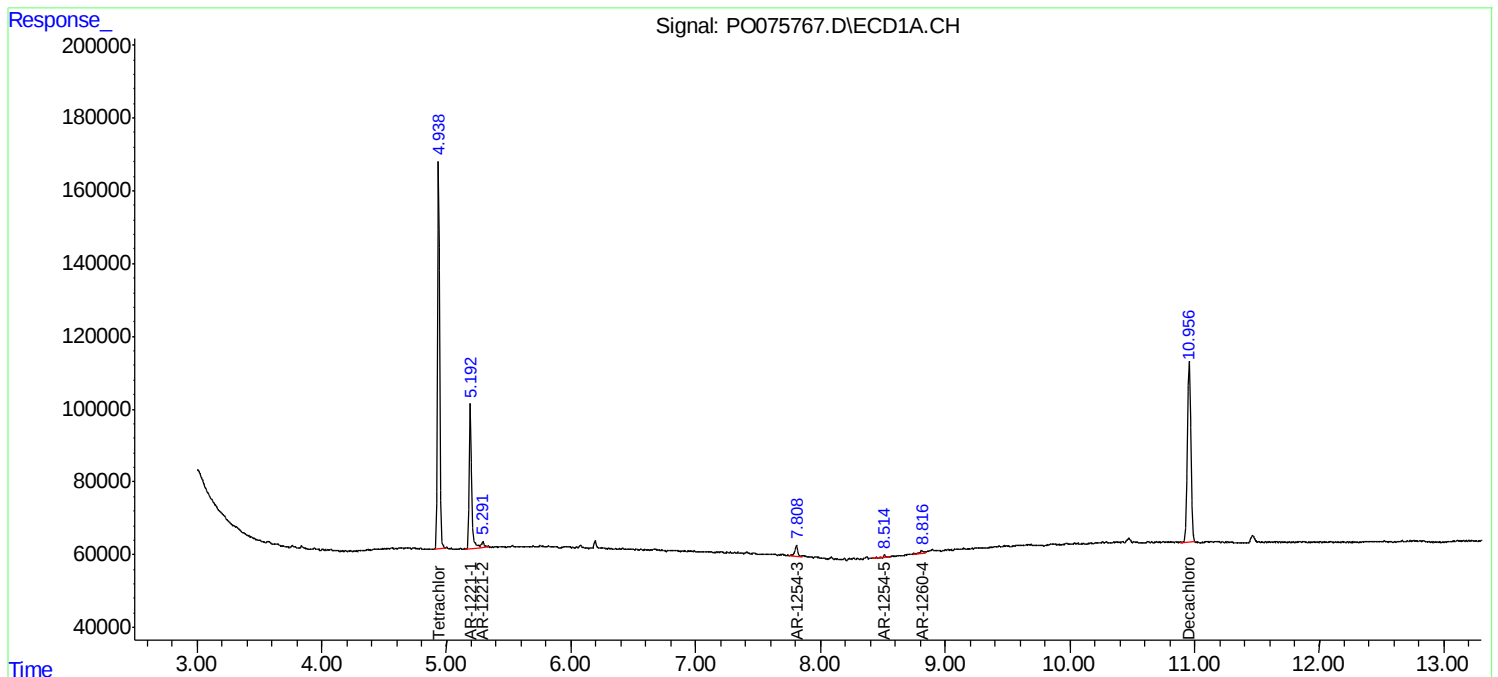


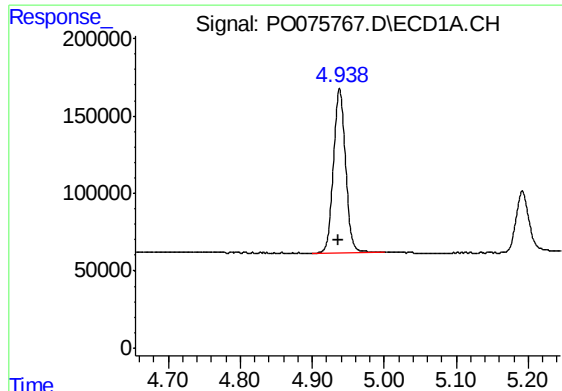

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: 0.002 min
Response: 1238624
Conc: 20.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134862BL

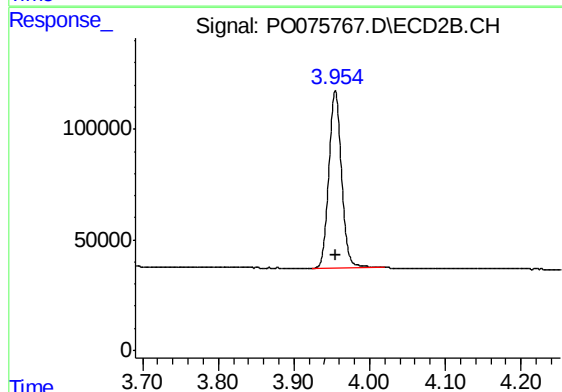


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 924816
Conc: 20.93 ng/ml

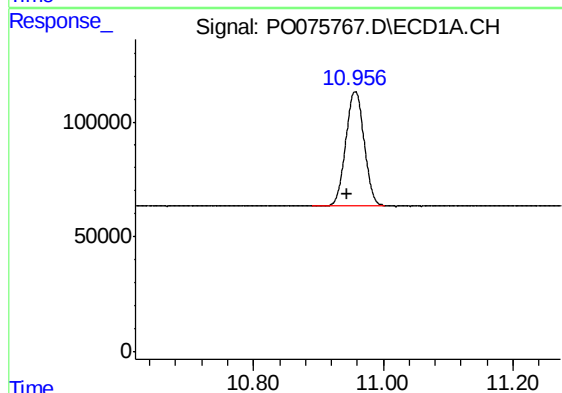


#2 Decachlorobiphenyl

R.T.: 10.957 min
Delta R.T.: 0.011 min
Response: 978274
Conc: 21.50 ng/ml

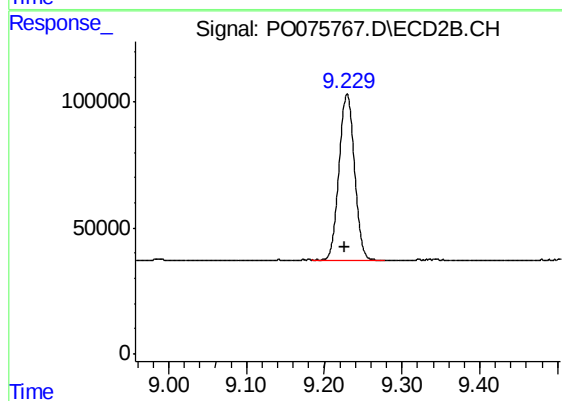

#2 Decachlorobiphenyl


R.T.: 9.229 min
Delta R.T.: 0.002 min
Response: 890956
Conc: 20.53 ng/ml

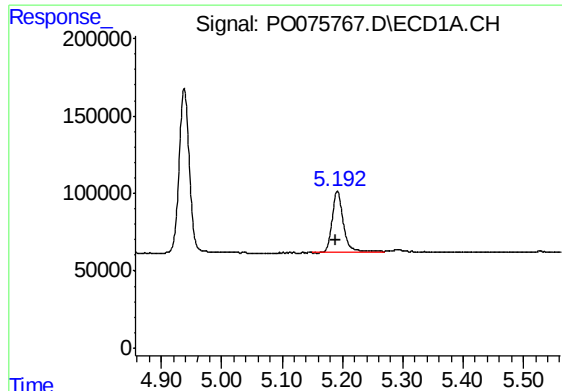

#8 AR-1221-1


R.T.: 5.192 min
Delta R.T.: 0.004 min
Response: 520967
Conc: 763.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134862BL

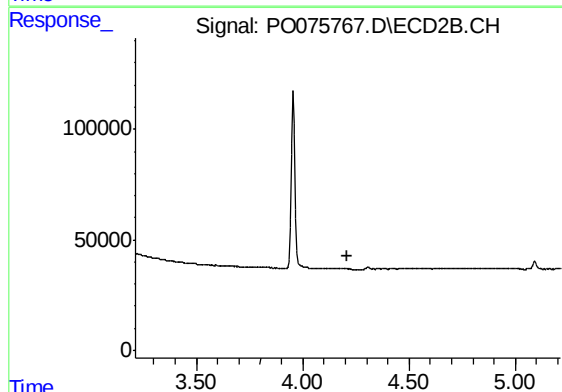


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.212 min
Response: 0
Conc: N.D.

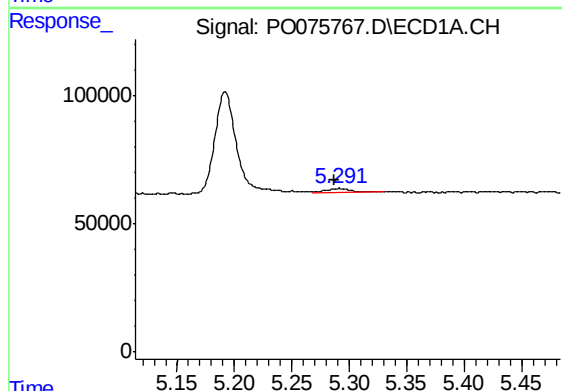


#9 AR-1221-2

R.T.: 5.292 min
Delta R.T.: 0.005 min
Response: 21838
Conc: 41.09 ng/ml

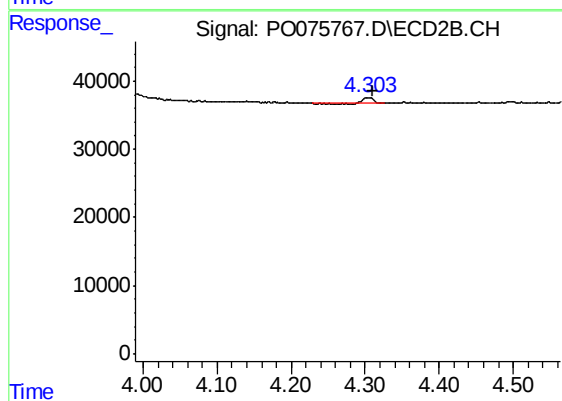

#9 AR-1221-2


R.T.: 4.304 min
Delta R.T.: -0.007 min
Response: 6916
Conc: 16.52 ng/ml

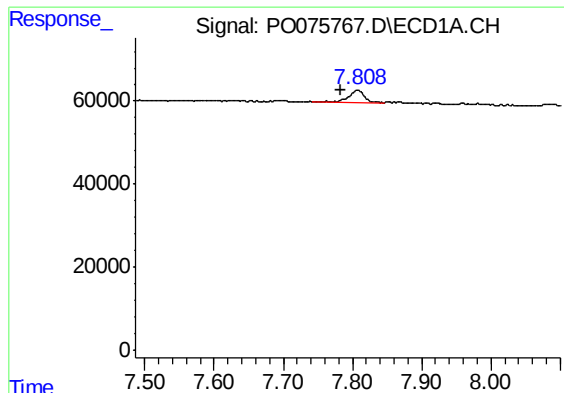

#28 AR-1254-3


R.T.: 7.807 min
Delta R.T.: 0.024 min
Response: 46317
Conc: 12.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134862BL

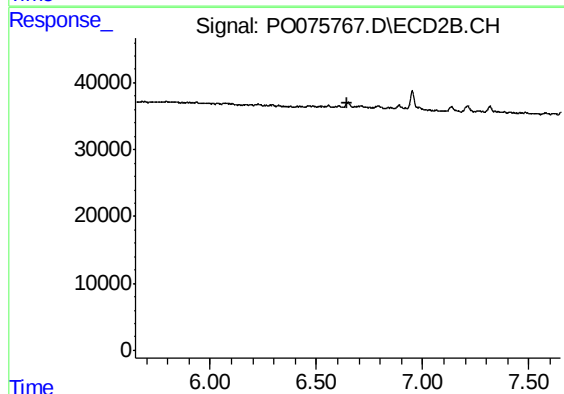


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.648 min
Response: 0
Conc: N.D.

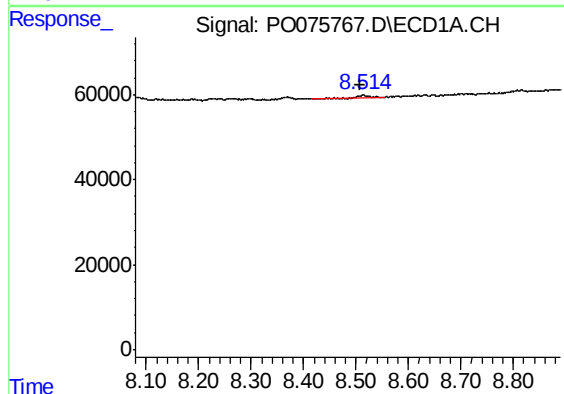


#30 AR-1254-5

R.T.: 8.514 min
Delta R.T.: 0.006 min
Response: 12039
Conc: 4.30 ng/ml

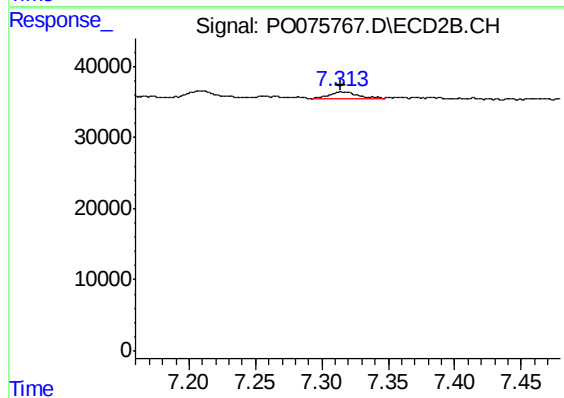

#30 AR-1254-5


R.T.: 7.315 min
Delta R.T.: 0.000 min
Response: 13497
Conc: 3.84 ng/ml

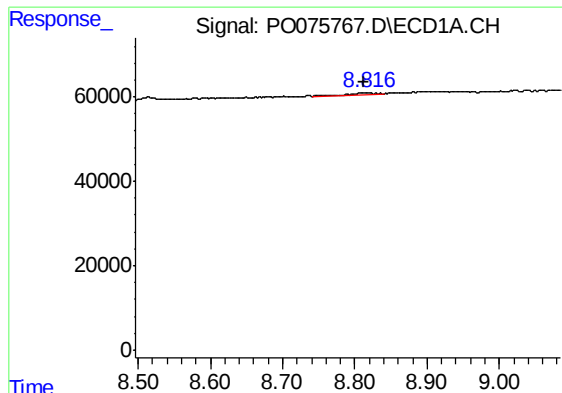

#34 AR-1260-4


R.T.: 8.816 min
Delta R.T.: 0.004 min
Response: 12420
Conc: 4.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134862BL

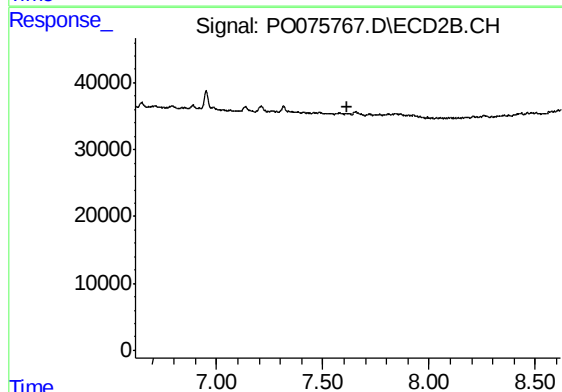


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.618 min
Response: 0
Conc: N.D.

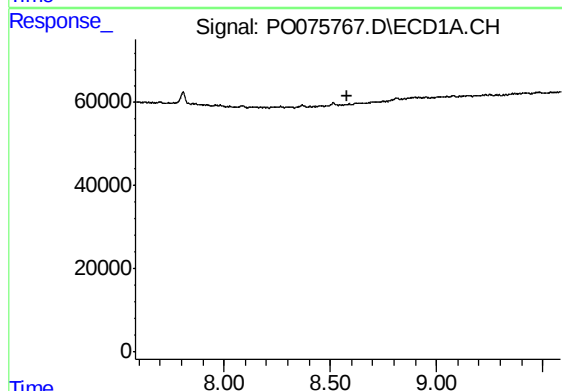


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.583 min
Response: 0
Conc: N.D.

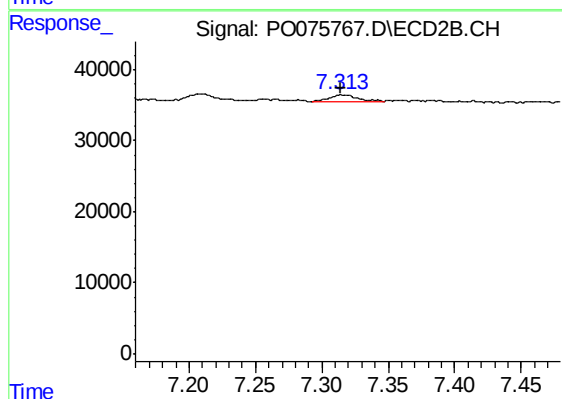

#36 AR-1262-1


R.T.: 7.315 min
Delta R.T.: 0.000 min
Response: 13497
Conc: 6.44 ng/ml

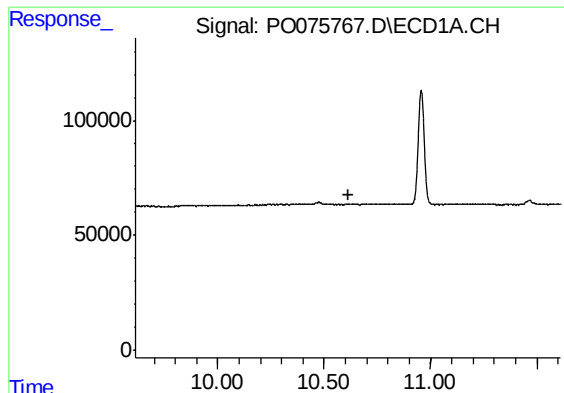

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB134862BL

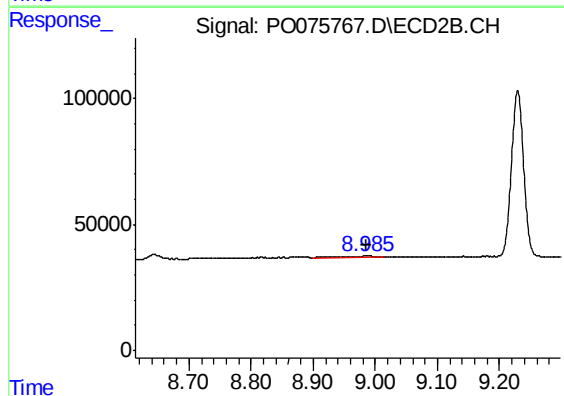

#45 AR-1268-5

R.T.: 8.985 min
Delta R.T.: -0.001 min
Response: 15607
Conc: 0.93 ng/ml