

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0030121\
 Data File : P0075771.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2021 15:16
 Operator : AJ/MA
 Sample : M1503-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEDGWICK-AVE

Manual Integrations
 APPROVED

Ankita
 3/2/2021 9:42:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 03:45:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.939	3.955	1425145	1073012	23.315	24.288
2) SA Decachlor...	10.958	9.230	919967	873208	20.218	20.122
Target Compounds						
31) L7 AR-1260-1	7.956	6.787	237387	333571	96.829	132.712 #
32) L7 AR-1260-2	8.222	6.984	311237	413672	104.377	136.052 #
33) L7 AR-1260-3	8.589	7.137	193793	306479	90.210	110.319
34) L7 AR-1260-4	8.818	7.620	271996	210052	104.606m	89.491
35) L7 AR-1260-5	9.146	7.866	517744	634716	99.194	111.542

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030121\
Data File : PO075771.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2021 15:16
Operator : AJ/MA
Sample : M1503-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 03:45:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

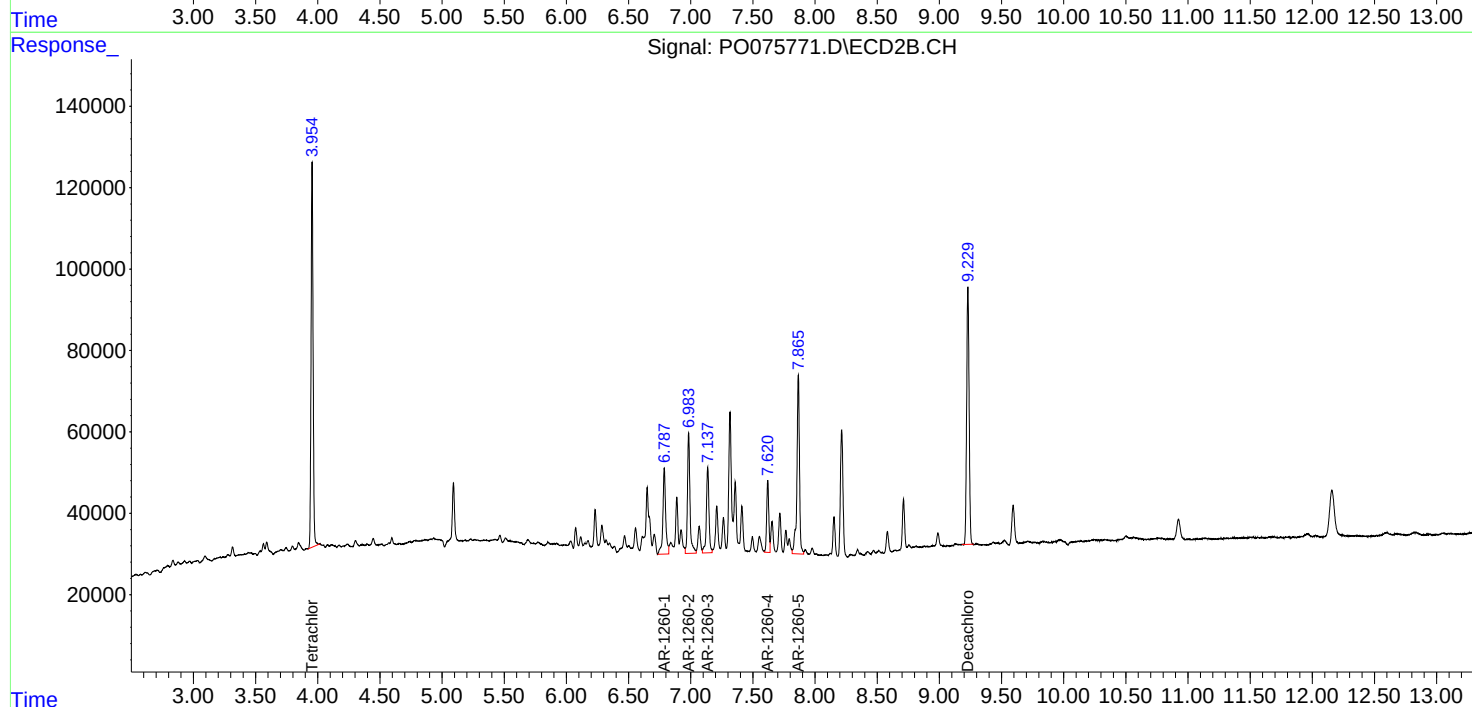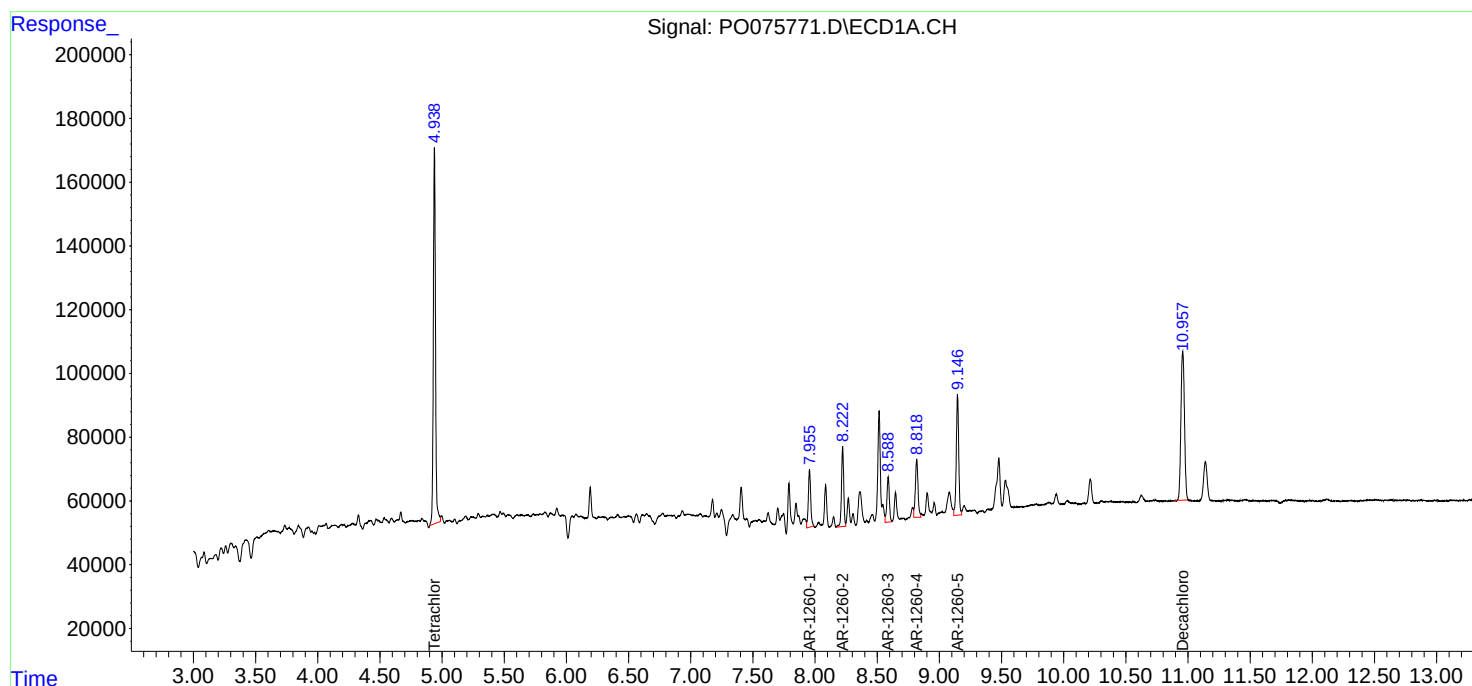

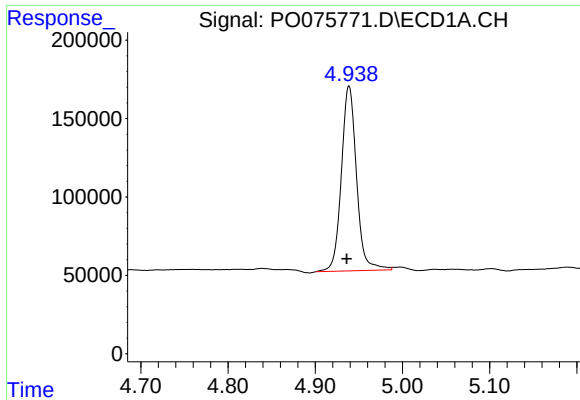


#1 Tetrachloro-m-xylene

R.T.: 4.939 min
Delta R.T.: 0.003 min
Response: 1425145
Conc: 23.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:34 AM

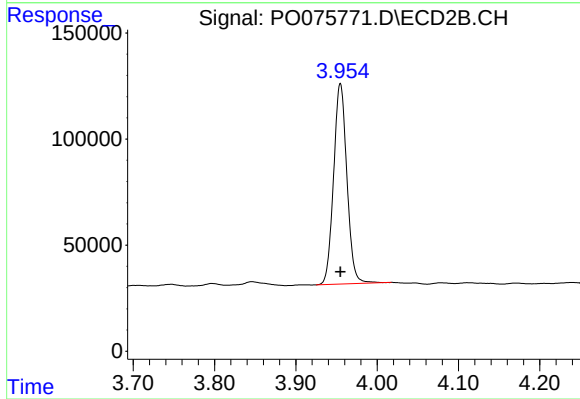


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 1073012
Conc: 24.29 ng/ml

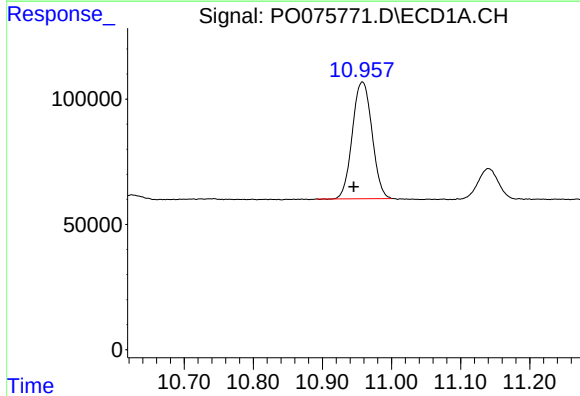


#2 Decachlorobiphenyl

R.T.: 10.958 min
Delta R.T.: 0.012 min
Response: 919967
Conc: 20.22 ng/ml

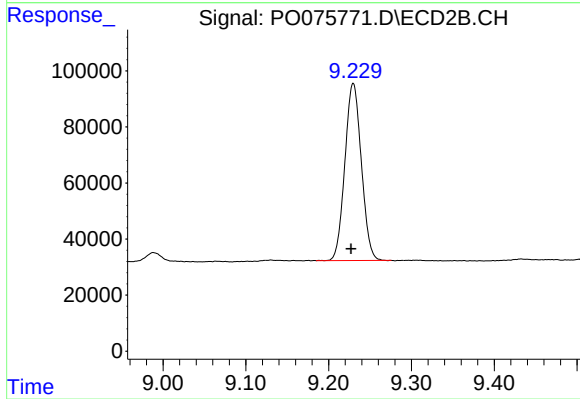

#2 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.003 min
Response: 873208
Conc: 20.12 ng/ml

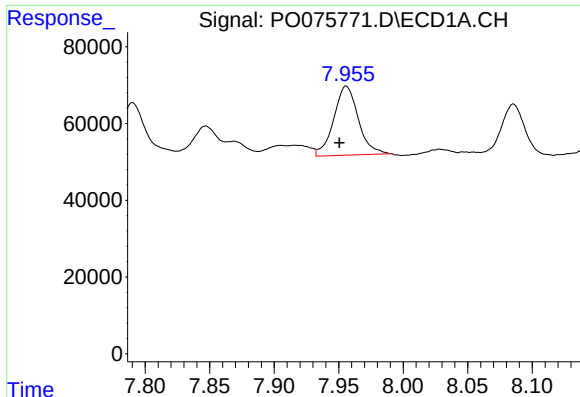


#31 AR-1260-1

R.T.: 7.956 min
Delta R.T.: 0.005 min
Response: 237387
Conc: 96.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:34 AM

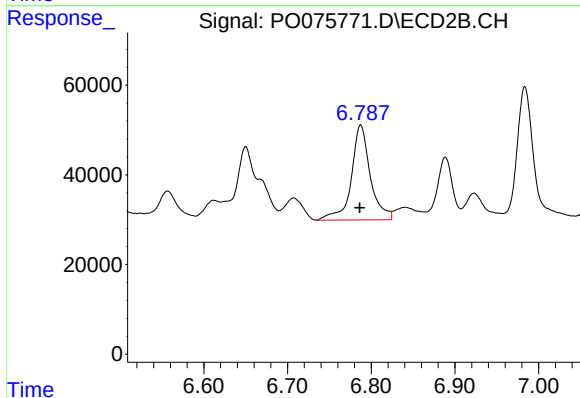


#31 AR-1260-1

R.T.: 6.787 min
Delta R.T.: 0.000 min
Response: 333571
Conc: 132.71 ng/ml

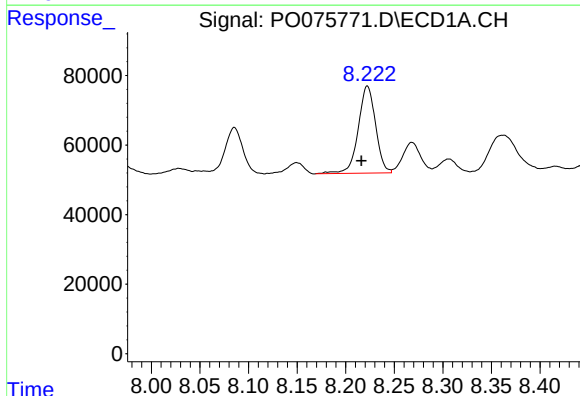


#32 AR-1260-2

R.T.: 8.222 min
Delta R.T.: 0.006 min
Response: 311237
Conc: 104.38 ng/ml

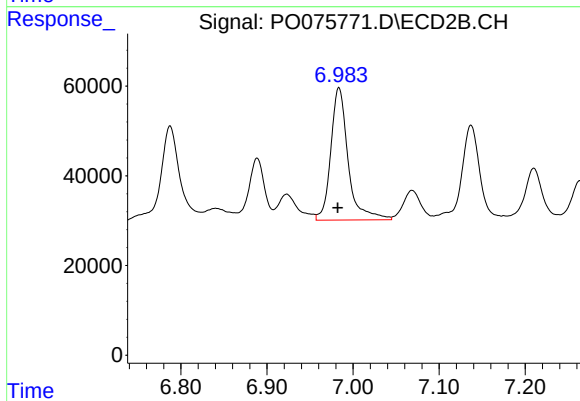

#32 AR-1260-2

R.T.: 6.984 min
Delta R.T.: 0.001 min
Response: 413672
Conc: 136.05 ng/ml

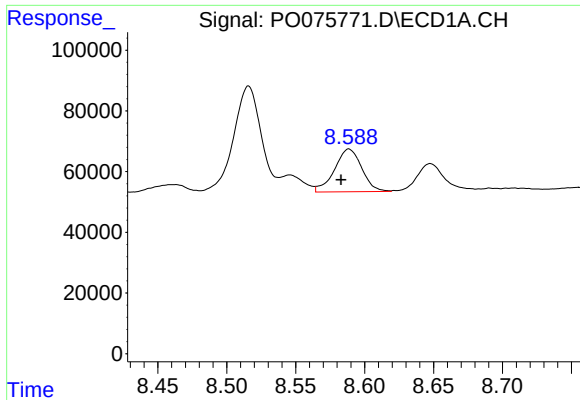


#33 AR-1260-3

R.T.: 8.589 min
Delta R.T.: 0.006 min
Response: 193793
Conc: 90.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:34 AM

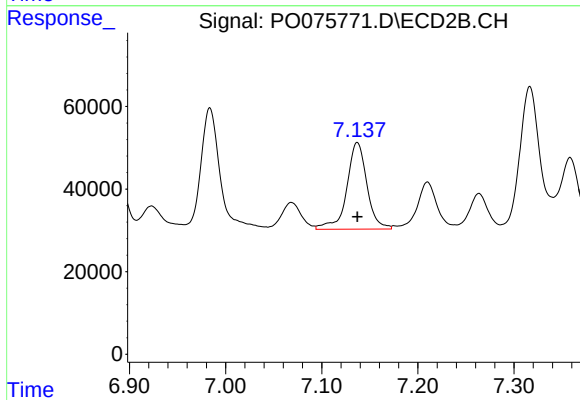


#33 AR-1260-3

R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 306479
Conc: 110.32 ng/ml

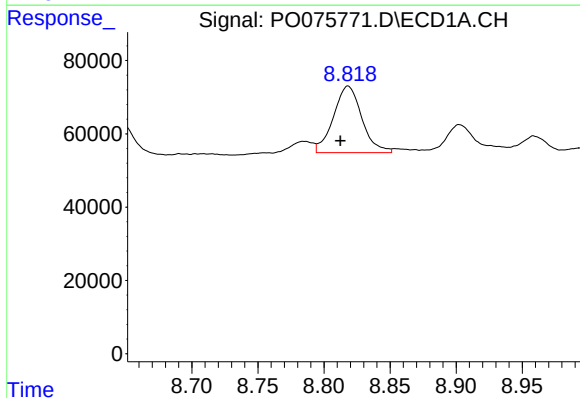


#34 AR-1260-4

R.T.: 8.818 min
Delta R.T.: 0.005 min
Response: 271996
Conc: 104.61 ng/ml m

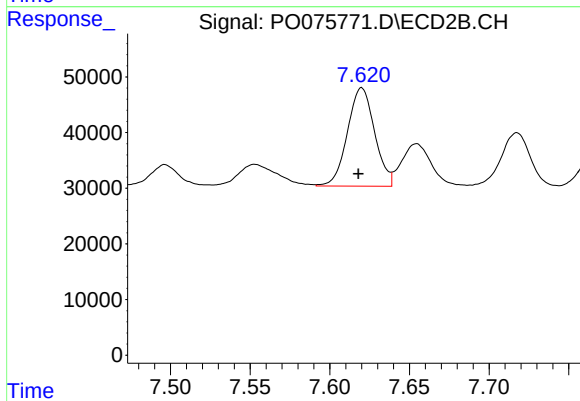

#34 AR-1260-4

R.T.: 7.620 min
Delta R.T.: 0.002 min
Response: 210052
Conc: 89.49 ng/ml

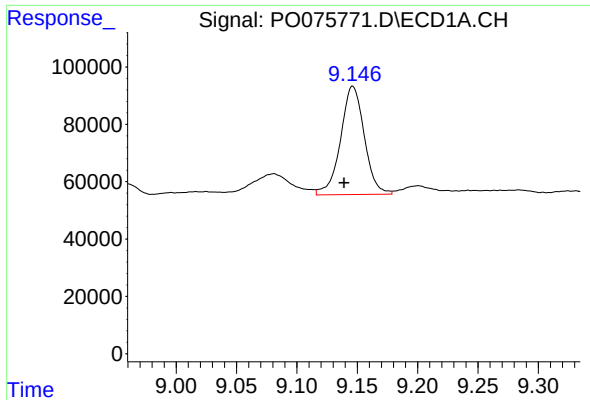


#35 AR-1260-5

R.T.: 9.146 min
Delta R.T.: 0.007 min
Response: 517744
Conc: 99.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEDGWICK-AVE

Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:34 AM

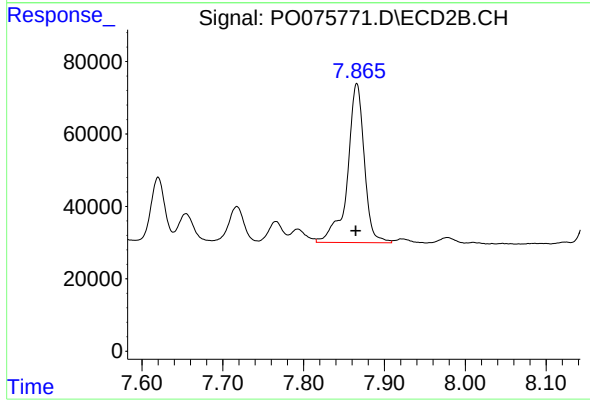

#35 AR-1260-5

R.T.: 7.866 min
Delta R.T.: 0.001 min
Response: 634716
Conc: 111.54 ng/ml