

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030121\
 Data File : P0075776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2021 16:42
 Operator : AJ/MA
 Sample : M1508-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-1138

Manual Integrations
 APPROVED

Ankita
 3/2/2021 9:42:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 03:48:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.955	826460	626670	13.520	14.185
2) SA Decachlor...	10.964f	9.236	654152	619790	14.376	14.282
Target Compounds						
26) L6 AR-1254-1	7.174	6.086f	646146	562774	274.753m	198.600m#
27) L6 AR-1254-2	7.382f	6.236	297025	453439	82.703m	183.101m#
28) L6 AR-1254-3	7.791	6.655	392692	272609	103.408	67.968 #
29) L6 AR-1254-4	8.088	6.895	271738	248704	97.933	94.640
30) L6 AR-1254-5	8.519	7.323	381820	410874	136.290	117.018

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030121\
Data File : PO075776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2021 16:42
Operator : AJ/MA
Sample : M1508-02
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 03:48:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

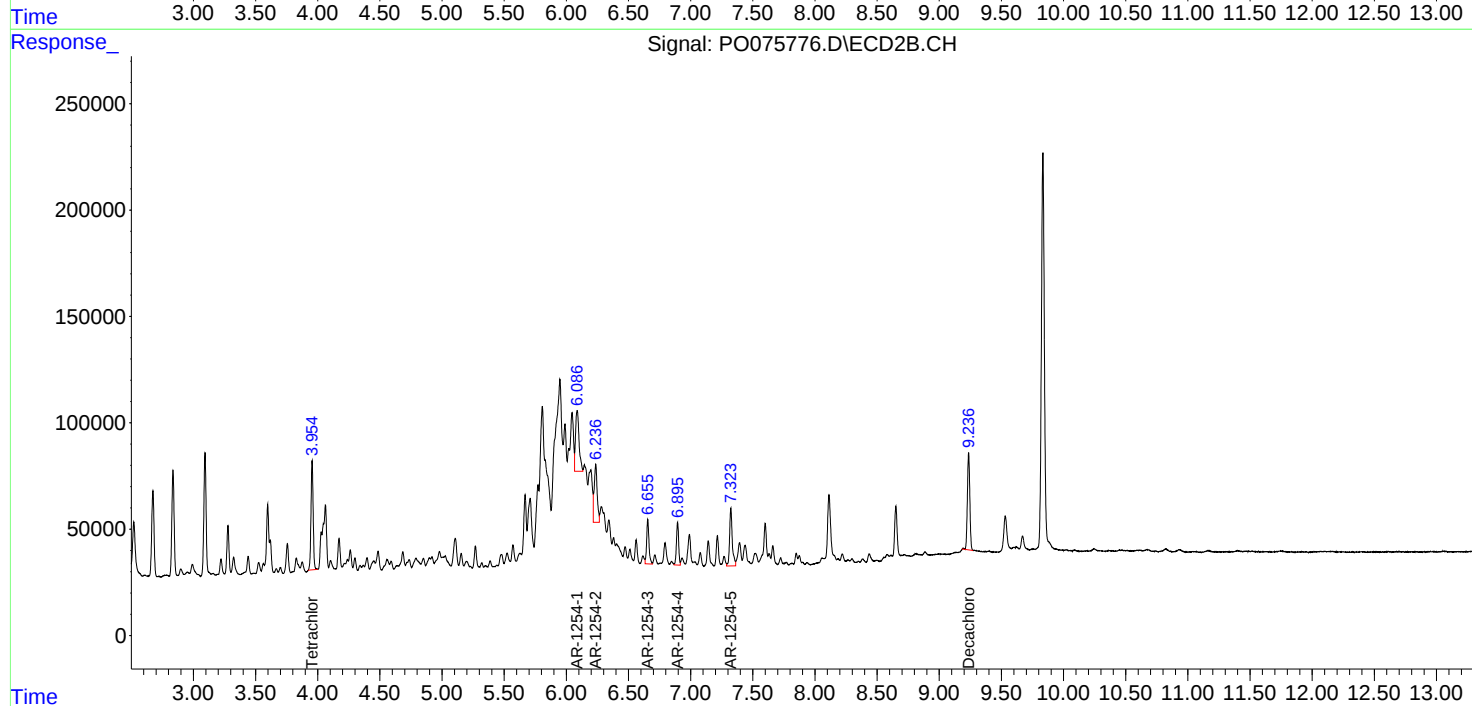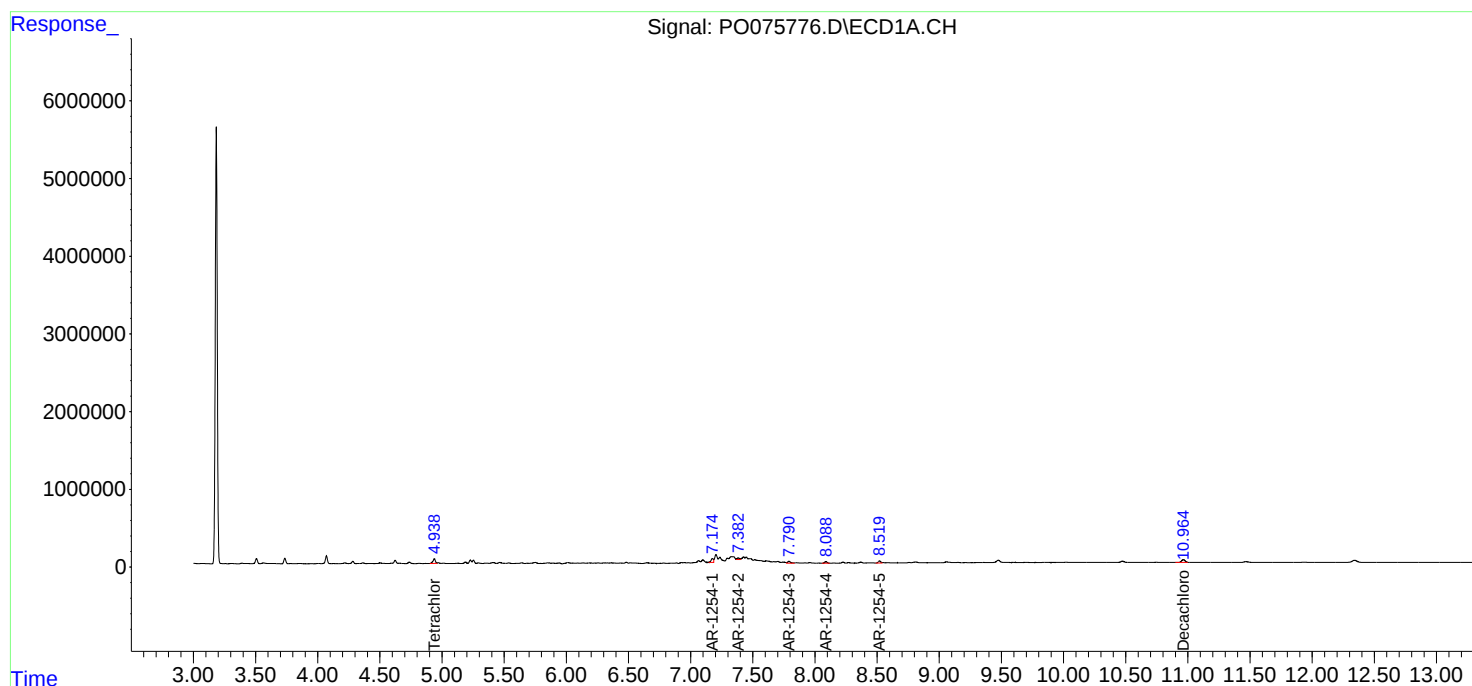

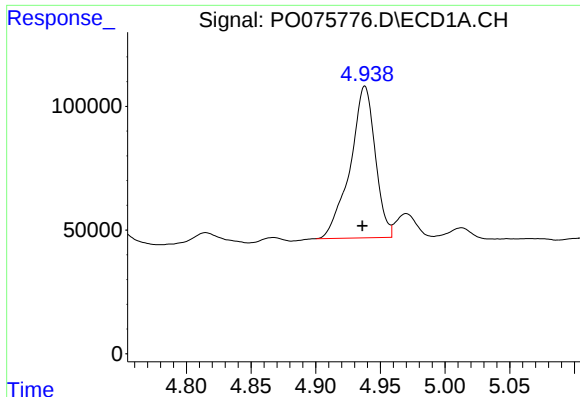


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: 0.002 min
Response: 826460
Conc: 13.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:38 AM

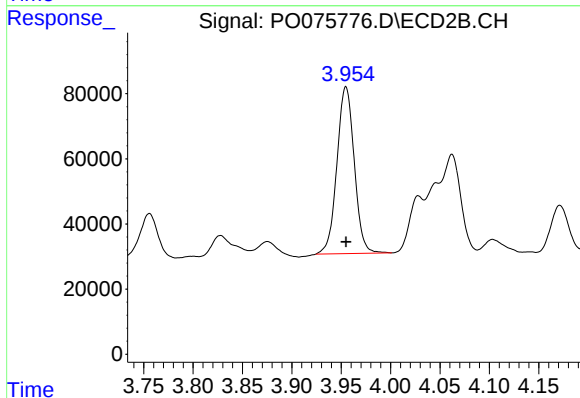


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 626670
Conc: 14.18 ng/ml

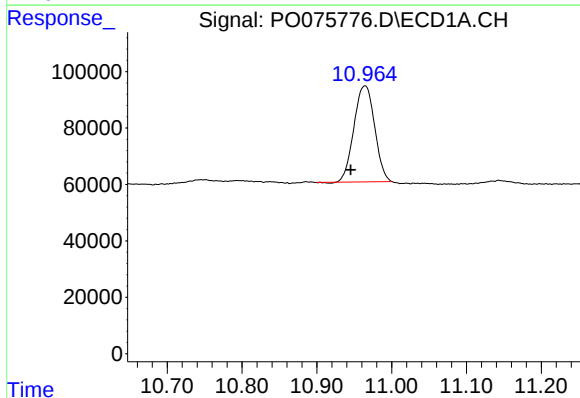


#2 Decachlorobiphenyl

R.T.: 10.964 min
Delta R.T.: 0.019 min
Response: 654152
Conc: 14.38 ng/ml

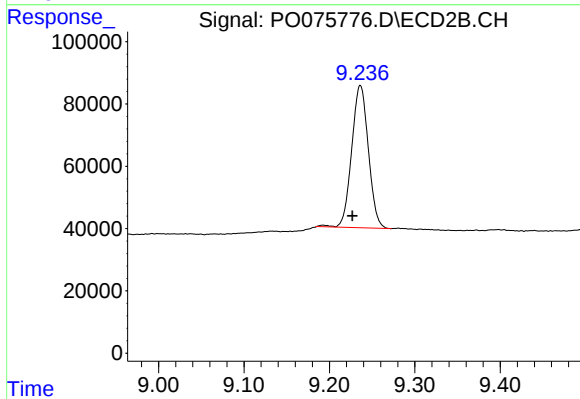

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.009 min
Response: 619790
Conc: 14.28 ng/ml

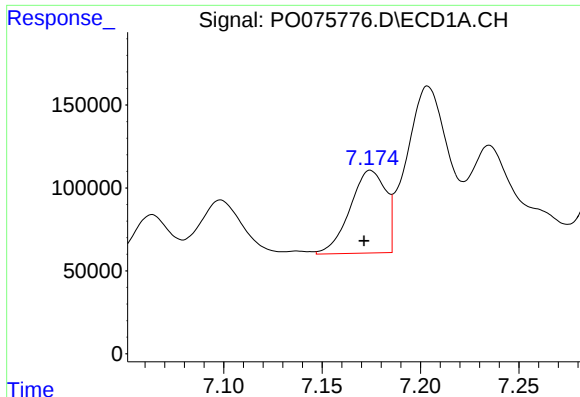


#26 AR-1254-1

R.T.: 7.174 min
Delta R.T.: 0.003 min
Response: 646146
Conc: 274.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:38 AM

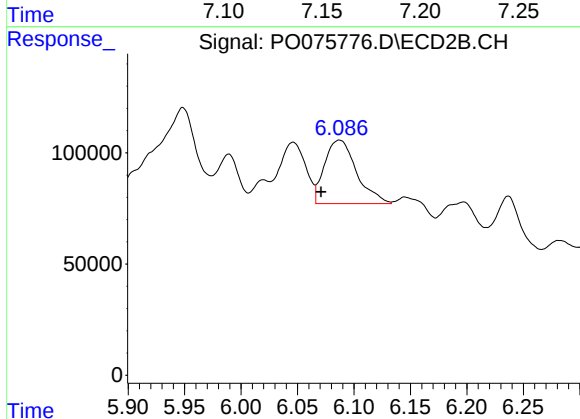


#26 AR-1254-1

R.T.: 6.086 min
Delta R.T.: 0.016 min
Response: 562774
Conc: 198.60 ng/ml m

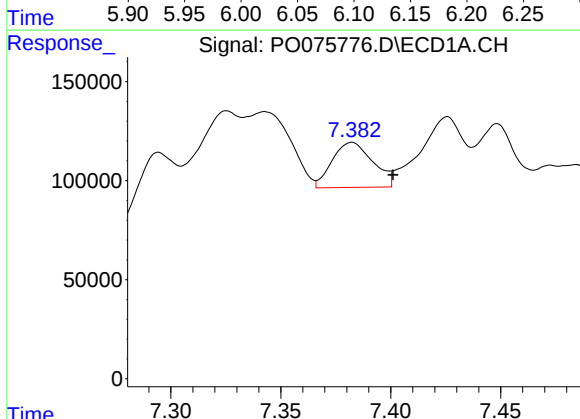


#27 AR-1254-2

R.T.: 7.382 min
Delta R.T.: -0.019 min
Response: 297025
Conc: 82.70 ng/ml m

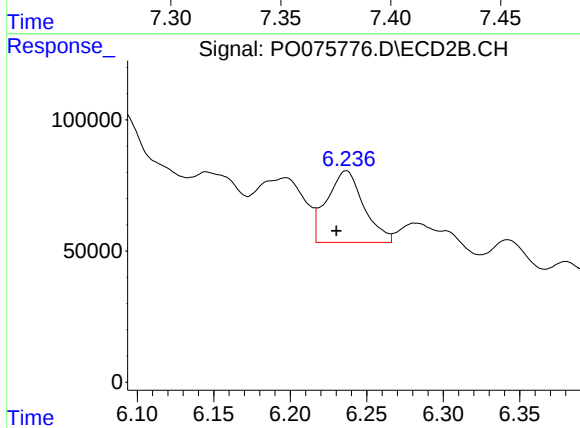

#27 AR-1254-2

R.T.: 6.236 min
Delta R.T.: 0.006 min
Response: 453439
Conc: 183.10 ng/ml m

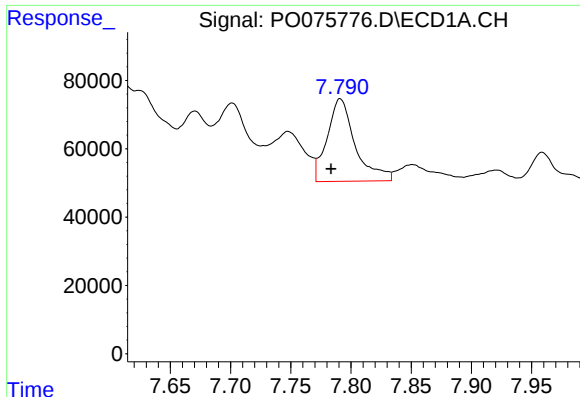


#28 AR-1254-3

R.T.: 7.791 min
Delta R.T.: 0.008 min
Response: 392692
Conc: 103.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:38 AM

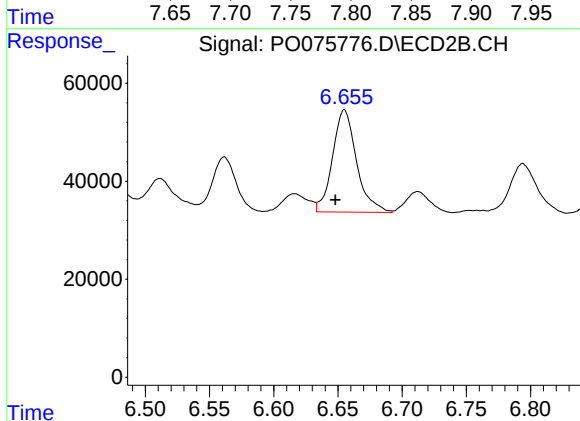


#28 AR-1254-3

R.T.: 6.655 min
Delta R.T.: 0.007 min
Response: 272609
Conc: 67.97 ng/ml

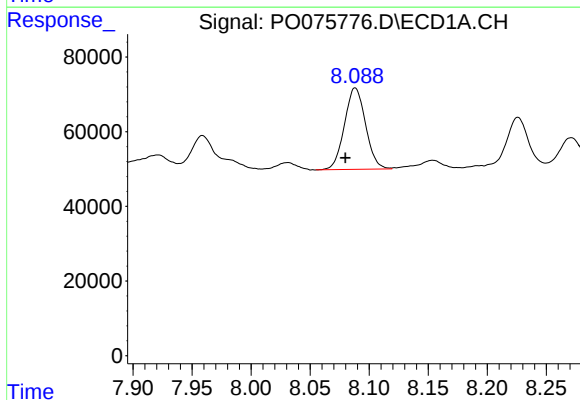


#29 AR-1254-4

R.T.: 8.088 min
Delta R.T.: 0.008 min
Response: 271738
Conc: 97.93 ng/ml

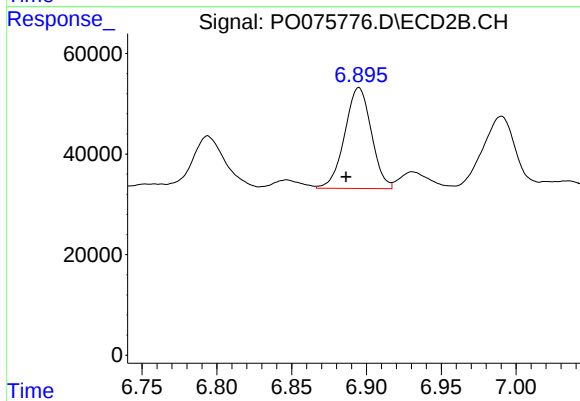

#29 AR-1254-4

R.T.: 6.895 min
Delta R.T.: 0.009 min
Response: 248704
Conc: 94.64 ng/ml

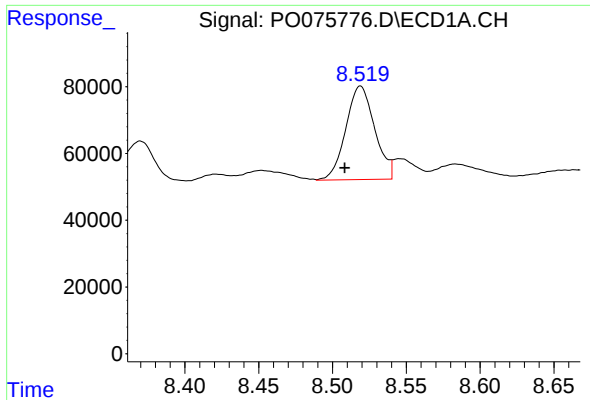


#30 AR-1254-5

R.T.: 8.519 min
Delta R.T.: 0.011 min
Response: 381820
Conc: 136.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1138

Manual Integrations
APPROVED

Ankita
3/2/2021 9:42:38 AM

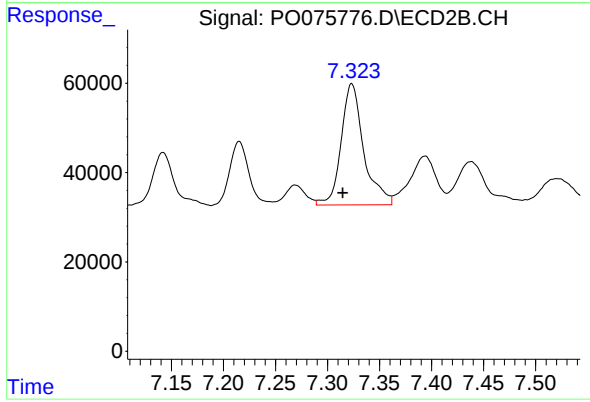

#30 AR-1254-5

R.T.: 7.323 min
Delta R.T.: 0.009 min
Response: 410874
Conc: 117.02 ng/ml