

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030122\
 Data File : P0084941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2022 14:37
 Operator : YP\AJ
 Sample : N1701-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220214-096-21-02-ELUTRIATE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:17:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.596	4286787	767970	15.332	17.077
2) SA Decachlor...	10.433	8.621	1999751	456458	11.408	12.422

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030122\
Data File : P0084941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2022 14:37
Operator : YP\AJ
Sample : N1701-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220214-096-21-02-ELUTRIATE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:17:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

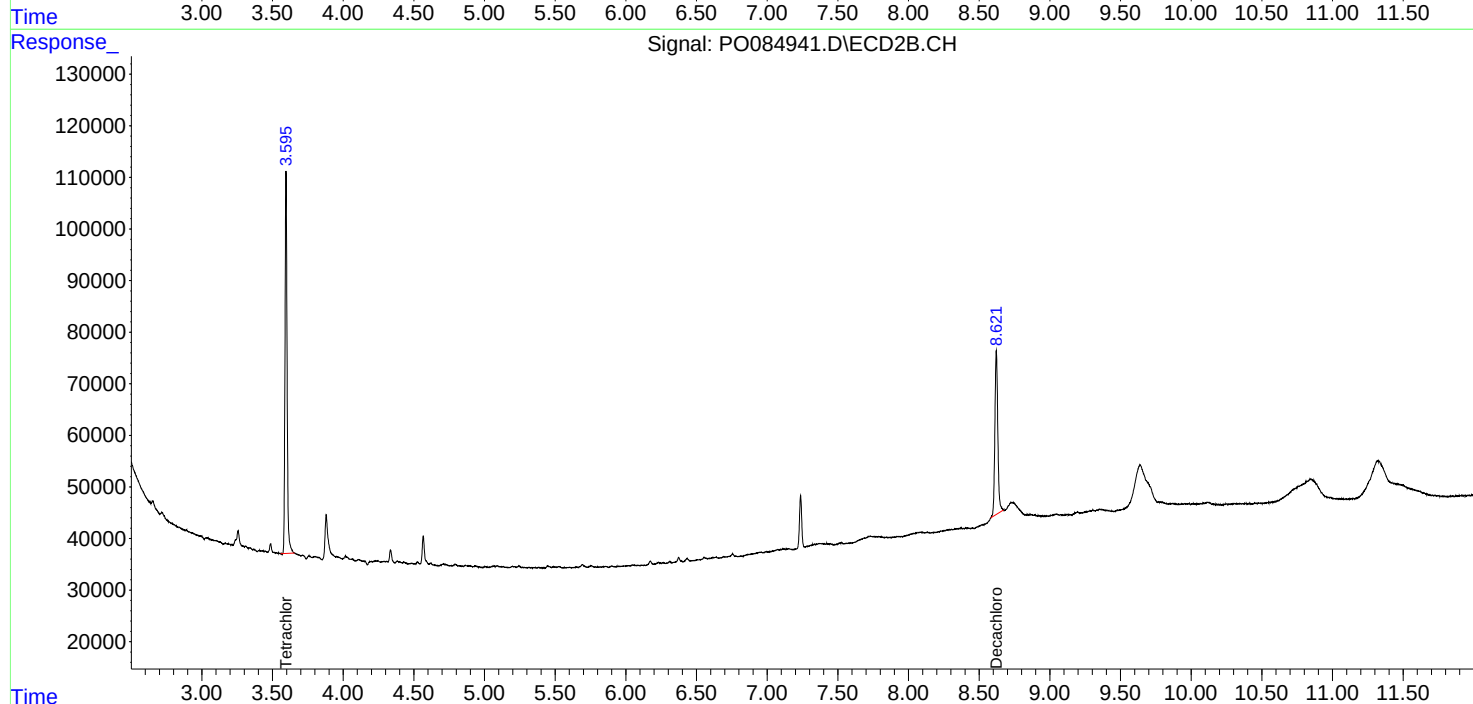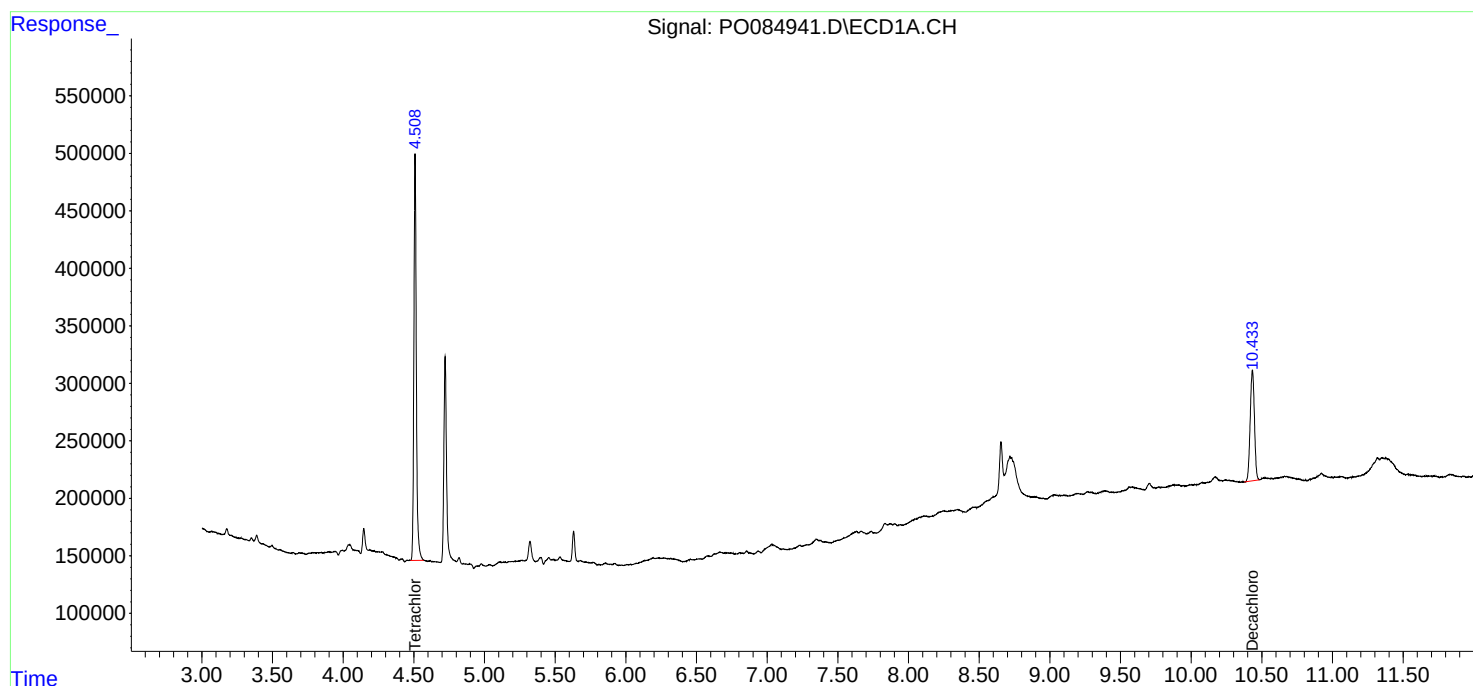


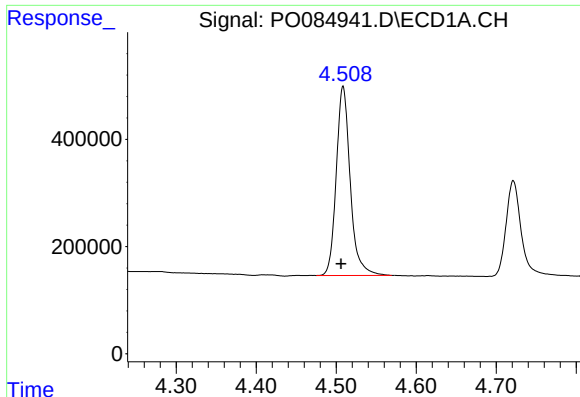

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 4286787
Conc: 15.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220214-096-21-02-ELUTRIATE

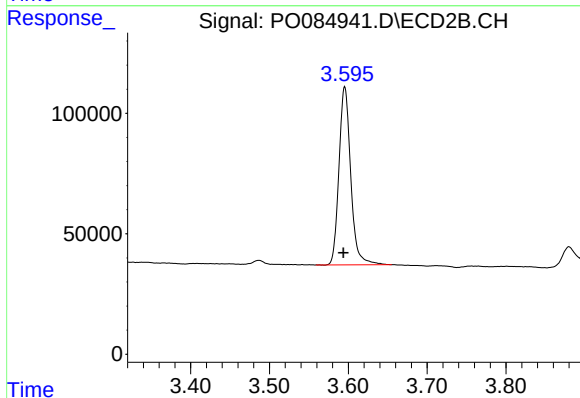


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.002 min
Response: 767970
Conc: 17.08 ng/ml

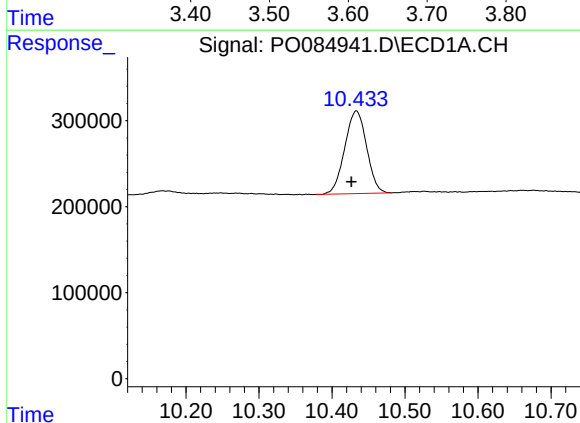

#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.007 min
Response: 1999751
Conc: 11.41 ng/ml

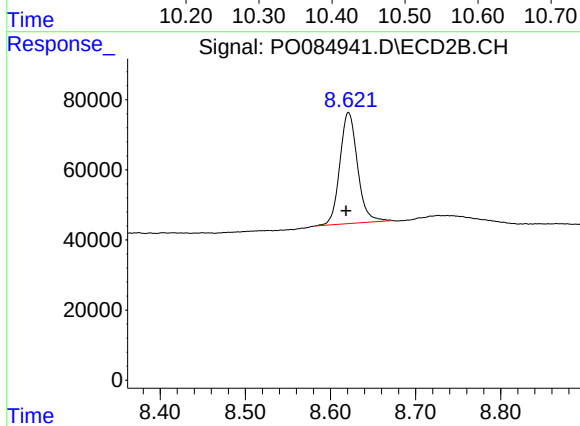

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: 0.003 min
Response: 456458
Conc: 12.42 ng/ml