

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030122\
 Data File : P0084950.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2022 17:01
 Operator : YP\AJ
 Sample : N1715-04 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-68B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/02/2022
 Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:24:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.594	305321	73199	1.092	1.628m#
2) SA Decachlor...	10.434	8.624	238817	59895	1.362	1.630

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030122\
Data File : P0084950.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2022 17:01
Operator : YP\AJ
Sample : N1715-04 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRV-2022-68B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:24:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

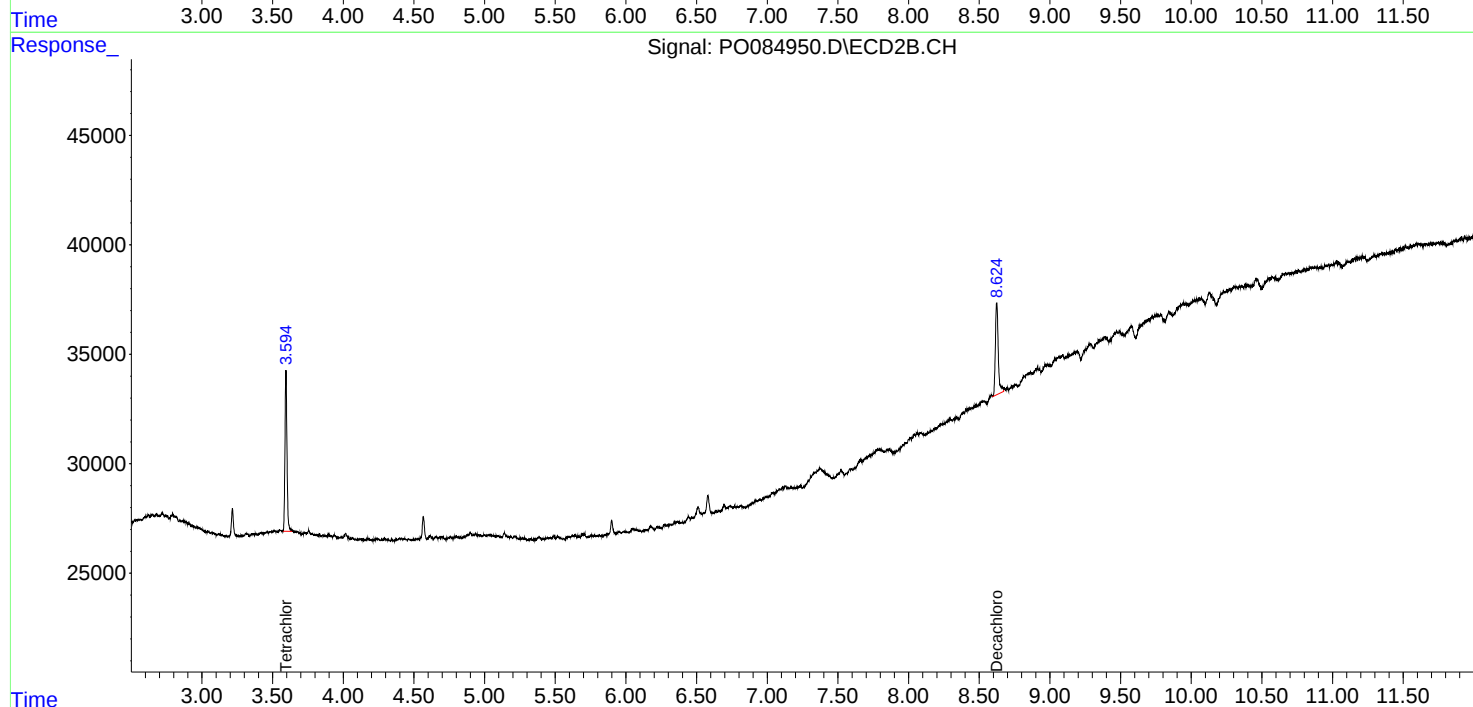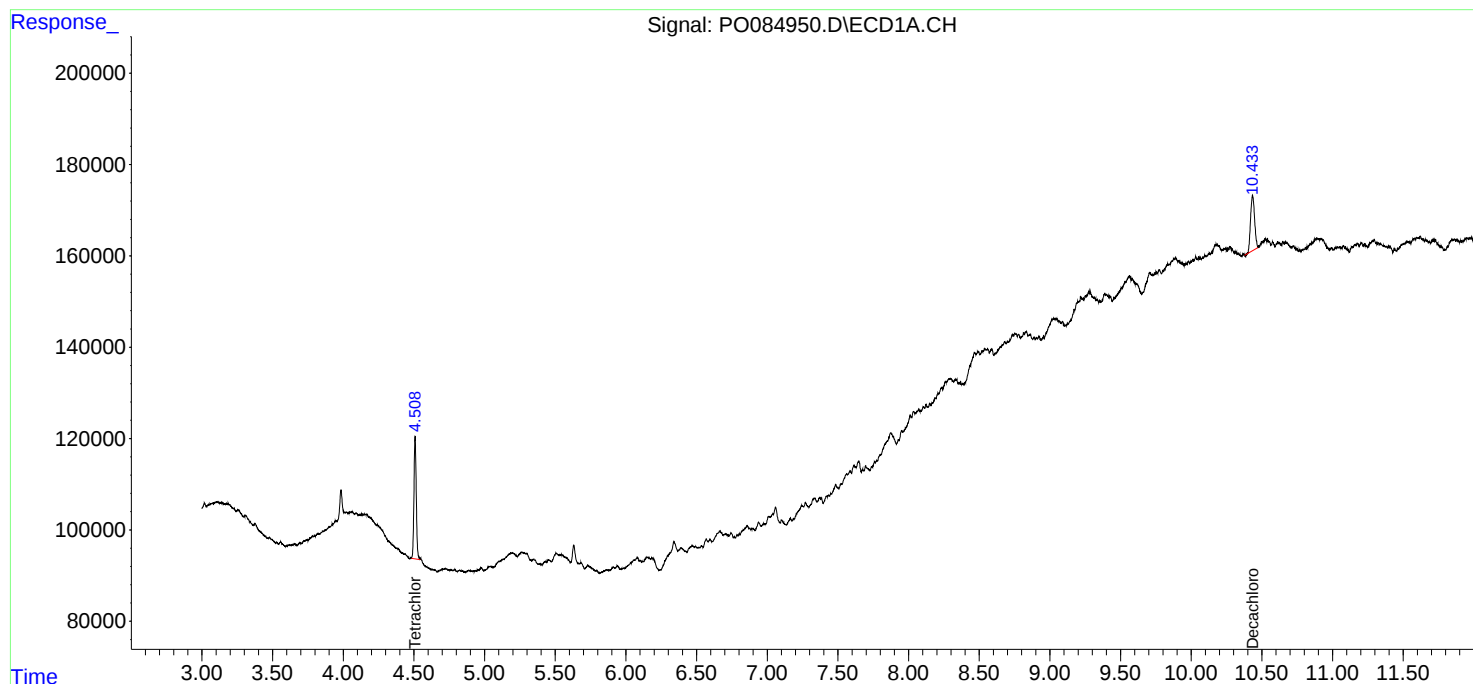

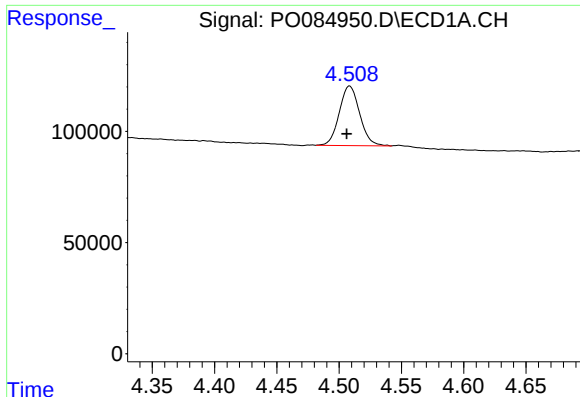


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: 0.002 min
Response: 305321
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

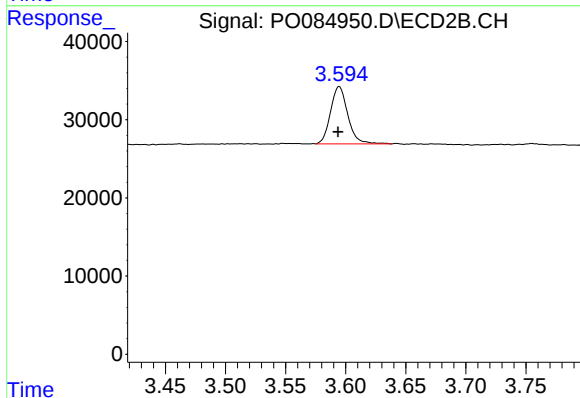


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 73199
Conc: 1.63 ng/ml m

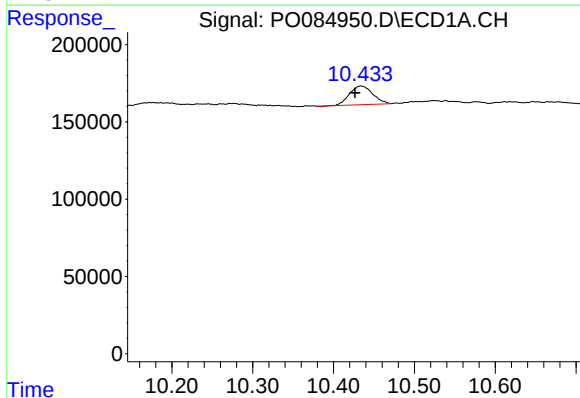

#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.007 min
Response: 238817
Conc: 1.36 ng/ml

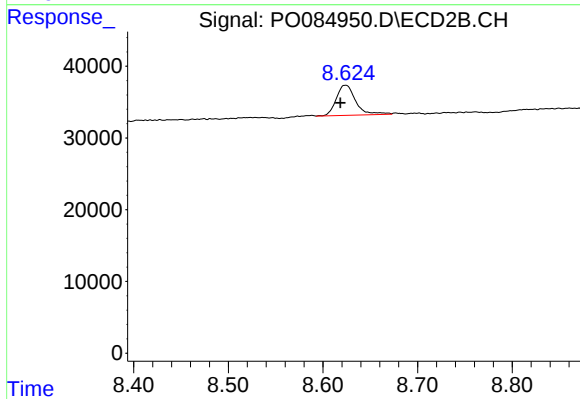

#2 Decachlorobiphenyl

R.T.: 8.624 min
Delta R.T.: 0.006 min
Response: 59895
Conc: 1.63 ng/ml