

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030122\
 Data File : P0084961.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2022 20:35
 Operator : YP\AJ
 Sample : N1716-06 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDA546E-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/02/2022
 Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:32:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.595	418482	83840	1.497m	1.864
2) SA Decachlor...	10.436	8.624	309385	66728	1.765	1.816
Target Compounds						
26) L6 AR-1254-1	6.567	5.491	2600232	898819	265.102	335.982 #
27) L6 AR-1254-2	6.789	5.640	4008087	841542	270.075	356.778 #
28) L6 AR-1254-3	7.161	6.044	3794331	1187053	250.596	315.738 #
29) L6 AR-1254-4	7.450	6.274	2911140	733704	271.415	313.027
30) L6 AR-1254-5	7.875	6.694	3017299	963714	256.243	284.814

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030122\
Data File : PO084961.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2022 20:35
Operator : YP\AJ
Sample : N1716-06 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FDA546E-END-1-2


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 03/02/2022
Supervised By : Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:32:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

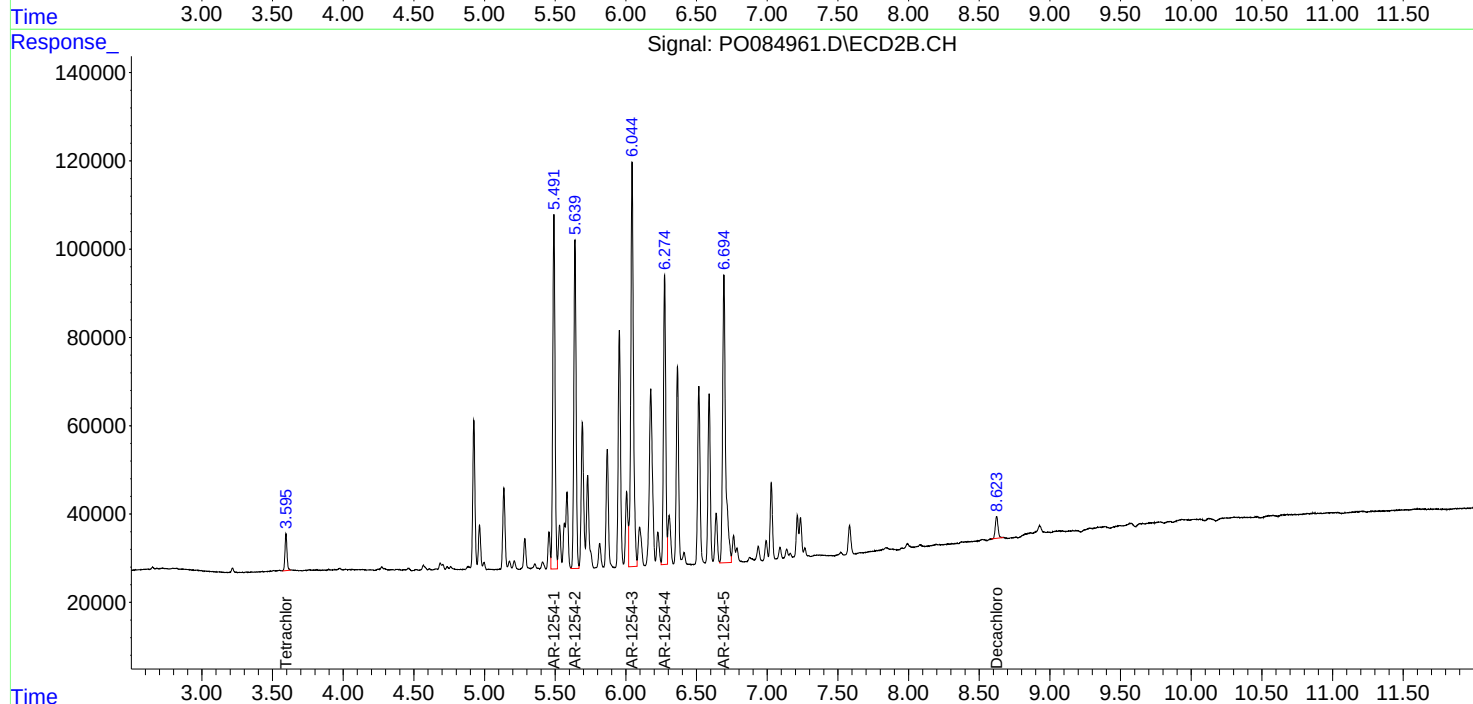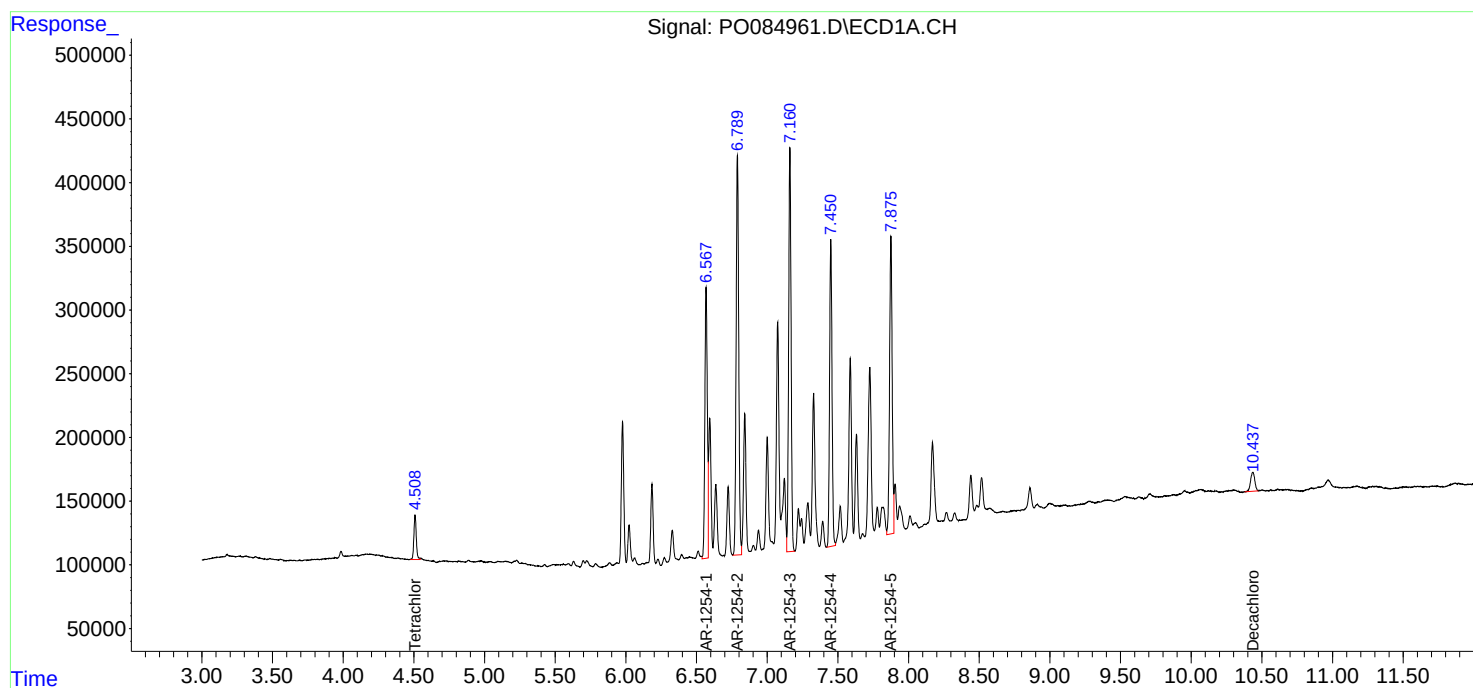

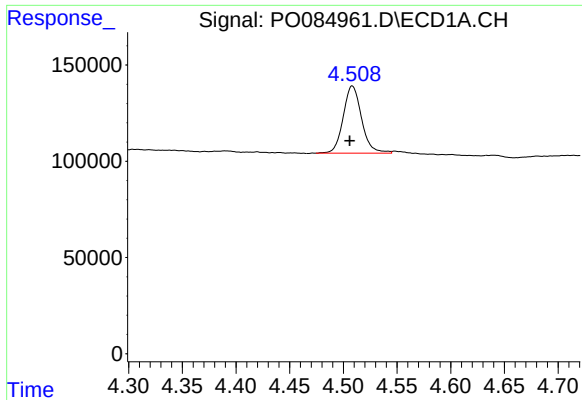


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: 0.002 min
Response: 418482
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDA546E-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

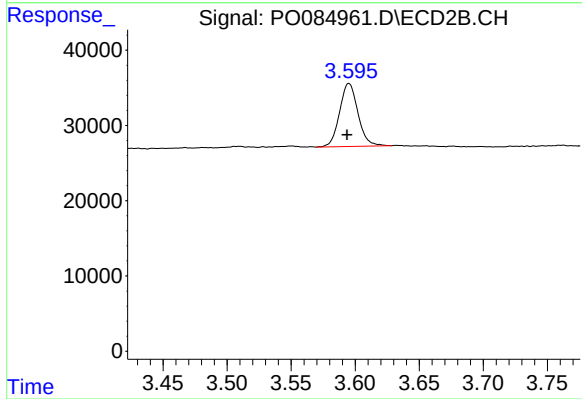


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.002 min
Response: 83840
Conc: 1.86 ng/ml

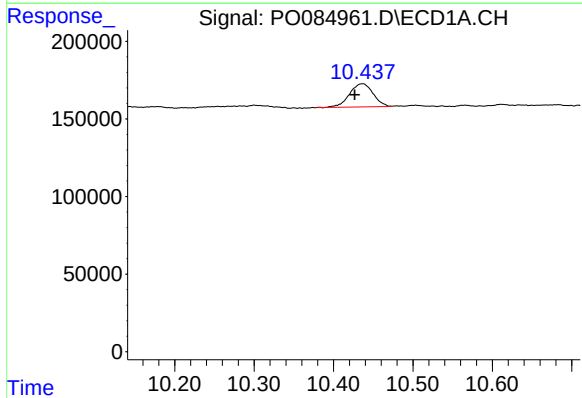


#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.010 min
Response: 309385
Conc: 1.77 ng/ml

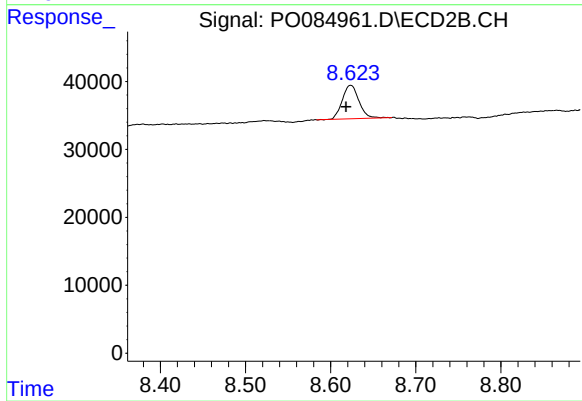

#2 Decachlorobiphenyl

R.T.: 8.624 min
Delta R.T.: 0.005 min
Response: 66728
Conc: 1.82 ng/ml

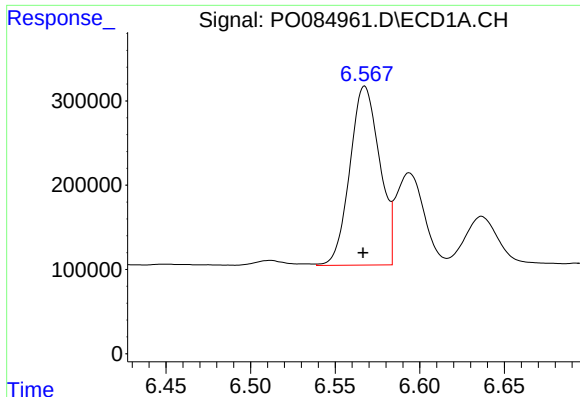


#26 AR-1254-1

R.T.: 6.567 min
Delta R.T.: 0.000 min
Response: 2600232
Conc: 265.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDA546E-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

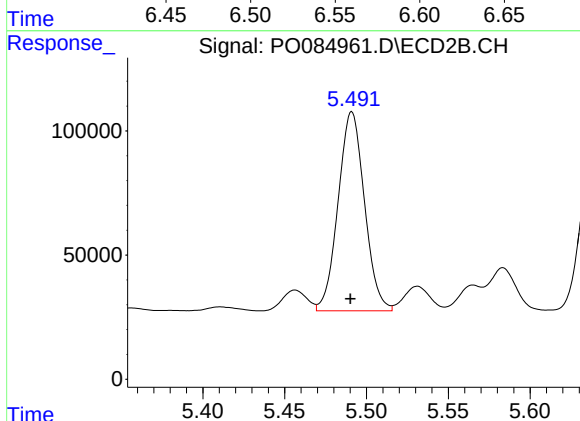


#26 AR-1254-1

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 898819
Conc: 335.98 ng/ml

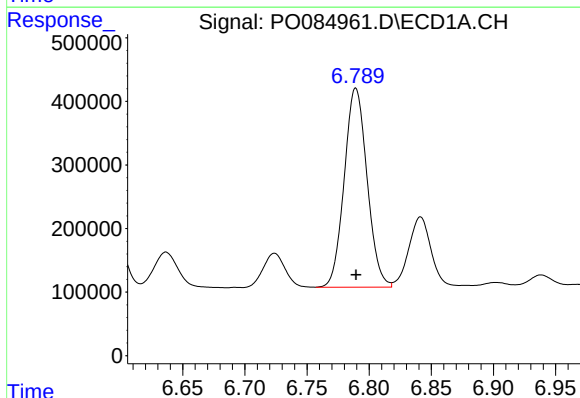


#27 AR-1254-2

R.T.: 6.789 min
Delta R.T.: 0.000 min
Response: 4008087
Conc: 270.08 ng/ml

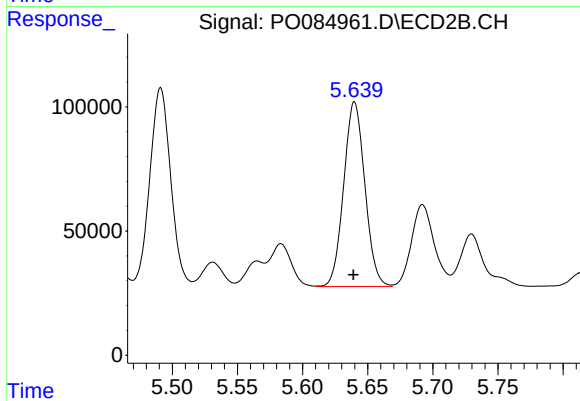

#27 AR-1254-2

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 841542
Conc: 356.78 ng/ml

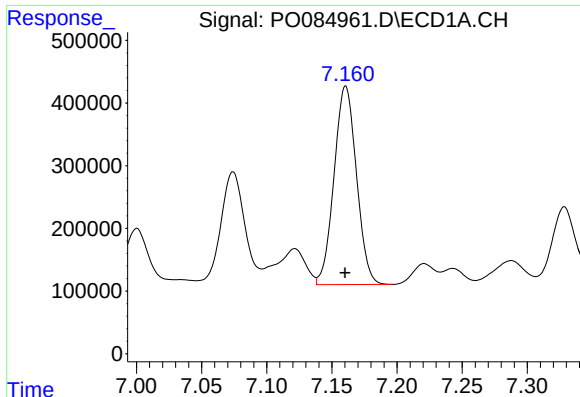


#28 AR-1254-3

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 3794331
Conc: 250.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDA546E-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

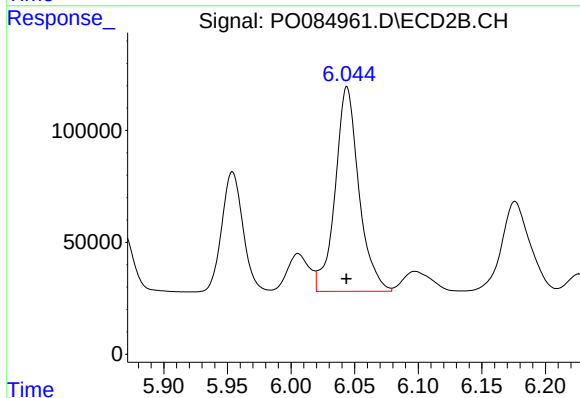


#28 AR-1254-3

R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 1187053
Conc: 315.74 ng/ml

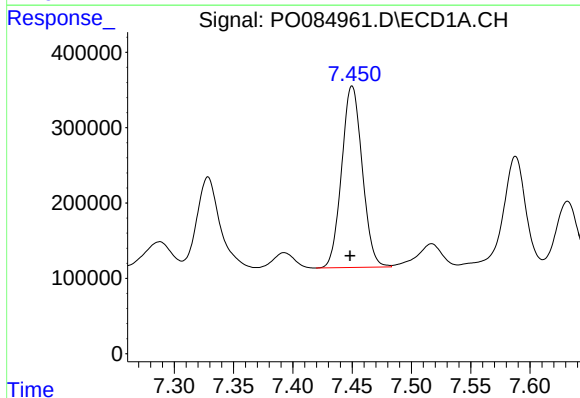


#29 AR-1254-4

R.T.: 7.450 min
Delta R.T.: 0.002 min
Response: 2911140
Conc: 271.42 ng/ml

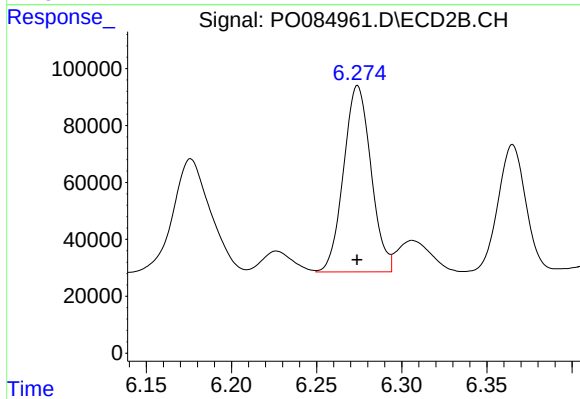

#29 AR-1254-4

R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 733704
Conc: 313.03 ng/ml

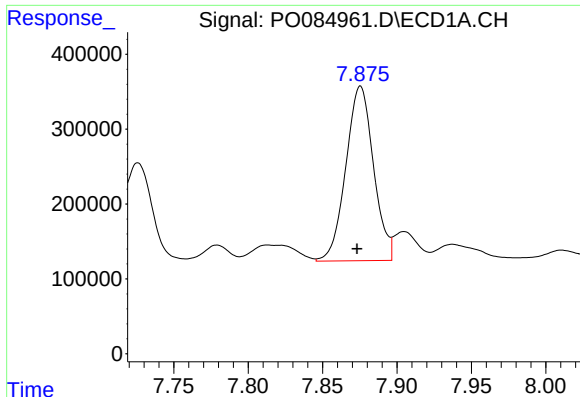


#30 AR-1254-5

R.T.: 7.875 min
Delta R.T.: 0.002 min
Response: 3017299
Conc: 256.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDA546E-END-1-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

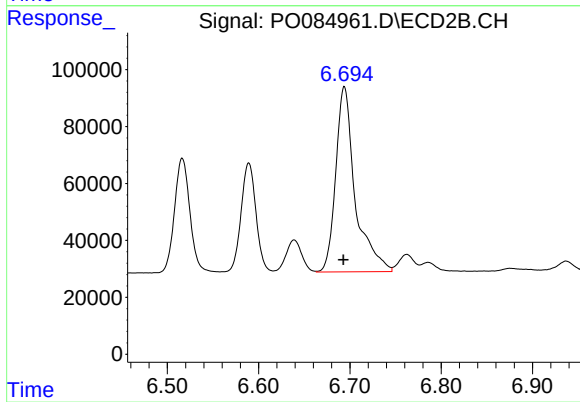

#30 AR-1254-5

R.T.: 6.694 min
Delta R.T.: 0.001 min
Response: 963714
Conc: 284.81 ng/ml