

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030124\
 Data File : P0102259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2024 11:20
 Operator : YP/AJ
 Sample : P1654-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC136902-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2024
 Supervised By :Ankita Jodhani 03/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:25:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.387	6194132	4355423	1.336m	1.340m
2) SA Decachlor...	9.814	8.256	4378063	2556600	1.719m	1.236m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030124\
Data File : PO102259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2024 11:20
Operator : YP/AJ
Sample : P1654-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC136902-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2024
Supervised By :Ankita Jodhani 03/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:25:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

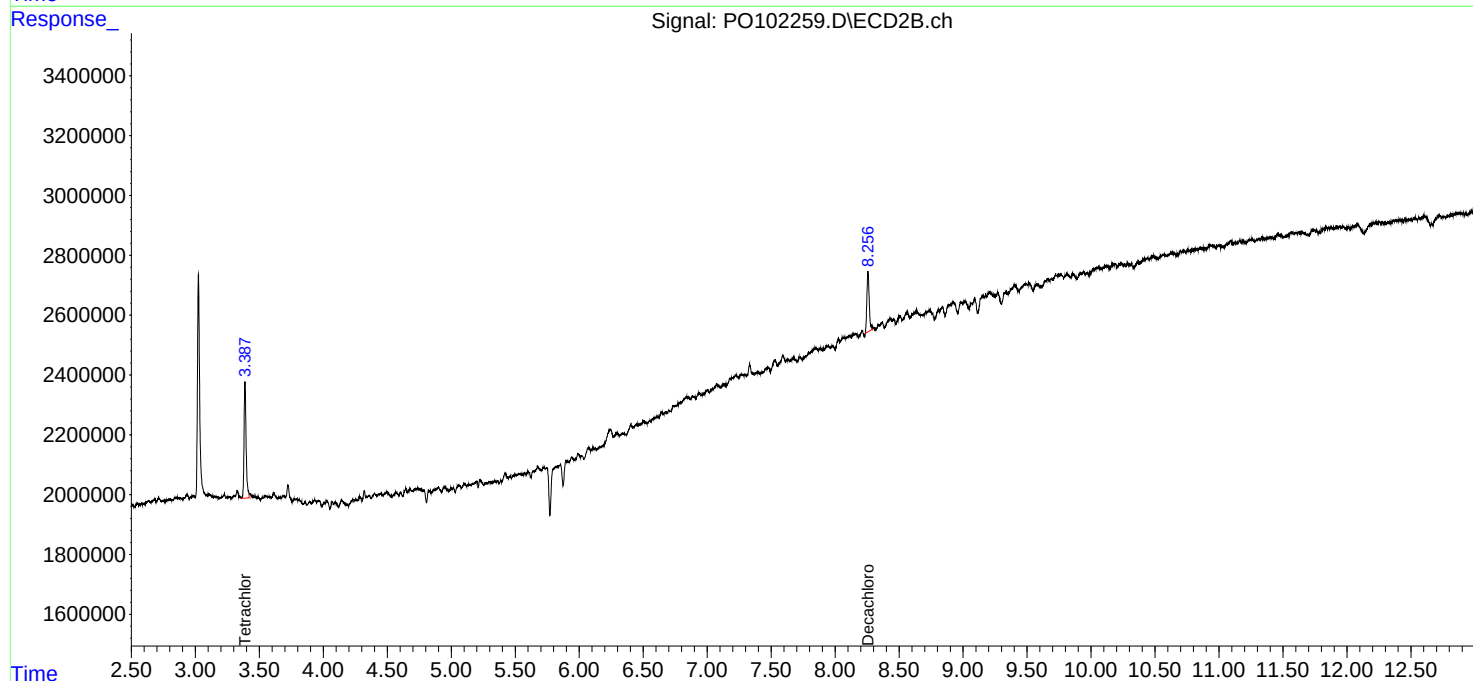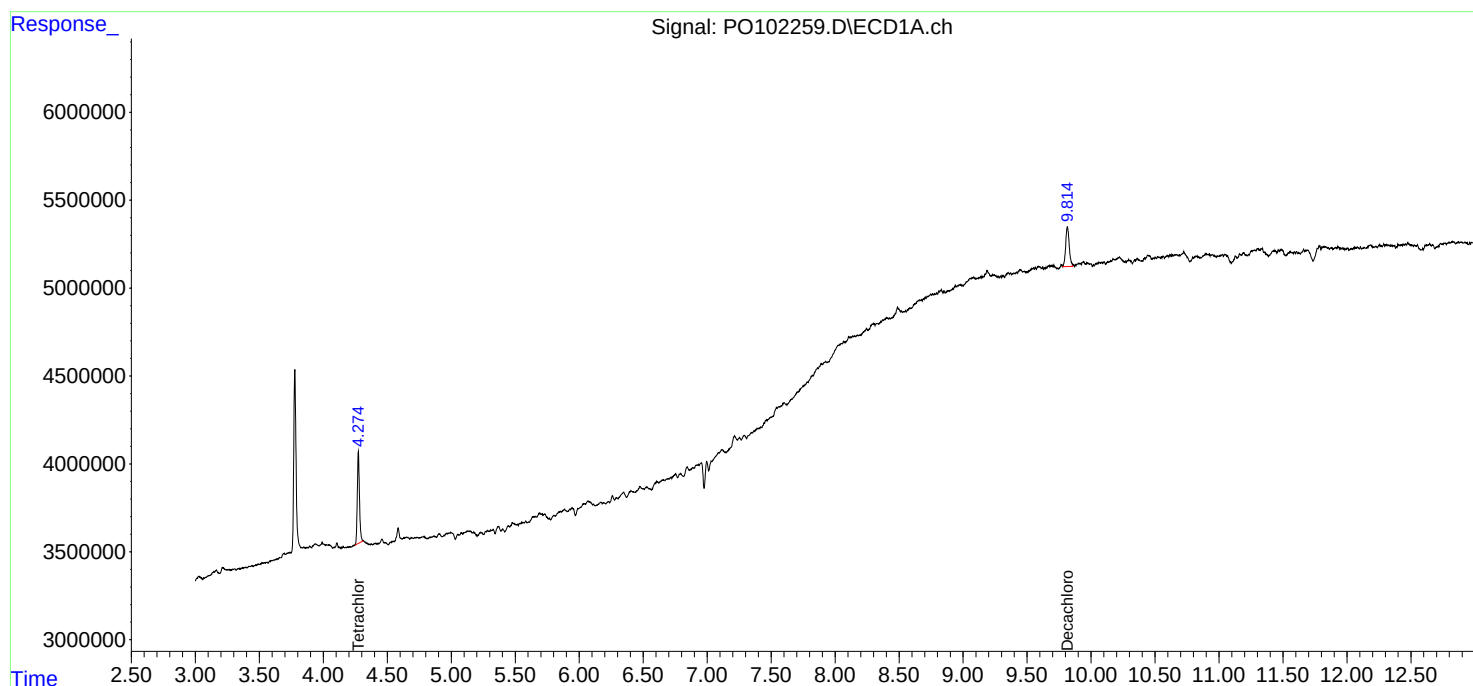

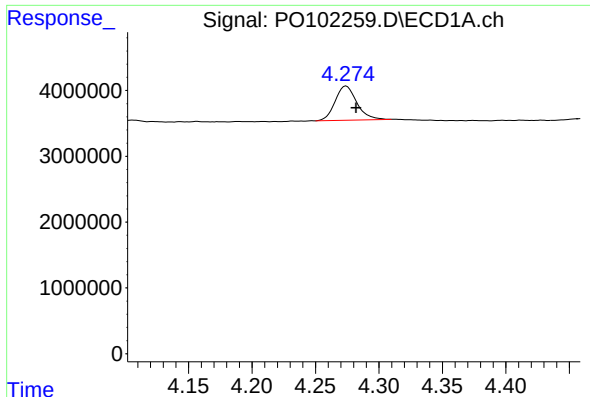


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.008 min
Response: 6194132
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC136902-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2024
Supervised By :Ankita Jodhani 03/04/2024

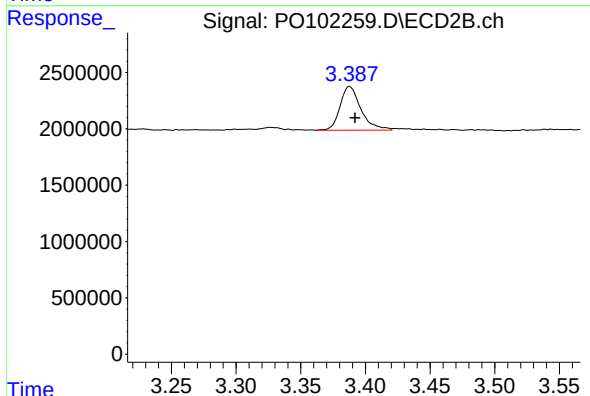


#1 Tetrachloro-m-xylene

R.T.: 3.387 min
Delta R.T.: -0.005 min
Response: 4355423
Conc: 1.34 ng/ml m

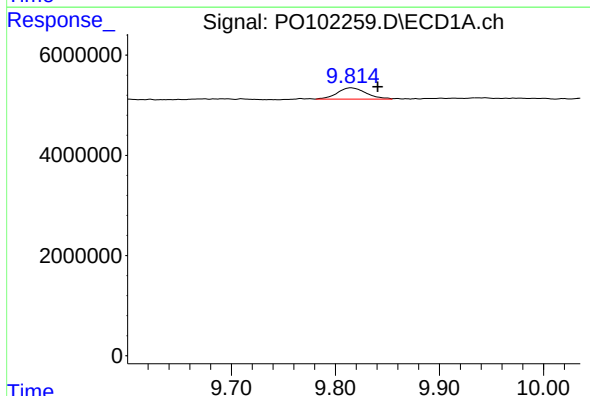

#2 Decachlorobiphenyl

R.T.: 9.814 min
Delta R.T.: -0.027 min
Response: 4378063
Conc: 1.72 ng/ml m

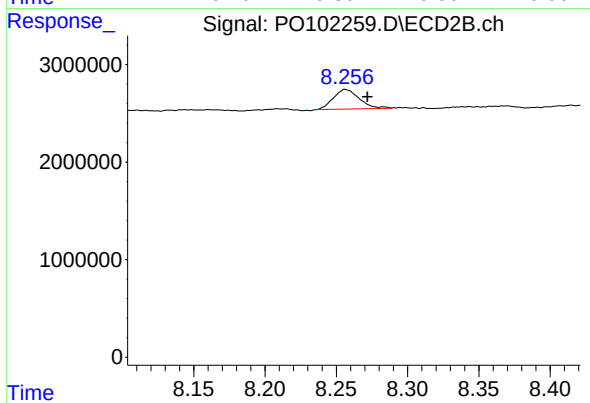

#2 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.016 min
Response: 2556600
Conc: 1.24 ng/ml m