

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030124\
 Data File : P0102293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2024 22:26
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2024
 Supervised By :Ankita Jodhani 03/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:44:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Feb 25 11:24:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.388	74278566	54312401	16.017	16.714
2) SA Decachlor...	9.815	8.256	51621965	36704508	20.273	17.742m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030124\
Data File : PO102293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2024 22:26
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2024
Supervised By :Ankita Jodhani 03/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:44:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022324.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Feb 25 11:24:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

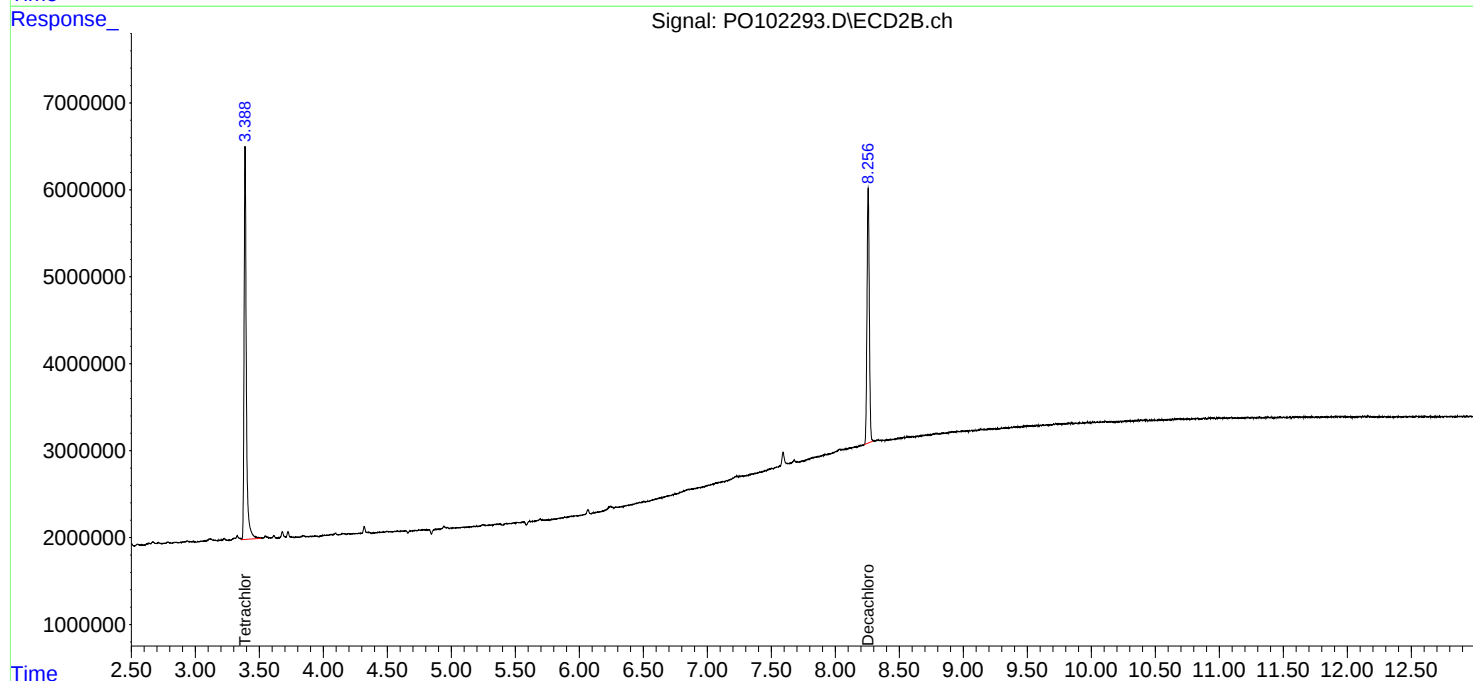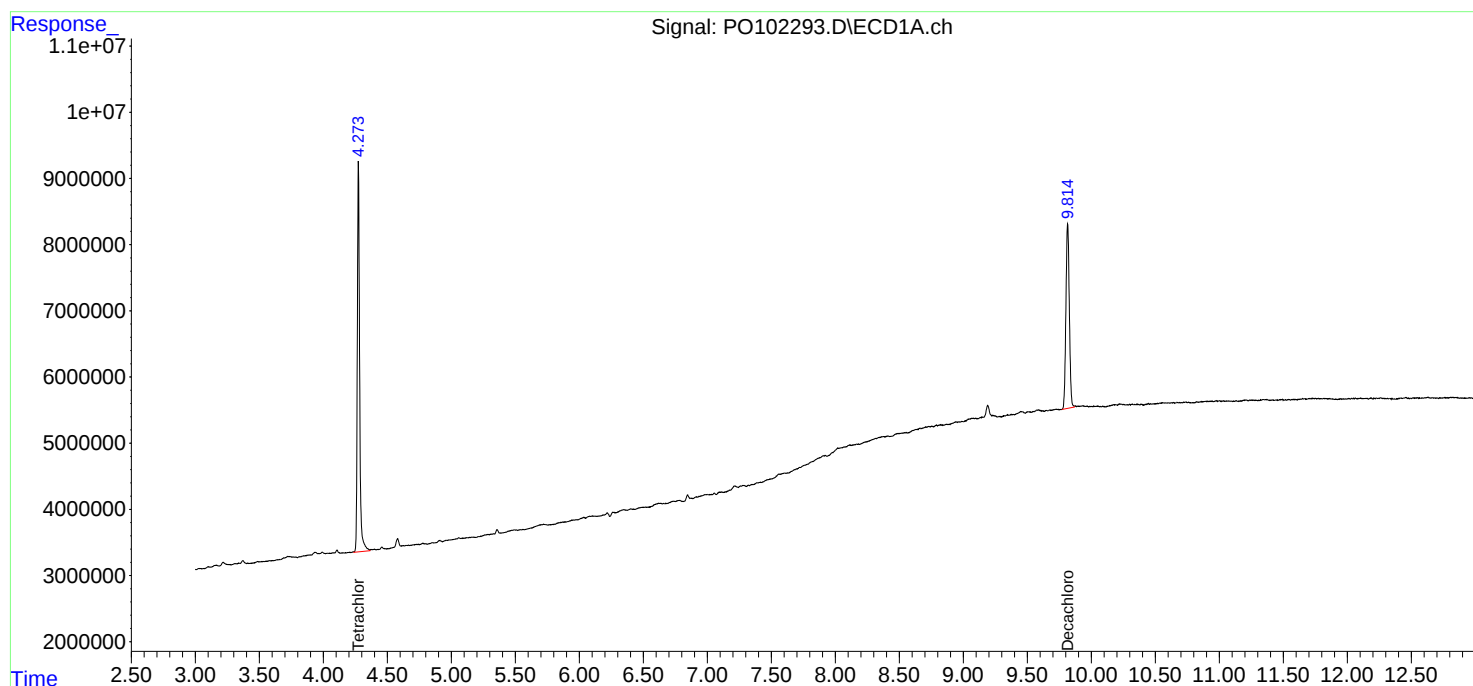

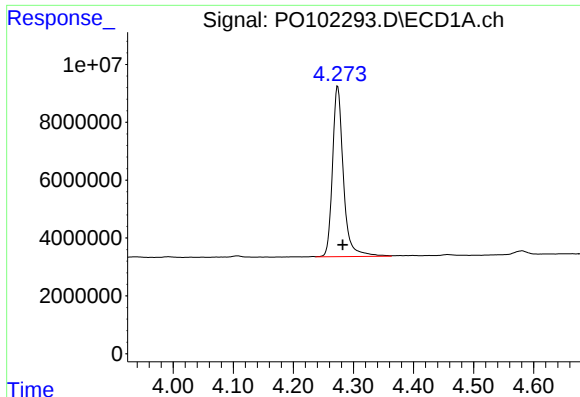

#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.008 min
Response: 74278566
Conc: 16.02 ng/ml

Instrument :


ECD_O

ClientSampleId :

I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2024
Supervised By :Ankita Jodhani 03/04/2024

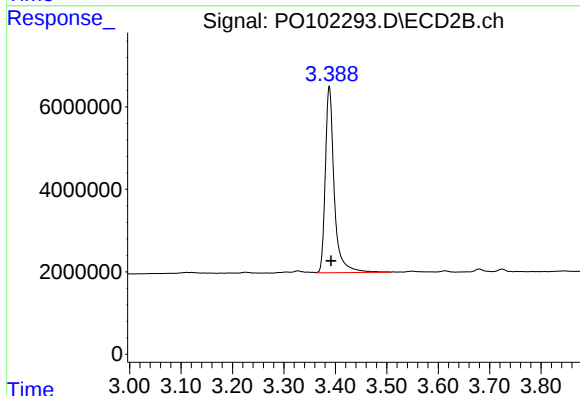


#1 Tetrachloro-m-xylene

R.T.: 3.388 min
Delta R.T.: -0.004 min
Response: 54312401
Conc: 16.71 ng/ml

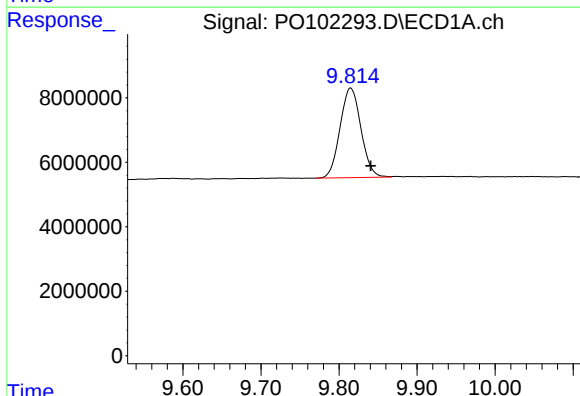

#2 Decachlorobiphenyl

R.T.: 9.815 min
Delta R.T.: -0.026 min
Response: 51621965
Conc: 20.27 ng/ml

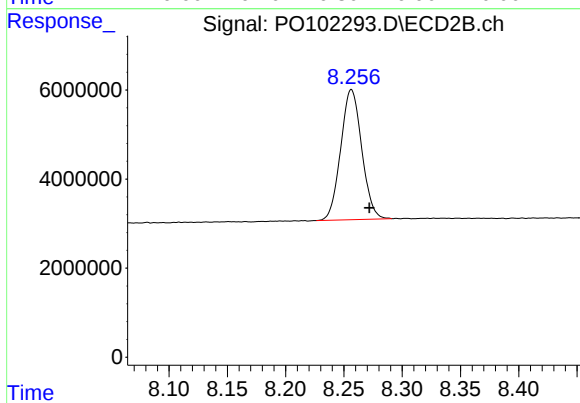

#2 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.016 min
Response: 36704508
Conc: 17.74 ng/ml m