

Data Path : P:\HPCHEM1\ECD 0\Data\P0030218\
 Data File : P0042707.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2018 9:37
 Operator : SM/UA
 Sample : J1705-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 230KV-CONCRETE-REACTOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 10:42:34 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.098	3.344	4026152	5452732	16.253	14.756
2) SA Decachlor...	9.472	8.125	4585655	7265697	18.144	18.842

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD 0\Data\P0030218\
Data File : P0042707.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2018 9:37
Operator : SM/UA
Sample : J1705-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
230KV-CONCRETE-REACTOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 10:42:34 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

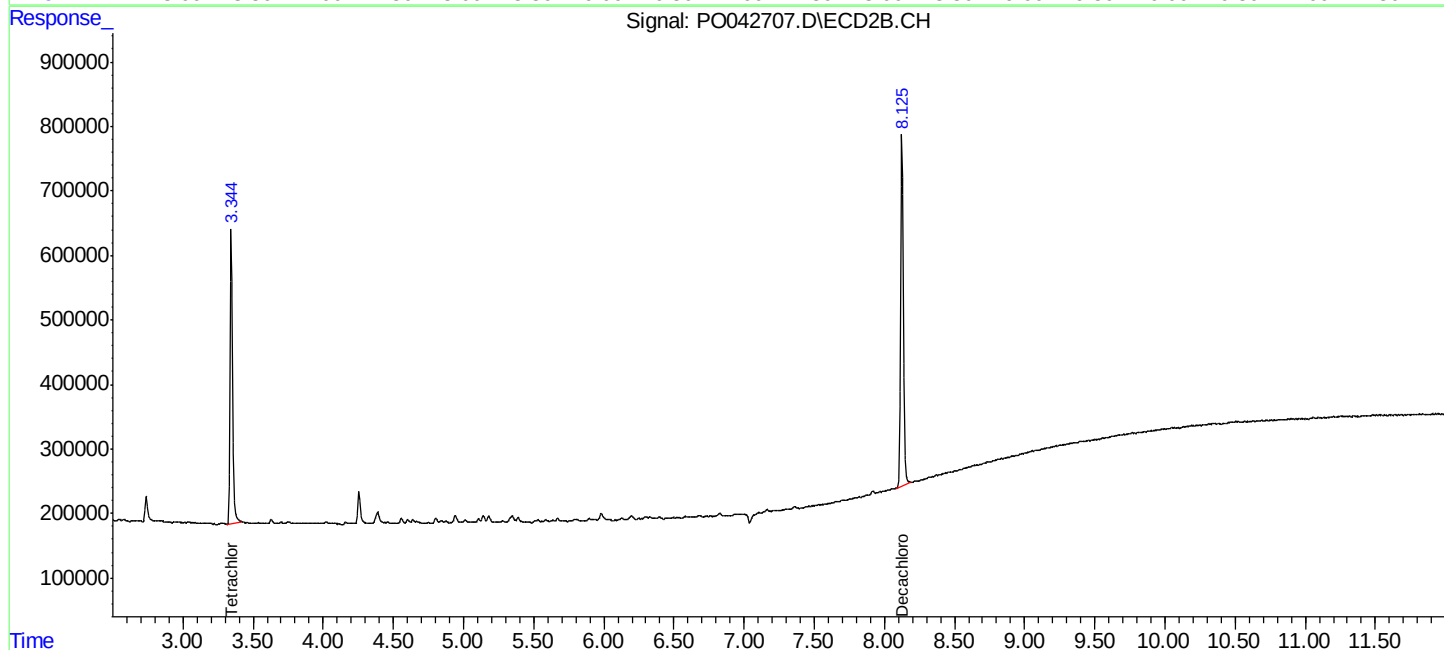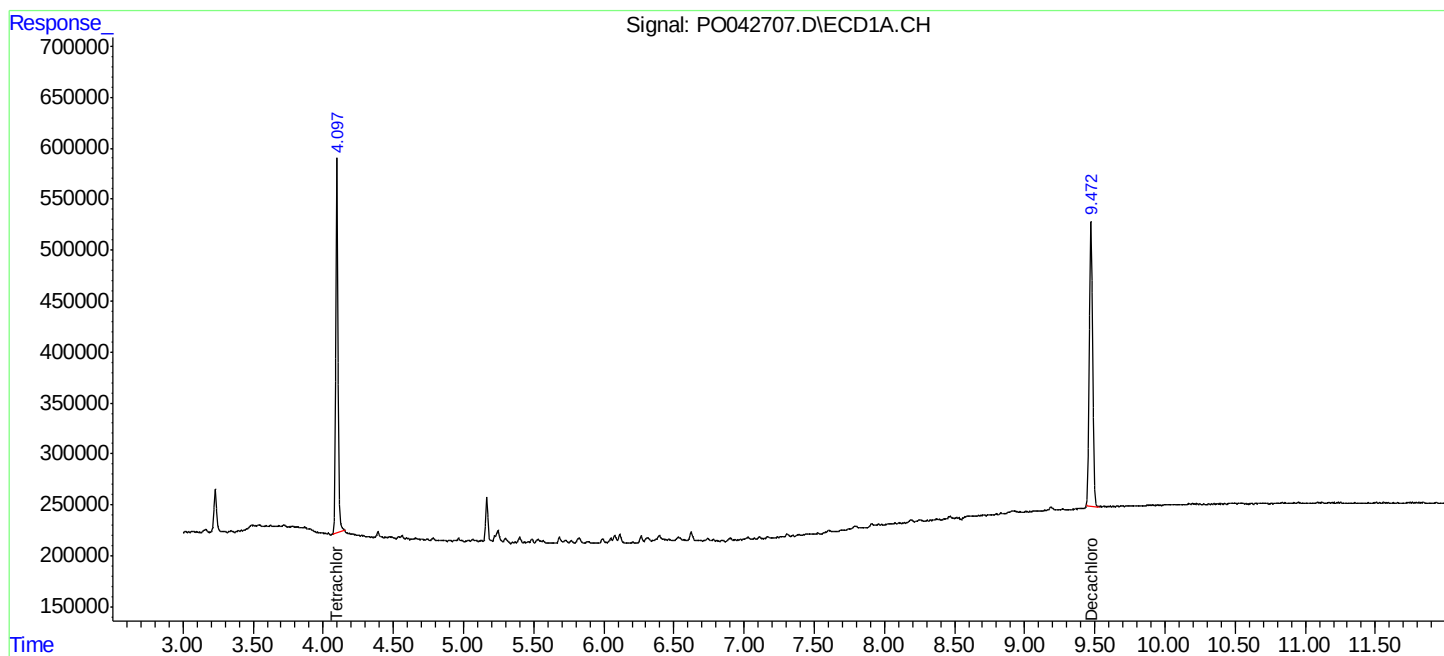


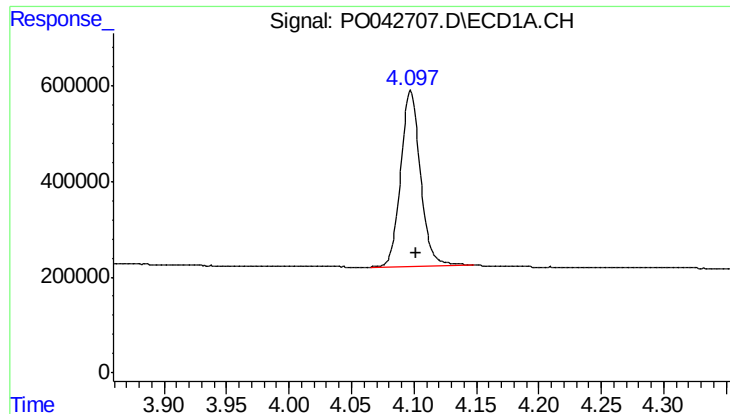

#1 Tetrachloro-m-xylene


R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 4026152
Conc: 16.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
230KV-CONCRETE-REACTOR

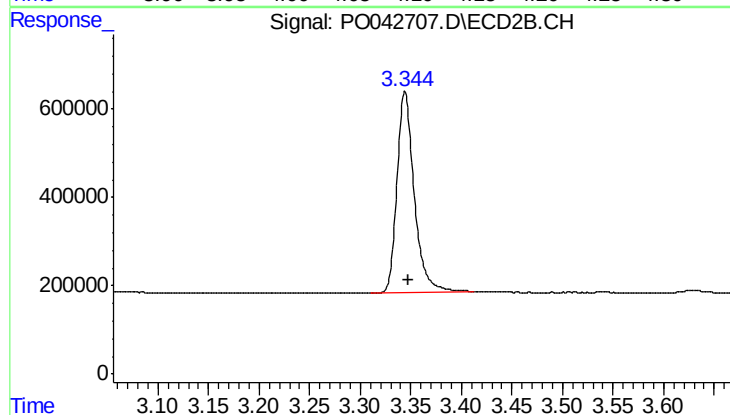


#1 Tetrachloro-m-xylene

R.T.: 3.344 min
Delta R.T.: -0.004 min
Response: 5452732
Conc: 14.76 ng/ml

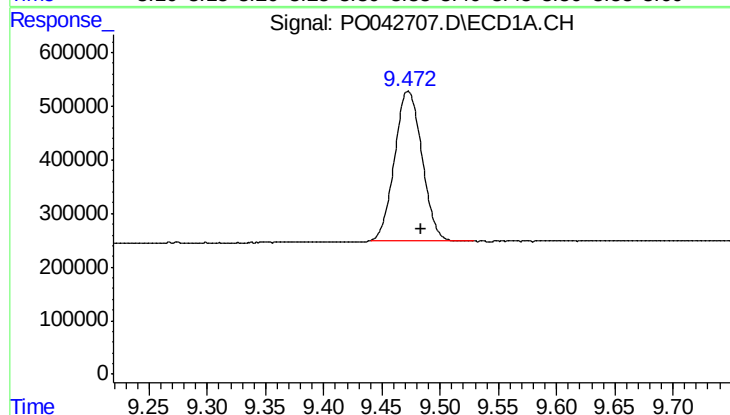

#2 Decachlorobiphenyl

R.T.: 9.472 min
Delta R.T.: -0.012 min
Response: 4585655
Conc: 18.14 ng/ml

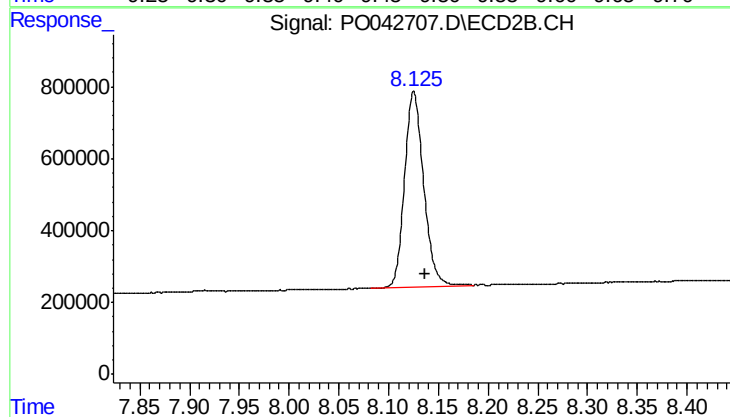

#2 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.011 min
Response: 7265697
Conc: 18.84 ng/ml