

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
 Data File : P0075800.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2021 11:33
 Operator : AJ/MA
 Sample : M1489-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-41087-88RE

Manual Integrations
 APPROVED

Ankita
 3/3/2021 11:19:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 16:47:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.952	419530	329206	6.863	7.452m
2) SA Decachlor...	10.946	9.222	214048	227444	4.704	5.241

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
Data File : P0075800.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2021 11:33
Operator : AJ/MA
Sample : M1489-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-41087-88RE


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 16:47:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

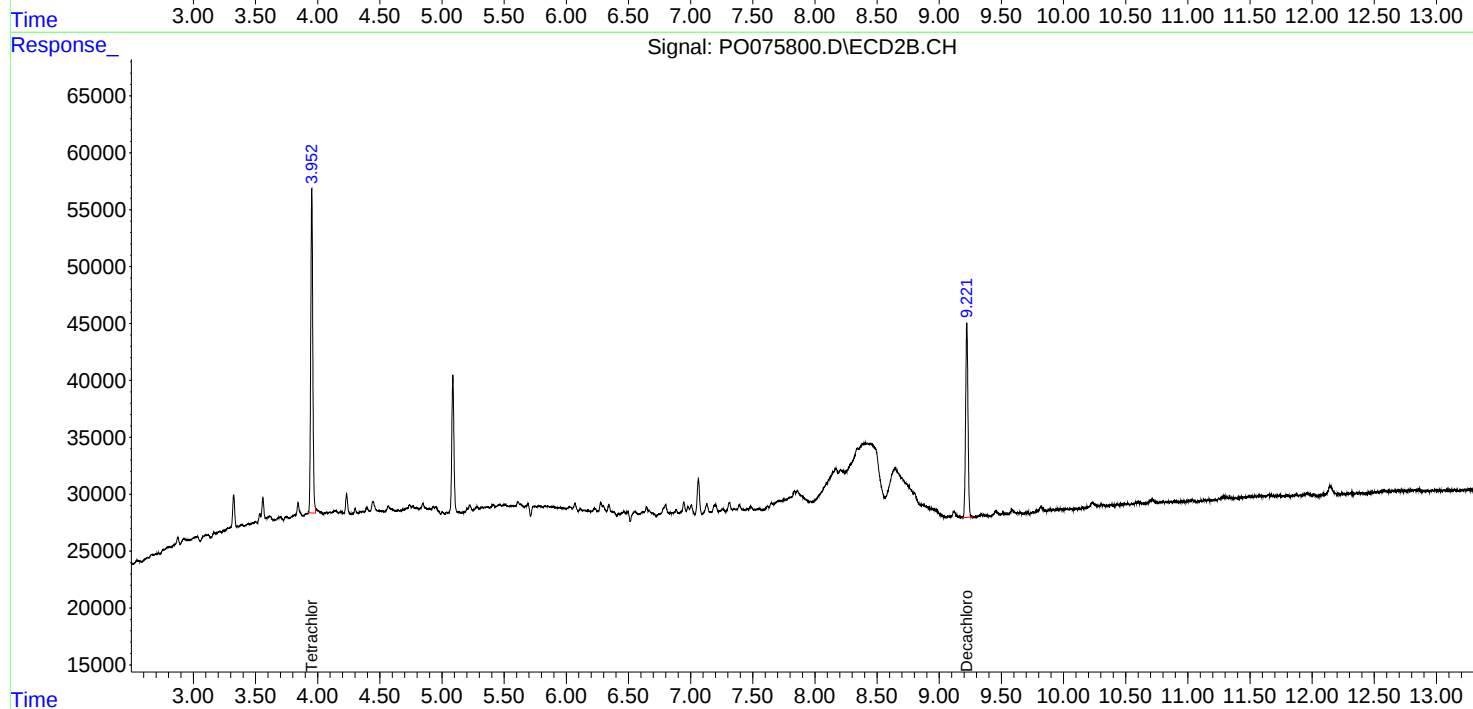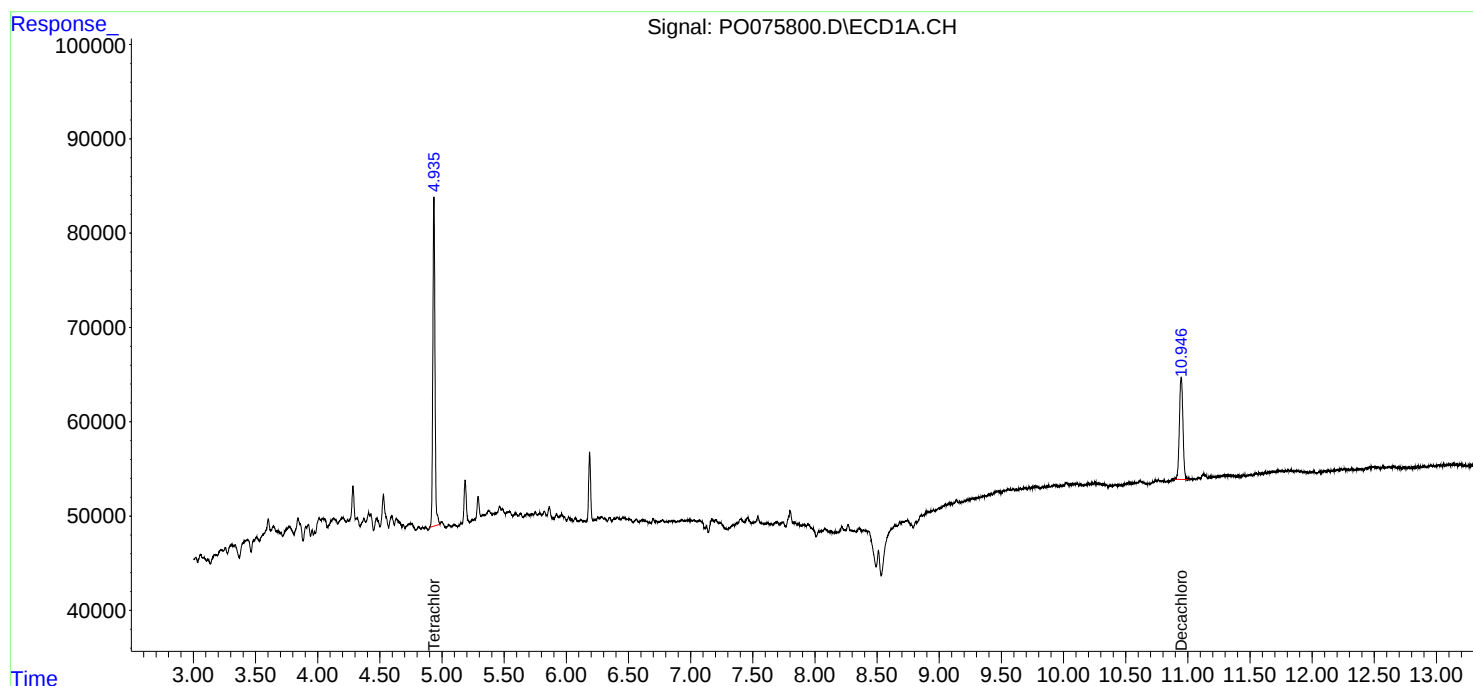

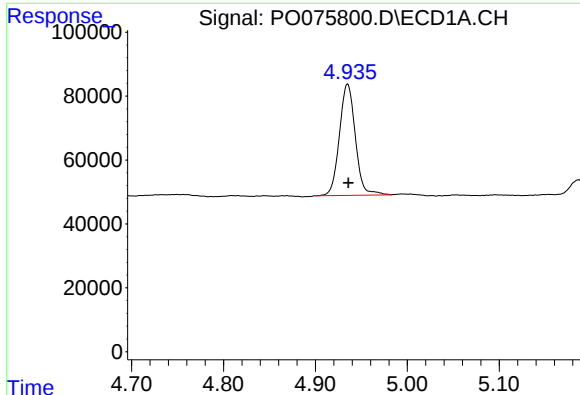


#1 Tetrachloro-m-xylene

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 419530
Conc: 6.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-41087-88RE


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:10 AM

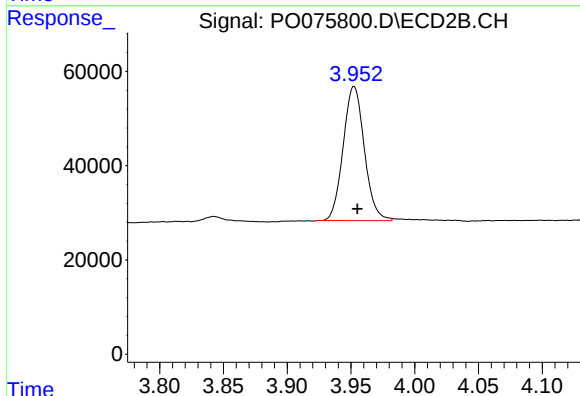


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: -0.003 min
Response: 329206
Conc: 7.45 ng/ml m

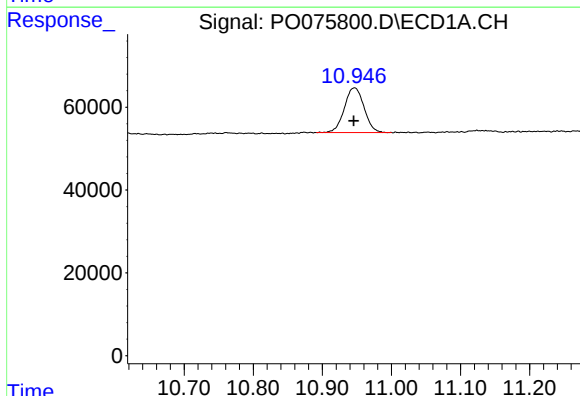

#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 214048
Conc: 4.70 ng/ml

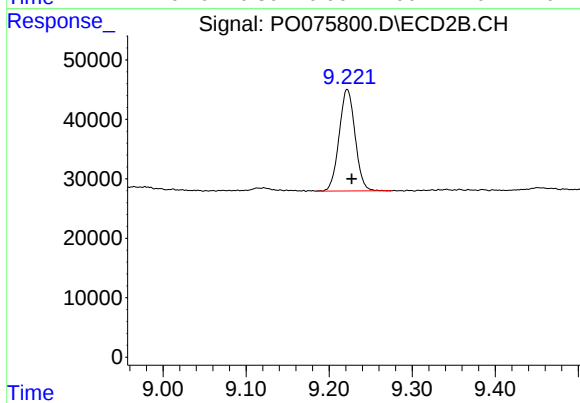

#2 Decachlorobiphenyl

R.T.: 9.222 min
Delta R.T.: -0.005 min
Response: 227444
Conc: 5.24 ng/ml