

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
 Data File : P0075802.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2021 12:08
 Operator : AJ/MA
 Sample : M1476-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ML-CON

Manual Integrations
 APPROVED

Ankita
 3/3/2021 11:19:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 16:48:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.953	828421	816999	13.552	18.493 #
2) SA Decachlor...	10.950	9.223	641168	764301	14.091	17.612
Target Compounds						
26) L6 AR-1254-1	7.177	6.072	41557	65126	17.671m	22.982 #
27) L6 AR-1254-2	7.406	6.229	106958	45843	29.781	18.512 #
28) L6 AR-1254-3	7.787	6.646	184121	88115	48.485	21.969m#
29) L6 AR-1254-4	8.081	6.887	85189	126372	30.702	48.089m#
30) L6 AR-1254-5	8.513	7.313	146751	366359	52.383m	104.340m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030221\
Data File : PO075802.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2021 12:08
Operator : AJ/MA
Sample : M1476-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
ML-CON


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 16:48:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

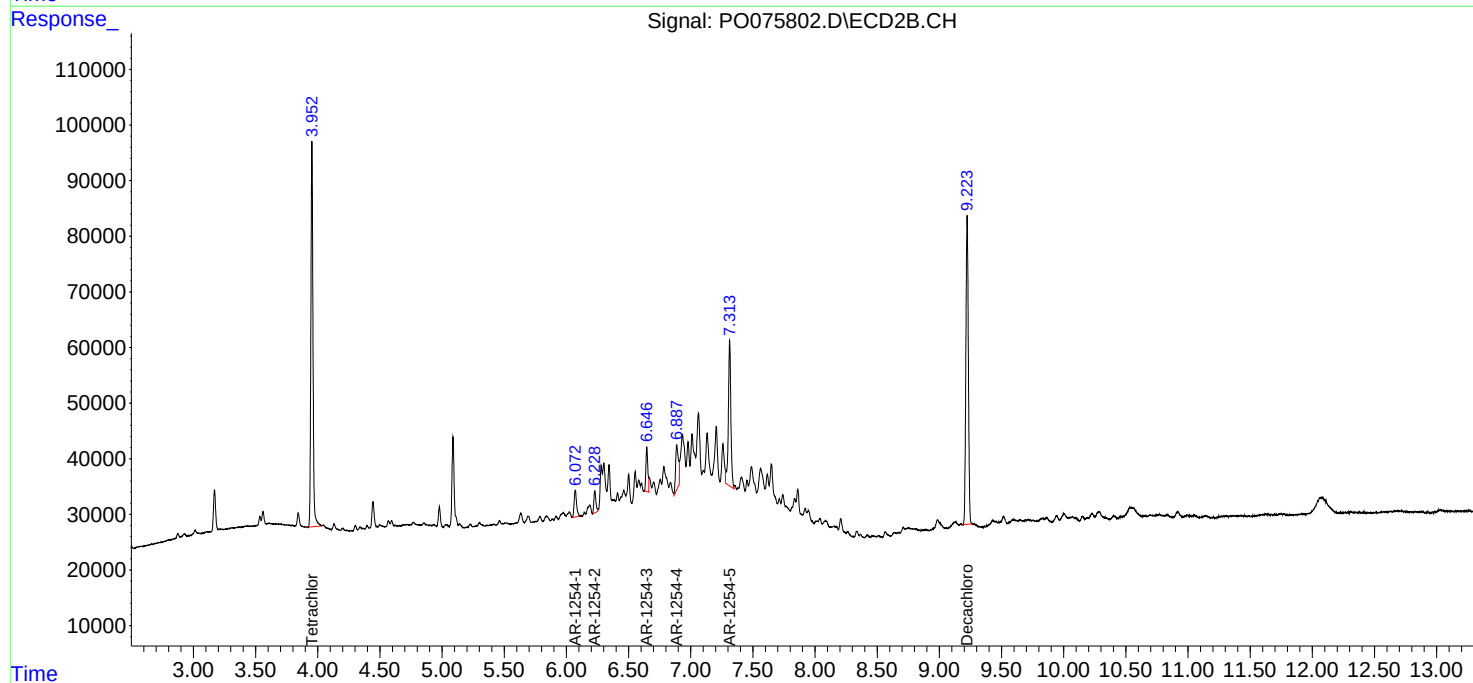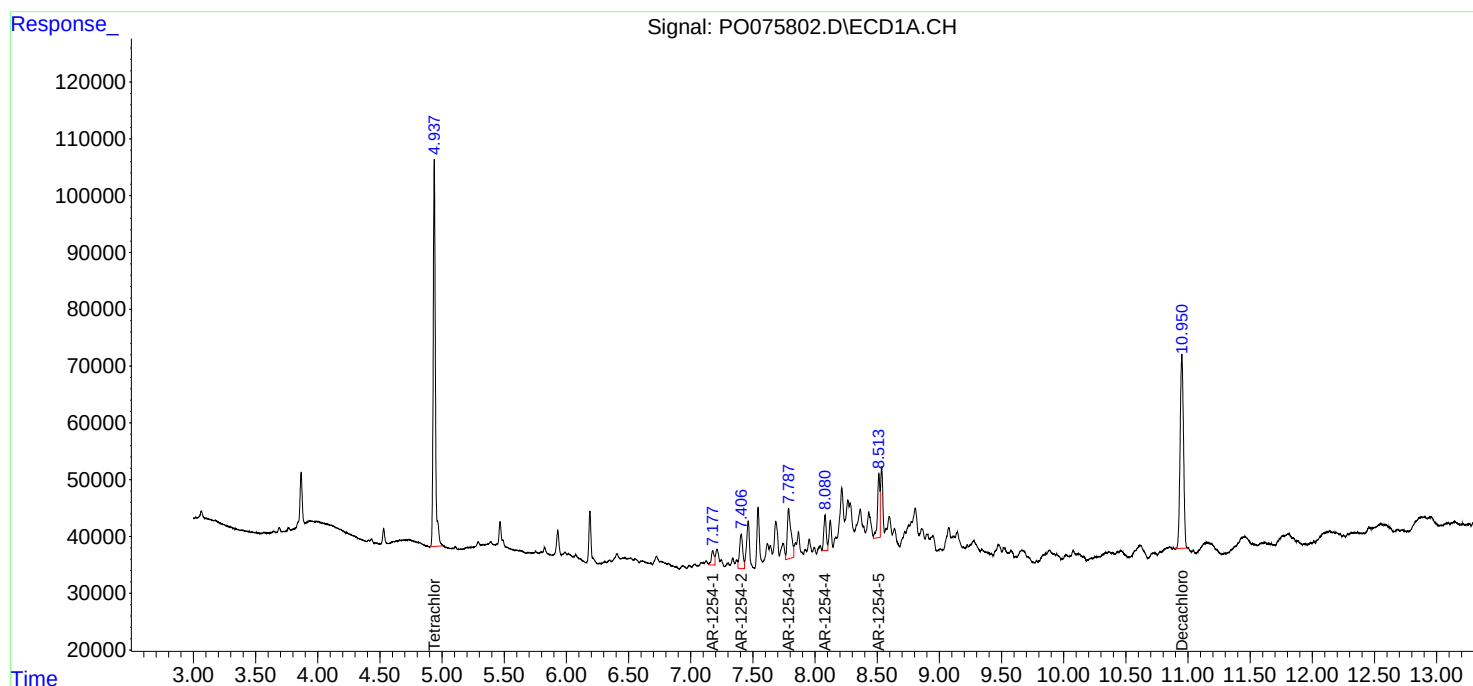

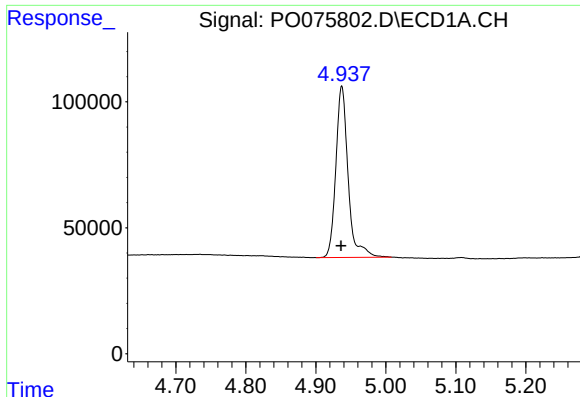


#1 Tetrachloro-m-xylene

R.T.: 4.937 min
Delta R.T.: 0.001 min
Response: 828421
Conc: 13.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
ML-CON


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:12 AM

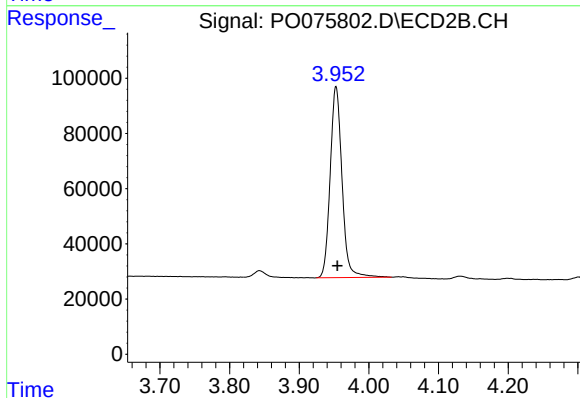


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.002 min
Response: 816999
Conc: 18.49 ng/ml

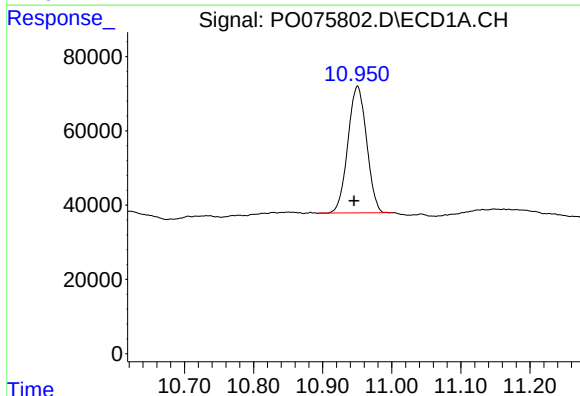


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.005 min
Response: 641168
Conc: 14.09 ng/ml

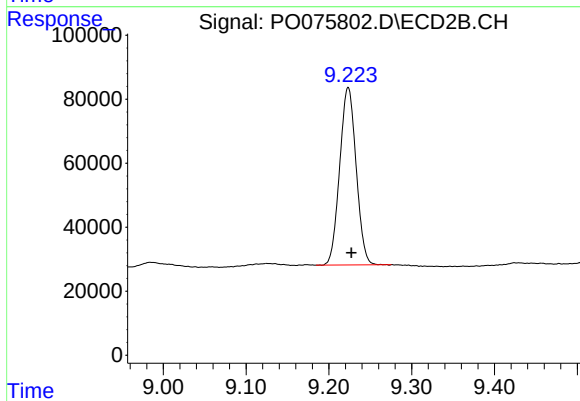

#2 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 764301
Conc: 17.61 ng/ml

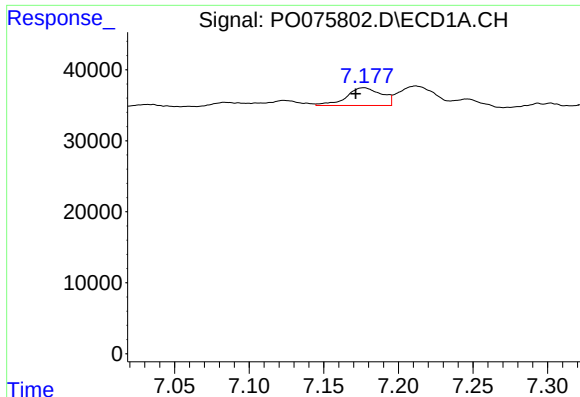


#26 AR-1254-1

R.T.: 7.177 min
Delta R.T.: 0.006 min
Response: 41557
Conc: 17.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ML-CON


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:12 AM

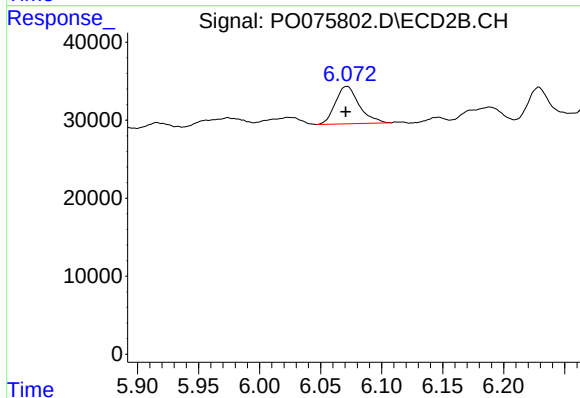


#26 AR-1254-1

R.T.: 6.072 min
Delta R.T.: 0.000 min
Response: 65126
Conc: 22.98 ng/ml

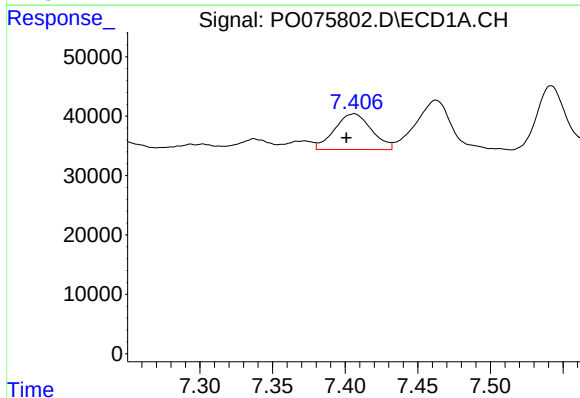


#27 AR-1254-2

R.T.: 7.406 min
Delta R.T.: 0.005 min
Response: 106958
Conc: 29.78 ng/ml

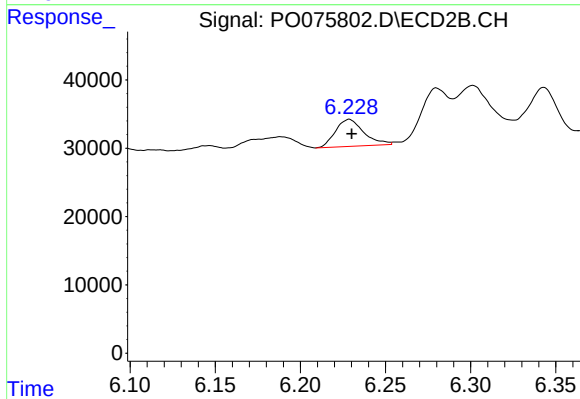

#27 AR-1254-2

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 45843
Conc: 18.51 ng/ml

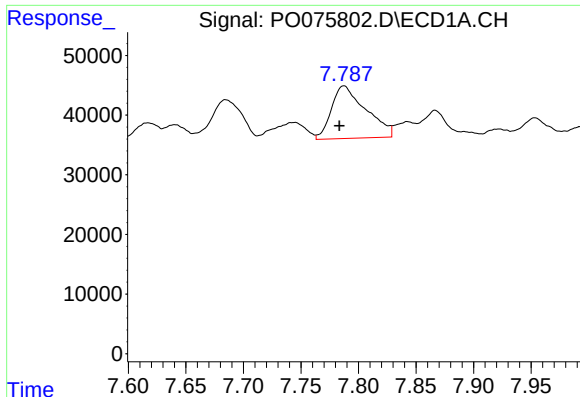


#28 AR-1254-3

R.T.: 7.787 min
Delta R.T.: 0.004 min
Response: 184121
Conc: 48.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
ML-CON


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:12 AM

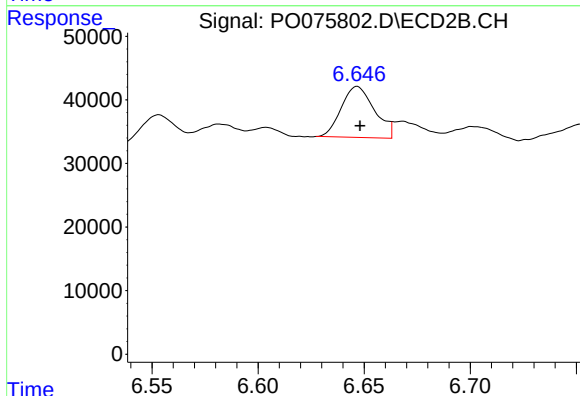


#28 AR-1254-3

R.T.: 6.646 min
Delta R.T.: -0.002 min
Response: 88115
Conc: 21.97 ng/ml m

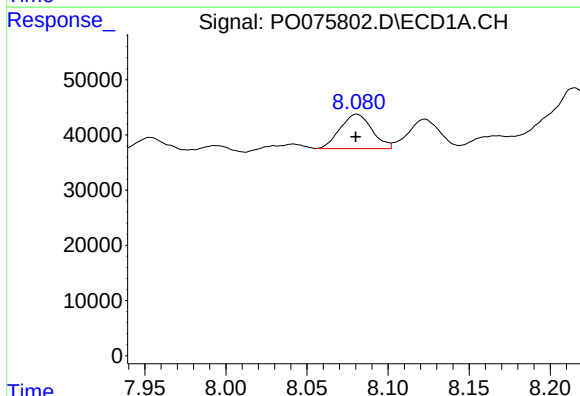


#29 AR-1254-4

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 85189
Conc: 30.70 ng/ml

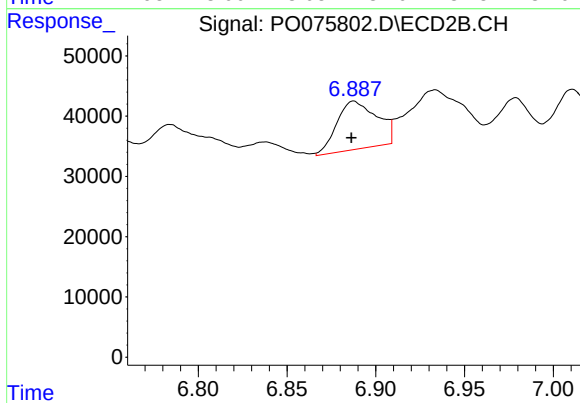

#29 AR-1254-4

R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 126372
Conc: 48.09 ng/ml m

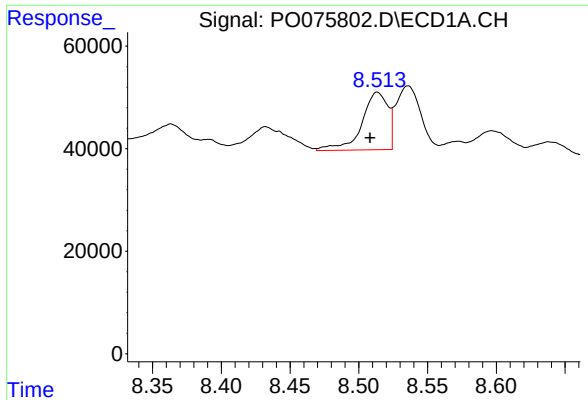


#30 AR-1254-5

R.T.: 8.513 min
Delta R.T.: 0.005 min
Response: 146751
Conc: 52.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ML-CON

Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:12 AM

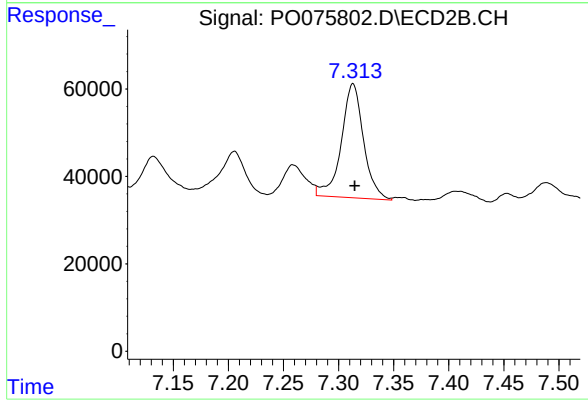

#30 AR-1254-5

R.T.: 7.313 min
Delta R.T.: -0.002 min
Response: 366359
Conc: 104.34 ng/ml m