

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
 Data File : P0075803.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2021 12:25
 Operator : AJ/MA
 Sample : M1508-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-1138

Manual Integrations
 APPROVED

Ankita
 3/3/2021 11:19:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 16:48:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.954	803143	615131	13.139	13.924
2) SA Decachlor...	10.957	9.232	652780	633045	14.346	14.588
Target Compounds						
26) L6 AR-1254-1	7.170	6.082	429175	322750	182.493m	113.897m#
27) L6 AR-1254-2	7.410	6.234	70977	260024	19.763m	104.999m#
28) L6 AR-1254-3	7.788	6.652	292764	296923	77.094m	74.030
29) L6 AR-1254-4	8.084	6.892	278978	262917	100.542	100.049
30) L6 AR-1254-5	8.516	7.320	421370	429733	150.407	122.389

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
Data File : P0075803.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2021 12:25
Operator : AJ/MA
Sample : M1508-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 16:48:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

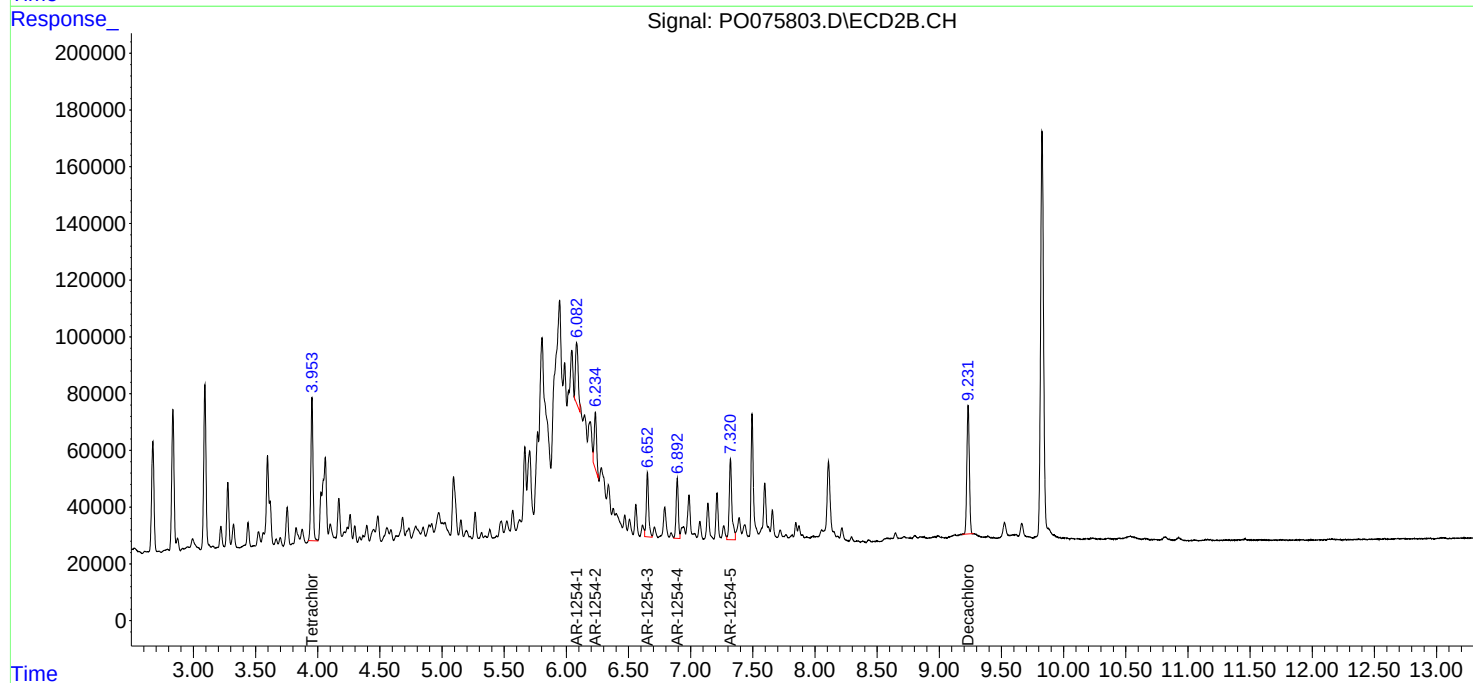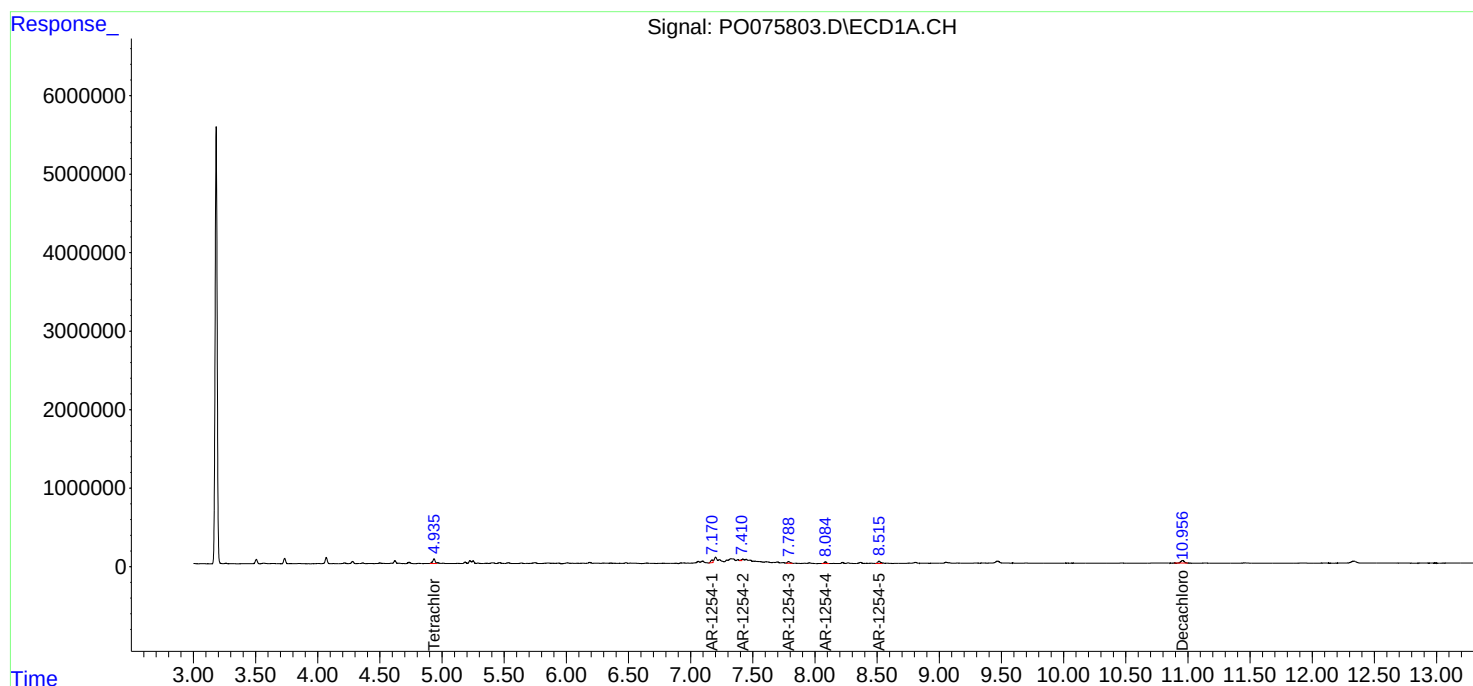

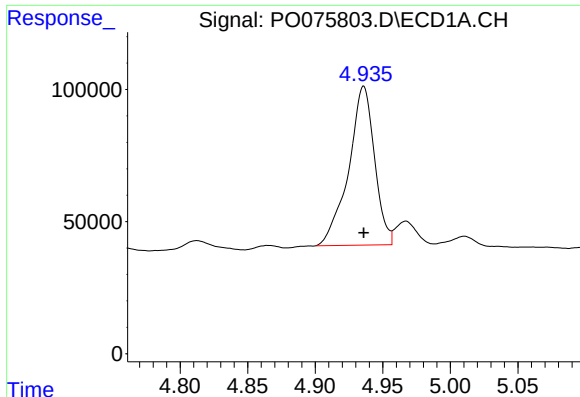


#1 Tetrachloro-m-xylene

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 803143
Conc: 13.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:14 AM

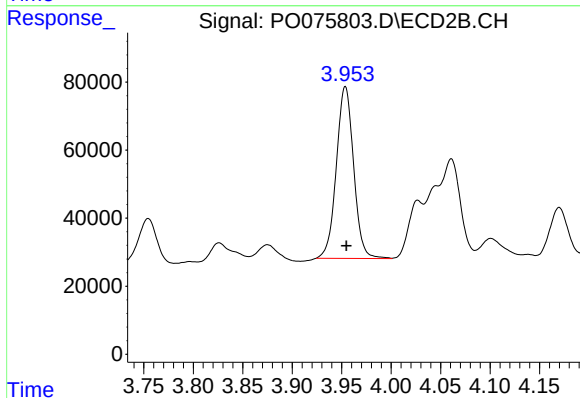


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.001 min
Response: 615131
Conc: 13.92 ng/ml

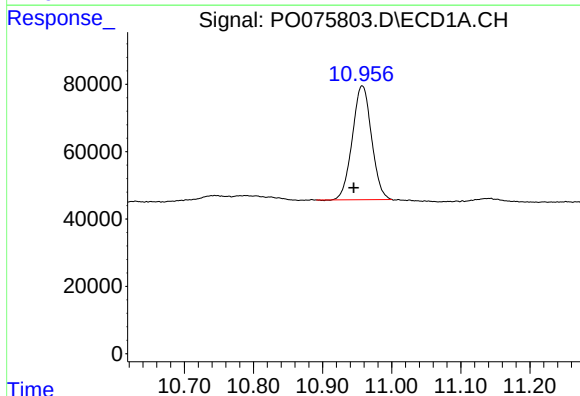


#2 Decachlorobiphenyl

R.T.: 10.957 min
Delta R.T.: 0.012 min
Response: 652780
Conc: 14.35 ng/ml

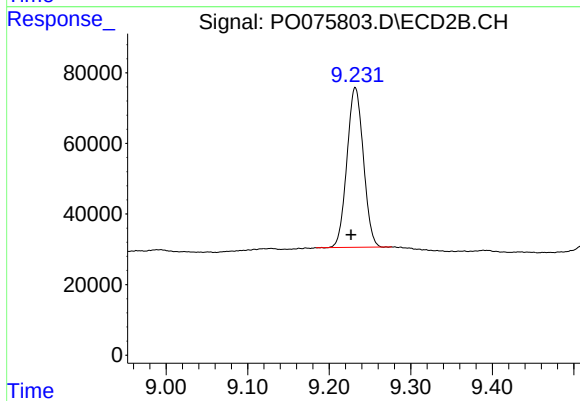

#2 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.005 min
Response: 633045
Conc: 14.59 ng/ml

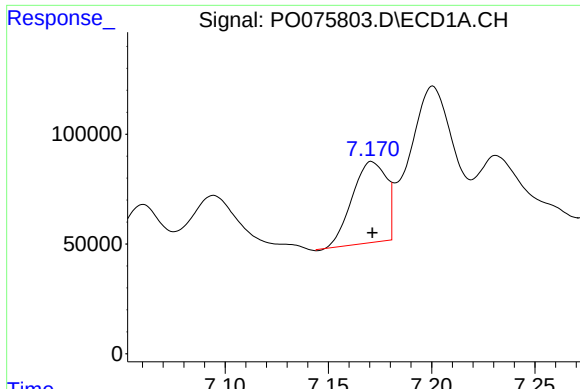


#26 AR-1254-1

R.T.: 7.170 min
Delta R.T.: -0.001 min
Response: 429175
Conc: 182.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:14 AM

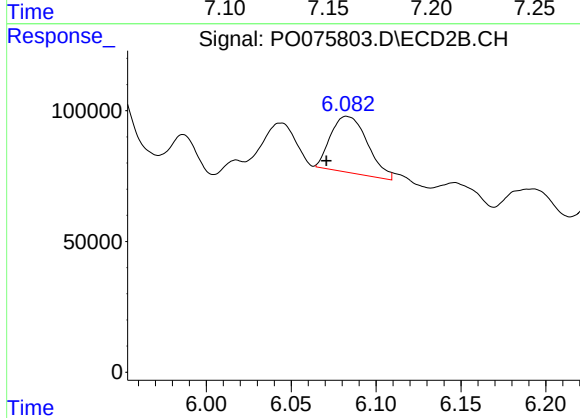


#26 AR-1254-1

R.T.: 6.082 min
Delta R.T.: 0.011 min
Response: 322750
Conc: 113.90 ng/ml m

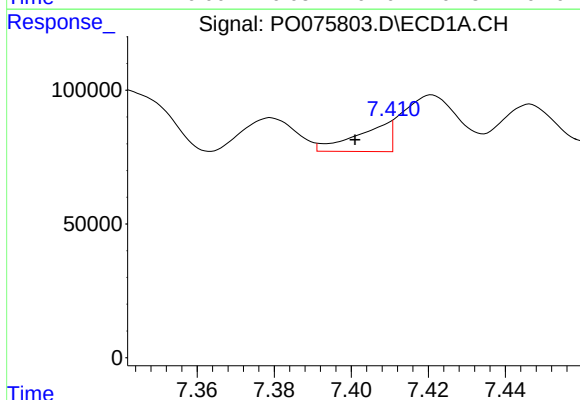


#27 AR-1254-2

R.T.: 7.410 min
Delta R.T.: 0.009 min
Response: 70977
Conc: 19.76 ng/ml m

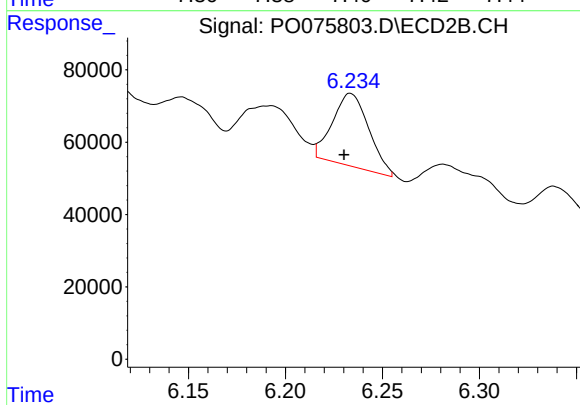

#27 AR-1254-2

R.T.: 6.234 min
Delta R.T.: 0.003 min
Response: 260024
Conc: 105.00 ng/ml m

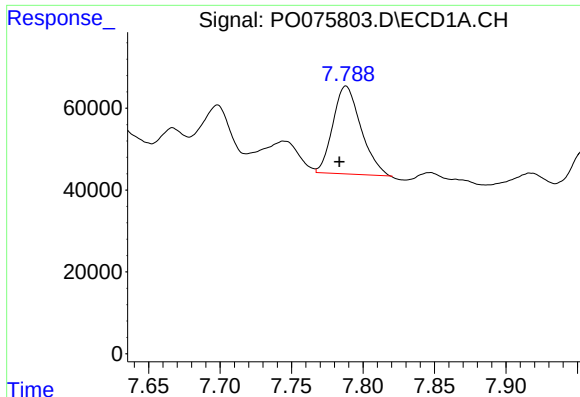


#28 AR-1254-3

R.T.: 7.788 min
Delta R.T.: 0.004 min
Response: 292764
Conc: 77.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TRE-1138


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:14 AM

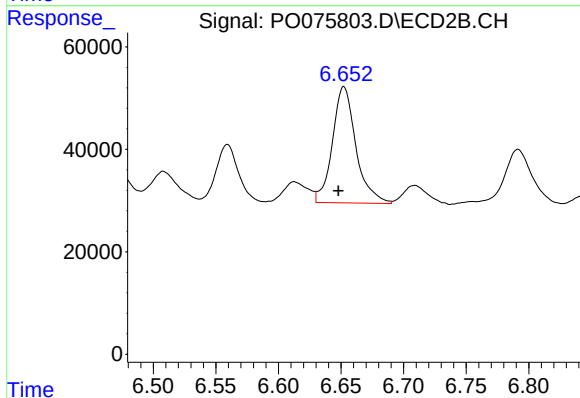


#28 AR-1254-3

R.T.: 6.652 min
Delta R.T.: 0.004 min
Response: 296923
Conc: 74.03 ng/ml

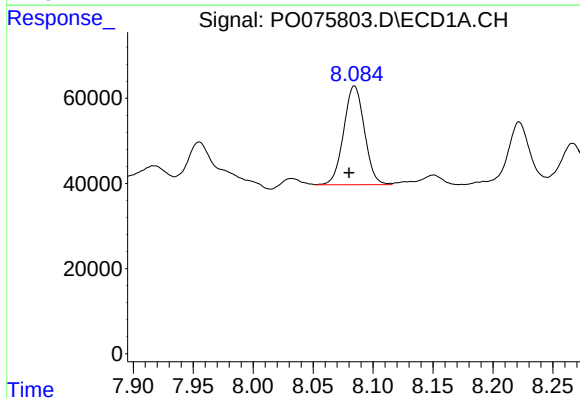


#29 AR-1254-4

R.T.: 8.084 min
Delta R.T.: 0.004 min
Response: 278978
Conc: 100.54 ng/ml

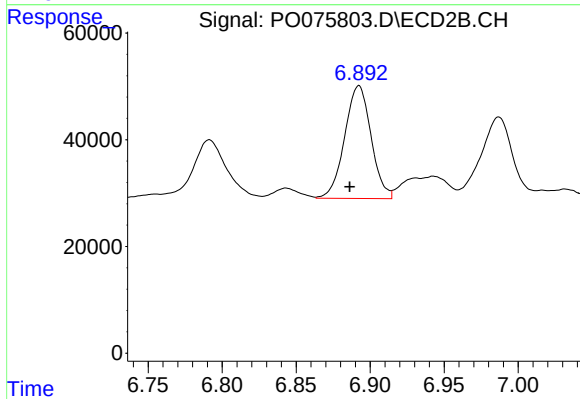

#29 AR-1254-4

R.T.: 6.892 min
Delta R.T.: 0.006 min
Response: 262917
Conc: 100.05 ng/ml

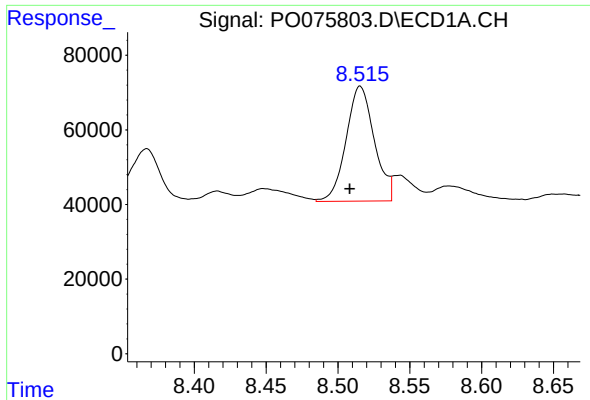


#30 AR-1254-5

R.T.: 8.516 min
Delta R.T.: 0.007 min
Response: 421370
Conc: 150.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1138

Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:14 AM

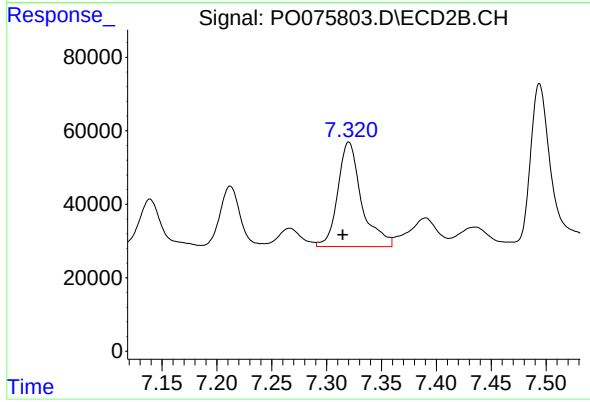

#30 AR-1254-5

R.T.: 7.320 min
Delta R.T.: 0.006 min
Response: 429733
Conc: 122.39 ng/ml