

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
 Data File : P0075807.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2021 13:33
 Operator : AJ/MA
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/3/2021 11:19:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 16:50:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.936	3.952	3364388	2423285	55.039	54.852m
2)	SA Decachlor...	10.949	9.223	2271160	2097167	49.913	48.327
Target Compounds							
21)	L5 AR-1248-1	6.261	5.203	642918	541517	492.918	481.255
22)	L5 AR-1248-2	6.556	5.465	837127	757300	481.008	479.898
23)	L5 AR-1248-3	6.774	5.509	992655	766003	481.851	480.321
24)	L5 AR-1248-4	7.203	5.692	1105618	888162	459.310	515.885
25)	L5 AR-1248-5	7.243	6.113	1082688	910518	469.556	473.294

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030221\
Data File : PO075807.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2021 13:33
Operator : AJ/MA
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 16:50:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

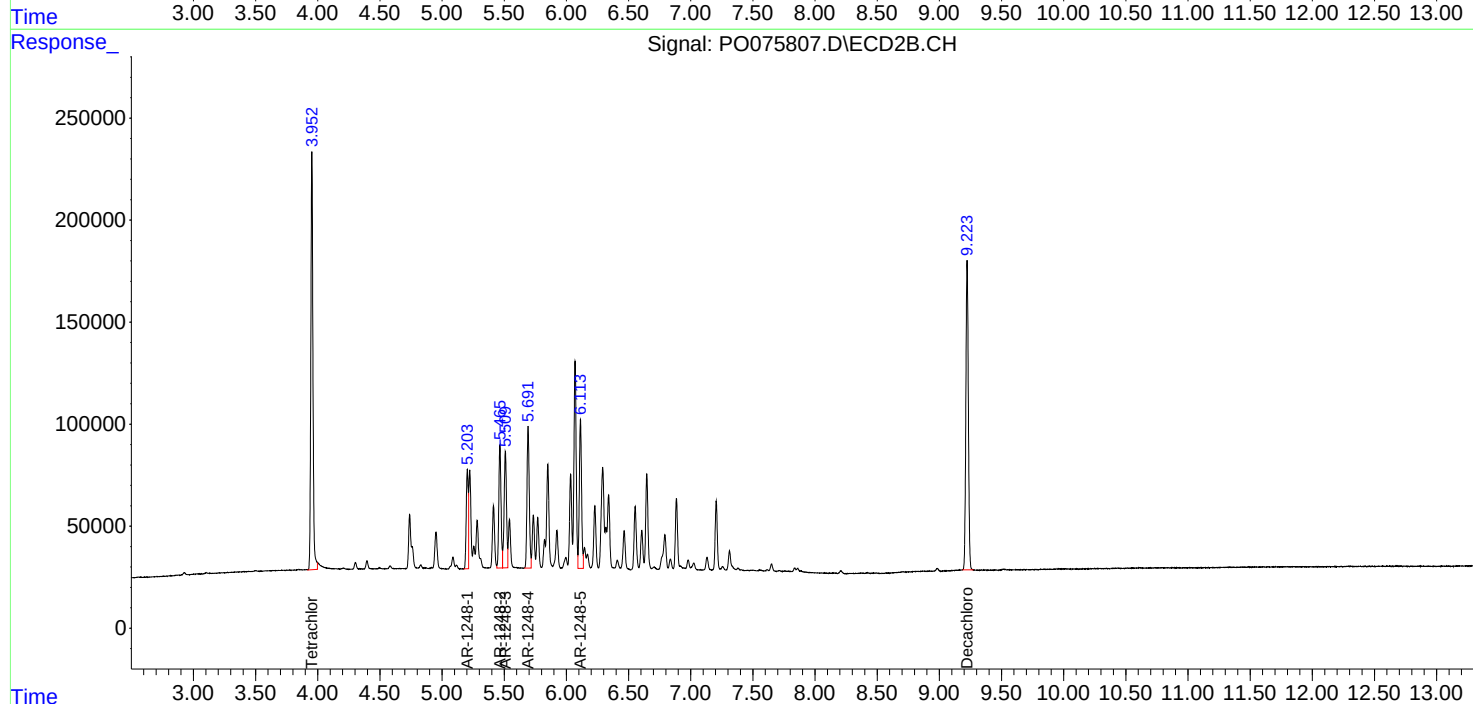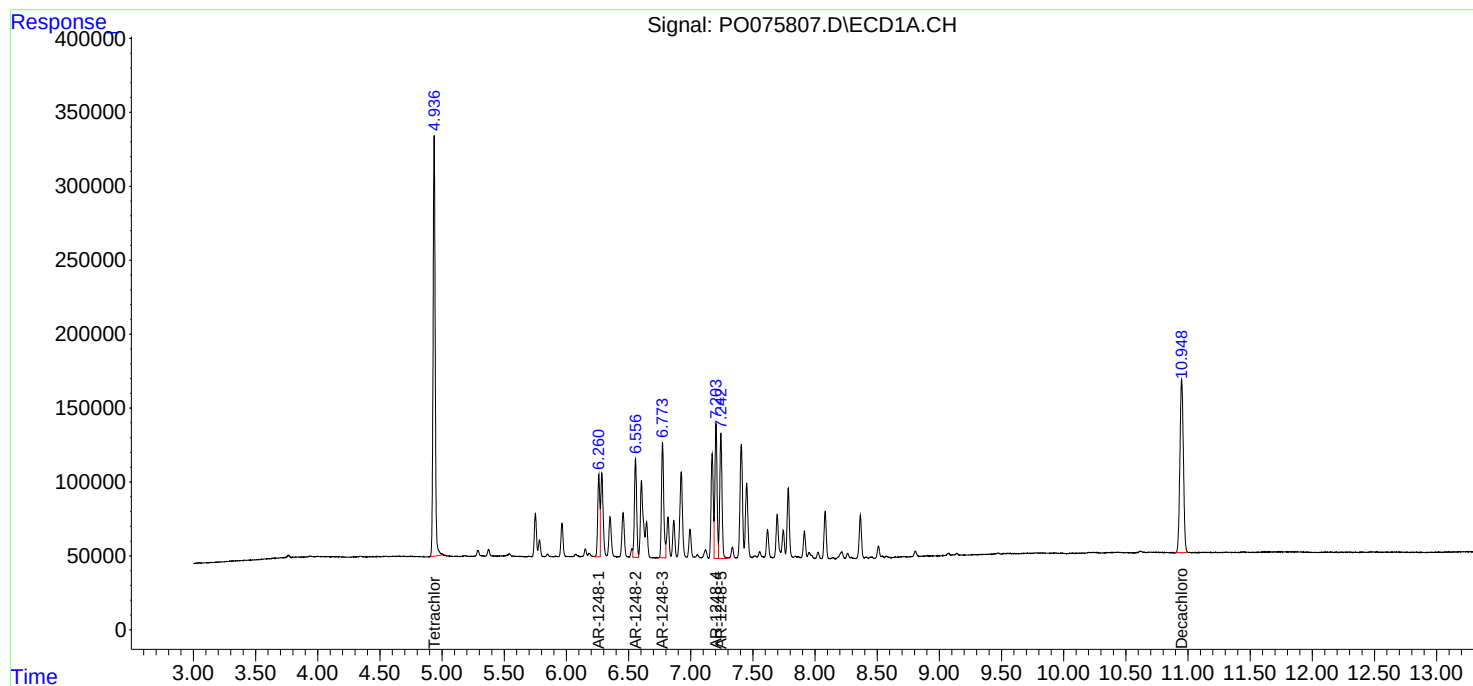

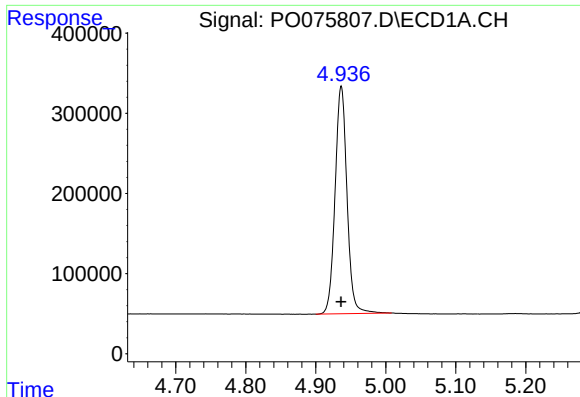


#1 Tetrachloro-m-xylene

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 3364388
Conc: 55.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:17 AM

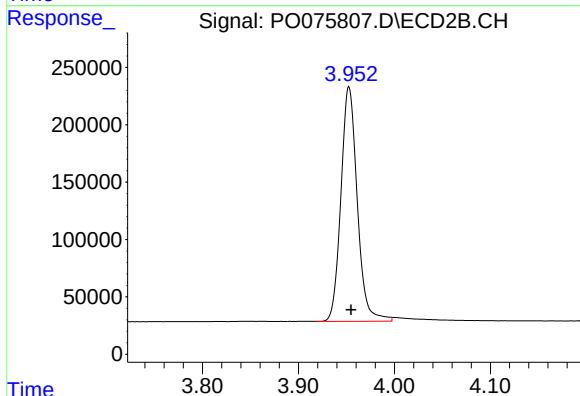


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: -0.003 min
Response: 2423285
Conc: 54.85 ng/ml m

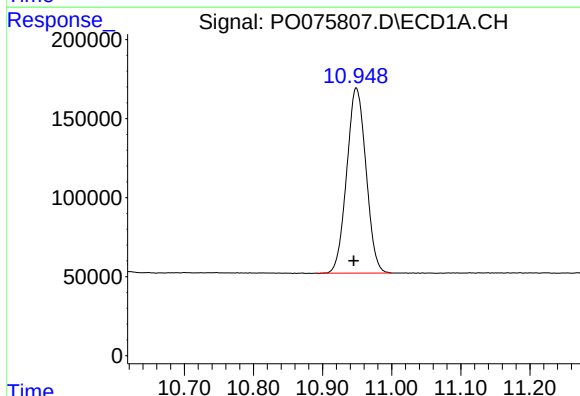


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.003 min
Response: 2271160
Conc: 49.91 ng/ml

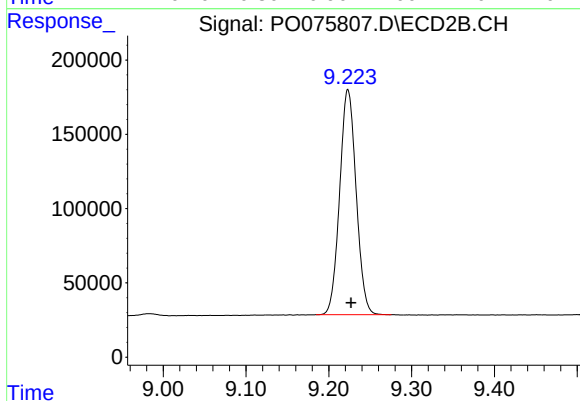

#2 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 2097167
Conc: 48.33 ng/ml

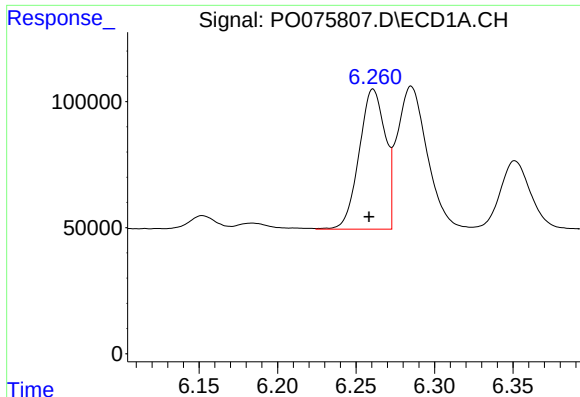


#21 AR-1248-1

R.T.: 6.261 min
Delta R.T.: 0.003 min
Response: 642918
Conc: 492.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:17 AM

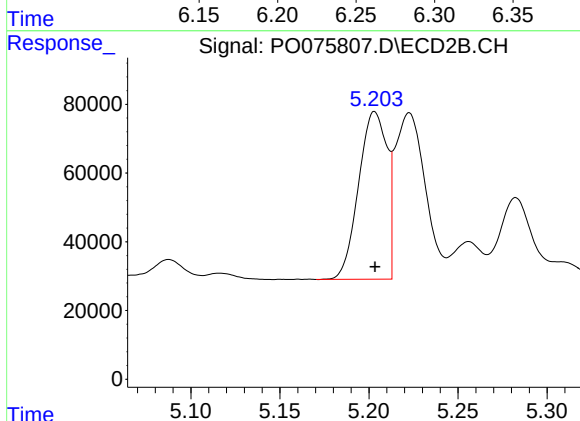


#21 AR-1248-1

R.T.: 5.203 min
Delta R.T.: 0.000 min
Response: 541517
Conc: 481.25 ng/ml

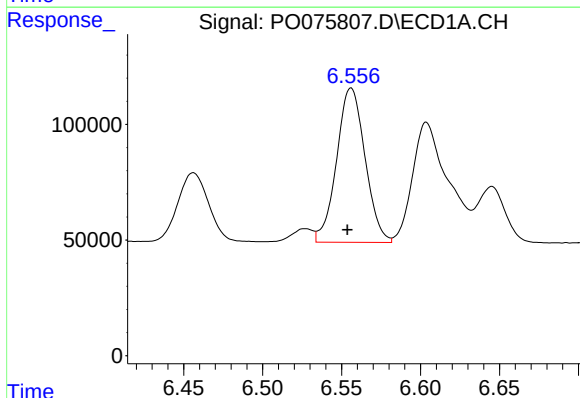


#22 AR-1248-2

R.T.: 6.556 min
Delta R.T.: 0.002 min
Response: 837127
Conc: 481.01 ng/ml

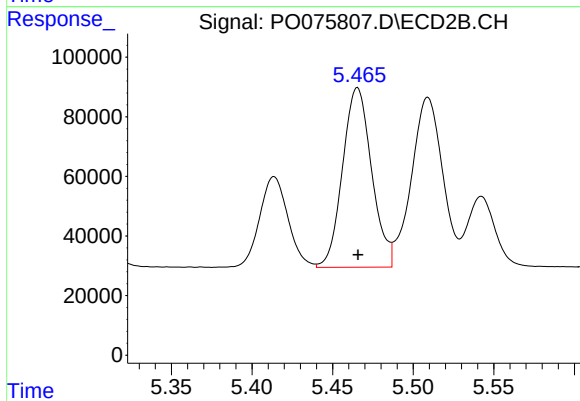

#22 AR-1248-2

R.T.: 5.465 min
Delta R.T.: 0.000 min
Response: 757300
Conc: 479.90 ng/ml

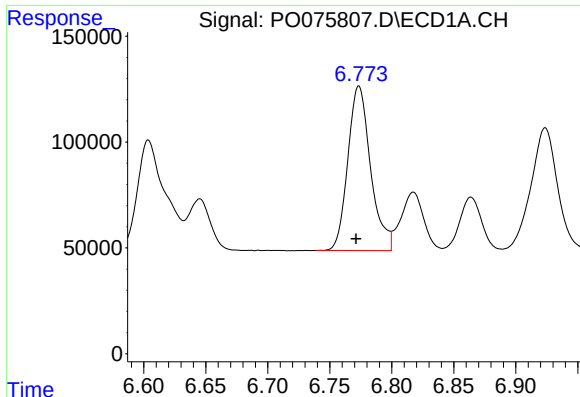


#23 AR-1248-3

R.T.: 6.774 min
Delta R.T.: 0.002 min
Response: 992655
Conc: 481.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:17 AM

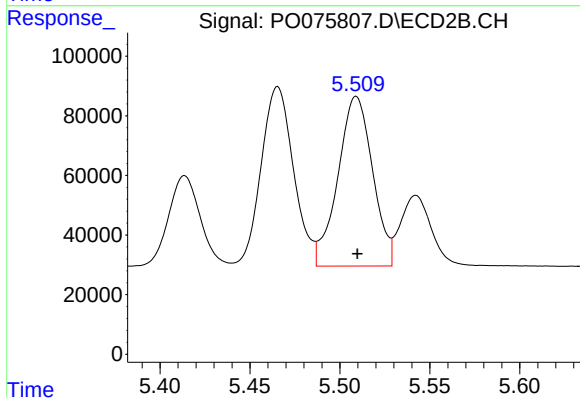


#23 AR-1248-3

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 766003
Conc: 480.32 ng/ml

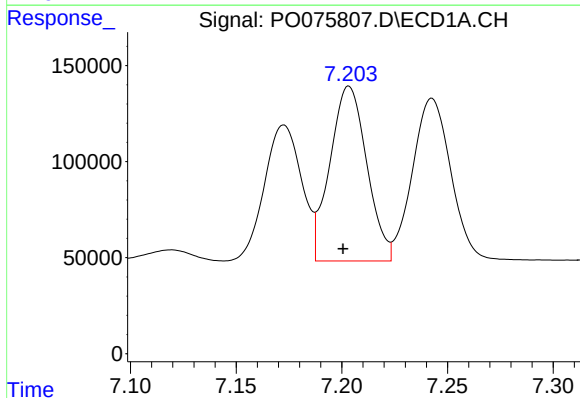


#24 AR-1248-4

R.T.: 7.203 min
Delta R.T.: 0.003 min
Response: 1105618
Conc: 459.31 ng/ml

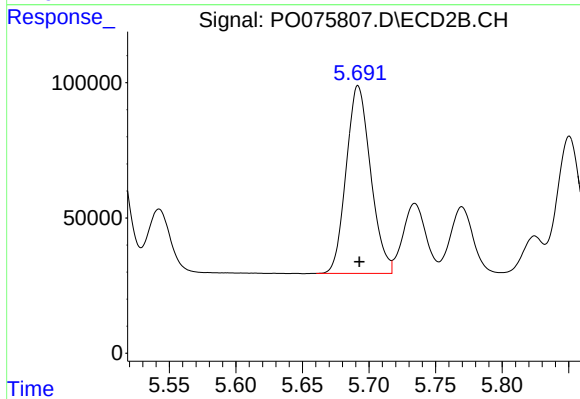

#24 AR-1248-4

R.T.: 5.692 min
Delta R.T.: 0.000 min
Response: 888162
Conc: 515.89 ng/ml

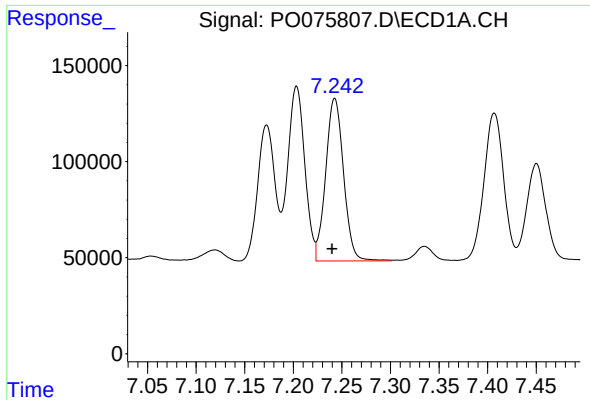


#25 AR-1248-5

R.T.: 7.243 min
Delta R.T.: 0.003 min
Response: 1082688
Conc: 469.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:17 AM

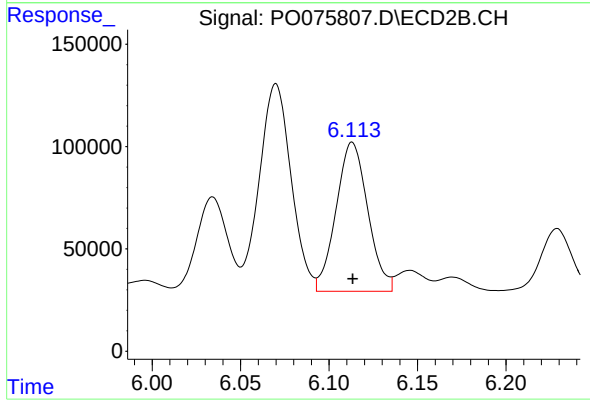

#25 AR-1248-5

R.T.: 6.113 min
Delta R.T.: 0.000 min
Response: 910518
Conc: 473.29 ng/ml