

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
 Data File : P0075812.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2021 16:00
 Operator : AJ/MA
 Sample : M1530-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF265P-1-1

Manual Integrations
 APPROVED

Ankita
 3/3/2021 11:19:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 16:52:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 27 03:46:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.953	104841	89818	1.715	2.033m
2) SA Decachlor...	10.954	9.223	69908	87334	1.536	2.013m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030221\
Data File : P0075812.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2021 16:00
Operator : AJ/MA
Sample : M1530-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HEF265P-1-1


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 16:52:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022621.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 27 03:46:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

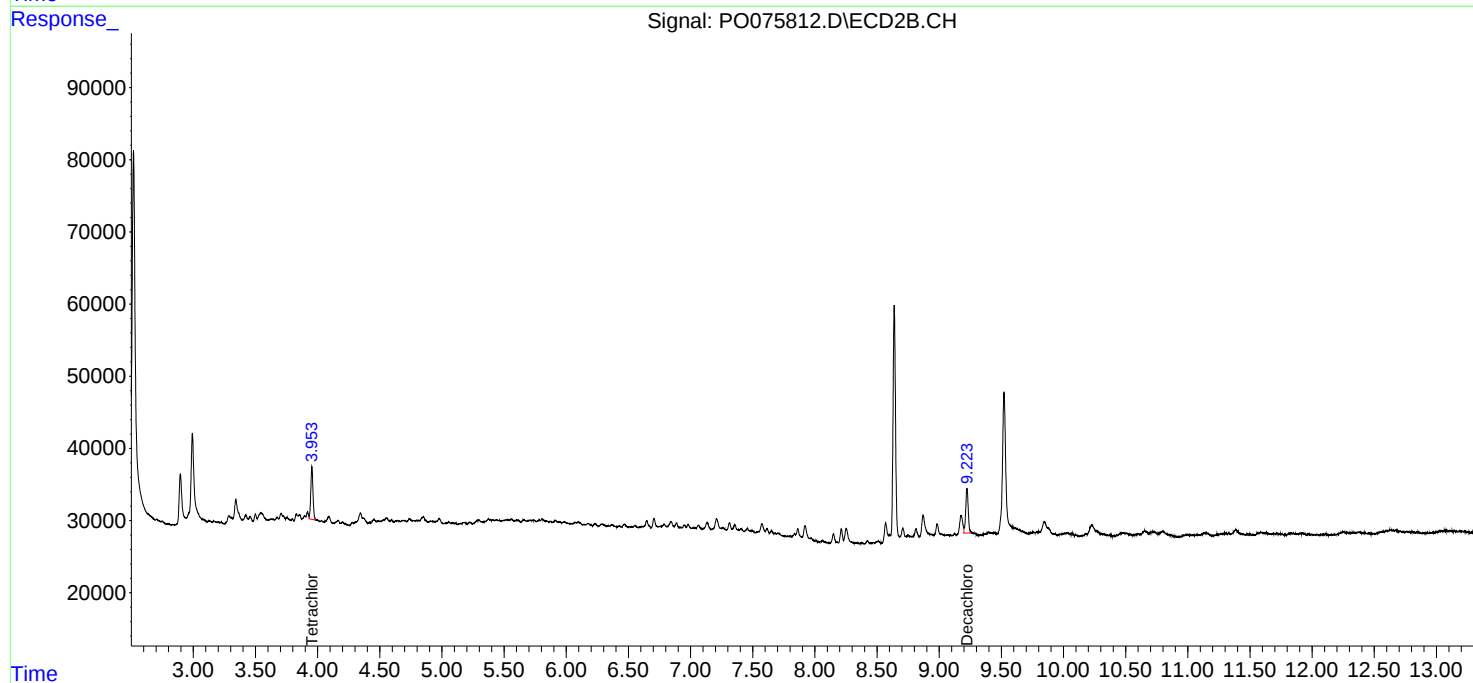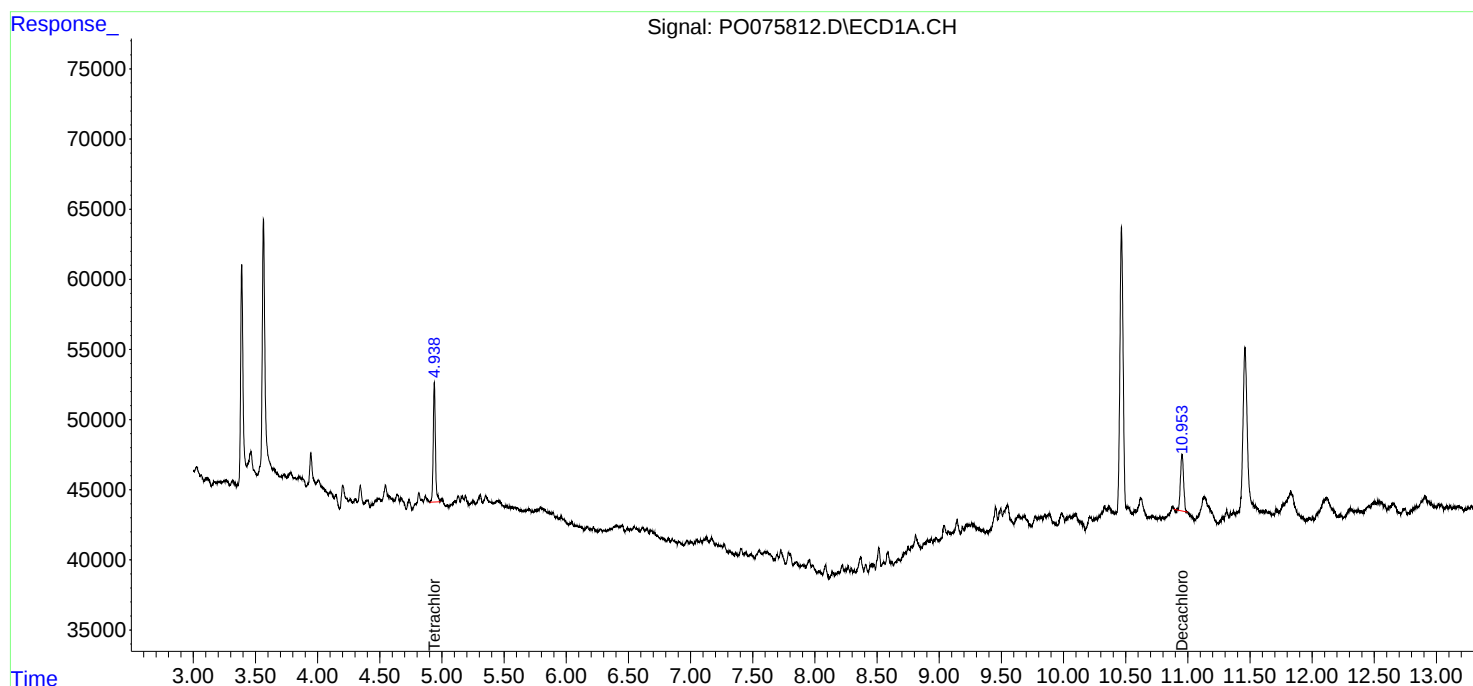

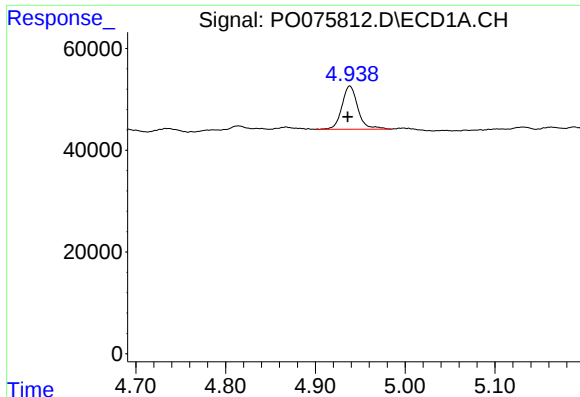


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: 0.002 min
Response: 104841
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF265P-1-1


Manual Integrations
APPROVED

Ankita
3/3/2021 11:19:19 AM

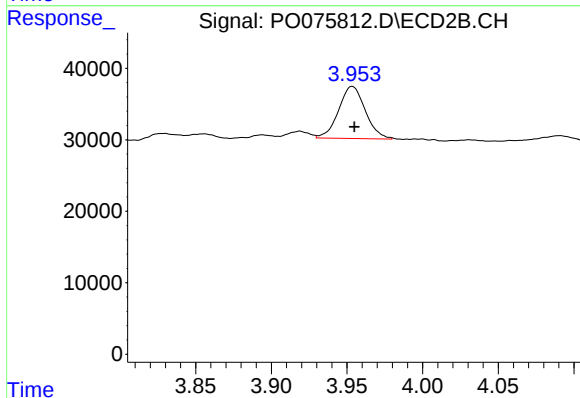


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.002 min
Response: 89818
Conc: 2.03 ng/ml m

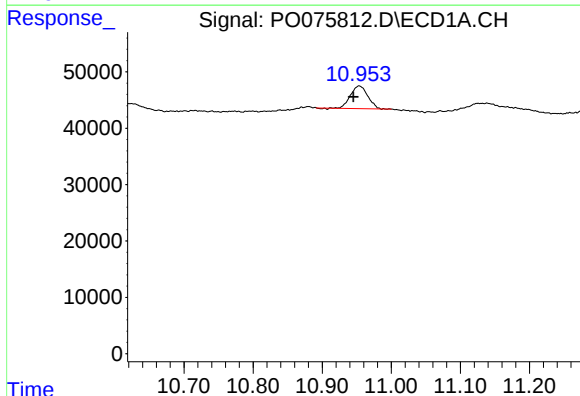

#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: 0.008 min
Response: 69908
Conc: 1.54 ng/ml

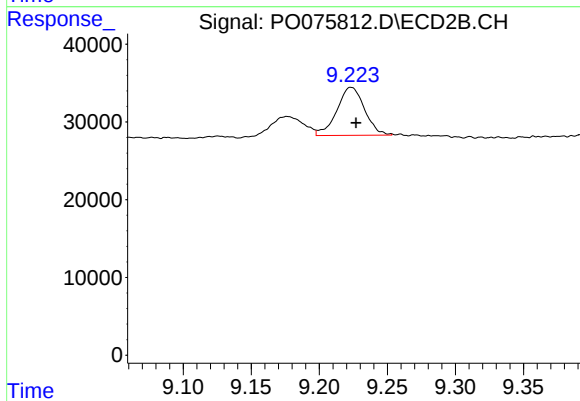

#2 Decachlorobiphenyl

R.T.: 9.223 min
Delta R.T.: -0.004 min
Response: 87334
Conc: 2.01 ng/ml m