

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0030222\
 Data File : P0084983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2022 10:22
 Operator : YP\AJ
 Sample : N1715-02 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 IRV-2022-67B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:53:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.509	3.595	362323	78212	1.296	1.739 #
2)	SA Decachlor...	10.432	8.622	289589	53390	1.652	1.453
Target Compounds							
3)	L1 AR-1016-1	5.681	0.000	15000	0	1.602	N.D. #
4)	L1 AR-1016-2	5.716	0.000	6780	0	0.508	N.D. #
5)	L1 AR-1016-3	5.803	0.000	4993	0	0.625	N.D. #
6)	L1 AR-1016-4	5.886	0.000	18656	0	2.777	N.D. #
7)	L1 AR-1016-5	6.156	5.162	21508	26117	3.402	19.707 #
8)	L2 AR-1221-1	4.722	3.757f	3850	28024	1.203	48.061 #
9)	L2 AR-1221-2	4.820	0.000	12566	0	5.212	N.D. #
10)	L2 AR-1221-3	4.883	0.000	13891	0	1.908	N.D. #
11)	L3 AR-1232-1	4.883	0.000	13891	0	2.270	N.D. #
12)	L3 AR-1232-2	5.425	0.000	936	0	0.315	N.D. #
13)	L3 AR-1232-3	5.716	0.000	6780	0	1.196	N.D. #
14)	L3 AR-1232-4	5.886	0.000	18656	0	6.532	N.D. #
15)	L3 AR-1232-5	5.984	5.162	3182	26117	1.409	47.096 #
16)	L4 AR-1242-1	5.681	0.000	15000	0	2.021	N.D. #
17)	L4 AR-1242-2	5.723	0.000	3173	0	0.299	N.D. #
18)	L4 AR-1242-3	5.803	0.000	4993	0	0.777	N.D. #
19)	L4 AR-1242-4	5.886	0.000	18656	0	3.441	N.D. #
20)	L4 AR-1242-5	6.651	5.515	153899	660115	29.261	532.629 #
21)	L5 AR-1248-1	5.681	0.000	15000	0	2.765	N.D. #
22)	L5 AR-1248-2	5.984	0.000	3182	0	0.414	N.D. #
23)	L5 AR-1248-3	6.156	0.000	21508	0	2.503	N.D. #
24)	L5 AR-1248-4	6.604	5.162	139906	26117	15.016	15.035
25)	L5 AR-1248-5	6.651	5.515	153899	660115	17.213	393.613 #
26)	L6 AR-1254-1	6.567	5.515	3403118	660115	346.959	246.753 #
27)	L6 AR-1254-2	6.785	0.000	31936	0	2.152	N.D. #
28)	L6 AR-1254-3	7.162	0.000	605845	0	40.013	N.D. #
29)	L6 AR-1254-4	7.443	6.343f	107695	66130	10.041	28.214 #
30)	L6 AR-1254-5	7.878	6.692	225793	6114	19.175	1.807 #
31)	L7 AR-1260-1	7.354	6.169	784780	5890	68.773	2.373 #
32)	L7 AR-1260-2	7.623f	6.343	1143234	66130	88.909	22.342 #
33)	L7 AR-1260-3	7.952	6.544	190800	6280	23.892	2.296 #
34)	L7 AR-1260-4	8.179	0.000	120123	0	12.629	N.D. #
35)	L7 AR-1260-5	8.544	0.000	16028	0	0.872	N.D. #
36)	L8 AR-1262-1	7.952	6.692	190800	6114	21.107	5.066 #
37)	L8 AR-1262-2	8.544	0.000	16028	0	1.005	N.D. #
38)	L8 AR-1262-3	8.823	7.532	48503	1238892	4.626	796.985 #
39)	L8 AR-1262-4	8.939	7.532f	17279	1238892	3.419	437.285 #
40)	L8 AR-1262-5	9.561f	0.000	32529	0	5.948	N.D. #
41)	L9 AR-1268-1	8.823	7.532	48503	1238892	1.736	181.609 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0084983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2022 10:22
 Operator : YP\AJ
 Sample : N1715-02 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-67B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:53:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.939	7.532f	17279	1238892	0.690	204.412 #
43) L9	AR-1268-3	9.205	7.743f	30433	302	1.425	0.060 #
44) L9	AR-1268-4	9.561f	0.000	32529	0	3.544	N.D. #
45) L9	AR-1268-5	10.060	0.000	3267	0	0.047	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
Data File : P0084983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2022 10:22
Operator : YP\AJ
Sample : N1715-02 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:53:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

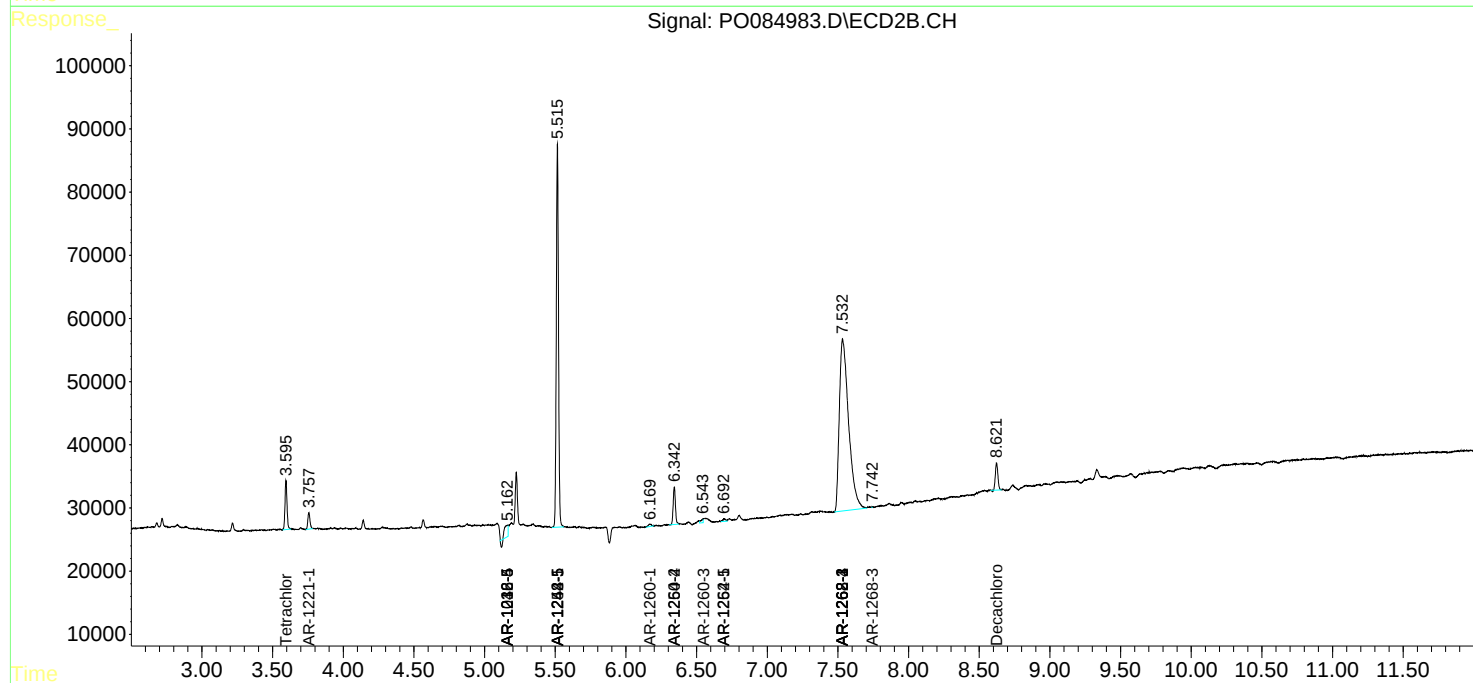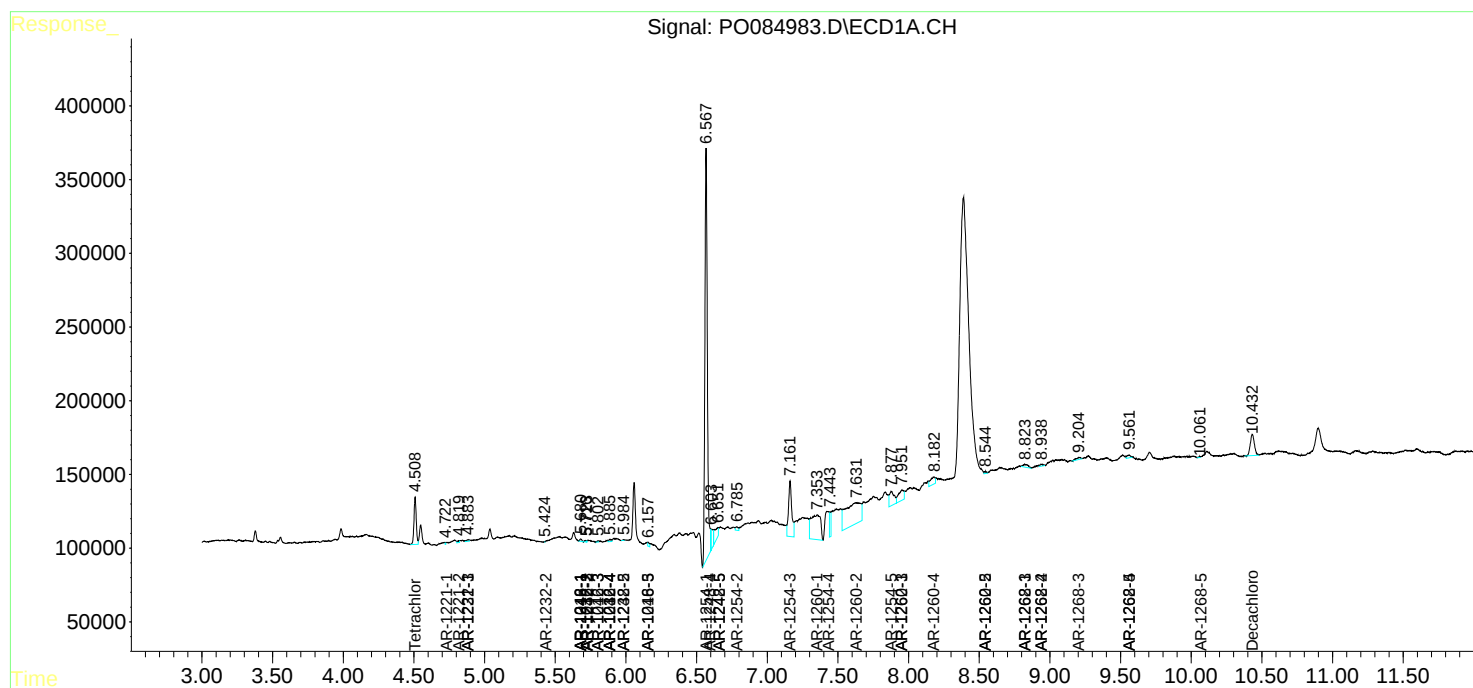


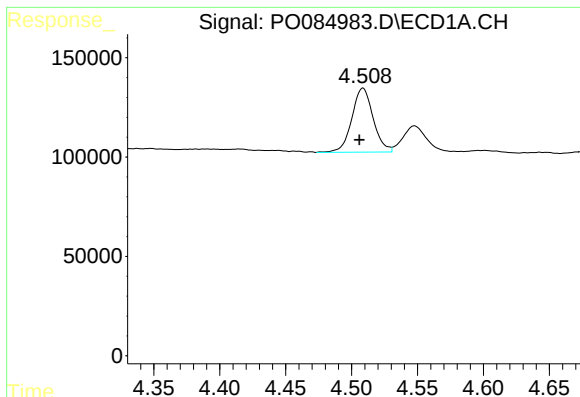

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 362323
Conc: 1.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

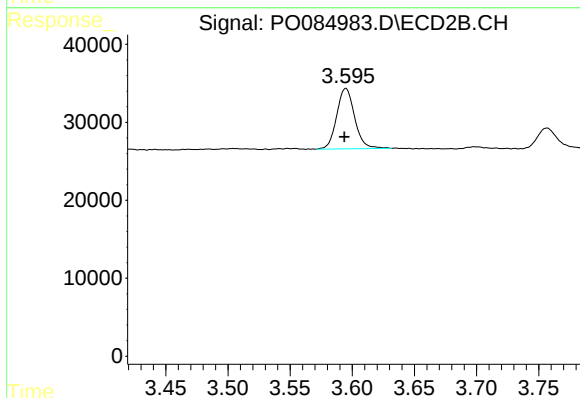


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.001 min
Response: 78212
Conc: 1.74 ng/ml

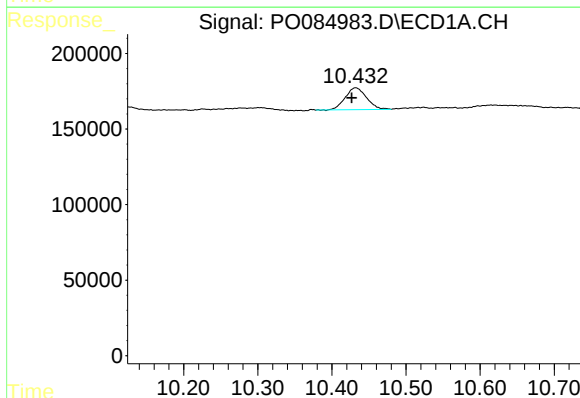


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.005 min
Response: 289589
Conc: 1.65 ng/ml

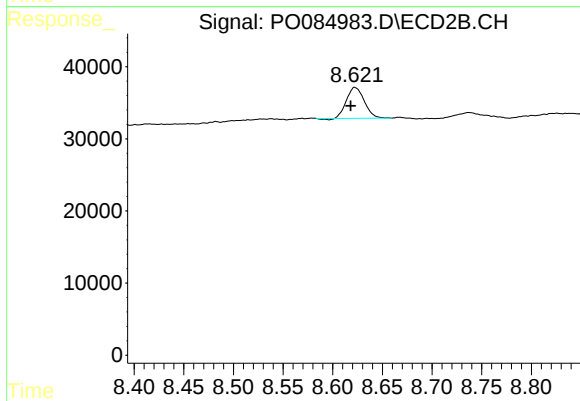

#2 Decachlorobiphenyl


R.T.: 8.622 min
Delta R.T.: 0.004 min
Response: 53390
Conc: 1.45 ng/ml

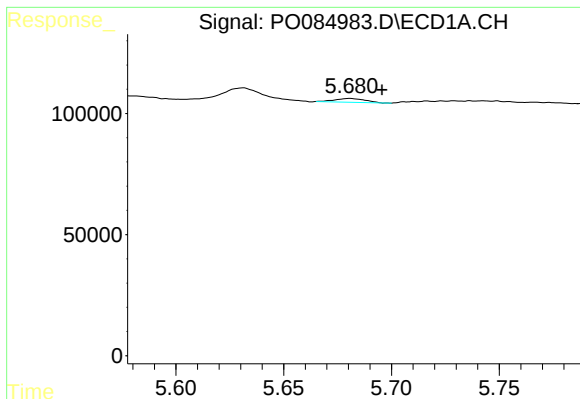

#3 AR-1016-1


R.T.: 5.681 min
Delta R.T.: -0.015 min
Response: 15000
Conc: 1.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

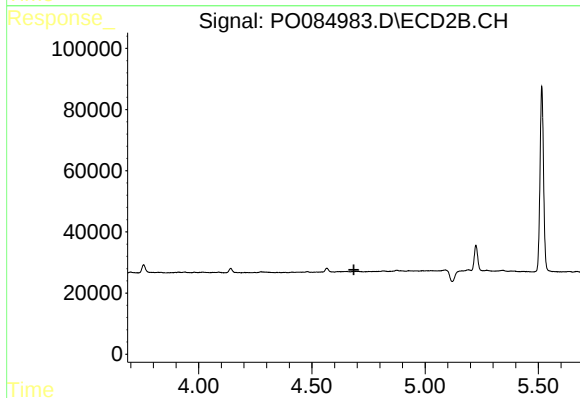


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

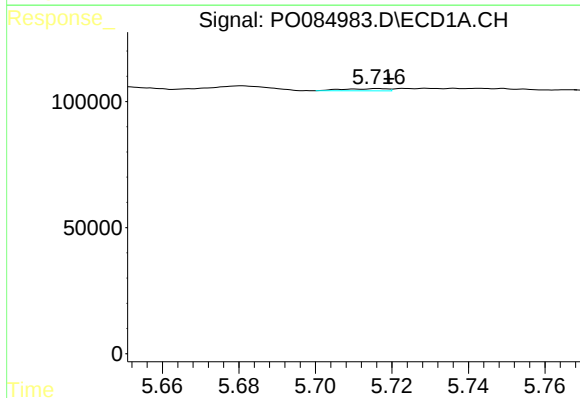


#4 AR-1016-2

R.T.: 5.716 min
Delta R.T.: -0.003 min
Response: 6780
Conc: 0.51 ng/ml

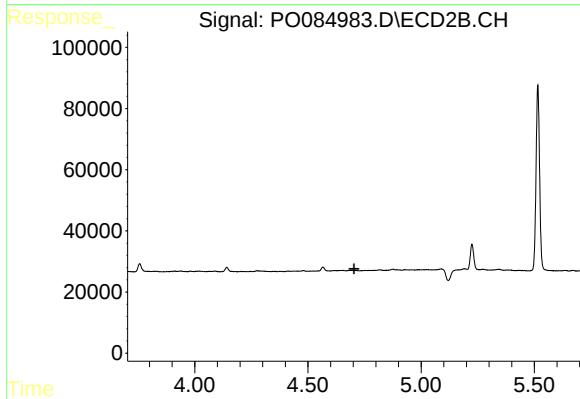

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

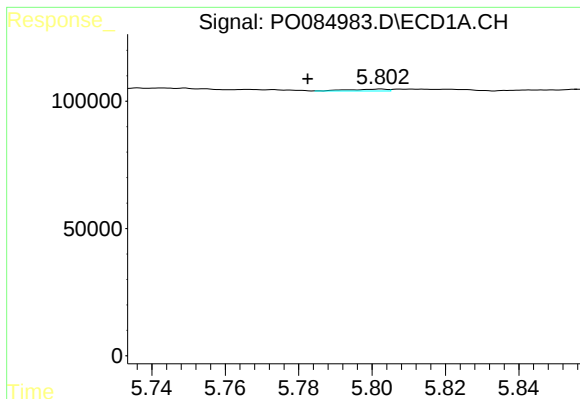

#5 AR-1016-3


R.T.: 5.803 min
Delta R.T.: 0.020 min
Response: 4993
Conc: 0.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

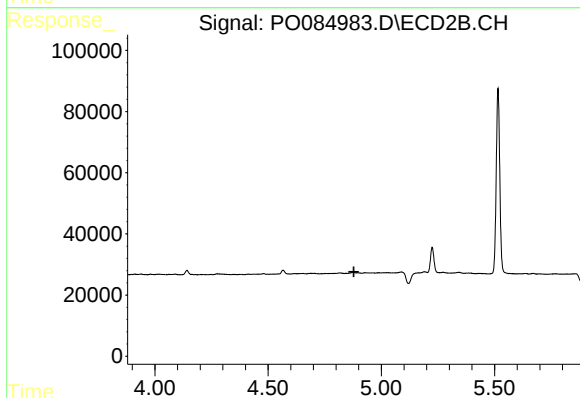


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.879 min
Response: 0
Conc: N.D.

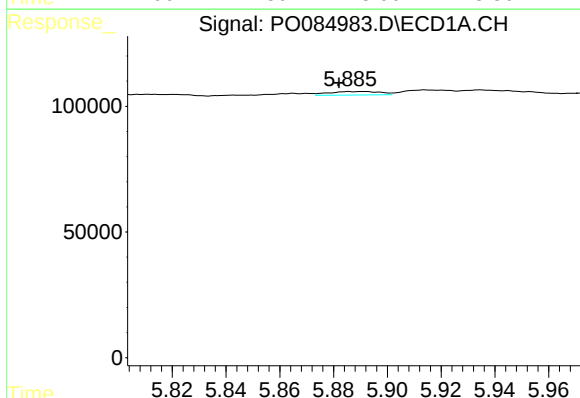


#6 AR-1016-4

R.T.: 5.886 min
Delta R.T.: 0.004 min
Response: 18656
Conc: 2.78 ng/ml

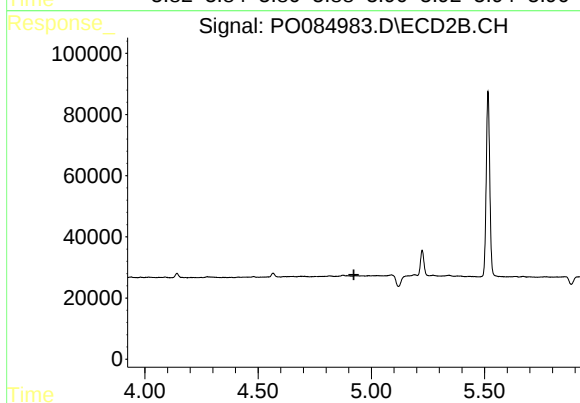

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.923 min
Response: 0
Conc: N.D.

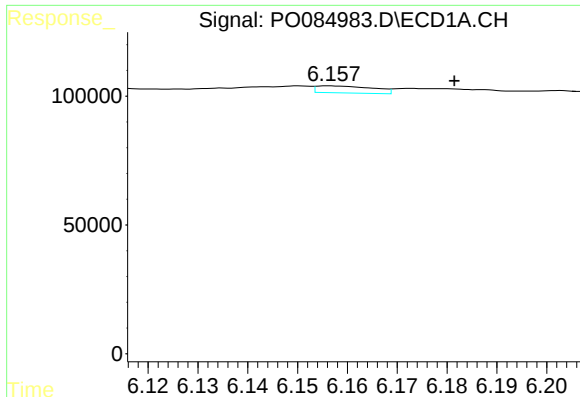

#7 AR-1016-5


R.T.: 6.156 min
Delta R.T.: -0.025 min
Response: 21508
Conc: 3.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

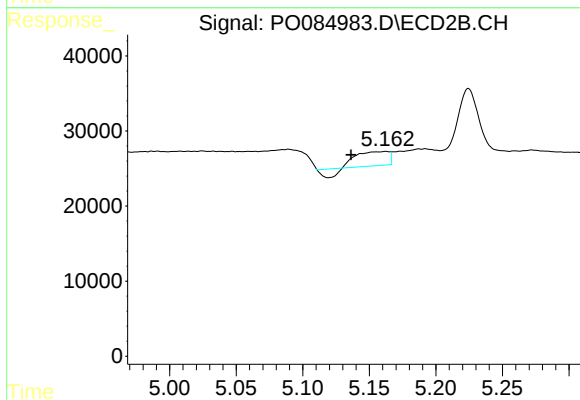


#7 AR-1016-5

R.T.: 5.162 min
Delta R.T.: 0.026 min
Response: 26117
Conc: 19.71 ng/ml

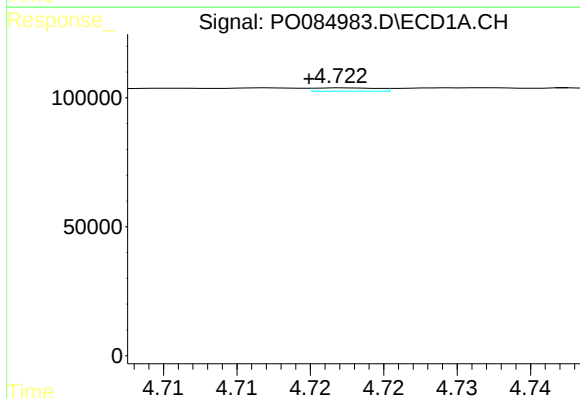


#8 AR-1221-1

R.T.: 4.722 min
Delta R.T.: 0.002 min
Response: 3850
Conc: 1.20 ng/ml

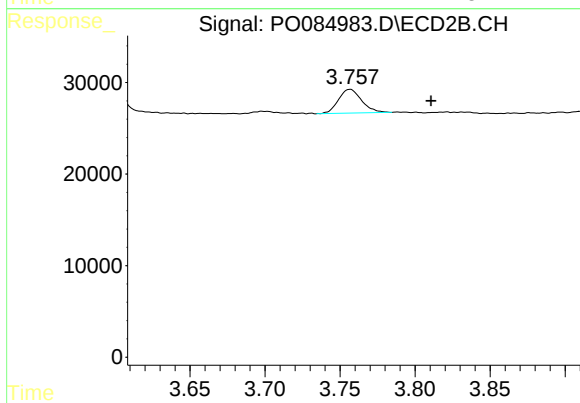

#8 AR-1221-1


R.T.: 3.757 min
Delta R.T.: -0.054 min
Response: 28024
Conc: 48.06 ng/ml

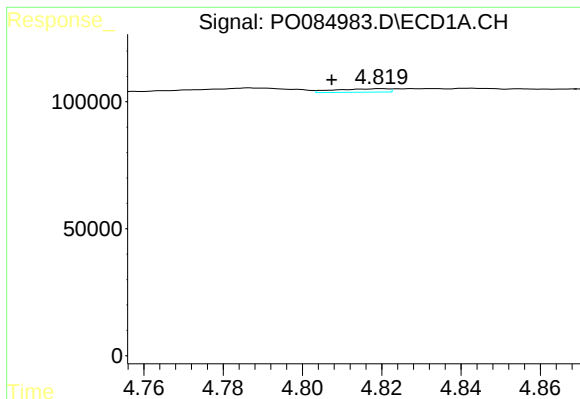

#9 AR-1221-2


R.T.: 4.820 min
Delta R.T.: 0.012 min
Response: 12566
Conc: 5.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

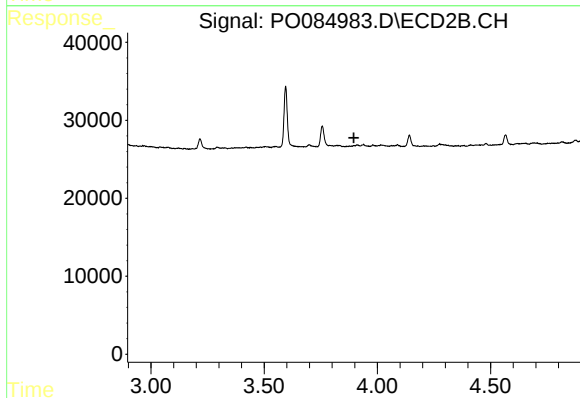


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

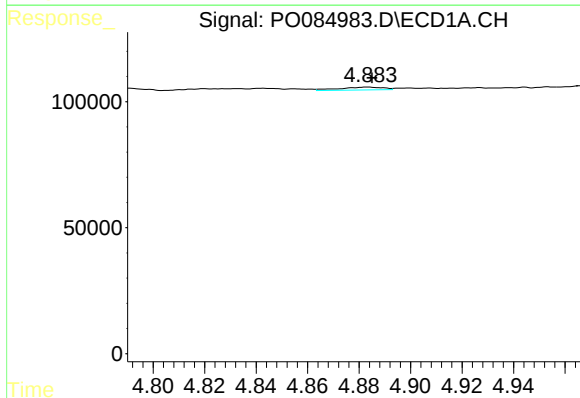


#10 AR-1221-3

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 13891
Conc: 1.91 ng/ml

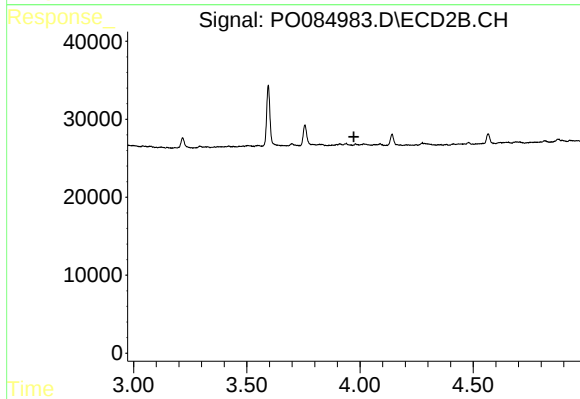

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.973 min
Response: 0
Conc: N.D.

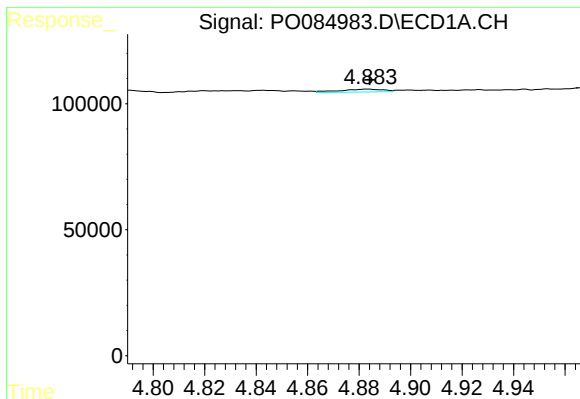

#11 AR-1232-1


R.T.: 4.883 min
Delta R.T.: 0.000 min
Response: 13891
Conc: 2.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

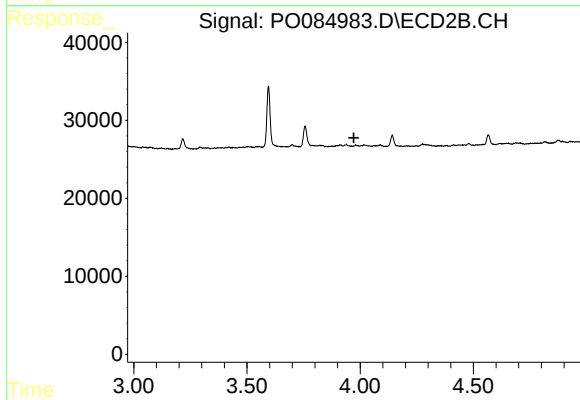


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

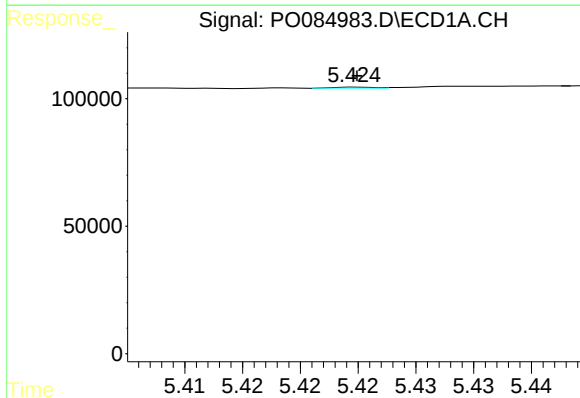


#12 AR-1232-2

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 936
Conc: 0.31 ng/ml

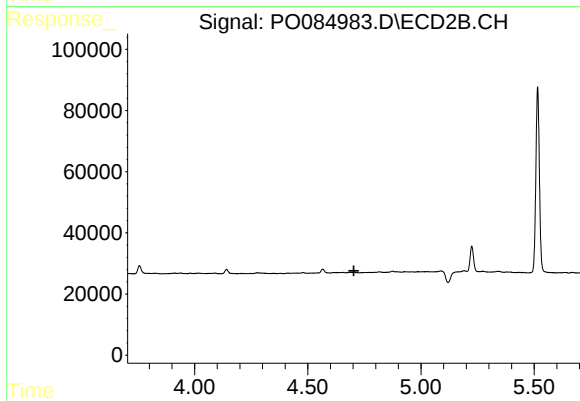

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

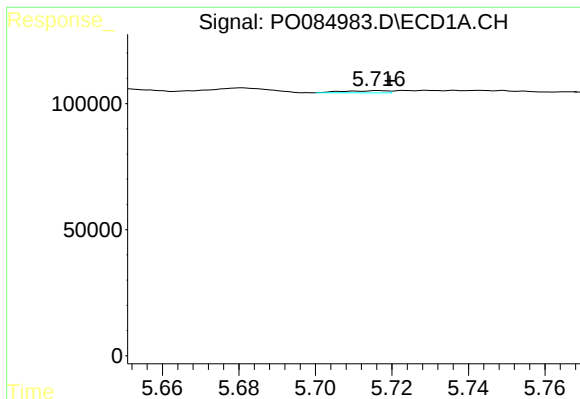

#13 AR-1232-3


R.T.: 5.716 min
Delta R.T.: -0.003 min
Response: 6780
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

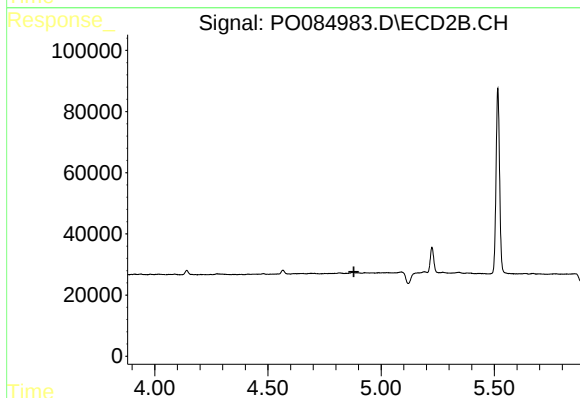


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.879 min
Response: 0
Conc: N.D.

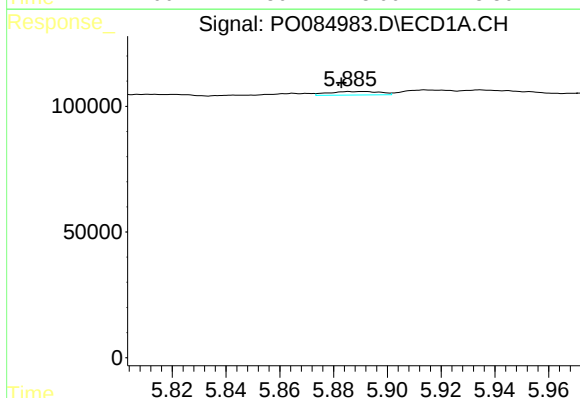


#14 AR-1232-4

R.T.: 5.886 min
Delta R.T.: 0.003 min
Response: 18656
Conc: 6.53 ng/ml

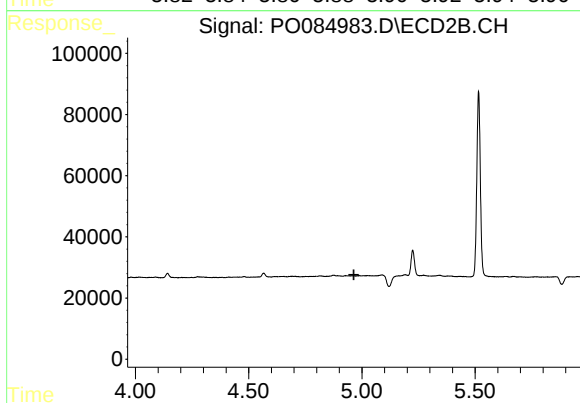

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.964 min
Response: 0
Conc: N.D.

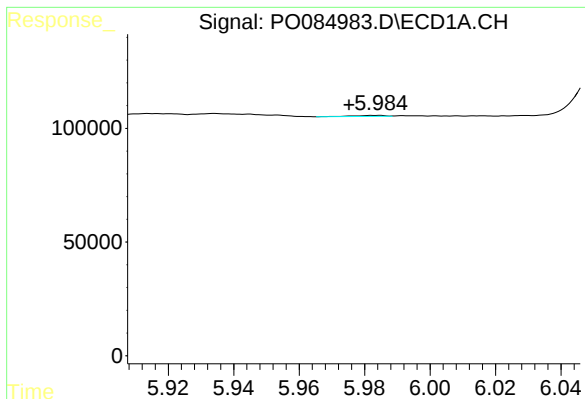

#15 AR-1232-5


R.T.: 5.984 min
Delta R.T.: 0.009 min
Response: 3182
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

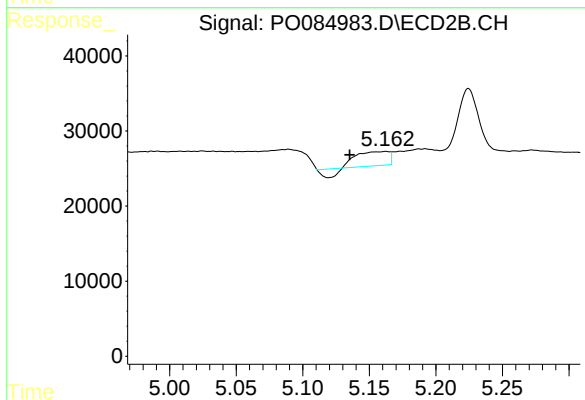


#15 AR-1232-5

R.T.: 5.162 min
Delta R.T.: 0.027 min
Response: 26117
Conc: 47.10 ng/ml

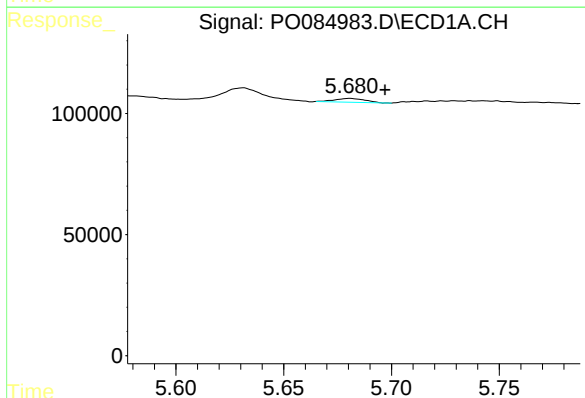


#16 AR-1242-1

R.T.: 5.681 min
Delta R.T.: -0.016 min
Response: 15000
Conc: 2.02 ng/ml

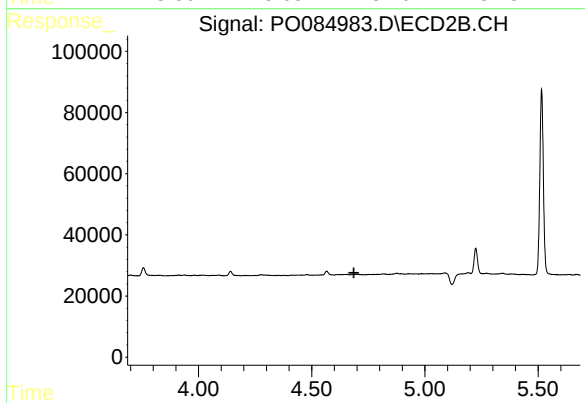

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 4.686 min
Response: 0
Conc: N.D.

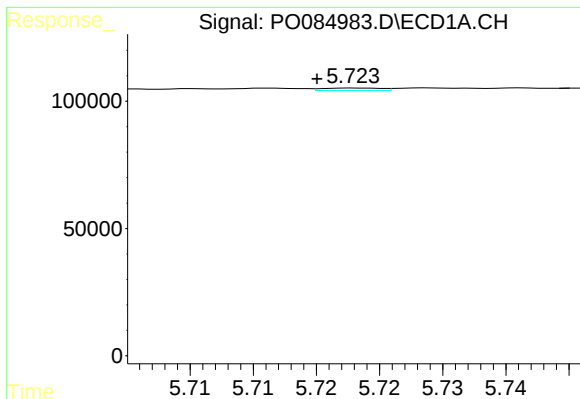

#17 AR-1242-2


R.T.: 5.723 min
Delta R.T.: 0.003 min
Response: 3173
Conc: 0.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

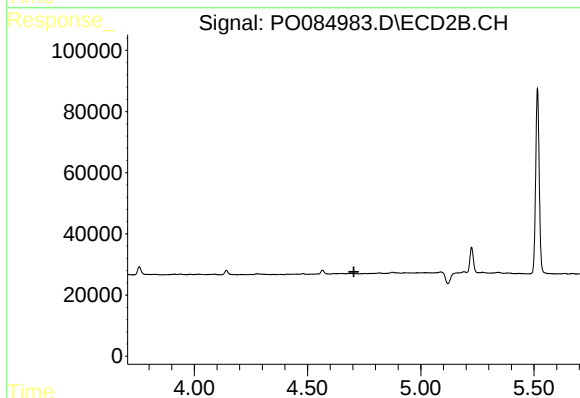


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.705 min
Response: 0
Conc: N.D.

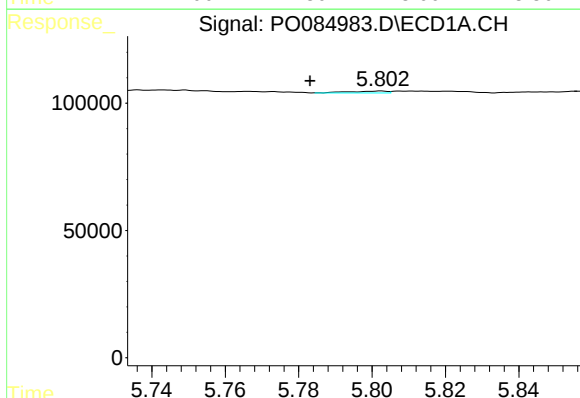


#18 AR-1242-3

R.T.: 5.803 min
Delta R.T.: 0.019 min
Response: 4993
Conc: 0.78 ng/ml

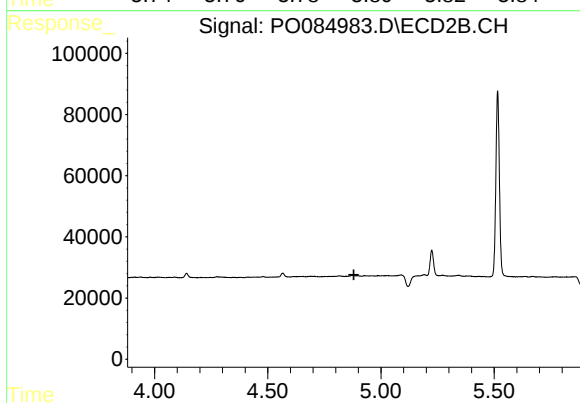

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.881 min
Response: 0
Conc: N.D.

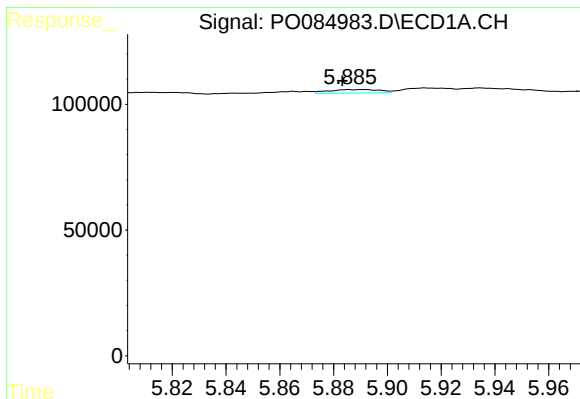

#19 AR-1242-4


R.T.: 5.886 min
Delta R.T.: 0.002 min
Response: 18656
Conc: 3.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

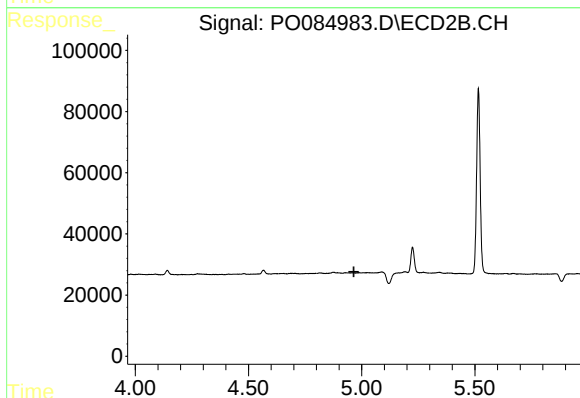


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

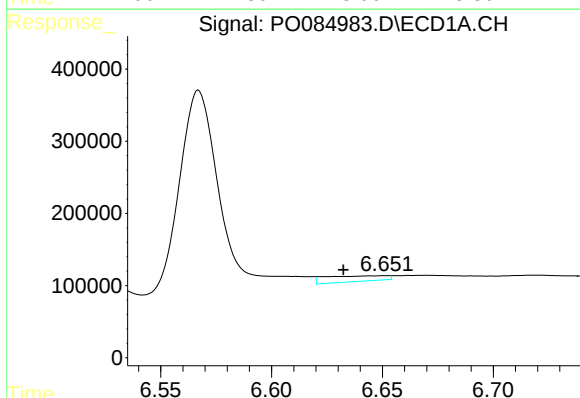


#20 AR-1242-5

R.T.: 6.651 min
Delta R.T.: 0.019 min
Response: 153899
Conc: 29.26 ng/ml

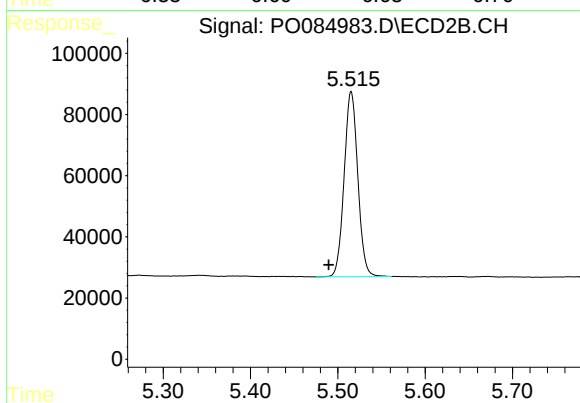

#20 AR-1242-5


R.T.: 5.515 min
Delta R.T.: 0.026 min
Response: 660115
Conc: 532.63 ng/ml

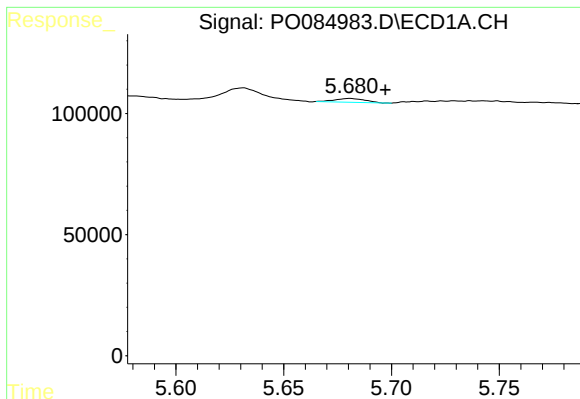

#21 AR-1248-1


R.T.: 5.681 min
Delta R.T.: -0.016 min
Response: 15000
Conc: 2.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

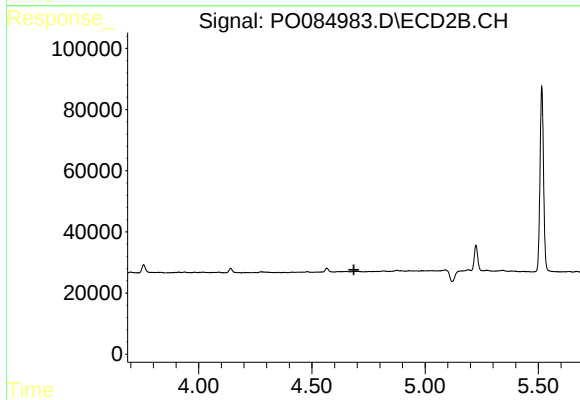


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

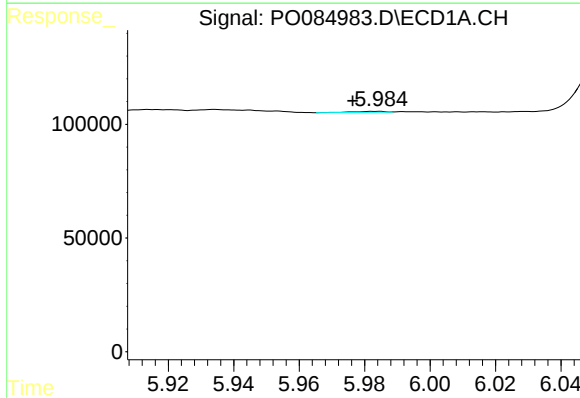


#22 AR-1248-2

R.T.: 5.984 min
Delta R.T.: 0.008 min
Response: 3182
Conc: 0.41 ng/ml

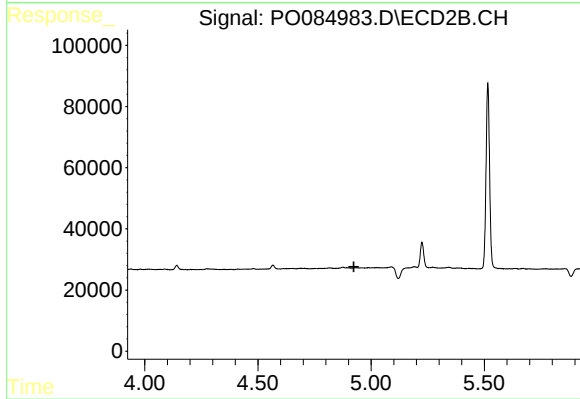

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.924 min
Response: 0
Conc: N.D.

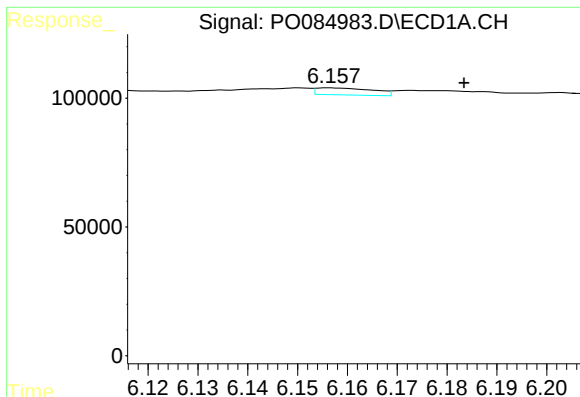

#23 AR-1248-3


R.T.: 6.156 min
Delta R.T.: -0.027 min
Response: 21508
Conc: 2.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

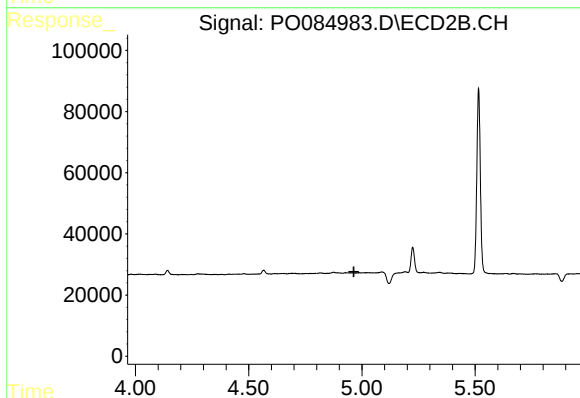


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.964 min
Response: 0
Conc: N.D.

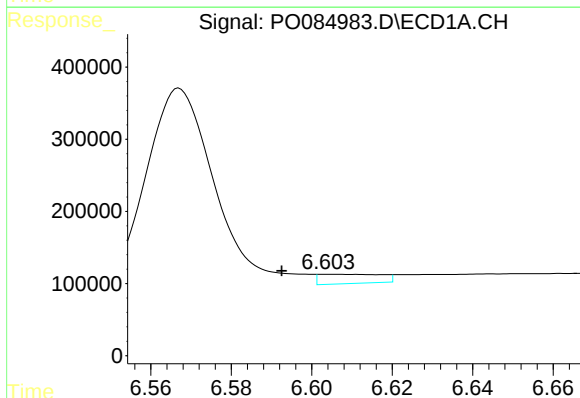


#24 AR-1248-4

R.T.: 6.604 min
Delta R.T.: 0.012 min
Response: 139906
Conc: 15.02 ng/ml

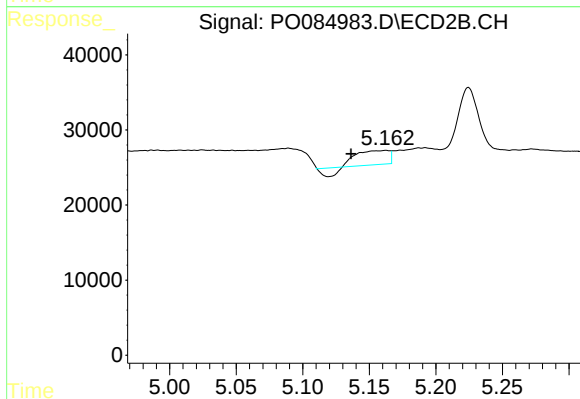

#24 AR-1248-4


R.T.: 5.162 min
Delta R.T.: 0.026 min
Response: 26117
Conc: 15.03 ng/ml

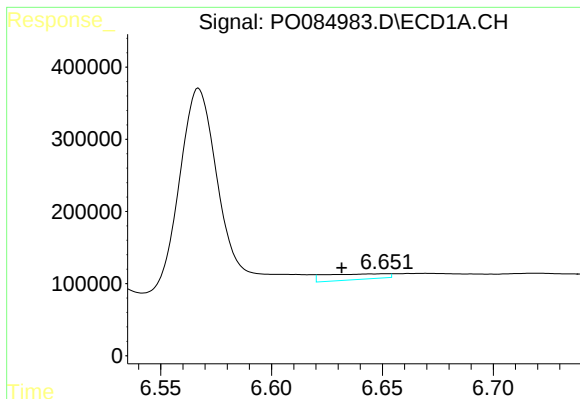

#25 AR-1248-5


R.T.: 6.651 min
Delta R.T.: 0.019 min
Response: 153899
Conc: 17.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

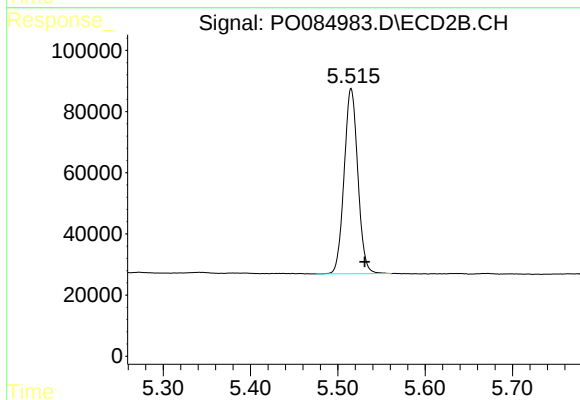


#25 AR-1248-5

R.T.: 5.515 min
Delta R.T.: -0.016 min
Response: 660115
Conc: 393.61 ng/ml

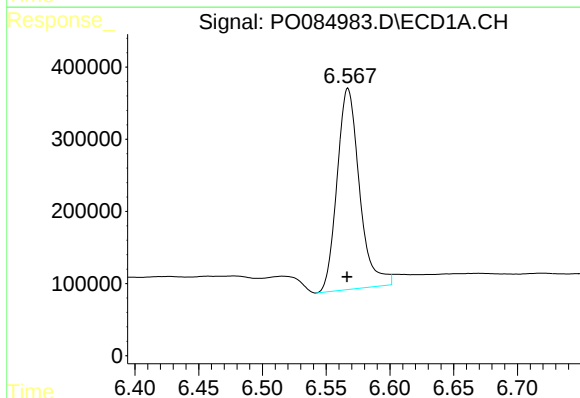


#26 AR-1254-1

R.T.: 6.567 min
Delta R.T.: 0.000 min
Response: 3403118
Conc: 346.96 ng/ml

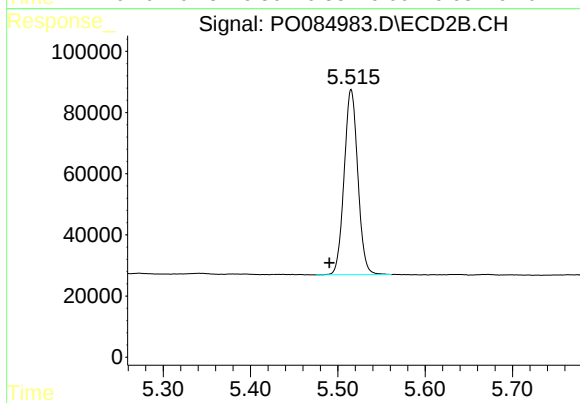

#26 AR-1254-1


R.T.: 5.515 min
Delta R.T.: 0.025 min
Response: 660115
Conc: 246.75 ng/ml

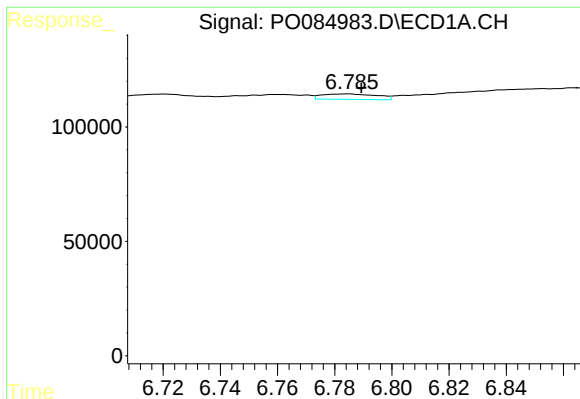

#27 AR-1254-2


R.T.: 6.785 min
Delta R.T.: -0.004 min
Response: 31936
Conc: 2.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

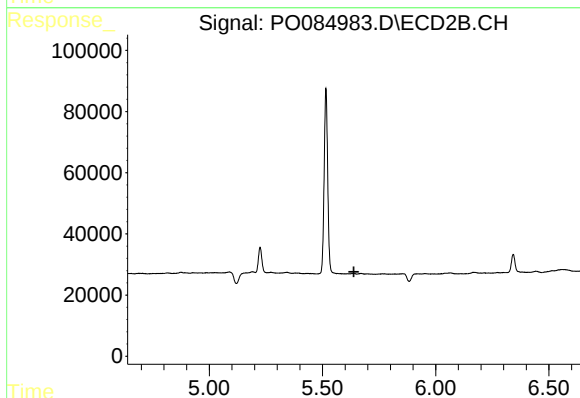


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.639 min
Response: 0
Conc: N.D.

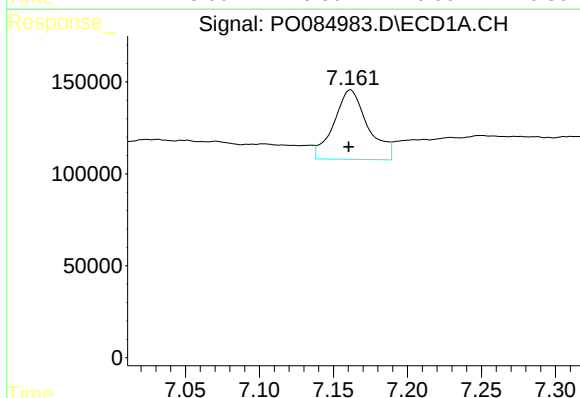


#28 AR-1254-3

R.T.: 7.162 min
Delta R.T.: 0.001 min
Response: 605845
Conc: 40.01 ng/ml

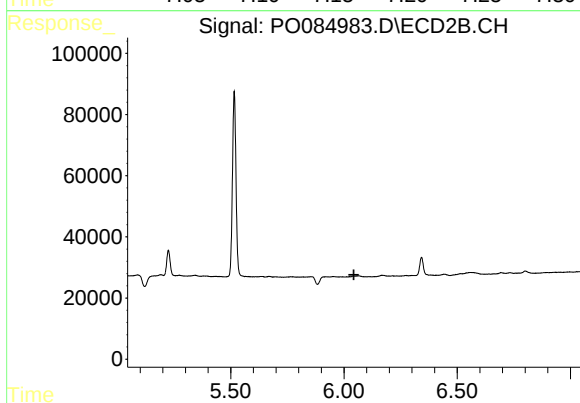

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.043 min
Response: 0
Conc: N.D.

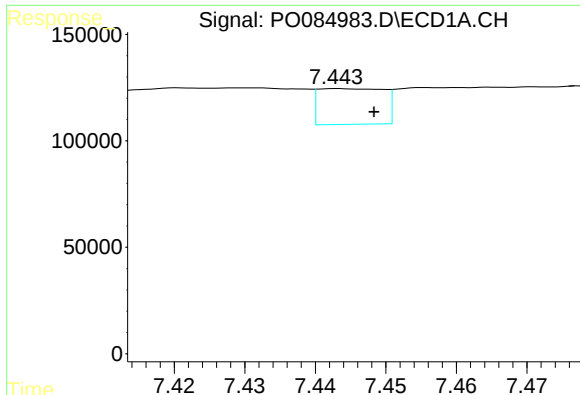

#29 AR-1254-4


R.T.: 7.443 min
Delta R.T.: -0.005 min
Response: 107695
Conc: 10.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

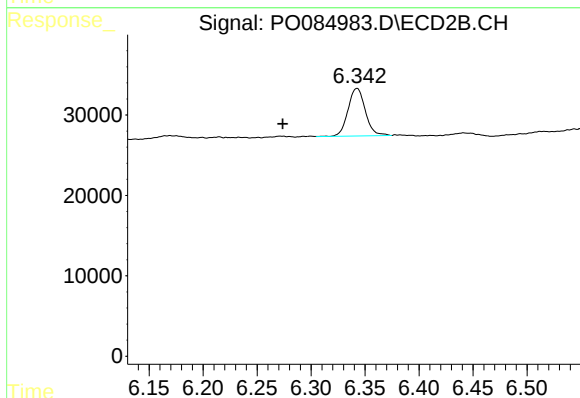


#29 AR-1254-4

R.T.: 6.343 min
Delta R.T.: 0.069 min
Response: 66130
Conc: 28.21 ng/ml

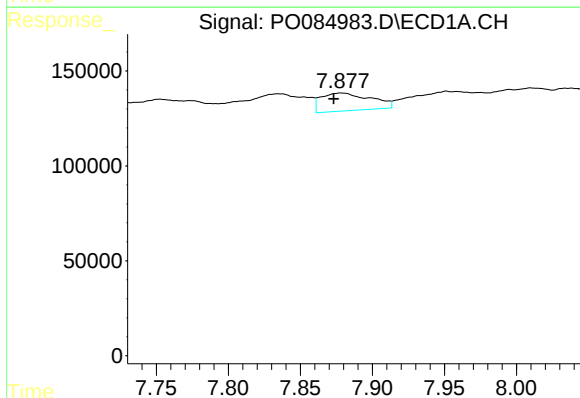


#30 AR-1254-5

R.T.: 7.878 min
Delta R.T.: 0.005 min
Response: 225793
Conc: 19.18 ng/ml

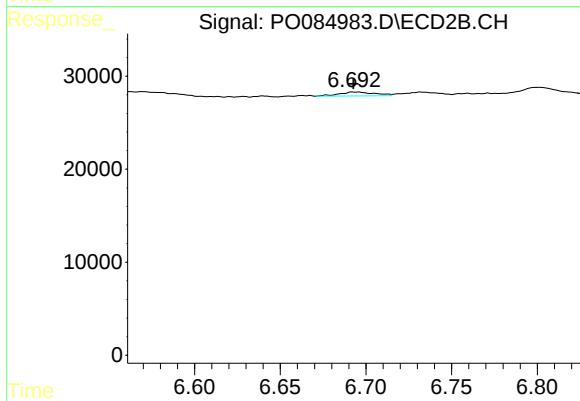

#30 AR-1254-5


R.T.: 6.692 min
Delta R.T.: 0.000 min
Response: 6114
Conc: 1.81 ng/ml

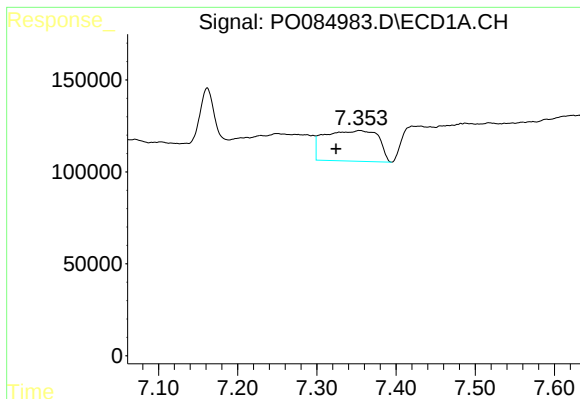

#31 AR-1260-1


R.T.: 7.354 min
Delta R.T.: 0.030 min
Response: 784780
Conc: 68.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

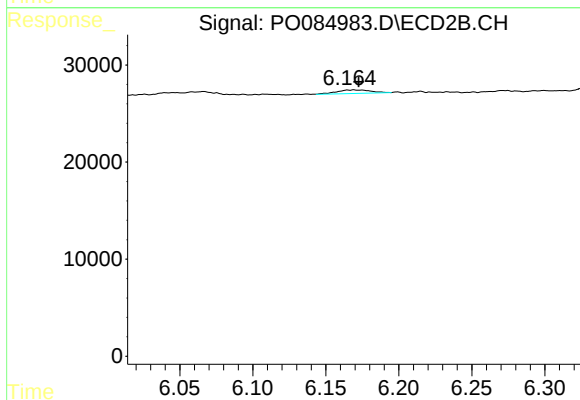


#31 AR-1260-1

R.T.: 6.169 min
Delta R.T.: -0.003 min
Response: 5890
Conc: 2.37 ng/ml

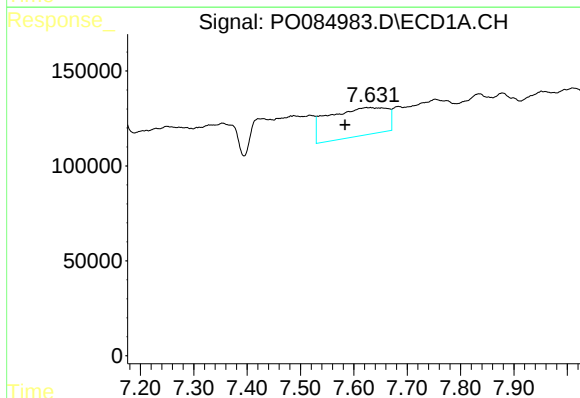


#32 AR-1260-2

R.T.: 7.623 min
Delta R.T.: 0.040 min
Response: 1143234
Conc: 88.91 ng/ml

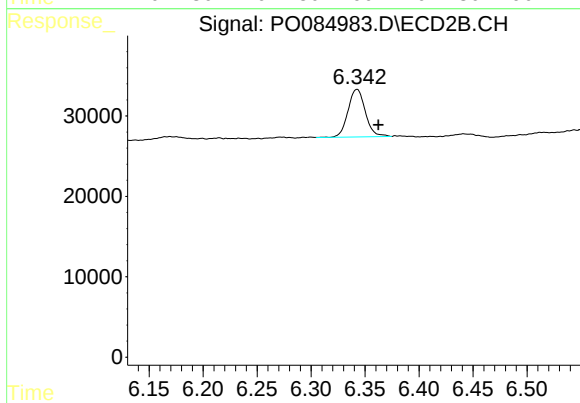

#32 AR-1260-2


R.T.: 6.343 min
Delta R.T.: -0.020 min
Response: 66130
Conc: 22.34 ng/ml

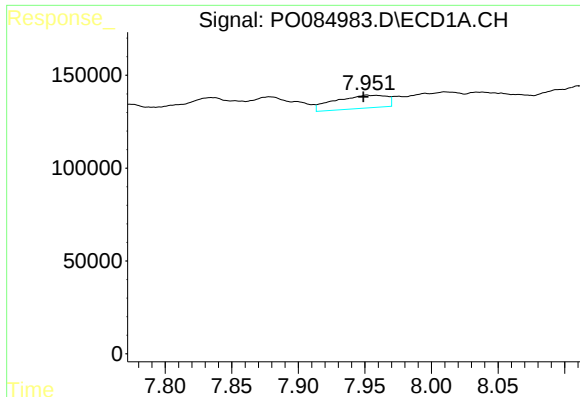

#33 AR-1260-3


R.T.: 7.952 min
Delta R.T.: 0.003 min
Response: 190800
Conc: 23.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

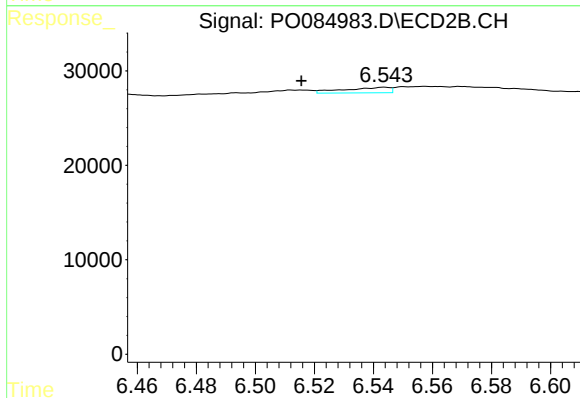


#33 AR-1260-3

R.T.: 6.544 min
Delta R.T.: 0.028 min
Response: 6280
Conc: 2.30 ng/ml

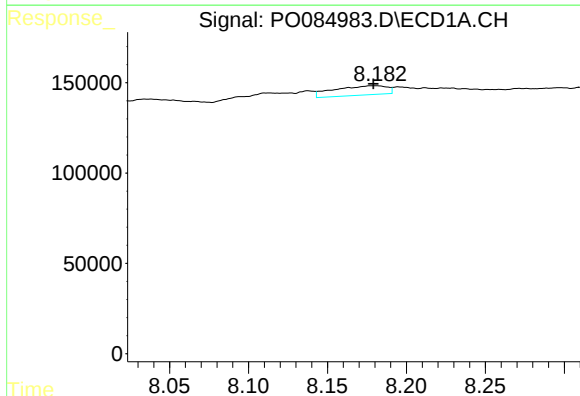


#34 AR-1260-4

R.T.: 8.179 min
Delta R.T.: 0.000 min
Response: 120123
Conc: 12.63 ng/ml

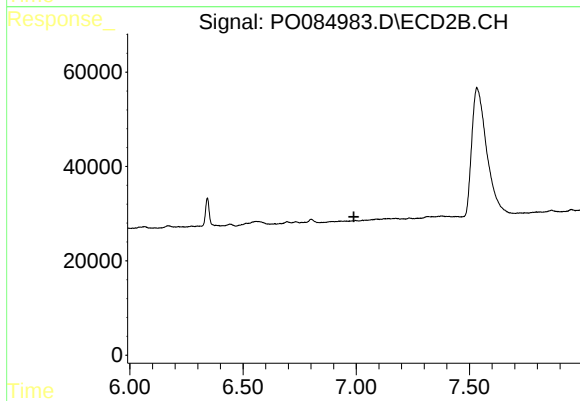

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.

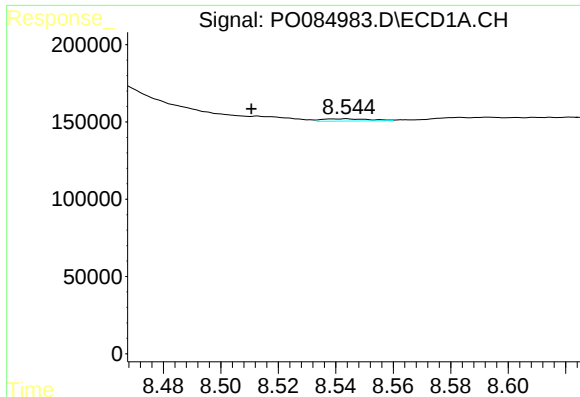

#35 AR-1260-5


R.T.: 8.544 min
Delta R.T.: 0.033 min
Response: 16028
Conc: 0.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

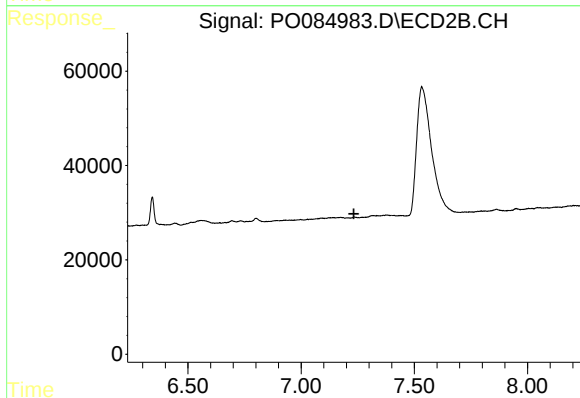


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.233 min
Response: 0
Conc: N.D.

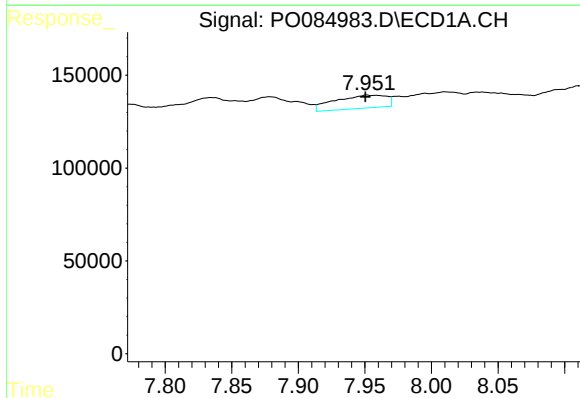


#36 AR-1262-1

R.T.: 7.952 min
Delta R.T.: 0.001 min
Response: 190800
Conc: 21.11 ng/ml

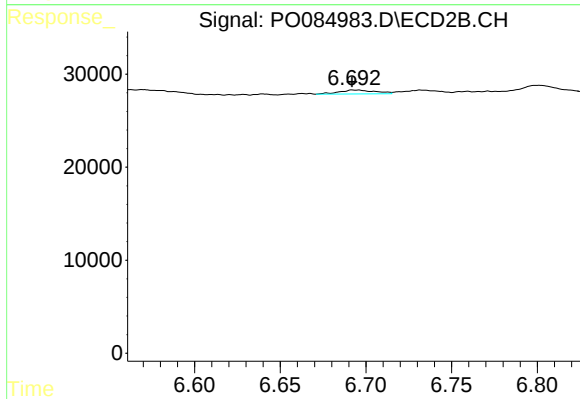

#36 AR-1262-1


R.T.: 6.692 min
Delta R.T.: 0.000 min
Response: 6114
Conc: 5.07 ng/ml

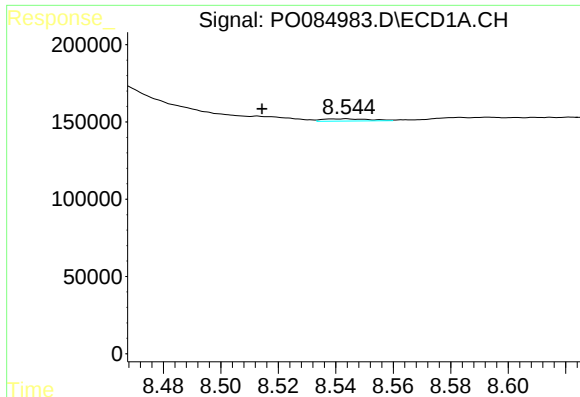

#37 AR-1262-2


R.T.: 8.544 min
Delta R.T.: 0.029 min
Response: 16028
Conc: 1.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

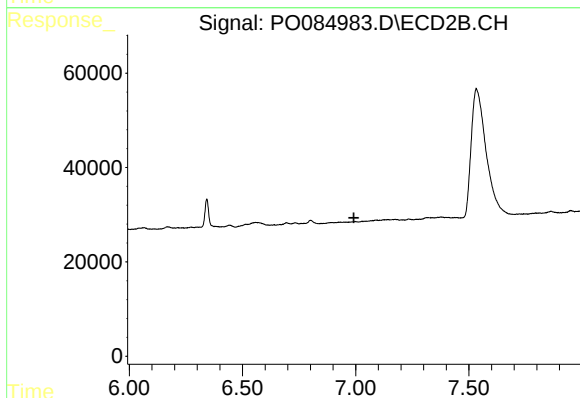


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 6.992 min
Response: 0
Conc: N.D.

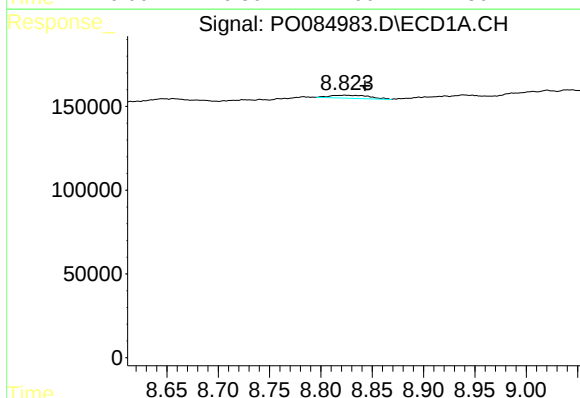


#38 AR-1262-3

R.T.: 8.823 min
Delta R.T.: -0.020 min
Response: 48503
Conc: 4.63 ng/ml

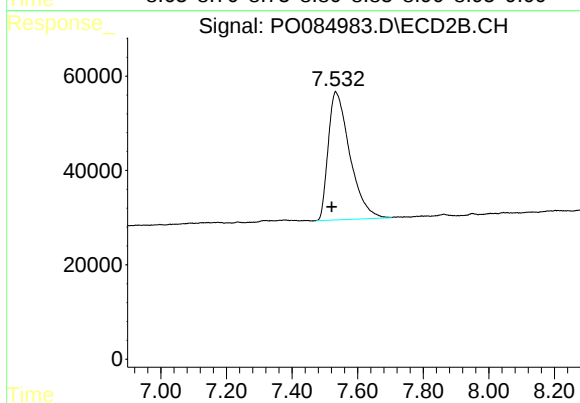

#38 AR-1262-3


R.T.: 7.532 min
Delta R.T.: 0.011 min
Response: 1238892
Conc: 796.99 ng/ml

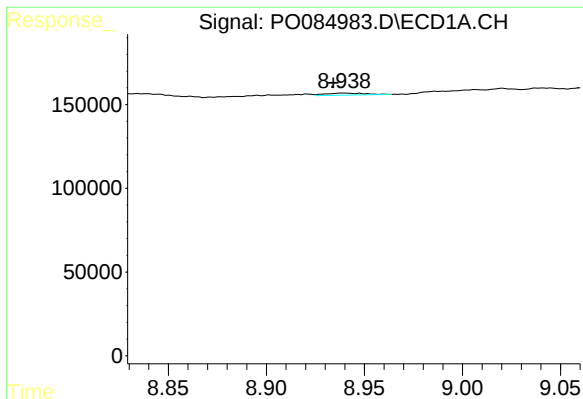

#39 AR-1262-4


R.T.: 8.939 min
Delta R.T.: 0.005 min
Response: 17279
Conc: 3.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

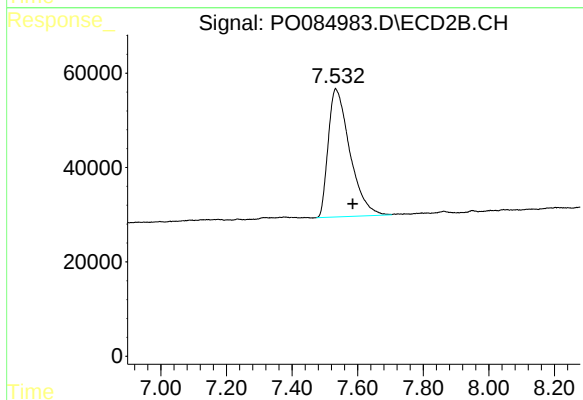


#39 AR-1262-4

R.T.: 7.532 min
Delta R.T.: -0.053 min
Response: 1238892
Conc: 437.29 ng/ml

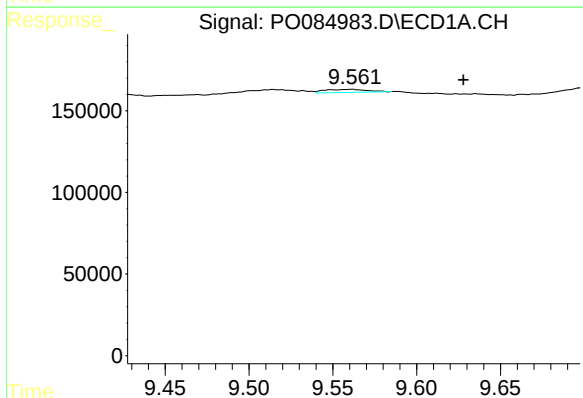


#40 AR-1262-5

R.T.: 9.561 min
Delta R.T.: -0.067 min
Response: 32529
Conc: 5.95 ng/ml

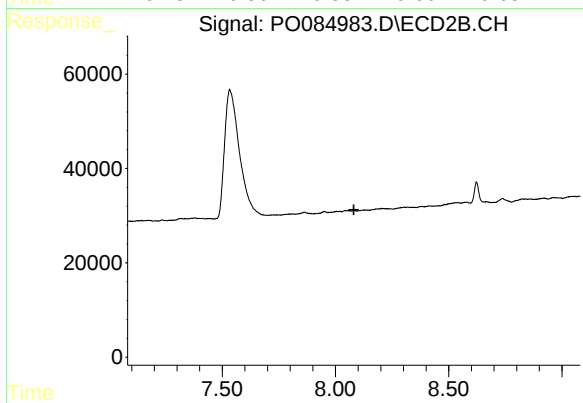

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

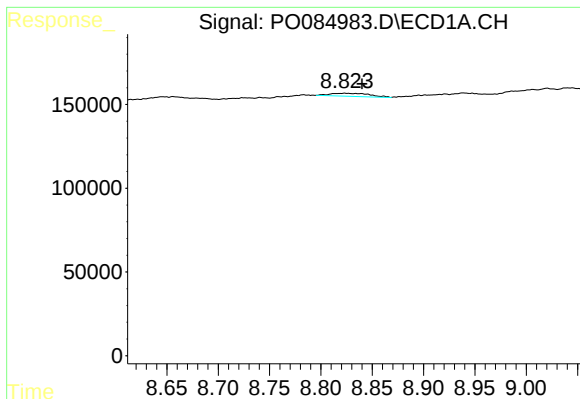

#41 AR-1268-1


R.T.: 8.823 min
Delta R.T.: -0.017 min
Response: 48503
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

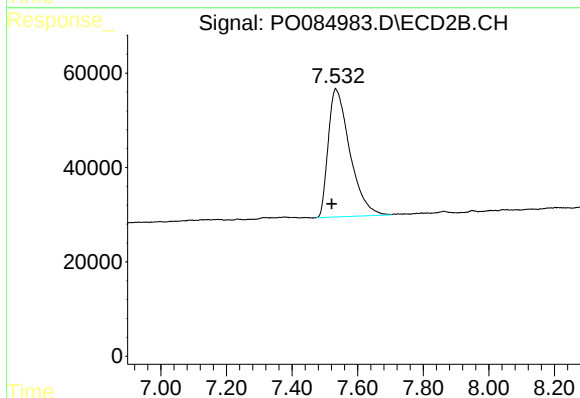


#41 AR-1268-1

R.T.: 7.532 min
Delta R.T.: 0.012 min
Response: 1238892
Conc: 181.61 ng/ml

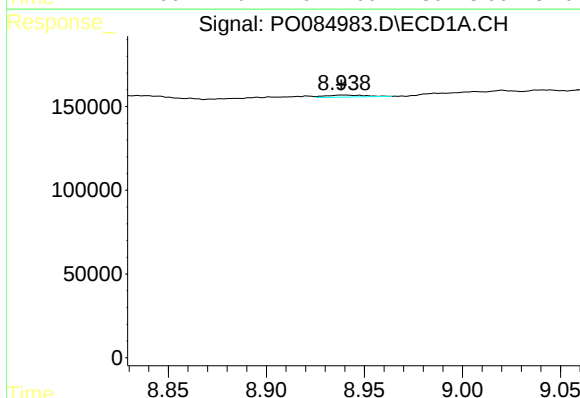


#42 AR-1268-2

R.T.: 8.939 min
Delta R.T.: 0.000 min
Response: 17279
Conc: 0.69 ng/ml

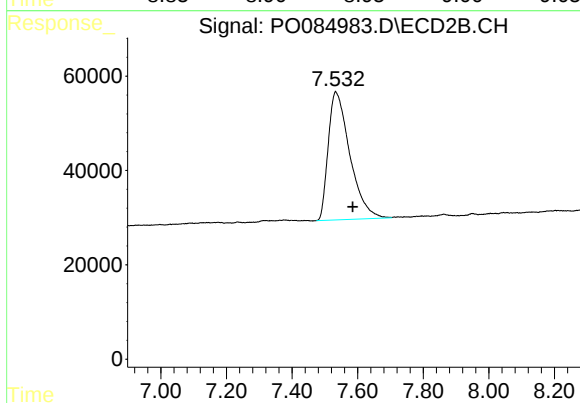

#42 AR-1268-2


R.T.: 7.532 min
Delta R.T.: -0.053 min
Response: 1238892
Conc: 204.41 ng/ml

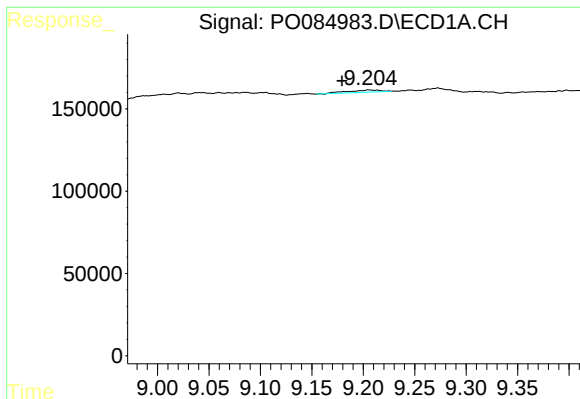

#43 AR-1268-3


R.T.: 9.205 min
Delta R.T.: 0.026 min
Response: 30433
Conc: 1.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

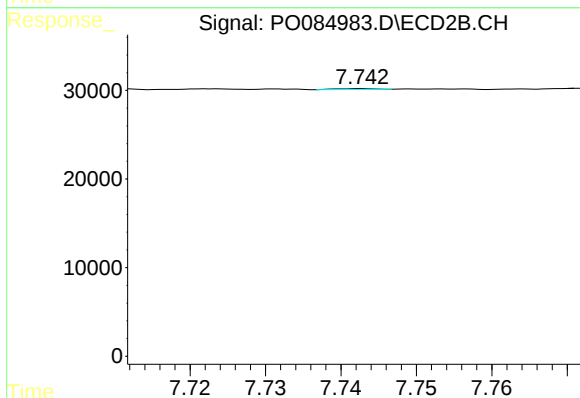


#43 AR-1268-3

R.T.: 7.743 min
Delta R.T.: -0.050 min
Response: 302
Conc: 0.06 ng/ml

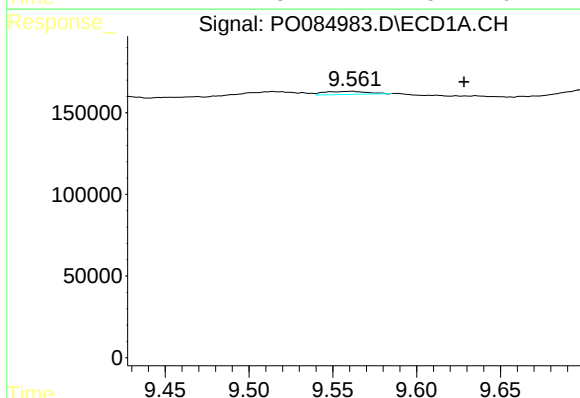


#44 AR-1268-4

R.T.: 9.561 min
Delta R.T.: -0.067 min
Response: 32529
Conc: 3.54 ng/ml

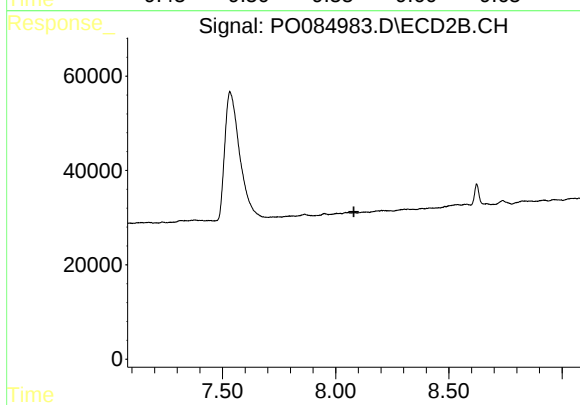

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

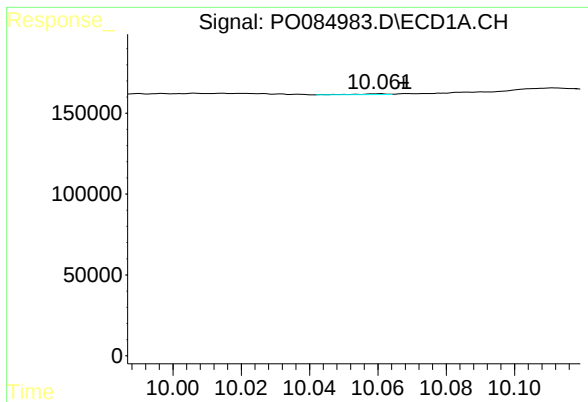

#45 AR-1268-5

R.T.: 10.060 min
Delta R.T.: -0.007 min
Response: 3267
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-67B

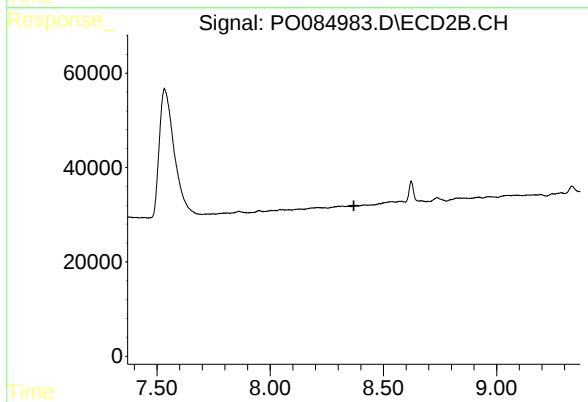

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.369 min
Response: 0
Conc: N.D.