

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0084984.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2022 10:38
 Operator : YP\AJ
 Sample : N1715-03 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-68A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:53:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.508	3.594	301451	74094	1.078	1.648 #
2)	SA Decachlor...	10.432	8.621	249116	58342	1.421	1.588
Target Compounds							
3)	L1 AR-1016-1	5.722	0.000	16337	0	1.745	N.D. #
4)	L1 AR-1016-2	5.722	0.000	16337	0	1.225	N.D. #
5)	L1 AR-1016-3	5.788	0.000	8915	0	1.116	N.D. #
6)	L1 AR-1016-4	5.885	0.000	4714	0	0.702	N.D. #
7)	L1 AR-1016-5	6.195	5.155	32503	25650	5.141	19.355 #
8)	L2 AR-1221-1	4.721	3.756f	26312	24215	8.224	41.528 #
9)	L2 AR-1221-2	4.824	0.000	15456	0	6.410	N.D. #
10)	L2 AR-1221-3	4.853	0.000	19194	0	2.636	N.D. #
11)	L3 AR-1232-1	4.853	0.000	19194	0	3.136	N.D. #
12)	L3 AR-1232-2	5.456	0.000	10802	0	3.630	N.D. #
13)	L3 AR-1232-3	5.722	0.000	16337	0	2.881	N.D. #
14)	L3 AR-1232-4	5.885	0.000	4714	0	1.651	N.D. #
15)	L3 AR-1232-5	5.976	5.155	26572	25650	11.761	46.254 #
16)	L4 AR-1242-1	5.722	0.000	16337	0	2.201	N.D. #
17)	L4 AR-1242-2	5.722	0.000	16337	0	1.542	N.D. #
18)	L4 AR-1242-3	5.788	0.000	8915	0	1.387	N.D. #
19)	L4 AR-1242-4	5.885	0.000	4714	0	0.869	N.D. #
20)	L4 AR-1242-5	6.648	5.515	62349	565034	11.854	455.911 #
21)	L5 AR-1248-1	5.722	0.000	16337	0	3.011	N.D. #
22)	L5 AR-1248-2	5.976	0.000	26572	0	3.456	N.D. #
23)	L5 AR-1248-3	6.195	0.000	32503	0	3.783	N.D. #
24)	L5 AR-1248-4	6.614	5.155	130581	25650	14.015	14.766
25)	L5 AR-1248-5	6.648	5.515	62349	565034	6.973	336.918 #
26)	L6 AR-1254-1	6.567	5.515	2562873	565034	261.293	211.212
27)	L6 AR-1254-2	6.787	0.000	15701	0	1.058	N.D. #
28)	L6 AR-1254-3	7.161	0.000	422076	0	27.876	N.D. #
29)	L6 AR-1254-4	7.457	6.342f	123736	56389	11.536	24.058 #
30)	L6 AR-1254-5	7.871	6.691	92236	4373	7.833	1.292 #
31)	L7 AR-1260-1	7.338	0.000	208988	0	18.314	N.D. #
32)	L7 AR-1260-2	7.580	6.342	180089	56389	14.006	19.051 #
33)	L7 AR-1260-3	7.950	6.561f	49537	22552	6.203	8.246 #
34)	L7 AR-1260-4	8.177	6.989	12774	5258	1.343	2.623 #
35)	L7 AR-1260-5	8.509	0.000	19579	0	1.065	N.D. #
36)	L8 AR-1262-1	7.950	6.691	49537	4373	5.480	3.624 #
37)	L8 AR-1262-2	8.509	6.989	19579	5258	1.227	2.589 #
38)	L8 AR-1262-3	8.844	7.536	17918	939919	1.709	604.655 #
39)	L8 AR-1262-4	8.935	7.536f	941	939919	0.186	331.758 #
40)	L8 AR-1262-5	9.663	8.054	2040	19959	0.373	15.078 #
41)	L9 AR-1268-1	8.844	7.536	17918	939919	0.641	137.783 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0084984.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2022 10:38
 Operator : YP\AJ
 Sample : N1715-03 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-68A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:53:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.935	7.536f	941	939919	0.038	155.083 #
43) L9	AR-1268-3	9.162	0.000	2934	0	0.137	N.D. #
44) L9	AR-1268-4	9.663	8.054	2040	19959	0.222	8.744 #
45) L9	AR-1268-5	10.070	8.422f	6316	4256	0.090	0.289 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
Data File : P0084984.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2022 10:38
Operator : YP\AJ
Sample : N1715-03 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:53:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

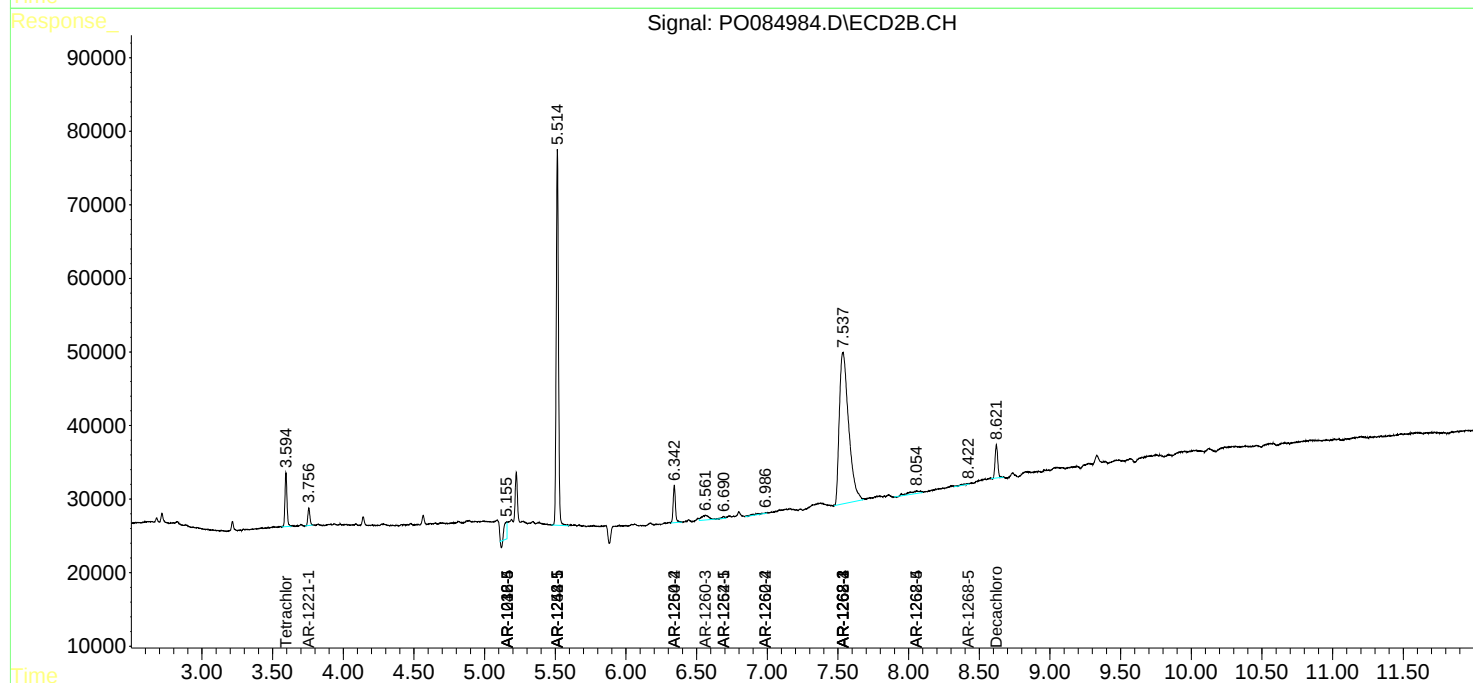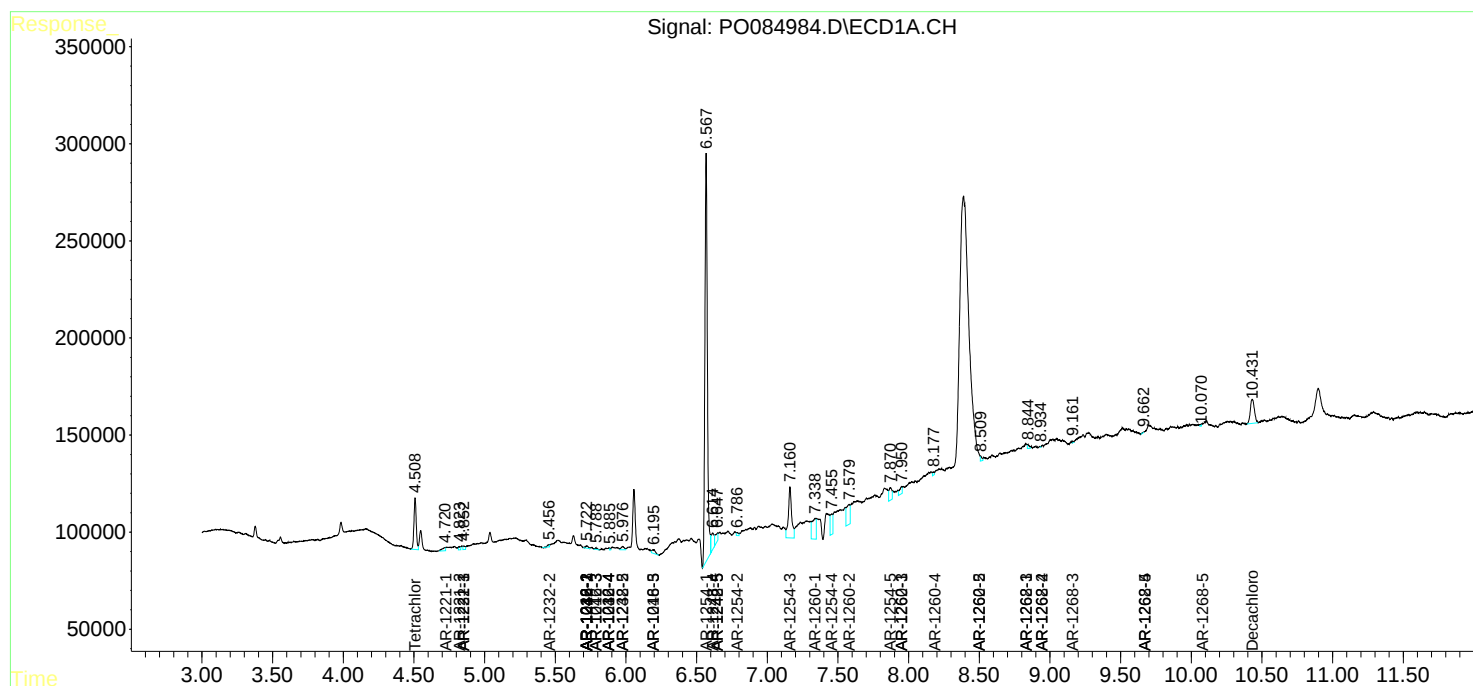


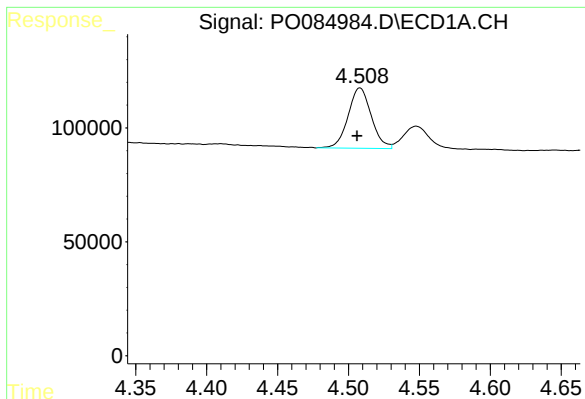

#1 Tetrachloro-m-xylene


R.T.: 4.508 min
Delta R.T.: 0.002 min
Response: 301451
Conc: 1.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

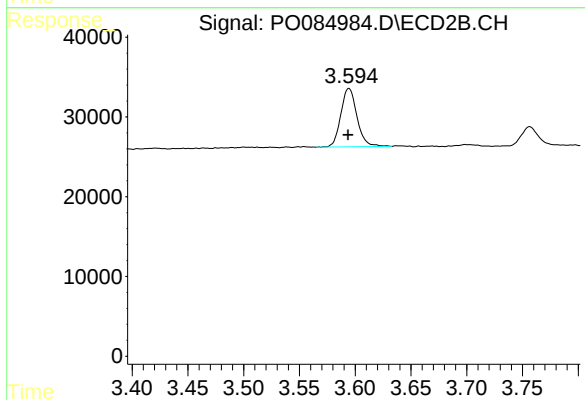


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 74094
Conc: 1.65 ng/ml

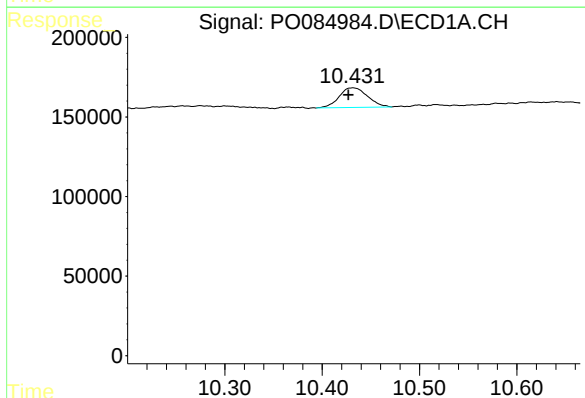


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.005 min
Response: 249116
Conc: 1.42 ng/ml

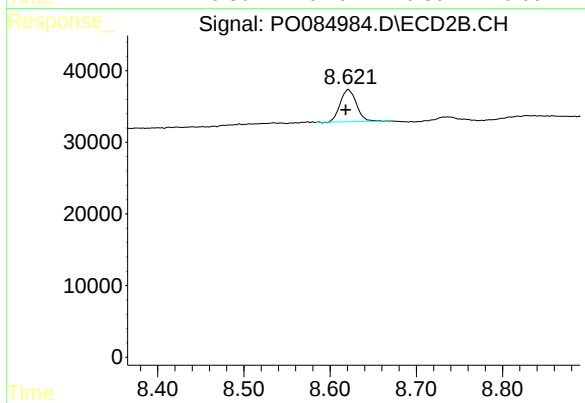

#2 Decachlorobiphenyl


R.T.: 8.621 min
Delta R.T.: 0.003 min
Response: 58342
Conc: 1.59 ng/ml

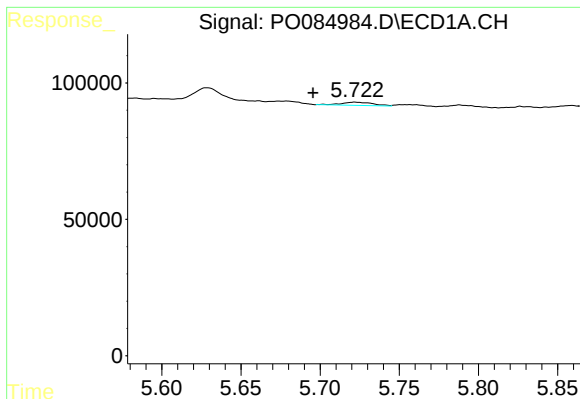

#3 AR-1016-1


R.T.: 5.722 min
Delta R.T.: 0.026 min
Response: 16337
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

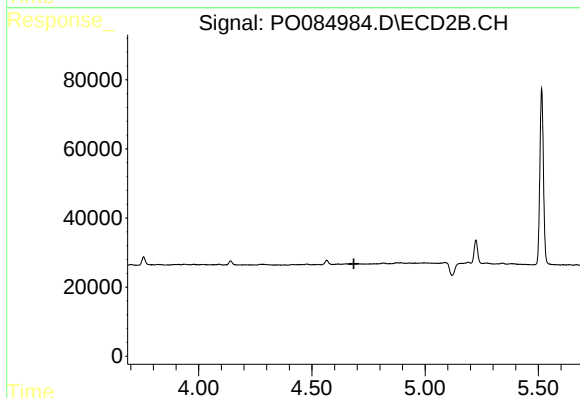


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

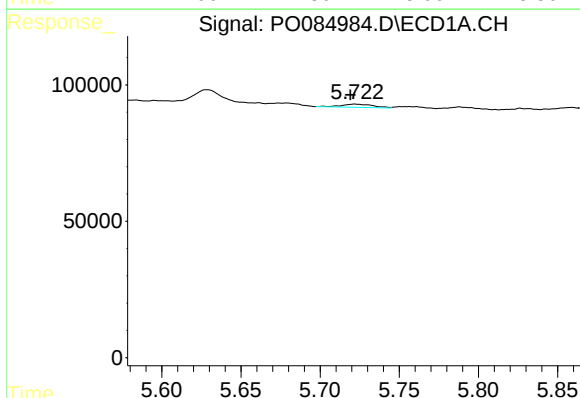


#4 AR-1016-2

R.T.: 5.722 min
Delta R.T.: 0.003 min
Response: 16337
Conc: 1.22 ng/ml

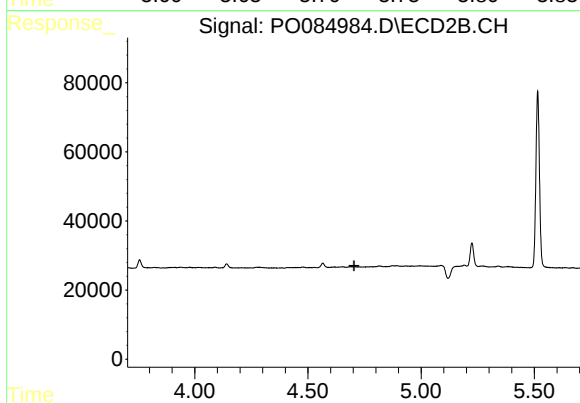

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

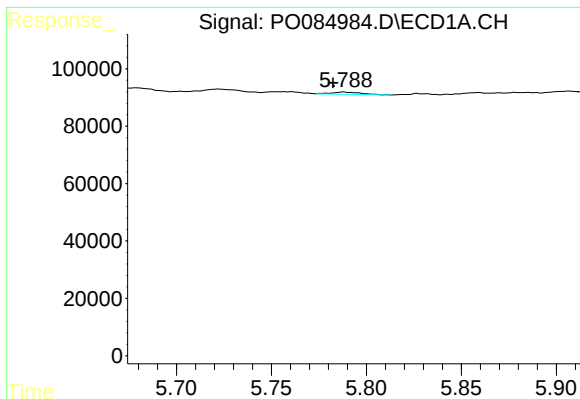

#5 AR-1016-3


R.T.: 5.788 min
Delta R.T.: 0.006 min
Response: 8915
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

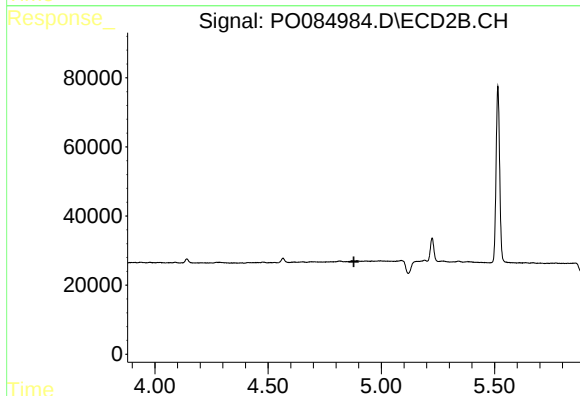


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.879 min
Response: 0
Conc: N.D.

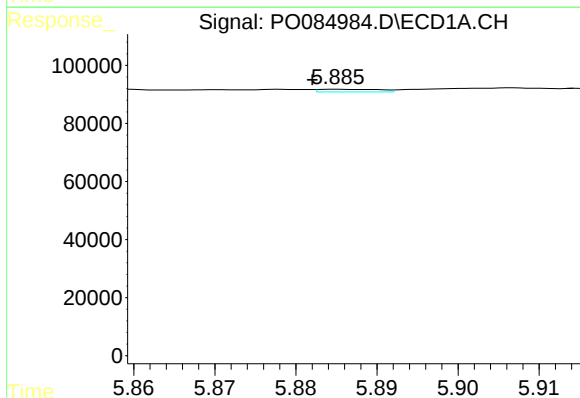


#6 AR-1016-4

R.T.: 5.885 min
Delta R.T.: 0.003 min
Response: 4714
Conc: 0.70 ng/ml

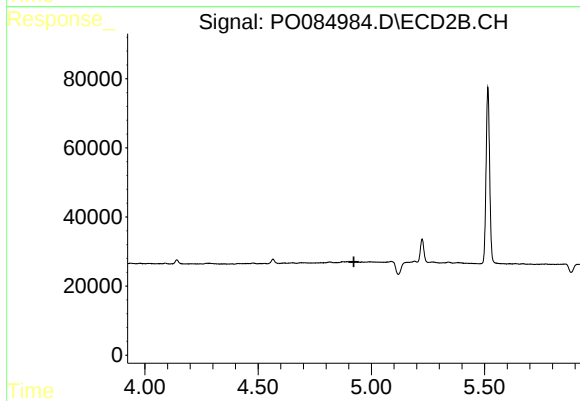

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.923 min
Response: 0
Conc: N.D.

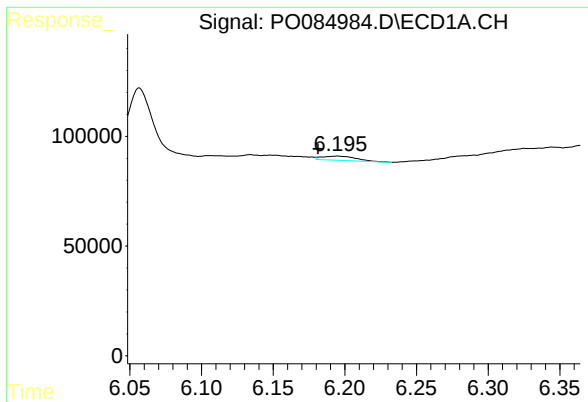

#7 AR-1016-5


R.T.: 6.195 min
Delta R.T.: 0.013 min
Response: 32503
Conc: 5.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

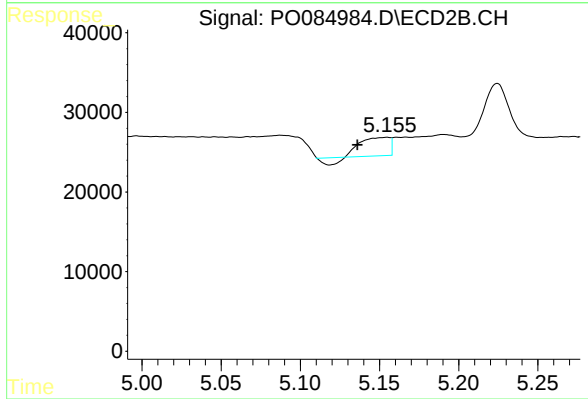


#7 AR-1016-5

R.T.: 5.155 min
Delta R.T.: 0.019 min
Response: 25650
Conc: 19.35 ng/ml

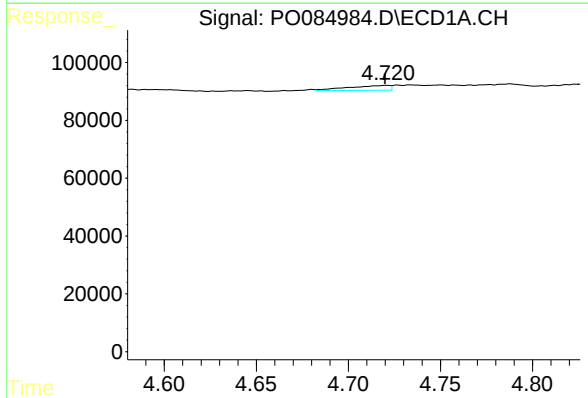


#8 AR-1221-1

R.T.: 4.721 min
Delta R.T.: 0.000 min
Response: 26312
Conc: 8.22 ng/ml

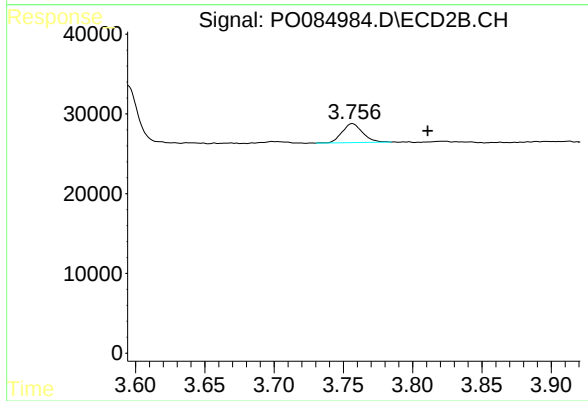

#8 AR-1221-1


R.T.: 3.756 min
Delta R.T.: -0.054 min
Response: 24215
Conc: 41.53 ng/ml

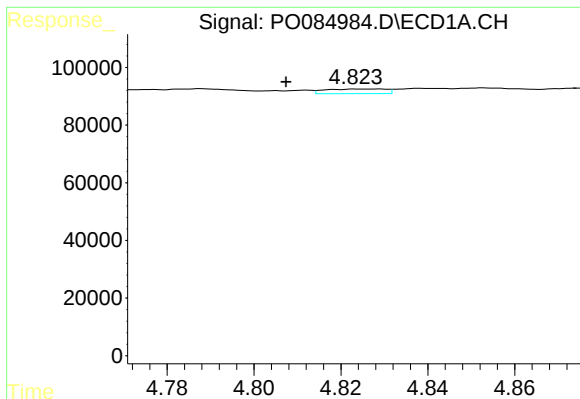

#9 AR-1221-2


R.T.: 4.824 min
Delta R.T.: 0.016 min
Response: 15456
Conc: 6.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

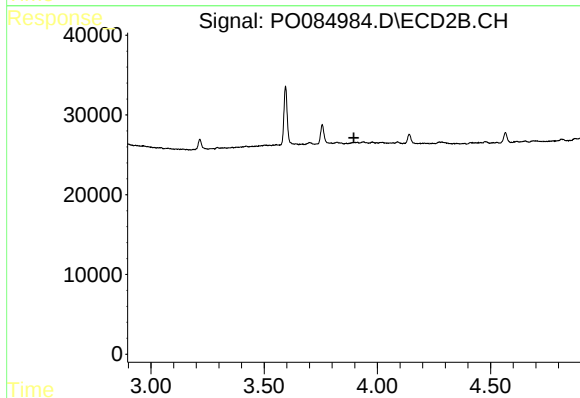


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

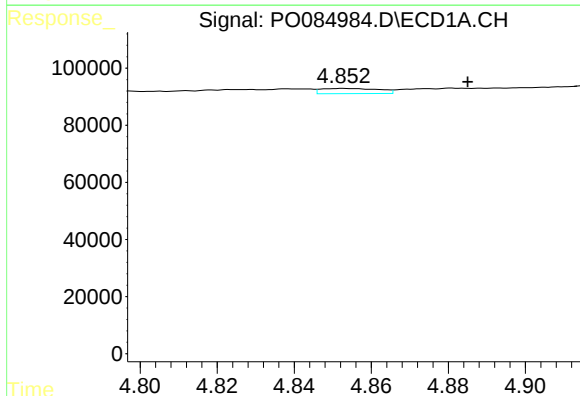


#10 AR-1221-3

R.T.: 4.853 min
Delta R.T.: -0.032 min
Response: 19194
Conc: 2.64 ng/ml

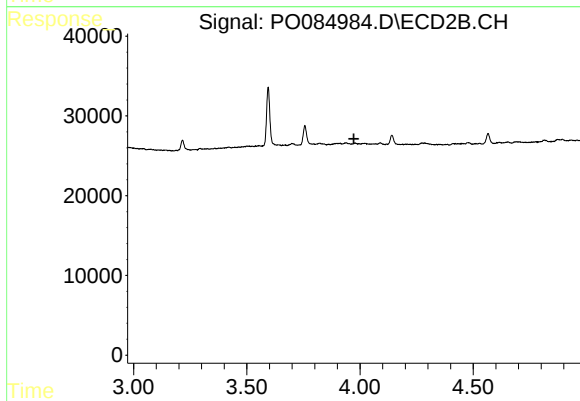

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.973 min
Response: 0
Conc: N.D.

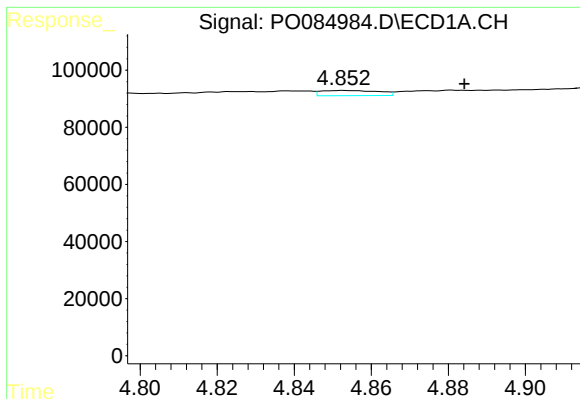

#11 AR-1232-1


R.T.: 4.853 min
Delta R.T.: -0.031 min
Response: 19194
Conc: 3.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

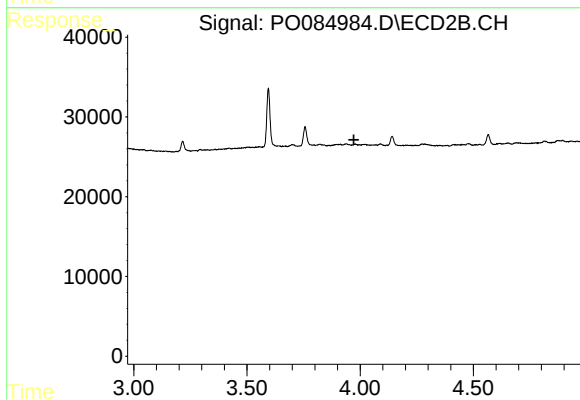


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

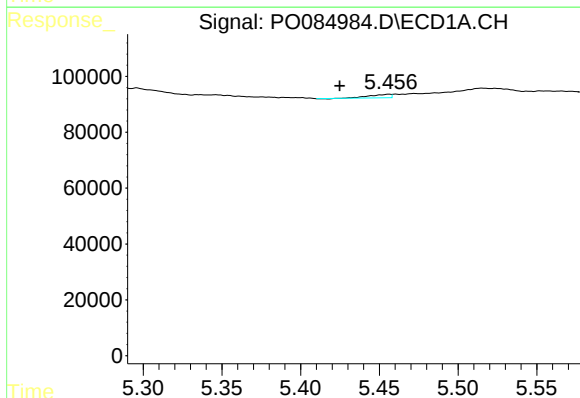


#12 AR-1232-2

R.T.: 5.456 min
Delta R.T.: 0.031 min
Response: 10802
Conc: 3.63 ng/ml

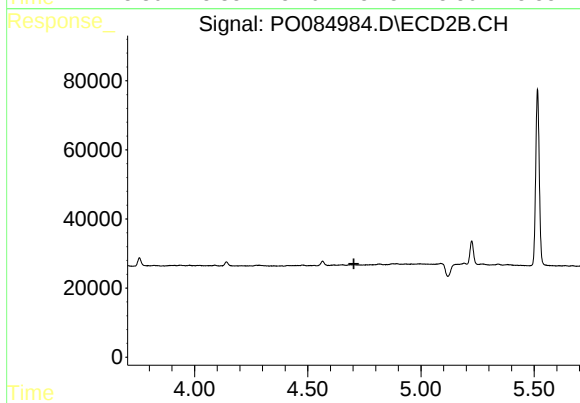

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

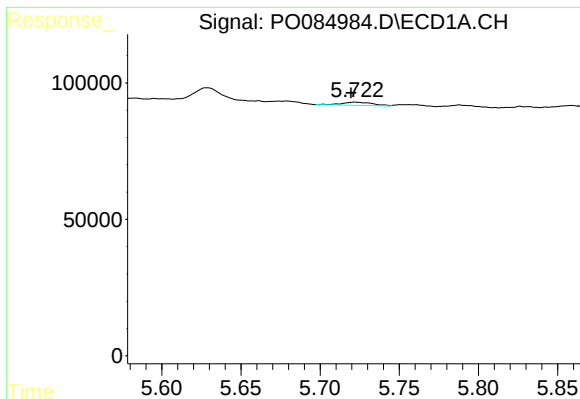

#13 AR-1232-3


R.T.: 5.722 min
Delta R.T.: 0.002 min
Response: 16337
Conc: 2.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

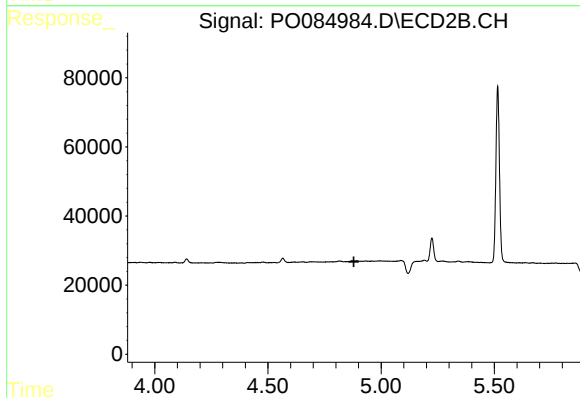


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.879 min
Response: 0
Conc: N.D.

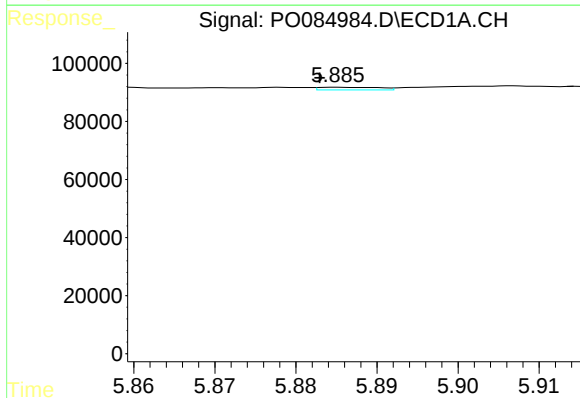


#14 AR-1232-4

R.T.: 5.885 min
Delta R.T.: 0.002 min
Response: 4714
Conc: 1.65 ng/ml

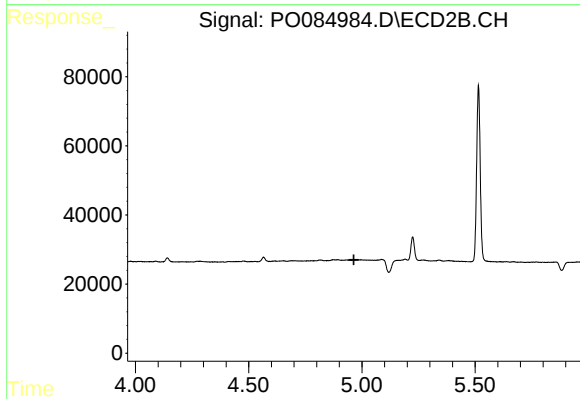

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.964 min
Response: 0
Conc: N.D.

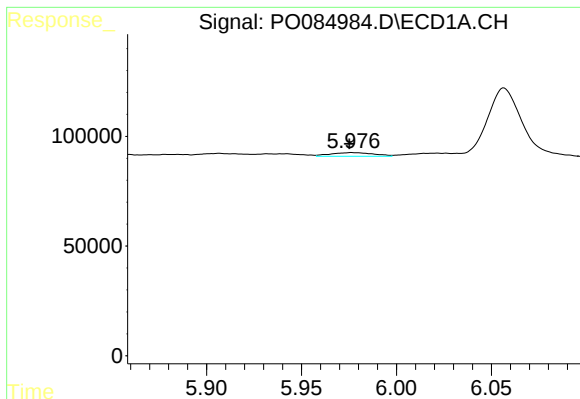

#15 AR-1232-5


R.T.: 5.976 min
Delta R.T.: 0.001 min
Response: 26572
Conc: 11.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

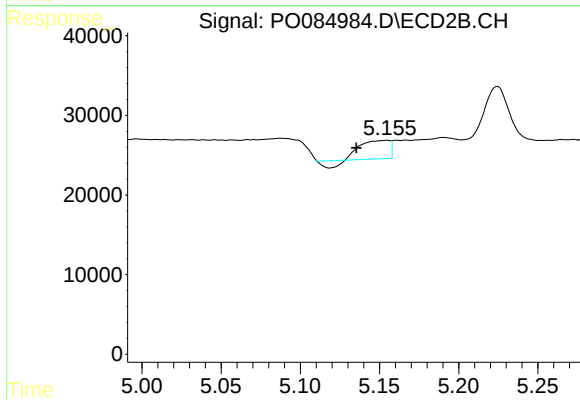


#15 AR-1232-5

R.T.: 5.155 min
Delta R.T.: 0.020 min
Response: 25650
Conc: 46.25 ng/ml

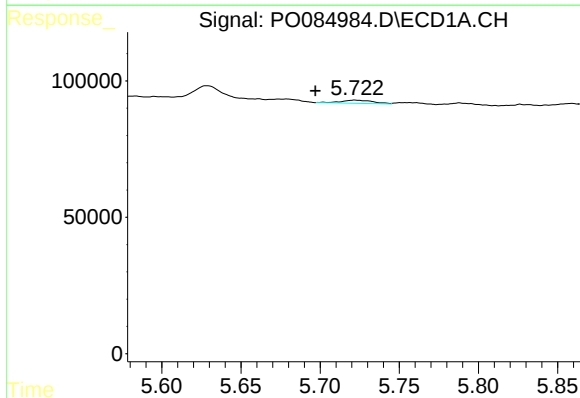


#16 AR-1242-1

R.T.: 5.722 min
Delta R.T.: 0.025 min
Response: 16337
Conc: 2.20 ng/ml

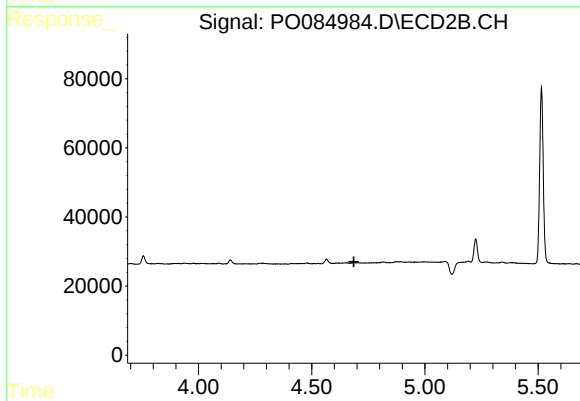

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

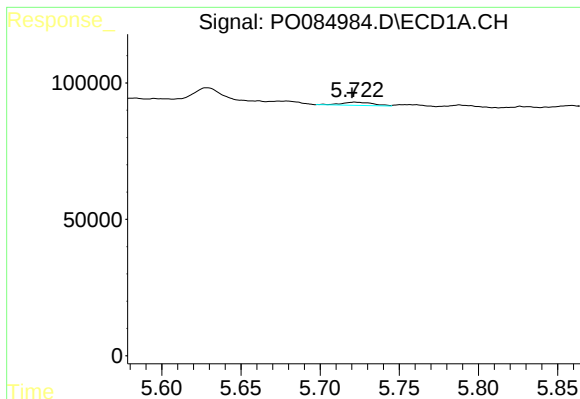

#17 AR-1242-2


R.T.: 5.722 min
Delta R.T.: 0.002 min
Response: 16337
Conc: 1.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

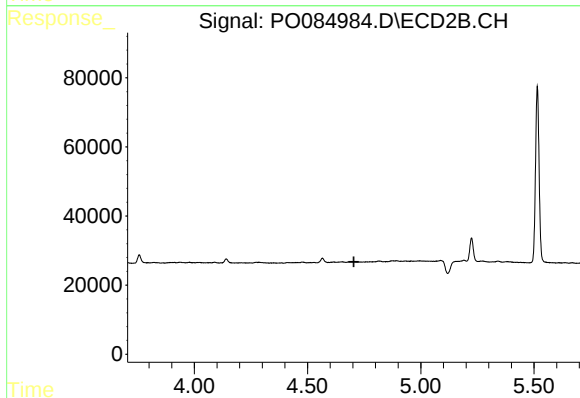


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.705 min
Response: 0
Conc: N.D.

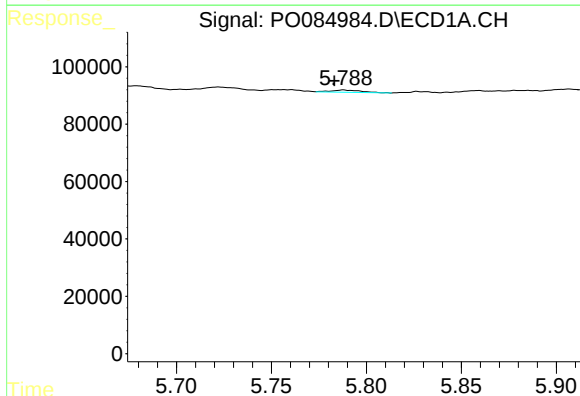


#18 AR-1242-3

R.T.: 5.788 min
Delta R.T.: 0.005 min
Response: 8915
Conc: 1.39 ng/ml

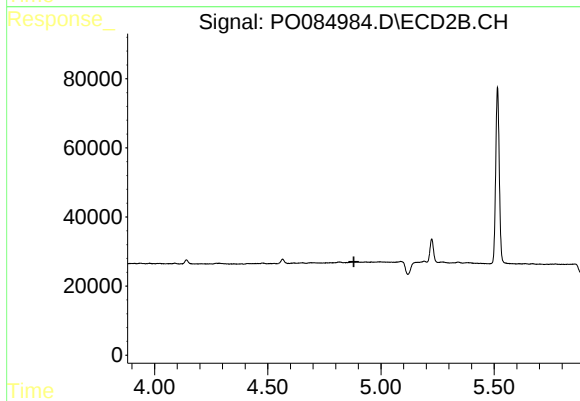

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.881 min
Response: 0
Conc: N.D.

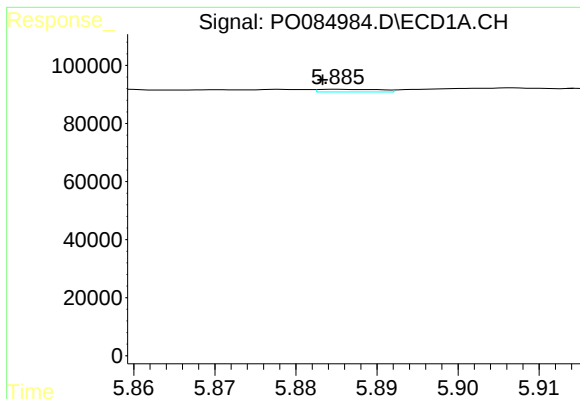

#19 AR-1242-4


R.T.: 5.885 min
Delta R.T.: 0.002 min
Response: 4714
Conc: 0.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

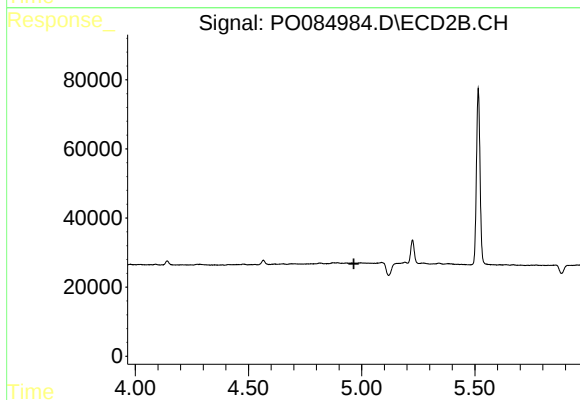


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

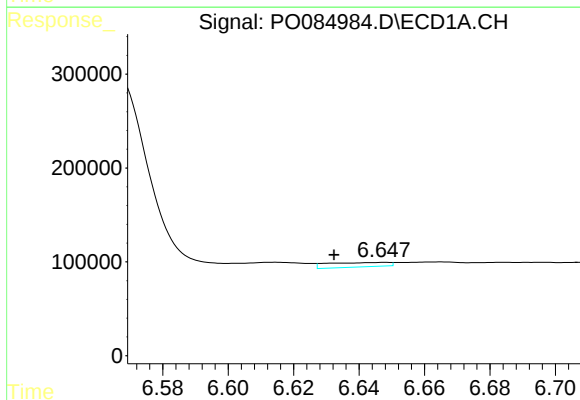


#20 AR-1242-5

R.T.: 6.648 min
Delta R.T.: 0.015 min
Response: 62349
Conc: 11.85 ng/ml

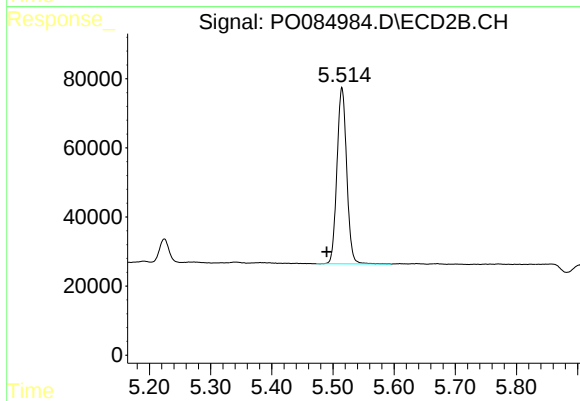

#20 AR-1242-5


R.T.: 5.515 min
Delta R.T.: 0.025 min
Response: 565034
Conc: 455.91 ng/ml

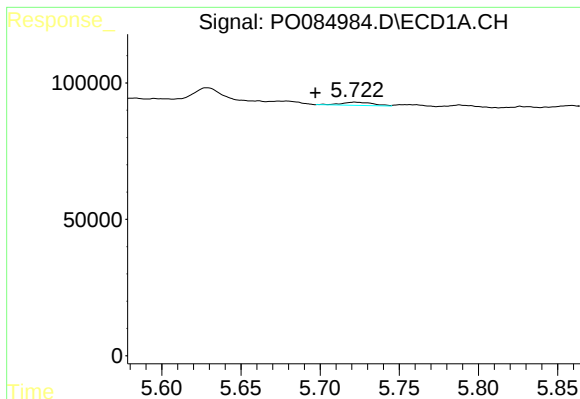

#21 AR-1248-1


R.T.: 5.722 min
Delta R.T.: 0.025 min
Response: 16337
Conc: 3.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

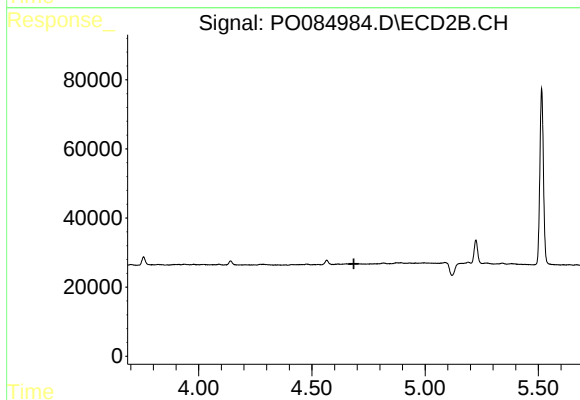


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

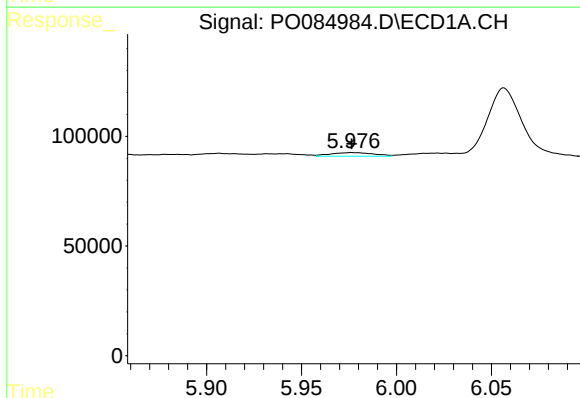


#22 AR-1248-2

R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 26572
Conc: 3.46 ng/ml

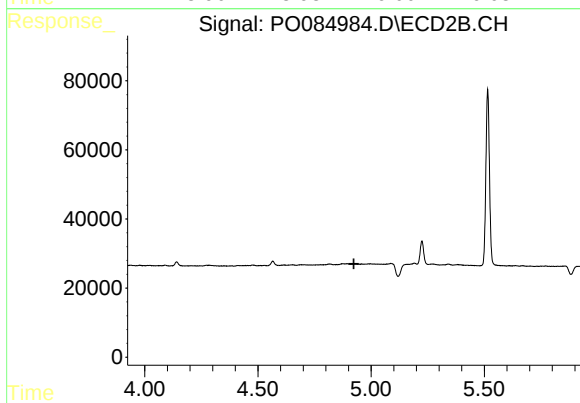

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.924 min
Response: 0
Conc: N.D.

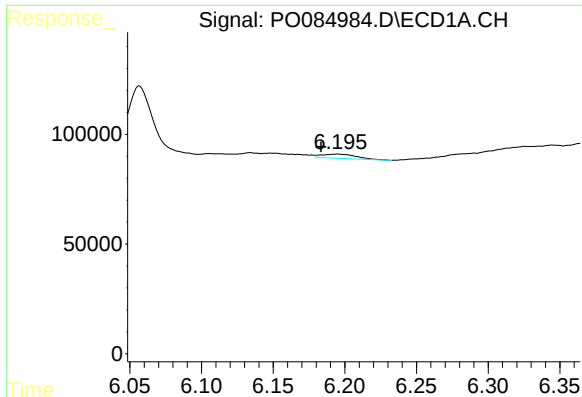

#23 AR-1248-3


R.T.: 6.195 min
Delta R.T.: 0.011 min
Response: 32503
Conc: 3.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

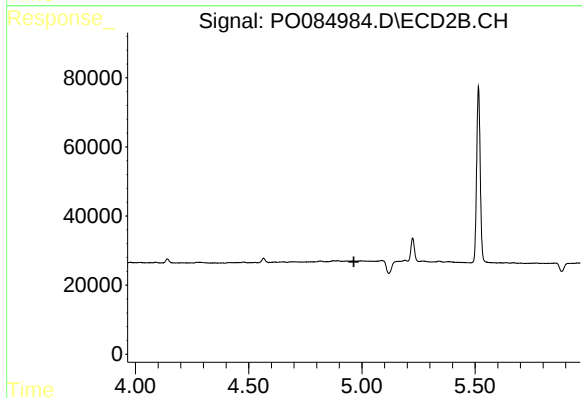


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.964 min
Response: 0
Conc: N.D.

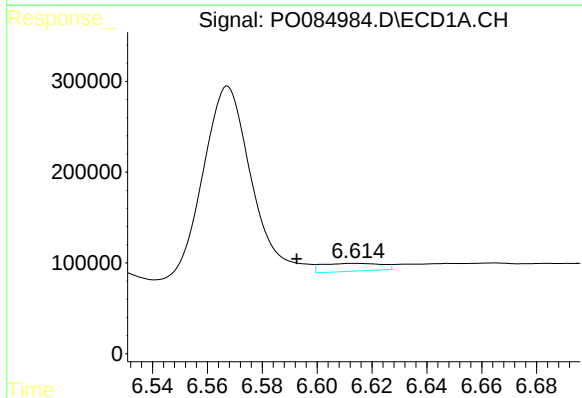


#24 AR-1248-4

R.T.: 6.614 min
Delta R.T.: 0.021 min
Response: 130581
Conc: 14.01 ng/ml

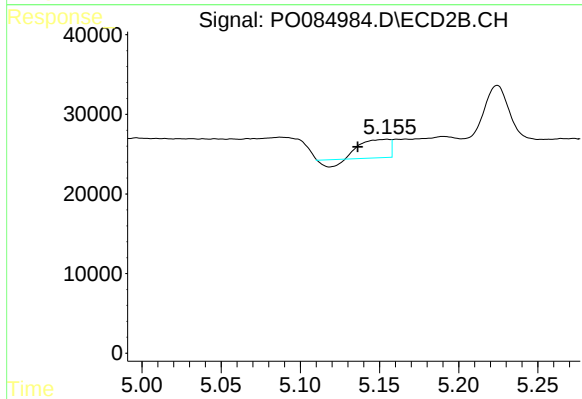

#24 AR-1248-4


R.T.: 5.155 min
Delta R.T.: 0.019 min
Response: 25650
Conc: 14.77 ng/ml

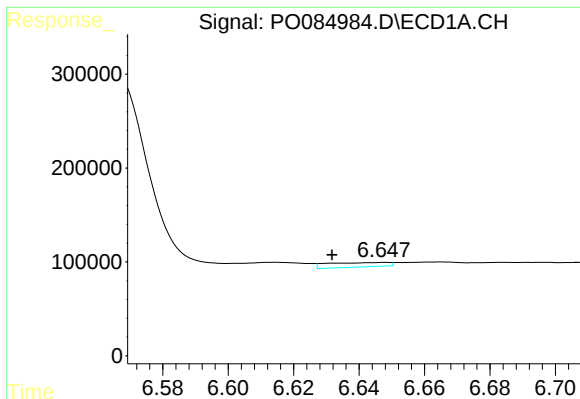

#25 AR-1248-5


R.T.: 6.648 min
Delta R.T.: 0.016 min
Response: 62349
Conc: 6.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

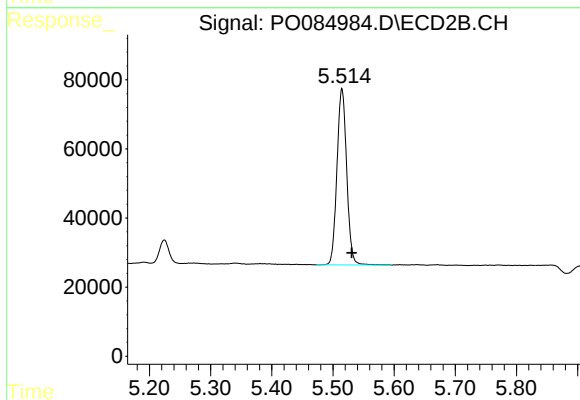


#25 AR-1248-5

R.T.: 5.515 min
Delta R.T.: -0.016 min
Response: 565034
Conc: 336.92 ng/ml

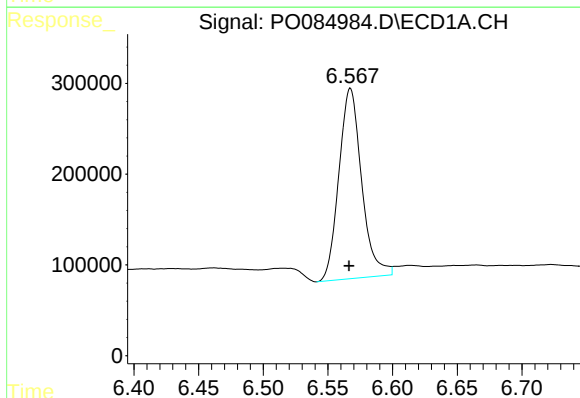


#26 AR-1254-1

R.T.: 6.567 min
Delta R.T.: 0.000 min
Response: 2562873
Conc: 261.29 ng/ml

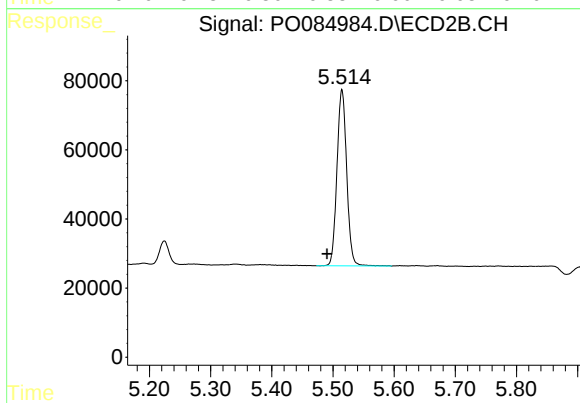

#26 AR-1254-1


R.T.: 5.515 min
Delta R.T.: 0.025 min
Response: 565034
Conc: 211.21 ng/ml

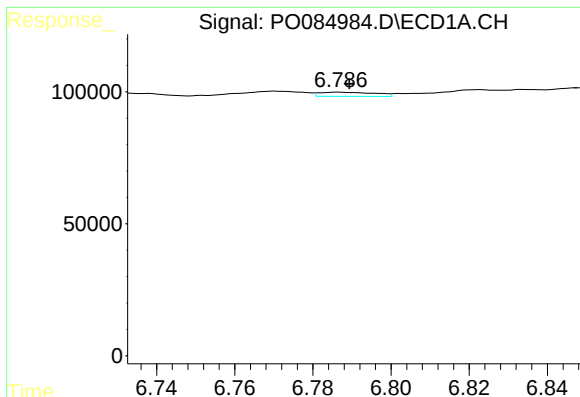

#27 AR-1254-2


R.T.: 6.787 min
Delta R.T.: -0.003 min
Response: 15701
Conc: 1.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

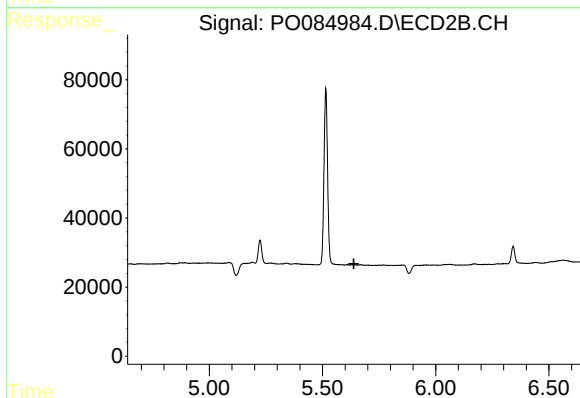


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.639 min
Response: 0
Conc: N.D.

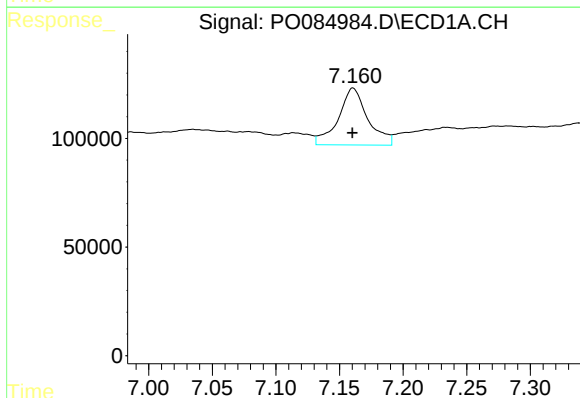


#28 AR-1254-3

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 422076
Conc: 27.88 ng/ml

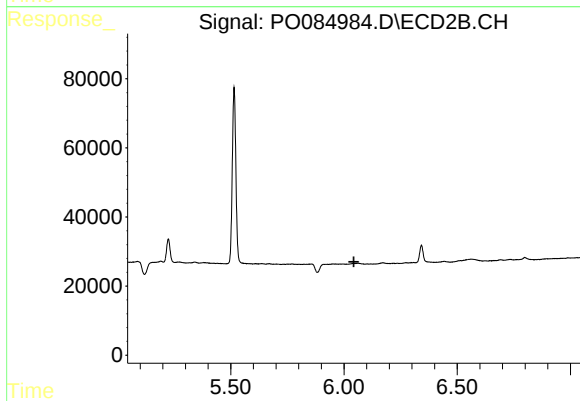

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.043 min
Response: 0
Conc: N.D.

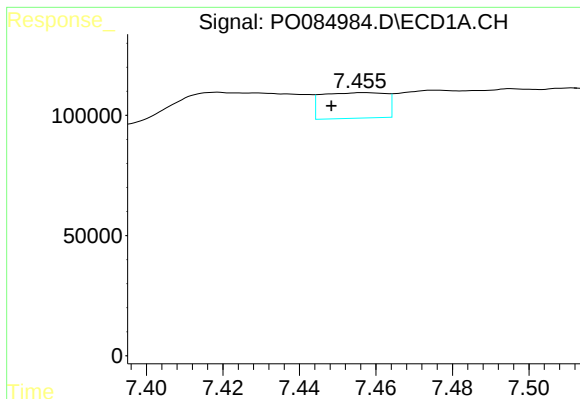

#29 AR-1254-4


R.T.: 7.457 min
Delta R.T.: 0.009 min
Response: 123736
Conc: 11.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

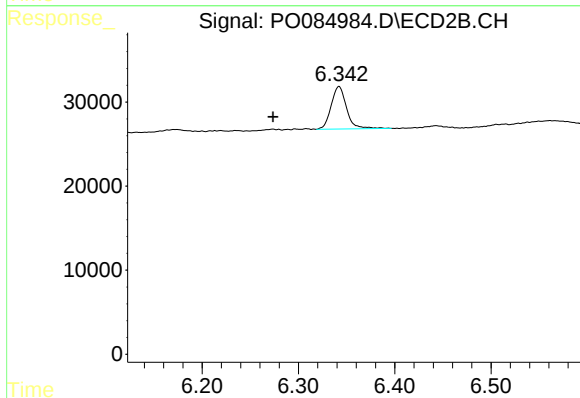


#29 AR-1254-4

R.T.: 6.342 min
Delta R.T.: 0.069 min
Response: 56389
Conc: 24.06 ng/ml

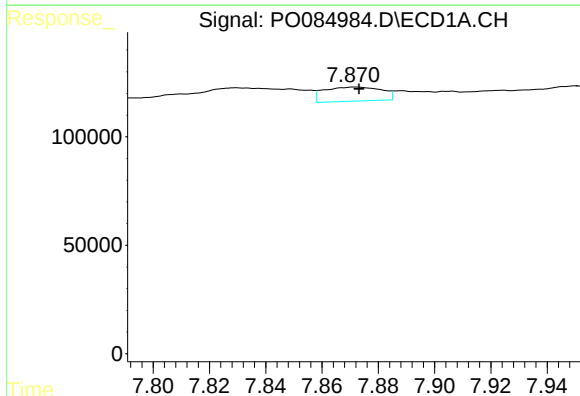


#30 AR-1254-5

R.T.: 7.871 min
Delta R.T.: -0.002 min
Response: 92236
Conc: 7.83 ng/ml

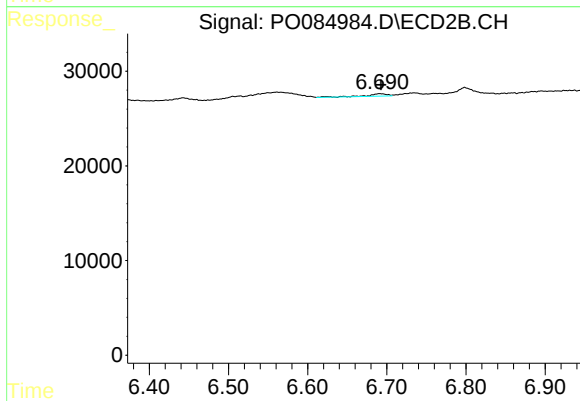

#30 AR-1254-5


R.T.: 6.691 min
Delta R.T.: -0.002 min
Response: 4373
Conc: 1.29 ng/ml

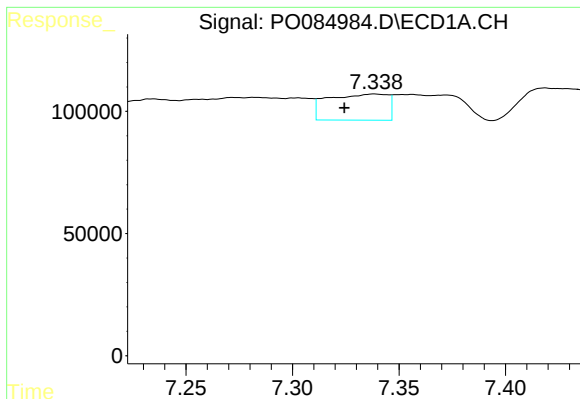

#31 AR-1260-1


R.T.: 7.338 min
Delta R.T.: 0.014 min
Response: 208988
Conc: 18.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

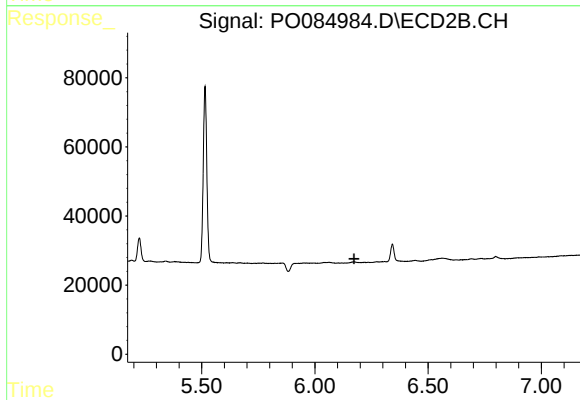


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.173 min
Response: 0
Conc: N.D.

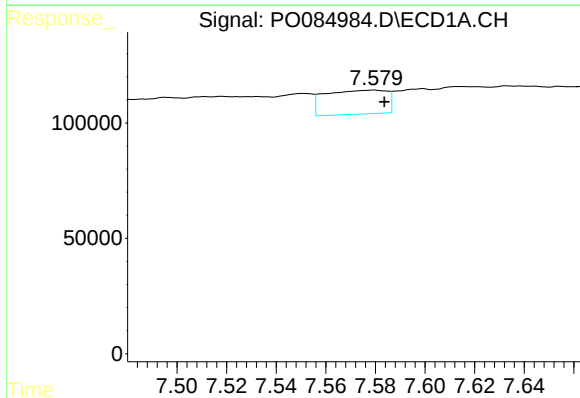


#32 AR-1260-2

R.T.: 7.580 min
Delta R.T.: -0.004 min
Response: 180089
Conc: 14.01 ng/ml

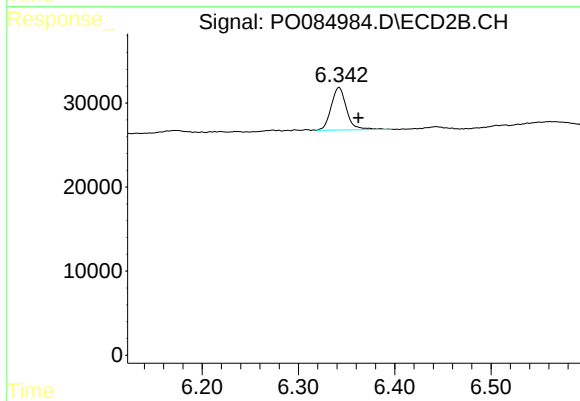

#32 AR-1260-2


R.T.: 6.342 min
Delta R.T.: -0.020 min
Response: 56389
Conc: 19.05 ng/ml

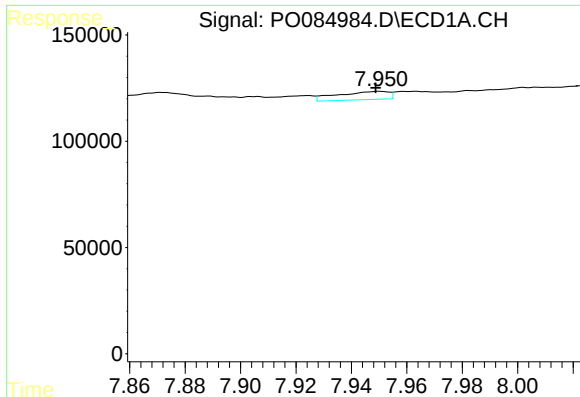

#33 AR-1260-3


R.T.: 7.950 min
Delta R.T.: 0.001 min
Response: 49537
Conc: 6.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

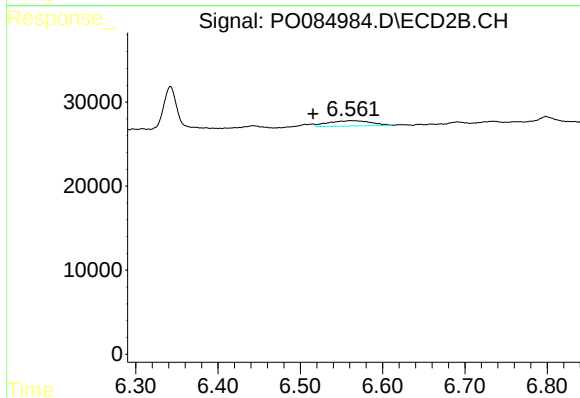


#33 AR-1260-3

R.T.: 6.561 min
Delta R.T.: 0.045 min
Response: 22552
Conc: 8.25 ng/ml

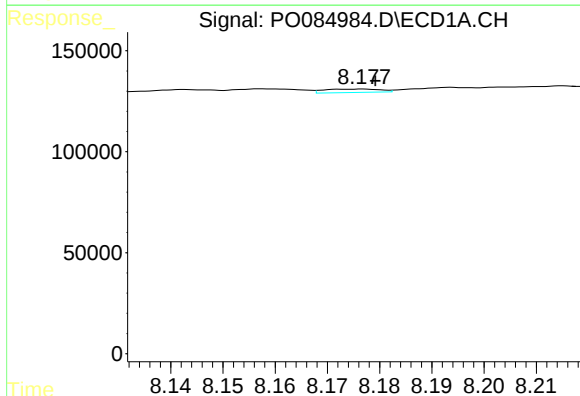


#34 AR-1260-4

R.T.: 8.177 min
Delta R.T.: -0.002 min
Response: 12774
Conc: 1.34 ng/ml

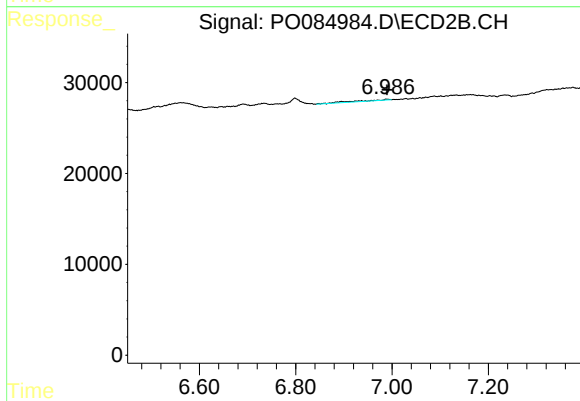

#34 AR-1260-4


R.T.: 6.989 min
Delta R.T.: 0.000 min
Response: 5258
Conc: 2.62 ng/ml

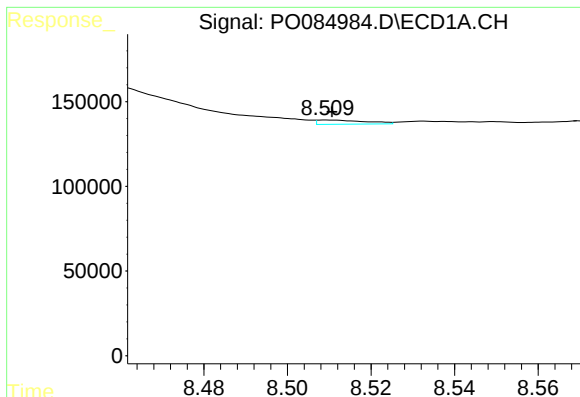

#35 AR-1260-5


R.T.: 8.509 min
Delta R.T.: -0.001 min
Response: 19579
Conc: 1.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

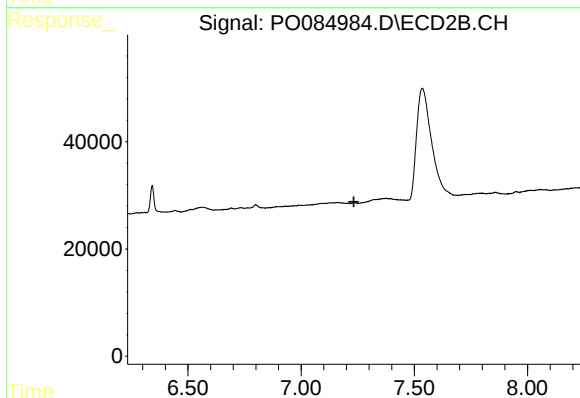


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.233 min
Response: 0
Conc: N.D.

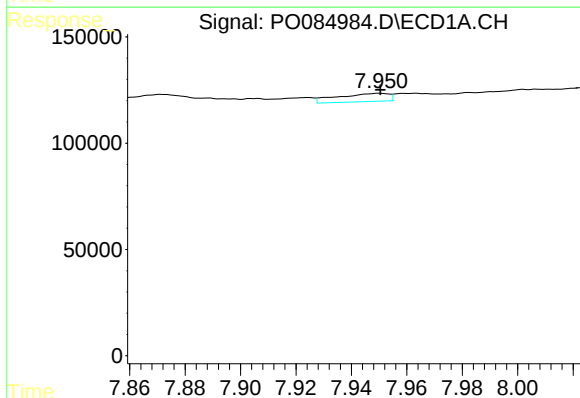


#36 AR-1262-1

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 49537
Conc: 5.48 ng/ml

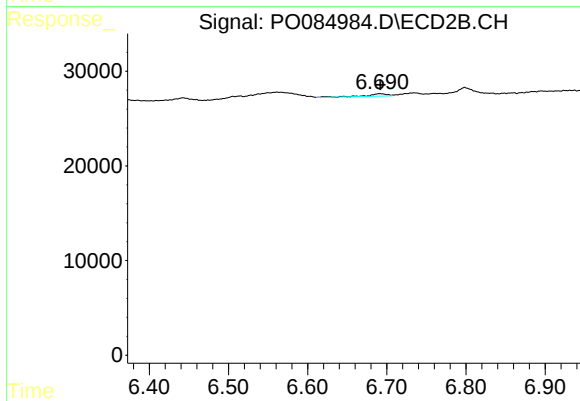

#36 AR-1262-1


R.T.: 6.691 min
Delta R.T.: 0.000 min
Response: 4373
Conc: 3.62 ng/ml

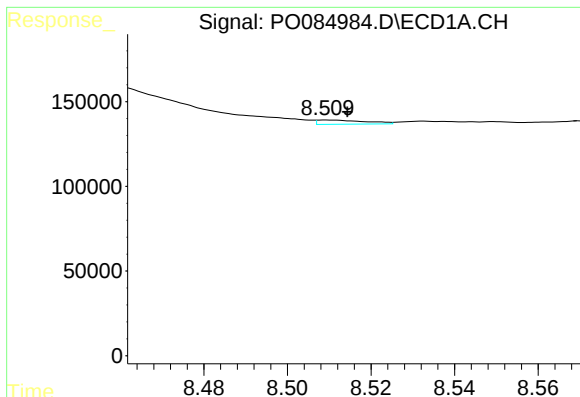

#37 AR-1262-2


R.T.: 8.509 min
Delta R.T.: -0.005 min
Response: 19579
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

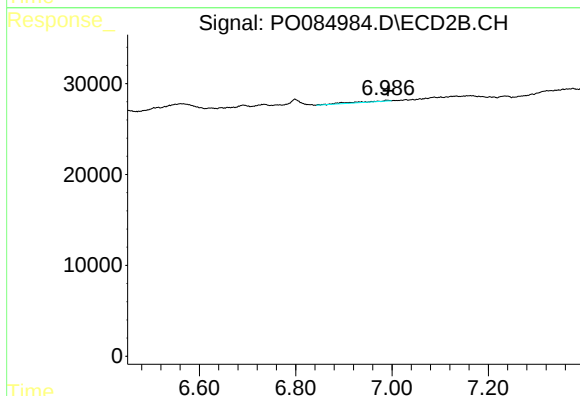


#37 AR-1262-2

R.T.: 6.989 min
Delta R.T.: -0.003 min
Response: 5258
Conc: 2.59 ng/ml

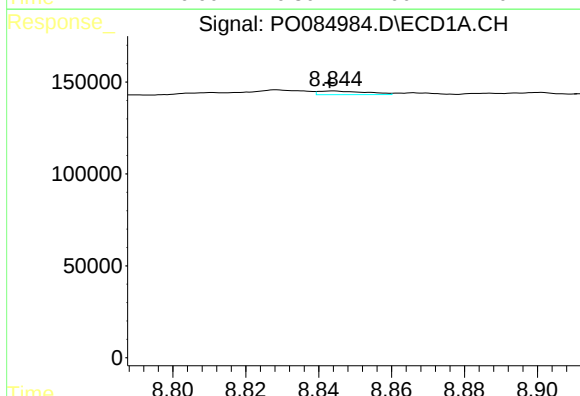


#38 AR-1262-3

R.T.: 8.844 min
Delta R.T.: 0.001 min
Response: 17918
Conc: 1.71 ng/ml

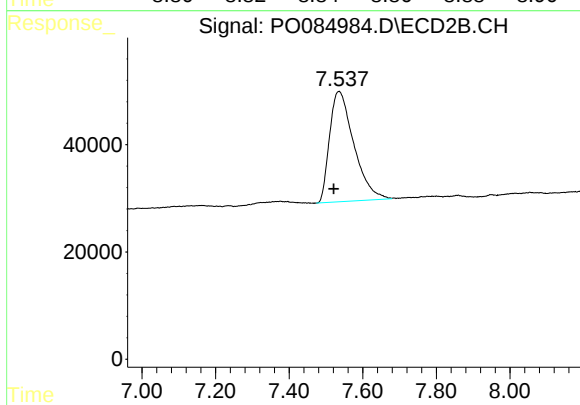

#38 AR-1262-3


R.T.: 7.536 min
Delta R.T.: 0.014 min
Response: 939919
Conc: 604.66 ng/ml

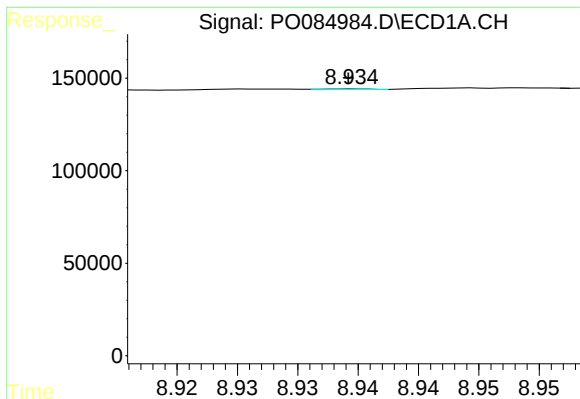

#39 AR-1262-4


R.T.: 8.935 min
Delta R.T.: 0.000 min
Response: 941
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

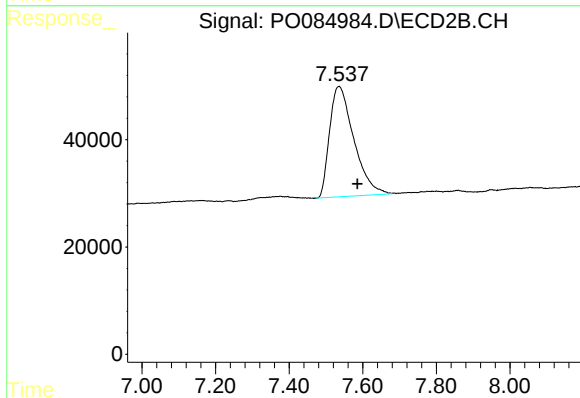


#39 AR-1262-4

R.T.: 7.536 min
Delta R.T.: -0.049 min
Response: 939919
Conc: 331.76 ng/ml

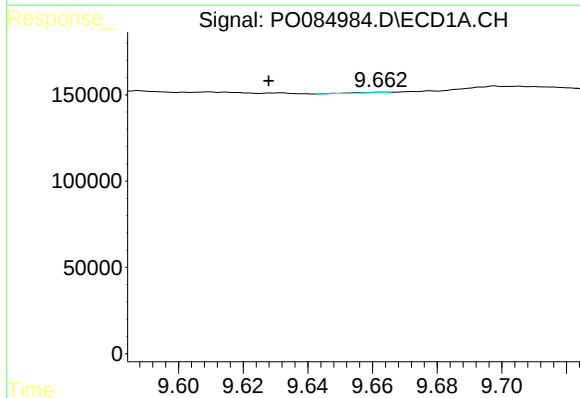


#40 AR-1262-5

R.T.: 9.663 min
Delta R.T.: 0.035 min
Response: 2040
Conc: 0.37 ng/ml

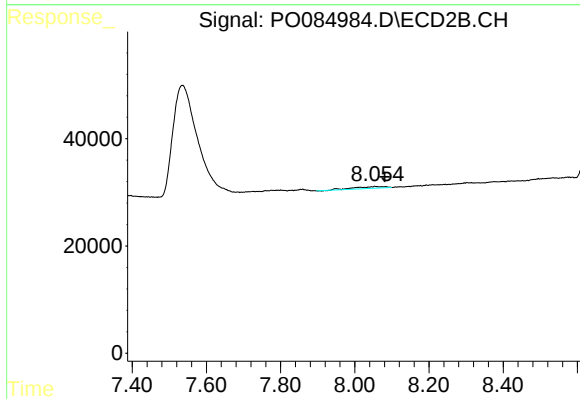

#40 AR-1262-5


R.T.: 8.054 min
Delta R.T.: -0.027 min
Response: 19959
Conc: 15.08 ng/ml

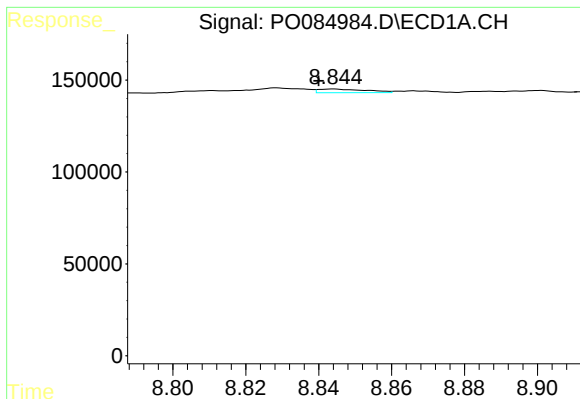

#41 AR-1268-1


R.T.: 8.844 min
Delta R.T.: 0.004 min
Response: 17918
Conc: 0.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

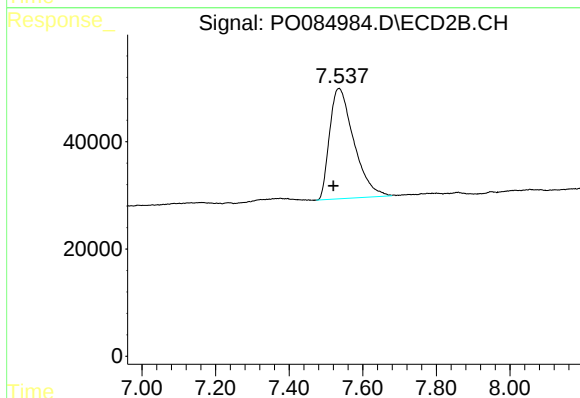


#41 AR-1268-1

R.T.: 7.536 min
Delta R.T.: 0.015 min
Response: 939919
Conc: 137.78 ng/ml

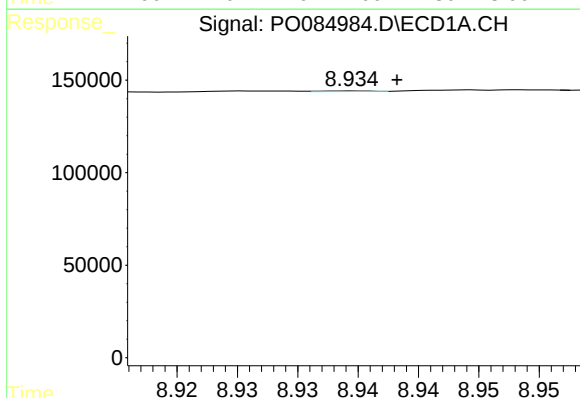


#42 AR-1268-2

R.T.: 8.935 min
Delta R.T.: -0.003 min
Response: 941
Conc: 0.04 ng/ml

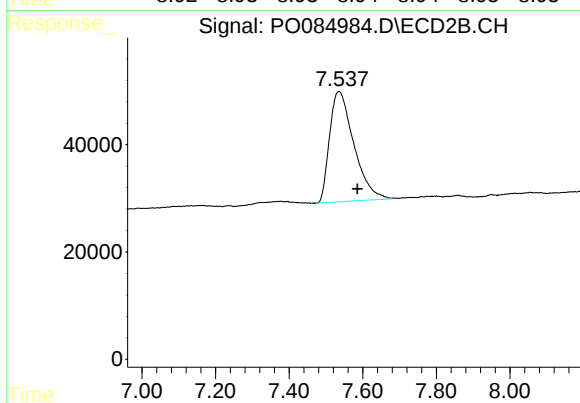

#42 AR-1268-2


R.T.: 7.536 min
Delta R.T.: -0.049 min
Response: 939919
Conc: 155.08 ng/ml

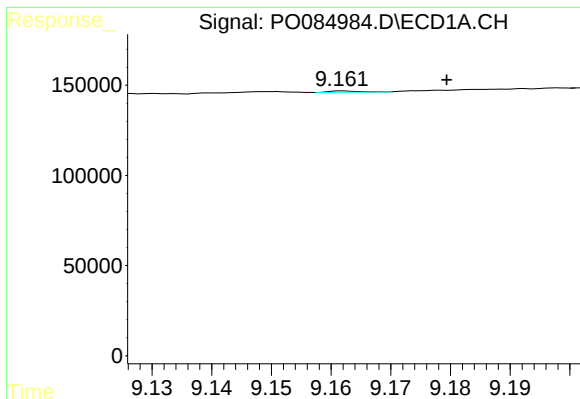

#43 AR-1268-3


R.T.: 9.162 min
Delta R.T.: -0.018 min
Response: 2934
Conc: 0.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

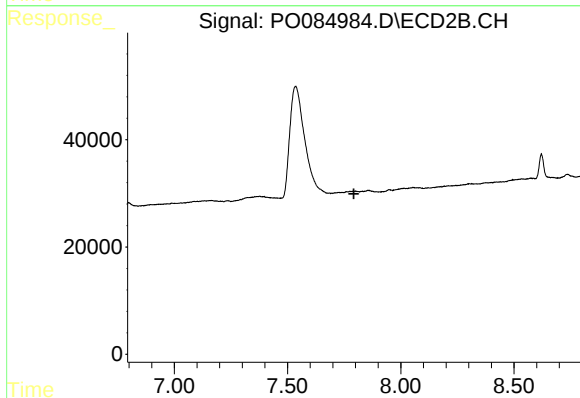


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

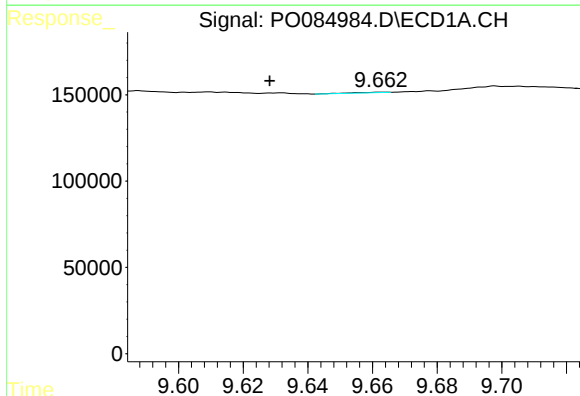


#44 AR-1268-4

R.T.: 9.663 min
Delta R.T.: 0.035 min
Response: 2040
Conc: 0.22 ng/ml

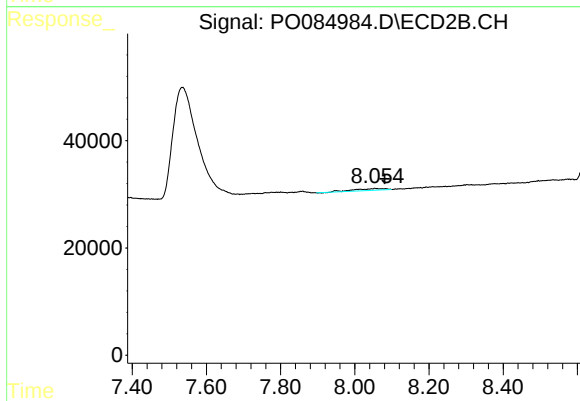

#44 AR-1268-4


R.T.: 8.054 min
Delta R.T.: -0.027 min
Response: 19959
Conc: 8.74 ng/ml

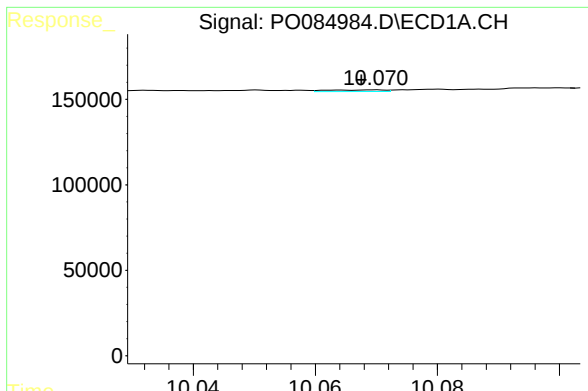

#45 AR-1268-5

R.T.: 10.070 min
Delta R.T.: 0.002 min
Response: 6316
Conc: 0.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-68A

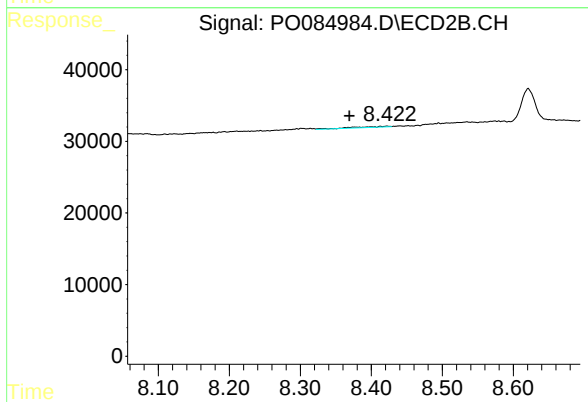

#45 AR-1268-5

R.T.: 8.422 min
Delta R.T.: 0.053 min
Response: 4256
Conc: 0.29 ng/ml