

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0084986.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2022 11:10
 Operator : YP\AJ
 Sample : N1715-05 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-69A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:55:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.509	3.595	290717	72313	1.040	1.608 #
2)	SA Decachlor...	10.432	8.622	257596	55311	1.470	1.505
Target Compounds							
3)	L1 AR-1016-1	5.697	0.000	8885	0	0.949	N.D. #
4)	L1 AR-1016-2	5.728	0.000	20511	0	1.538	N.D. #
5)	L1 AR-1016-3	5.728f	4.897	20511	4428	2.567	3.466 #
6)	L1 AR-1016-4	5.882	4.897	15350	4428	2.285	4.212 #
7)	L1 AR-1016-5	6.182	5.145	46318	7963	7.326	6.009
8)	L2 AR-1221-1	4.718	3.757f	14496	25330	4.531	43.440 #
9)	L2 AR-1221-2	4.813	0.000	9514	0	3.946	N.D. #
10)	L2 AR-1221-3	4.883	0.000	7291	0	1.001	N.D. #
11)	L3 AR-1232-1	4.883	0.000	7291	0	1.191	N.D. #
12)	L3 AR-1232-2	5.427	0.000	7310	0	2.457	N.D. #
13)	L3 AR-1232-3	5.728	4.897	20511	4428	3.617	8.153 #
14)	L3 AR-1232-4	5.882	4.897f	15350	4428	5.375	8.727 #
15)	L3 AR-1232-5	5.978	5.145	4075	7963	1.804	14.359 #
16)	L4 AR-1242-1	5.697	0.000	8885	0	1.197	N.D. #
17)	L4 AR-1242-2	5.728	0.000	20511	0	1.936	N.D. #
18)	L4 AR-1242-3	5.728f	4.897	20511	4428	3.191	4.325 #
19)	L4 AR-1242-4	5.882	4.897f	15350	4428	2.831	4.250 #
20)	L4 AR-1242-5	6.659	5.515	124047	307479	23.585	248.096 #
21)	L5 AR-1248-1	5.697	0.000	8885	0	1.638	N.D. #
22)	L5 AR-1248-2	5.978	4.897	4075	4428	0.530	3.077 #
23)	L5 AR-1248-3	6.182	4.897f	46318	4428	5.390	2.950 #
24)	L5 AR-1248-4	6.602	5.145	58285	7963	6.256	4.584 #
25)	L5 AR-1248-5	6.659	5.515	124047	307479	13.874	183.343 #
26)	L6 AR-1254-1	6.567	5.515	1390858	307479	141.802	114.937
27)	L6 AR-1254-2	6.791	5.687f	9514	13497	0.641	5.722 #
28)	L6 AR-1254-3	7.161	6.043	319694	12078	21.114	3.213 #
29)	L6 AR-1254-4	7.449	6.273	57100	1485	5.324	0.634 #
30)	L6 AR-1254-5	7.875	0.000	45490	0	3.863	N.D. #
31)	L7 AR-1260-1	7.328	6.174	140415	7260	12.305	2.925 #
32)	L7 AR-1260-2	7.583	6.379	45706	5956	3.555	2.012 #
33)	L7 AR-1260-3	7.950	6.562f	16617	3881	2.081	1.419 #
34)	L7 AR-1260-4	8.187	0.000	16995	0	1.787	N.D. #
35)	L7 AR-1260-5	8.521	0.000	18899	0	1.028	N.D. #
36)	L8 AR-1262-1	7.950	0.000	16617	0	1.838	N.D. #
37)	L8 AR-1262-2	8.521	0.000	18899	0	1.185	N.D. #
38)	L8 AR-1262-3	8.831	7.537	41839	429688	3.990	276.421 #
39)	L8 AR-1262-4	8.970f	7.537f	-308	429688	N.D.	151.665 #
40)	L8 AR-1262-5	9.563f	8.031f	14892	259	2.723	0.196 #
41)	L9 AR-1268-1	8.831	7.537	41839	429688	1.498	62.988 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
Data File : P0084986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2022 11:10
Operator : YP\AJ
Sample : N1715-05 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:55:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.970	7.537f	-308	429688	N.D.	70.897 #
43)	L9 AR-1268-3	9.180	7.729f	7741	74	0.362	0.015 #
44)	L9 AR-1268-4	9.563f	8.031f	14892	259	1.623	0.114 #
45)	L9 AR-1268-5	10.066	0.000	7843	0	0.112	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO084986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2022 11:10
Operator : YP\AJ
Sample : N1715-05 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:55:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

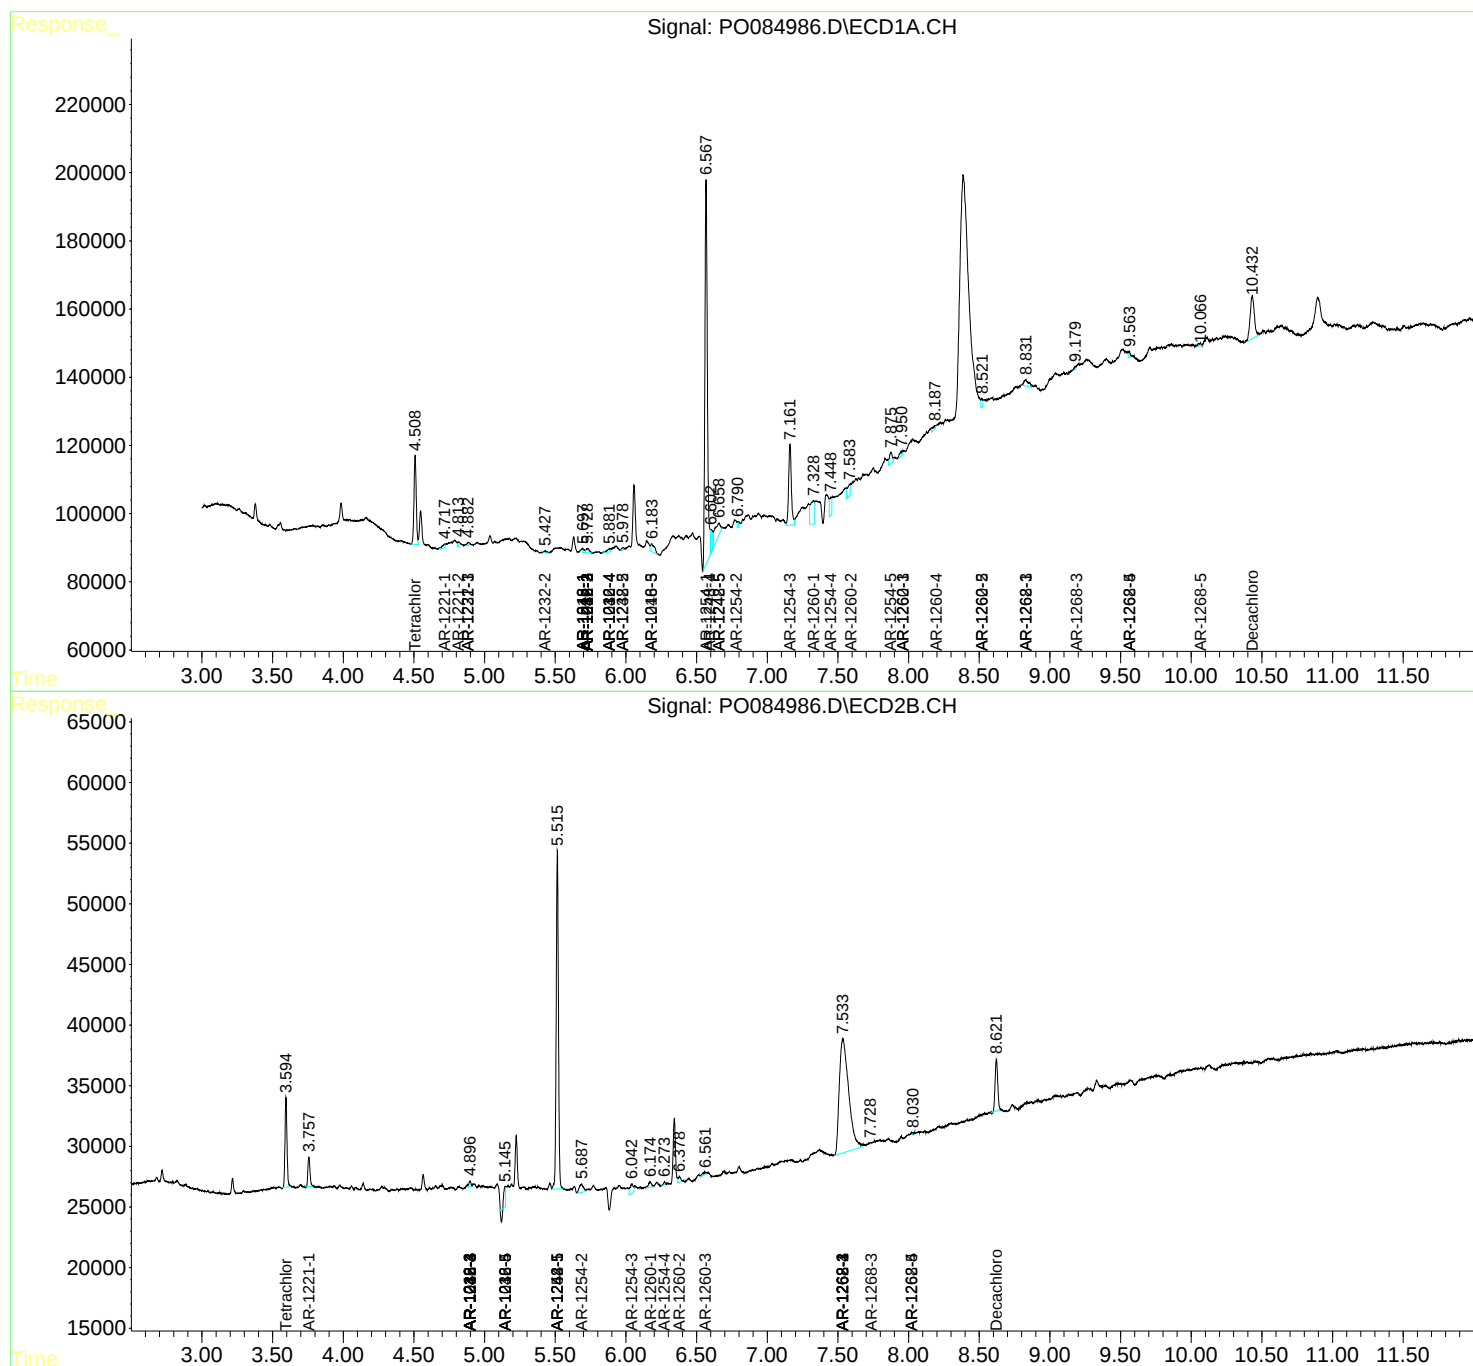


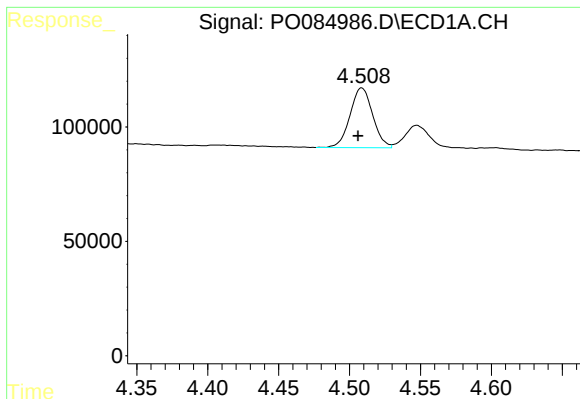

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 290717
Conc: 1.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

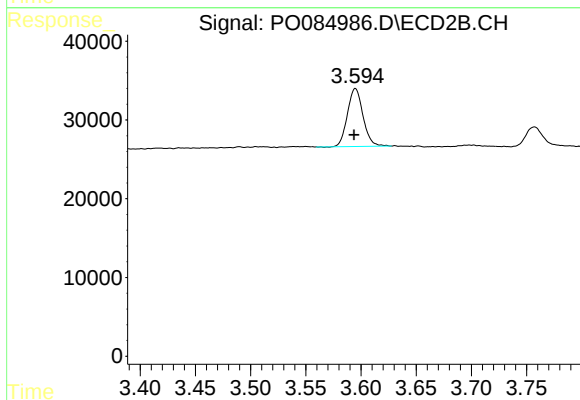


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.001 min
Response: 72313
Conc: 1.61 ng/ml

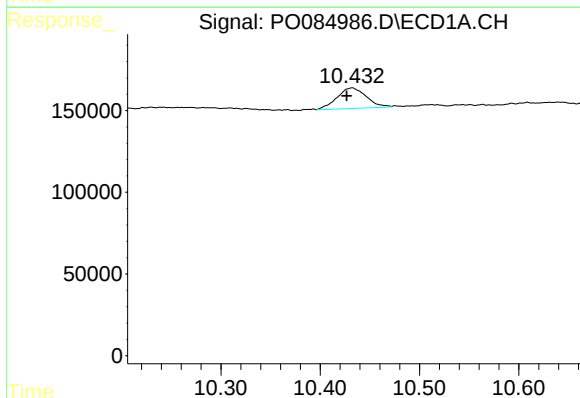


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.006 min
Response: 257596
Conc: 1.47 ng/ml

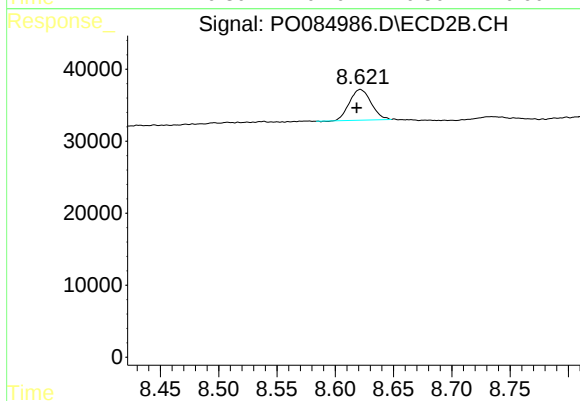

#2 Decachlorobiphenyl


R.T.: 8.622 min
Delta R.T.: 0.003 min
Response: 55311
Conc: 1.51 ng/ml

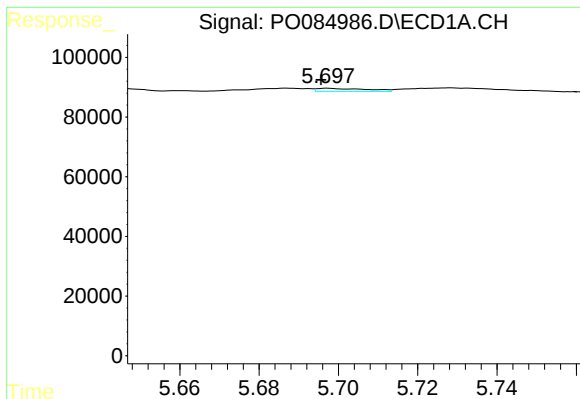

#3 AR-1016-1


R.T.: 5.697 min
Delta R.T.: 0.002 min
Response: 8885
Conc: 0.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

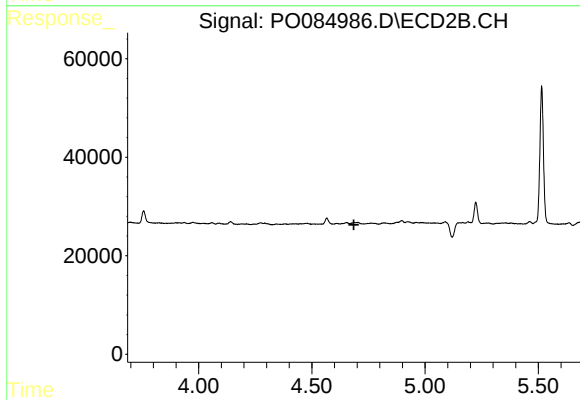


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

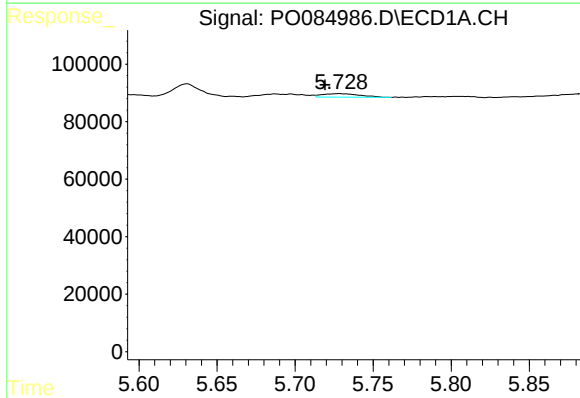


#4 AR-1016-2

R.T.: 5.728 min
Delta R.T.: 0.009 min
Response: 20511
Conc: 1.54 ng/ml

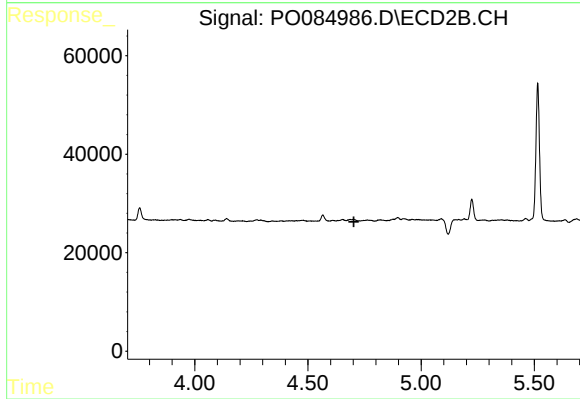

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

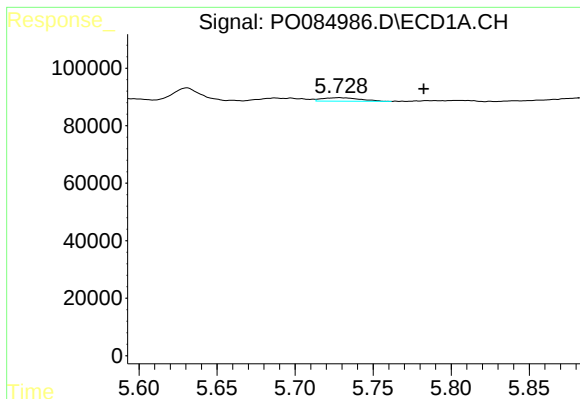

#5 AR-1016-3


R.T.: 5.728 min
Delta R.T.: -0.054 min
Response: 20511
Conc: 2.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

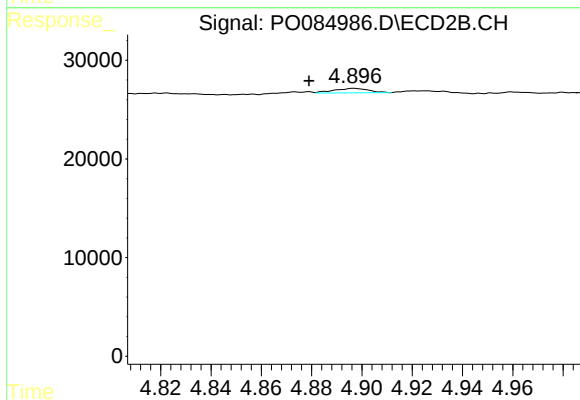


#5 AR-1016-3

R.T.: 4.897 min
Delta R.T.: 0.018 min
Response: 4428
Conc: 3.47 ng/ml

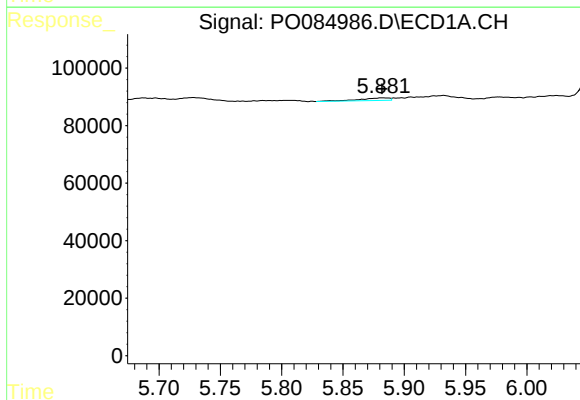


#6 AR-1016-4

R.T.: 5.882 min
Delta R.T.: 0.000 min
Response: 15350
Conc: 2.29 ng/ml

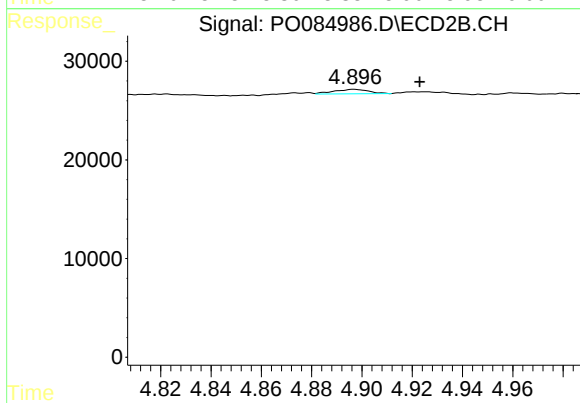

#6 AR-1016-4


R.T.: 4.897 min
Delta R.T.: -0.026 min
Response: 4428
Conc: 4.21 ng/ml

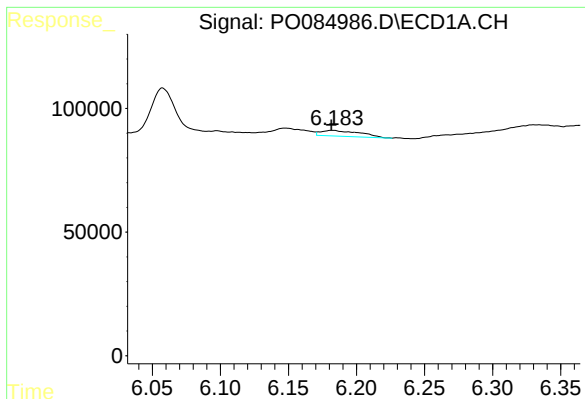

#7 AR-1016-5


R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 46318
Conc: 7.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

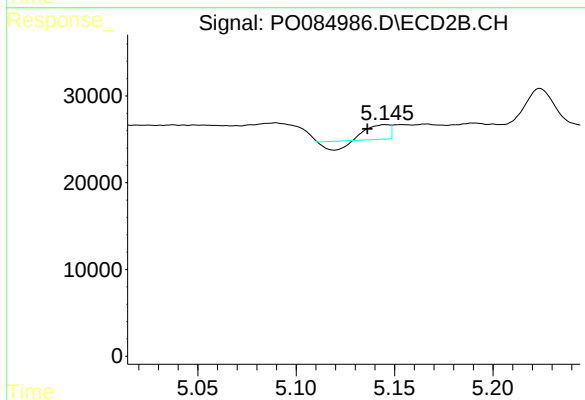


#7 AR-1016-5

R.T.: 5.145 min
Delta R.T.: 0.009 min
Response: 7963
Conc: 6.01 ng/ml

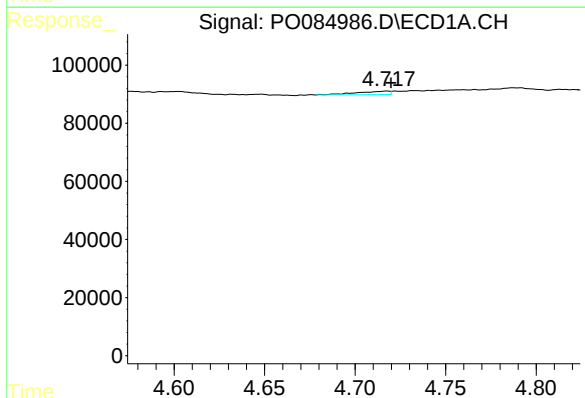


#8 AR-1221-1

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 14496
Conc: 4.53 ng/ml

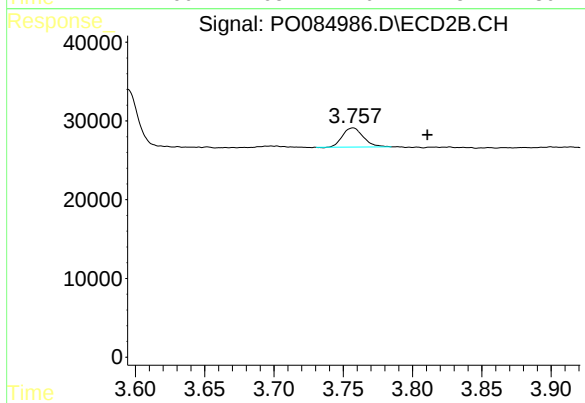

#8 AR-1221-1


R.T.: 3.757 min
Delta R.T.: -0.054 min
Response: 25330
Conc: 43.44 ng/ml

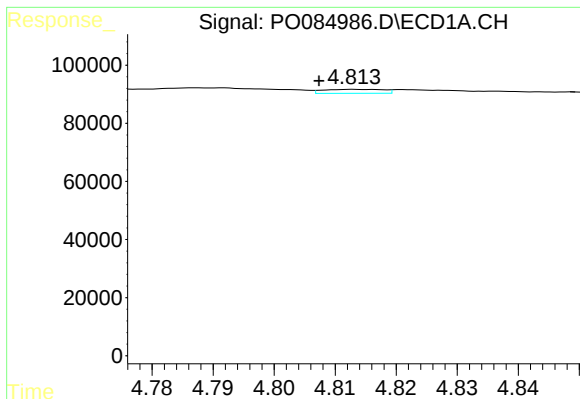

#9 AR-1221-2


R.T.: 4.813 min
Delta R.T.: 0.006 min
Response: 9514
Conc: 3.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

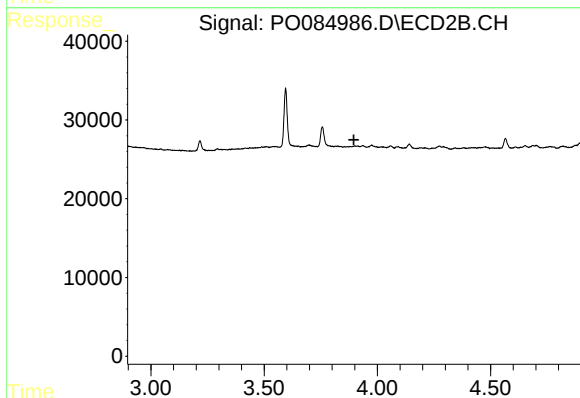


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

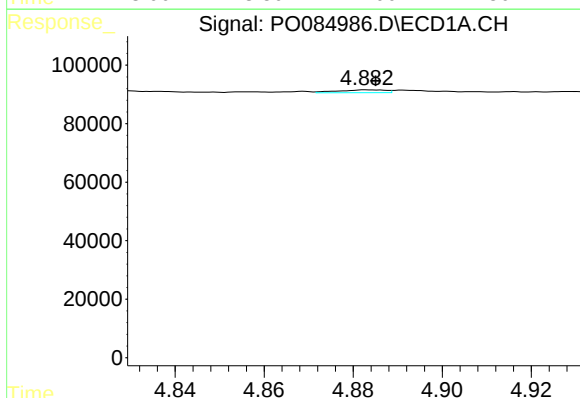


#10 AR-1221-3

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 7291
Conc: 1.00 ng/ml

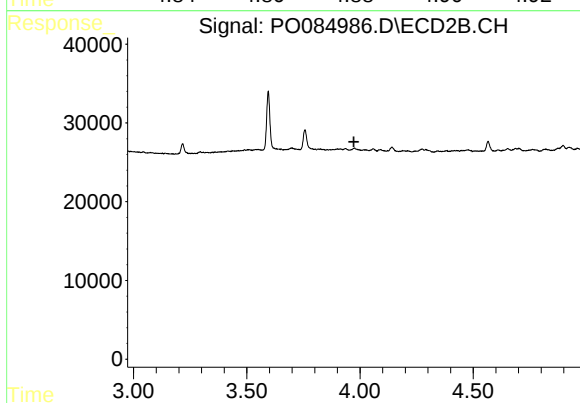

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.973 min
Response: 0
Conc: N.D.

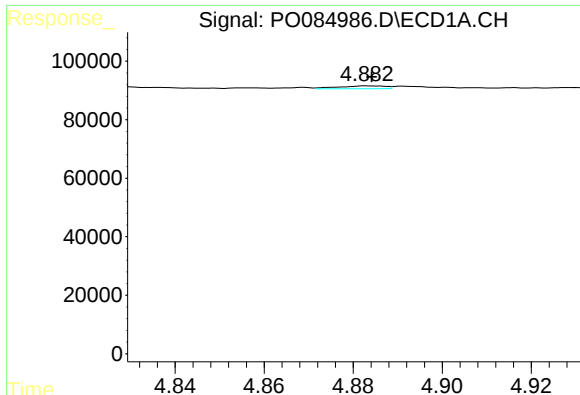

#11 AR-1232-1


R.T.: 4.883 min
Delta R.T.: -0.001 min
Response: 7291
Conc: 1.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

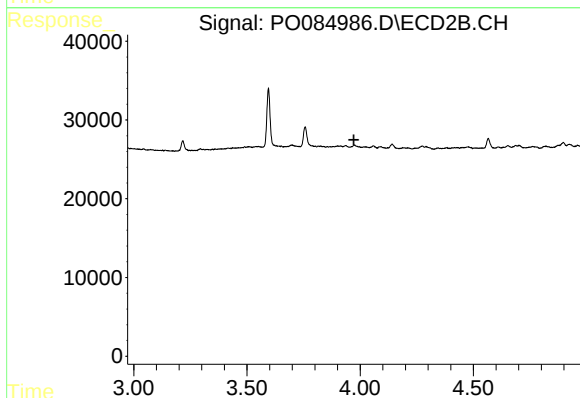


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

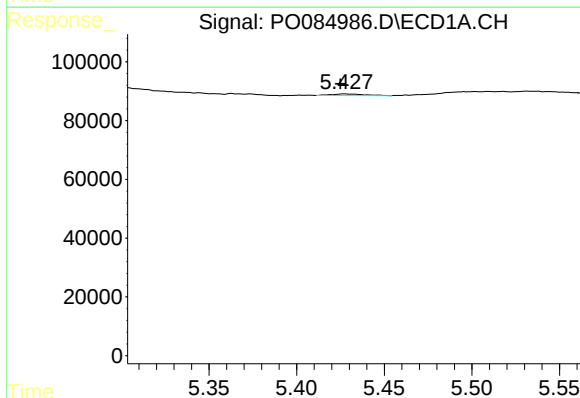


#12 AR-1232-2

R.T.: 5.427 min
Delta R.T.: 0.002 min
Response: 7310
Conc: 2.46 ng/ml

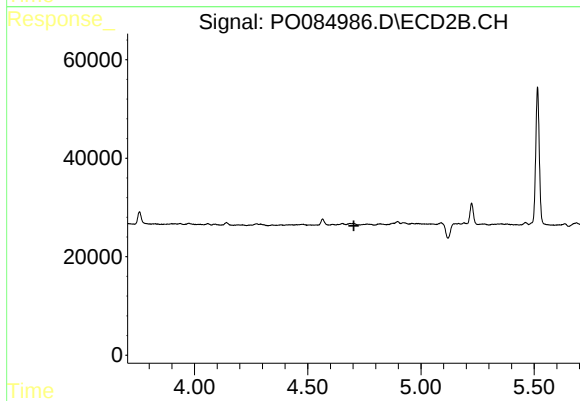

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

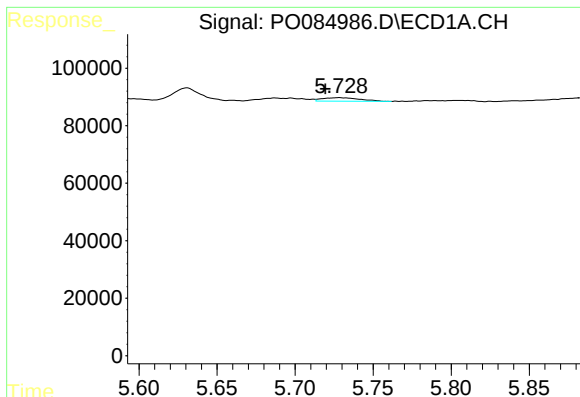

#13 AR-1232-3


R.T.: 5.728 min
Delta R.T.: 0.009 min
Response: 20511
Conc: 3.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

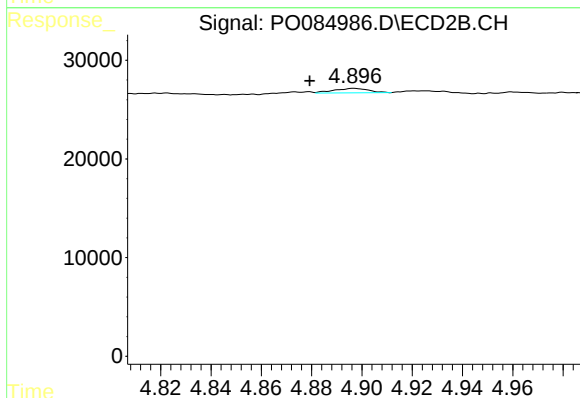


#13 AR-1232-3

R.T.: 4.897 min
Delta R.T.: 0.017 min
Response: 4428
Conc: 8.15 ng/ml

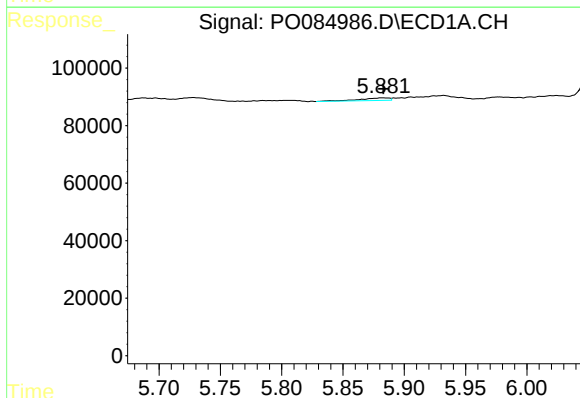


#14 AR-1232-4

R.T.: 5.882 min
Delta R.T.: -0.001 min
Response: 15350
Conc: 5.37 ng/ml

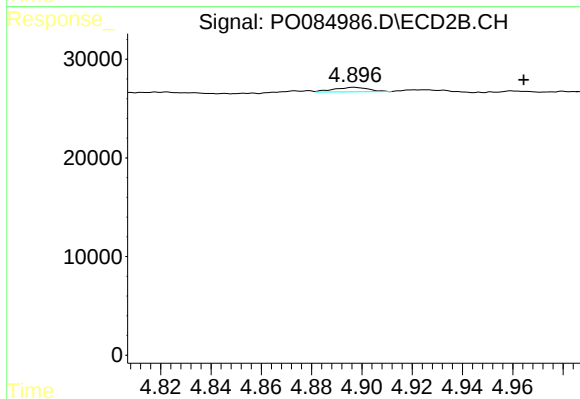

#14 AR-1232-4


R.T.: 4.897 min
Delta R.T.: -0.068 min
Response: 4428
Conc: 8.73 ng/ml

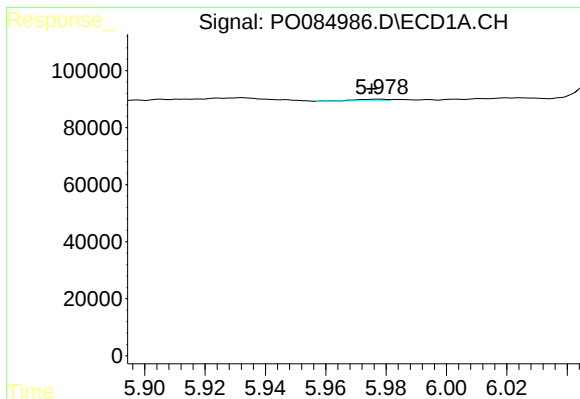

#15 AR-1232-5


R.T.: 5.978 min
Delta R.T.: 0.002 min
Response: 4075
Conc: 1.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

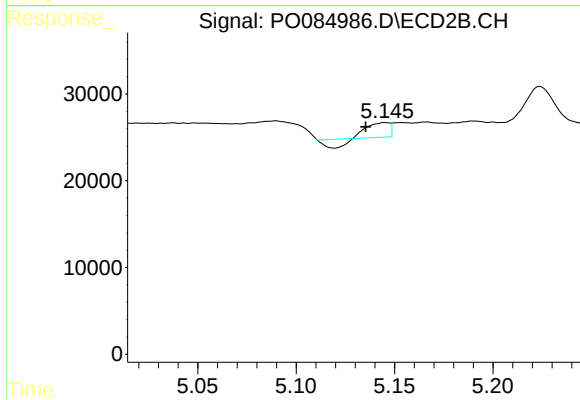


#15 AR-1232-5

R.T.: 5.145 min
Delta R.T.: 0.010 min
Response: 7963
Conc: 14.36 ng/ml

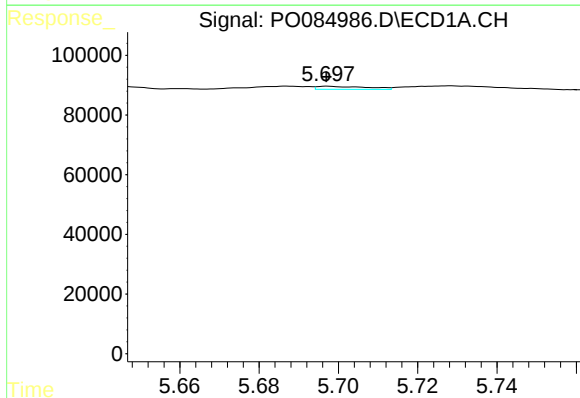


#16 AR-1242-1

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 8885
Conc: 1.20 ng/ml

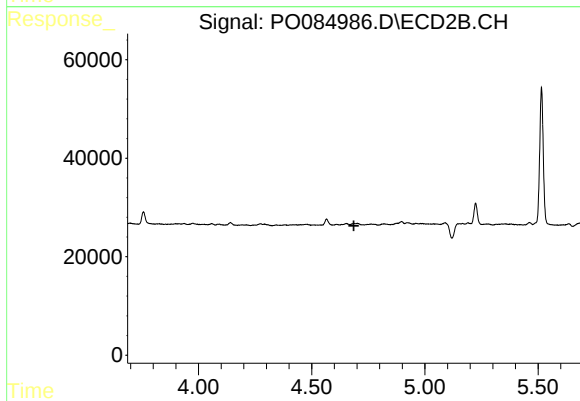

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

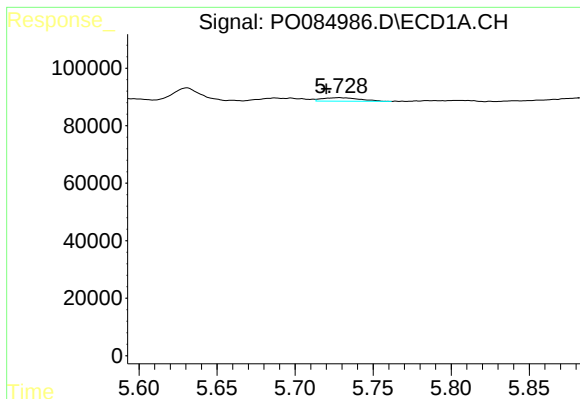

#17 AR-1242-2


R.T.: 5.728 min
Delta R.T.: 0.008 min
Response: 20511
Conc: 1.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

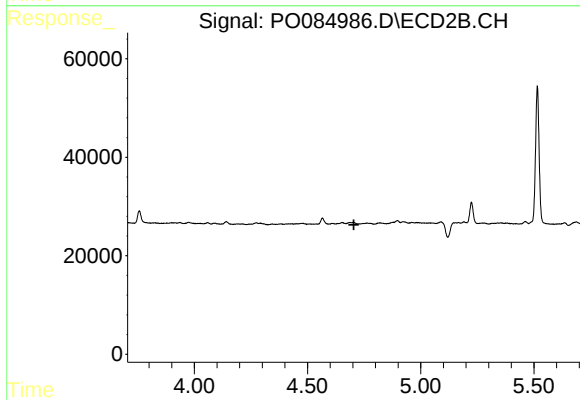


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.705 min
Response: 0
Conc: N.D.

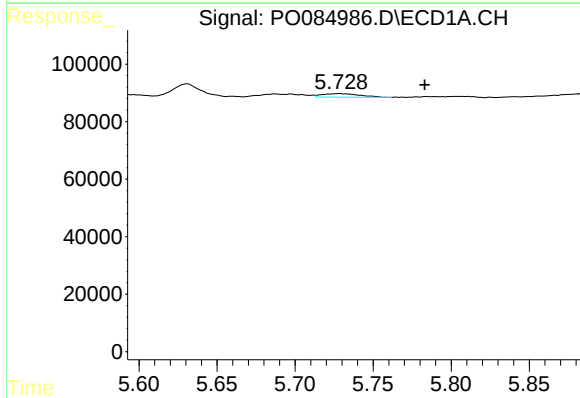


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: -0.055 min
Response: 20511
Conc: 3.19 ng/ml

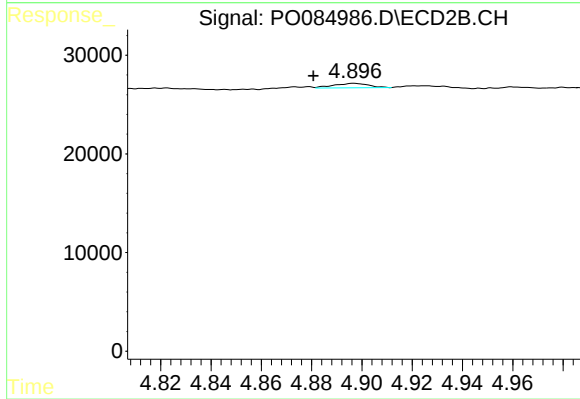

#18 AR-1242-3


R.T.: 4.897 min
Delta R.T.: 0.016 min
Response: 4428
Conc: 4.33 ng/ml

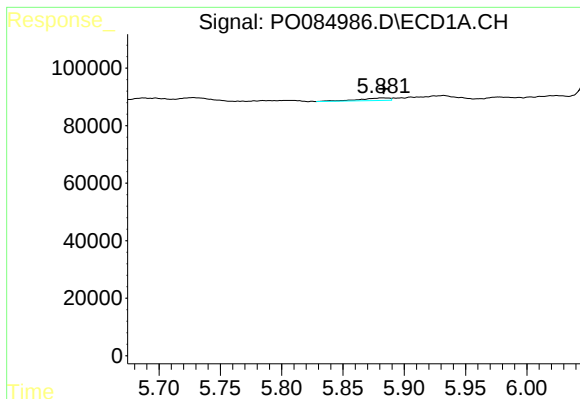

#19 AR-1242-4


R.T.: 5.882 min
Delta R.T.: -0.001 min
Response: 15350
Conc: 2.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

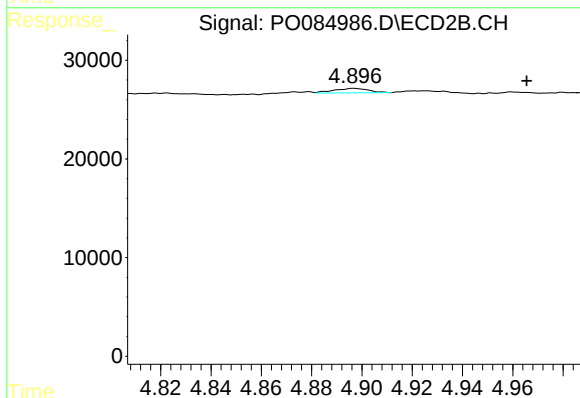


#19 AR-1242-4

R.T.: 4.897 min
Delta R.T.: -0.069 min
Response: 4428
Conc: 4.25 ng/ml

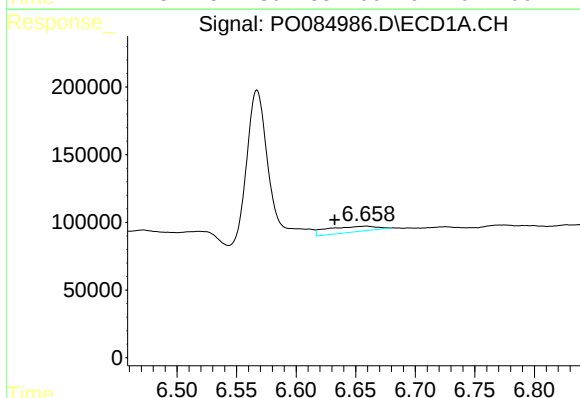


#20 AR-1242-5

R.T.: 6.659 min
Delta R.T.: 0.027 min
Response: 124047
Conc: 23.58 ng/ml

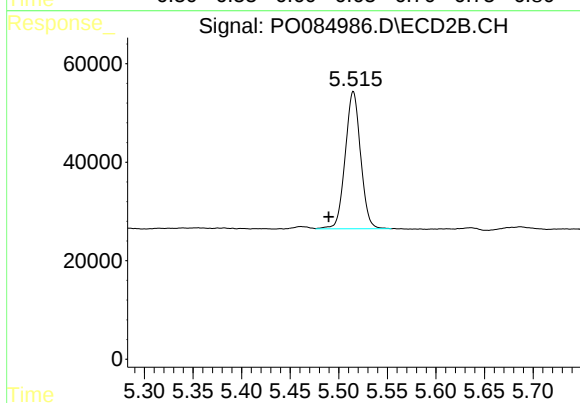

#20 AR-1242-5


R.T.: 5.515 min
Delta R.T.: 0.025 min
Response: 307479
Conc: 248.10 ng/ml

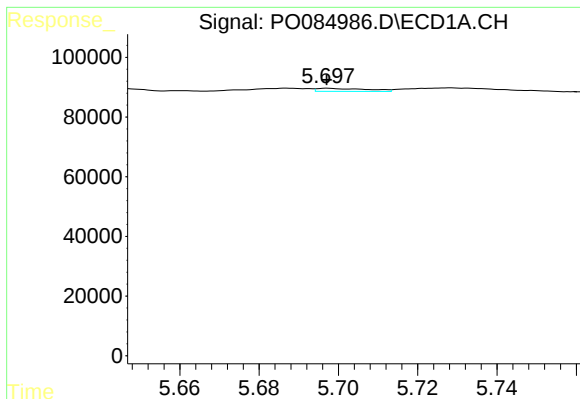

#21 AR-1248-1


R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 8885
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

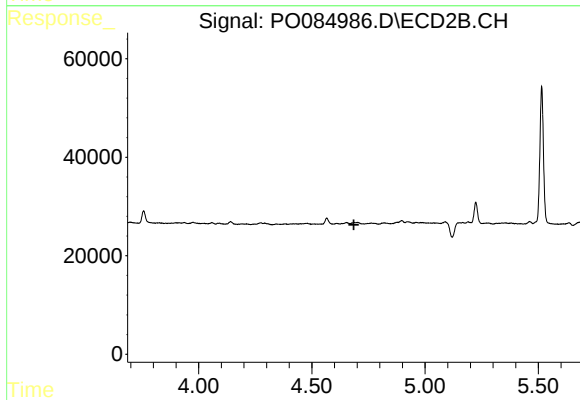


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

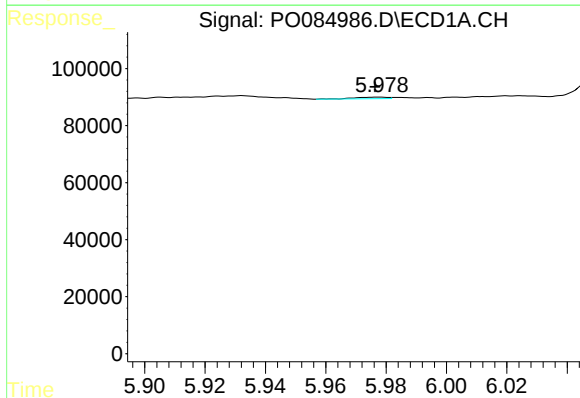


#22 AR-1248-2

R.T.: 5.978 min
Delta R.T.: 0.001 min
Response: 4075
Conc: 0.53 ng/ml

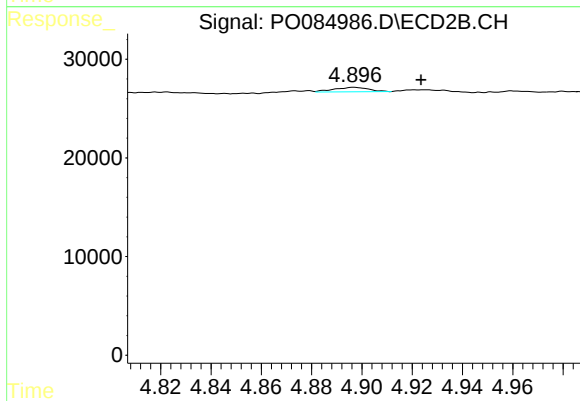

#22 AR-1248-2


R.T.: 4.897 min
Delta R.T.: -0.027 min
Response: 4428
Conc: 3.08 ng/ml

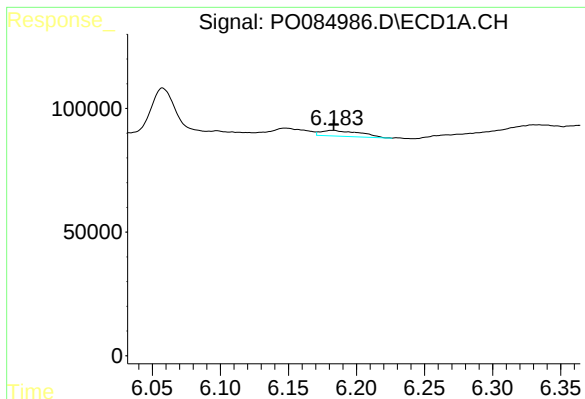

#23 AR-1248-3


R.T.: 6.182 min
Delta R.T.: -0.002 min
Response: 46318
Conc: 5.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

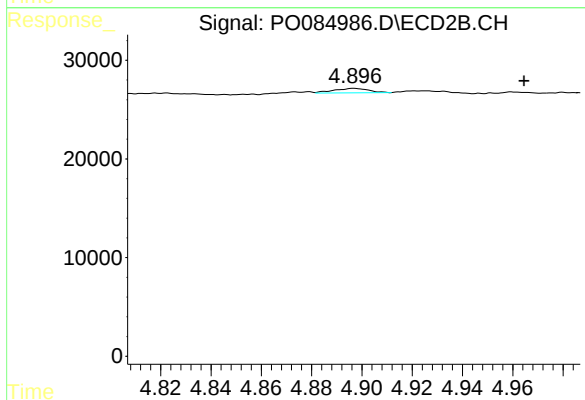


#23 AR-1248-3

R.T.: 4.897 min
Delta R.T.: -0.068 min
Response: 4428
Conc: 2.95 ng/ml

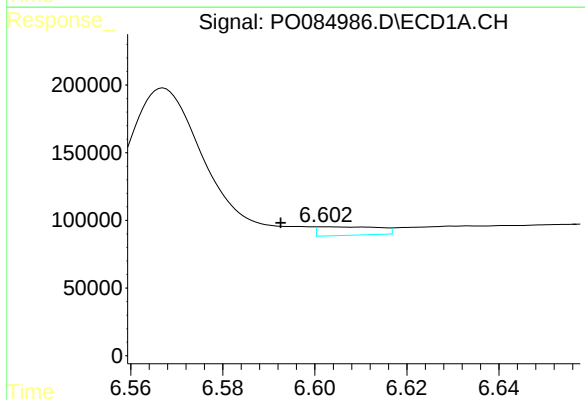


#24 AR-1248-4

R.T.: 6.602 min
Delta R.T.: 0.010 min
Response: 58285
Conc: 6.26 ng/ml

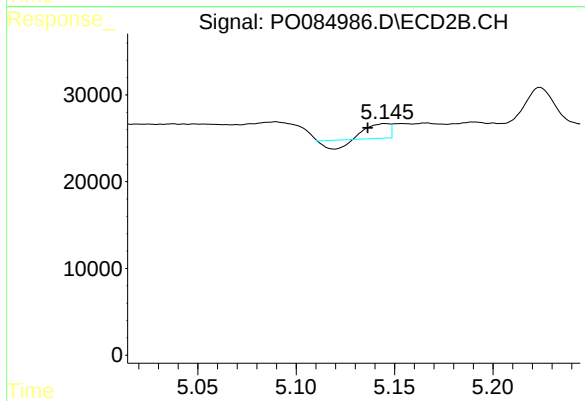

#24 AR-1248-4


R.T.: 5.145 min
Delta R.T.: 0.009 min
Response: 7963
Conc: 4.58 ng/ml

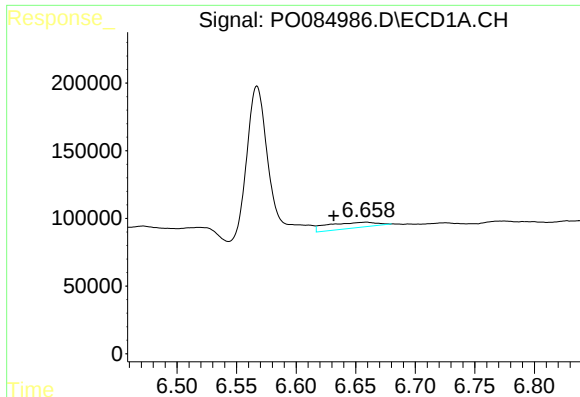

#25 AR-1248-5


R.T.: 6.659 min
Delta R.T.: 0.027 min
Response: 124047
Conc: 13.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

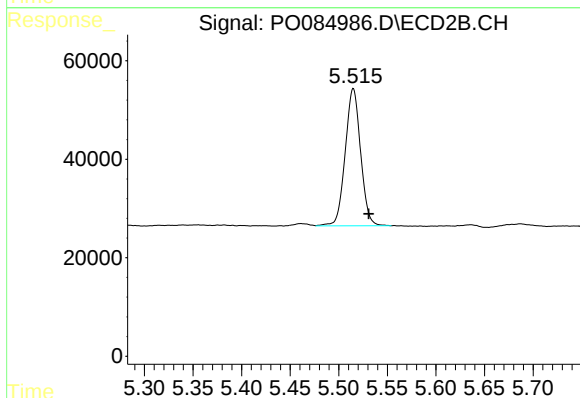


#25 AR-1248-5

R.T.: 5.515 min
Delta R.T.: -0.016 min
Response: 307479
Conc: 183.34 ng/ml

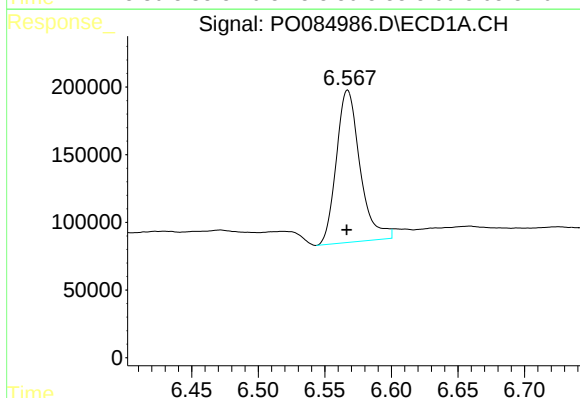


#26 AR-1254-1

R.T.: 6.567 min
Delta R.T.: 0.000 min
Response: 1390858
Conc: 141.80 ng/ml

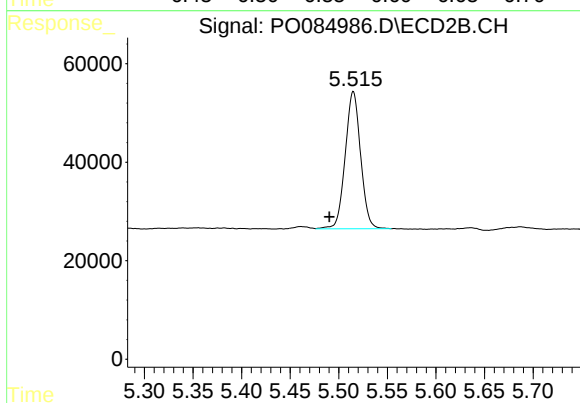

#26 AR-1254-1


R.T.: 5.515 min
Delta R.T.: 0.025 min
Response: 307479
Conc: 114.94 ng/ml

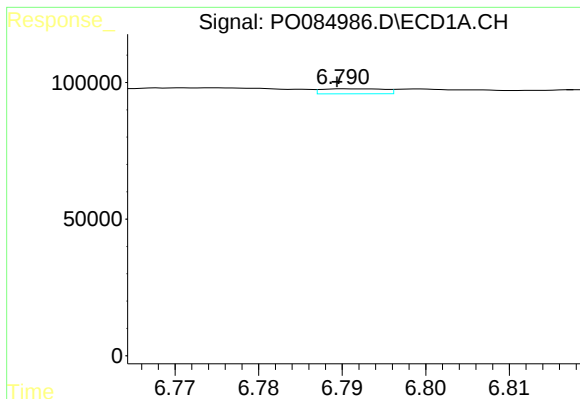

#27 AR-1254-2


R.T.: 6.791 min
Delta R.T.: 0.001 min
Response: 9514
Conc: 0.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

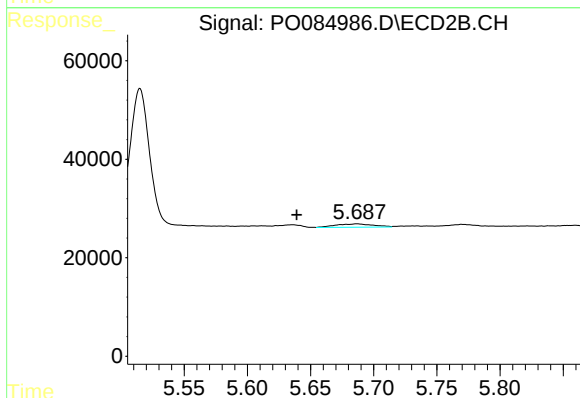


#27 AR-1254-2

R.T.: 5.687 min
Delta R.T.: 0.048 min
Response: 13497
Conc: 5.72 ng/ml

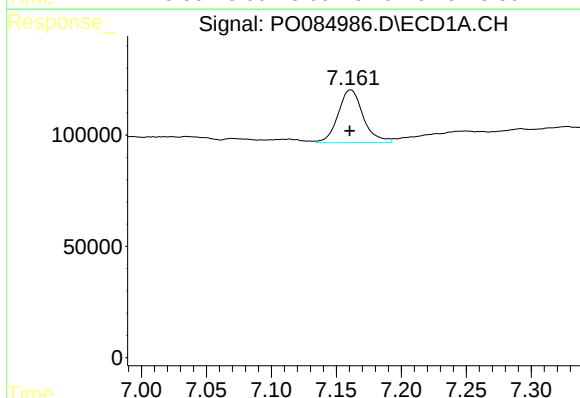


#28 AR-1254-3

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 319694
Conc: 21.11 ng/ml

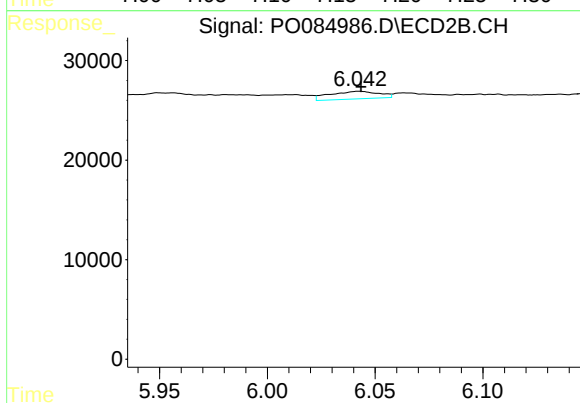

#28 AR-1254-3


R.T.: 6.043 min
Delta R.T.: 0.000 min
Response: 12078
Conc: 3.21 ng/ml

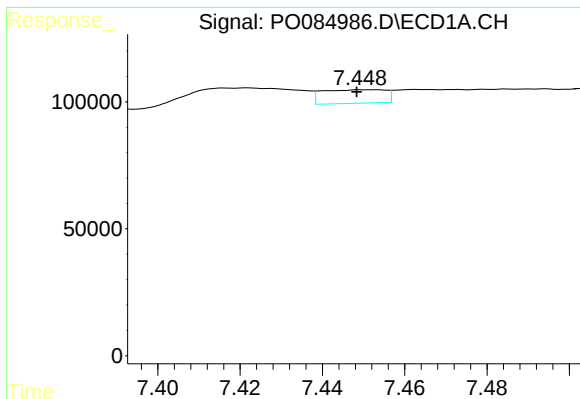

#29 AR-1254-4


R.T.: 7.449 min
Delta R.T.: 0.000 min
Response: 57100
Conc: 5.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

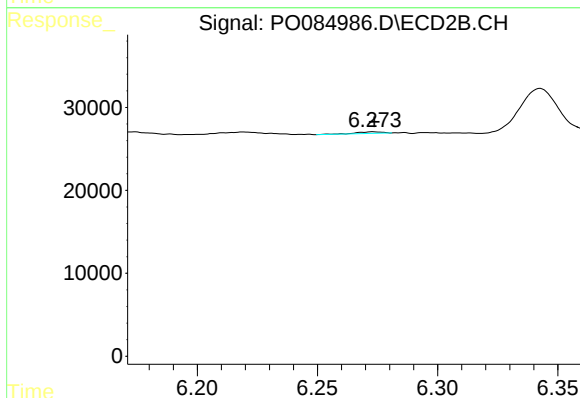


#29 AR-1254-4

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 1485
Conc: 0.63 ng/ml

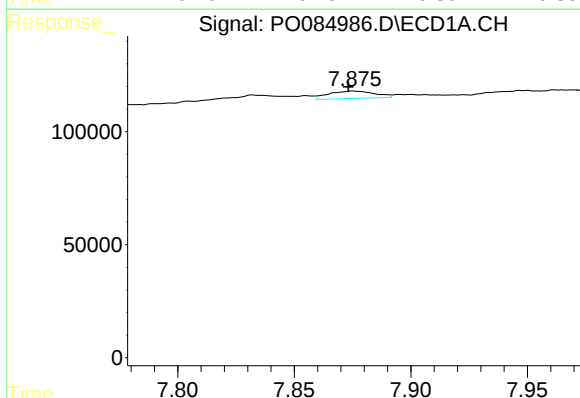


#30 AR-1254-5

R.T.: 7.875 min
Delta R.T.: 0.002 min
Response: 45490
Conc: 3.86 ng/ml

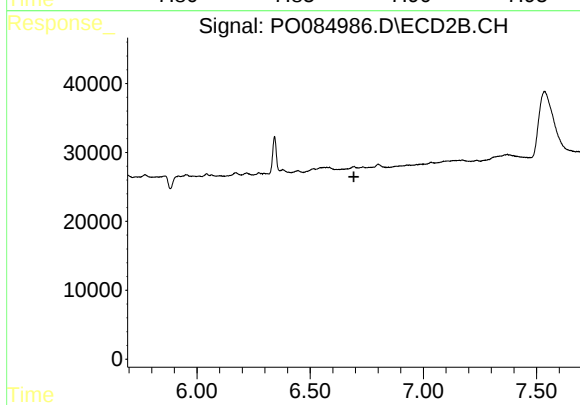

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

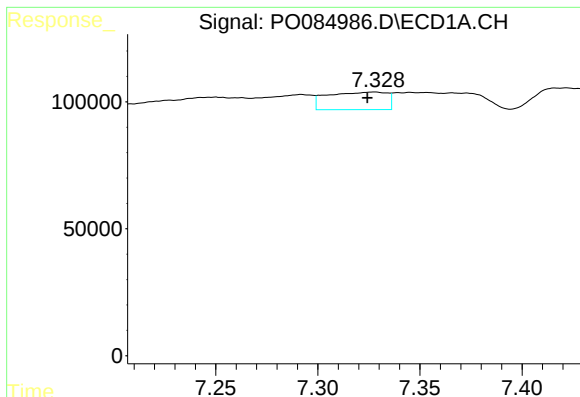

#31 AR-1260-1


R.T.: 7.328 min
Delta R.T.: 0.004 min
Response: 140415
Conc: 12.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

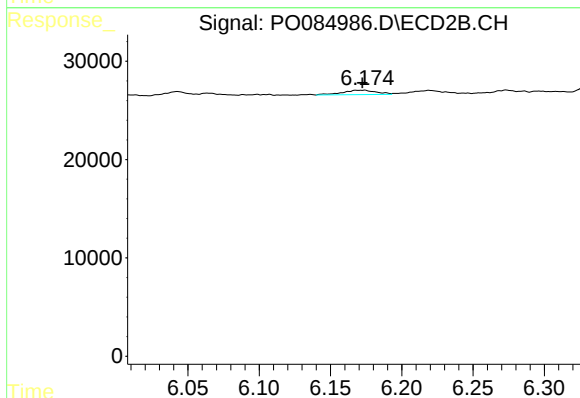


#31 AR-1260-1

R.T.: 6.174 min
Delta R.T.: 0.002 min
Response: 7260
Conc: 2.93 ng/ml

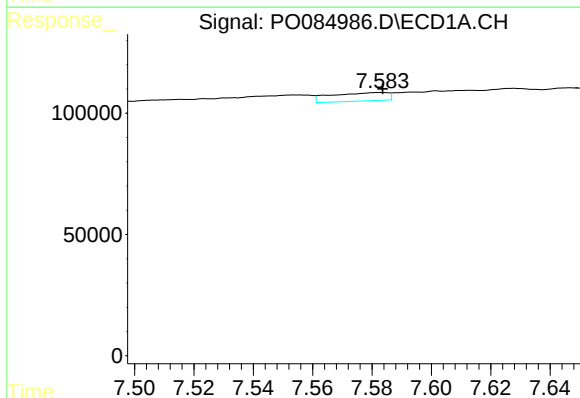


#32 AR-1260-2

R.T.: 7.583 min
Delta R.T.: 0.000 min
Response: 45706
Conc: 3.55 ng/ml

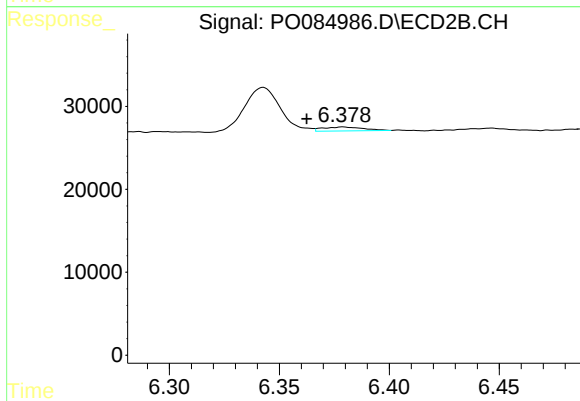

#32 AR-1260-2


R.T.: 6.379 min
Delta R.T.: 0.016 min
Response: 5956
Conc: 2.01 ng/ml

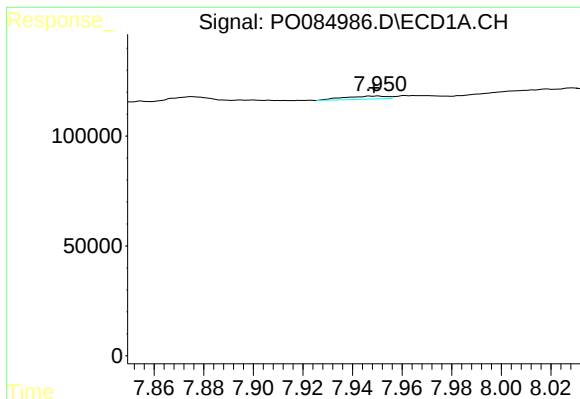

#33 AR-1260-3


R.T.: 7.950 min
Delta R.T.: 0.001 min
Response: 16617
Conc: 2.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

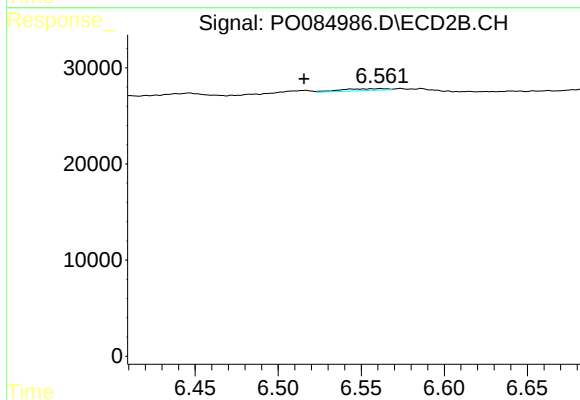


#33 AR-1260-3

R.T.: 6.562 min
Delta R.T.: 0.046 min
Response: 3881
Conc: 1.42 ng/ml

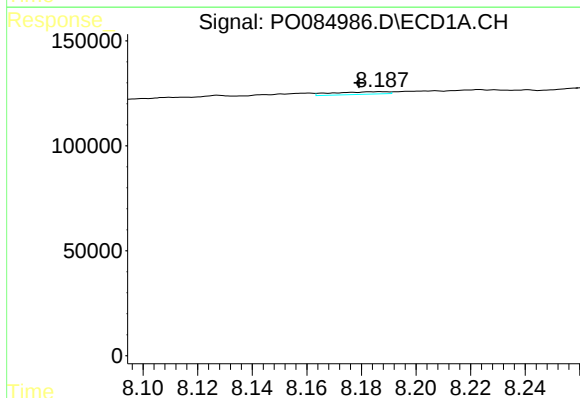


#34 AR-1260-4

R.T.: 8.187 min
Delta R.T.: 0.008 min
Response: 16995
Conc: 1.79 ng/ml

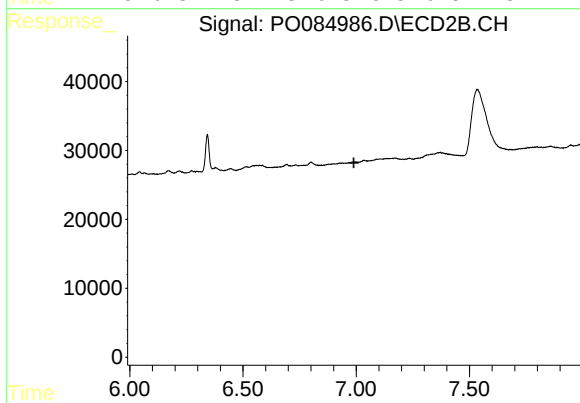

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.

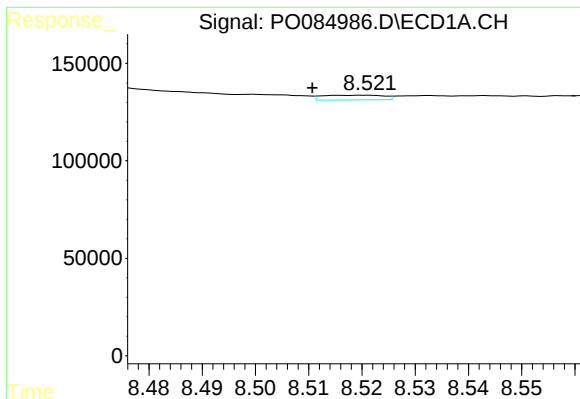

#35 AR-1260-5


R.T.: 8.521 min
Delta R.T.: 0.010 min
Response: 18899
Conc: 1.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

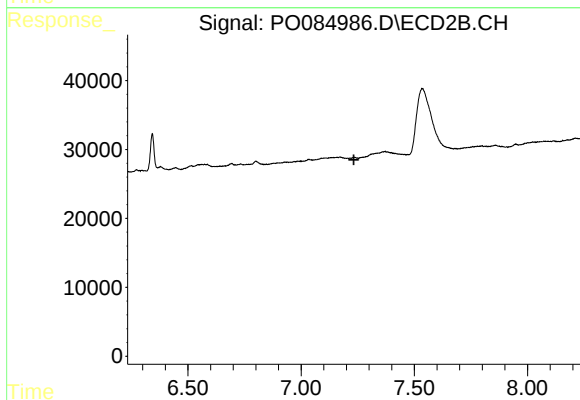


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.233 min
Response: 0
Conc: N.D.

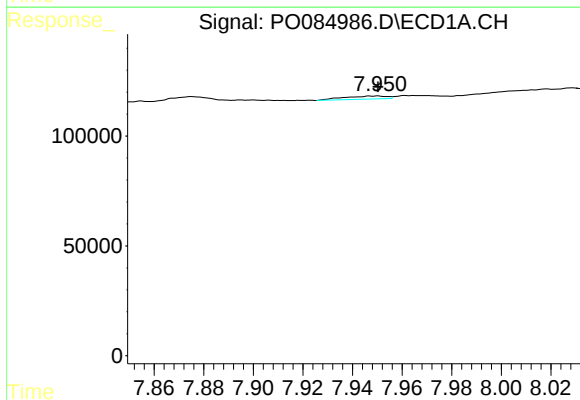


#36 AR-1262-1

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 16617
Conc: 1.84 ng/ml

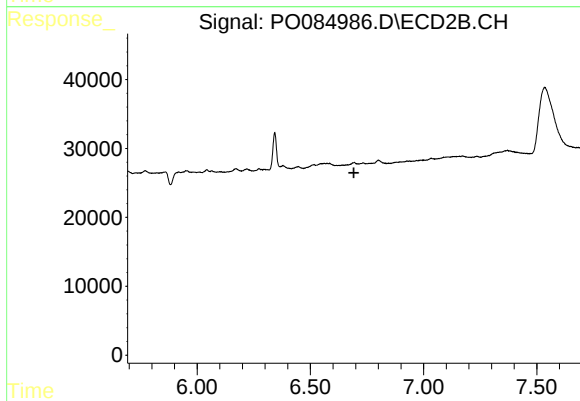

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.692 min
Response: 0
Conc: N.D.

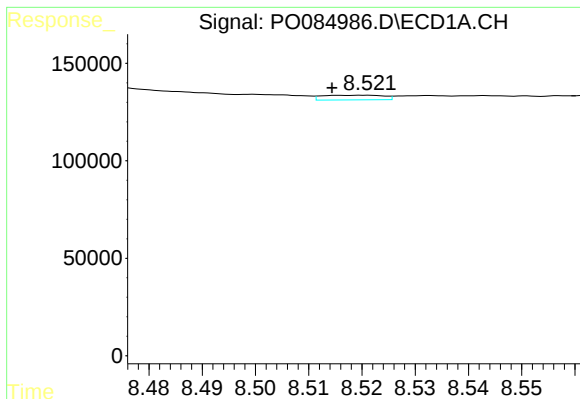

#37 AR-1262-2


R.T.: 8.521 min
Delta R.T.: 0.006 min
Response: 18899
Conc: 1.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

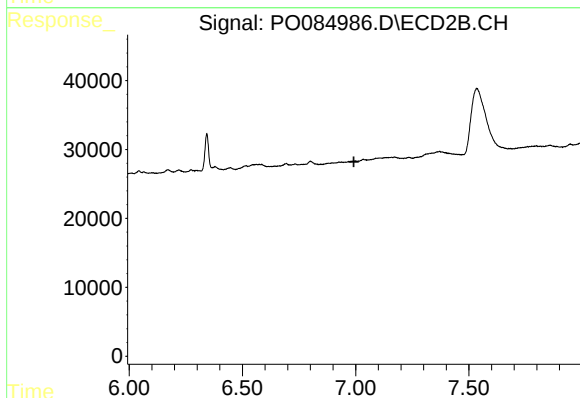


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 6.992 min
Response: 0
Conc: N.D.

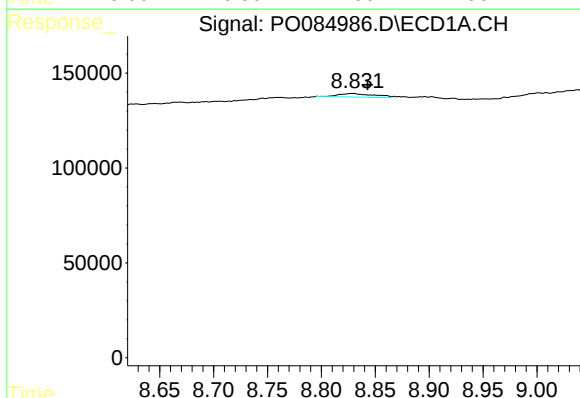


#38 AR-1262-3

R.T.: 8.831 min
Delta R.T.: -0.012 min
Response: 41839
Conc: 3.99 ng/ml

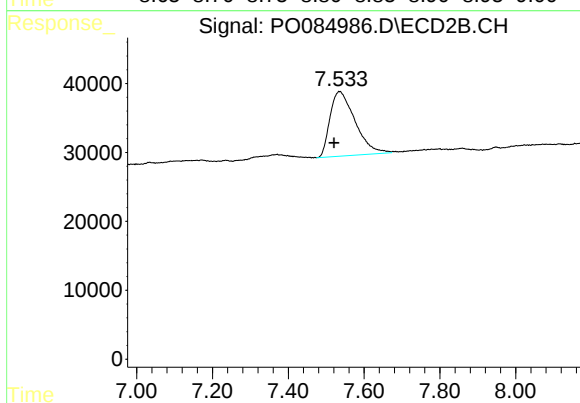

#38 AR-1262-3


R.T.: 7.537 min
Delta R.T.: 0.016 min
Response: 429688
Conc: 276.42 ng/ml

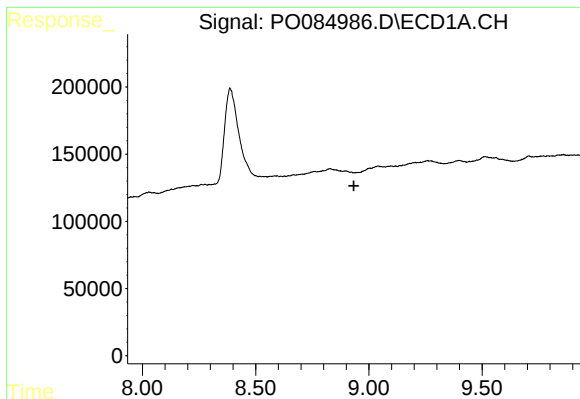

#39 AR-1262-4


R.T.: 8.970 min
Delta R.T.: 0.036 min
Response: -308
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

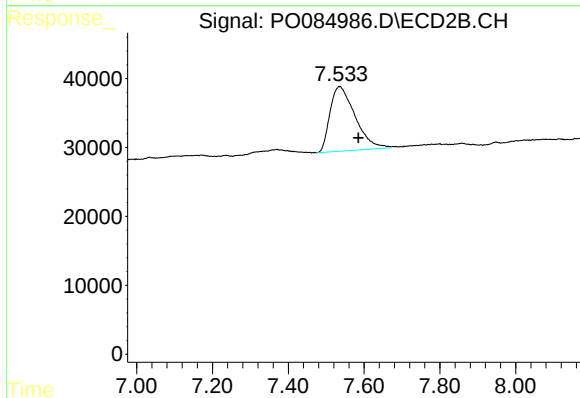


#39 AR-1262-4

R.T.: 7.537 min
Delta R.T.: -0.048 min
Response: 429688
Conc: 151.66 ng/ml

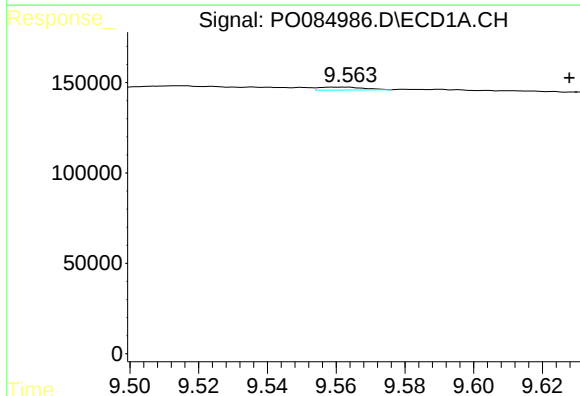


#40 AR-1262-5

R.T.: 9.563 min
Delta R.T.: -0.065 min
Response: 14892
Conc: 2.72 ng/ml

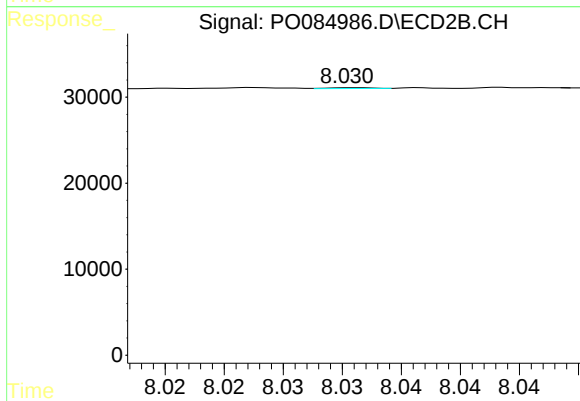

#40 AR-1262-5


R.T.: 8.031 min
Delta R.T.: -0.050 min
Response: 259
Conc: 0.20 ng/ml

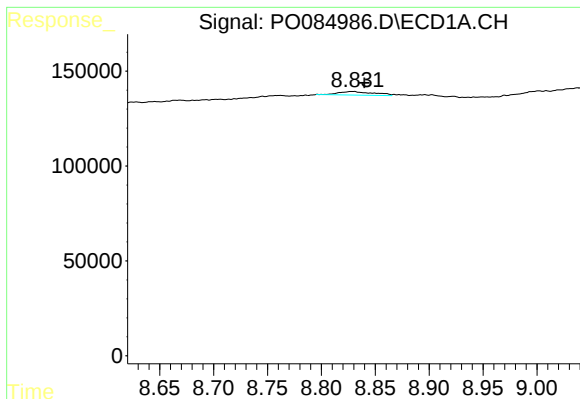

#41 AR-1268-1


R.T.: 8.831 min
Delta R.T.: -0.009 min
Response: 41839
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

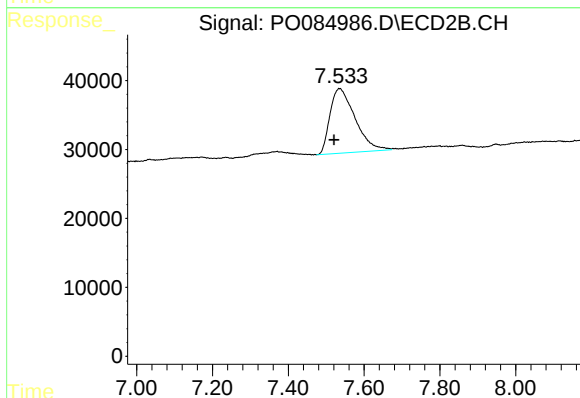


#41 AR-1268-1

R.T.: 7.537 min
Delta R.T.: 0.017 min
Response: 429688
Conc: 62.99 ng/ml

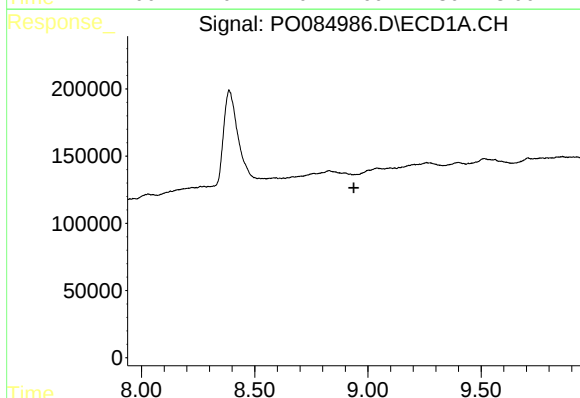


#42 AR-1268-2

R.T.: 8.970 min
Delta R.T.: 0.032 min
Response: -308
Conc: N.D.

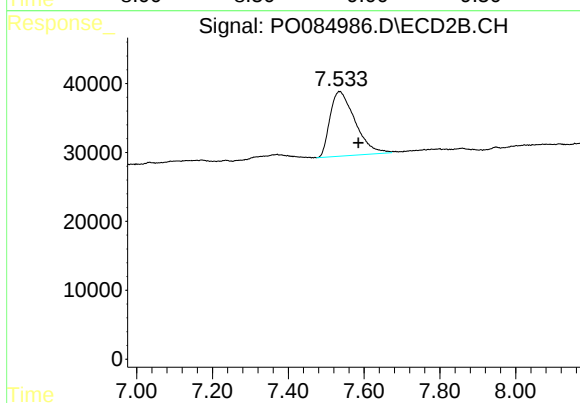

#42 AR-1268-2


R.T.: 7.537 min
Delta R.T.: -0.048 min
Response: 429688
Conc: 70.90 ng/ml

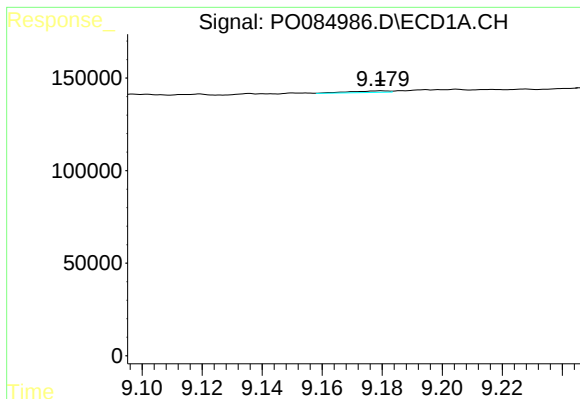

#43 AR-1268-3


R.T.: 9.180 min
Delta R.T.: 0.000 min
Response: 7741
Conc: 0.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

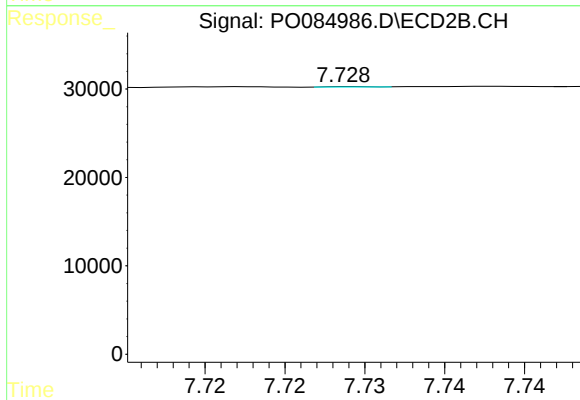


#43 AR-1268-3

R.T.: 7.729 min
Delta R.T.: -0.063 min
Response: 74
Conc: 0.01 ng/ml

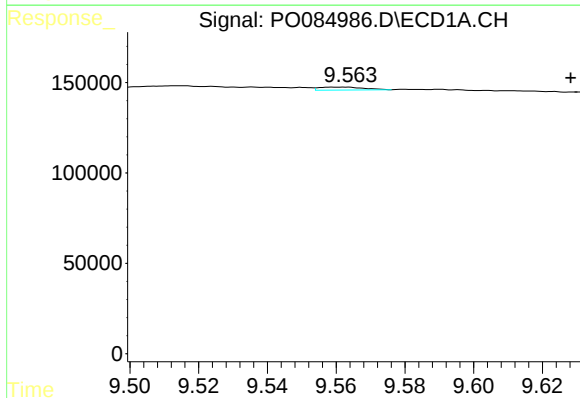


#44 AR-1268-4

R.T.: 9.563 min
Delta R.T.: -0.065 min
Response: 14892
Conc: 1.62 ng/ml

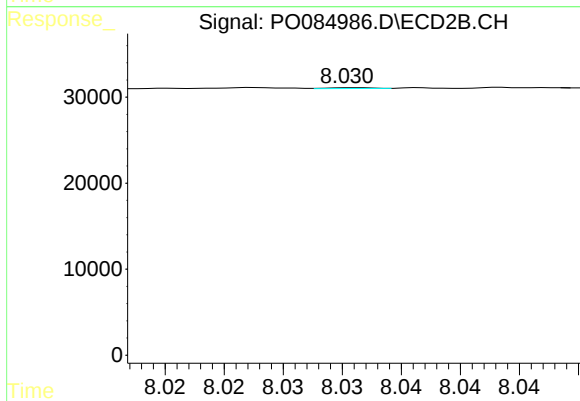

#44 AR-1268-4


R.T.: 8.031 min
Delta R.T.: -0.049 min
Response: 259
Conc: 0.11 ng/ml

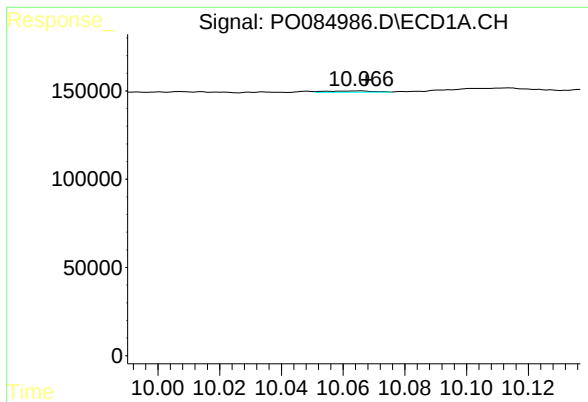

#45 AR-1268-5

R.T.: 10.066 min
Delta R.T.: -0.002 min
Response: 7843
Conc: 0.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-69A

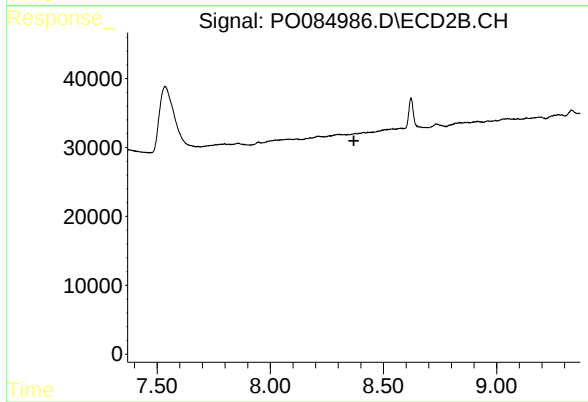

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.369 min
Response: 0
Conc: N.D.