

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0085034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 4:45
 Operator : YP\AJ
 Sample : N1715-28 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-81A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 06:51:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.509	3.594	389780	76239	1.394	1.695
2)	SA Decachlor...	10.434	8.622	317803	68846	1.813	1.874
Target Compounds							
3)	L1 AR-1016-1	5.684	0.000	7315	0	0.781	N.D. #
4)	L1 AR-1016-2	5.734	0.000	3440	0	0.258	N.D. #
5)	L1 AR-1016-3	5.784	4.926f	4050	4896	0.507	3.832 #
6)	L1 AR-1016-4	5.890	4.926	8492	4896	1.264	4.656 #
7)	L1 AR-1016-5	6.182	0.000	38100	0	6.026	N.D. #
8)	L2 AR-1221-1	4.695	0.000	16060	0	5.019	N.D. #
9)	L2 AR-1221-2	4.821	0.000	15542	0	6.446	N.D. #
10)	L2 AR-1221-3	4.892	0.000	55868	0	7.672	N.D. #
11)	L3 AR-1232-1	4.892	0.000	55868	0	9.129	N.D. #
12)	L3 AR-1232-2	5.426	0.000	1928	0	0.648	N.D. #
13)	L3 AR-1232-3	5.734	4.926f	3440	4896	0.607	9.014 #
14)	L3 AR-1232-4	5.890	4.926f	8492	4896	2.973	9.649 #
15)	L3 AR-1232-5	5.978	0.000	26109	0	11.556	N.D. #
16)	L4 AR-1242-1	5.684	0.000	7315	0	0.985	N.D. #
17)	L4 AR-1242-2	5.734	0.000	3440	0	0.325	N.D. #
18)	L4 AR-1242-3	5.784	4.926f	4050	4896	0.630	4.782 #
19)	L4 AR-1242-4	5.890	4.926f	8492	4896	1.566	4.699 #
20)	L4 AR-1242-5	6.659	5.490	59742	9971	11.359	8.046 #
21)	L5 AR-1248-1	5.684	0.000	7315	0	1.348	N.D. #
22)	L5 AR-1248-2	5.978	4.926	26109	4896	3.396	3.402
23)	L5 AR-1248-3	6.182	4.926f	38100	4896	4.434	3.261 #
24)	L5 AR-1248-4	6.598	0.000	33197	0	3.563	N.D. #
25)	L5 AR-1248-5	6.659	5.490f	59742	9971	6.682	5.946
26)	L6 AR-1254-1	6.566	5.490	51794	9971	5.281	3.727 #
27)	L6 AR-1254-2	6.789	5.639	76446	11534	5.151	4.890
28)	L6 AR-1254-3	7.161	6.042	93584	18395	6.181	4.893
29)	L6 AR-1254-4	7.451	6.273	81977	12003	7.643	5.121 #
30)	L6 AR-1254-5	7.877	6.693	134705	18906	11.440	5.588 #
31)	L7 AR-1260-1	7.328	6.174	55098	21328	4.828	8.594 #
32)	L7 AR-1260-2	7.590	6.365	69591	17139	5.412	5.790
33)	L7 AR-1260-3	7.954	6.514	13150	9789	1.647	3.579 #
34)	L7 AR-1260-4	8.177	7.029f	25719	5695	2.704	2.841
35)	L7 AR-1260-5	8.521	7.235	60494	13636	3.290	2.932
36)	L8 AR-1262-1	7.954	6.693	13150	18906	1.455	15.665 #
37)	L8 AR-1262-2	8.521	7.029f	60494	5695	3.792	2.804 #
38)	L8 AR-1262-3	8.845	7.521	5202	7732	0.496	4.974 #
39)	L8 AR-1262-4	8.933	7.584	3218	7184	0.637	2.536 #
40)	L8 AR-1262-5	9.634	8.082	11512	24537	2.105	18.537 #
41)	L9 AR-1268-1	8.837	7.521	10184	7732	0.365	1.133 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0085034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 4:45
 Operator : YP\AJ
 Sample : N1715-28 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-81A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 06:51:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.943	7.584	6966	7184	0.278	1.185 #
43) L9	AR-1268-3	9.178	0.000	9440	0	0.442	N.D. #
44) L9	AR-1268-4	9.634	8.082	11512	24537	1.254	10.750 #
45) L9	AR-1268-5	10.070	8.385	843	30077	0.012	2.044 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO085034.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 4:45
Operator : YP\AJ
Sample : N1715-28 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 06:51:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

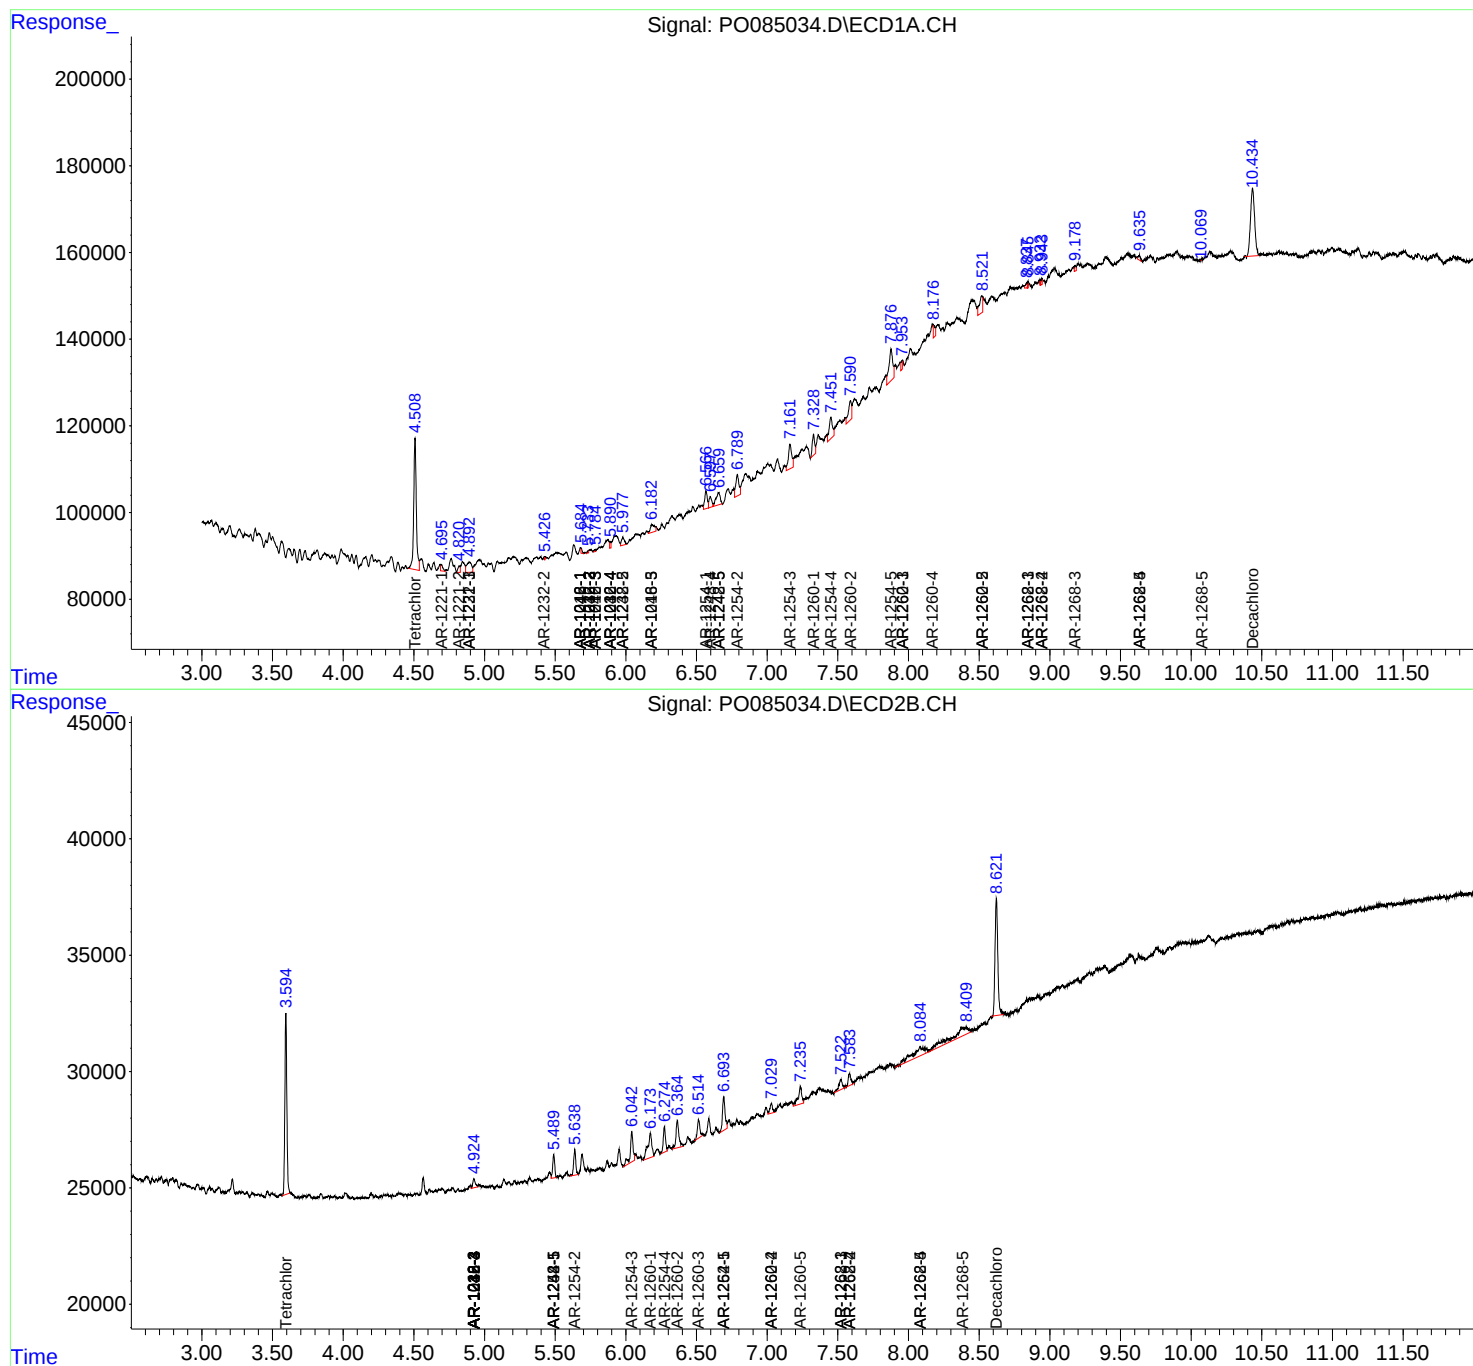


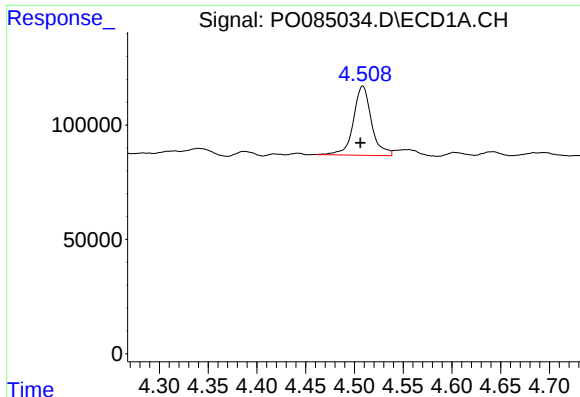

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 389780
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

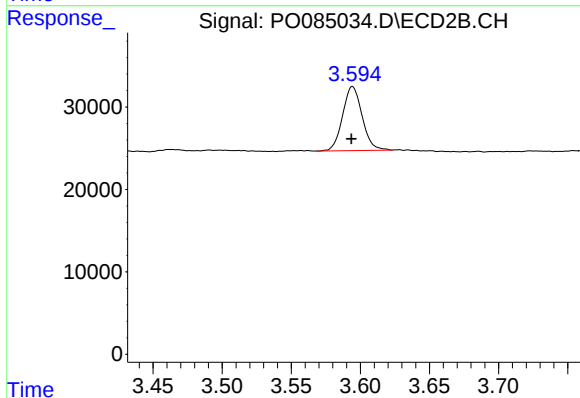


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 76239
Conc: 1.70 ng/ml

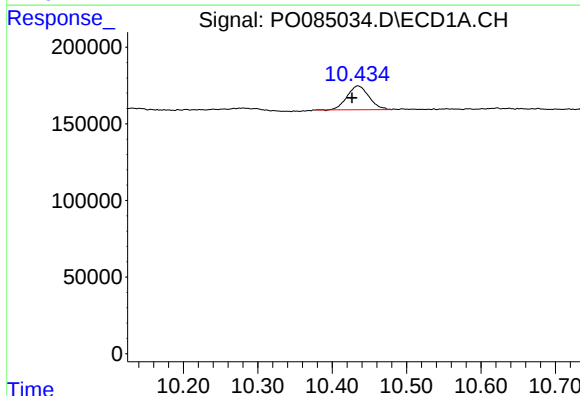


#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.008 min
Response: 317803
Conc: 1.81 ng/ml

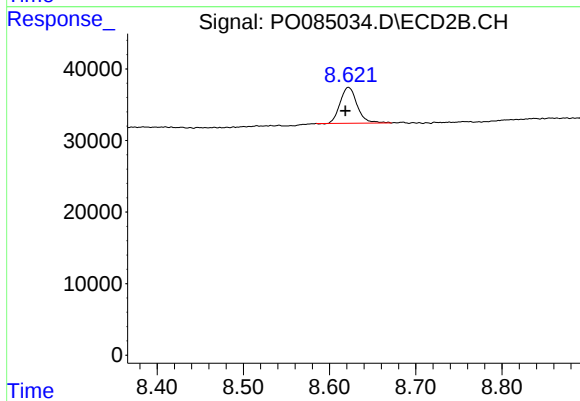

#2 Decachlorobiphenyl


R.T.: 8.622 min
Delta R.T.: 0.004 min
Response: 68846
Conc: 1.87 ng/ml

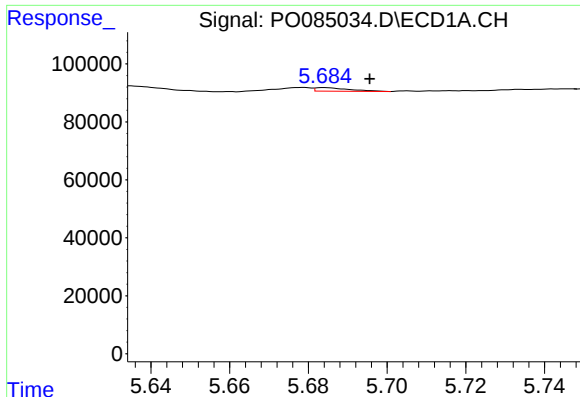

#3 AR-1016-1


R.T.: 5.684 min
Delta R.T.: -0.011 min
Response: 7315
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

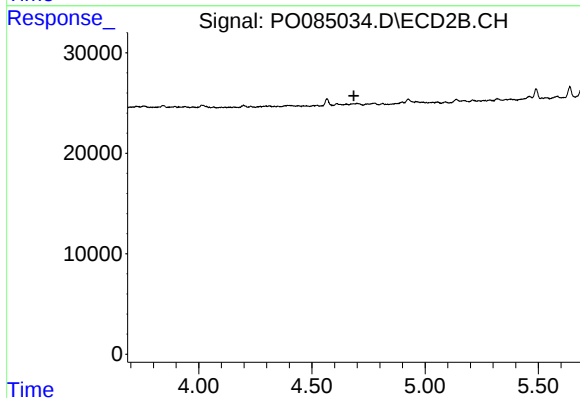


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

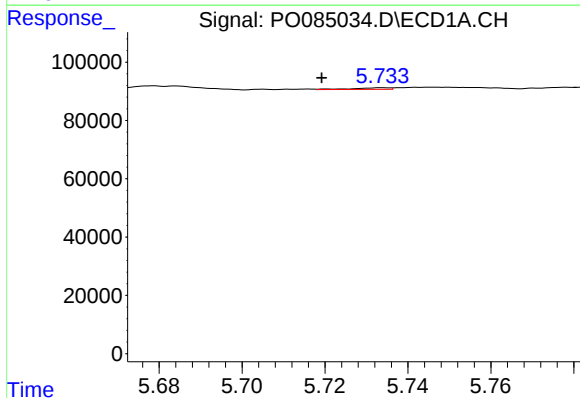


#4 AR-1016-2

R.T.: 5.734 min
Delta R.T.: 0.015 min
Response: 3440
Conc: 0.26 ng/ml

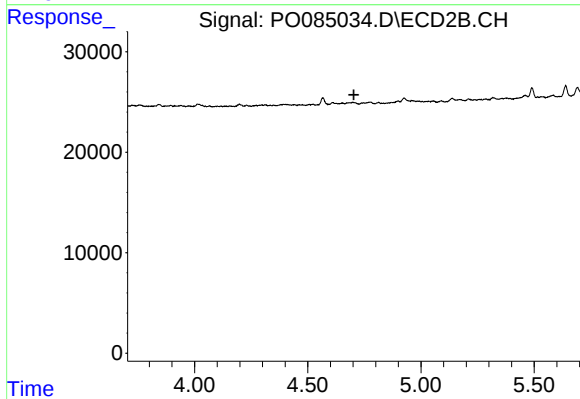

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

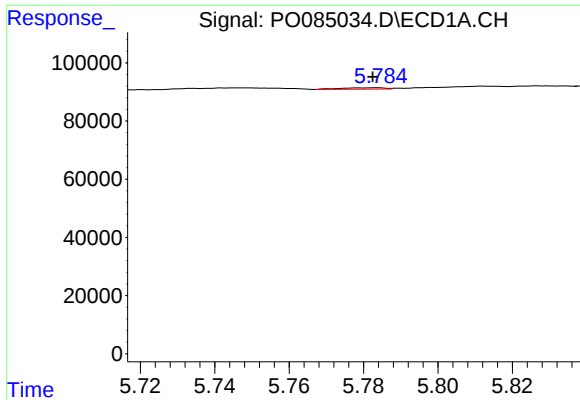

#5 AR-1016-3


R.T.: 5.784 min
Delta R.T.: 0.001 min
Response: 4050
Conc: 0.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

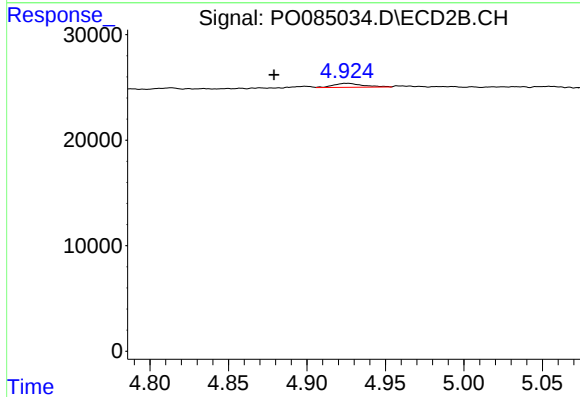


#5 AR-1016-3

R.T.: 4.926 min
Delta R.T.: 0.047 min
Response: 4896
Conc: 3.83 ng/ml

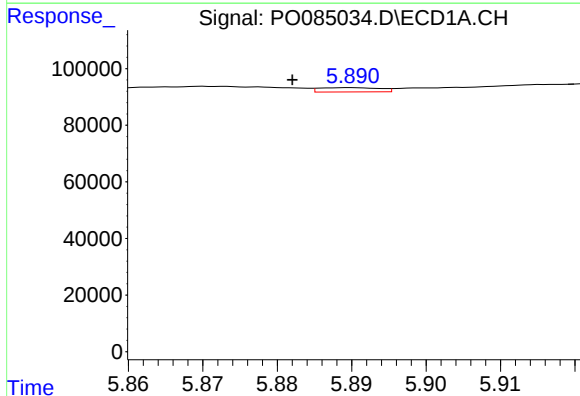


#6 AR-1016-4

R.T.: 5.890 min
Delta R.T.: 0.008 min
Response: 8492
Conc: 1.26 ng/ml

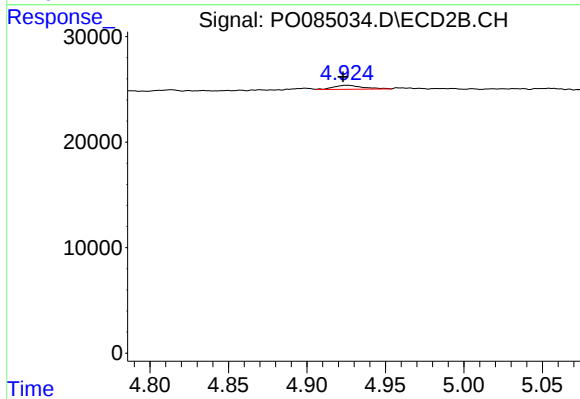

#6 AR-1016-4


R.T.: 4.926 min
Delta R.T.: 0.003 min
Response: 4896
Conc: 4.66 ng/ml

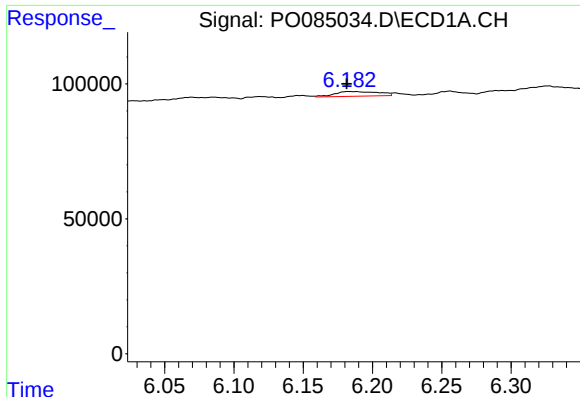

#7 AR-1016-5


R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 38100
Conc: 6.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

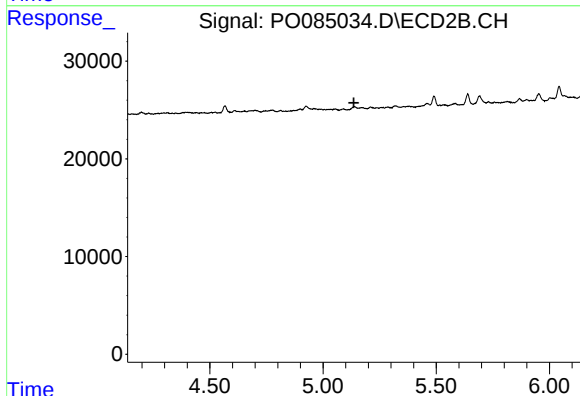


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.136 min
Response: 0
Conc: N.D.

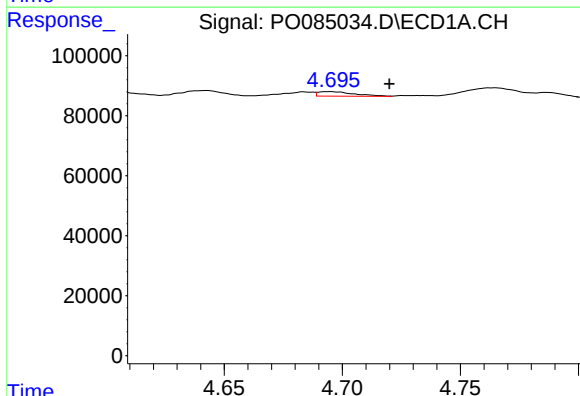


#8 AR-1221-1

R.T.: 4.695 min
Delta R.T.: -0.025 min
Response: 16060
Conc: 5.02 ng/ml

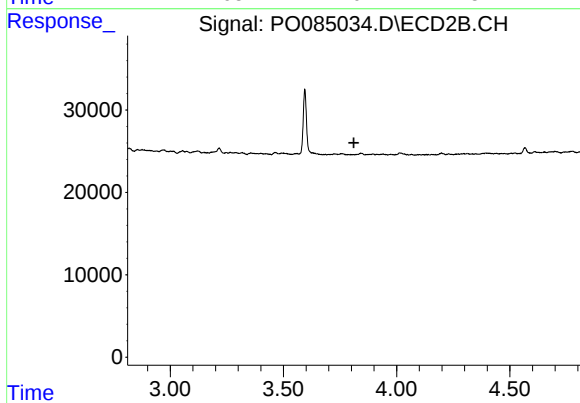

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.811 min
Response: 0
Conc: N.D.

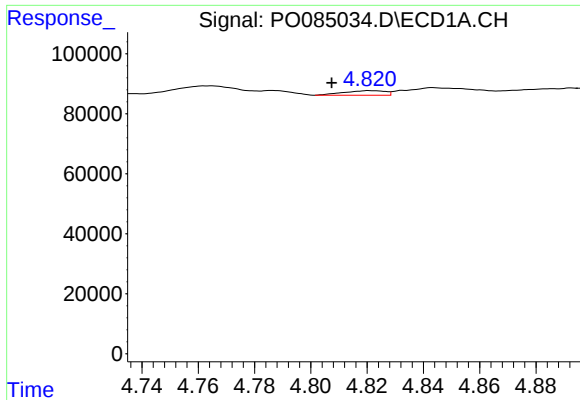

#9 AR-1221-2


R.T.: 4.821 min
Delta R.T.: 0.013 min
Response: 15542
Conc: 6.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

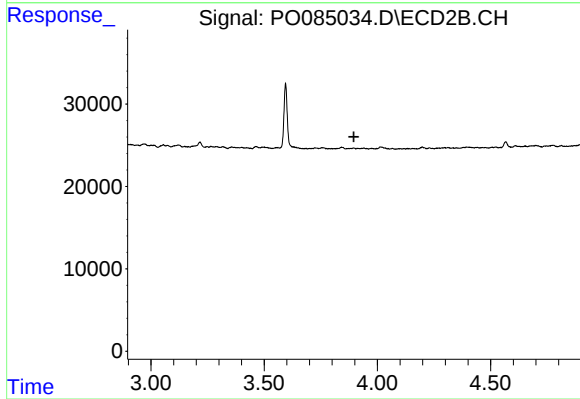


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

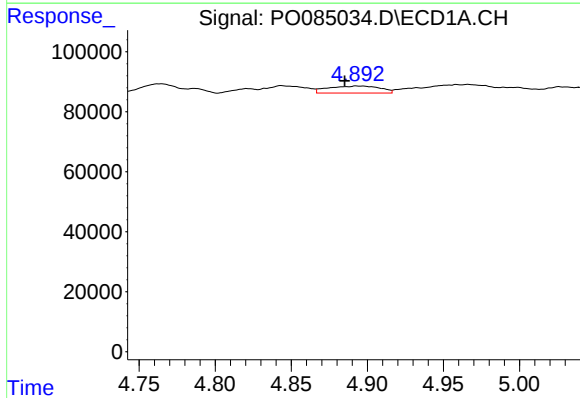


#10 AR-1221-3

R.T.: 4.892 min
Delta R.T.: 0.007 min
Response: 55868
Conc: 7.67 ng/ml

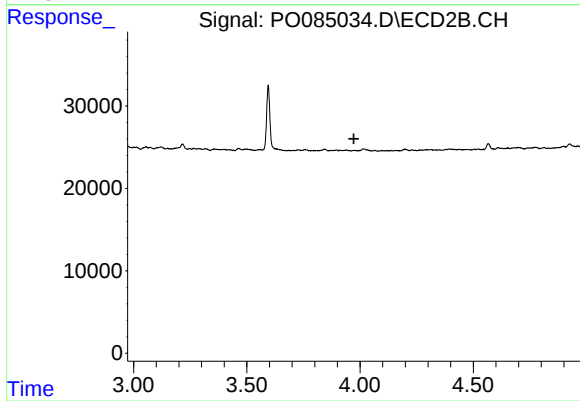

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.973 min
Response: 0
Conc: N.D.

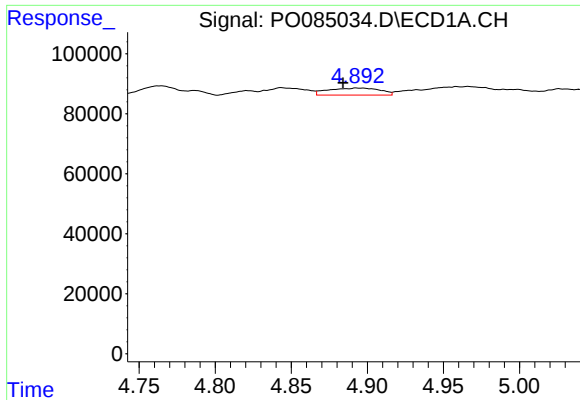

#11 AR-1232-1


R.T.: 4.892 min
Delta R.T.: 0.008 min
Response: 55868
Conc: 9.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

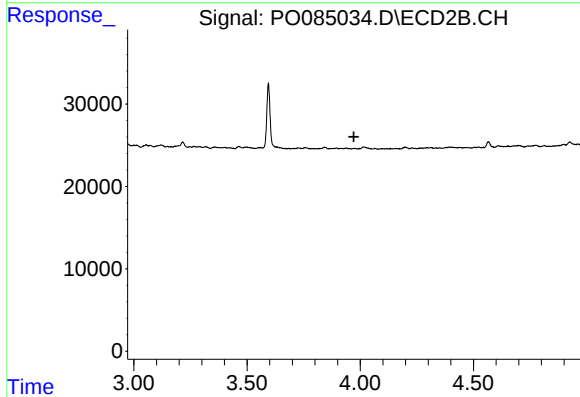


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

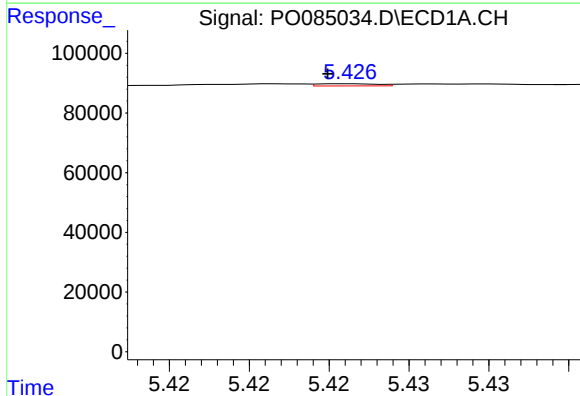


#12 AR-1232-2

R.T.: 5.426 min
Delta R.T.: 0.001 min
Response: 1928
Conc: 0.65 ng/ml

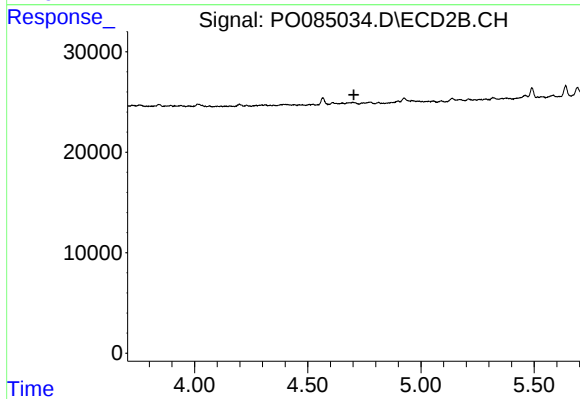

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

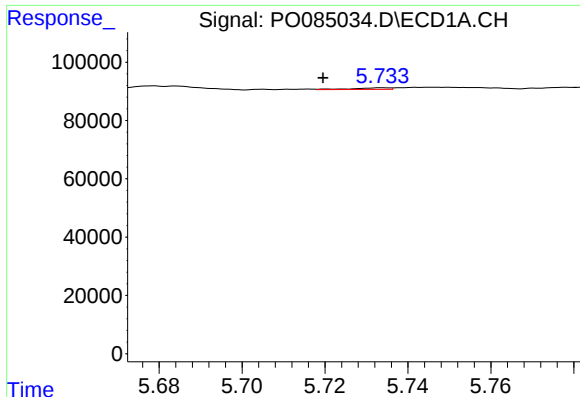

#13 AR-1232-3


R.T.: 5.734 min
Delta R.T.: 0.014 min
Response: 3440
Conc: 0.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

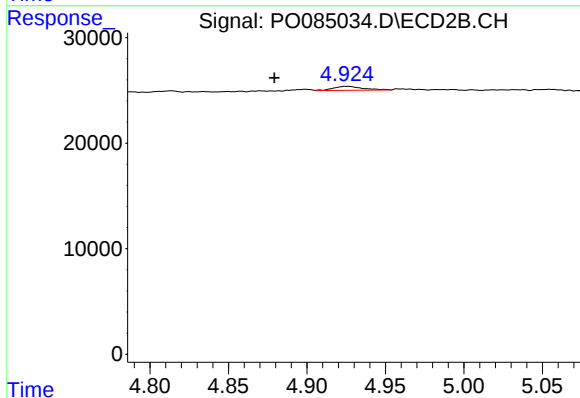


#13 AR-1232-3

R.T.: 4.926 min
Delta R.T.: 0.046 min
Response: 4896
Conc: 9.01 ng/ml

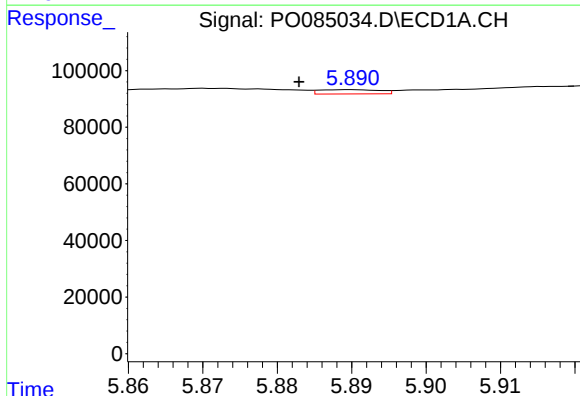


#14 AR-1232-4

R.T.: 5.890 min
Delta R.T.: 0.007 min
Response: 8492
Conc: 2.97 ng/ml

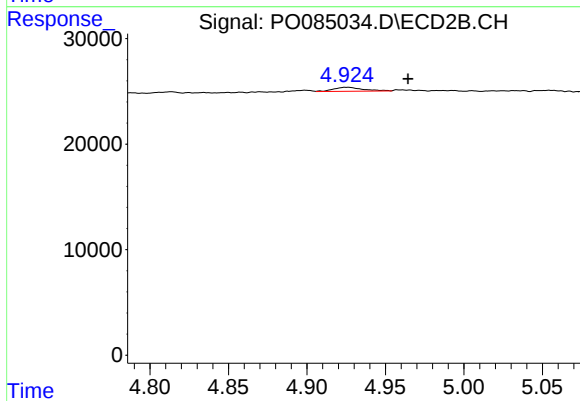

#14 AR-1232-4


R.T.: 4.926 min
Delta R.T.: -0.039 min
Response: 4896
Conc: 9.65 ng/ml

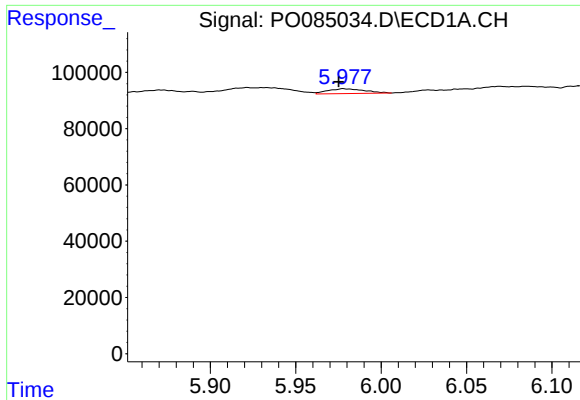

#15 AR-1232-5


R.T.: 5.978 min
Delta R.T.: 0.003 min
Response: 26109
Conc: 11.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

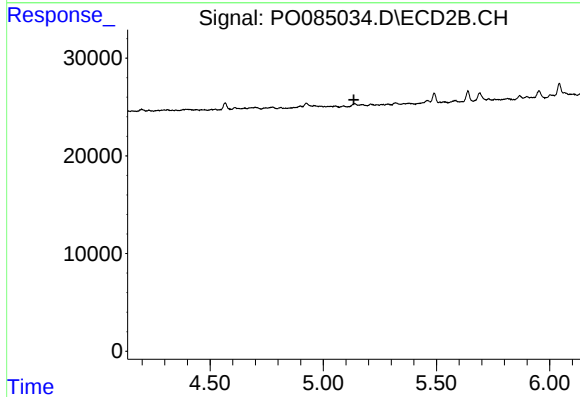


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.135 min
Response: 0
Conc: N.D.

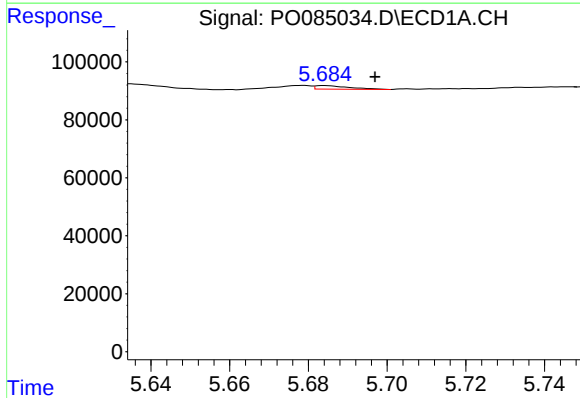


#16 AR-1242-1

R.T.: 5.684 min
Delta R.T.: -0.013 min
Response: 7315
Conc: 0.99 ng/ml

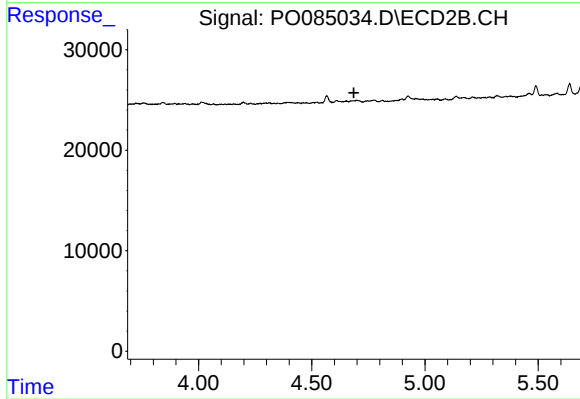

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

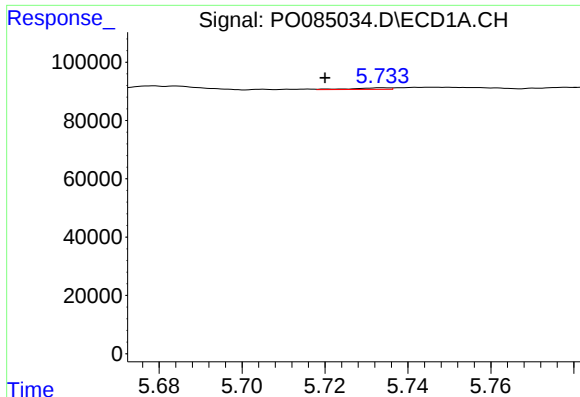

#17 AR-1242-2


R.T.: 5.734 min
Delta R.T.: 0.014 min
Response: 3440
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

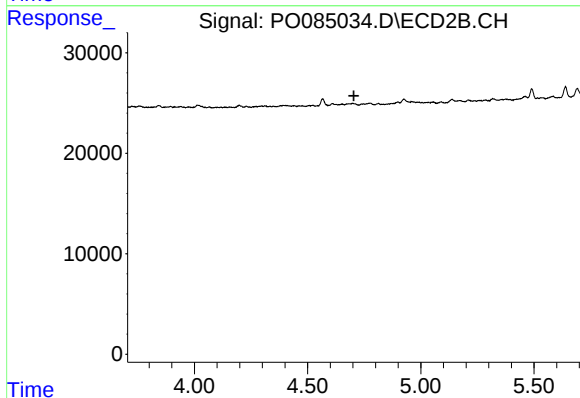


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.705 min
Response: 0
Conc: N.D.

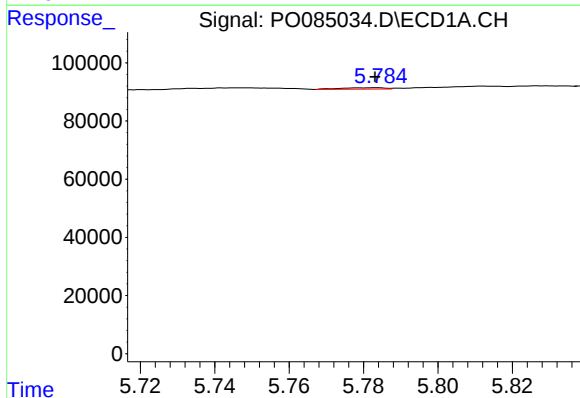


#18 AR-1242-3

R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 4050
Conc: 0.63 ng/ml

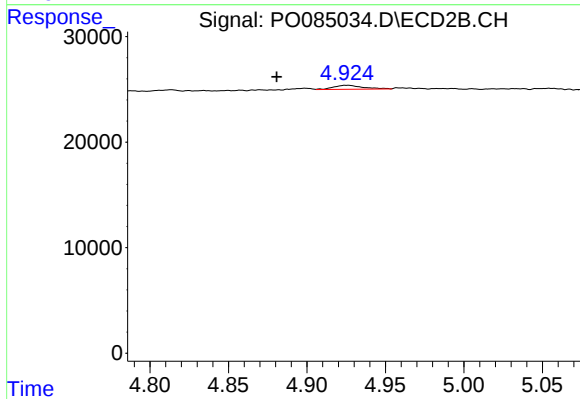

#18 AR-1242-3


R.T.: 4.926 min
Delta R.T.: 0.045 min
Response: 4896
Conc: 4.78 ng/ml

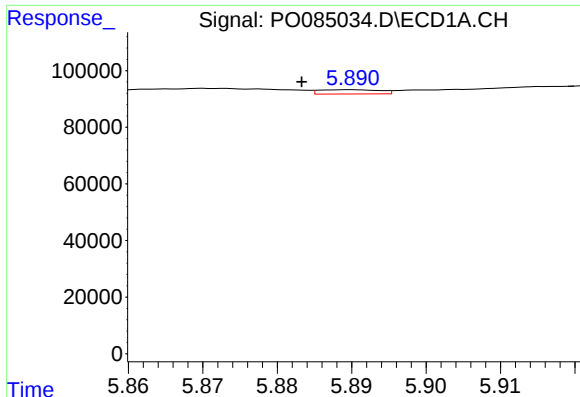

#19 AR-1242-4


R.T.: 5.890 min
Delta R.T.: 0.007 min
Response: 8492
Conc: 1.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

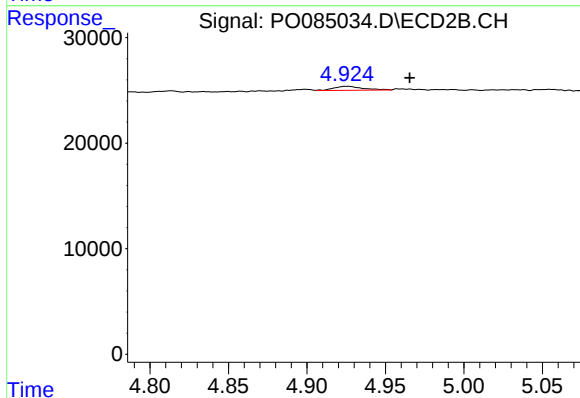


#19 AR-1242-4

R.T.: 4.926 min
Delta R.T.: -0.040 min
Response: 4896
Conc: 4.70 ng/ml

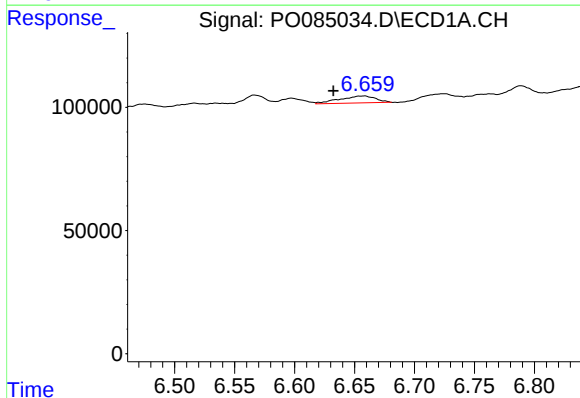


#20 AR-1242-5

R.T.: 6.659 min
Delta R.T.: 0.026 min
Response: 59742
Conc: 11.36 ng/ml

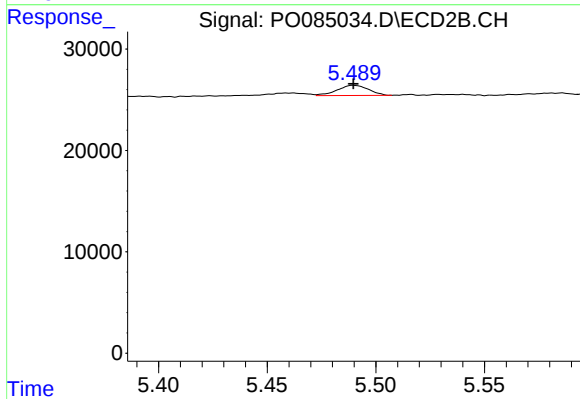

#20 AR-1242-5


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 9971
Conc: 8.05 ng/ml

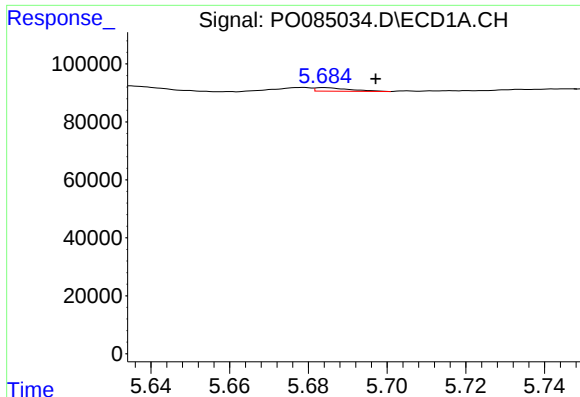

#21 AR-1248-1


R.T.: 5.684 min
Delta R.T.: -0.013 min
Response: 7315
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

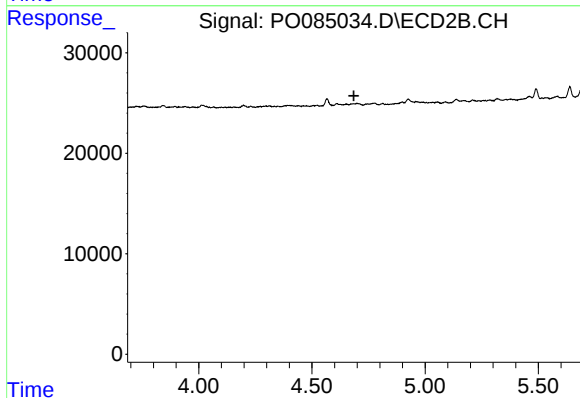


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

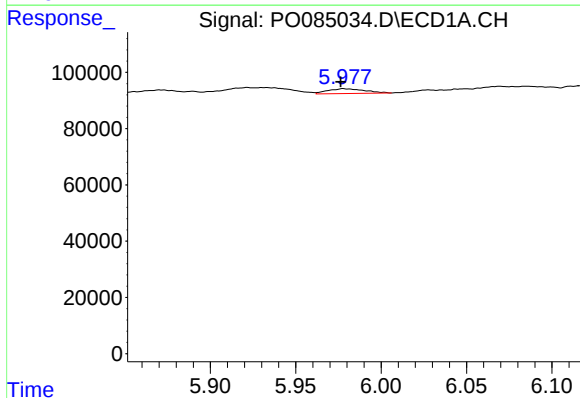


#22 AR-1248-2

R.T.: 5.978 min
Delta R.T.: 0.001 min
Response: 26109
Conc: 3.40 ng/ml

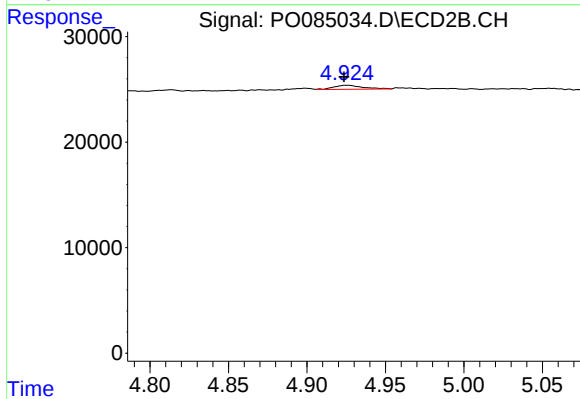

#22 AR-1248-2


R.T.: 4.926 min
Delta R.T.: 0.002 min
Response: 4896
Conc: 3.40 ng/ml

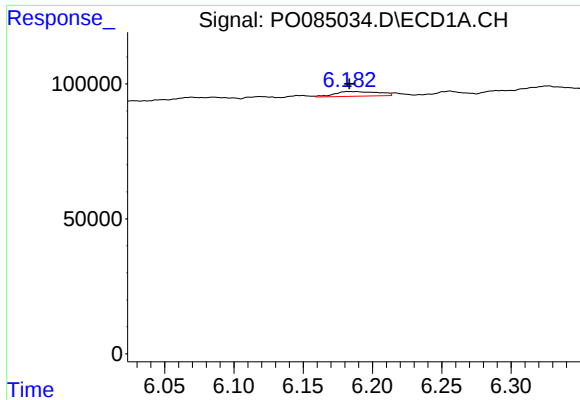

#23 AR-1248-3


R.T.: 6.182 min
Delta R.T.: -0.001 min
Response: 38100
Conc: 4.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

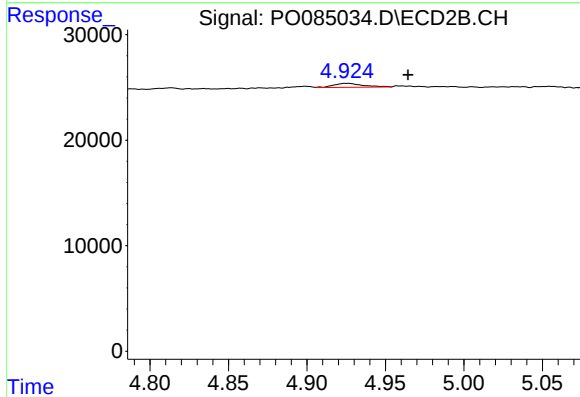


#23 AR-1248-3

R.T.: 4.926 min
Delta R.T.: -0.039 min
Response: 4896
Conc: 3.26 ng/ml

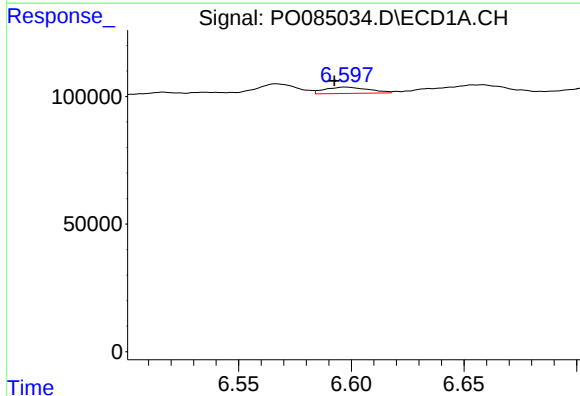


#24 AR-1248-4

R.T.: 6.598 min
Delta R.T.: 0.005 min
Response: 33197
Conc: 3.56 ng/ml

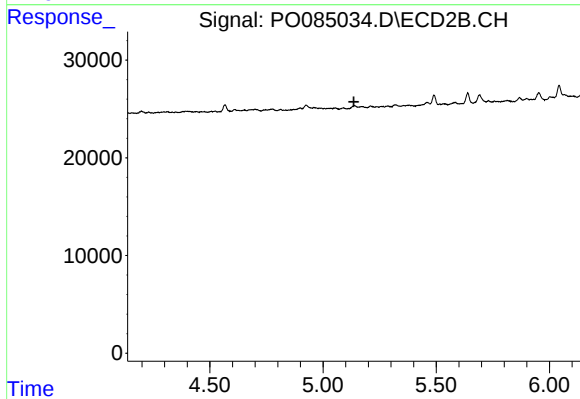

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.136 min
Response: 0
Conc: N.D.

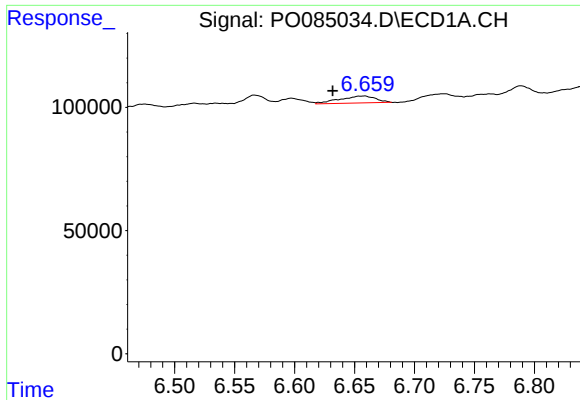

#25 AR-1248-5


R.T.: 6.659 min
Delta R.T.: 0.027 min
Response: 59742
Conc: 6.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

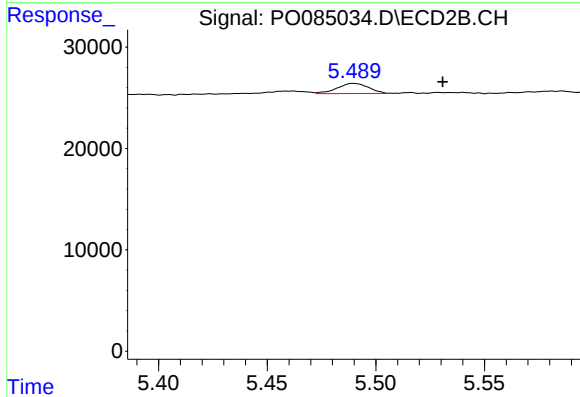


#25 AR-1248-5

R.T.: 5.490 min
Delta R.T.: -0.041 min
Response: 9971
Conc: 5.95 ng/ml

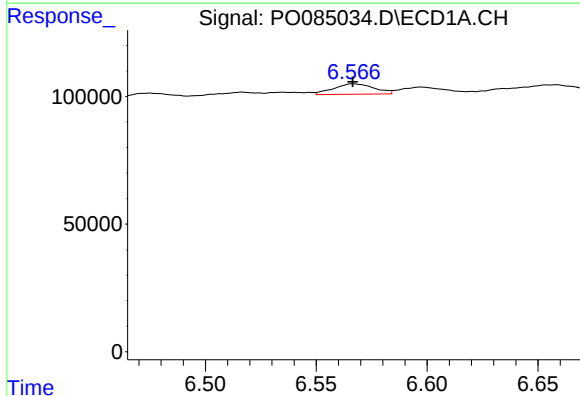


#26 AR-1254-1

R.T.: 6.566 min
Delta R.T.: 0.000 min
Response: 51794
Conc: 5.28 ng/ml

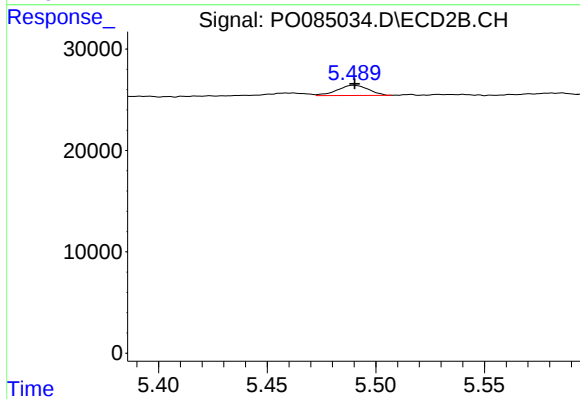

#26 AR-1254-1


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 9971
Conc: 3.73 ng/ml

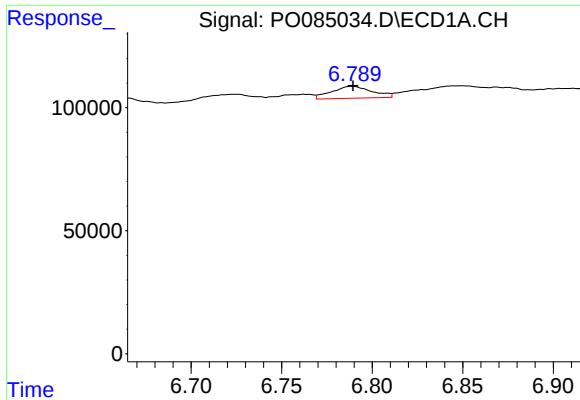

#27 AR-1254-2


R.T.: 6.789 min
Delta R.T.: 0.000 min
Response: 76446
Conc: 5.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

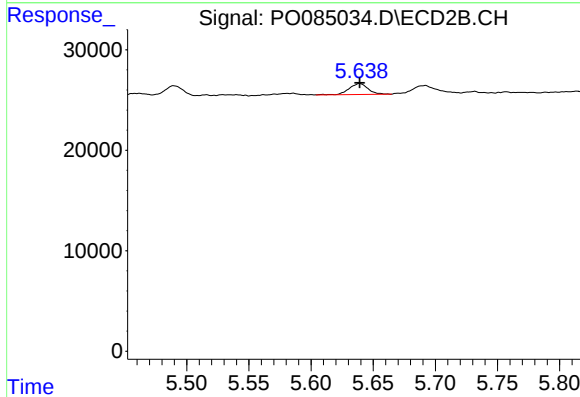


#27 AR-1254-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 11534
Conc: 4.89 ng/ml

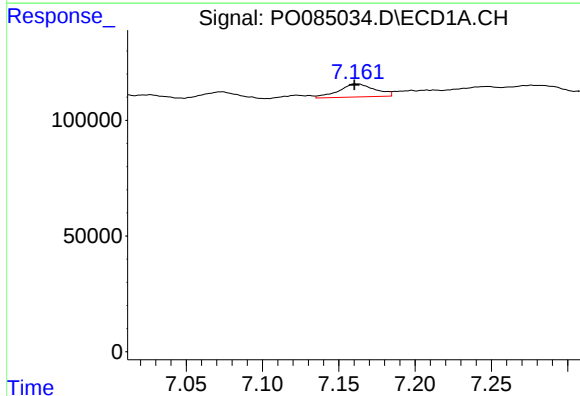


#28 AR-1254-3

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 93584
Conc: 6.18 ng/ml

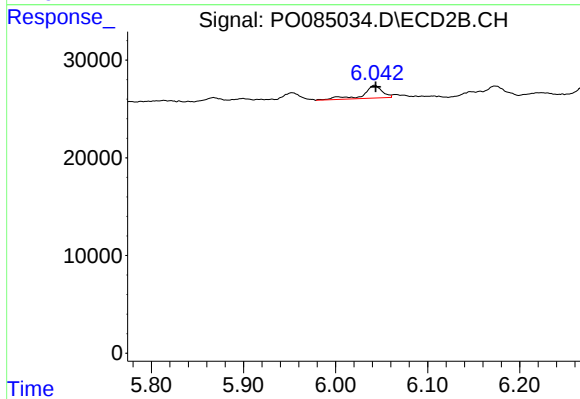

#28 AR-1254-3


R.T.: 6.042 min
Delta R.T.: -0.001 min
Response: 18395
Conc: 4.89 ng/ml

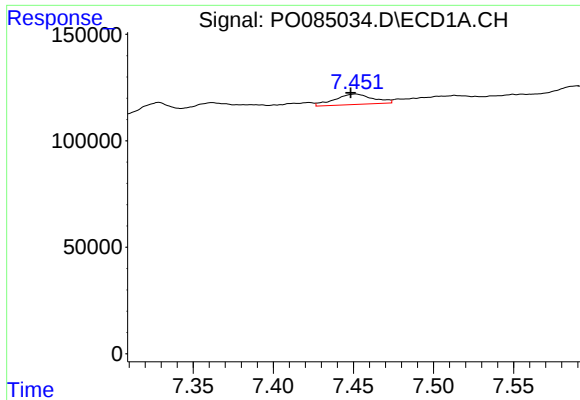

#29 AR-1254-4


R.T.: 7.451 min
Delta R.T.: 0.003 min
Response: 81977
Conc: 7.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

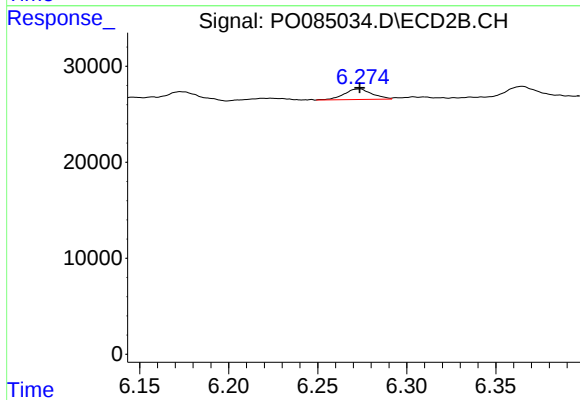


#29 AR-1254-4

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 12003
Conc: 5.12 ng/ml

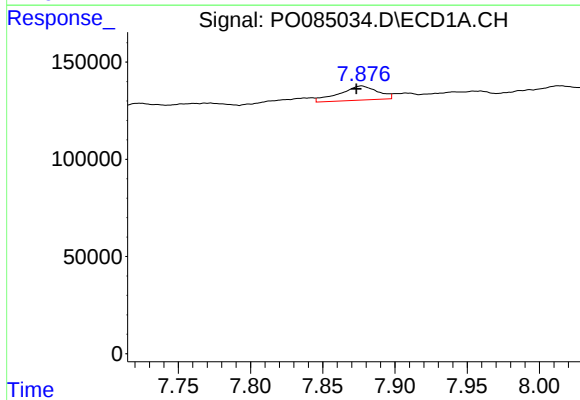


#30 AR-1254-5

R.T.: 7.877 min
Delta R.T.: 0.004 min
Response: 134705
Conc: 11.44 ng/ml

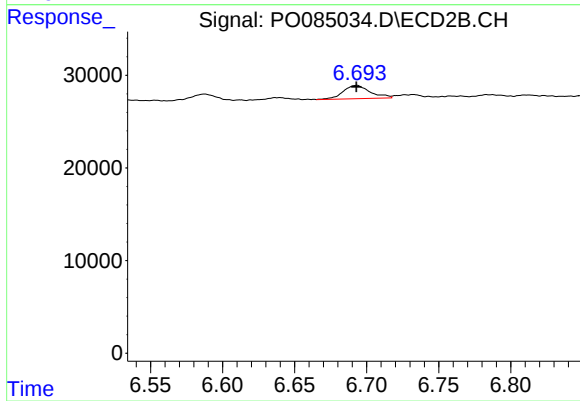

#30 AR-1254-5


R.T.: 6.693 min
Delta R.T.: 0.000 min
Response: 18906
Conc: 5.59 ng/ml

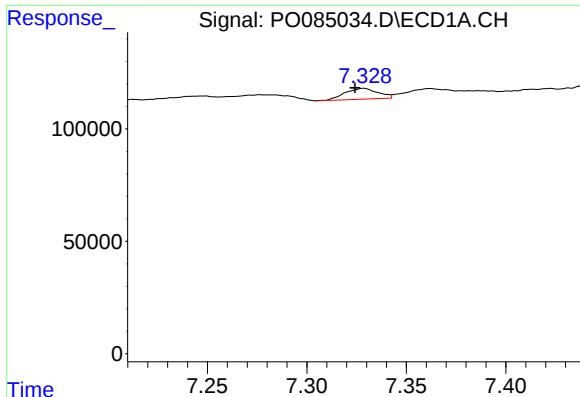

#31 AR-1260-1


R.T.: 7.328 min
Delta R.T.: 0.004 min
Response: 55098
Conc: 4.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

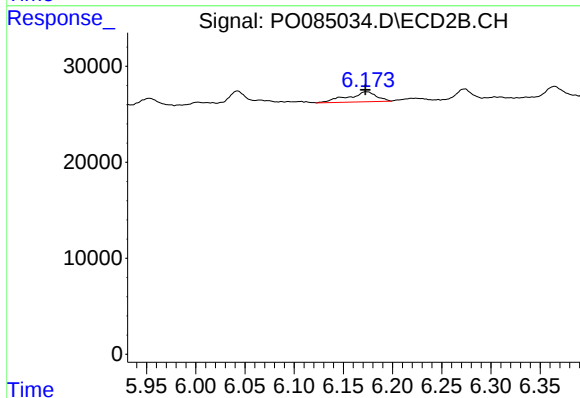


#31 AR-1260-1

R.T.: 6.174 min
Delta R.T.: 0.001 min
Response: 21328
Conc: 8.59 ng/ml

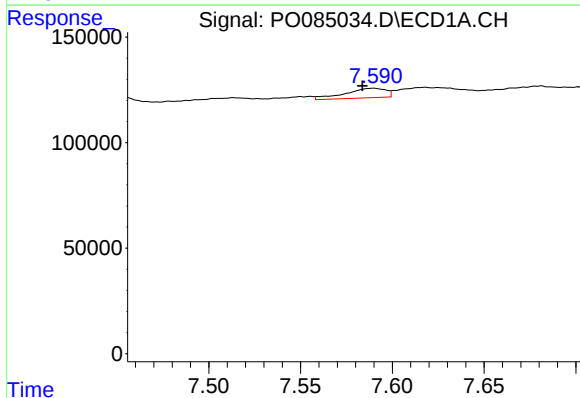


#32 AR-1260-2

R.T.: 7.590 min
Delta R.T.: 0.006 min
Response: 69591
Conc: 5.41 ng/ml

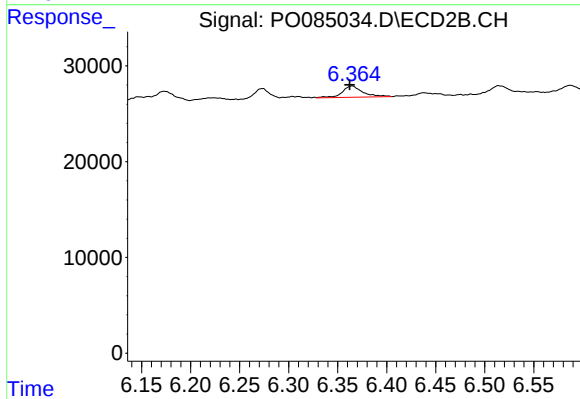

#32 AR-1260-2


R.T.: 6.365 min
Delta R.T.: 0.002 min
Response: 17139
Conc: 5.79 ng/ml

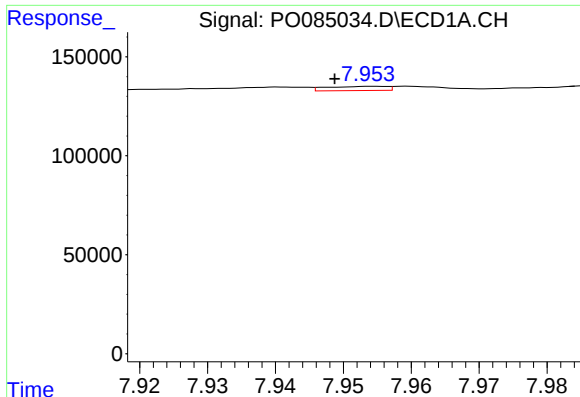

#33 AR-1260-3


R.T.: 7.954 min
Delta R.T.: 0.006 min
Response: 13150
Conc: 1.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

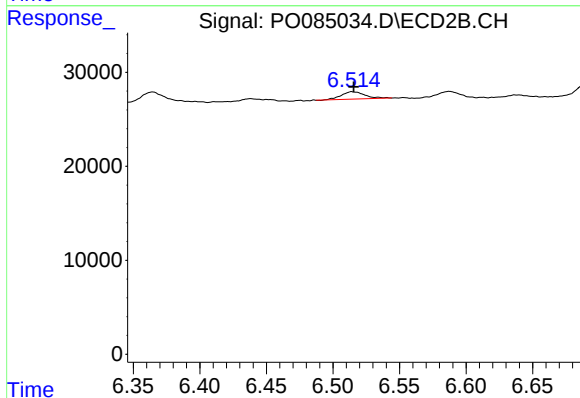


#33 AR-1260-3

R.T.: 6.514 min
Delta R.T.: -0.001 min
Response: 9789
Conc: 3.58 ng/ml

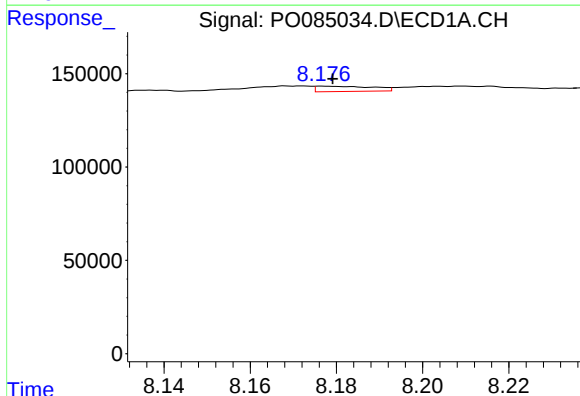


#34 AR-1260-4

R.T.: 8.177 min
Delta R.T.: -0.002 min
Response: 25719
Conc: 2.70 ng/ml

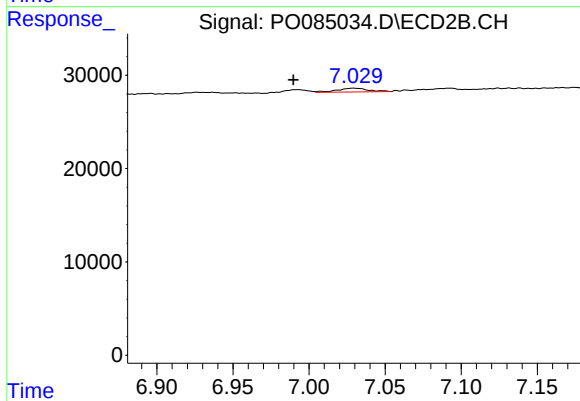

#34 AR-1260-4


R.T.: 7.029 min
Delta R.T.: 0.040 min
Response: 5695
Conc: 2.84 ng/ml

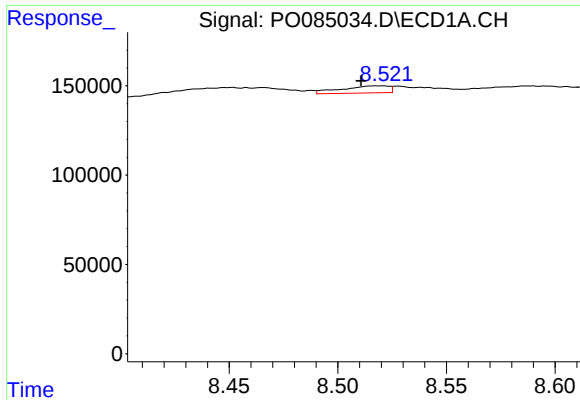

#35 AR-1260-5


R.T.: 8.521 min
Delta R.T.: 0.010 min
Response: 60494
Conc: 3.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

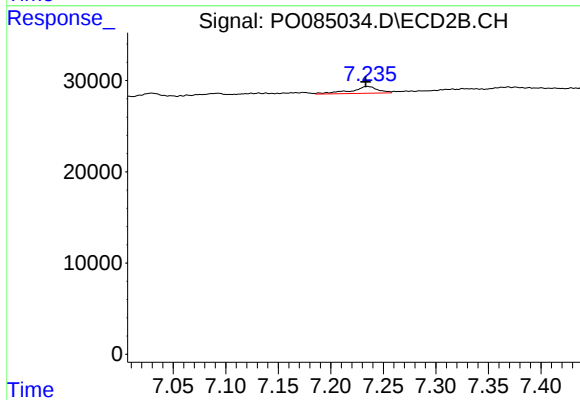


#35 AR-1260-5

R.T.: 7.235 min
Delta R.T.: 0.002 min
Response: 13636
Conc: 2.93 ng/ml

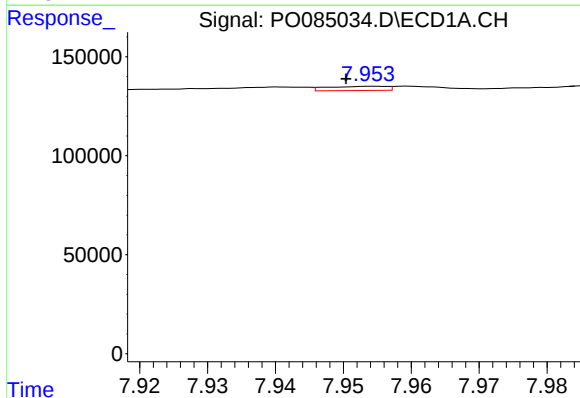


#36 AR-1262-1

R.T.: 7.954 min
Delta R.T.: 0.004 min
Response: 13150
Conc: 1.45 ng/ml

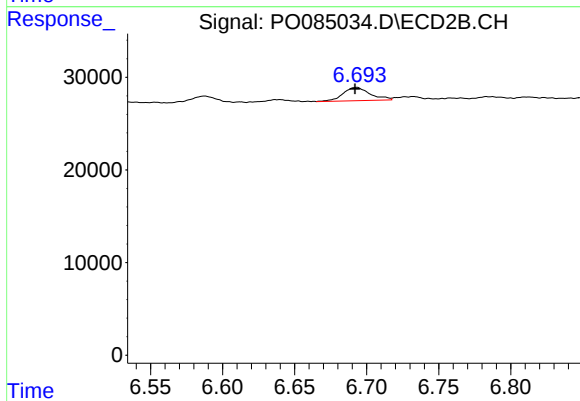

#36 AR-1262-1


R.T.: 6.693 min
Delta R.T.: 0.000 min
Response: 18906
Conc: 15.67 ng/ml

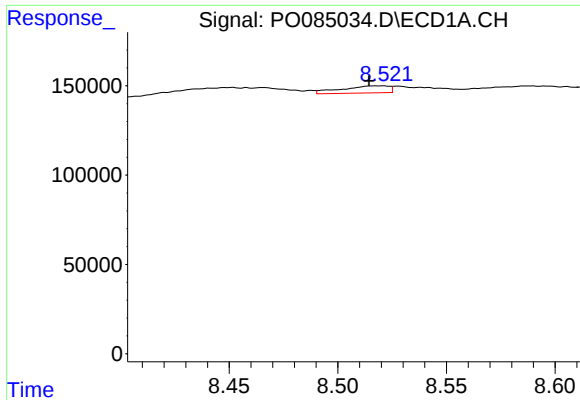

#37 AR-1262-2


R.T.: 8.521 min
Delta R.T.: 0.007 min
Response: 60494
Conc: 3.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

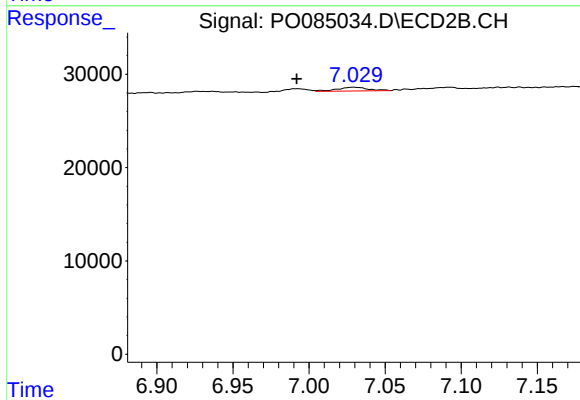


#37 AR-1262-2

R.T.: 7.029 min
Delta R.T.: 0.037 min
Response: 5695
Conc: 2.80 ng/ml

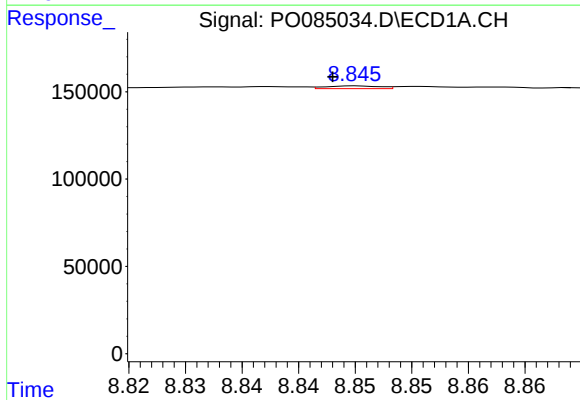


#38 AR-1262-3

R.T.: 8.845 min
Delta R.T.: 0.002 min
Response: 5202
Conc: 0.50 ng/ml

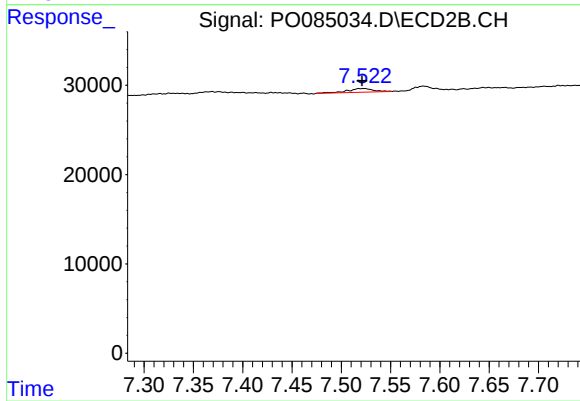

#38 AR-1262-3


R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 7732
Conc: 4.97 ng/ml

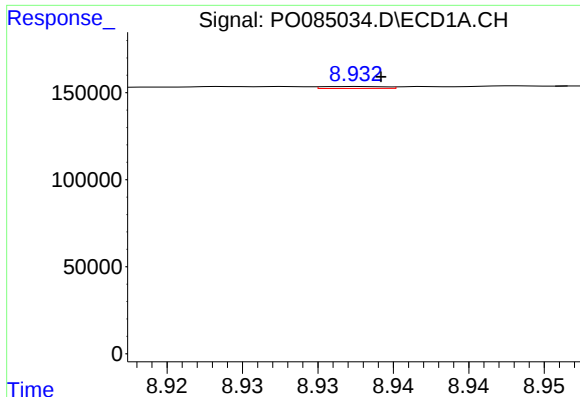

#39 AR-1262-4


R.T.: 8.933 min
Delta R.T.: -0.002 min
Response: 3218
Conc: 0.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

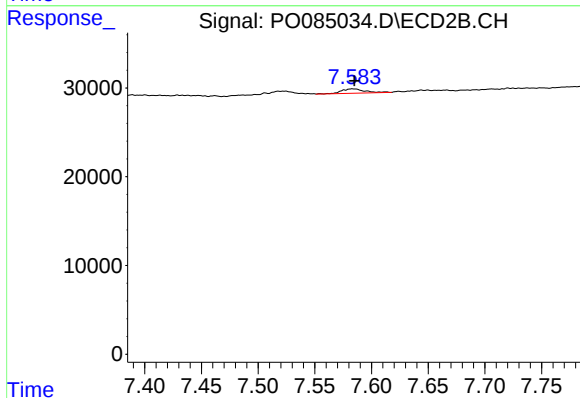


#39 AR-1262-4

R.T.: 7.584 min
Delta R.T.: -0.001 min
Response: 7184
Conc: 2.54 ng/ml

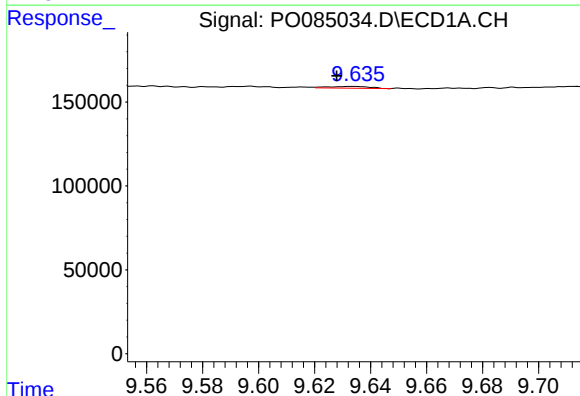


#40 AR-1262-5

R.T.: 9.634 min
Delta R.T.: 0.006 min
Response: 11512
Conc: 2.11 ng/ml

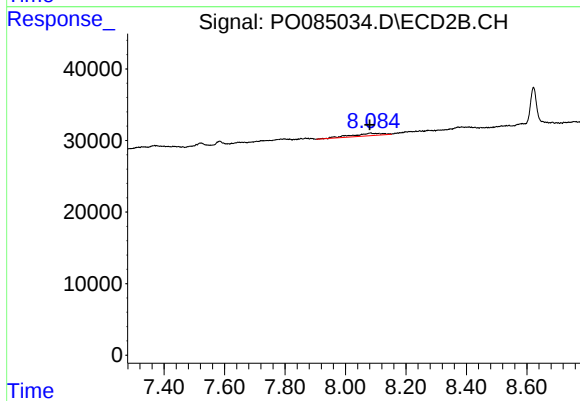

#40 AR-1262-5


R.T.: 8.082 min
Delta R.T.: 0.001 min
Response: 24537
Conc: 18.54 ng/ml

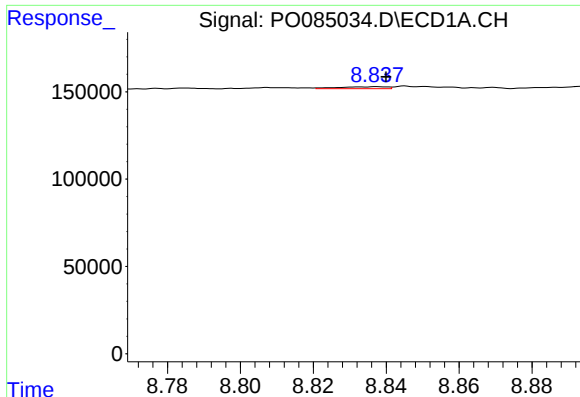

#41 AR-1268-1


R.T.: 8.837 min
Delta R.T.: -0.003 min
Response: 10184
Conc: 0.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

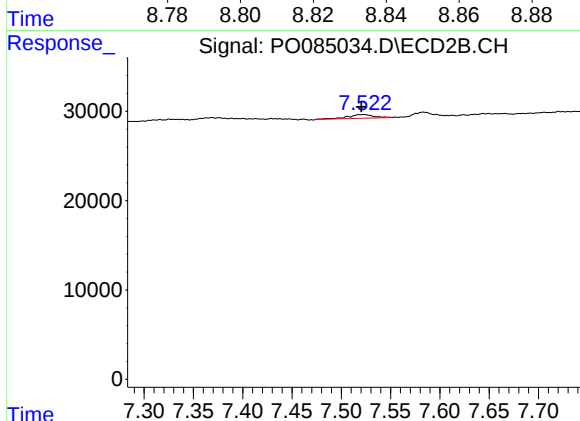


#41 AR-1268-1

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 7732
Conc: 1.13 ng/ml

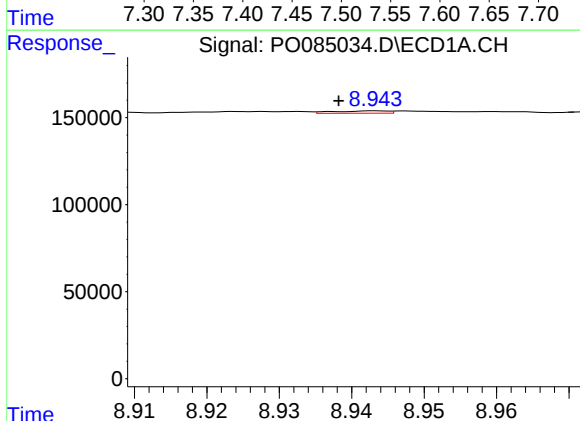


#42 AR-1268-2

R.T.: 8.943 min
Delta R.T.: 0.005 min
Response: 6966
Conc: 0.28 ng/ml

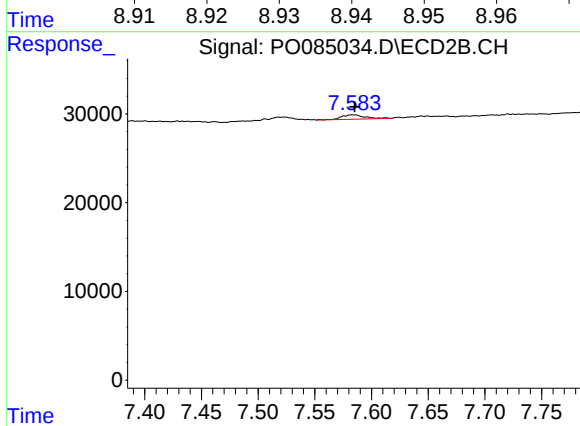

#42 AR-1268-2


R.T.: 7.584 min
Delta R.T.: -0.001 min
Response: 7184
Conc: 1.19 ng/ml

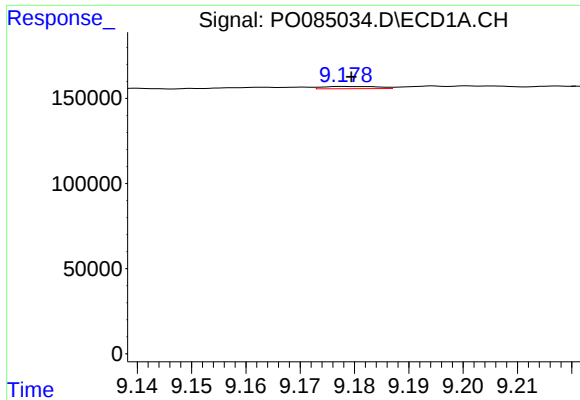

#43 AR-1268-3


R.T.: 9.178 min
Delta R.T.: -0.001 min
Response: 9440
Conc: 0.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

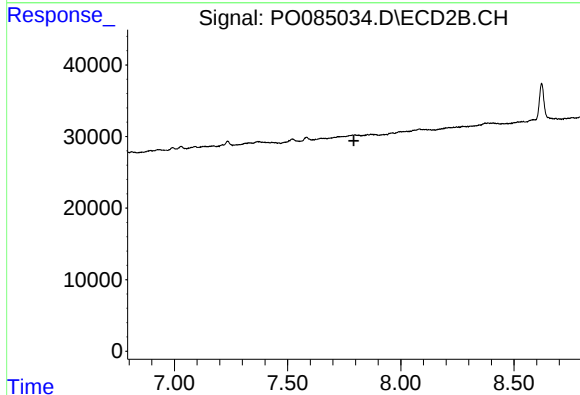


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

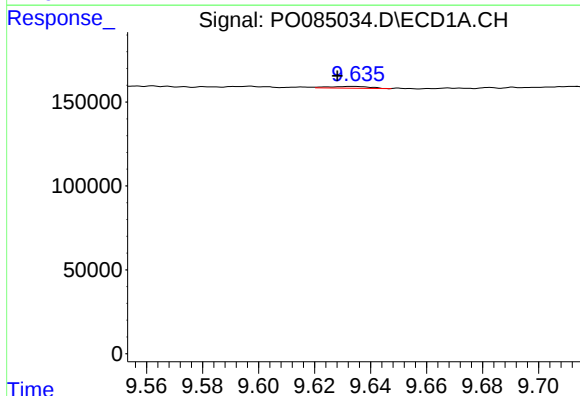


#44 AR-1268-4

R.T.: 9.634 min
Delta R.T.: 0.006 min
Response: 11512
Conc: 1.25 ng/ml

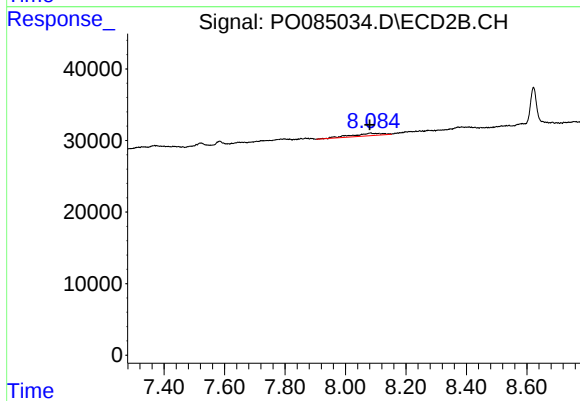

#44 AR-1268-4


R.T.: 8.082 min
Delta R.T.: 0.002 min
Response: 24537
Conc: 10.75 ng/ml

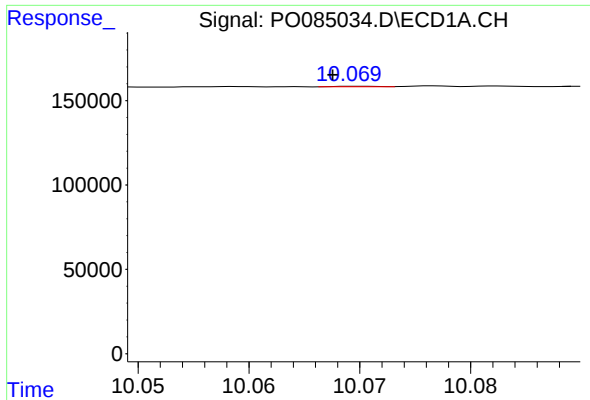

#45 AR-1268-5

R.T.: 10.070 min
Delta R.T.: 0.002 min
Response: 843
Conc: 0.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-81A

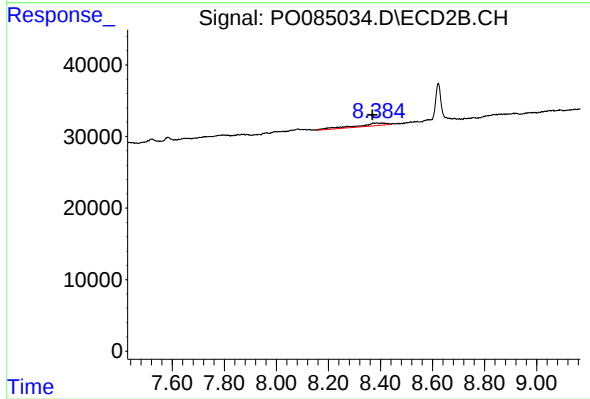

#45 AR-1268-5

R.T.: 8.385 min
Delta R.T.: 0.016 min
Response: 30077
Conc: 2.04 ng/ml