

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0085036.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 5:17
 Operator : YP\AJ
 Sample : N1715-34 10X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-82A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 06:52:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.509	3.595	292526	78063	1.046	1.736 #
2)	SA Decachlor...	10.436	8.623	225667	63636	1.287	1.732 #
Target Compounds							
3)	L1 AR-1016-1	5.726	0.000	8732	0	0.932	N.D. #
4)	L1 AR-1016-2	5.726	0.000	8732	0	0.655	N.D. #
5)	L1 AR-1016-3	5.817	4.898	-522	3564	N.D.	2.790 #
6)	L1 AR-1016-4	5.880	4.898	4156	3564	0.619	3.390 #
7)	L1 AR-1016-5	6.191	0.000	19400	0	3.069	N.D. #
8)	L2 AR-1221-1	4.762f	0.000	419	0	0.131	N.D. #
9)	L2 AR-1221-2	4.823	0.000	2831	0	1.174	N.D. #
10)	L2 AR-1221-3	4.889	0.000	5611	0	0.771	N.D. #
11)	L3 AR-1232-1	4.889	0.000	5611	0	0.917	N.D. #
12)	L3 AR-1232-2	5.407	0.000	24566	0	8.257	N.D. #
13)	L3 AR-1232-3	5.726	4.898	8732	3564	1.540	6.563 #
14)	L3 AR-1232-4	5.880	4.898f	4156	3564	1.455	7.024 #
15)	L3 AR-1232-5	5.977	0.000	8839	0	3.912	N.D. #
16)	L4 AR-1242-1	5.726	0.000	8732	0	1.176	N.D. #
17)	L4 AR-1242-2	5.726	0.000	8732	0	0.824	N.D. #
18)	L4 AR-1242-3	5.817	4.898	-522	3564	N.D.	3.482 #
19)	L4 AR-1242-4	5.880	4.898f	4156	3564	0.766	3.421 #
20)	L4 AR-1242-5	6.639	0.000	24335	0	4.627	N.D. #
21)	L5 AR-1248-1	5.726	0.000	8732	0	1.609	N.D. #
22)	L5 AR-1248-2	5.977	4.898	8839	3564	1.150	2.476 #
23)	L5 AR-1248-3	6.191	4.898f	19400	3564	2.258	2.374
24)	L5 AR-1248-4	6.595	0.000	7847	0	0.842	N.D. #
25)	L5 AR-1248-5	6.639	0.000	24335	0	2.722	N.D. #
26)	L6 AR-1254-1	6.568	0.000	26666	0	2.719	N.D. #
27)	L6 AR-1254-2	6.784	5.689f	12124	5883	0.817	2.494 #
28)	L6 AR-1254-3	7.163	6.041	17975	3697	1.187	0.983
29)	L6 AR-1254-4	7.452	6.273	14290	3367	1.332	1.437
30)	L6 AR-1254-5	7.880	6.693	37826	4330	3.212	1.280 #
31)	L7 AR-1260-1	7.333	0.000	29226	0	2.561	N.D. #
32)	L7 AR-1260-2	7.585	0.000	10941	0	0.851	N.D. #
33)	L7 AR-1260-3	7.947	0.000	6051	0	0.758	N.D. #
34)	L7 AR-1260-4	8.191	0.000	7313	0	0.769	N.D. #
35)	L7 AR-1260-5	8.513	0.000	38695	0	2.105	N.D. #
36)	L8 AR-1262-1	7.947	6.693	6051	4330	0.669	3.587 #
37)	L8 AR-1262-2	8.513	0.000	38695	0	2.426	N.D. #
38)	L8 AR-1262-3	8.826	0.000	23529	0	2.244	N.D. #
39)	L8 AR-1262-4	8.946	0.000	13061	0	2.584	N.D. #
40)	L8 AR-1262-5	9.619	8.121f	2714	9108	0.496	6.881 #
41)	L9 AR-1268-1	8.826	0.000	23529	0	0.842	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
Data File : P0085036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 5:17
Operator : YP\AJ
Sample : N1715-34 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 06:52:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.946	0.000	13061	0	0.522	N.D. #
43)	L9 AR-1268-3	9.234f	0.000	3338	0	0.156	N.D. #
44)	L9 AR-1268-4	9.619	8.121f	2714	9108	0.296	3.990 #
45)	L9 AR-1268-5	10.062	0.000	6326	0	0.090	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO085036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 5:17
Operator : YP\AJ
Sample : N1715-34 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 06:52:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

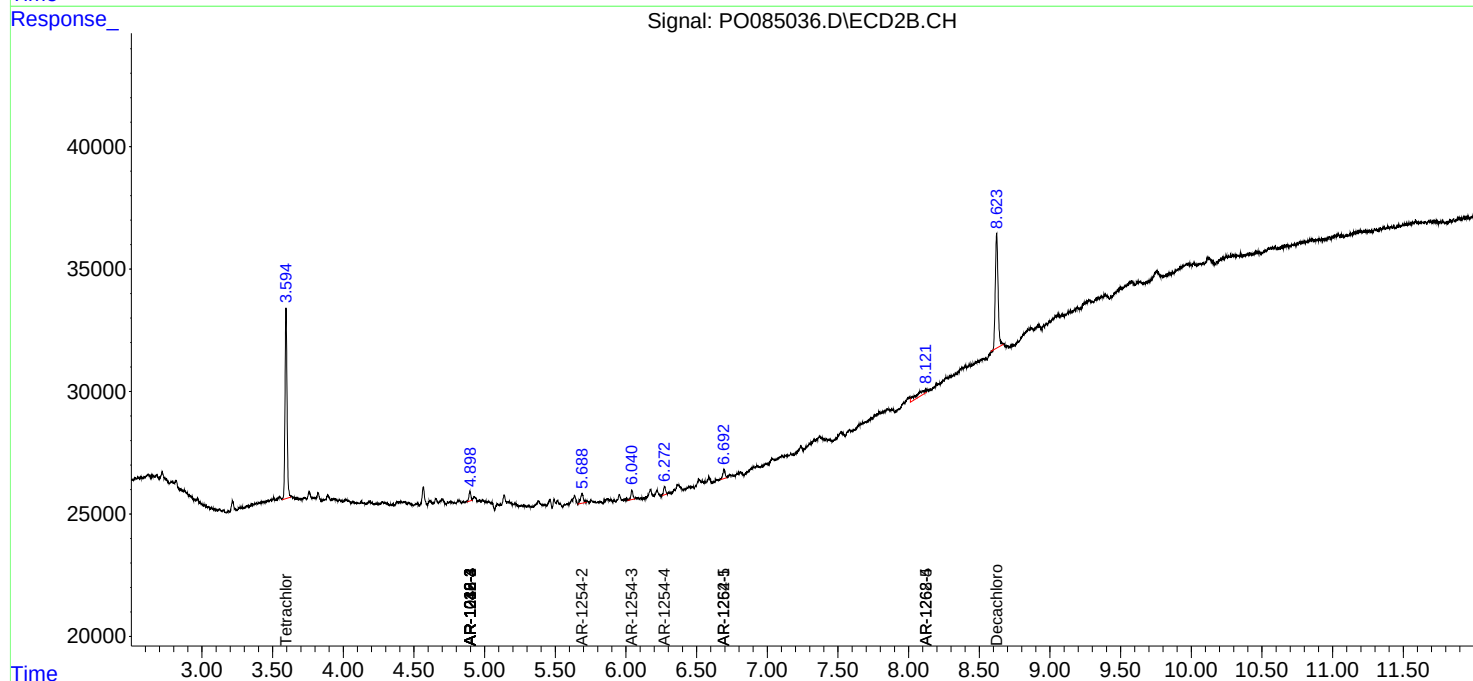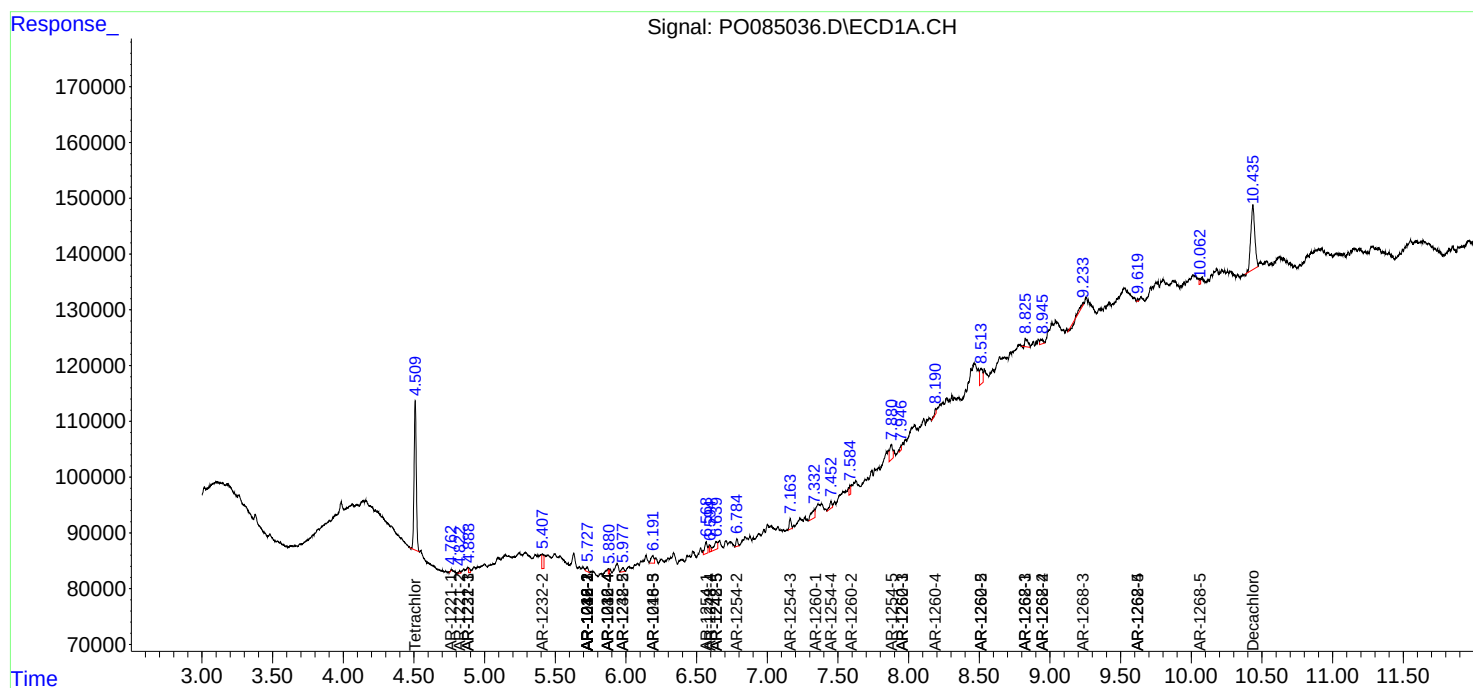


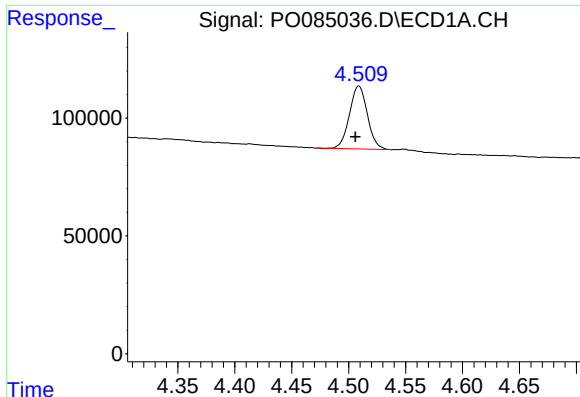

#1 Tetrachloro-m-xylene


R.T.: 4.509 min
Delta R.T.: 0.003 min
Response: 292526
Conc: 1.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

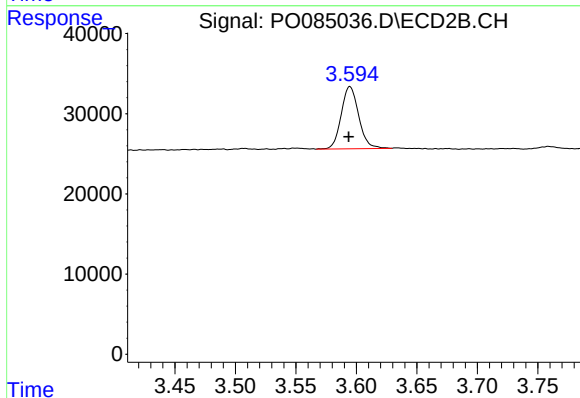


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.001 min
Response: 78063
Conc: 1.74 ng/ml

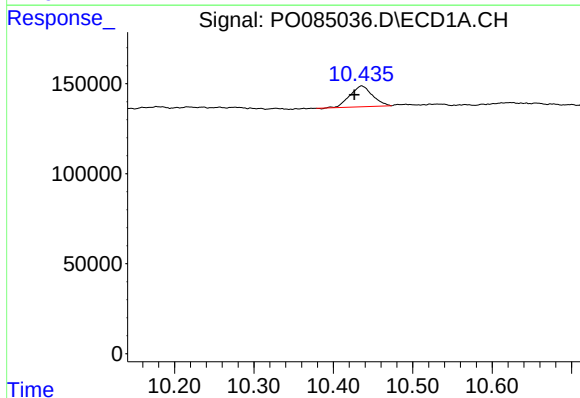


#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.009 min
Response: 225667
Conc: 1.29 ng/ml

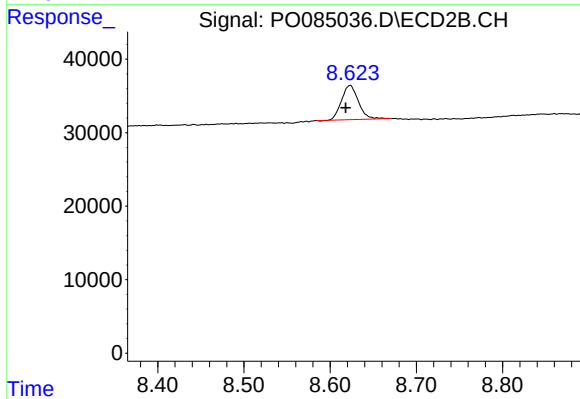

#2 Decachlorobiphenyl


R.T.: 8.623 min
Delta R.T.: 0.005 min
Response: 63636
Conc: 1.73 ng/ml

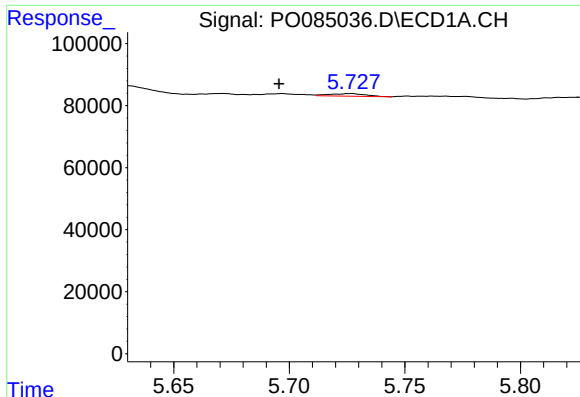

#3 AR-1016-1


R.T.: 5.726 min
Delta R.T.: 0.031 min
Response: 8732
Conc: 0.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

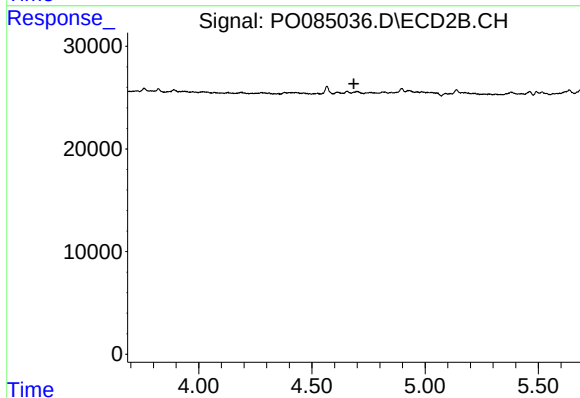


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

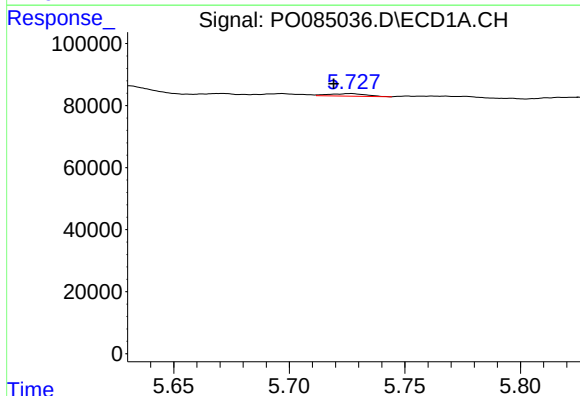


#4 AR-1016-2

R.T.: 5.726 min
Delta R.T.: 0.007 min
Response: 8732
Conc: 0.65 ng/ml

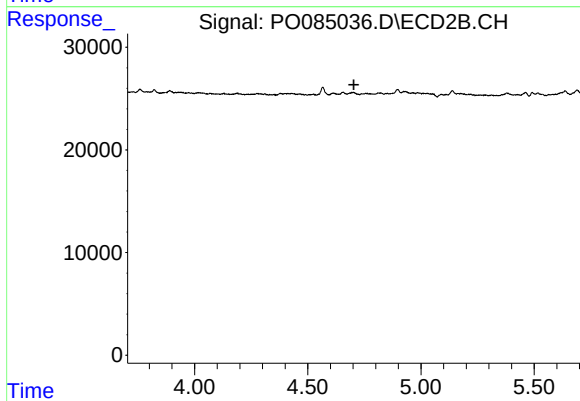

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

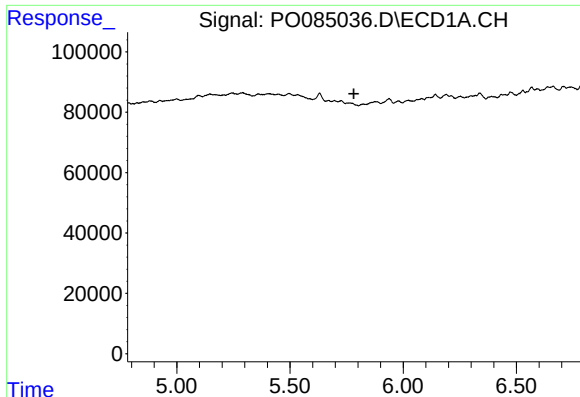

#5 AR-1016-3


R.T.: 5.817 min
Delta R.T.: 0.034 min
Response: -522
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

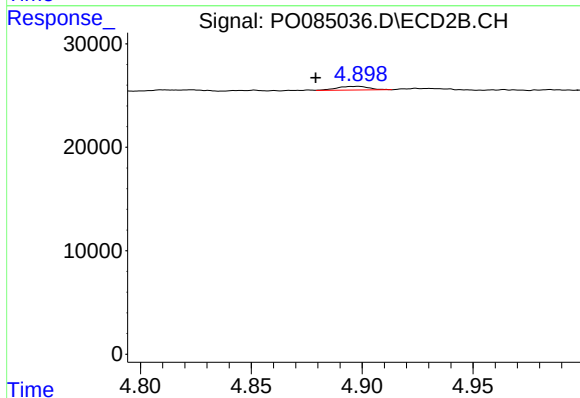


#5 AR-1016-3

R.T.: 4.898 min
Delta R.T.: 0.019 min
Response: 3564
Conc: 2.79 ng/ml

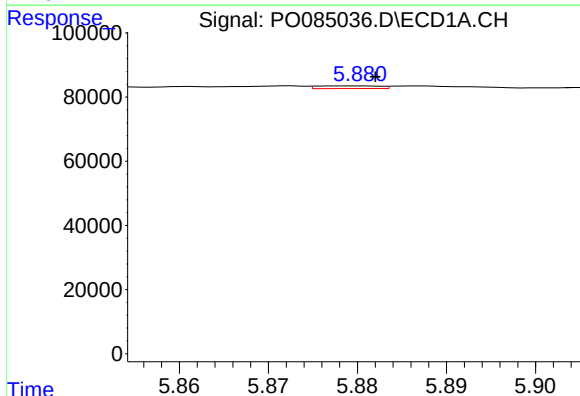


#6 AR-1016-4

R.T.: 5.880 min
Delta R.T.: -0.002 min
Response: 4156
Conc: 0.62 ng/ml

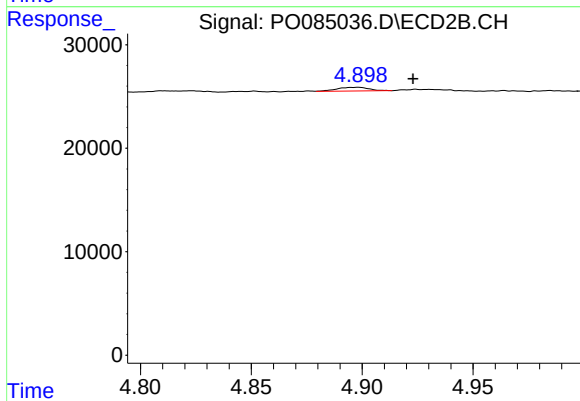

#6 AR-1016-4


R.T.: 4.898 min
Delta R.T.: -0.025 min
Response: 3564
Conc: 3.39 ng/ml

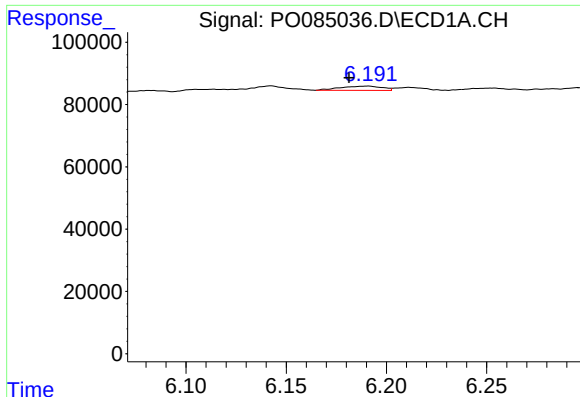

#7 AR-1016-5


R.T.: 6.191 min
Delta R.T.: 0.010 min
Response: 19400
Conc: 3.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

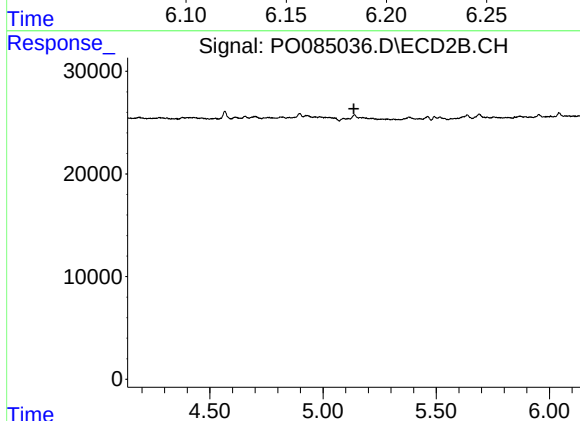


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.136 min
Response: 0
Conc: N.D.

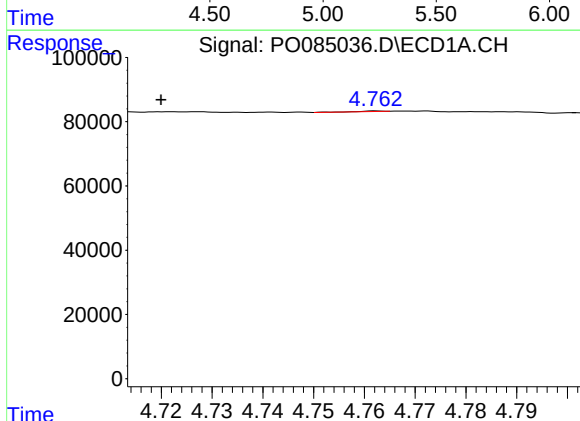


#8 AR-1221-1

R.T.: 4.762 min
Delta R.T.: 0.042 min
Response: 419
Conc: 0.13 ng/ml

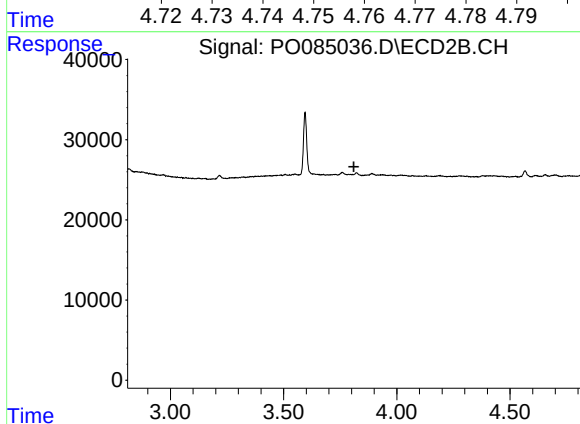

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.811 min
Response: 0
Conc: N.D.

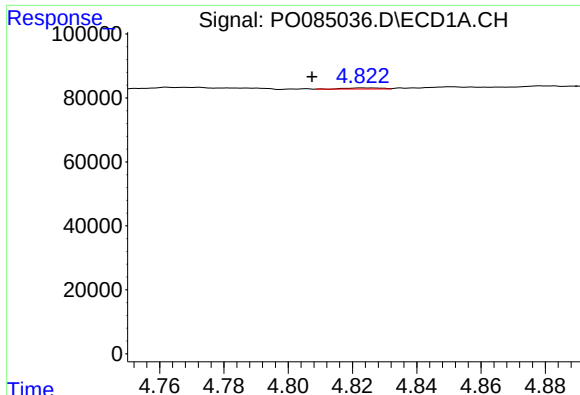

#9 AR-1221-2


R.T.: 4.823 min
Delta R.T.: 0.015 min
Response: 2831
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

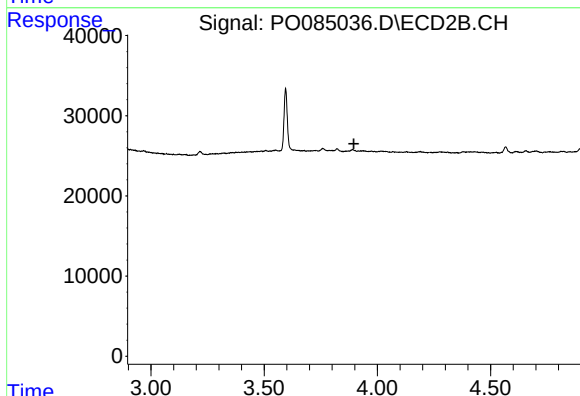


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

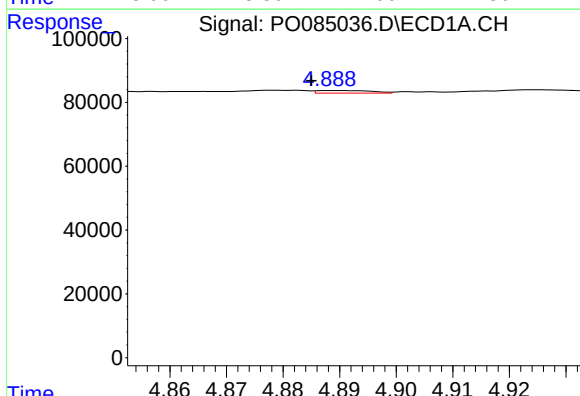


#10 AR-1221-3

R.T.: 4.889 min
Delta R.T.: 0.004 min
Response: 5611
Conc: 0.77 ng/ml

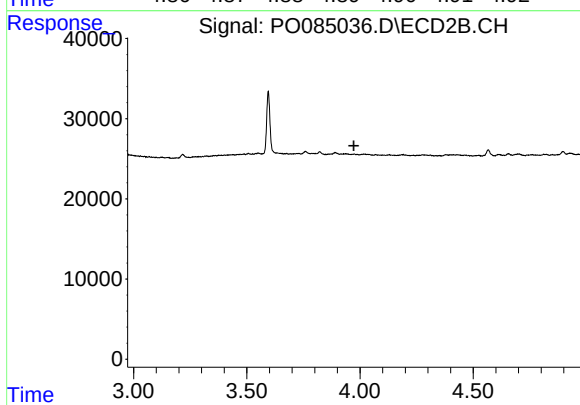

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.973 min
Response: 0
Conc: N.D.

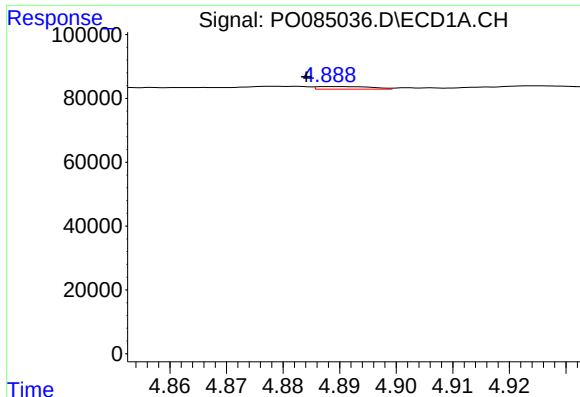

#11 AR-1232-1


R.T.: 4.889 min
Delta R.T.: 0.005 min
Response: 5611
Conc: 0.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

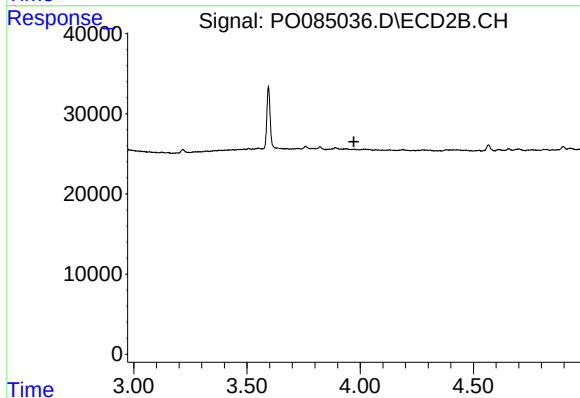


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

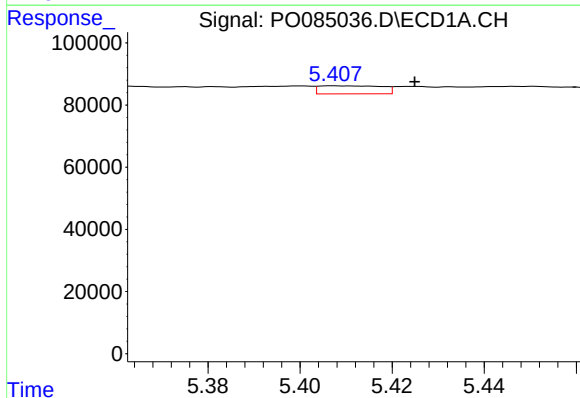


#12 AR-1232-2

R.T.: 5.407 min
Delta R.T.: -0.018 min
Response: 24566
Conc: 8.26 ng/ml

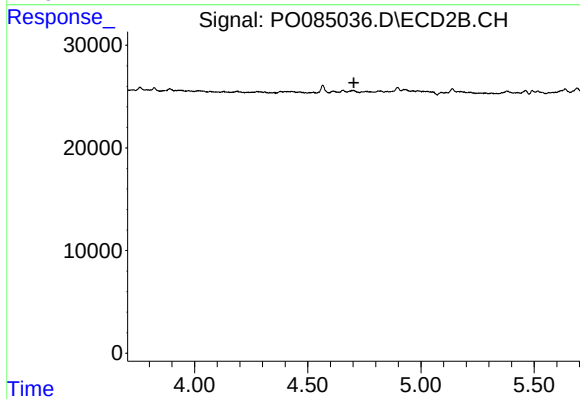

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

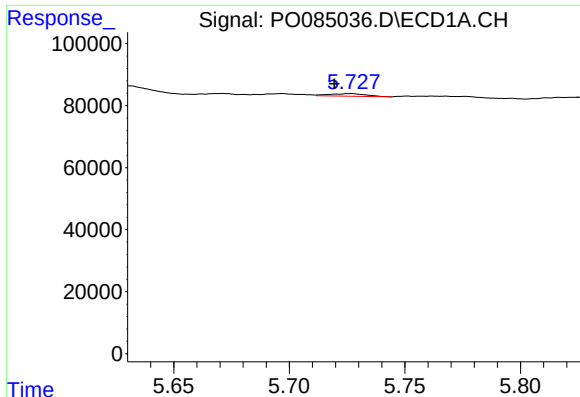

#13 AR-1232-3


R.T.: 5.726 min
Delta R.T.: 0.007 min
Response: 8732
Conc: 1.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

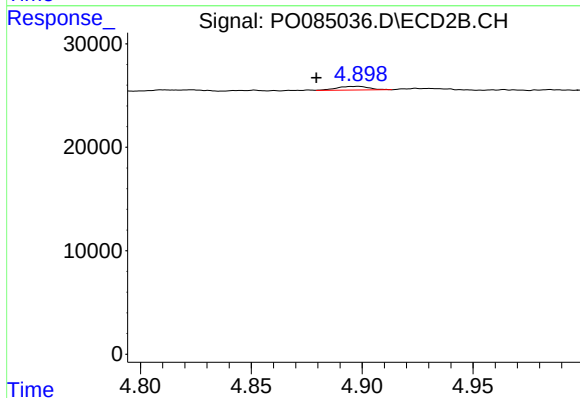


#13 AR-1232-3

R.T.: 4.898 min
Delta R.T.: 0.019 min
Response: 3564
Conc: 6.56 ng/ml

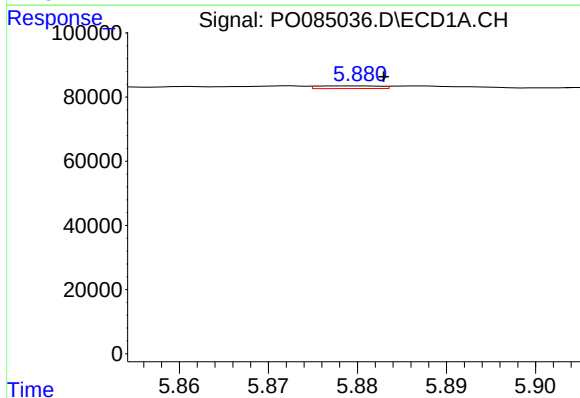


#14 AR-1232-4

R.T.: 5.880 min
Delta R.T.: -0.003 min
Response: 4156
Conc: 1.46 ng/ml

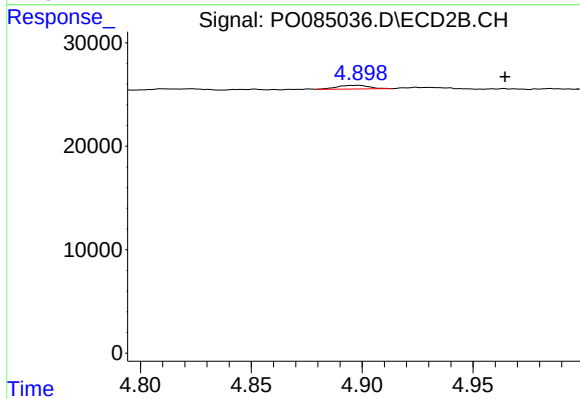

#14 AR-1232-4


R.T.: 4.898 min
Delta R.T.: -0.066 min
Response: 3564
Conc: 7.02 ng/ml

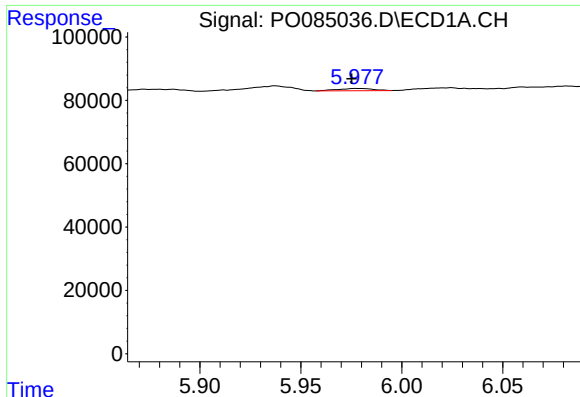

#15 AR-1232-5


R.T.: 5.977 min
Delta R.T.: 0.002 min
Response: 8839
Conc: 3.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

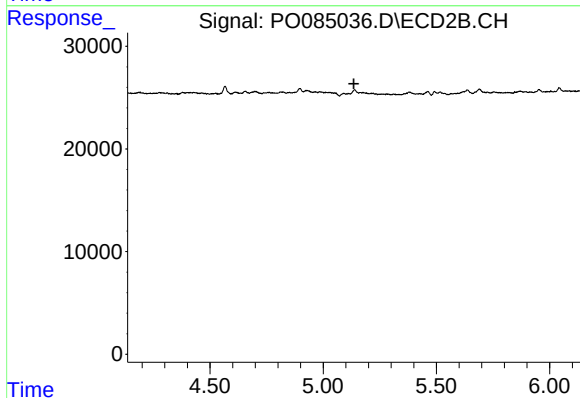


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.135 min
Response: 0
Conc: N.D.

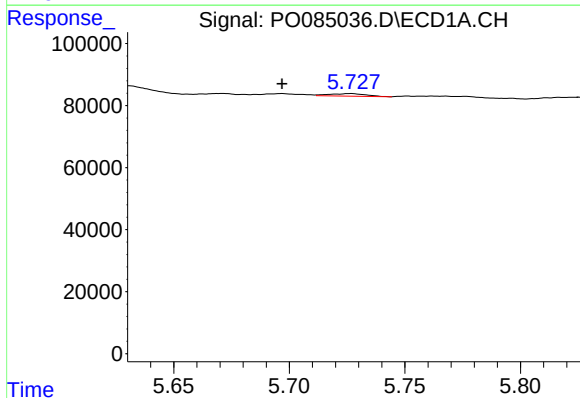


#16 AR-1242-1

R.T.: 5.726 min
Delta R.T.: 0.029 min
Response: 8732
Conc: 1.18 ng/ml

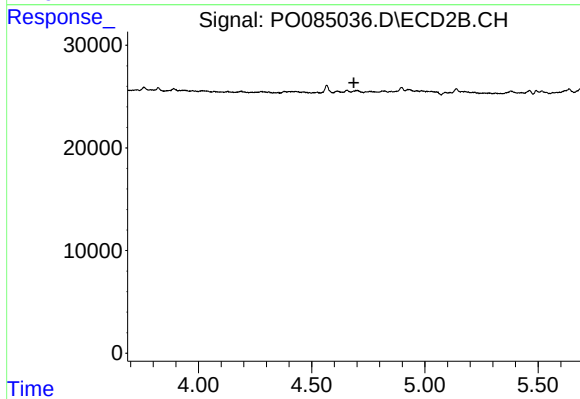

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

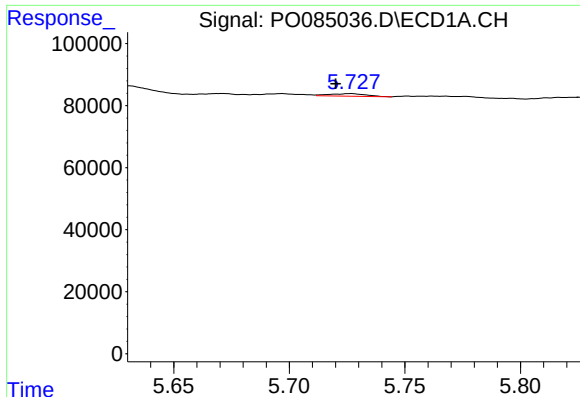

#17 AR-1242-2


R.T.: 5.726 min
Delta R.T.: 0.006 min
Response: 8732
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

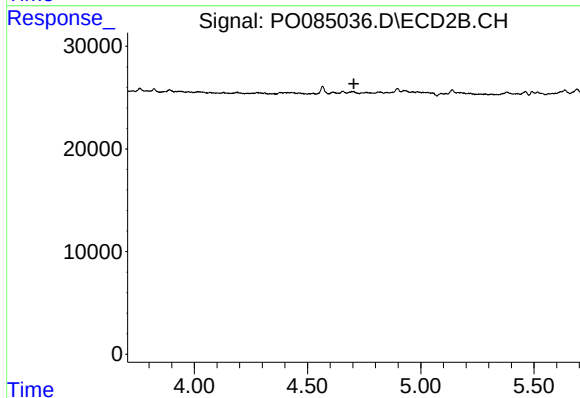


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.705 min
Response: 0
Conc: N.D.

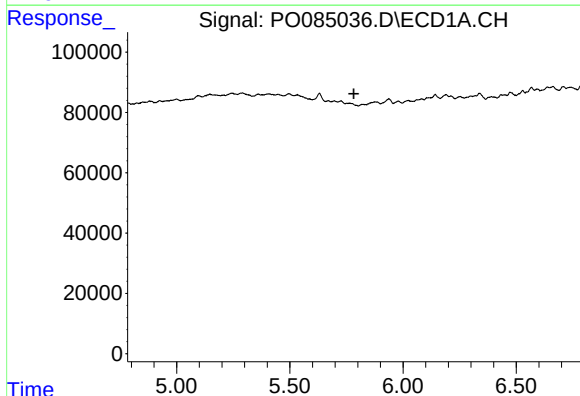


#18 AR-1242-3

R.T.: 5.817 min
Delta R.T.: 0.034 min
Response: -522
Conc: N.D.

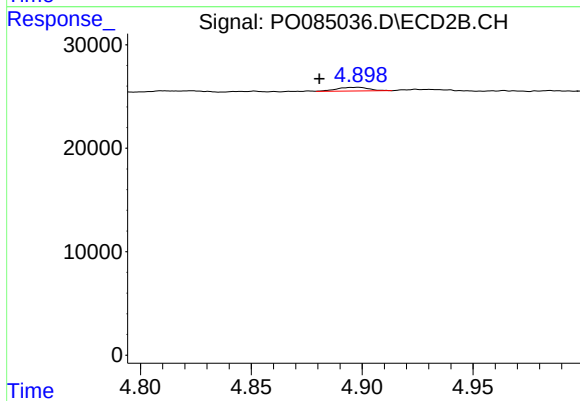

#18 AR-1242-3


R.T.: 4.898 min
Delta R.T.: 0.018 min
Response: 3564
Conc: 3.48 ng/ml

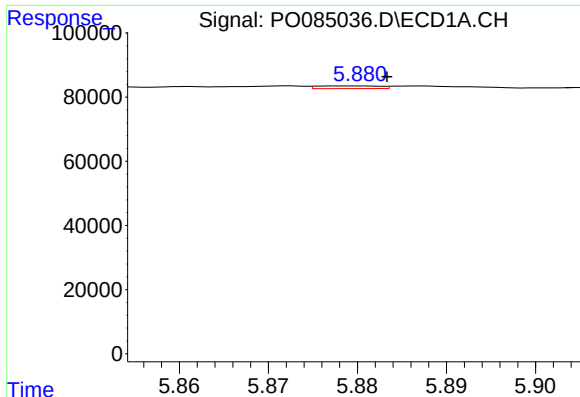

#19 AR-1242-4


R.T.: 5.880 min
Delta R.T.: -0.003 min
Response: 4156
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

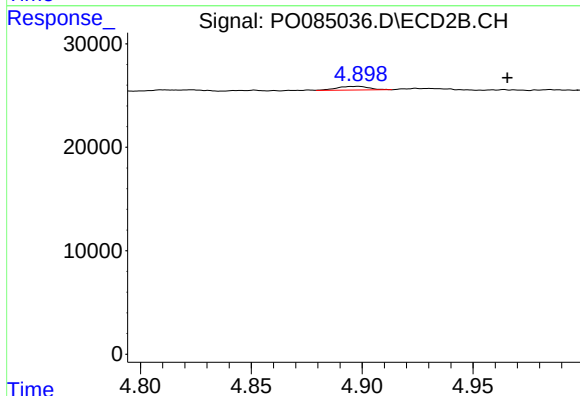


#19 AR-1242-4

R.T.: 4.898 min
Delta R.T.: -0.067 min
Response: 3564
Conc: 3.42 ng/ml

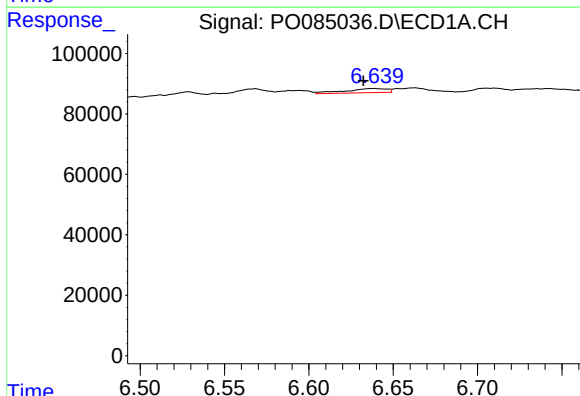


#20 AR-1242-5

R.T.: 6.639 min
Delta R.T.: 0.007 min
Response: 24335
Conc: 4.63 ng/ml

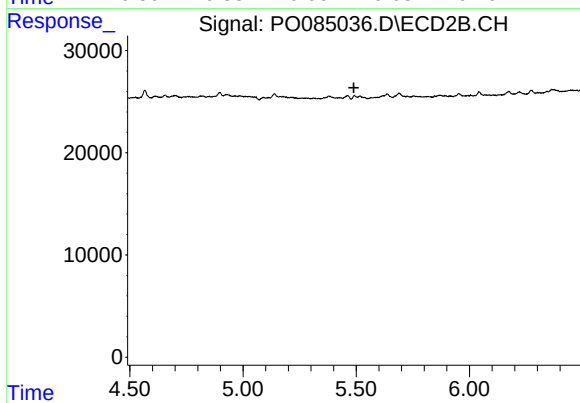

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.490 min
Response: 0
Conc: N.D.

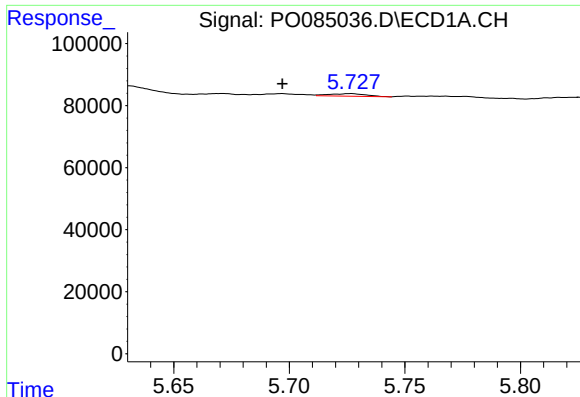

#21 AR-1248-1


R.T.: 5.726 min
Delta R.T.: 0.029 min
Response: 8732
Conc: 1.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

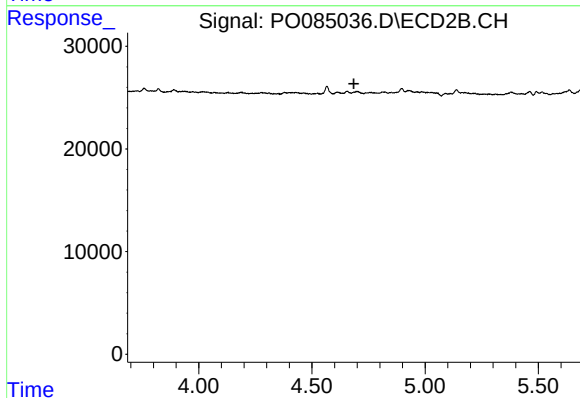


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.685 min
Response: 0
Conc: N.D.

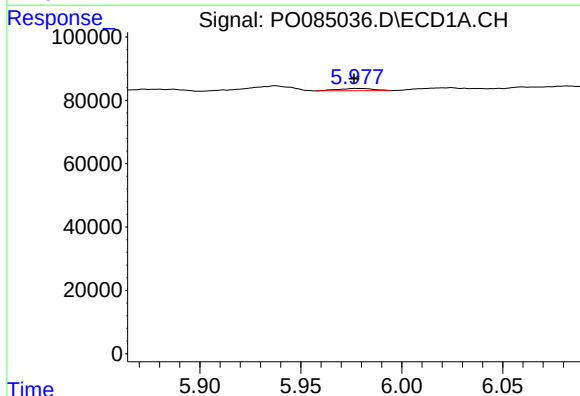


#22 AR-1248-2

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 8839
Conc: 1.15 ng/ml

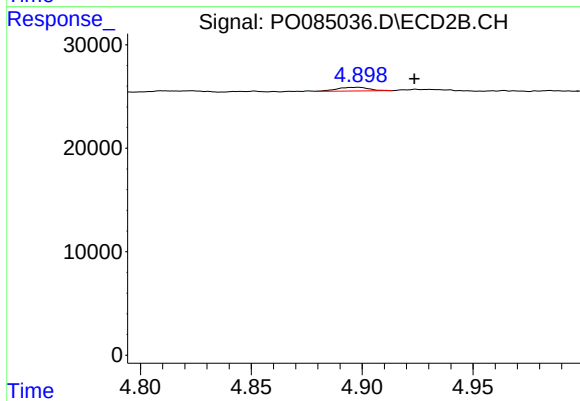

#22 AR-1248-2


R.T.: 4.898 min
Delta R.T.: -0.025 min
Response: 3564
Conc: 2.48 ng/ml

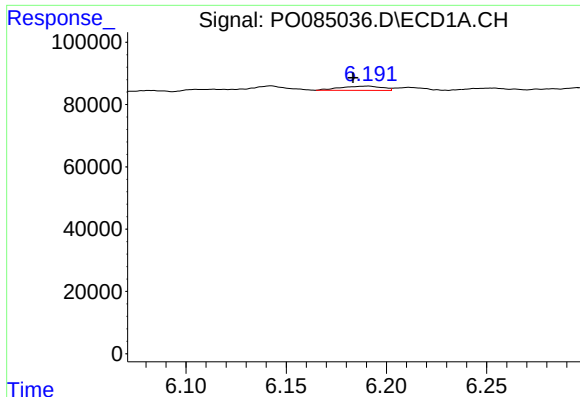

#23 AR-1248-3


R.T.: 6.191 min
Delta R.T.: 0.008 min
Response: 19400
Conc: 2.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

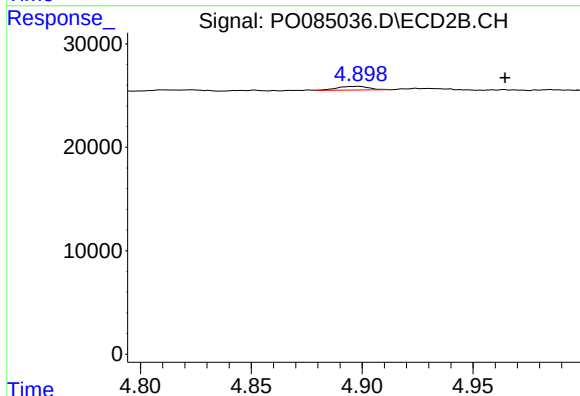


#23 AR-1248-3

R.T.: 4.898 min
Delta R.T.: -0.066 min
Response: 3564
Conc: 2.37 ng/ml

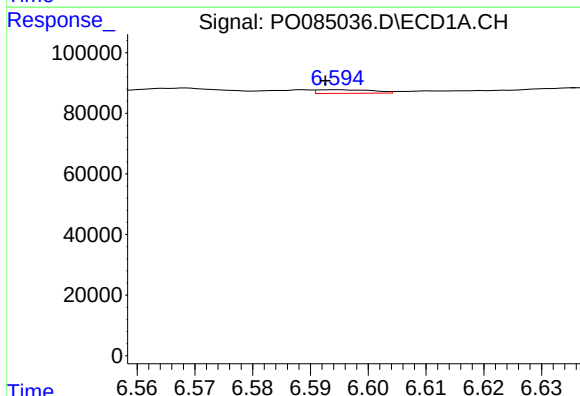


#24 AR-1248-4

R.T.: 6.595 min
Delta R.T.: 0.002 min
Response: 7847
Conc: 0.84 ng/ml

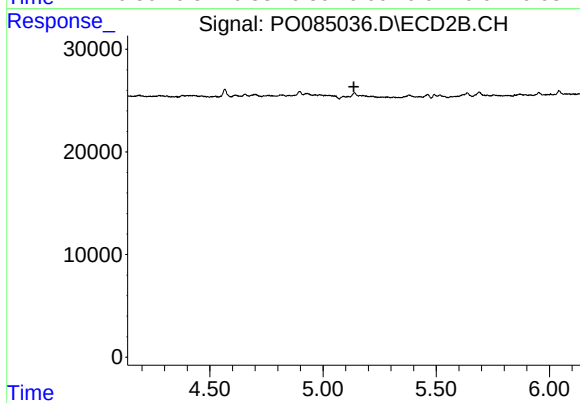

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.136 min
Response: 0
Conc: N.D.

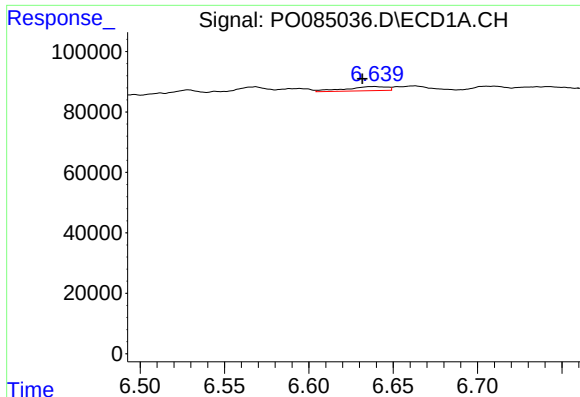

#25 AR-1248-5


R.T.: 6.639 min
Delta R.T.: 0.007 min
Response: 24335
Conc: 2.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

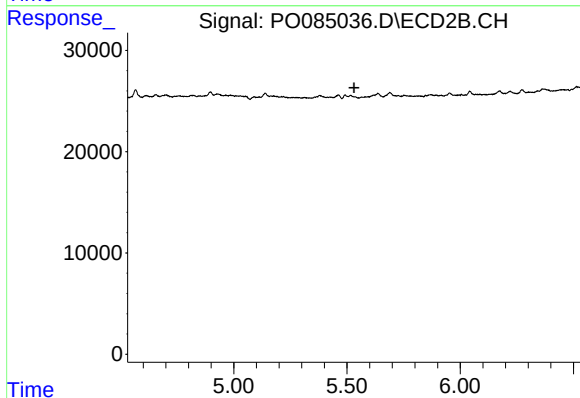


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.531 min
Response: 0
Conc: N.D.

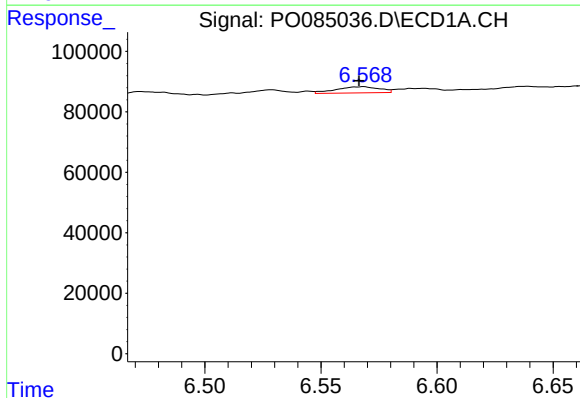


#26 AR-1254-1

R.T.: 6.568 min
Delta R.T.: 0.002 min
Response: 26666
Conc: 2.72 ng/ml

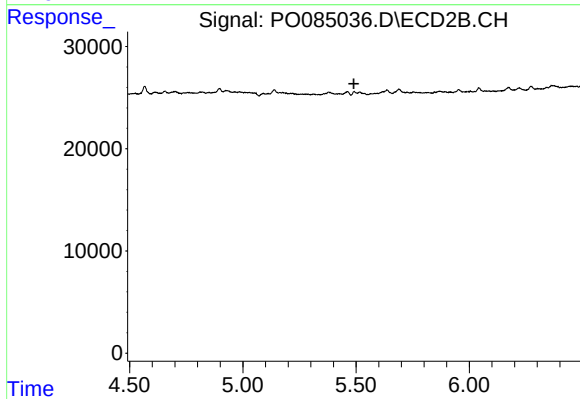

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.490 min
Response: 0
Conc: N.D.

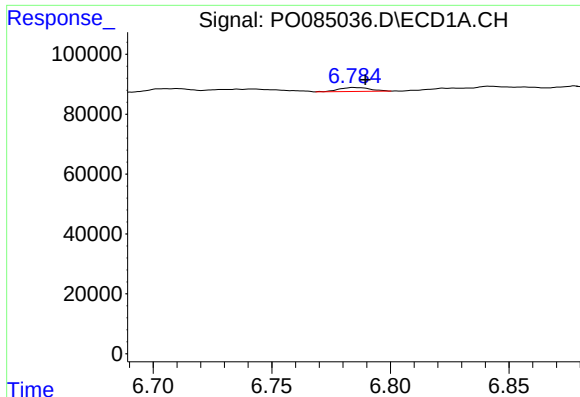

#27 AR-1254-2


R.T.: 6.784 min
Delta R.T.: -0.005 min
Response: 12124
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

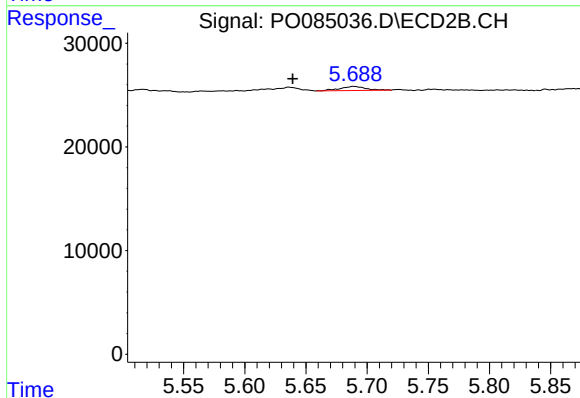


#27 AR-1254-2

R.T.: 5.689 min
Delta R.T.: 0.050 min
Response: 5883
Conc: 2.49 ng/ml

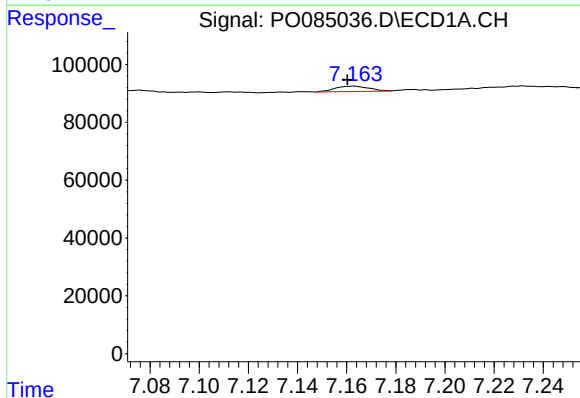


#28 AR-1254-3

R.T.: 7.163 min
Delta R.T.: 0.003 min
Response: 17975
Conc: 1.19 ng/ml

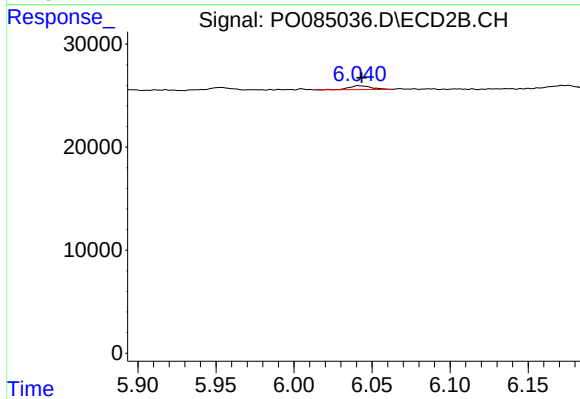

#28 AR-1254-3


R.T.: 6.041 min
Delta R.T.: -0.003 min
Response: 3697
Conc: 0.98 ng/ml

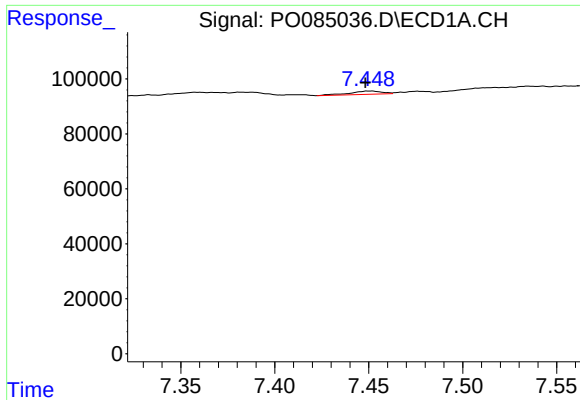

#29 AR-1254-4


R.T.: 7.452 min
Delta R.T.: 0.004 min
Response: 14290
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

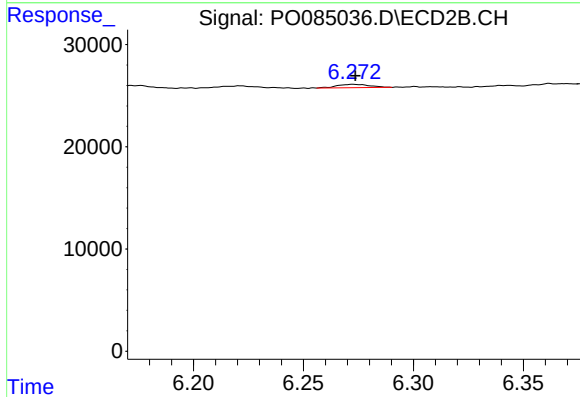


#29 AR-1254-4

R.T.: 6.273 min
Delta R.T.: -0.001 min
Response: 3367
Conc: 1.44 ng/ml

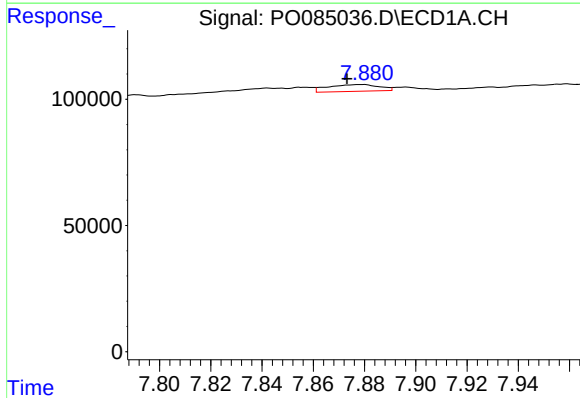


#30 AR-1254-5

R.T.: 7.880 min
Delta R.T.: 0.006 min
Response: 37826
Conc: 3.21 ng/ml

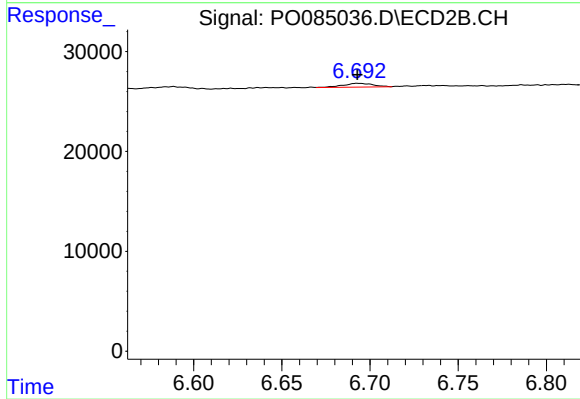

#30 AR-1254-5


R.T.: 6.693 min
Delta R.T.: 0.000 min
Response: 4330
Conc: 1.28 ng/ml

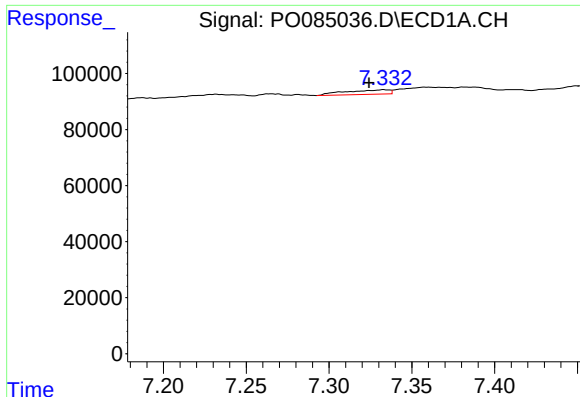

#31 AR-1260-1


R.T.: 7.333 min
Delta R.T.: 0.009 min
Response: 29226
Conc: 2.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

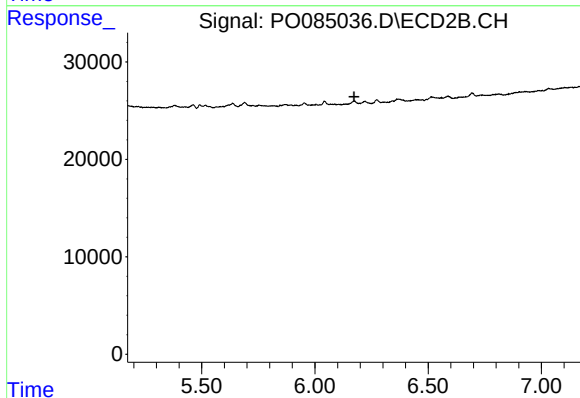


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.173 min
Response: 0
Conc: N.D.

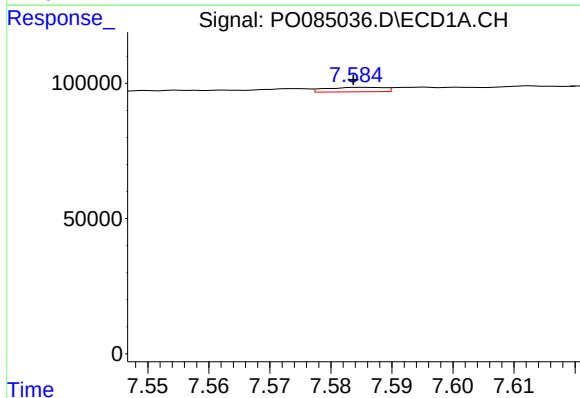


#32 AR-1260-2

R.T.: 7.585 min
Delta R.T.: 0.001 min
Response: 10941
Conc: 0.85 ng/ml

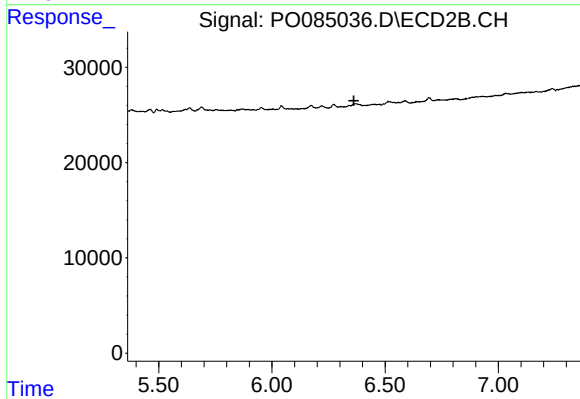

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.362 min
Response: 0
Conc: N.D.

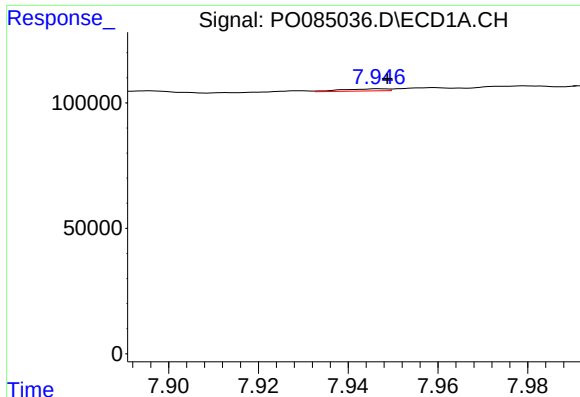

#33 AR-1260-3


R.T.: 7.947 min
Delta R.T.: -0.002 min
Response: 6051
Conc: 0.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

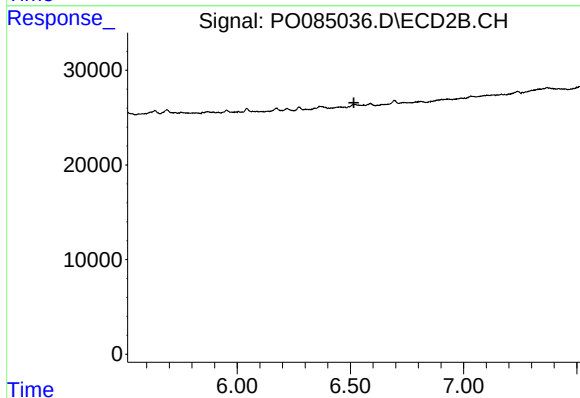


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.516 min
Response: 0
Conc: N.D.

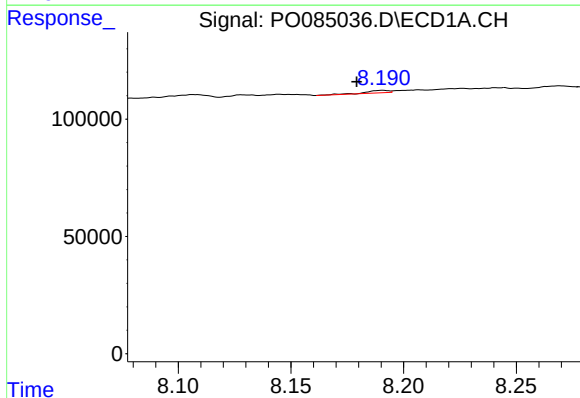


#34 AR-1260-4

R.T.: 8.191 min
Delta R.T.: 0.012 min
Response: 7313
Conc: 0.77 ng/ml

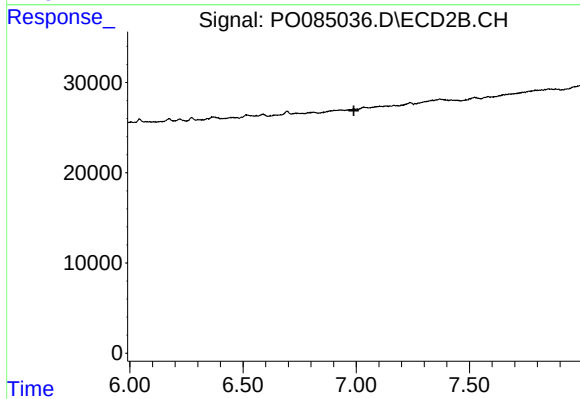

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.

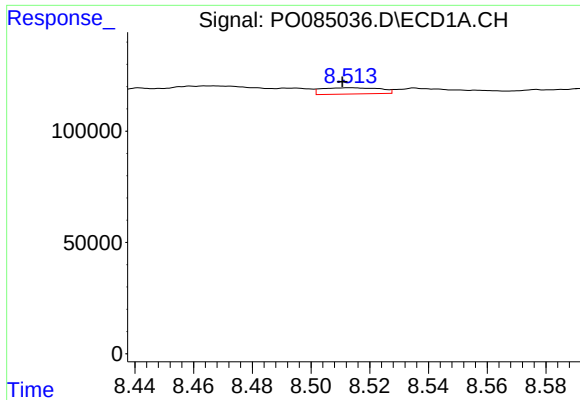

#35 AR-1260-5


R.T.: 8.513 min
Delta R.T.: 0.003 min
Response: 38695
Conc: 2.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

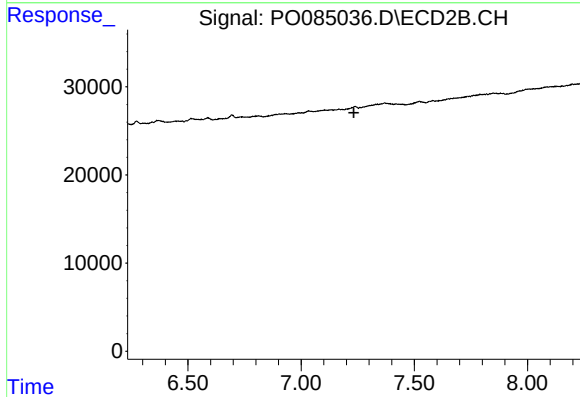


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.233 min
Response: 0
Conc: N.D.

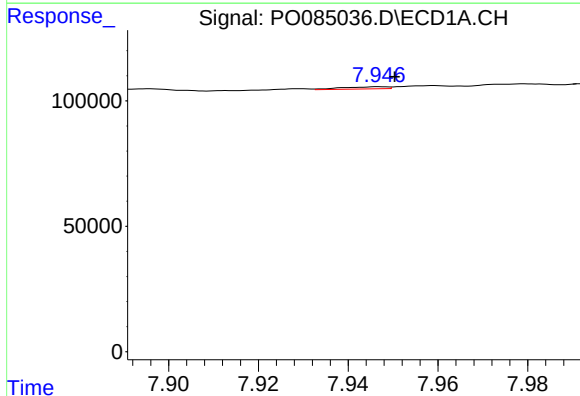


#36 AR-1262-1

R.T.: 7.947 min
Delta R.T.: -0.004 min
Response: 6051
Conc: 0.67 ng/ml

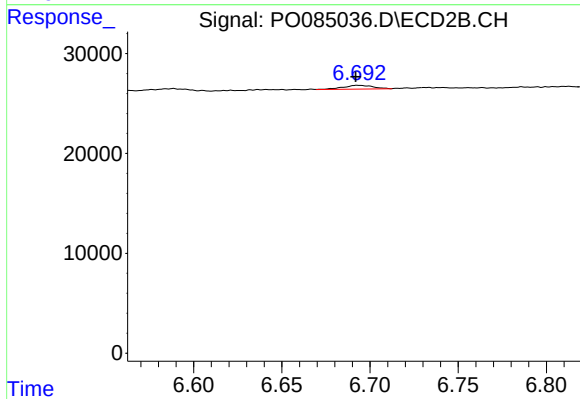

#36 AR-1262-1


R.T.: 6.693 min
Delta R.T.: 0.001 min
Response: 4330
Conc: 3.59 ng/ml

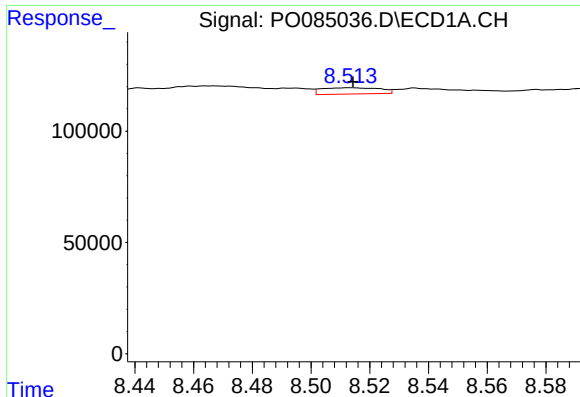

#37 AR-1262-2


R.T.: 8.513 min
Delta R.T.: 0.000 min
Response: 38695
Conc: 2.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

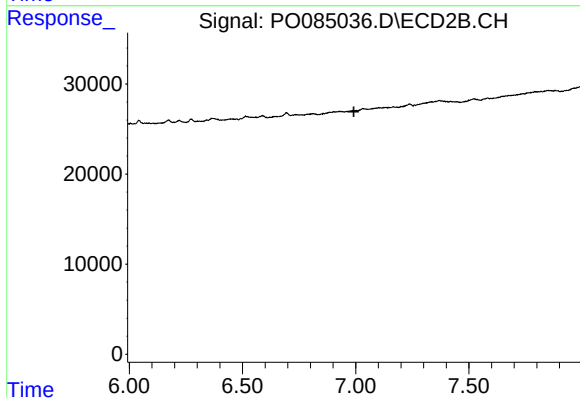


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 6.992 min
Response: 0
Conc: N.D.

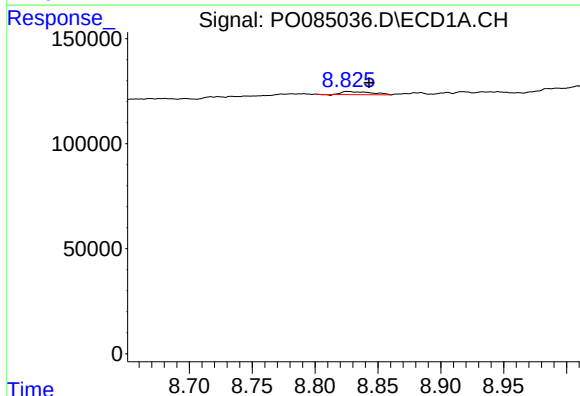


#38 AR-1262-3

R.T.: 8.826 min
Delta R.T.: -0.017 min
Response: 23529
Conc: 2.24 ng/ml

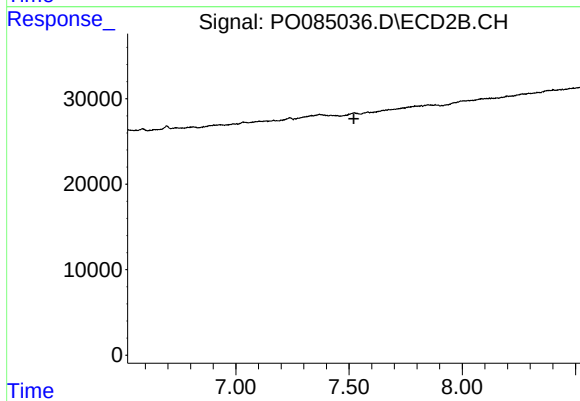

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.521 min
Response: 0
Conc: N.D.

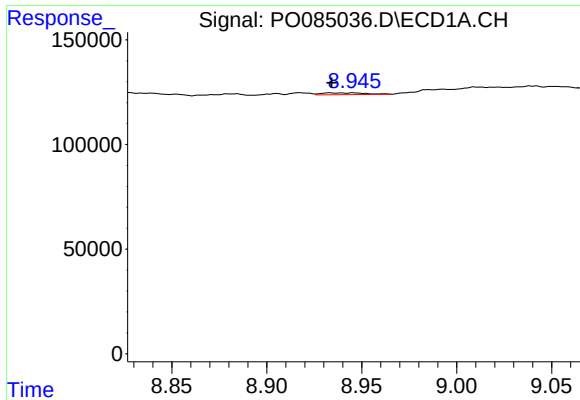

#39 AR-1262-4


R.T.: 8.946 min
Delta R.T.: 0.011 min
Response: 13061
Conc: 2.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

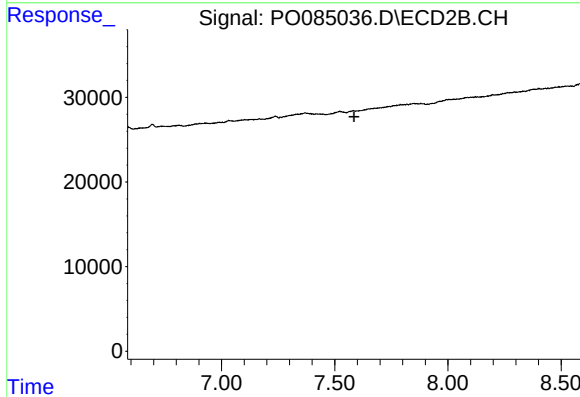


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.585 min
Response: 0
Conc: N.D.

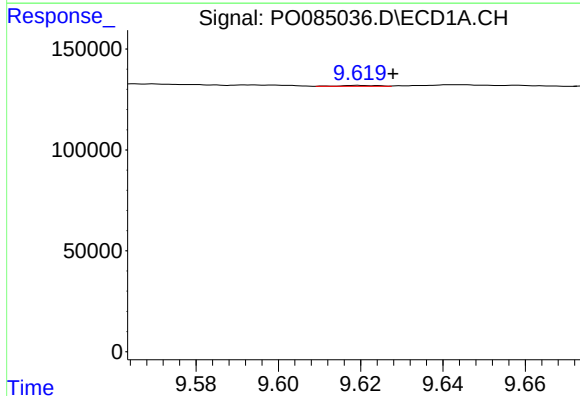


#40 AR-1262-5

R.T.: 9.619 min
Delta R.T.: -0.009 min
Response: 2714
Conc: 0.50 ng/ml

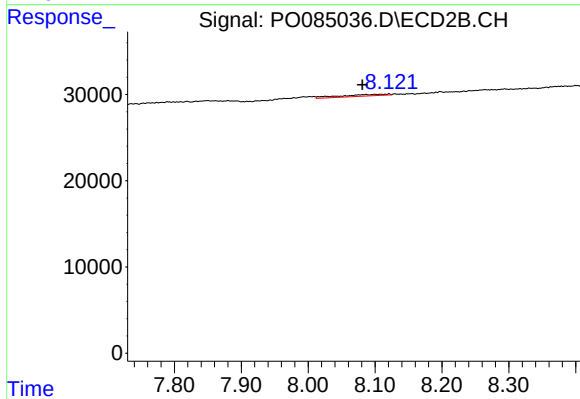

#40 AR-1262-5


R.T.: 8.121 min
Delta R.T.: 0.040 min
Response: 9108
Conc: 6.88 ng/ml

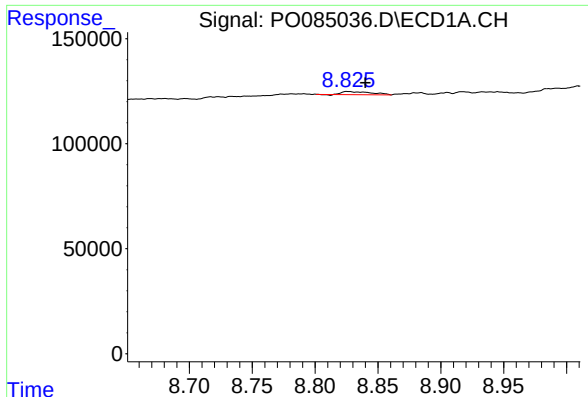

#41 AR-1268-1


R.T.: 8.826 min
Delta R.T.: -0.014 min
Response: 23529
Conc: 0.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

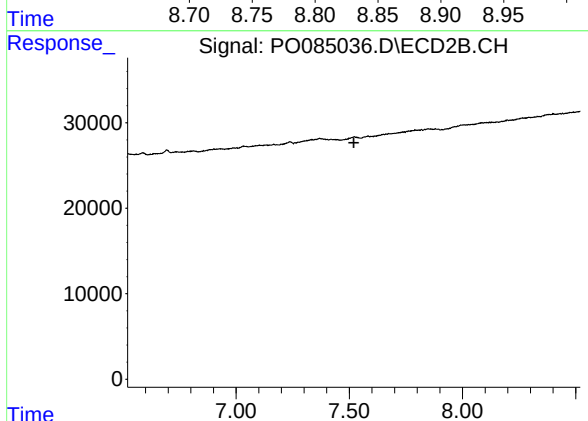


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.521 min
Response: 0
Conc: N.D.

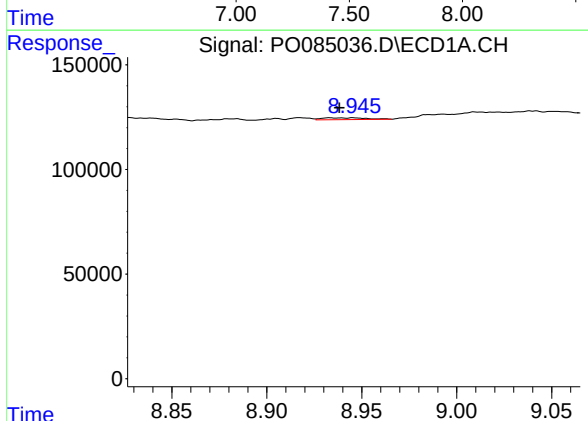


#42 AR-1268-2

R.T.: 8.946 min
Delta R.T.: 0.007 min
Response: 13061
Conc: 0.52 ng/ml

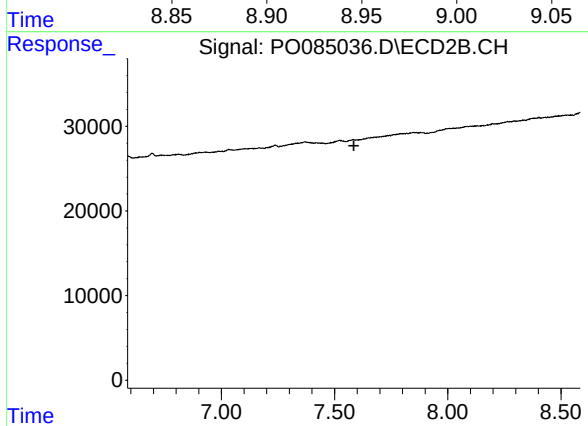

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.585 min
Response: 0
Conc: N.D.

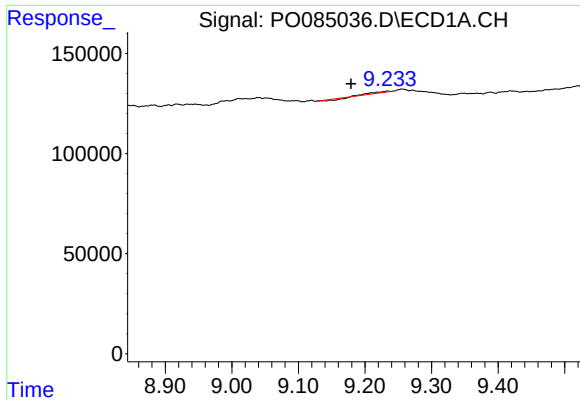

#43 AR-1268-3


R.T.: 9.234 min
Delta R.T.: 0.055 min
Response: 3338
Conc: 0.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

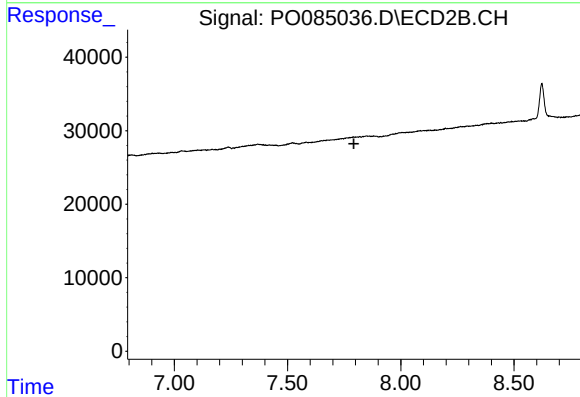


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

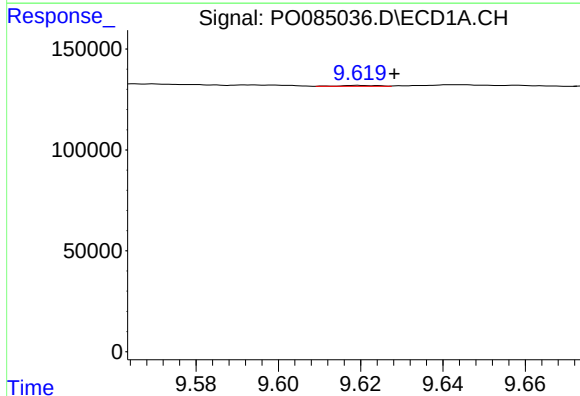


#44 AR-1268-4

R.T.: 9.619 min
Delta R.T.: -0.009 min
Response: 2714
Conc: 0.30 ng/ml

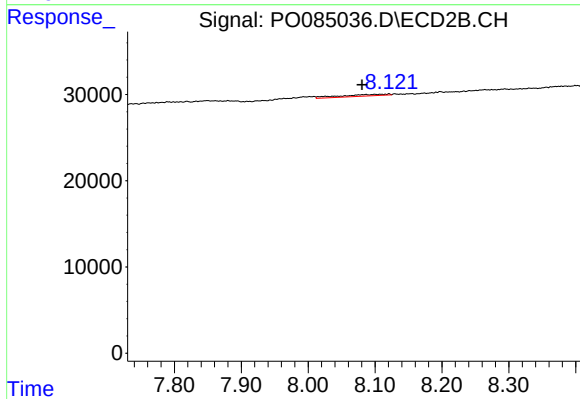

#44 AR-1268-4


R.T.: 8.121 min
Delta R.T.: 0.040 min
Response: 9108
Conc: 3.99 ng/ml

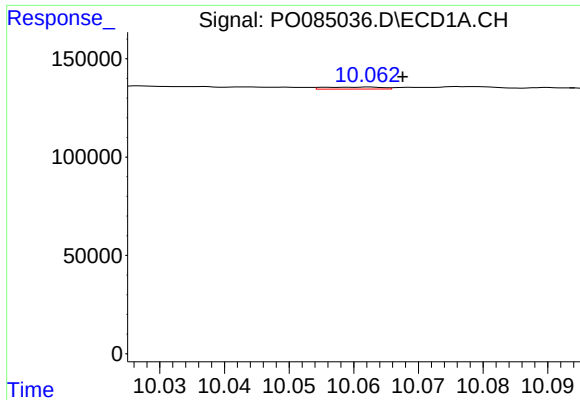

#45 AR-1268-5

R.T.: 10.062 min
Delta R.T.: -0.006 min
Response: 6326
Conc: 0.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-82A

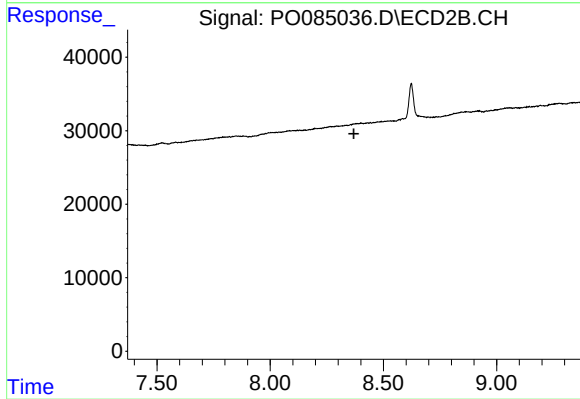

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.369 min
Response: 0
Conc: N.D.