Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO084981.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2022 9:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:49:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.508	3.594	5846937	1055695	20.912	23.475
2)	SA Decachlor...	10.431	8.620	4016182	858172	22.912	23.354
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO084981.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2022 9:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:49:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

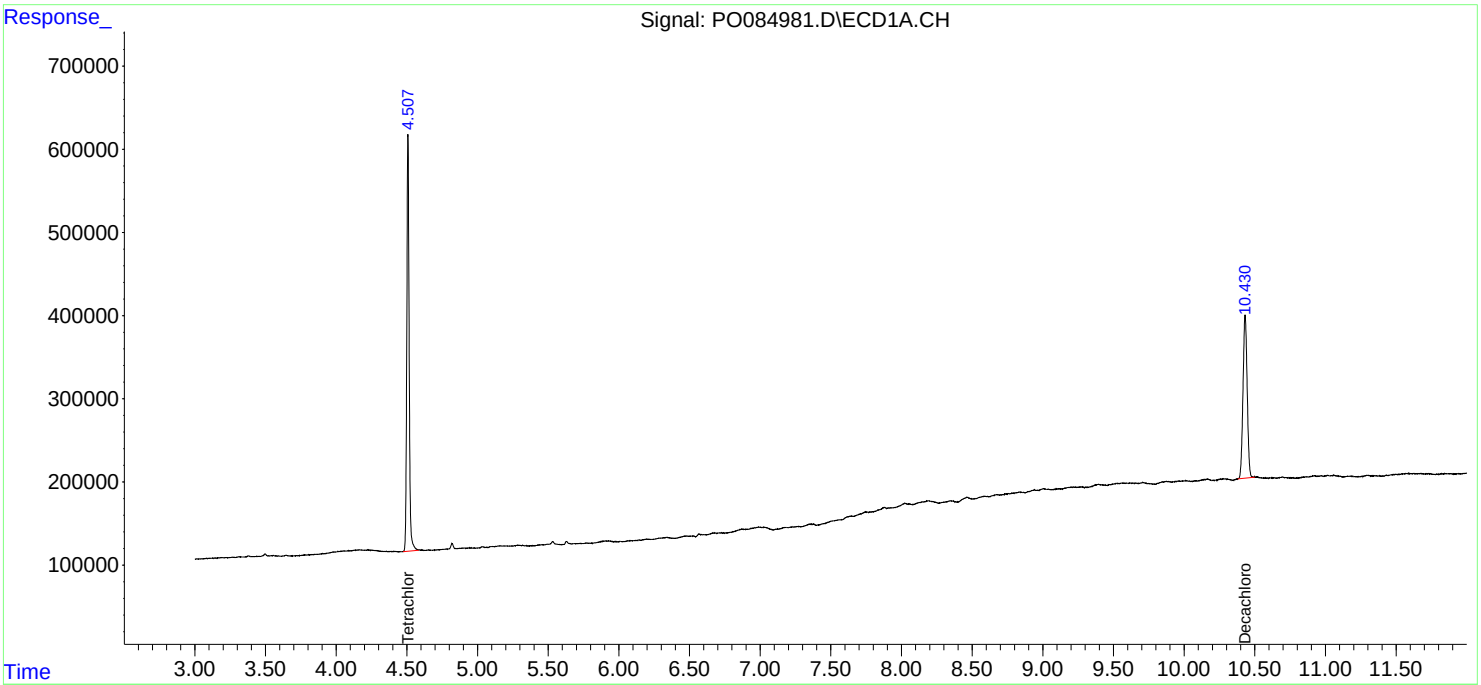

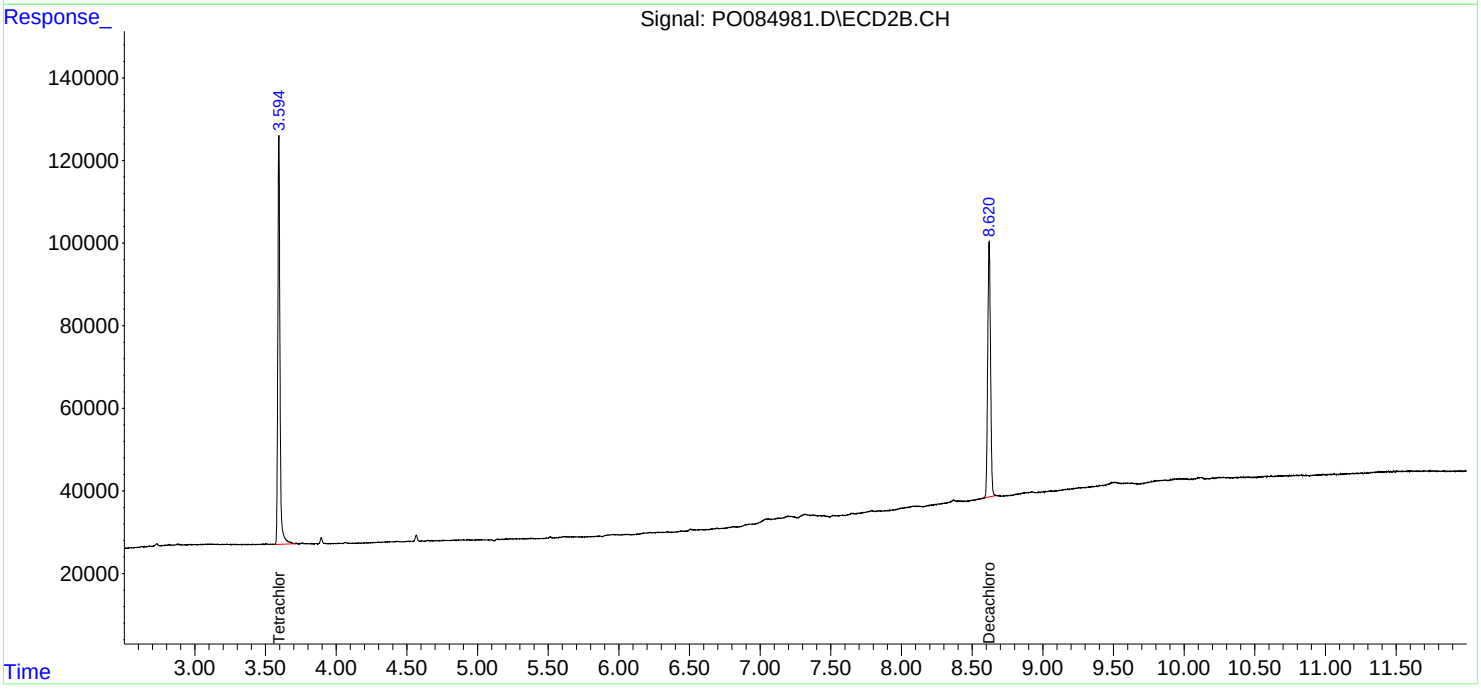

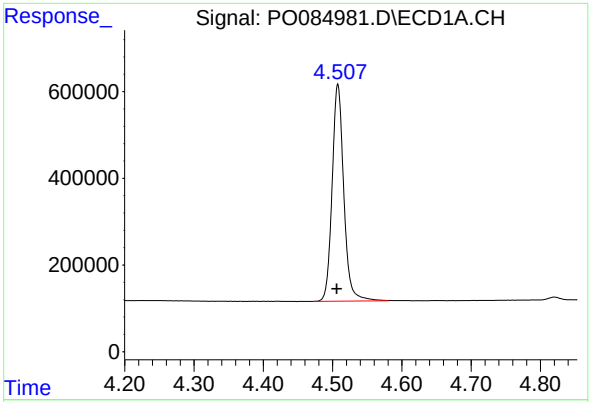

#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: 0.002 min
Response: 5846937
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

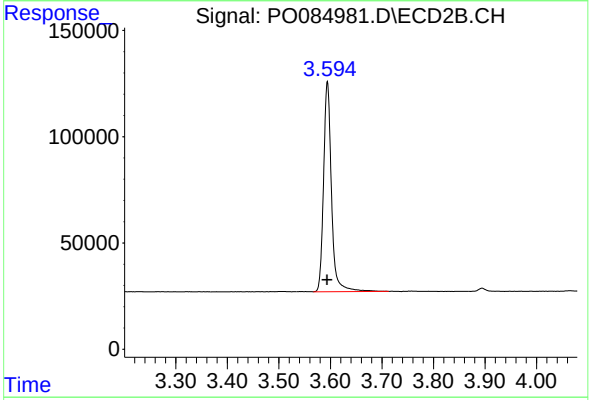

#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 1055695
Conc: 23.48 ng/ml

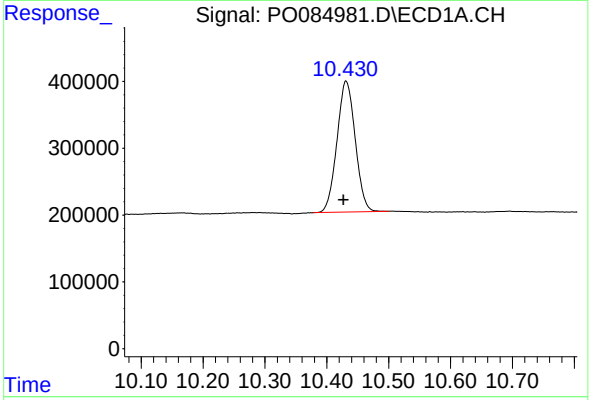

#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.004 min
Response: 4016182
Conc: 22.91 ng/ml

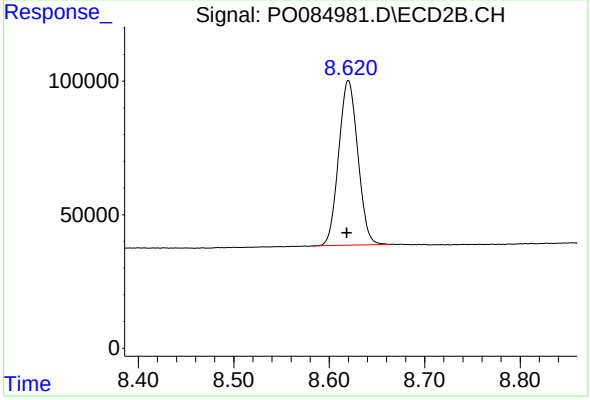

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: 0.002 min
Response: 858172
Conc: 23.35 ng/ml