

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030222\
 Data File : P0085024.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Mar 2022 00:08
 Operator : YP\AJ
 Sample : N1718-03 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-022322-03

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/03/2022
 Supervised By :Ankita Jodhani 03/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 04:27:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 28 18:40:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.595	488049	111801	1.746m	2.486m#
2) SA Decachlor...	10.436	8.621	514215	76002	2.934m	2.068m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030222\
Data File : PO085024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Mar 2022 00:08
Operator : YP\AJ
Sample : N1718-03 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-022322-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/03/2022
Supervised By :Ankita Jodhani 03/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 04:27:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022822.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 28 18:40:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

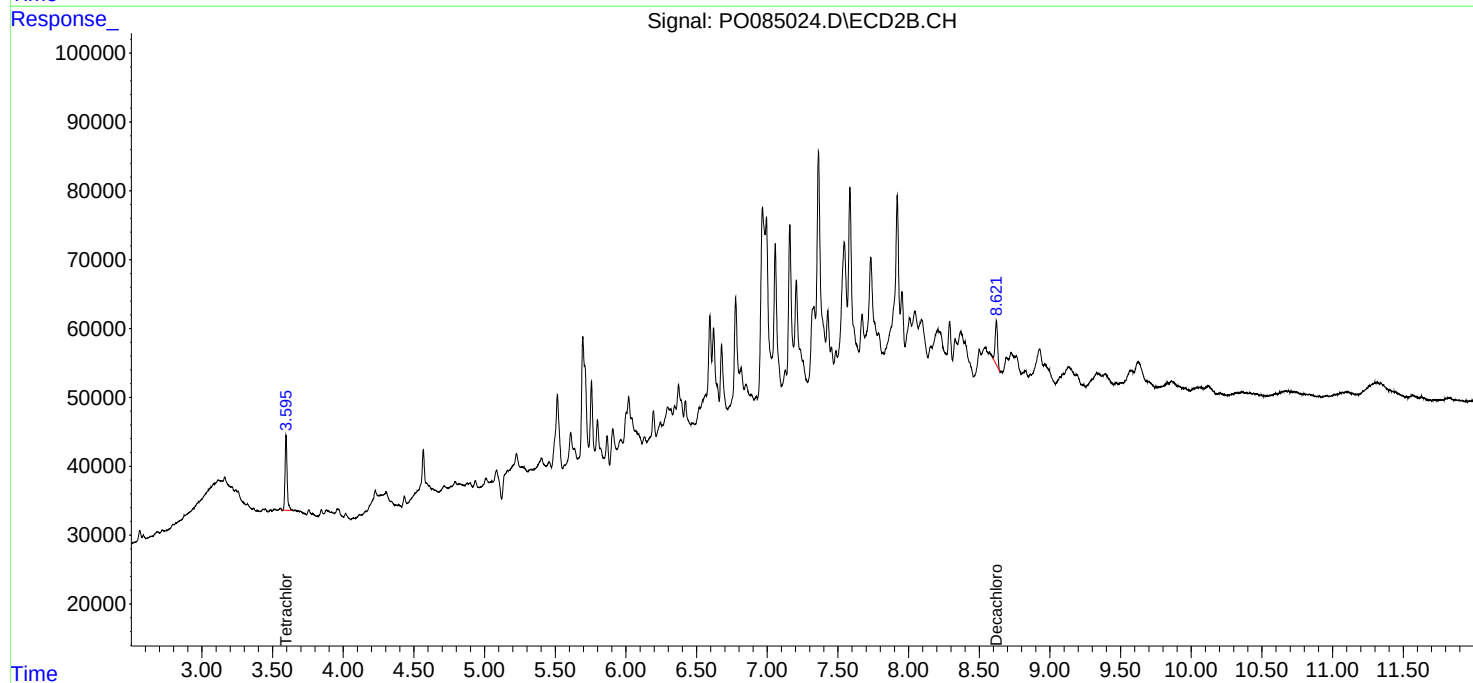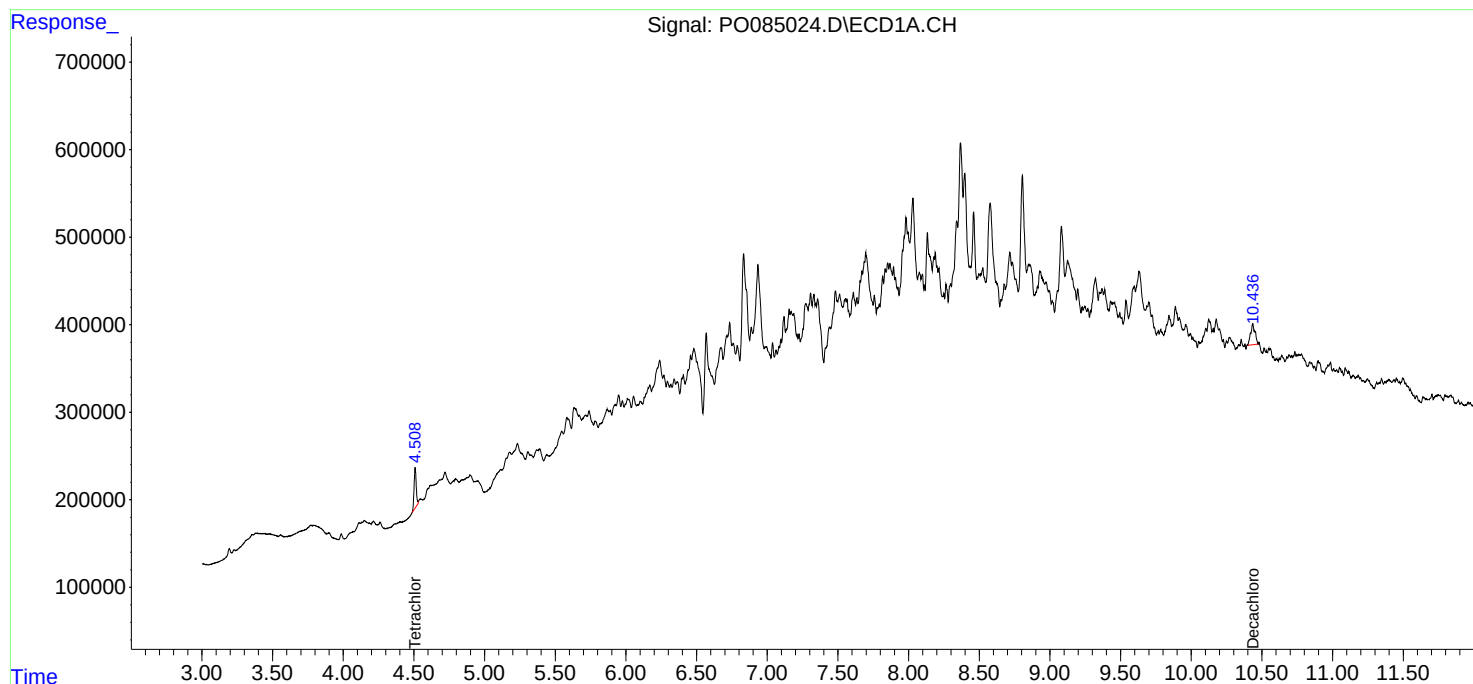

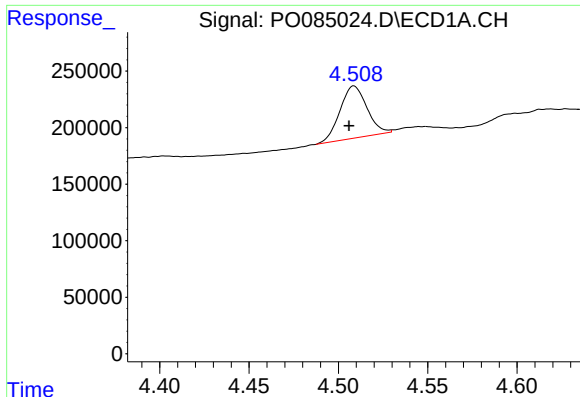


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: 0.002 min
Response: 488049
Conc: 1.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-022322-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/03/2022
Supervised By :Ankita Jodhani 03/03/2022

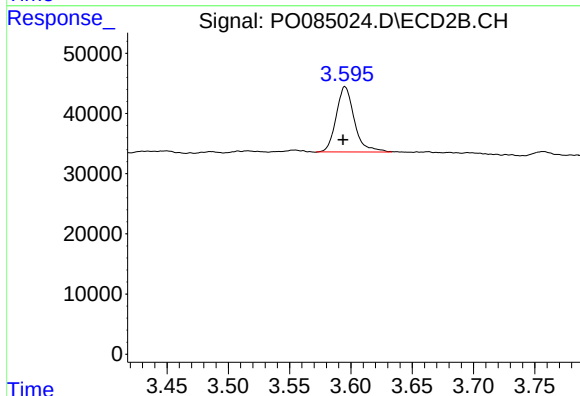


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.001 min
Response: 111801
Conc: 2.49 ng/ml m

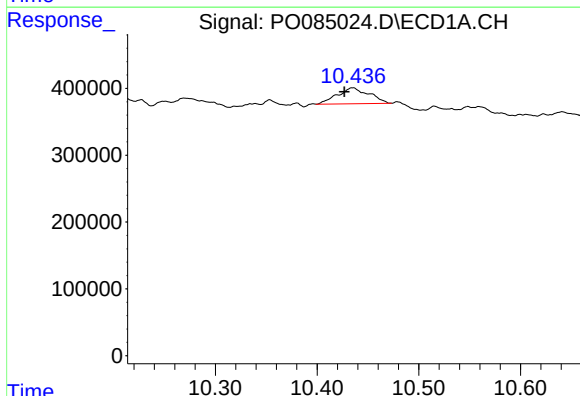

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.009 min
Response: 514215
Conc: 2.93 ng/ml m

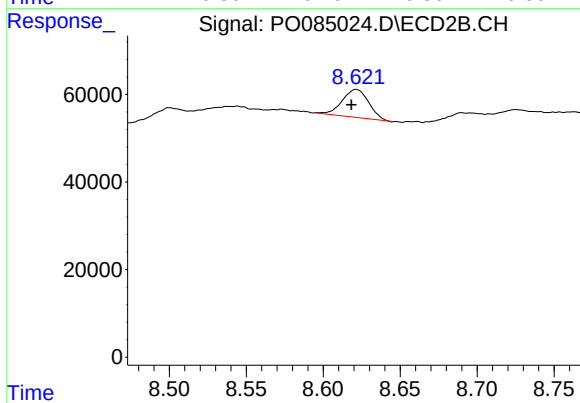

#2 Decachlorobiphenyl

R.T.: 8.621 min
Delta R.T.: 0.003 min
Response: 76002
Conc: 2.07 ng/ml m